STAT Analysis Corporation

This canister has been cleaned and certified per the indicated data below and is acceptable for field sampling

Can #: [illegible] Batch Certification #: [illegible]

Date Cleaned: [illegible]

Initial Can Pressure [illegible] psig

Flow Controller #: [illegible] Timed: _____ hr

U-HAUL
SCEPTR
40"
LCD HDTV
•Sleek & Slim LCD 1080P HDTV
•4 x HDMI High Definition Inputs
•ATSC/NTSC/Clear QAM
•Response Time 8ms
•450 cd/m2 Brightness
•Panel Resolution 192
•90,000:1 Dynamic Cor
•10W x 2 Speakers
•7-BAND EQ
•USB 2.0 for JPEG / Aud
•1.07 Billion Colors
•Swivel Base
WWW.SCEPTRE.COM
DELL

U-HAUL
SCEPTR
40"
LCD HDTV
•Sleek & Slim LCD 1080P HDTV
•4 x HDMI High Definition Inputs
•ATSC/NTSC/Clear QAM
•Response Time 8ms
•450 cd/m2 Brightness
•10W x 2 Speakers
•7-BAND EQ
•USB 2.0 for JPEG
•1.07 Billion Colors
•Swivel Base
WWW.SCEPTRE.COM
STAT Analysis Corporation

TOURNAMENT XO
8-PLAYER ELECTRONIC DARTBOARD WITH INTEGRATED CABINET
CIBLE ÉLECTRONIQUE 8 JOUEURS À BOÎTIER INTÉGRÉ

STAT Analysis Corporation

This canister has been cleaned and certified per the indicated date below and is acceptable for field sampling

Can # [illegible] Batch Certification # [illegible]

Date Cleaned : [illegible]

[illegible] Pressure [illegible] psig

[illegible]ifier # [illegible] Timed : ____ hr

Richmond
9
YEAR
PRESS TO CLOSE
LIFT TO OPEN

DEWALT
HIGH-TECH CABINET
COFFRET HAUTE TECHNOLOGIE
Great Value

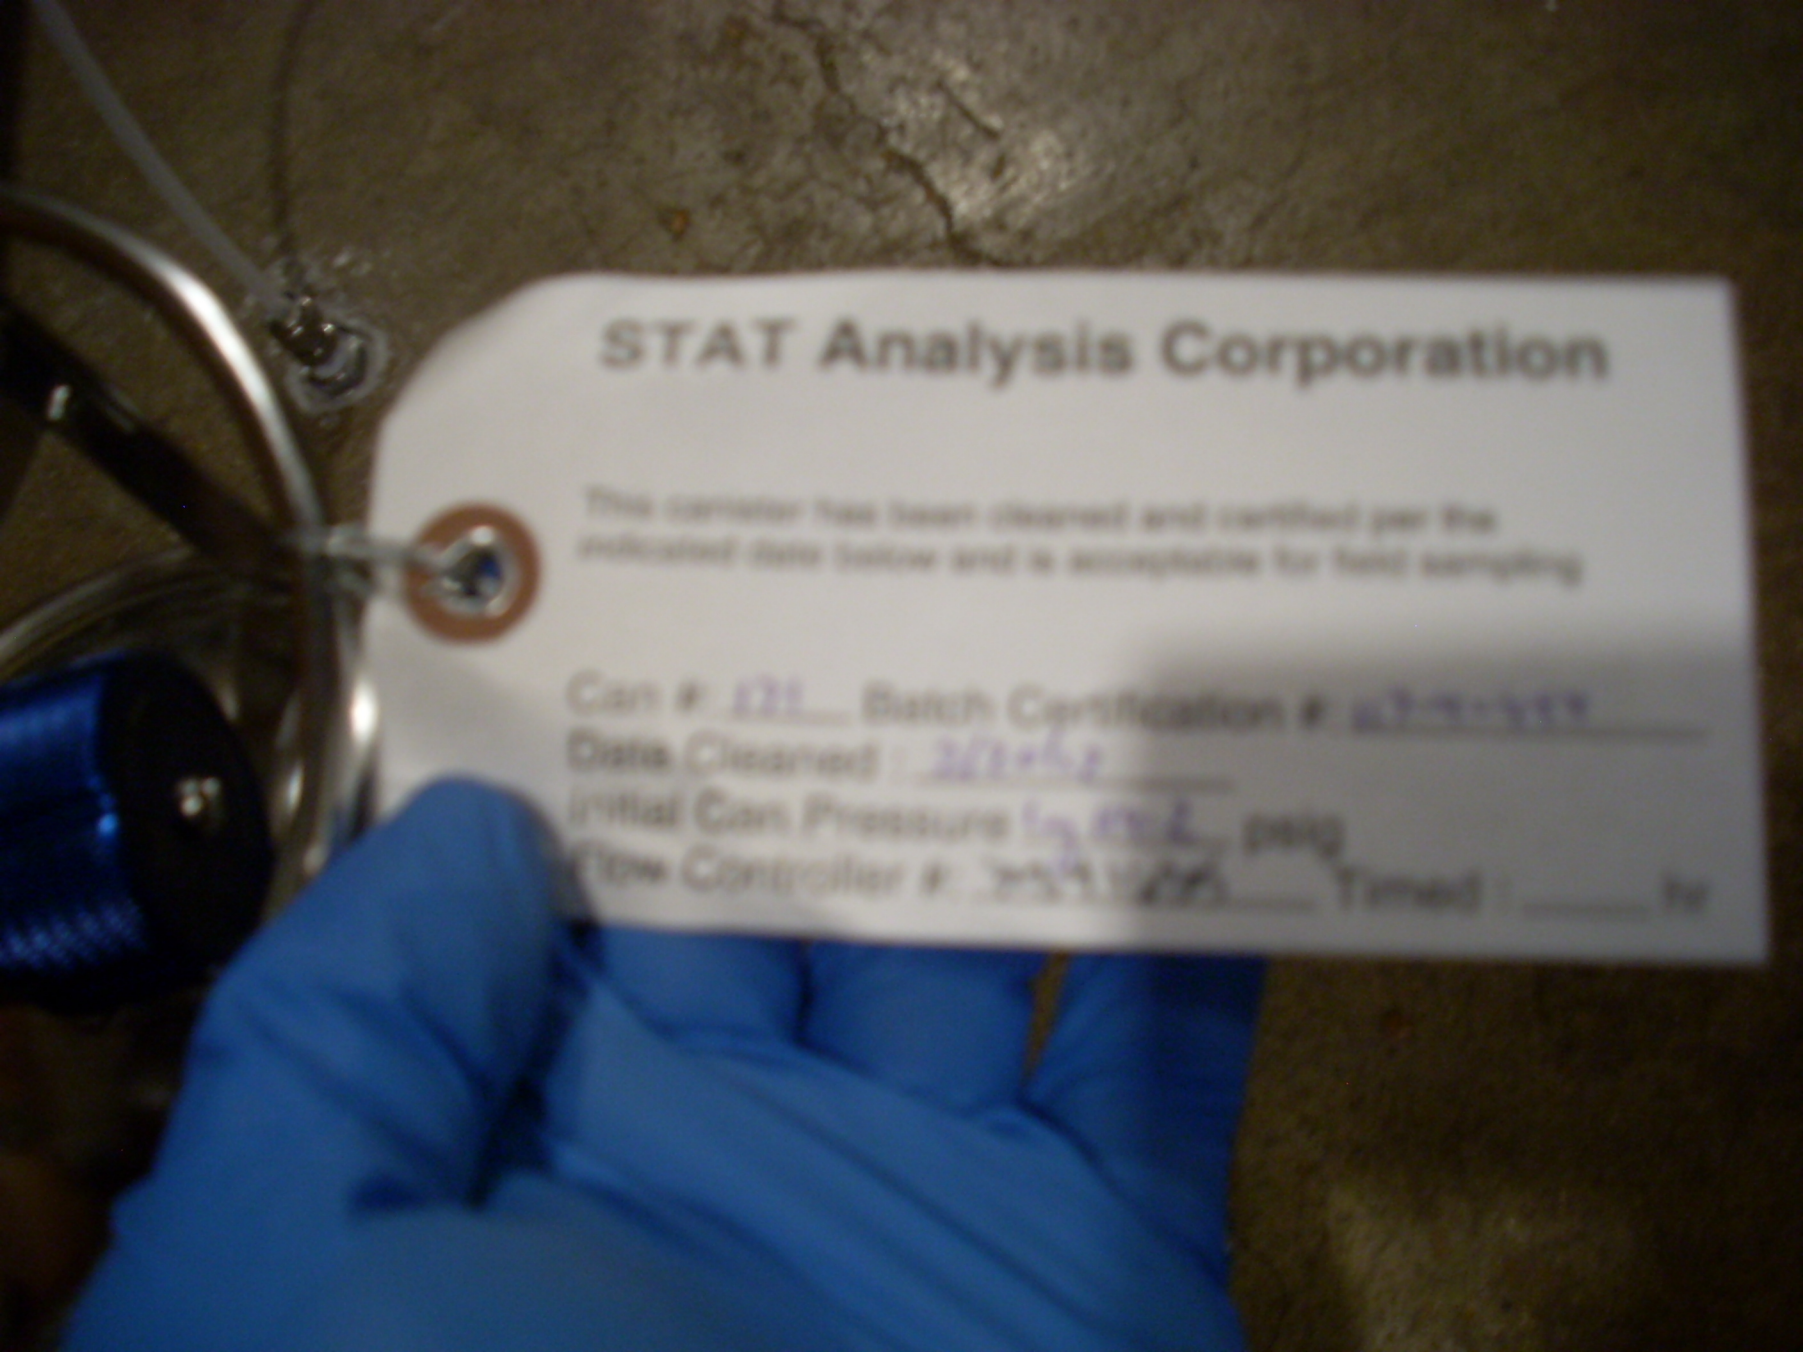
STAT Analysis Corporation
This canister has been cleaned and certified per the indicated date below and is acceptable for field sampling
Can #: 121 Batch Certification #:
Date Cleaned:
Initial Can Pressure psig
Flow Controller #: Timed: hr

TE 16-C

DEWALT
DEWALT
D CABINET
STAT Analysis Corporation

STAT Analysis Corporation

This canister has been cleaned and certified per the indicated data below and is acceptable for field sampling.

Can #: [illegible] Batch Certification #: [illegible]

Date Cleaned: [illegible]

Initial Can Pressure [illegible] psig

Flow Controller #: _____ Timed: _____ hr

Armstrong