TestAmerica
ANALYTICAL TESTING CORPORATION
17461Derian Ave. Suite 100 Irvine CA 92614 (949) 261-1022 FAX (949) 260-3297

QA/QC PACKAGE: LEVEL IV
PREPARED FOR: GPL LABORATORIES
LABORATORY NUMBER: IQG1460
PROJECT: OMEGA CHEMICAL OU-2 SSID-BC
OMEGA CHEMICAL 335392.FI.01

SAMPLED: 07/17/07

TestAmerica
ANALYTICAL TESTING CORPORATION

CASE NARRATIVE

Client:	GPL Laboratories	**Date Sampled:**	7/17/2007
Project:	Omega Chemical OU-2 SSID-BC Omega Chemical	**Date Received:**	7/17/2007
Lab:	IQG1460		

SAMPLE RECEIPT: Samples were received intact, on ice, and with chain of custody documentation. The sample temperature was measured at 5.6° C upon receipt at the laboratory.

HOLDING TIMES: All samples were analyzed within holding times.

PROBLEMS ENCOUNTERED: No problems were encountered.

QA/QC CRITERIA: There was no MS/MSD analyzed with EPA 1625C-CI Mod QC batch 7G19061 due to insufficient sample volume. See LCS/LCSD.

OBSERVATIONS: No significant observations were made.

SUBCONTRACTED: EPA 524.2 Mod analysis was performed at TestAmerica - Ontario, CA.

TestAmerica - Irvine, CA

Michele Chamberlin

Michele Chamberlin for Trevor Brenner
Client Services Manager
BB

17461 Derian Avenue. Suite 100 Irvine, CA 92614 (949) 261-1022 (949) 260-3297

The case narrative is an integral part of the report. This report shall not be reproduced, except in full, without written permission from TestAmerica.

TestAmerica
ANALYTICAL TESTING CORPORATION
17461 Derian Avenue. Suite 100, Irvine, CA 92614 (949) 261-1022 Fax:(949) 260-3297

LABORATORY REPORT

Prepared For: GPL Laboratories
7210-A Corporate Court
Frederick, MD 21703
Attention: Pat Huebschman

Project: Omega Chemical OU-2 SSID-BC
Omega Chemical

Sampled: 07/17/07
Received: 07/17/07
Issued: 07/26/07 17:02

NELAP #01108CA California ELAP#1197 CSDLAC #10256

The results listed within this Laboratory Report pertain only to the samples tested in the laboratory. The analyses contained in this report were performed in accordance with the applicable certifications as noted. All soil samples are reported on a wet weight basis unless otherwise noted in the report. This Laboratory Report is confidential and is intended for the sole use of TestAmerica and its client. This report shall not be reproduced, except in full, without written permission from TestAmerica. The Chain of Custody, 1 page, is included and is an integral part of this report.
This entire report was reviewed and approved for release.

SAMPLE CROSS REFERENCE

SUBCONTRACTED: Refer to the last page for specific subcontract laboratory information included in this report.

LABORATORY ID	CLIENT ID	MATRIX
IQG1460-01	OC2-MW8D-W-0-603	Water
IQG1460-02	OC2-MW8C-W-0-604	Water
IQG1460-03	OC2-MW8B-W-0-605	Water
IQG1460-04	OC2-MW8A-W-0-606	Water
IQG1460-05	OC2-MW12-W-0-607	Water
IQG1460-06	OC2-MW12-W-1-608	Water

Reviewed By:

TestAmerica - Irvine, CA

Trevor Brenner
Client Services Manager

TestAmerica
ANALYTICAL TESTING CORPORATION
17461Derian Ave. Suite 100 Irvine CA 92614 (949) 261-1022 FAX (949) 260-3297

QA/QC PACKAGE: LEVEL IV
PREPARED FOR: GPL LABORATORIES
LABORATORY NUMBER: IQG1460
PROJECT: OMEGA CHEMICAL OU-2 SSID-BC
OMEGA CHEMICAL 335392.FI.01

CHAIN OF CUSTODY FORM

17461 Derian Ave., #100, Irvine, CA 92614 (949) 261-1022 FAX (949) 260-3299
1014 E. Cooley Dr., Suite A, Colton, CA 92324 (909) 370-4687 FAX (909) 370-1046
9830 South 51st St., Suite B-12D, Phoenix, AZ 85044 (480) 785-0043 FAX (480) 785-0851
2520 E. Sunset Rd. #3, Las Vegas, NV 89120 (702) 796-3620 FAX (702) 798-3628

TestAmerica
ANALYTICAL TESTING CORPORATION

CHAIN OF CUSTODY FORM

IQG1460

Page 1 of 1

Client Name/Address: CH2MHILL, 3 Hutton Centre Drive, Suite 200, Santa Ana, CA 92707

Project/PO Number: Omega Chemical 335392.FI.01

Project Manager: Dan Jablonski

Phone Number: (213) 228-8271

Sampler: Mike Palm

Fax Number:

Sample Description	Sample Matrix	Container Type	# of Cont.	Sampling Date	Sampling Time	Preservatives	NDMA	1,2,3-TCP	Hex Cr.							Special Instructions
OC2-MW8D-W-0-603	BW	VAR	6	7.17.07	0812	VAR	X	X	X							
OC2-MW8C-W-0-604			6		0900		X	X	X							
OC2-MW8B-W-0-605			6		0935		X	X	X							
OC2-MW8A-W-0-606			6		1020		X	X	X							
OC2-MW12-W-0-607			6		1130		X	X	X							
OC2-MW12-W-1-608			6		1200		X	X	X							
																HE 7-17-07 1400

Relinquished By:	Date/Time:	Received By:	Date/Time:	Turnaround Time: (Check)
[signature]	7.17.07 1330	[signature]	7/17/07 1330	same day ____ 72 hours ____
[signature]	7/17/07 1420	Received By:	Date/Time:	24 hours ____ 5 days ____
				48 hours ____ normal X
Relinquished By:	Date/Time:	Received in Lab By: [signature]	Date/Time: 7-17-07 1420	Sample Integrity: (Check) intact + on ice + 5.6C

Note: By relinquishing samples to Test America, client agrees to pay for the services requested on this chain of custody form and any additional analyses performed on this project. Payment for services is due within 30 days from the date of invoice. Sample(s) will be disposed of after 30 days.

SUBCONTRACT ORDER

TestAmerica - Irvine, CA

IQG1460

SENDING LABORATORY:

TestAmerica - Irvine, CA
17461 Derian Avenue. Suite 100
Irvine, CA 92614
Phone: (949) 261-1022
Fax: (949) 260-3297
Project Manager: Trevor Brenner
Client: GPL Laboratories

RECEIVING LABORATORY:

TestAmerica - Ontario, CA
1014 E. Cooley Drive, Suite AB
Colton, CA 92324
Phone :(909) 370-4667
Fax: (909) 370-1046
Project Location: California
Receipt Temperature:_____°C Ice: Y / N

Analysis	Due	Expires	Interlab	Surch	Comments
Sample ID: IQG1460-01	**Water**		Sampled: **07/17/07 08:12**		
524.2 CA 123-TCP (SIM) DN	07/26/07 12:00	07/31/07 08:12	$110.00	0%	
Level 4 + EDD-Colton - Out	07/26/07 12:00	08/14/07 08:12	$0.00	0%	
Containers Supplied:					
40 mL VOA w/Ascorbic acid (A)	40 mL VOA w/Ascorbic acid (B)	40 mL VOA w/Ascorbic acid (C)			
Sample ID: IQG1460-02	**Water**		Sampled: **07/17/07 09:00**		
524.2 CA 123-TCP (SIM) DN	07/26/07 12:00	07/31/07 09:00	$110.00	0%	
Level 4 + EDD-Colton - Out	07/26/07 12:00	08/14/07 09:00	$0.00	0%	
Containers Supplied:					
40 mL VOA w/Ascorbic acid (A)	40 mL VOA w/Ascorbic acid (B)	40 mL VOA w/Ascorbic acid (C)			
Sample ID: IQG1460-03	**Water**		Sampled: **07/17/07 09:35**		
524.2 CA 123-TCP (SIM) DN	07/26/07 12:00	07/31/07 09:35	$110.00	0%	
Level 4 + EDD-Colton - Out	07/26/07 12:00	08/14/07 09:35	$0.00	0%	
Containers Supplied:					
40 mL VOA w/Ascorbic acid (A)	40 mL VOA w/Ascorbic acid (B)	40 mL VOA w/Ascorbic acid (C)			
Sample ID: IQG1460-04	**Water**		Sampled: **07/17/07 10:20**		
524.2 CA 123-TCP (SIM) DN	07/26/07 12:00	07/31/07 10:20	$110.00	0%	
Level 4 + EDD-Colton - Out	07/26/07 12:00	08/14/07 10:20	$0.00	0%	
Containers Supplied:					
40 mL VOA w/Ascorbic acid (A)	40 mL VOA w/Ascorbic acid (B)	40 mL VOA w/Ascorbic acid (C)			
Sample ID: IQG1460-05	**Water**		Sampled: **07/17/07 11:30**		
524.2 CA 123-TCP (SIM) DN	07/26/07 12:00	07/31/07 11:30	$110.00	0%	
Level 4 + EDD-Colton - Out	07/26/07 12:00	08/14/07 11:30	$0.00	0%	
Containers Supplied:					
40 mL VOA w/Ascorbic acid (A)	40 mL VOA w/Ascorbic acid (B)	40 mL VOA w/Ascorbic acid (C)			

Released By	Date/Time	Received By	Date/Time
Released By	Date/Time	Received By	Date/Time

SUBCONTRACT ORDER

TestAmerica - Irvine, CA

IQG1460

Analysis	Due	Expires	Interlab	Surch	Comments
Sample ID: IQG1460-06	**Water**		Sampled: **07/17/07 12:00**		
524.2 CA 123-TCP (SIM) DN	07/26/07 12:00	07/31/07 12:00	$110.00	0%	
Level 4 + EDD-Colton - Out	07/26/07 12:00	08/14/07 12:00	$0.00	0%	
Containers Supplied:					
40 mL VOA w/Ascorbic acid (A)	40 mL VOA w/Ascorbic acid (B)	40 mL VOA w/Ascorbic acid (C)			

TestAmerica
ANALYTICAL TESTING CORPORATION
17461Derian Ave. Suite 100 Irvine CA 92614 (949) 261-1022 FAX (949) 260-3297

QA/QC PACKAGE: LEVEL IV
PREPARED FOR: GPL LABORATORIES
LABORATORY NUMBER: IQG1460
PROJECT: OMEGA CHEMICAL OU-2 SSID-BC
OMEGA CHEMICAL 335392.FI.01

ANALYTICAL REPORT

TestAmerica
ANALYTICAL TESTING CORPORATION
17461 Derian Avenue. Suite 100, Irvine, CA 92614 (949) 261-1022 Fax:(949) 260-3297

GPL Laboratories
7210-A Corporate Court
Frederick, MD 21703
Attention: Pat Huebschman

Project ID: Omega Chemical OU-2 SSID-BC
Omega Chemical
Report Number: IQG1460

Sampled: 07/17/07
Received: 07/17/07

SEMI-VOL ORGANICS by GC/MS-CHEMICAL IONIZATION (EPA 3520C/1625C-CI MOD)

Analyte	Method	Batch	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IQG1460-01 (OC2-MW8D-W-0-603 - Water)								
Reporting Units: ug/l								
N-Nitrosodimethylamine	EPA 1625C-CI Mod	7G19061	0.0020	ND	0.98	7/19/2007	7/20/2007	
Sample ID: IQG1460-02 (OC2-MW8C-W-0-604 - Water)								
Reporting Units: ug/l								
N-Nitrosodimethylamine	EPA 1625C-CI Mod	7G19061	0.0019	ND	0.966	7/19/2007	7/20/2007	
Sample ID: IQG1460-03 (OC2-MW8B-W-0-605 - Water)								
Reporting Units: ug/l								
N-Nitrosodimethylamine	EPA 1625C-CI Mod	7G19061	0.0019	ND	0.952	7/19/2007	7/20/2007	
Sample ID: IQG1460-04 (OC2-MW8A-W-0-606 - Water)								
Reporting Units: ug/l								
N-Nitrosodimethylamine	EPA 1625C-CI Mod	7G19061	0.0019	ND	0.966	7/19/2007	7/20/2007	
Sample ID: IQG1460-05 (OC2-MW12-W-0-607 - Water)								
Reporting Units: ug/l								
N-Nitrosodimethylamine	EPA 1625C-CI Mod	7G19061	0.0019	**0.0022**	0.952	7/19/2007	7/20/2007	
Sample ID: IQG1460-06 (OC2-MW12-W-1-608 - Water)								
Reporting Units: ug/l								
N-Nitrosodimethylamine	EPA 1625C-CI Mod	7G19061	0.0019	ND	0.943	7/19/2007	7/20/2007	

TestAmerica - Irvine, CA

Trevor Brenner
Client Services Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

TestAmerica
ANALYTICAL TESTING CORPORATION
17461 Derian Avenue. Suite 100, Irvine, CA 92614 (949) 261-1022 Fax:(949) 260-3297

GPL Laboratories
7210-A Corporate Court
Frederick, MD 21703
Attention: Pat Huebschman

Project ID: Omega Chemical OU-2 SSID-BC
Omega Chemical
Report Number: IQG1460

Sampled: 07/17/07
Received: 07/17/07

INORGANICS

Analyte	Method	Batch	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: IQG1460-01 (OC2-MW8D-W-0-603 - Water)								
Reporting Units: mg/l								
Chromium VI	EPA 218.6	7G17075	0.00030	**0.0020**	1	7/17/2007	7/17/2007	
Sample ID: IQG1460-02 (OC2-MW8C-W-0-604 - Water)								
Reporting Units: mg/l								
Chromium VI	EPA 218.6	7G17075	0.00030	**0.0056**	1	7/17/2007	7/17/2007	
Sample ID: IQG1460-03 (OC2-MW8B-W-0-605 - Water)								
Reporting Units: mg/l								
Chromium VI	EPA 218.6	7G17075	0.00030	**0.0082**	1	7/17/2007	7/17/2007	
Sample ID: IQG1460-04 (OC2-MW8A-W-0-606 - Water)								
Reporting Units: mg/l								
Chromium VI	EPA 218.6	7G17075	0.0030	**0.20**	10	7/17/2007	7/17/2007	
Sample ID: IQG1460-05 (OC2-MW12-W-0-607 - Water)								
Reporting Units: mg/l								
Chromium VI	EPA 218.6	7G17075	0.00030	**0.00099**	1	7/17/2007	7/17/2007	
Sample ID: IQG1460-06 (OC2-MW12-W-1-608 - Water)								
Reporting Units: mg/l								
Chromium VI	EPA 218.6	7G17075	0.00030	**0.0017**	1	7/17/2007	7/17/2007	

TestAmerica - Irvine, CA

Trevor Brenner
Client Services Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

TestAmerica
ANALYTICAL TESTING CORPORATION
17461 Derian Avenue. Suite 100, Irvine, CA 92614 (949) 261-1022 Fax:(949) 260-3297

GPL Laboratories
7210-A Corporate Court
Frederick, MD 21703
Attention: Pat Huebschman

Project ID: Omega Chemical OU-2 SSID-BC
Omega Chemical
Report Number: IQG1460

Sampled: 07/17/07
Received: 07/17/07

SHORT HOLD TIME DETAIL REPORT

	Hold Time (in days)	Date/Time Sampled	Date/Time Received	Date/Time Extracted	Date/Time Analyzed
Sample ID: OC2-MW8D-W-0-603 (IQG1460-01) - Water					
EPA 218.6	1	07/17/2007 08:12	07/17/2007 14:20	07/17/2007 16:40	07/17/2007 17:25
Sample ID: OC2-MW8C-W-0-604 (IQG1460-02) - Water					
EPA 218.6	1	07/17/2007 09:00	07/17/2007 14:20	07/17/2007 16:40	07/17/2007 17:36
Sample ID: OC2-MW8B-W-0-605 (IQG1460-03) - Water					
EPA 218.6	1	07/17/2007 09:35	07/17/2007 14:20	07/17/2007 16:40	07/17/2007 17:47
Sample ID: OC2-MW8A-W-0-606 (IQG1460-04) - Water					
EPA 218.6	1	07/17/2007 10:20	07/17/2007 14:20	07/17/2007 16:40	07/17/2007 18:32
Sample ID: OC2-MW12-W-0-607 (IQG1460-05) - Water					
EPA 218.6	1	07/17/2007 11:30	07/17/2007 14:20	07/17/2007 16:40	07/17/2007 18:10
Sample ID: OC2-MW12-W-1-608 (IQG1460-06) - Water					
EPA 218.6	1	07/17/2007 12:00	07/17/2007 14:20	07/17/2007 16:40	07/17/2007 18:21

TestAmerica - Irvine, CA

Trevor Brenner
Client Services Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

TestAmerica
ANALYTICAL TESTING CORPORATION
17461Derian Ave. Suite 100 Irvine CA 92614 (949) 261-1022 FAX (949) 260-3297

QA/QC PACKAGE: LEVEL IV
PREPARED FOR: GPL LABORATORIES
LABORATORY NUMBER: IQG1460
PROJECT: OMEGA CHEMICAL OU-2 SSID-BC
OMEGA CHEMICAL 335392.FI.01

QUALITY CONTROL SUMMARY

- METHOD BLANKS
- MS/MSD DATA REPORTS
- LCS DATA REPORTS

TestAmerica
ANALYTICAL TESTING CORPORATION
17461 Derian Avenue. Suite 100, Irvine, CA 92614 (949) 261-1022 Fax:(949) 260-3297

GPL Laboratories	Project ID:	Omega Chemical OU-2 SSID-BC	
7210-A Corporate Court		Omega Chemical	Sampled: 07/17/07
Frederick, MD 21703	Report Number:	IQG1460	Received: 07/17/07
Attention: Pat Huebschman			

METHOD BLANK/QC DATA

SEMI-VOL ORGANICS by GC/MS-CHEMICAL IONIZATION (EPA 3520C/1625C-CI MOD)

Analyte	Result	Reporting Limit	Units	Spike Level	Source Result	%REC	%REC Limits	RPD	RPD Limit	Data Qualifiers
Batch: 7G19061 Extracted: 07/19/07										
Blank Analyzed: 07/20/2007 (7G19061-BLK1)										
N-Nitrosodimethylamine	ND	0.0020	ug/l							
LCS Analyzed: 07/20/2007 (7G19061-BS1)										**MNR1**
N-Nitrosodimethylamine	0.00944	0.0020	ug/l	0.0100		94	60-140			
LCS Analyzed: 07/20/2007 (7G19061-BS2)										
N-Nitrosodimethylamine	0.00206	0.0020	ug/l	0.00200		103	60-140			
LCS Dup Analyzed: 07/20/2007 (7G19061-BSD1)										
N-Nitrosodimethylamine	0.00960	0.0020	ug/l	0.0100		96	60-140	2	30	

TestAmerica - Irvine, CA

Trevor Brenner
Client Services Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

TestAmerica
ANALYTICAL TESTING CORPORATION
17461 Derian Avenue. Suite 100, Irvine, CA 92614 (949) 261-1022 Fax:(949) 260-3297

GPL Laboratories	Project ID: Omega Chemical OU-2 SSID-BC	
7210-A Corporate Court	Omega Chemical	Sampled: 07/17/07
Frederick, MD 21703	Report Number: IQG1460	Received: 07/17/07
Attention: Pat Huebschman		

METHOD BLANK/QC DATA

INORGANICS

Analyte	Result	Reporting Limit	Units	Spike Level	Source Result	%REC	%REC Limits	RPD	RPD Limit	Data Qualifiers
Batch: 7G17075 Extracted: 07/17/07										
Blank Analyzed: 07/17/2007 (7G17075-BLK1)										
Chromium VI	ND	0.00030	mg/l							
LCS Analyzed: 07/17/2007 (7G17075-BS1)										
Chromium VI	0.0458	0.00030	mg/l	0.0500		92	90-110			
Matrix Spike Analyzed: 07/17/2007 (7G17075-MS1)					**Source: IQG1425-03**					
Chromium VI	0.0520	0.00030	mg/l	0.0500	ND	104	90-110			
Matrix Spike Dup Analyzed: 07/17/2007 (7G17075-MSD1)					**Source: IQG1425-03**					
Chromium VI	0.0519	0.00030	mg/l	0.0500	ND	104	90-110	0	10	

TestAmerica - Irvine, CA

Trevor Brenner
Client Services Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

TestAmerica
ANALYTICAL TESTING CORPORATION
17461 Derian Avenue. Suite 100, Irvine, CA 92614 (949) 261-1022 Fax:(949) 260-3297

GPL Laboratories	Project ID: Omega Chemical OU-2 SSID-BC	
7210-A Corporate Court	Omega Chemical	Sampled: 07/17/07
Frederick, MD 21703	Report Number: IQG1460	Received: 07/17/07
Attention: Pat Huebschman		

DATA QUALIFIERS AND DEFINITIONS

MNR1 There was no MS/MSD analyzed with this batch due to insufficient sample volume. See Blank Spike/Blank Spike Duplicate.

ND Analyte NOT DETECTED at or above the reporting limit or MDL, if MDL is specified.

RPD Relative Percent Difference

TestAmerica - Irvine, CA

Trevor Brenner
Client Services Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

TestAmerica
ANALYTICAL TESTING CORPORATION
17461 Derian Avenue. Suite 100, Irvine, CA 92614 (949) 261-1022 Fax:(949) 260-3297

GPL Laboratories	Project ID:	Omega Chemical OU-2 SSID-BC	
7210-A Corporate Court		Omega Chemical	Sampled: 07/17/07
Frederick, MD 21703	Report Number:	IQG1460	Received: 07/17/07
Attention: Pat Huebschman			

Certification Summary

TestAmerica - Irvine, CA

Method	Matrix	Nelac	California
EPA 1625C-CI Mod	Water		
EPA 218.6	Water	X	X

Nevada and NELAP provide analyte specific accreditations. Analyte specific information for TestAmerica may be obtained by contacting the laboratory or visiting our website at www.testamericainc.com

Subcontracted Laboratories

TestAmerica - Ontario, CA *California Cert #1169, Arizona Cert #AZ0062, Nevada Cert #CA-242*
1014 E. Cooley Drive, Suite AB - Colton, CA 92324
Analysis Performed: 524.2 CA 123-TCP (SIM) DMAC
Samples: IQG1460-01, IQG1460-02, IQG1460-03, IQG1460-04, IQG1460-05, IQG1460-06

TestAmerica - Irvine, CA

Trevor Brenner
Client Services Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

TestAmerica
ANALYTICAL TESTING CORPORATION
17461Derian Ave. Suite 100 Irvine CA 92614 (949) 261-1022 FAX (949) 260-3297

QA/QC PACKAGE: LEVEL IV
PREPARED FOR: GPL LABORATORIES
LABORATORY NUMBER: IQG1460
PROJECT: OMEGA CHEMICAL OU-2 SSID-BC
OMEGA CHEMICAL 335392.FI.01

EPA 1625C-CI MOD. LABORATORY RAW DATA

- INITIAL CALIBRATION
- CONTINUING CALIBRATION
- EXTRACTION LOG
- RUN LOG
- TUNE REPORT
- QUANTITATION REPORTS
- CHROMATOGRAMS

GC/MS DAILY LOG SUMMARY

DATE: 06-14-07 DATAFILE C:\MSDCHEM\1 \DATA\ 07JUN14

ANALYST: LB GCM #37 EPA METHOD: n-Nitrosamines-1625

#	SAMPLE NAME	Dil	FILENAME	S/W	CLIENT	Prep	Batch #	Posted	Rev'd	Comments
1	10 ppb ICV STANDARD	***	NMA010	***	*****	KS ISarea:	ICAL	updated Water 6/19/07	6/19/07	#7060221
2	1 ppb STD ICAL	–	001	↓				↓	↓	218
3	2 ppb	–	002						RR	219
4	5 ppb	–	005					updated 6/19/07	6/19/07	220
5	20 ppb	–	020							222
6	50 ppb	–	050							223
7	100 ppb	–	100							224
8	150 ppb	–	150							225
9	200 ppb	–	200							226
10	10 ppb LCS	–	MLCS010							#7060264
11	2 ppb STD ICAL	–	MMA002A	↓				RR		#7060219
12		–	NMA002B					updated 6/19/07	6/19/07	7060219
13	1625C (mod)	N-	Nitrosamines							
14	C7F14NW									
15										
16										
17										
18										
19										
20										
21										
22										
23										
24										
25										
26										
27										
28										
29										
30										

Standard Code: See above

Methylene Chloride Lot#: See above

GCMS INITIAL CALIBRATION CHECK LIST
N-Nitrosamines by 1625C Modified

2nd Level Review:	[illegible]	Analyst:	[illegible]
Date:	6/19/07	Analysis Date:	6/14/07
		GCMS #:	37

2nd Level Rev	Analyst Rev	
		Calibration :
/	✓	• Minimum 5-point calibration – lowest standard at RL
/	✓	• RSD of RF: <= ±20 %.
		LCS check :
/	✓	• After initial calibration
		• 80% recovery met
		Datafile:
/	✓	Print out calibration curve (include software or calculator-generated r^2 coefficient)
		Generate:
/	✓	• Response Factor summary sheet
/	✓	• List compound summary sheet
/	✓	• List compound history summary sheet
/	✓	Print all levels with area count for all compounds
		Check all levels for:
/	✓	• Manual integration
/	✓	• Print data before and after integration
/	✓	• Transcription errors
/	✓	Mint Miner Check
/	/	Corrective Action Report attached (if applicable)

Comments:

GC/MS QA-QC Check Report

Tune File : C:\MSDCHEM\1\DATA\07JUN14\NNA010.D
Tune Time : 14 Jun 2007 8:50 am

Daily Calibration File : C:\MSDCHEM\1\DATA\07JUN14\NNA010.D

File	Sample	Internal Standard Responses		
		2812	5388	4883
NLCS010.D	10ppb LC	2820	5489	4947
NNA001.D	1ppb Std	2914	5557	4982
NNA002B.D	2ppb Std	2696	5345	5002
NNA005.D	5ppb Std	3006	5992	5087
NNA020.D	20ppb St	2991	5836	5092
NNA050.D	50ppb St	3015	5896	5432
NNA100.D	100ppb S	2989	5837	5188
NNA150.D	150ppb S	3079	5791	5290
NNA200.D	200ppb S	3031	5900	5851

t - fails 12hr time check * - fails criteria

Created: Thu Jun 14 18:46:48 2007 gcms37

RESPONSE FACTOR REPORT

gcms37

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration

Calibration File
1 =NNA001.D 2 =NNA002B.D 5 =NNA005.D 10 =NNA010.D 20 =NNA020.D
50 =NNA050.D 100 =NNA100.D 150 =NNA150.D 200 =NNA200.D

	COMPOUND	1	2	5	10	20	50	100	150	200	AVG	%RSD
I	NDMA-D6	ISTD										
T	NDMA	1.970	2.029	1.987	2.112	1.939	1.966	2.029	1.955	2.030	2.002	2.68
I	NDEA-D10	ISTD										
T	NDEA	1.128	1.088	1.056	1.130	1.026	1.034	1.066	1.051	1.068	1.072	3.47
I	NDPA-D14	ISTD										
T	NDPA		0.905	0.845	0.938	0.748	0.736	0.777	0.743	0.738	0.804	10.11
T	NPYR		0.640	0.699	0.823	0.728	0.809	0.934	0.901	0.868	0.800	12.90

(#) = Out of Range

C7F14NW.M Thu Jun 14 16:47:18 2007

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA010.D Vial: 1
Acq On : 14 Jun 2007 8:50 am Operator: DF/AI
Sample : 10ppb Std.# 7060221 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:25 2007 Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration
DataAcq Meth : C7E29NWA

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) NDMA-D6	10.90	81	2812	10.00 PPB	0.00
3) NDEA-D10	13.37	113	5388	10.00 PPB	0.00
5) NDPA-D14	15.81	145	4883	10.00 PPB	0.00
Target Compounds					**Qvalue**
2) NDMA	10.83	92	5938	10.53 PPB	100
4) NDEA	13.32	120	6086	10.61 PPB	99
6) NDPA	15.77	148	4580	11.14 PPB	99
7) NPYR	17.20	118	4021	10.17 PPB	98

(#) = qualifier out of range (m) = manual integration
NNA010.D C7F14NW.M Thu Jun 14 16:25:33 2007 Page 1

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA010.D Vial: 1
Acq On : 14 Jun 2007 8:50 am Operator: DF/AI
Sample : 10ppb Std.# 7060221 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:25 2007 Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration

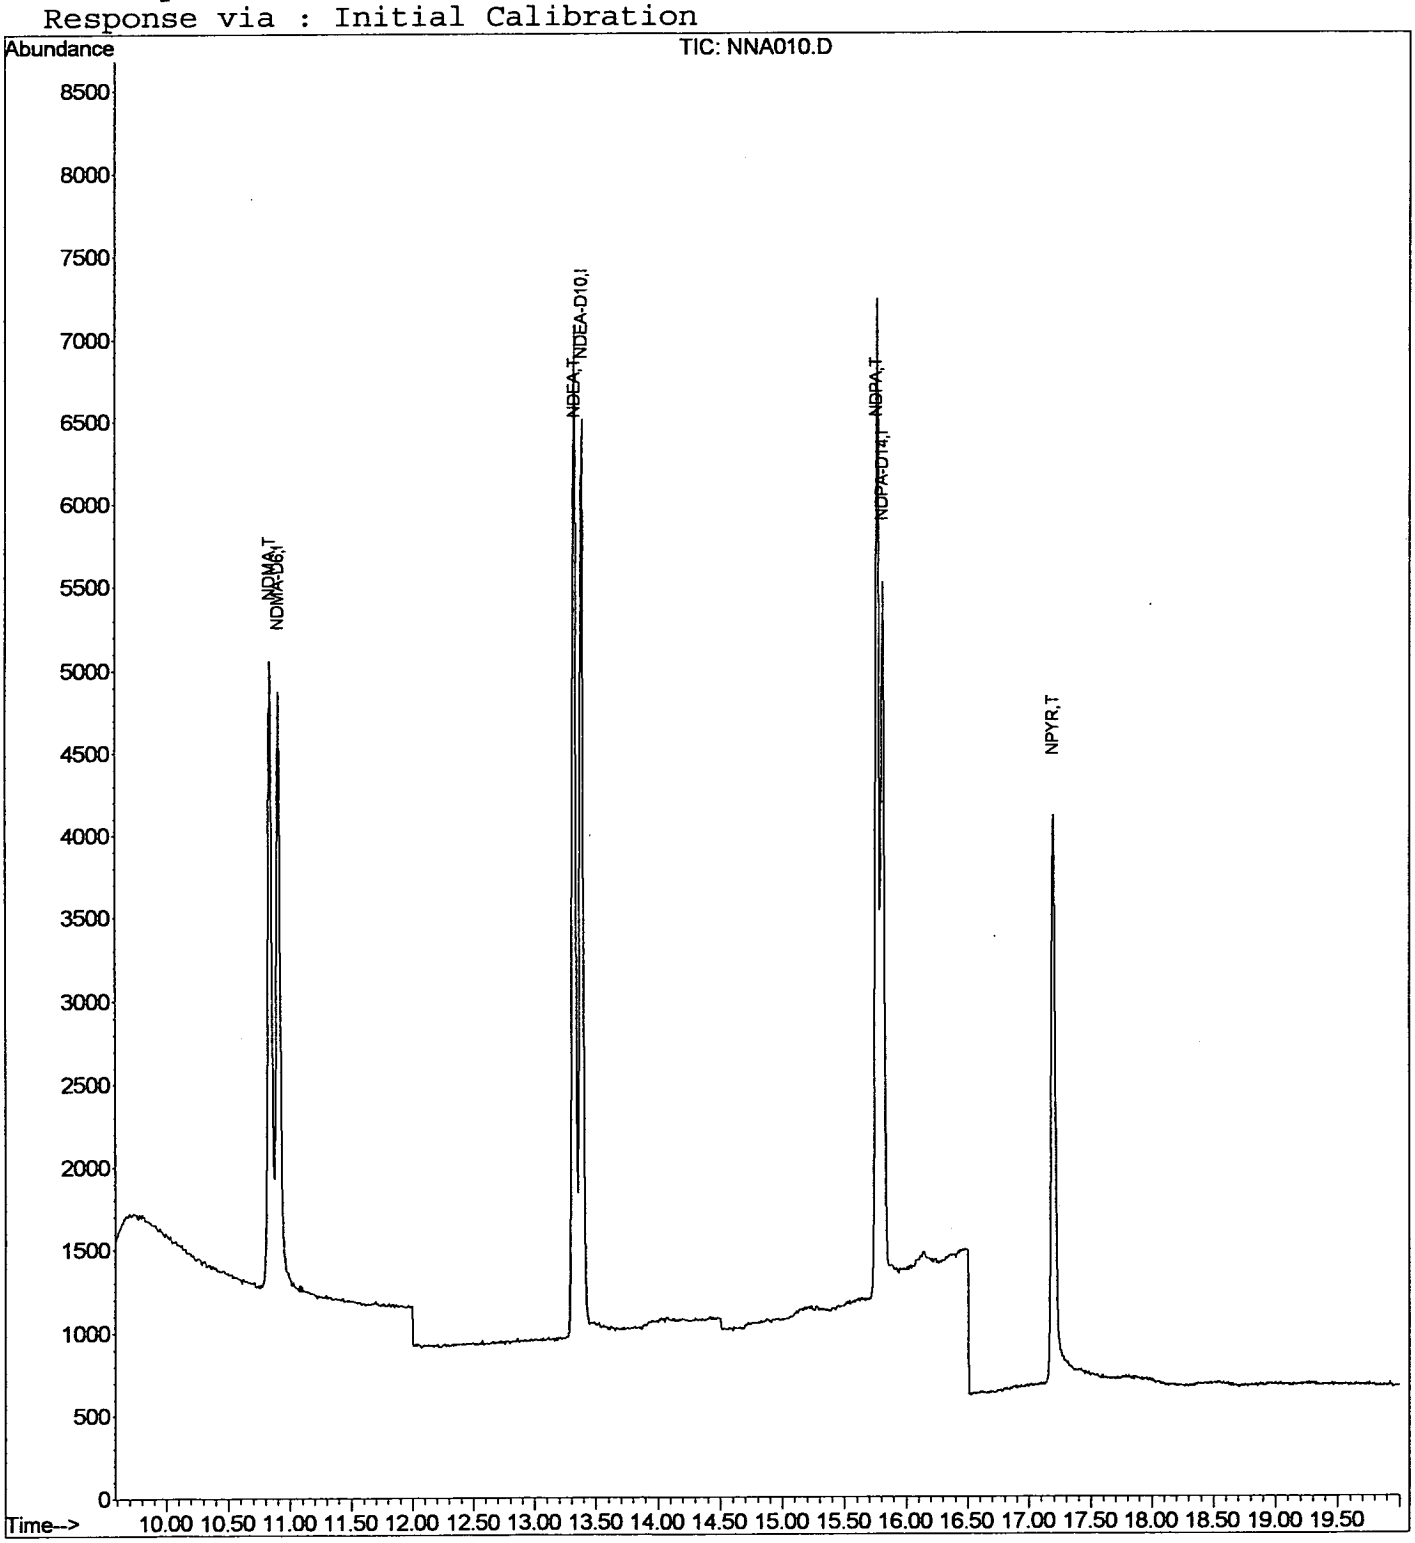

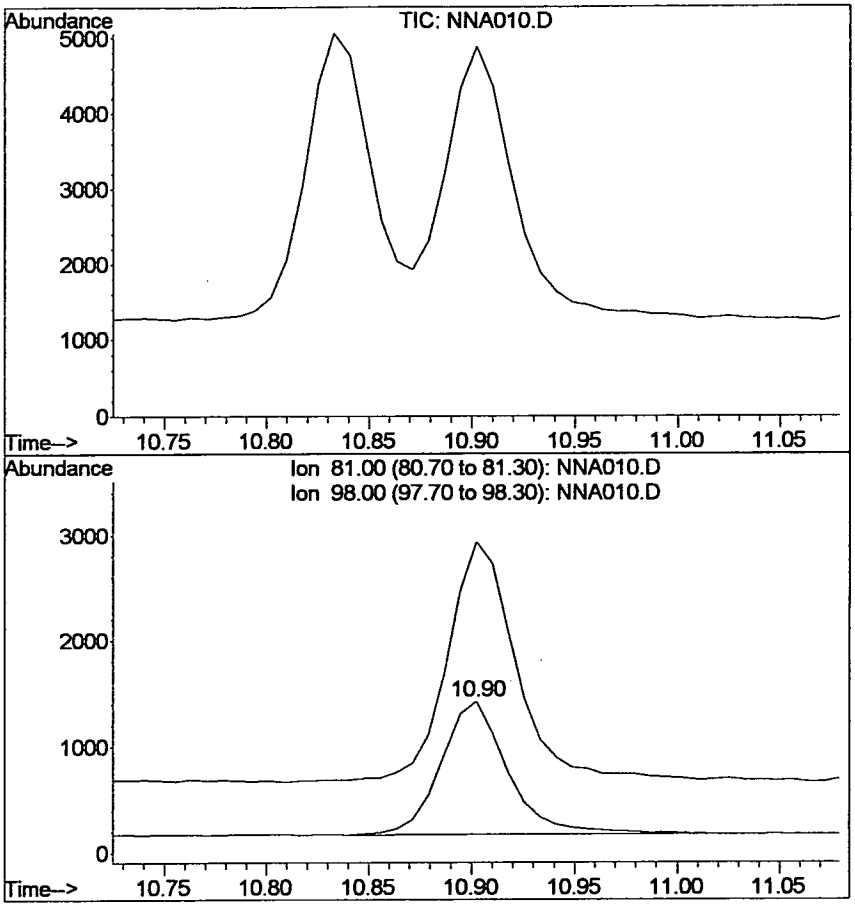

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.90 min Scan# 172
Delta R.T. 0.00 min
Lab File: NNA010.D
Acq: 14 Jun 2007 8:50 am

Tgt Ion: 81 Resp: 2812

Ion	Ratio	Lower	Upper
81	100		
98	184.5	144.1	224.1

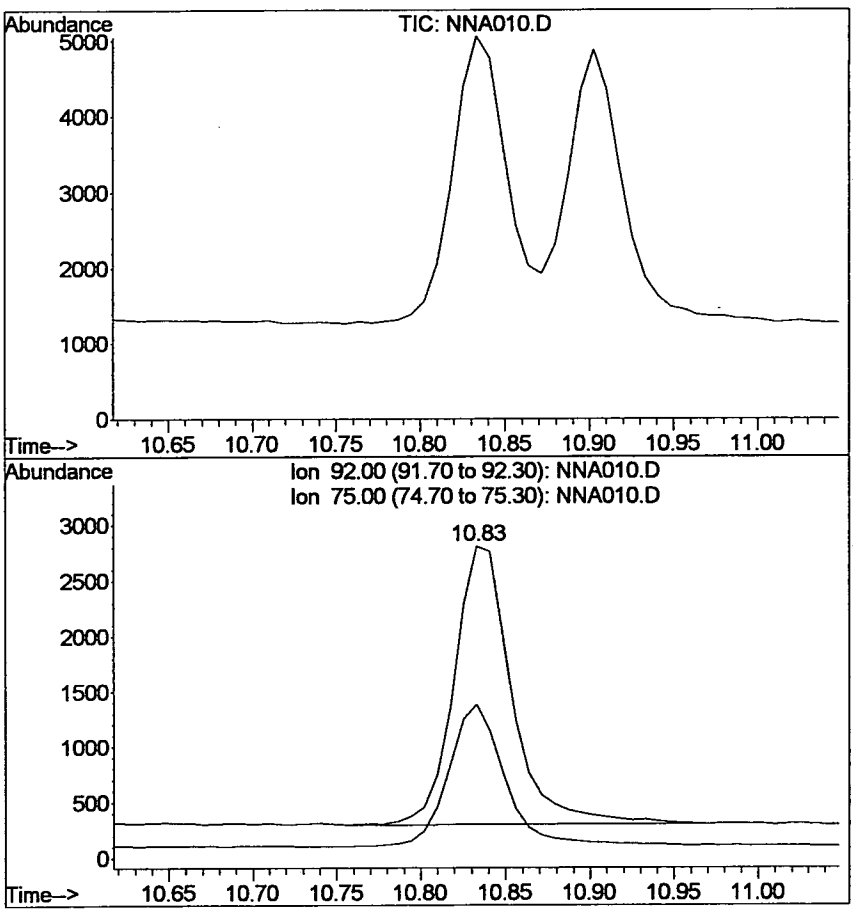

#2
NDMA
Concen: 10.53 PPB
RT: 10.83 min Scan# 163
Delta R.T. 0.00 min
Lab File: NNA010.D
Acq: 14 Jun 2007 8:50 am

Tgt Ion: 92 Resp: 5938

Ion	Ratio	Lower	Upper
92	100		
75	48.9	31.8	66.0

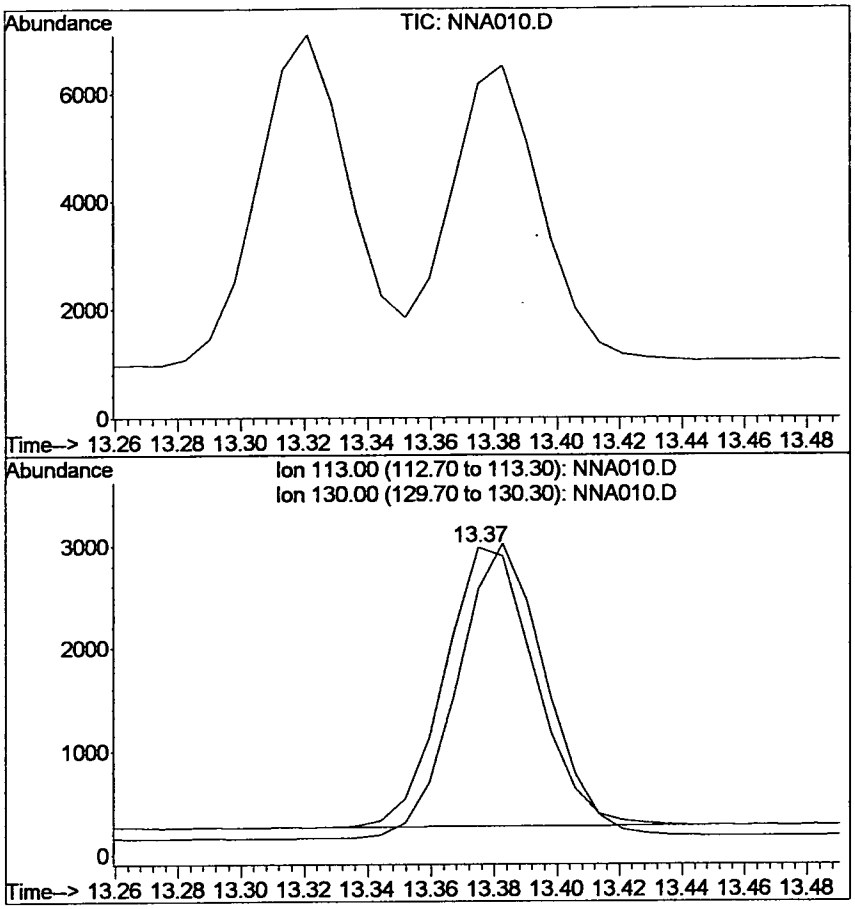

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.37 min Scan# 493
Delta R.T. 0.00 min
Lab File: NNA010.D
Acq: 14 Jun 2007 8:50 am

Tgt Ion:113 Resp: 5388

Ion	Ratio	Lower	Upper
113	100		
130	101.6	67.1	137.1

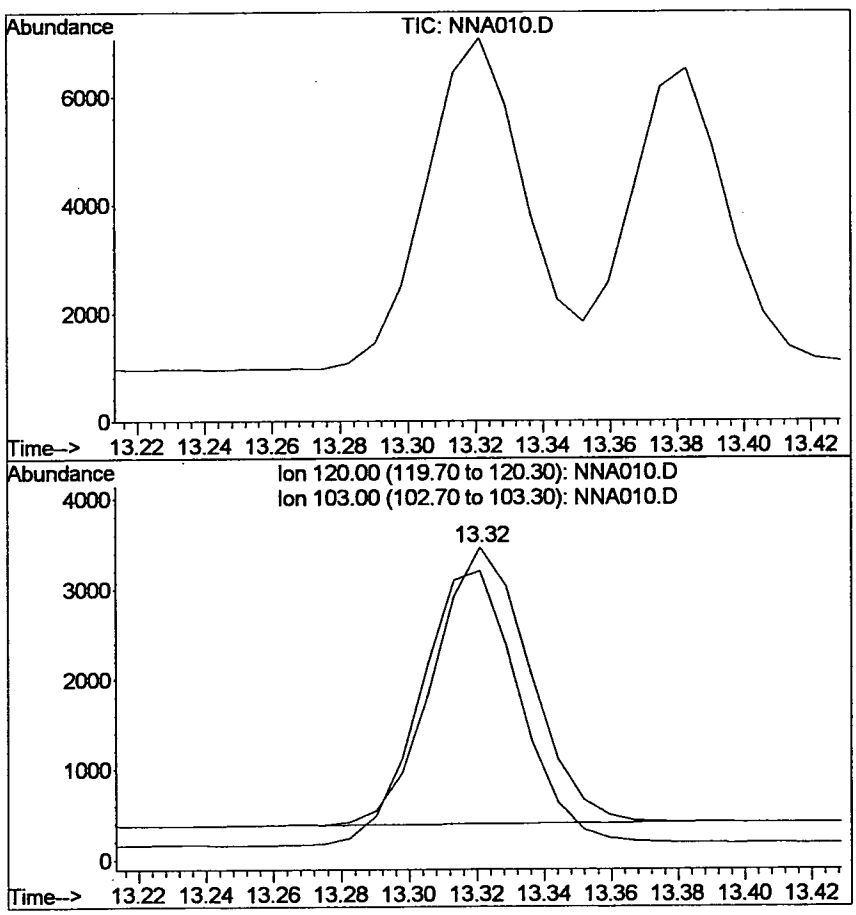

#4
NDEA
Concen: 10.61 PPB
RT: 13.32 min Scan# 486
Delta R.T. 0.00 min
Lab File: NNA010.D
Acq: 14 Jun 2007 8:50 am

Tgt Ion:120 Resp: 6086

Ion	Ratio	Lower	Upper
120	100		
103	101.4	65.3	135.5

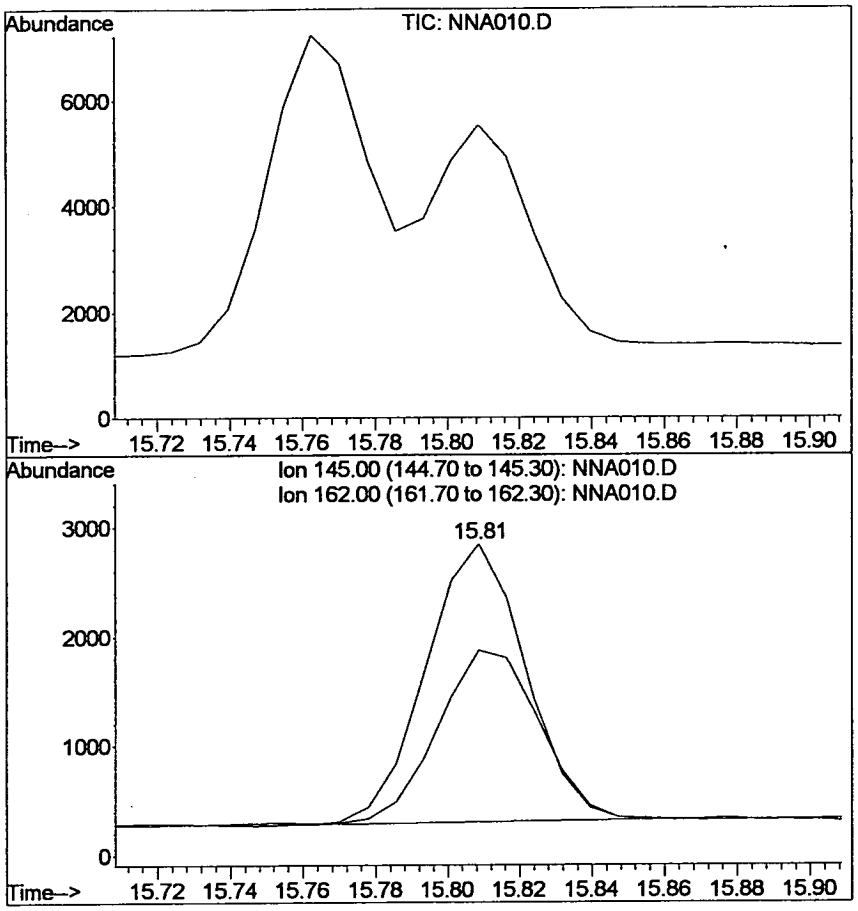

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.81 min Scan# 809
Delta R.T. 0.00 min
Lab File: NNA010.D
Acq: 14 Jun 2007 8:50 am

Tgt Ion:145 Resp: 4883

Ion	Ratio	Lower	Upper
145	100		
162	63.1	22.4	102.4

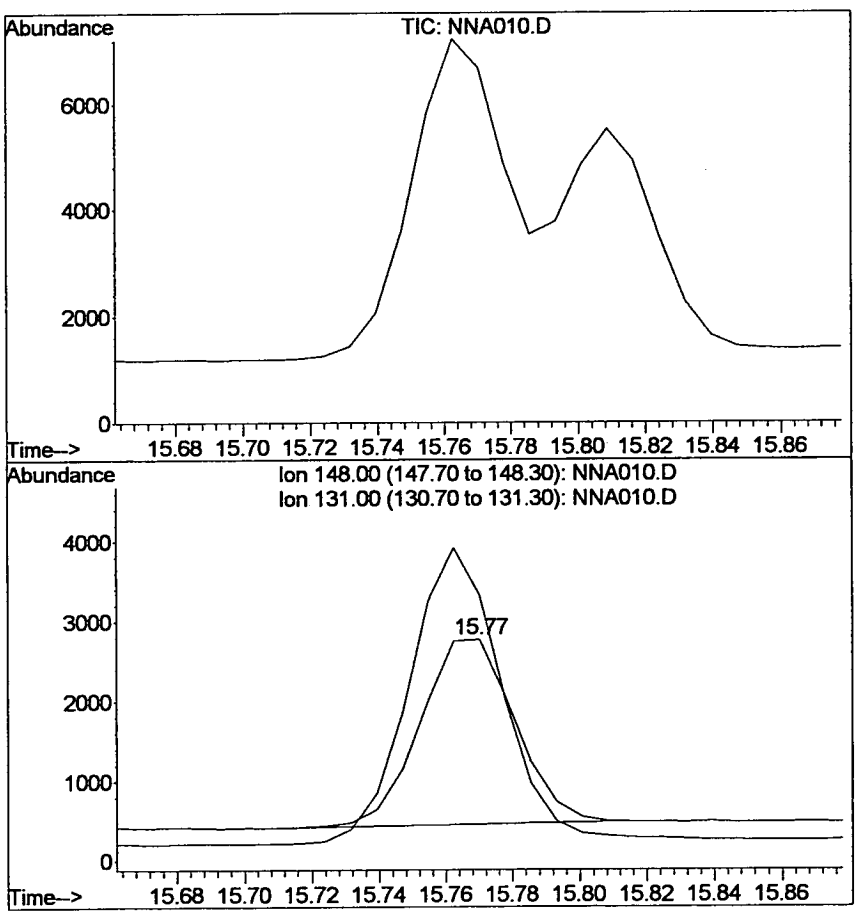

#6
NDPA
Concen: 11.14 PPB
RT: 15.77 min Scan# 804
Delta R.T. 0.00 min
Lab File: NNA010.D
Acq: 14 Jun 2007 8:50 am

Tgt Ion:148 Resp: 4580

Ion	Ratio	Lower	Upper
148	100		
131	154.9	99.8	207.2

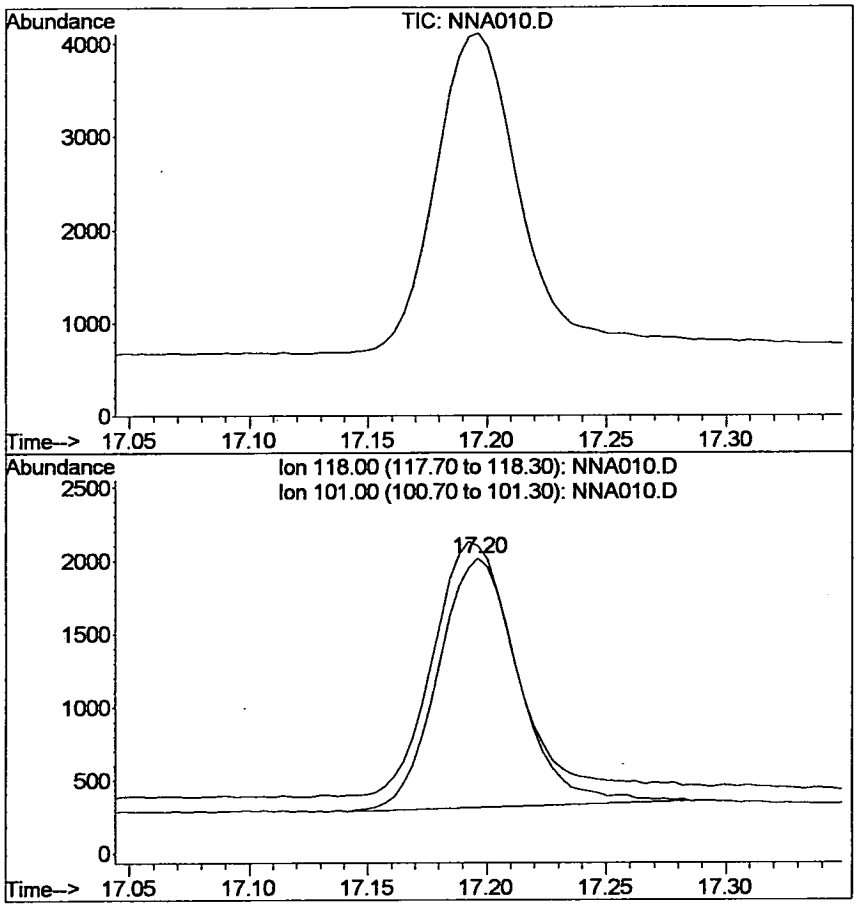

#7
NPYR
Concen: 10.17 PPB
RT: 17.20 min Scan# 1076
Delta R.T. 0.00 min
Lab File: NNA010.D
Acq: 14 Jun 2007 8:50 am

Tgt Ion:118 Resp: 4021

Ion	Ratio	Lower	Upper
118	100		
101	98.0	62.6	130.0

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\TEST\NNA001.D
Acq On : 14 Jun 2007 9:14 am
Sample : 1ppb Std.# 7060218
Misc : n-Nitrosamines Water ICV
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:24 2007

Vial: 2
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration
DataAcq Meth : C7E29NWA

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) NDMA-D6	10.90	81	2914	10.00	PPB	0.00
3) NDEA-D10	13.38	113	5557	10.00	PPB	0.00
5) NDPA-D14	15.81	145	4982	10.00	PPB	0.00
Target Compounds						**Qvalue**
2) NDMA	10.84	92	574	0.98	PPB	98
4) NDEA	13.32	120	627	1.06	PPB	98
6) NDPA	15.76	148	615	1.47	PPB	90
7) NPYR	17.19	118	320	0.79	PPB	89

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\TEST\NNA001.D
Acq On : 14 Jun 2007 9:14 am
Sample : 1ppb Std.# 7060218
Misc : n-Nitrosamines Water ICV
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:24 2007

Vial: 2
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration

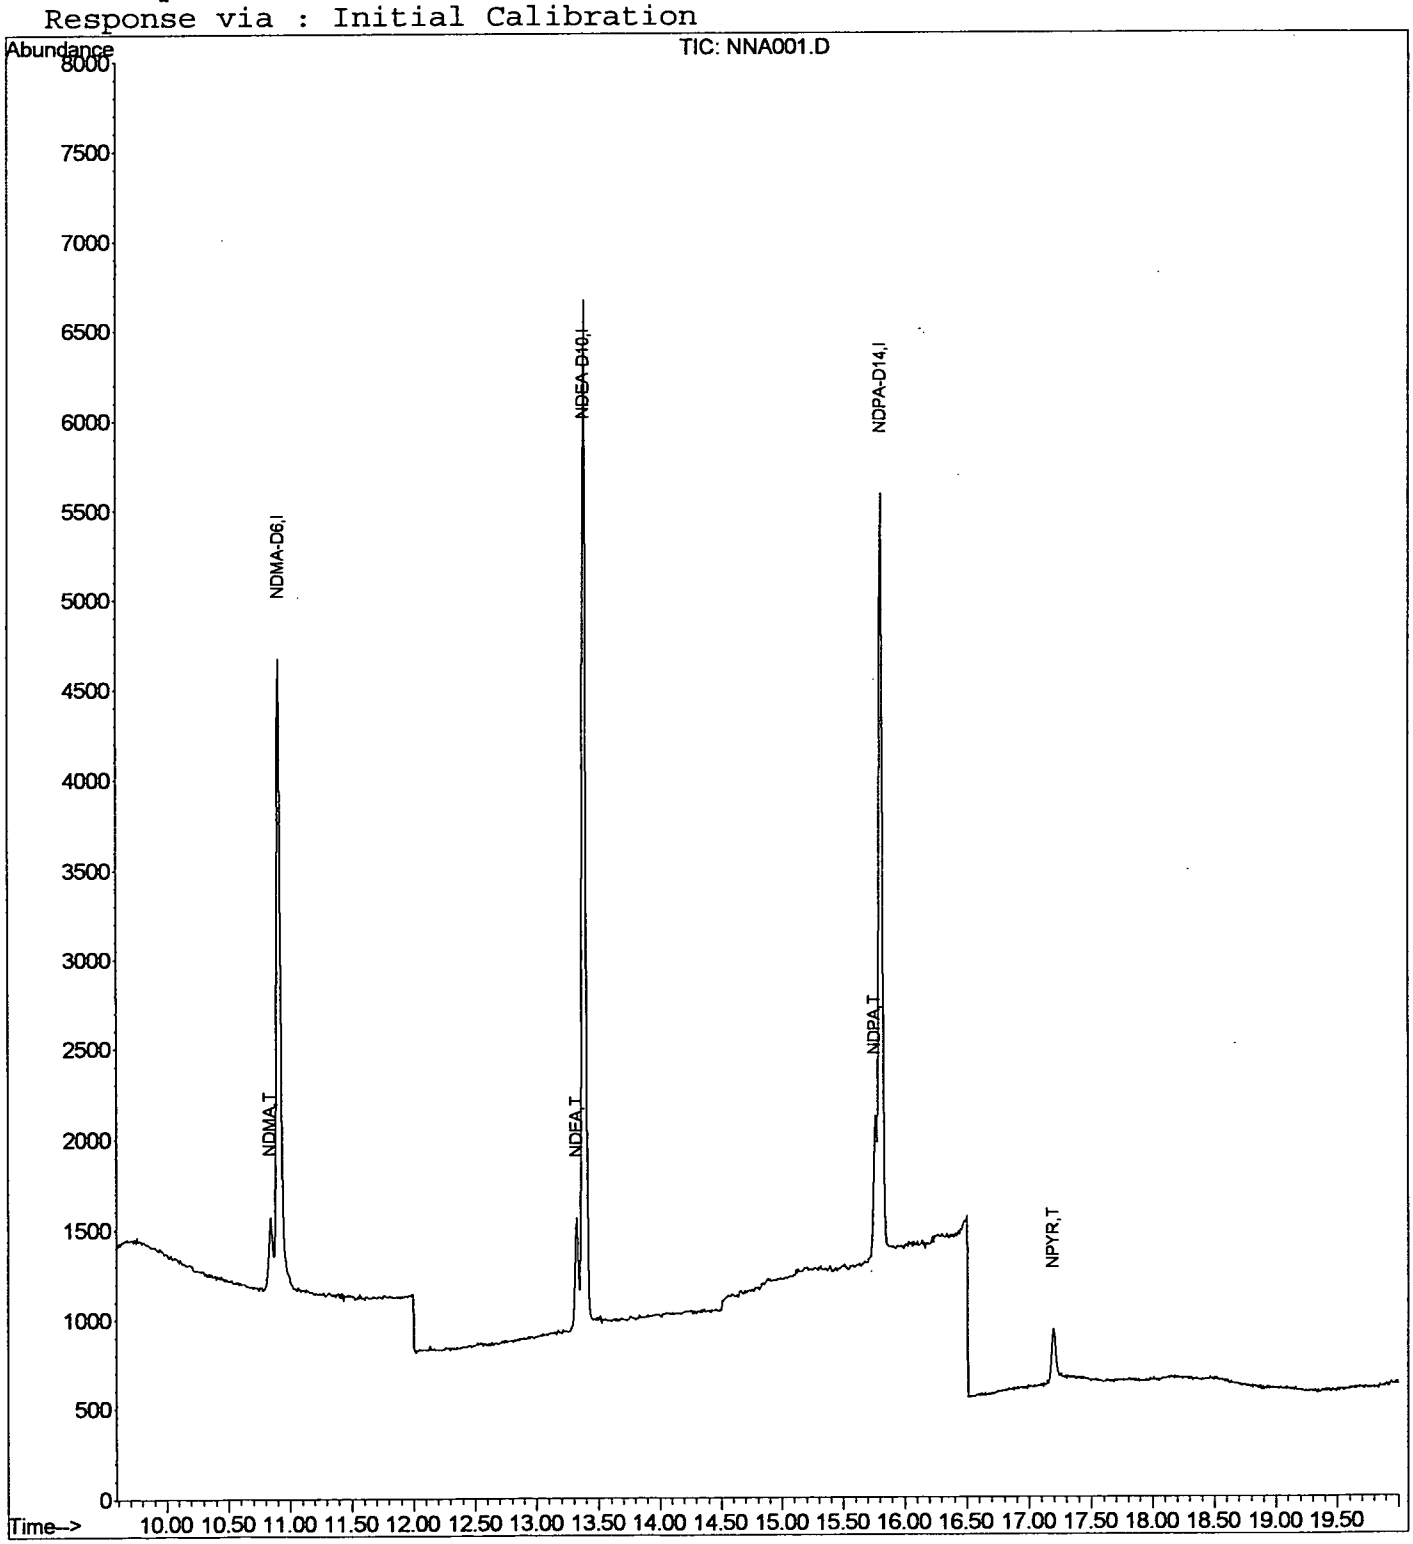

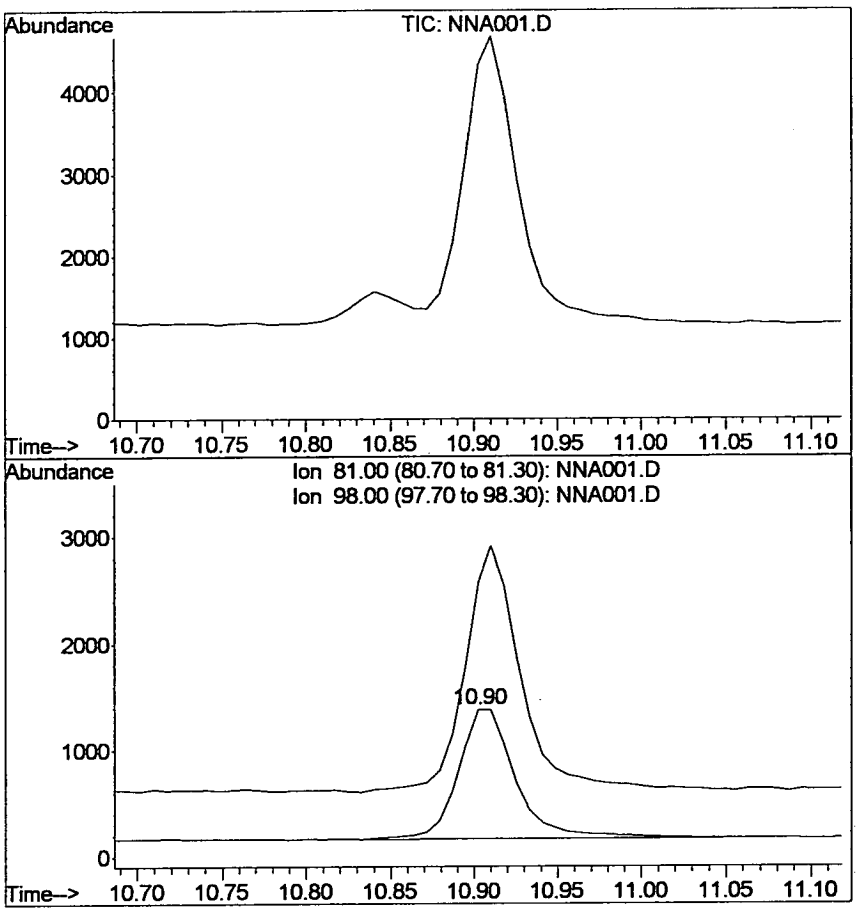

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.90 min Scan# 172
Delta R.T. 0.00 min
Lab File: NNA001.D
Acq: 14 Jun 2007 9:14 am

Tgt Ion: 81 Resp: 2914

Ion	Ratio	Lower	Upper
81	100		
98	183.6	144.1	224.1

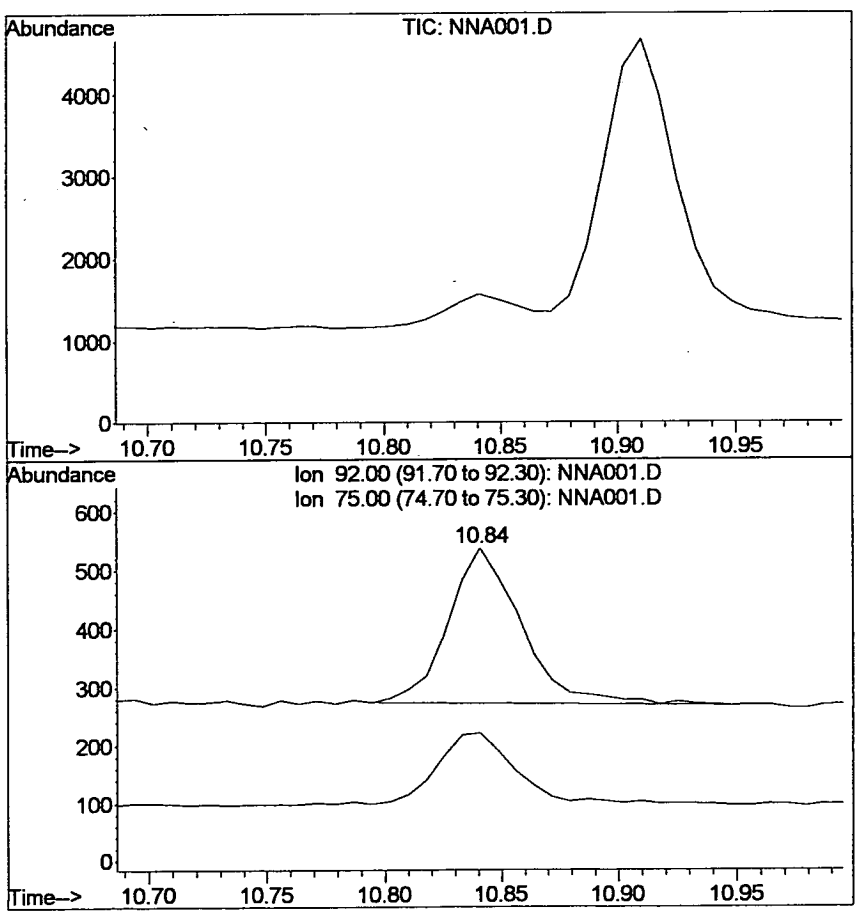

#2
NDMA
Concen: 0.98 PPB
RT: 10.84 min Scan# 164
Delta R.T. 0.01 min
Lab File: NNA001.D
Acq: 14 Jun 2007 9:14 am

Tgt Ion: 92 Resp: 574

Ion	Ratio	Lower	Upper
92	100		
75	50.2	31.8	66.0

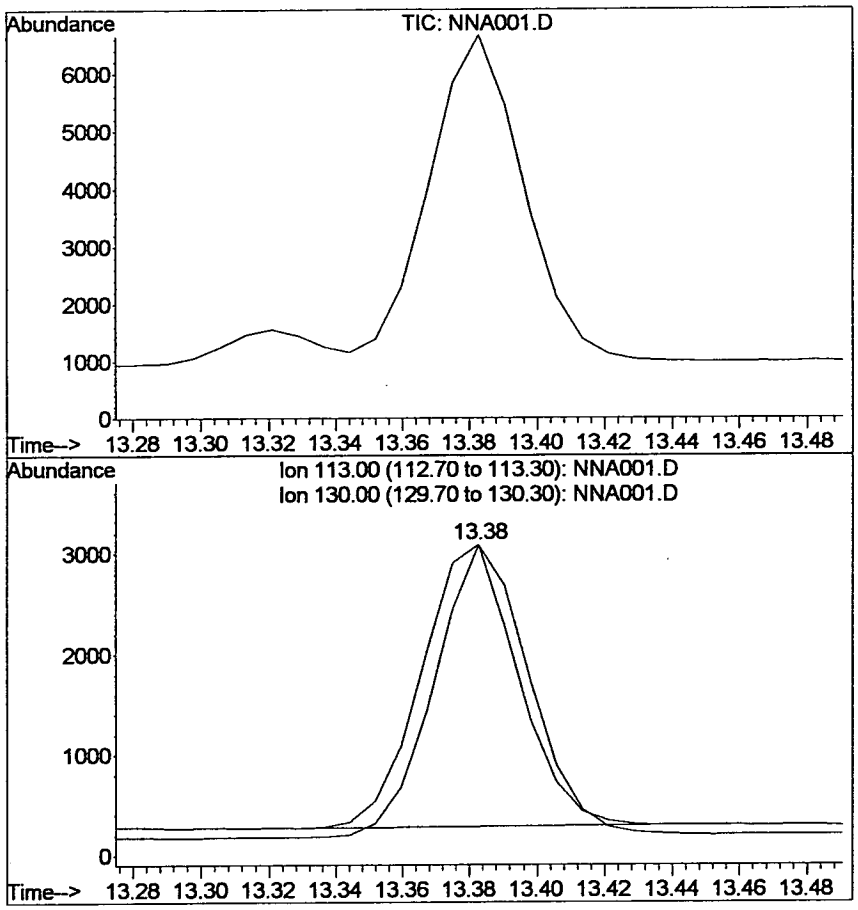

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.38 min Scan# 494
Delta R.T. 0.01 min
Lab File: NNA001.D
Acq: 14 Jun 2007 9:14 am

Tgt Ion:113 Resp: 5557

Ion	Ratio	Lower	Upper
113	100		
130	101.2	67.1	137.1

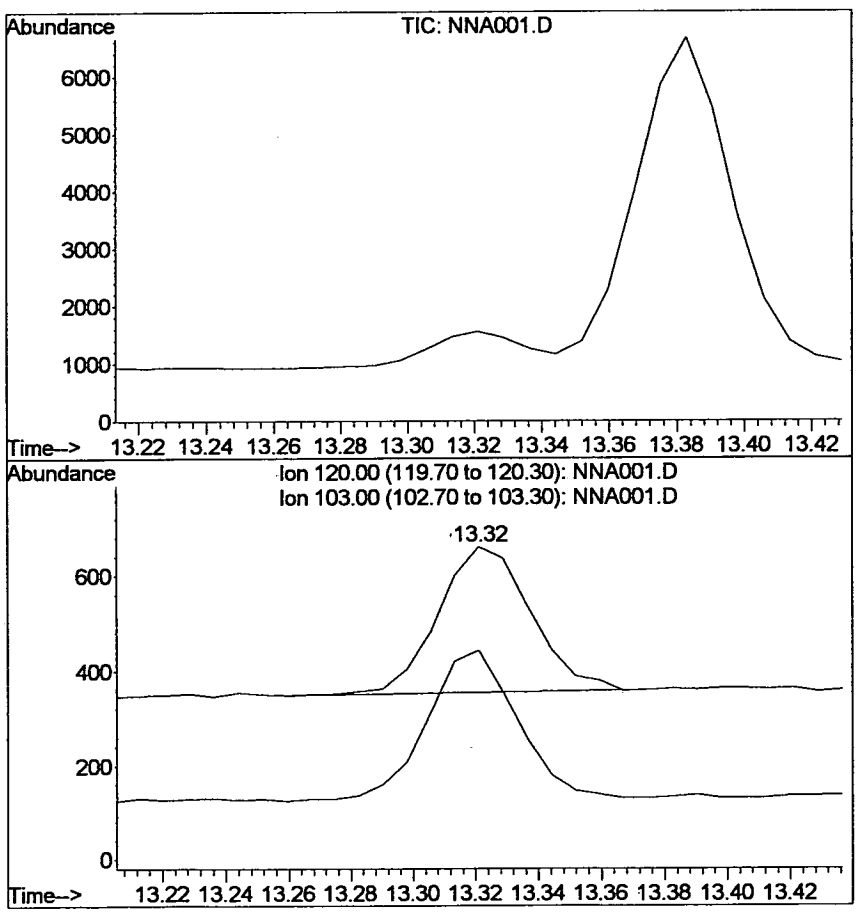

#4
NDEA
Concen: 1.06 PPB
RT: 13.32 min Scan# 486
Delta R.T. 0.00 min
Lab File: NNA001.D
Acq: 14 Jun 2007 9:14 am

Tgt Ion:120 Resp: 627

Ion	Ratio	Lower	Upper
120	100		
103	97.9	65.3	135.5

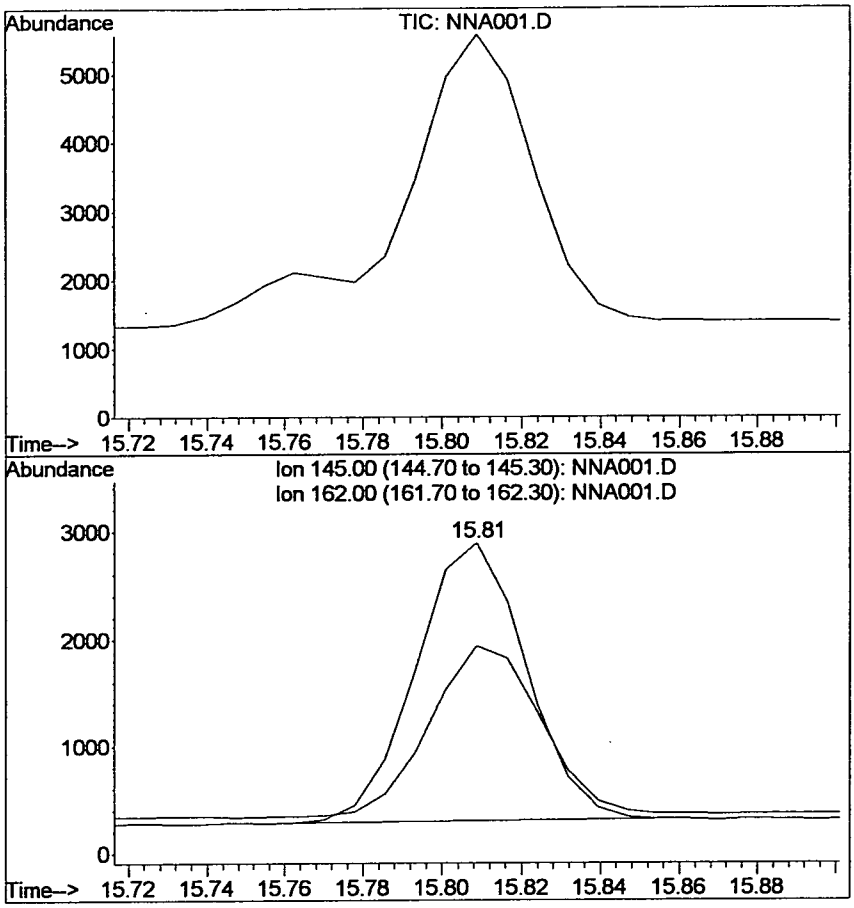

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.81 min Scan# 809
Delta R.T. 0.00 min
Lab File: NNA001.D
Acq: 14 Jun 2007 9:14 am

Tgt Ion:145 Resp: 4982

Ion	Ratio	Lower	Upper
145	100		
162	61.1	22.4	102.4

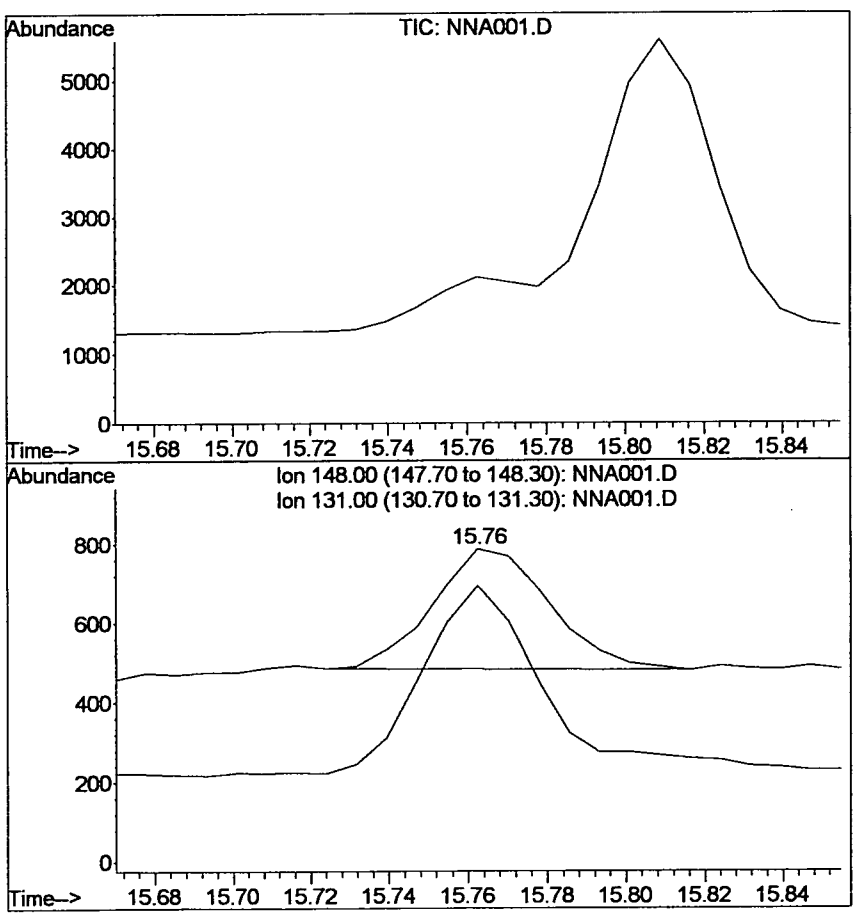

#6
NDPA
Concen: 1.47 PPB
RT: 15.76 min Scan# 803
Delta R.T. -0.01 min
Lab File: NNA001.D
Acq: 14 Jun 2007 9:14 am

Tgt Ion:148 Resp: 615

Ion	Ratio	Lower	Upper
148	100		
131	167.0	99.8	207.2

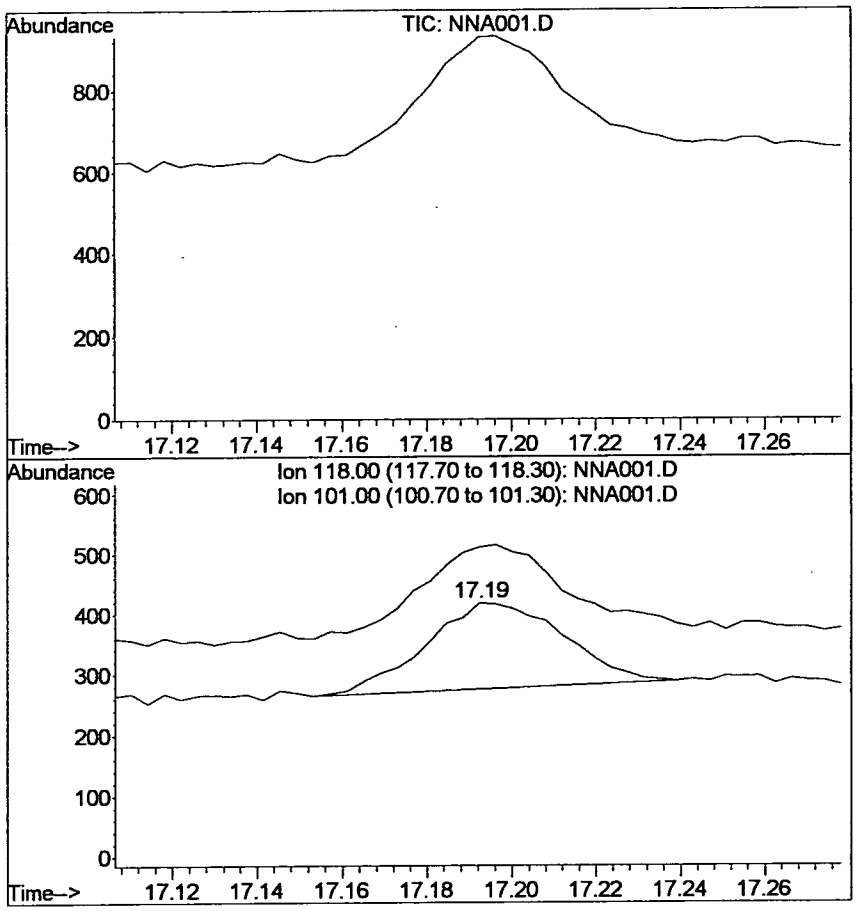

#7
NPYR
Concen: 0.79 PPB
RT: 17.19 min Scan# 1075
Delta R.T. -0.00 min
Lab File: NNA001.D
Acq: 14 Jun 2007 9:14 am

Tgt Ion:118 Resp: 320

Ion	Ratio	Lower	Upper
118	100		
101	106.9	62.6	130.0

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA005.D
Acq On : 14 Jun 2007 10:01 am
Sample : 5ppb Std.# 7060220
Misc : n-Nitrosamines Water ICV
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:25 2007

Vial: 4
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration
DataAcq Meth : C7E29NWA

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) NDMA-D6	10.91	81	3006	10.00 PPB	0.00
3) NDEA-D10	13.38	113	5992	10.00 PPB	0.00
5) NDPA-D14	15.81	145	5087	10.00 PPB	0.00
Target Compounds					**Qvalue**
2) NDMA	10.84	92	2987	4.95 PPB	99
4) NDEA	13.32	120	3164	4.96 PPB	99
6) NDPA	15.77	148	2150	5.02 PPB	96
7) NPYR	17.20	118	1777	4.32 PPB	92

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA005.D Vial: 4
Acq On : 14 Jun 2007 10:01 am Operator: DF/AI
Sample : 5ppb Std.# 7060220 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:25 2007 Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration

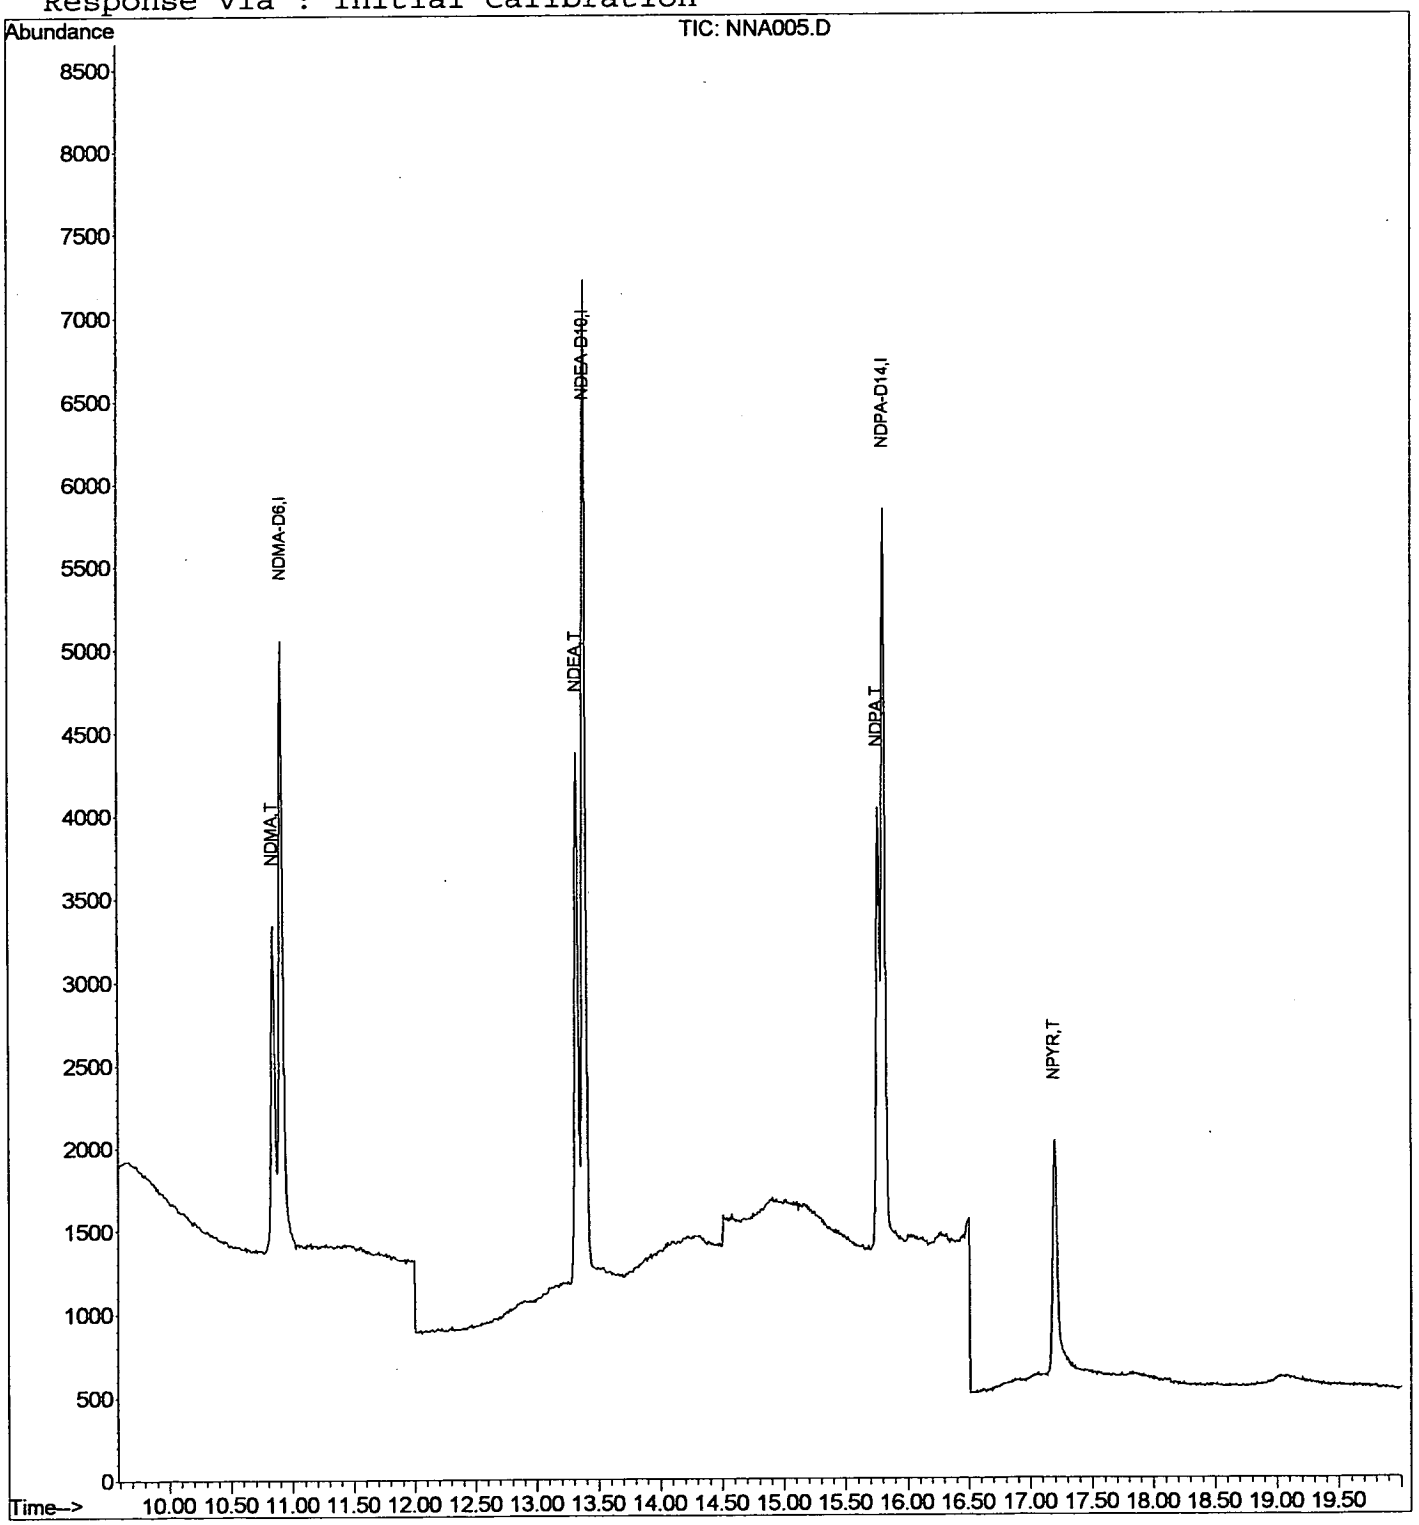

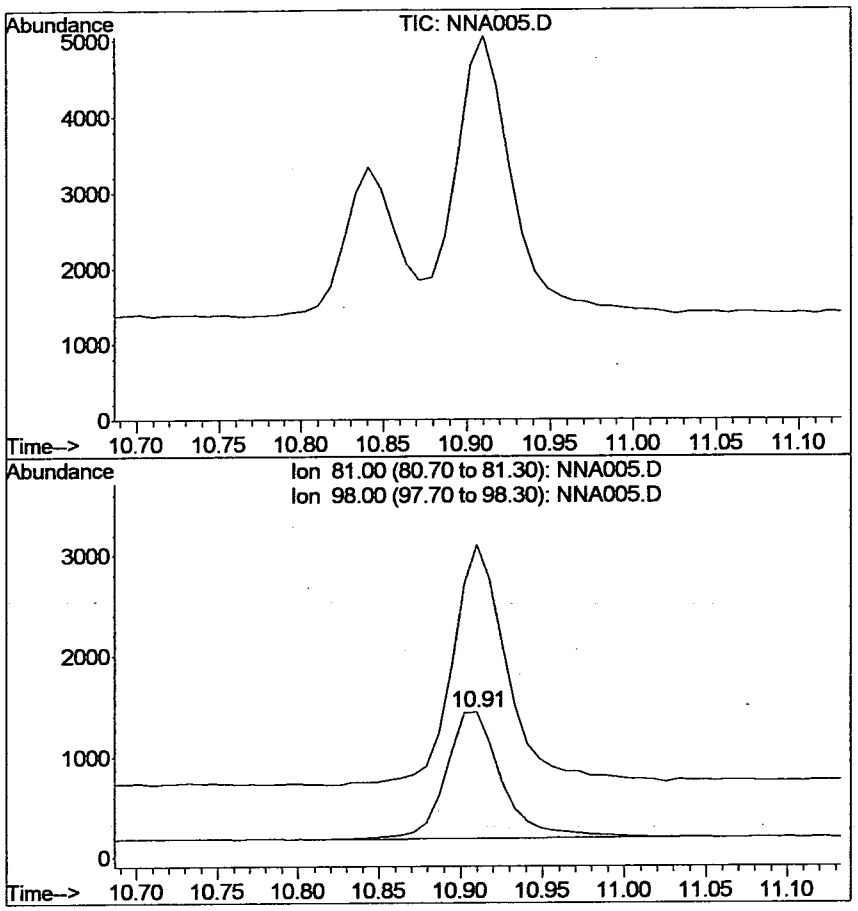

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.91 min Scan# 173
Delta R.T. 0.01 min
Lab File: NNA005.D
Acq: 14 Jun 2007 10:01 am

Tgt Ion: 81 Resp: 3006

Ion	Ratio	Lower	Upper
81	100		
98	184.3	144.1	224.1

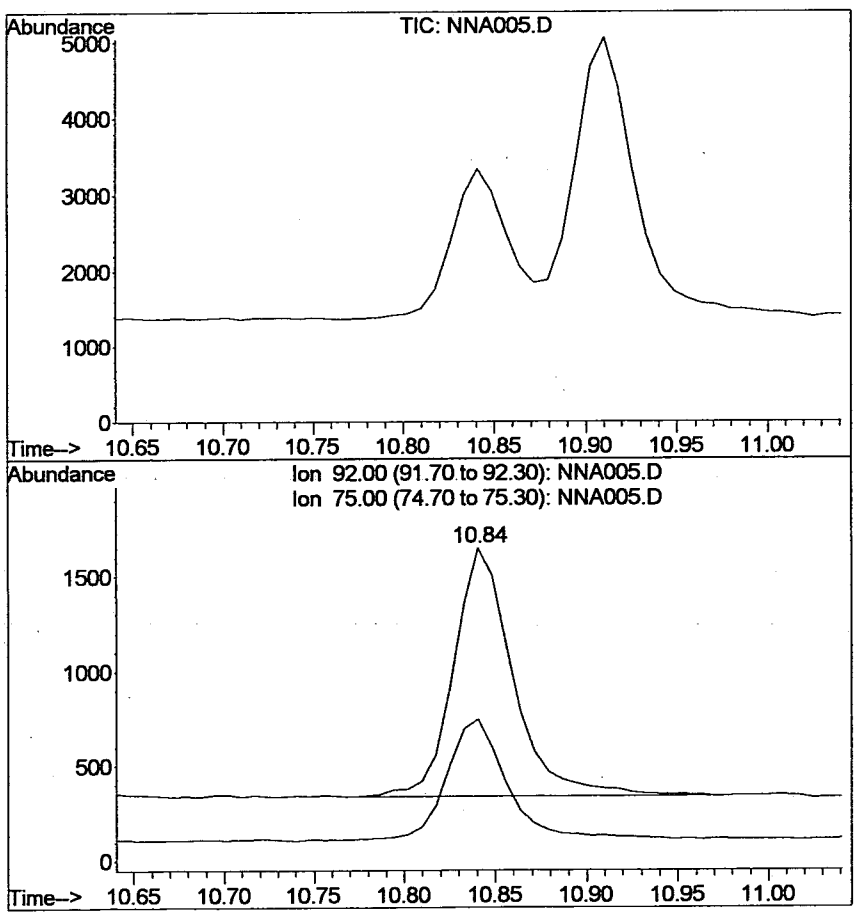

#2
NDMA
Concen: 4.95 PPB
RT: 10.84 min Scan# 164
Delta R.T. 0.01 min
Lab File: NNA005.D
Acq: 14 Jun 2007 10:01 am

Tgt Ion: 92 Resp: 2987

Ion	Ratio	Lower	Upper
92	100		
75	49.8	31.8	66.0

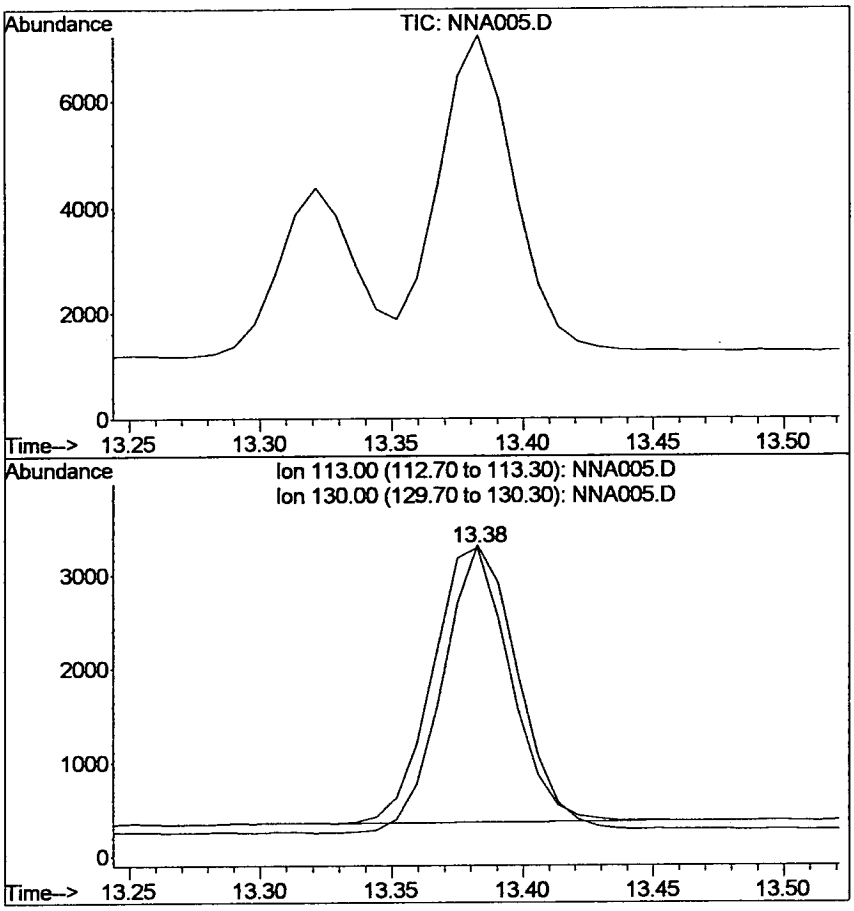

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.38 min Scan# 494
Delta R.T. 0.01 min
Lab File: NNA005.D
Acq: 14 Jun 2007 10:01 am

Tgt Ion:113 Resp: 5992

Ion	Ratio	Lower	Upper
113	100		
130	100.3	67.1	137.1

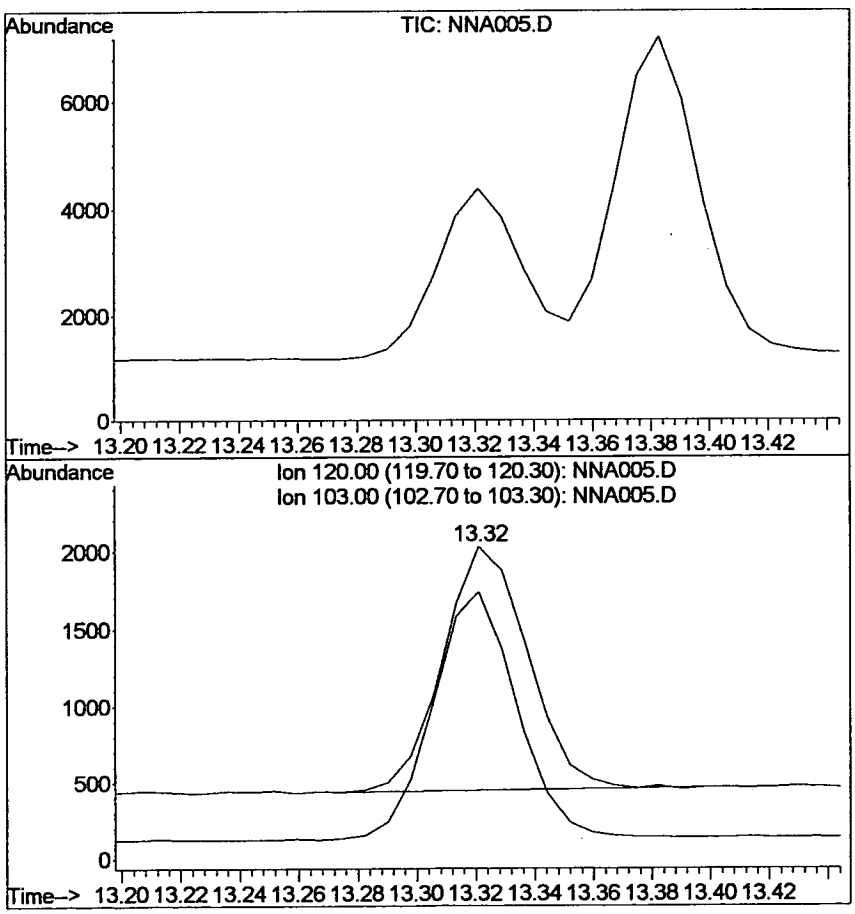

#4
NDEA
Concen: 4.96 PPB
RT: 13.32 min Scan# 486
Delta R.T. -0.00 min
Lab File: NNA005.D
Acq: 14 Jun 2007 10:01 am

Tgt Ion:120 Resp: 3164

Ion	Ratio	Lower	Upper
120	100		
103	99.8	65.3	135.5

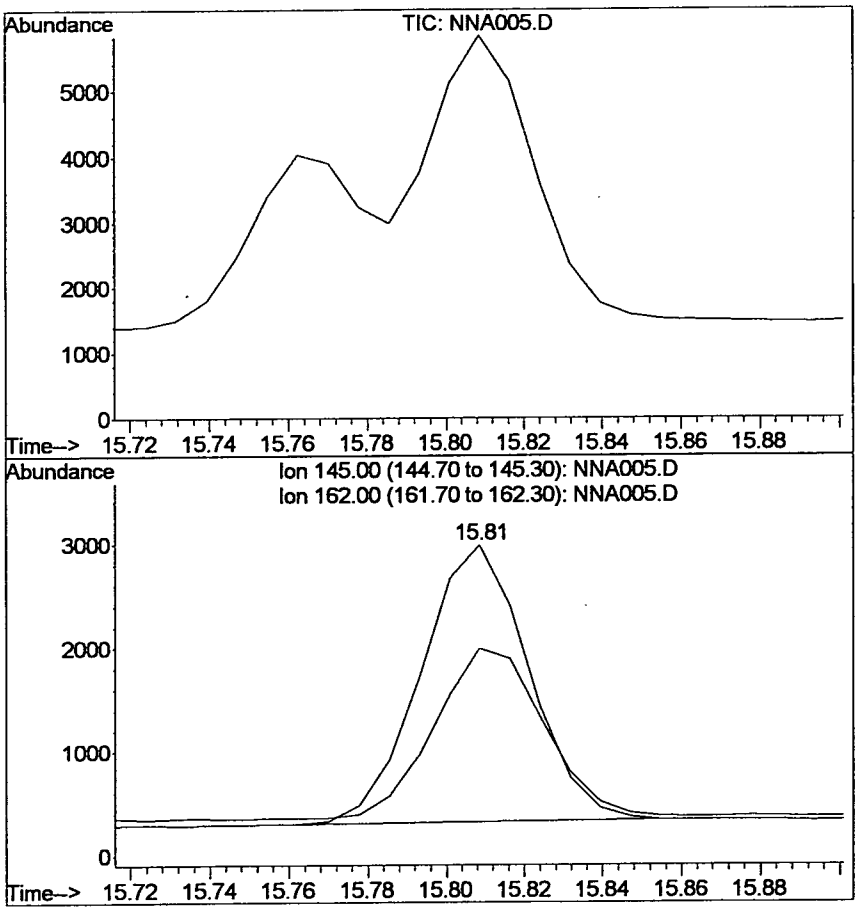

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.81 min Scan# 809
Delta R.T. -0.00 min
Lab File: NNA005.D
Acq: 14 Jun 2007 10:01 am

Tgt Ion:145 Resp: 5087

Ion	Ratio	Lower	Upper
145	100		
162	61.9	22.4	102.4

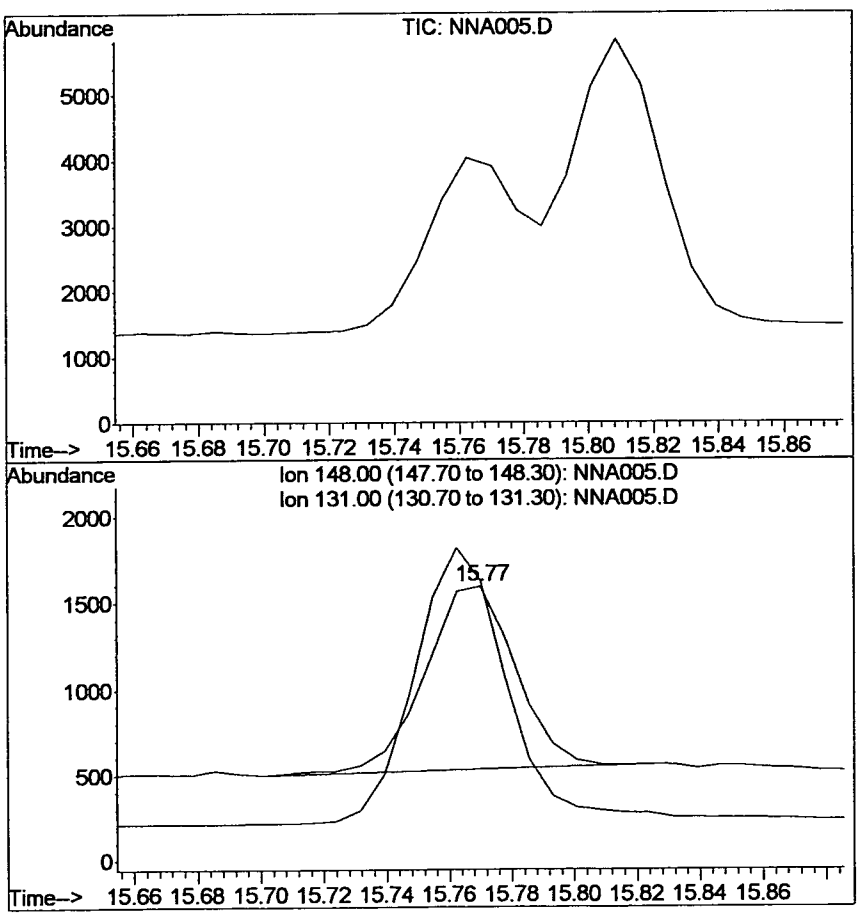

#6
NDPA
Concen: 5.02 PPB
RT: 15.77 min Scan# 804
Delta R.T. -0.00 min
Lab File: NNA005.D
Acq: 14 Jun 2007 10:01 am

Tgt Ion:148 Resp: 2150

Ion	Ratio	Lower	Upper
148	100		
131	148.6	99.8	207.2

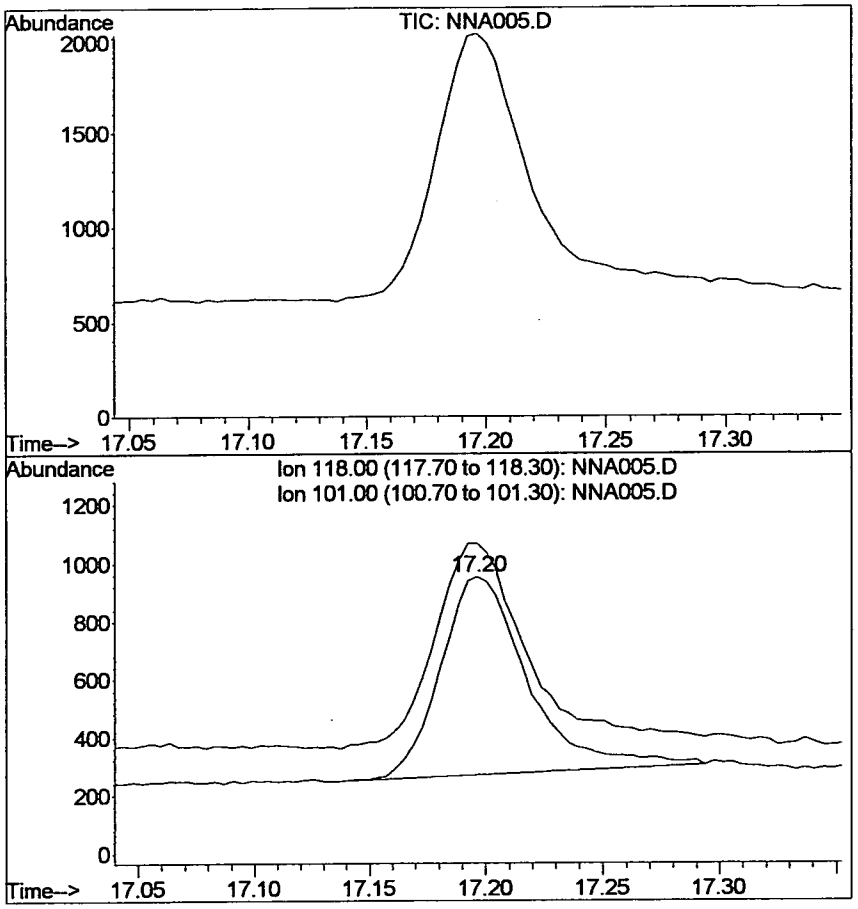

#7
NPYR
Concen: 4.32 PPB
RT: 17.20 min Scan# 1076
Delta R.T. -0.00 min
Lab File: NNA005.D
Acq: 14 Jun 2007 10:01 am

Tgt Ion:118 Resp: 1777

Ion	Ratio	Lower	Upper
118	100		
101	104.4	62.6	130.0

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA020.D Vial: 5
Acq On : 14 Jun 2007 10:24 am Operator: DF/AI
Sample : 20ppb Std.# 7060222 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:27 2007 Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration
DataAcq Meth : C7E29NWA

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) NDMA-D6	10.91	81	2991	10.00 PPB	0.00
3) NDEA-D10	13.38	113	5836	10.00 PPB	0.00
5) NDPA-D14	15.81	145	5092	10.00 PPB	0.00
Target Compounds					**Qvalue**
2) NDMA	10.84	92	11598	19.34 PPB	100
4) NDEA	13.32	120	11973	19.27 PPB	99
6) NDPA	15.77	148	7622	17.77 PPB	96
7) NPYR	17.20	118	7418	18.00 PPB	91

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA020.D Vial: 5
Acq On : 14 Jun 2007 10:24 am Operator: DF/AI
Sample : 20ppb Std.# 7060222 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:27 2007 Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration

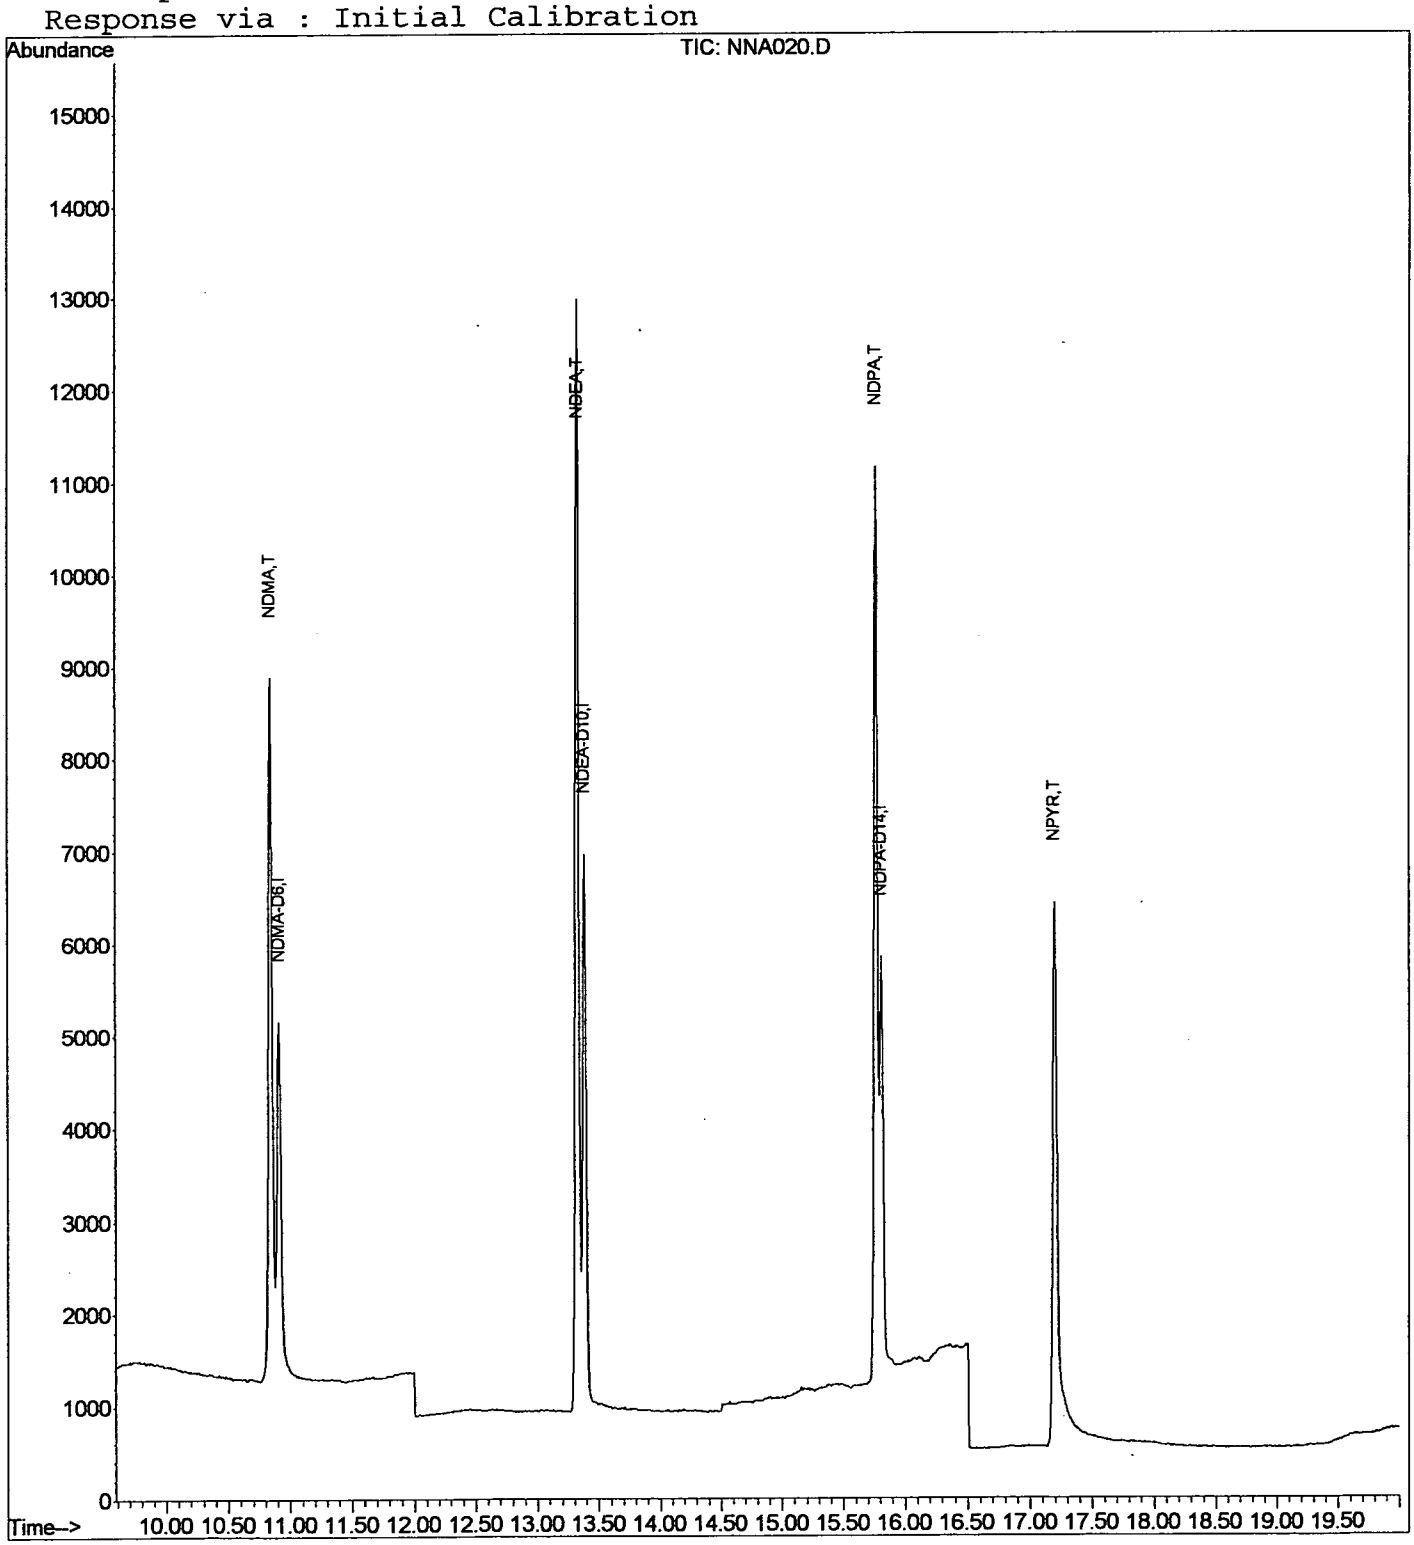

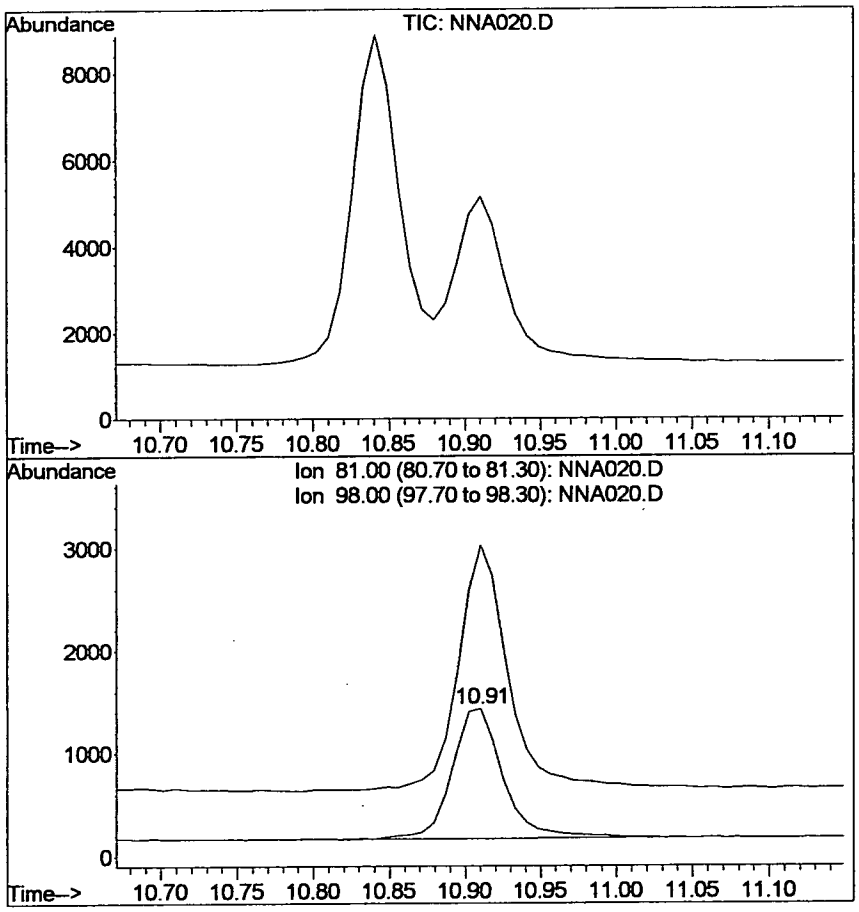

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.91 min Scan# 173
Delta R.T. 0.01 min
Lab File: NNA020.D
Acq: 14 Jun 2007 10:24 am

Tgt Ion: 81 Resp: 2991

Ion	Ratio	Lower	Upper
81	100		
98	177.3	144.1	224.1

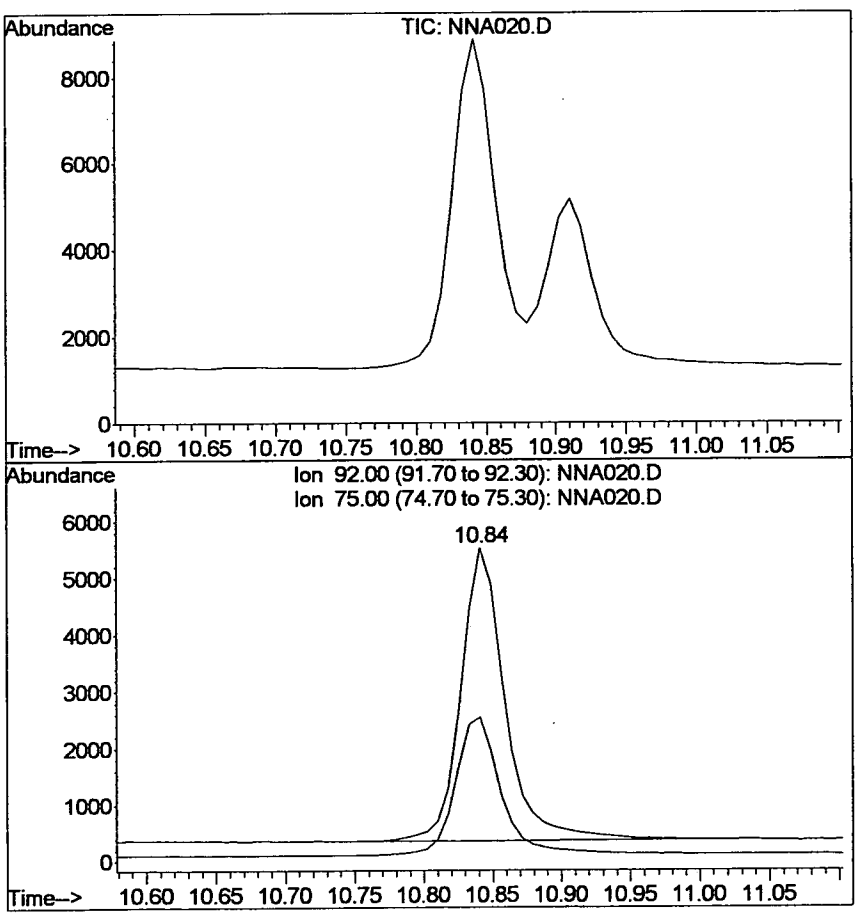

#2
NDMA
Concen: 19.34 PPB
RT: 10.84 min Scan# 164
Delta R.T. 0.01 min
Lab File: NNA020.D
Acq: 14 Jun 2007 10:24 am

Tgt Ion: 92 Resp: 11598

Ion	Ratio	Lower	Upper
92	100		
75	48.7	31.8	66.0

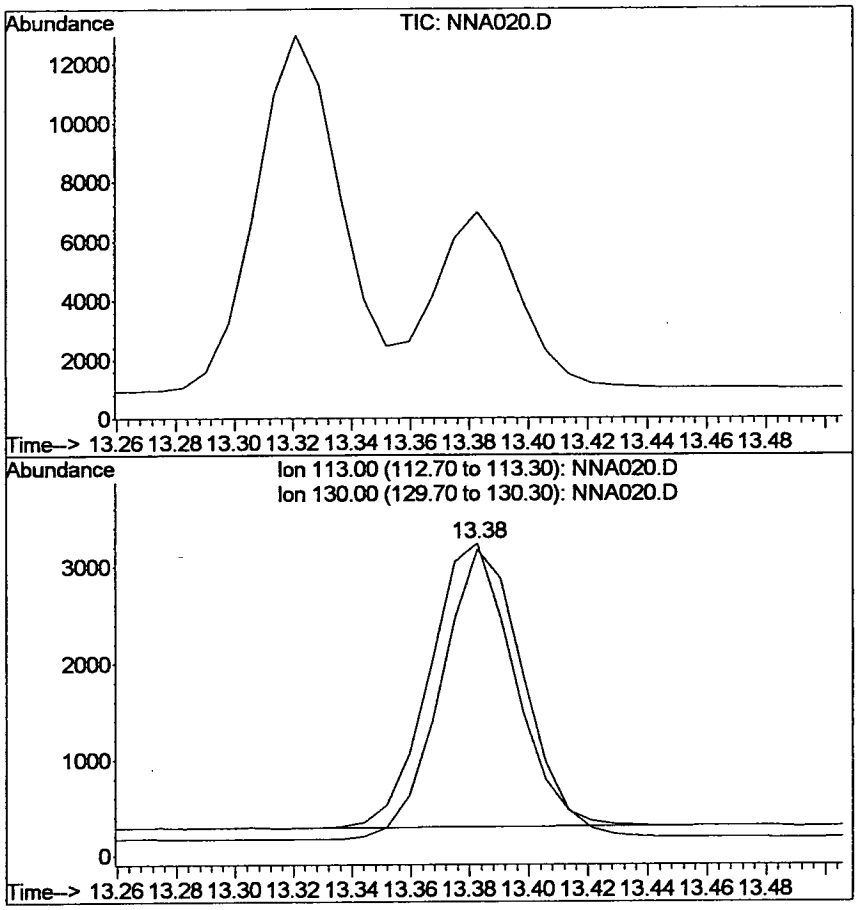

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.38 min Scan# 494
Delta R.T. 0.01 min
Lab File: NNA020.D
Acq: 14 Jun 2007 10:24 am

Tgt Ion:113 Resp: 5836

Ion	Ratio	Lower	Upper
113	100		
130	101.0	67.1	137.1

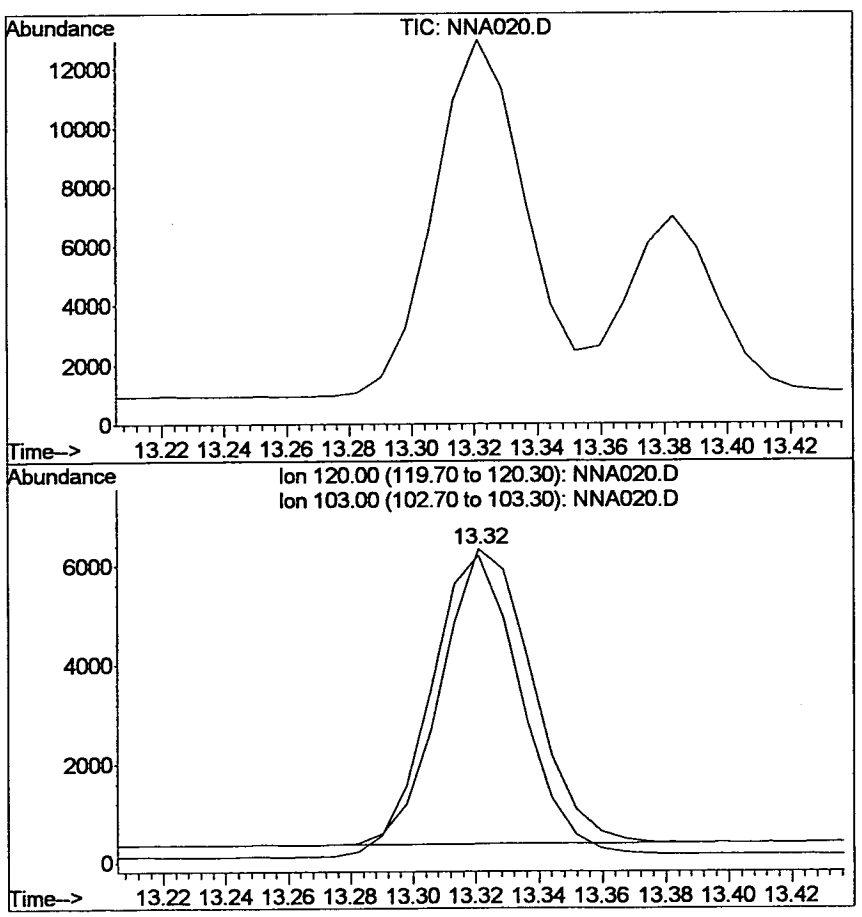

#4
NDEA
Concen: 19.27 PPB
RT: 13.32 min Scan# 486
Delta R.T. 0.00 min
Lab File: NNA020.D
Acq: 14 Jun 2007 10:24 am

Tgt Ion:120 Resp: 11973

Ion	Ratio	Lower	Upper
120	100		
103	101.0	65.3	135.5

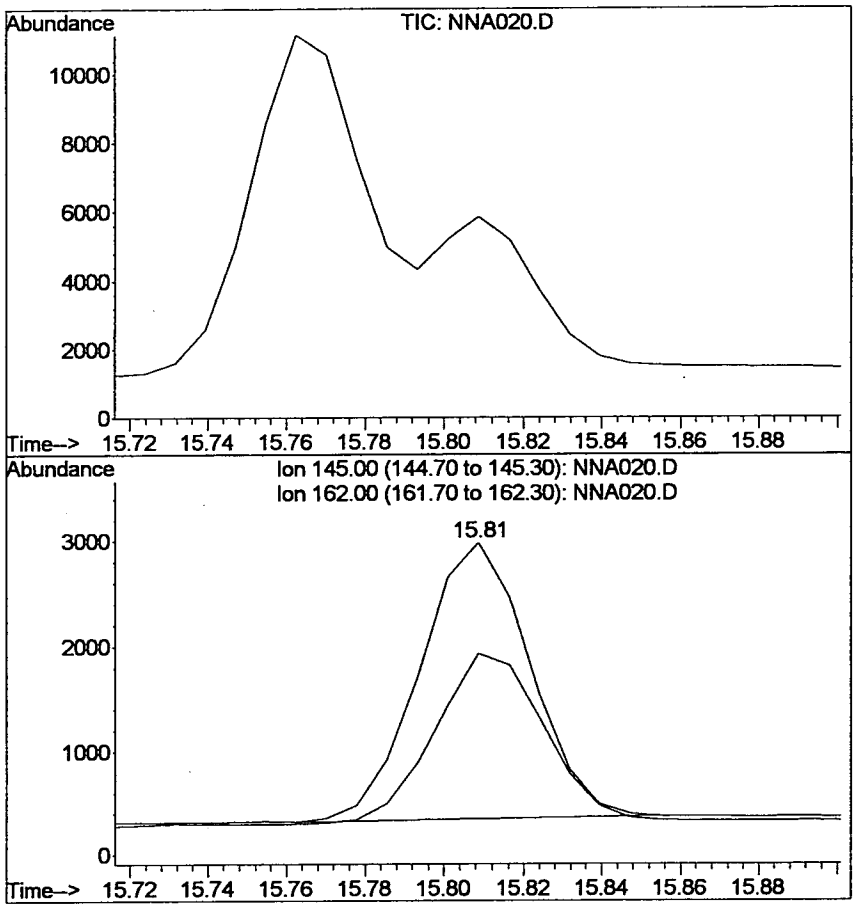

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.81 min Scan# 809
Delta R.T. 0.00 min
Lab File: NNA020.D
Acq: 14 Jun 2007 10:24 am

Tgt Ion:145 Resp: 5092

Ion	Ratio	Lower	Upper
145	100		
162	61.0	22.4	102.4

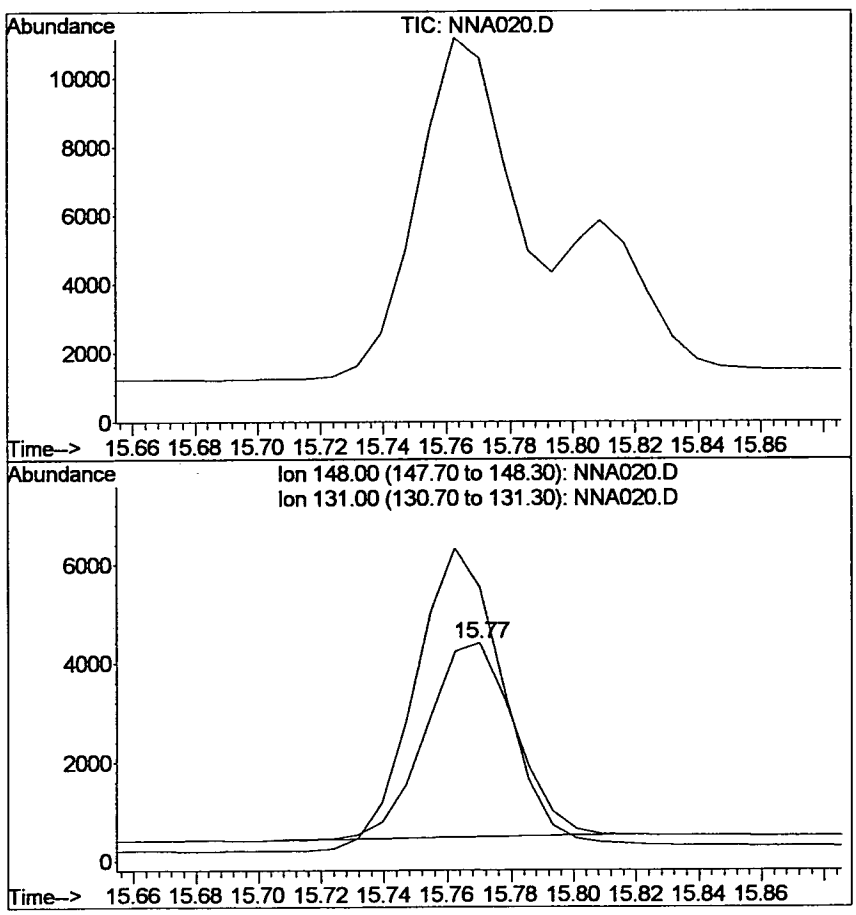

#6
NDPA
Concen: 17.77 PPB
RT: 15.77 min Scan# 804
Delta R.T. 0.00 min
Lab File: NNA020.D
Acq: 14 Jun 2007 10:24 am

Tgt Ion:148 Resp: 7622

Ion	Ratio	Lower	Upper
148	100		
131	158.8	99.8	207.2

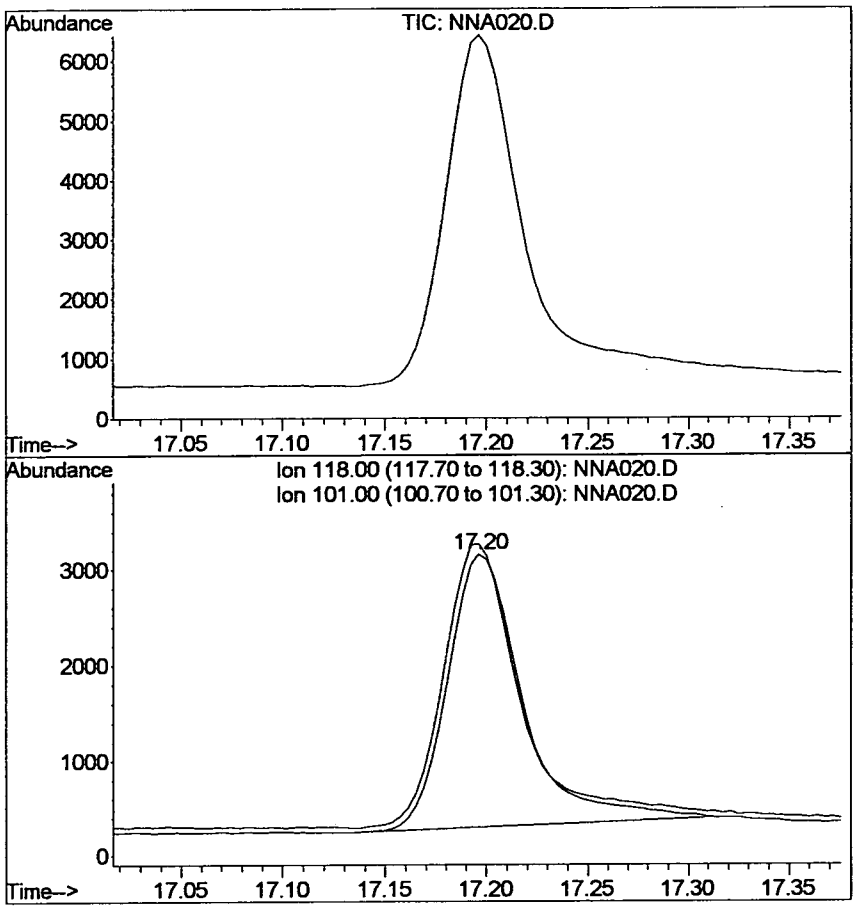

#7
NPYR
Concen: 18.00 PPB
RT: 17.20 min Scan# 1076
Delta R.T. 0.00 min
Lab File: NNA020.D
Acq: 14 Jun 2007 10:24 am

Tgt Ion:118 Resp: 7418

Ion	Ratio	Lower	Upper
118	100		
101	104.9	62.6	130.0

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA050.D
Vial: 6
Acq On : 14 Jun 2007 10:47 am
Operator: DF/AI
Sample : 50ppb Std.# 7060223
Inst : gcms37
Misc : n-Nitrosamines Water ICV
Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:27 2007
Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration
DataAcq Meth : C7E29NWA

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) NDMA-D6	10.90	81	3015	10.00	PPB	0.00
3) NDEA-D10	13.38	113	5896	10.00	PPB	0.00
5) NDPA-D14	15.81	145	5432	10.00	PPB	0.00
Target Compounds						**Qvalue**
2) NDMA	10.84	92	29636	49.01	PPB	99
4) NDEA	13.32	120	30485	48.57	PPB	99
6) NDPA	15.76	148	19990	43.69	PPB	94
7) NPYR	17.20	118	21971	49.98	PPB	94

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA050.D
Vial: 6
Acq On : 14 Jun 2007 10:47 am
Operator: DF/AI
Sample : 50ppb Std.# 7060223
Inst : gcms37
Misc : n-Nitrosamines Water ICV
Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:27 2007
Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration

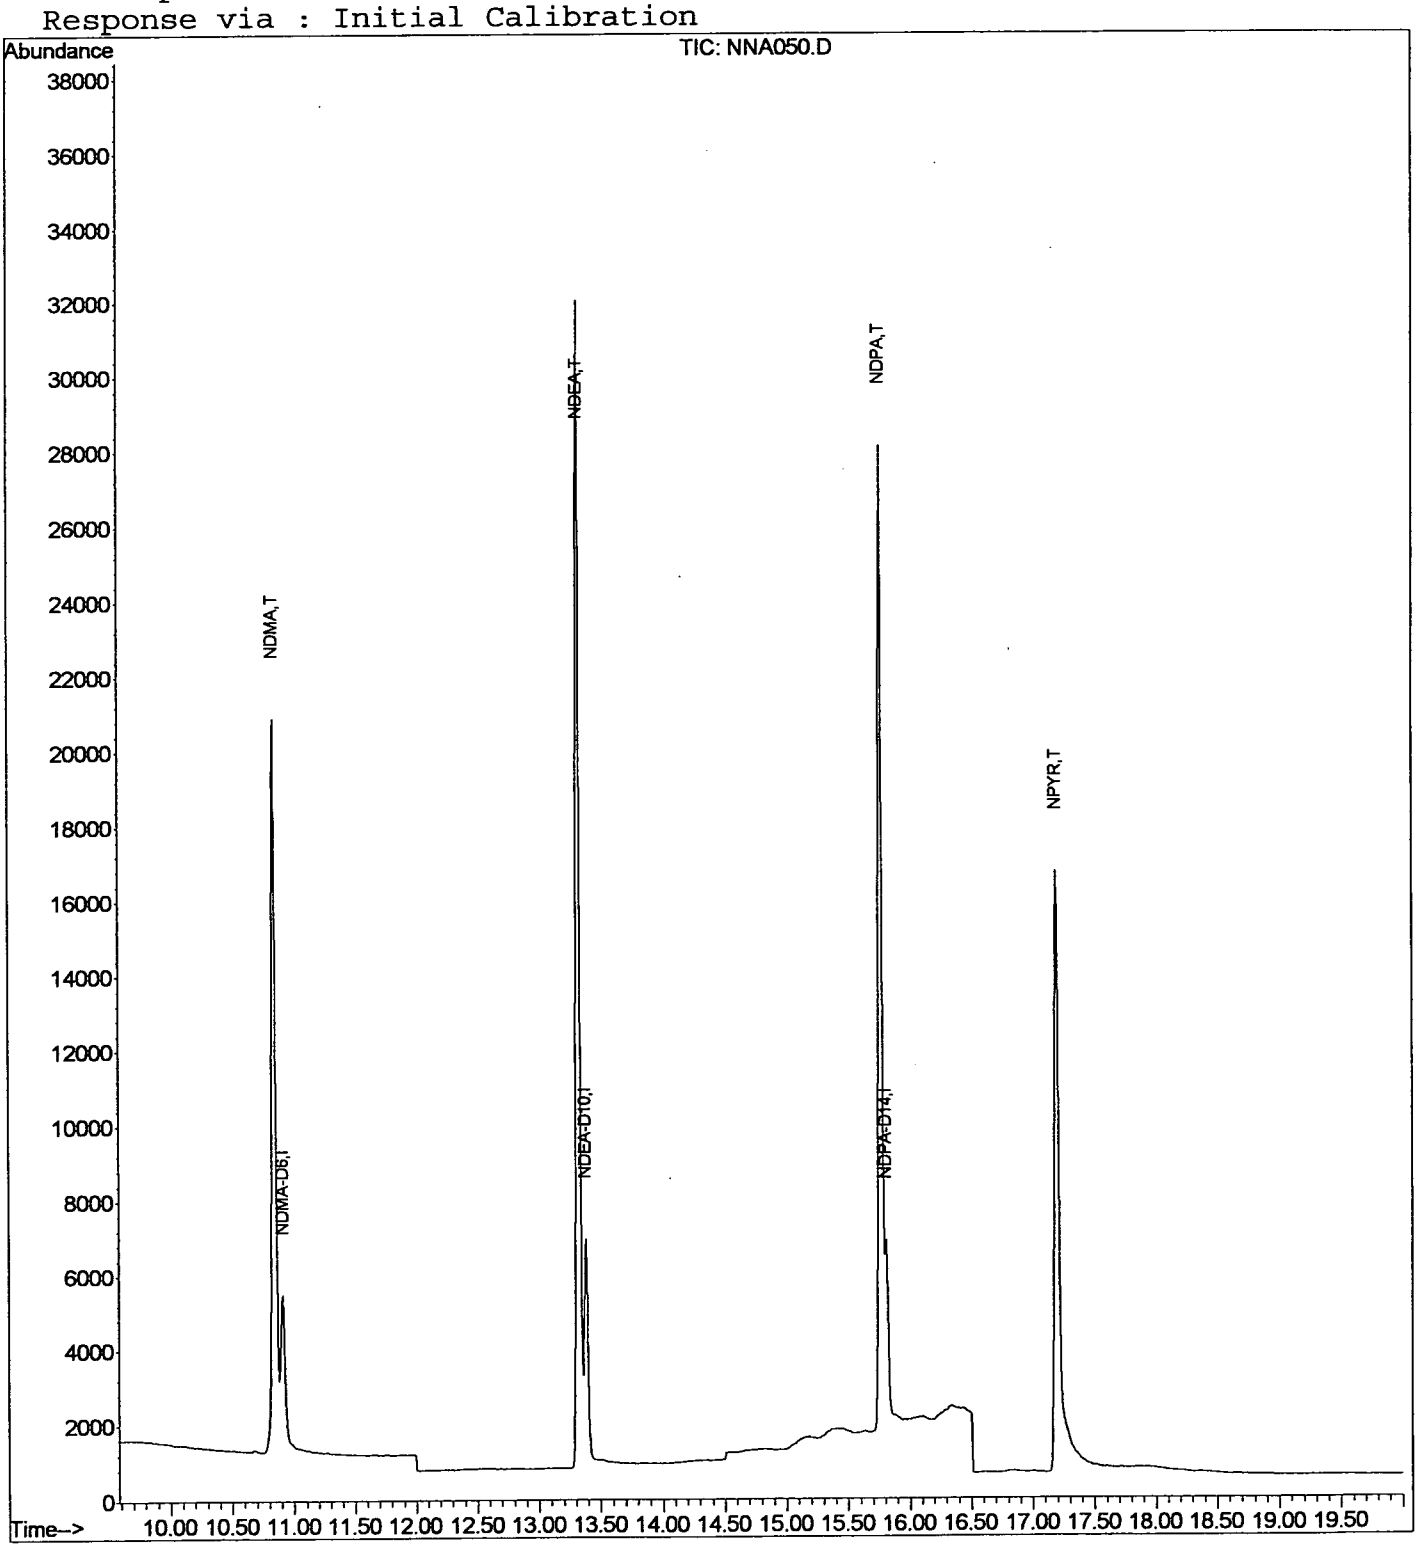

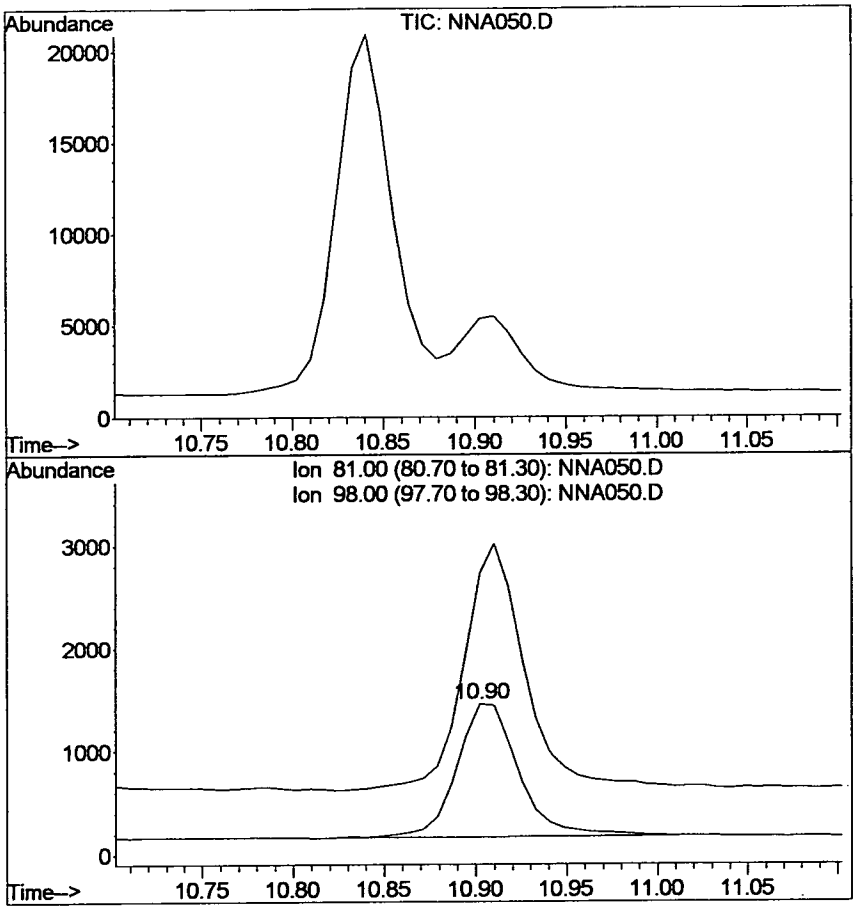

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.90 min Scan# 172
Delta R.T. -0.00 min
Lab File: NNA050.D
Acq: 14 Jun 2007 10:47 am

Tgt Ion: 81 Resp: 3015

Ion	Ratio	Lower	Upper
81	100		
98	180.3	144.1	224.1

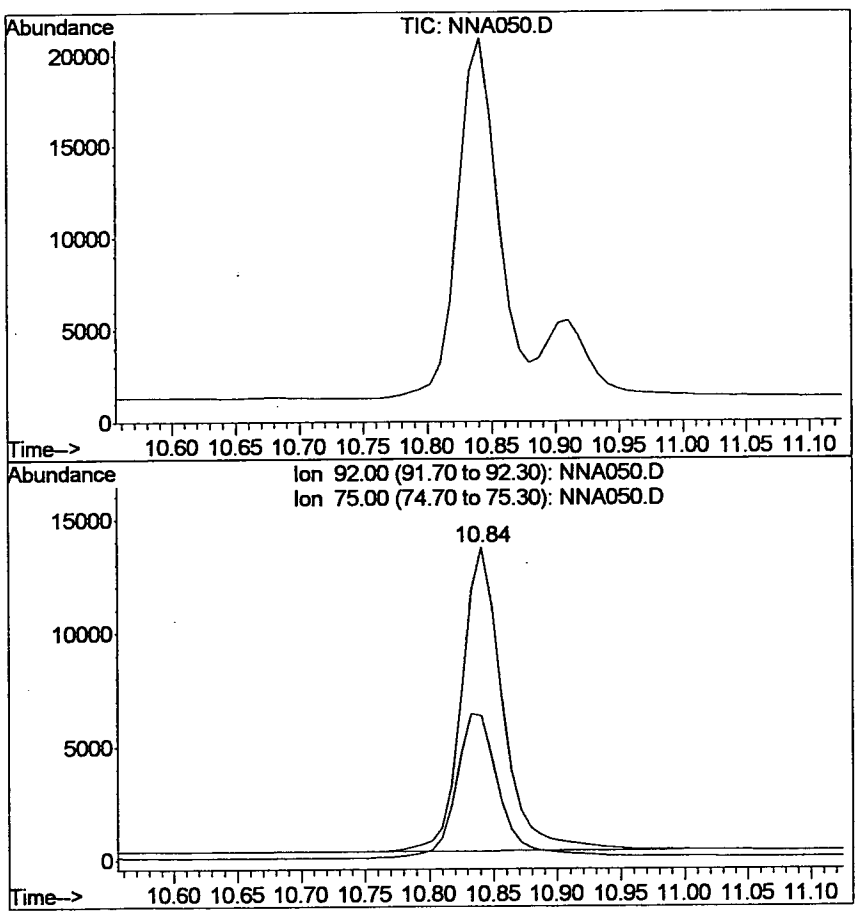

#2
NDMA
Concen: 49.01 PPB
RT: 10.84 min Scan# 164
Delta R.T. 0.01 min
Lab File: NNA050.D
Acq: 14 Jun 2007 10:47 am

Tgt Ion: 92 Resp: 29636

Ion	Ratio	Lower	Upper
92	100		
75	49.4	31.8	66.0

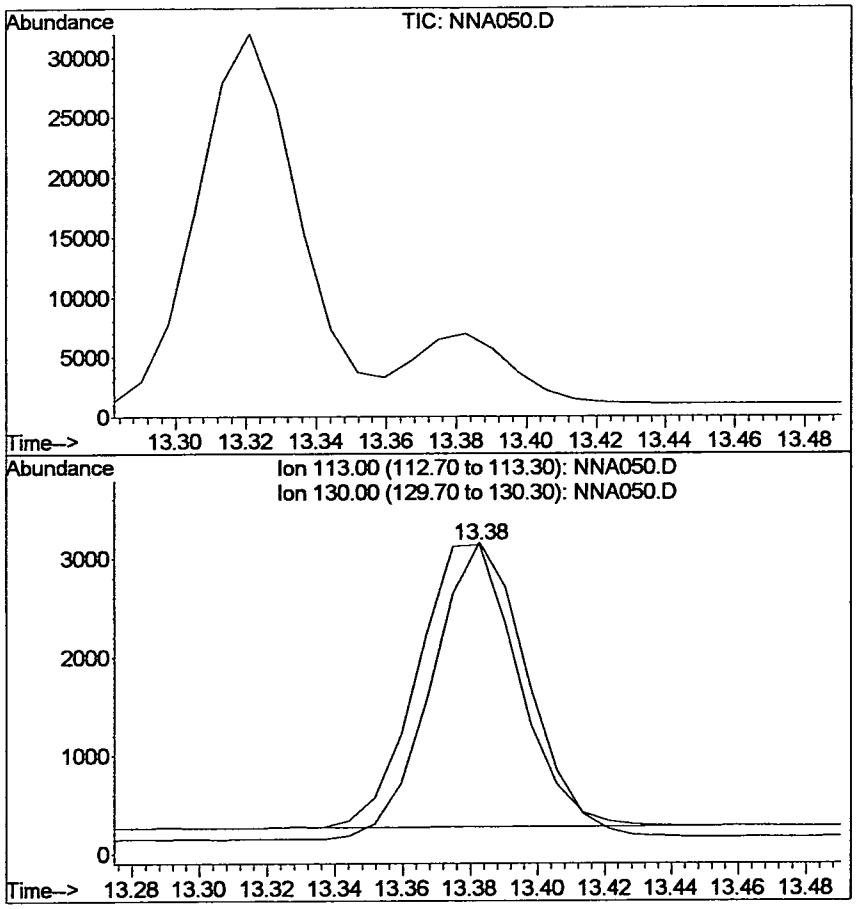

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.38 min Scan# 494
Delta R.T. 0.01 min
Lab File: NNA050.D
Acq: 14 Jun 2007 10:47 am

Tgt Ion:113 Resp: 5896

Ion	Ratio	Lower	Upper
113	100		
130	100.2	67.1	137.1

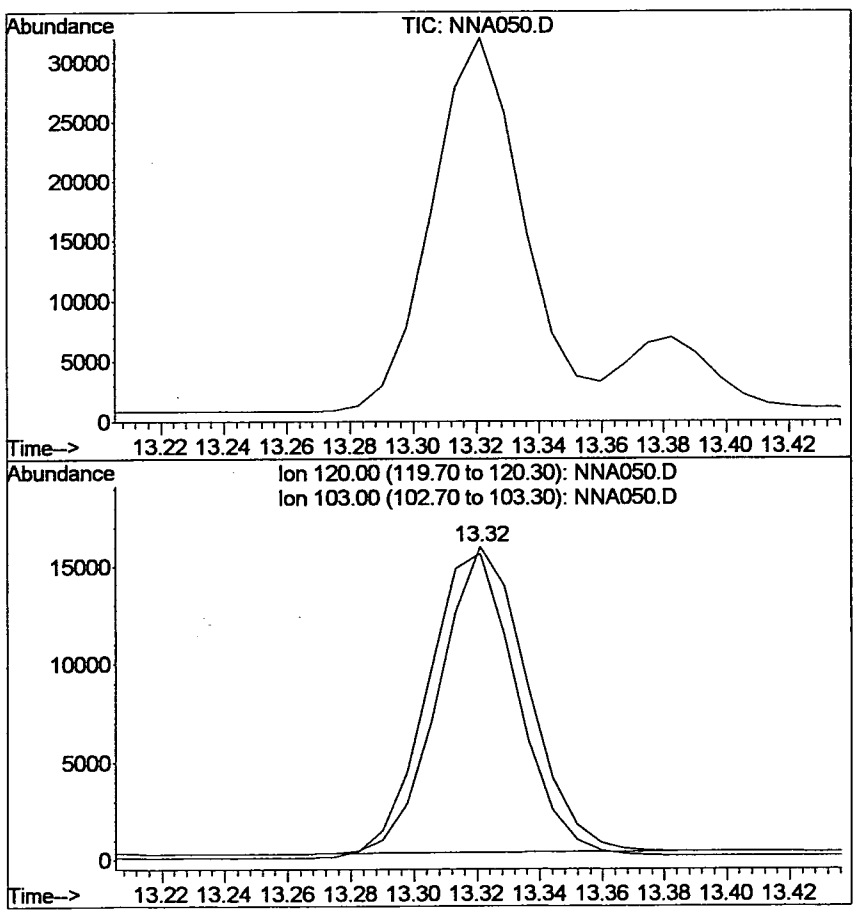

#4
NDEA
Concen: 48.57 PPB
RT: 13.32 min Scan# 486
Delta R.T. -0.00 min
Lab File: NNA050.D
Acq: 14 Jun 2007 10:47 am

Tgt Ion:120 Resp: 30485

Ion	Ratio	Lower	Upper
120	100		
103	101.6	65.3	135.5

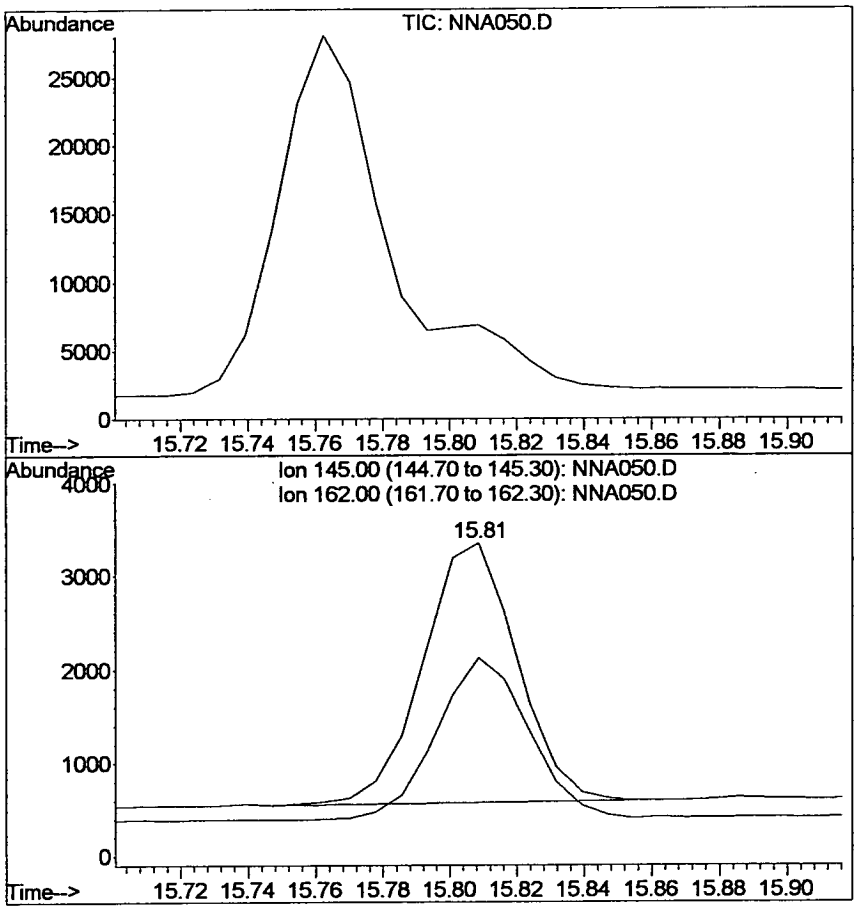

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.81 min Scan# 809
Delta R.T. -0.00 min
Lab File: NNA050.D
Acq: 14 Jun 2007 10:47 am

Tgt Ion:145 Resp: 5432

Ion	Ratio	Lower	Upper
145	100		
162	60.8	22.4	102.4

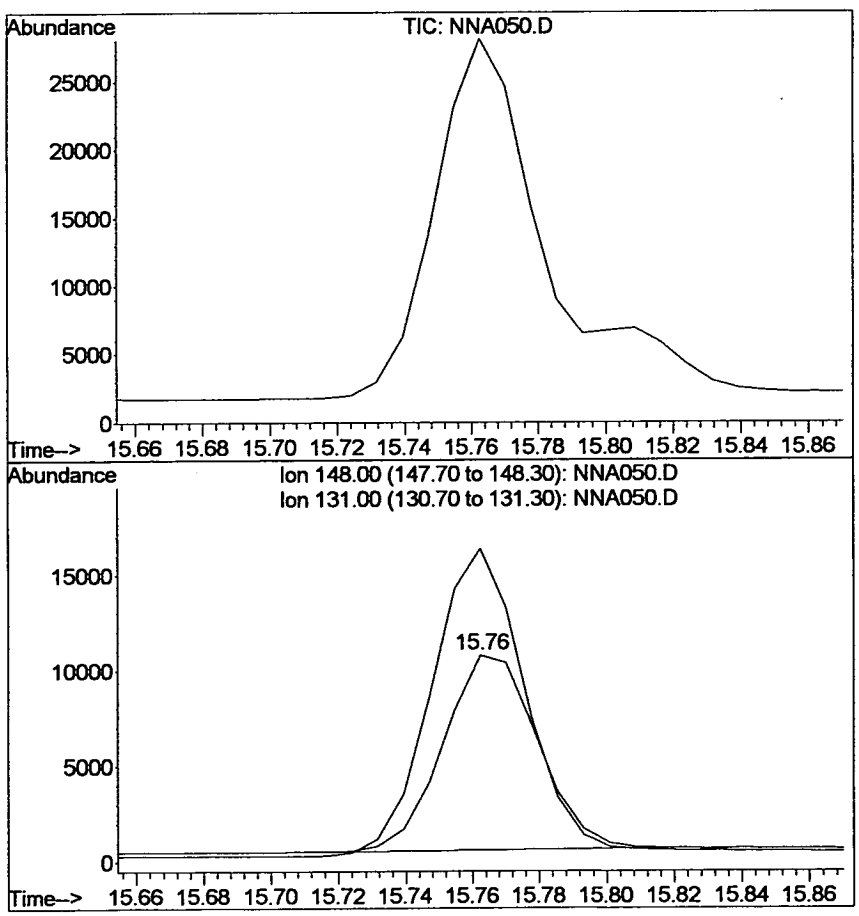

#6
NDPA
Concen: 43.69 PPB
RT: 15.76 min Scan# 803
Delta R.T. -0.01 min
Lab File: NNA050.D
Acq: 14 Jun 2007 10:47 am

Tgt Ion:148 Resp: 19990

Ion	Ratio	Lower	Upper
148	100		
131	161.6	99.8	207.2

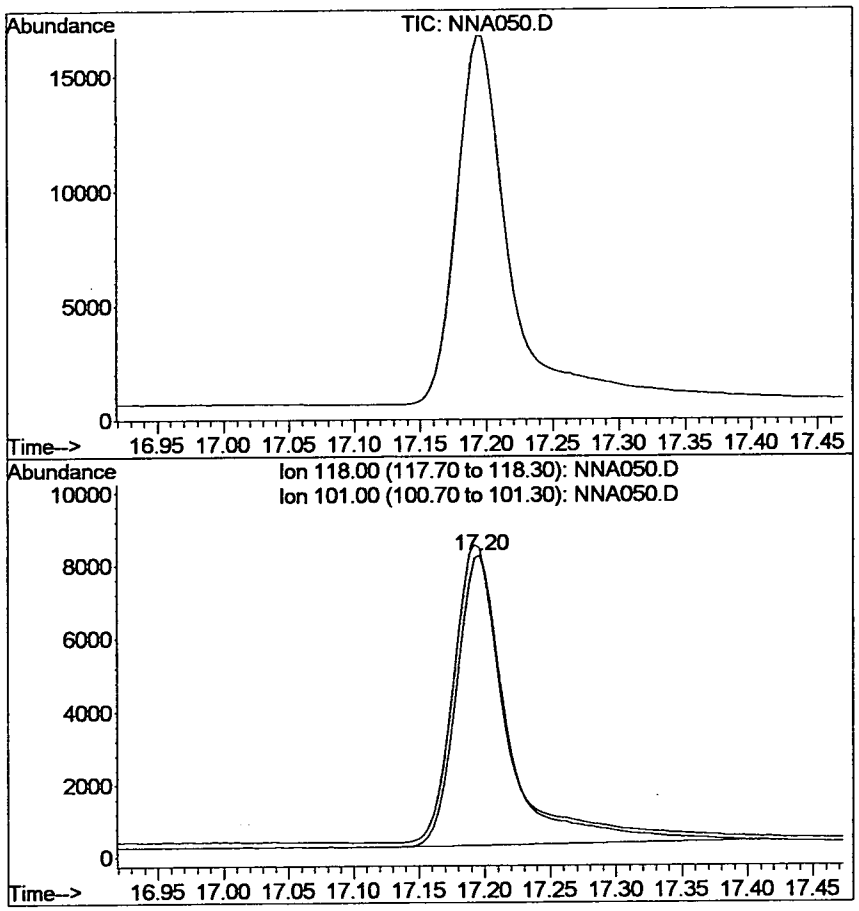

#7
NPYR
Concen: 49.98 PPB
RT: 17.20 min Scan# 1076
Delta R.T. -0.00 min
Lab File: NNA050.D
Acq: 14 Jun 2007 10:47 am

Tgt Ion:118 Resp: 21971

Ion	Ratio	Lower	Upper
118	100		
101	102.6	62.6	130.0

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA100.D Vial: 7
Acq On : 14 Jun 2007 11:11 am Operator: DF/AI
Sample : 100ppb Std.# 7060224 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:27 2007 Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration
DataAcq Meth : C7E29NWA

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) NDMA-D6	10.90	81	2989	10.00 PPB	0.00
3) NDEA-D10	13.38	113	5837	10.00 PPB	0.00
5) NDPA-D14	15.81	145	5188	10.00 PPB	0.00
Target Compounds					**Qvalue**
2) NDMA	10.84	92	60647	101.17 PPB	99
4) NDEA	13.32	120	62234	100.15 PPB	99
6) NDPA	15.76	148	40333	92.31 PPB	100
7) NPYR	17.20	118	48456	115.41 PPB	97

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA100.D Vial: 7
Acq On : 14 Jun 2007 11:11 am Operator: DF/AI
Sample : 100ppb Std.# 7060224 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:27 2007 Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration

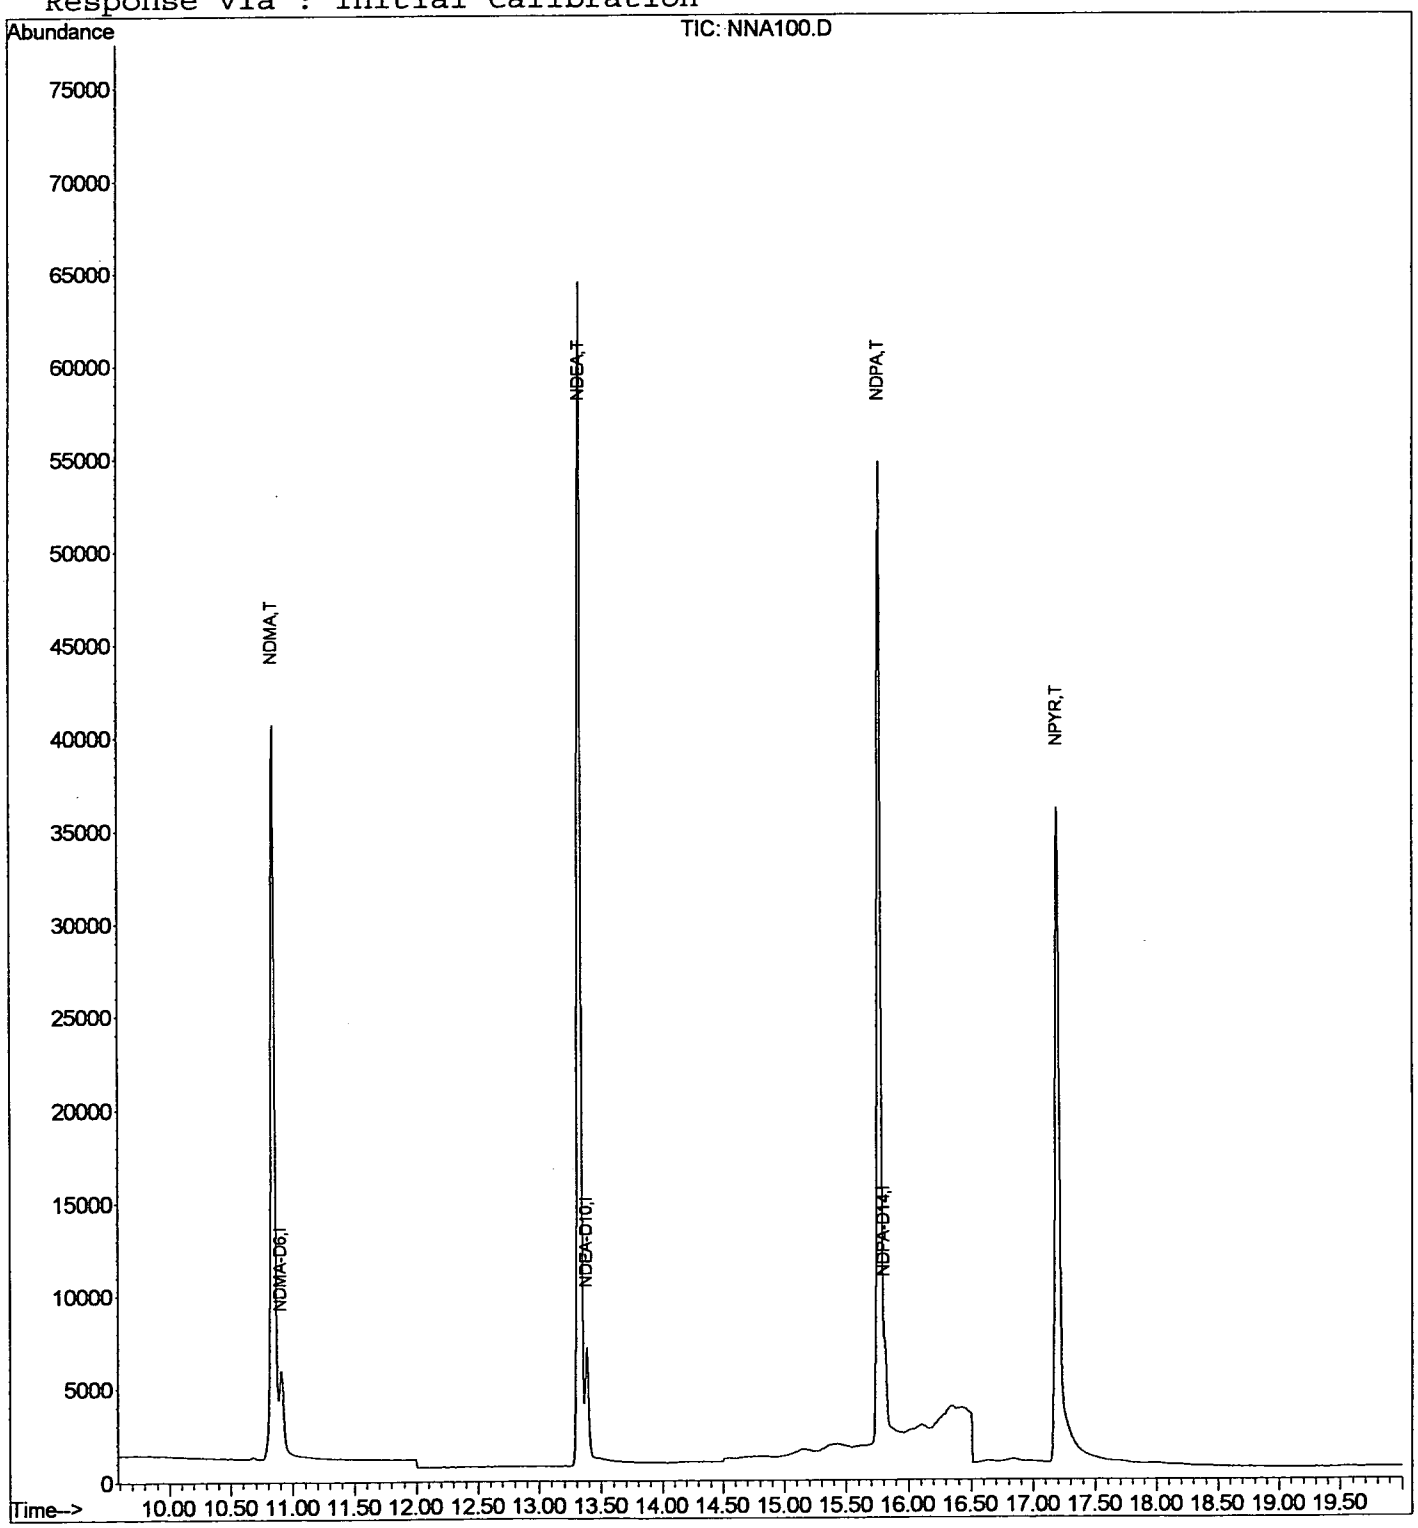

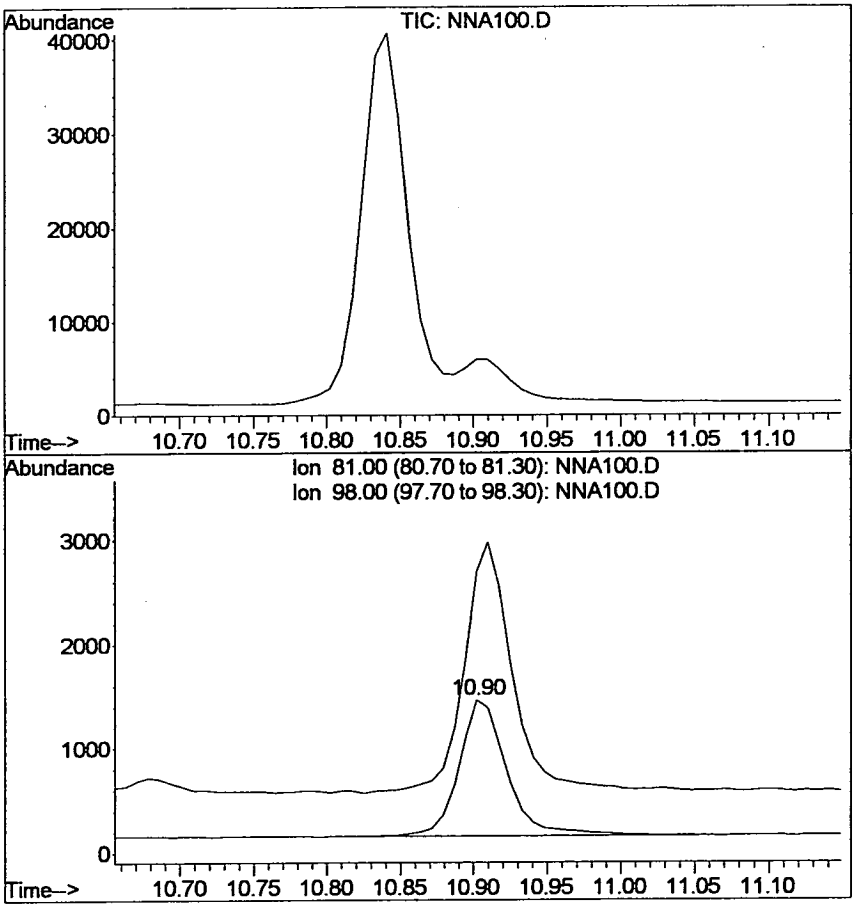

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.90 min Scan# 172
Delta R.T. -0.00 min
Lab File: NNA100.D
Acq: 14 Jun 2007 11:11 am

Tgt Ion: 81 Resp: 2989

Ion	Ratio	Lower	Upper
81	100		
98	179.9	144.1	224.1

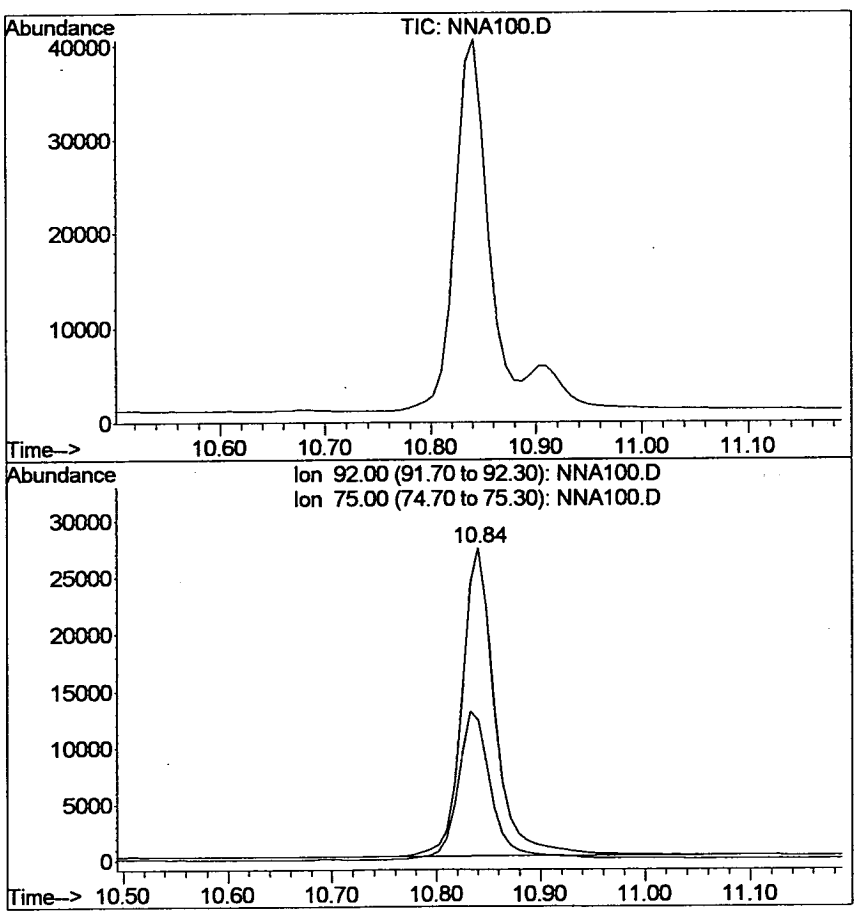

#2
NDMA
Concen: 101.17 PPB
RT: 10.84 min Scan# 164
Delta R.T. 0.01 min
Lab File: NNA100.D
Acq: 14 Jun 2007 11:11 am

Tgt Ion: 92 Resp: 60647

Ion	Ratio	Lower	Upper
92	100		
75	48.5	31.8	66.0

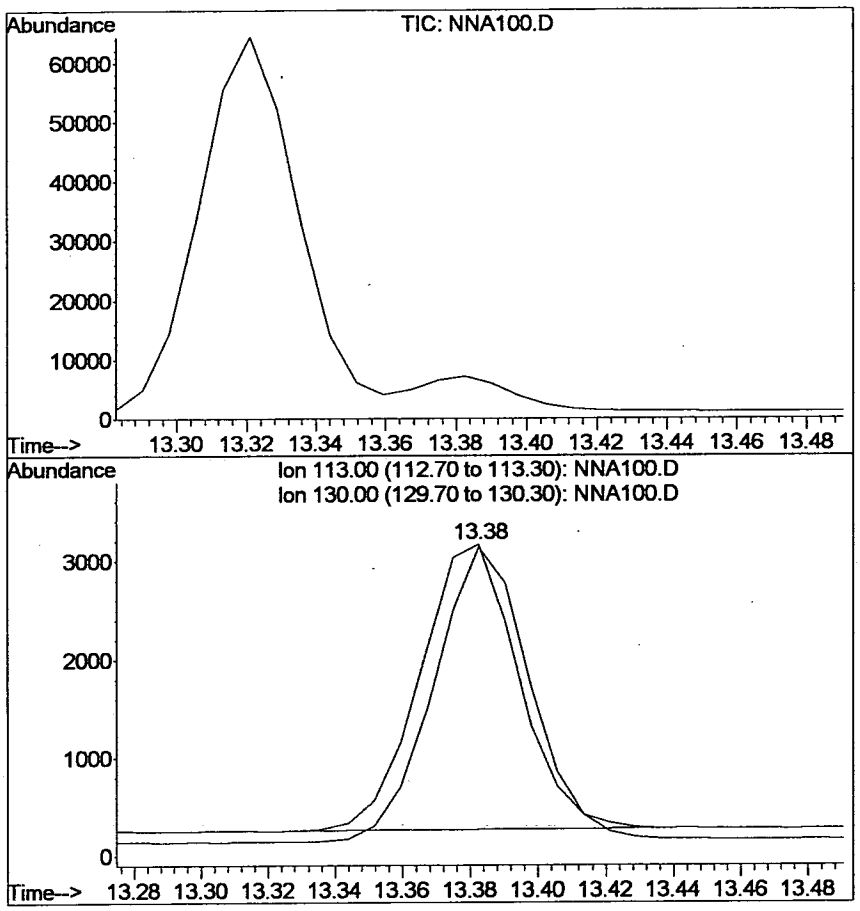

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.38 min Scan# 494
Delta R.T. 0.01 min
Lab File: NNA100.D
Acq: 14 Jun 2007 11:11 am

Tgt Ion:113 Resp: 5837

Ion	Ratio	Lower	Upper
113	100		
130	100.3	67.1	137.1

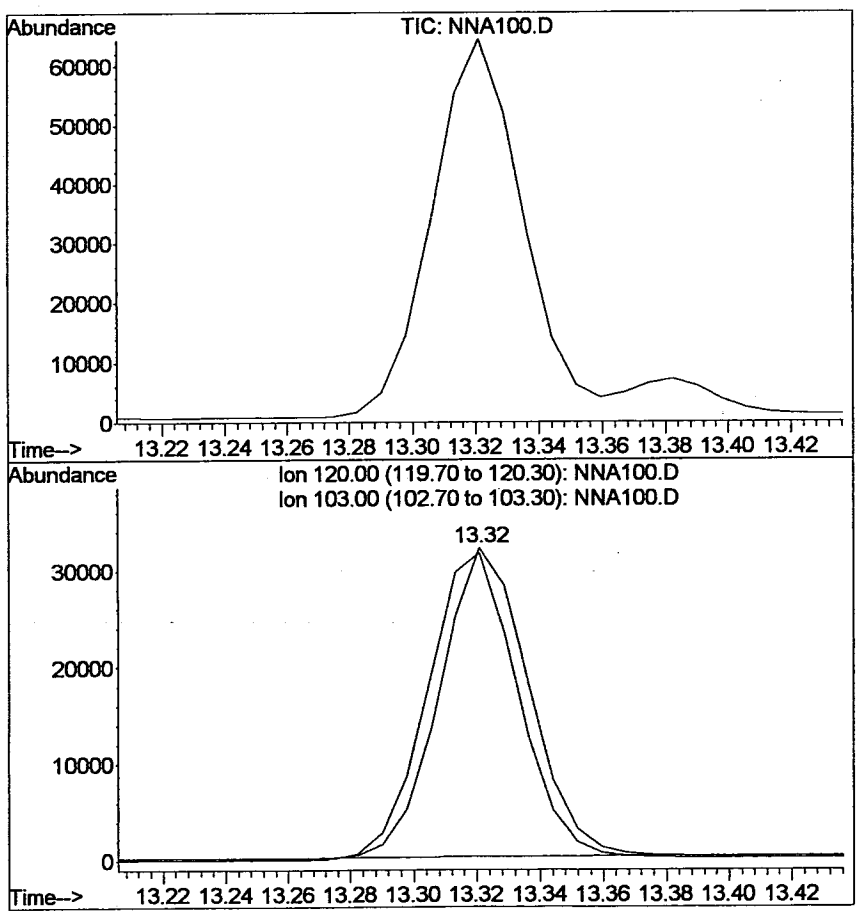

#4
NDEA
Concen: 100.15 PPB
RT: 13.32 min Scan# 486
Delta R.T. -0.00 min
Lab File: NNA100.D
Acq: 14 Jun 2007 11:11 am

Tgt Ion:120 Resp: 62234

Ion	Ratio	Lower	Upper
120	100		
103	101.0	65.3	135.5

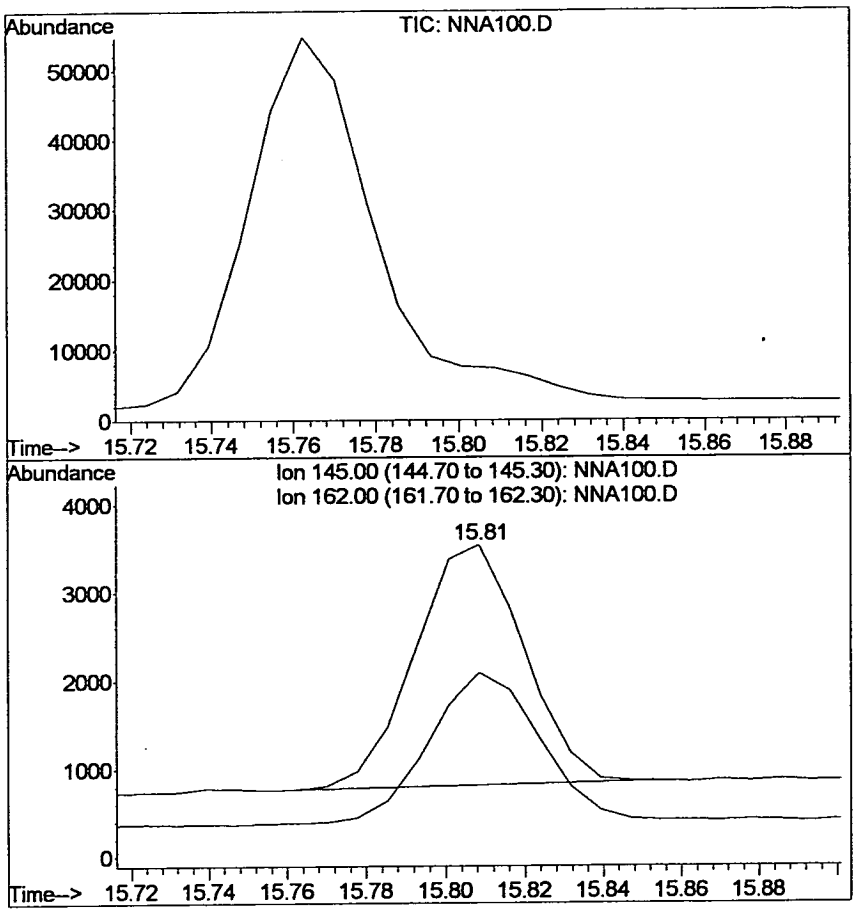

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.81 min Scan# 809
Delta R.T. -0.00 min
Lab File: NNA100.D
Acq: 14 Jun 2007 11:11 am

Tgt Ion:145 Resp: 5188

Ion	Ratio	Lower	Upper
145	100		
162	63.0	22.4	102.4

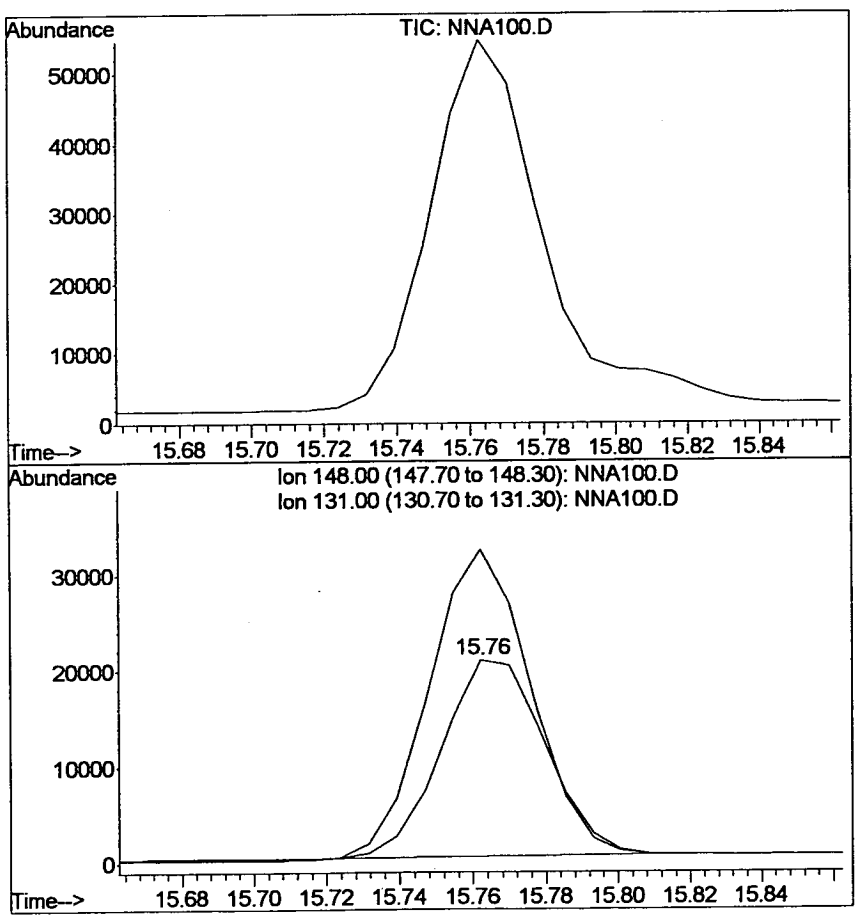

#6
NDPA
Concen: 92.31 PPB
RT: 15.76 min Scan# 803
Delta R.T. -0.01 min
Lab File: NNA100.D
Acq: 14 Jun 2007 11:11 am

Tgt Ion:148 Resp: 40333

Ion	Ratio	Lower	Upper
148	100		
131	153.0	99.8	207.2

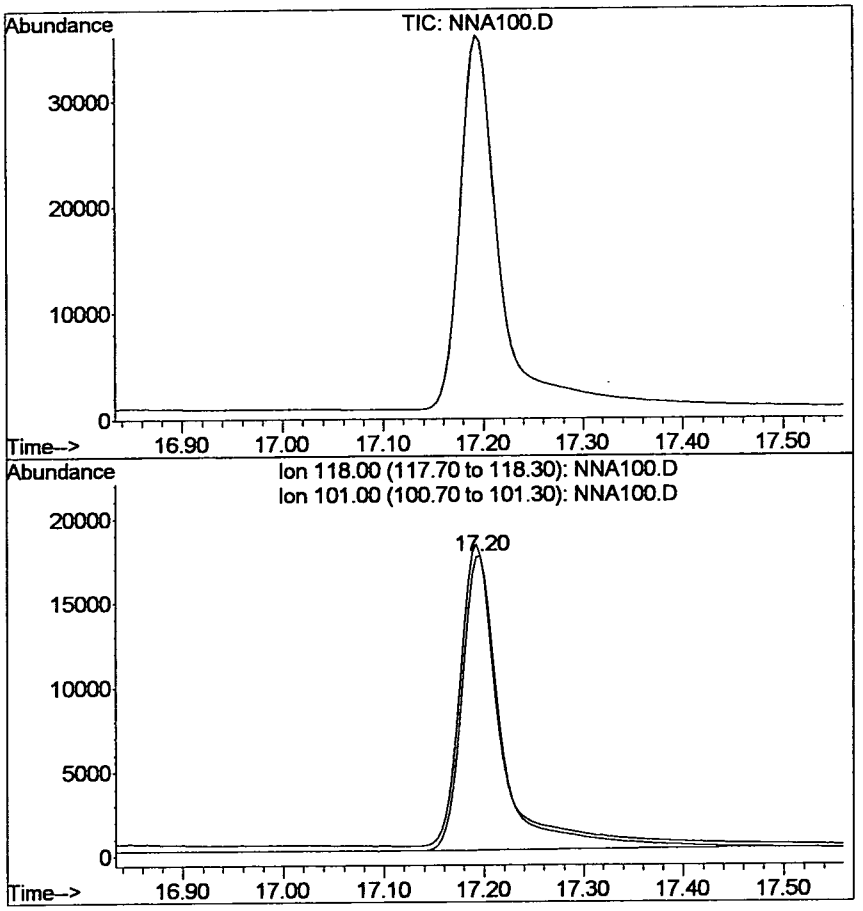

#7
NPYR
Concen: 115.41 PPB
RT: 17.20 min Scan# 1076
Delta R.T. -0.00 min
Lab File: NNA100.D
Acq: 14 Jun 2007 11:11 am

Tgt Ion:118 Resp: 48456

Ion	Ratio	Lower	Upper
118	100		
101	99.7	62.6	130.0

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA150.D Vial: 8
Acq On : 14 Jun 2007 11:34 am Operator: DF/AI
Sample : 150ppb Std.# 7060225 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:27 2007 Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration
DataAcq Meth : C7E29NWA

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) NDMA-D6	10.90	81	3079	10.00 PPB	0.00
3) NDEA-D10	13.38	113	5791	10.00 PPB	0.00
5) NDPA-D14	15.81	145	5290	10.00 PPB	0.00
Target Compounds					**Qvalue**
2) NDMA	10.84	92	90278	146.20 PPB	99
4) NDEA	13.32	120	91277	148.05 PPB	99
6) NDPA	15.76	148	58976	132.37 PPB	99
7) NPYR	17.20	118	71527	167.07 PPB	96

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA150.D Vial: 8
Acq On : 14 Jun 2007 11:34 am Operator: DF/AI
Sample : 150ppb Std.# 7060225 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:27 2007 Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration

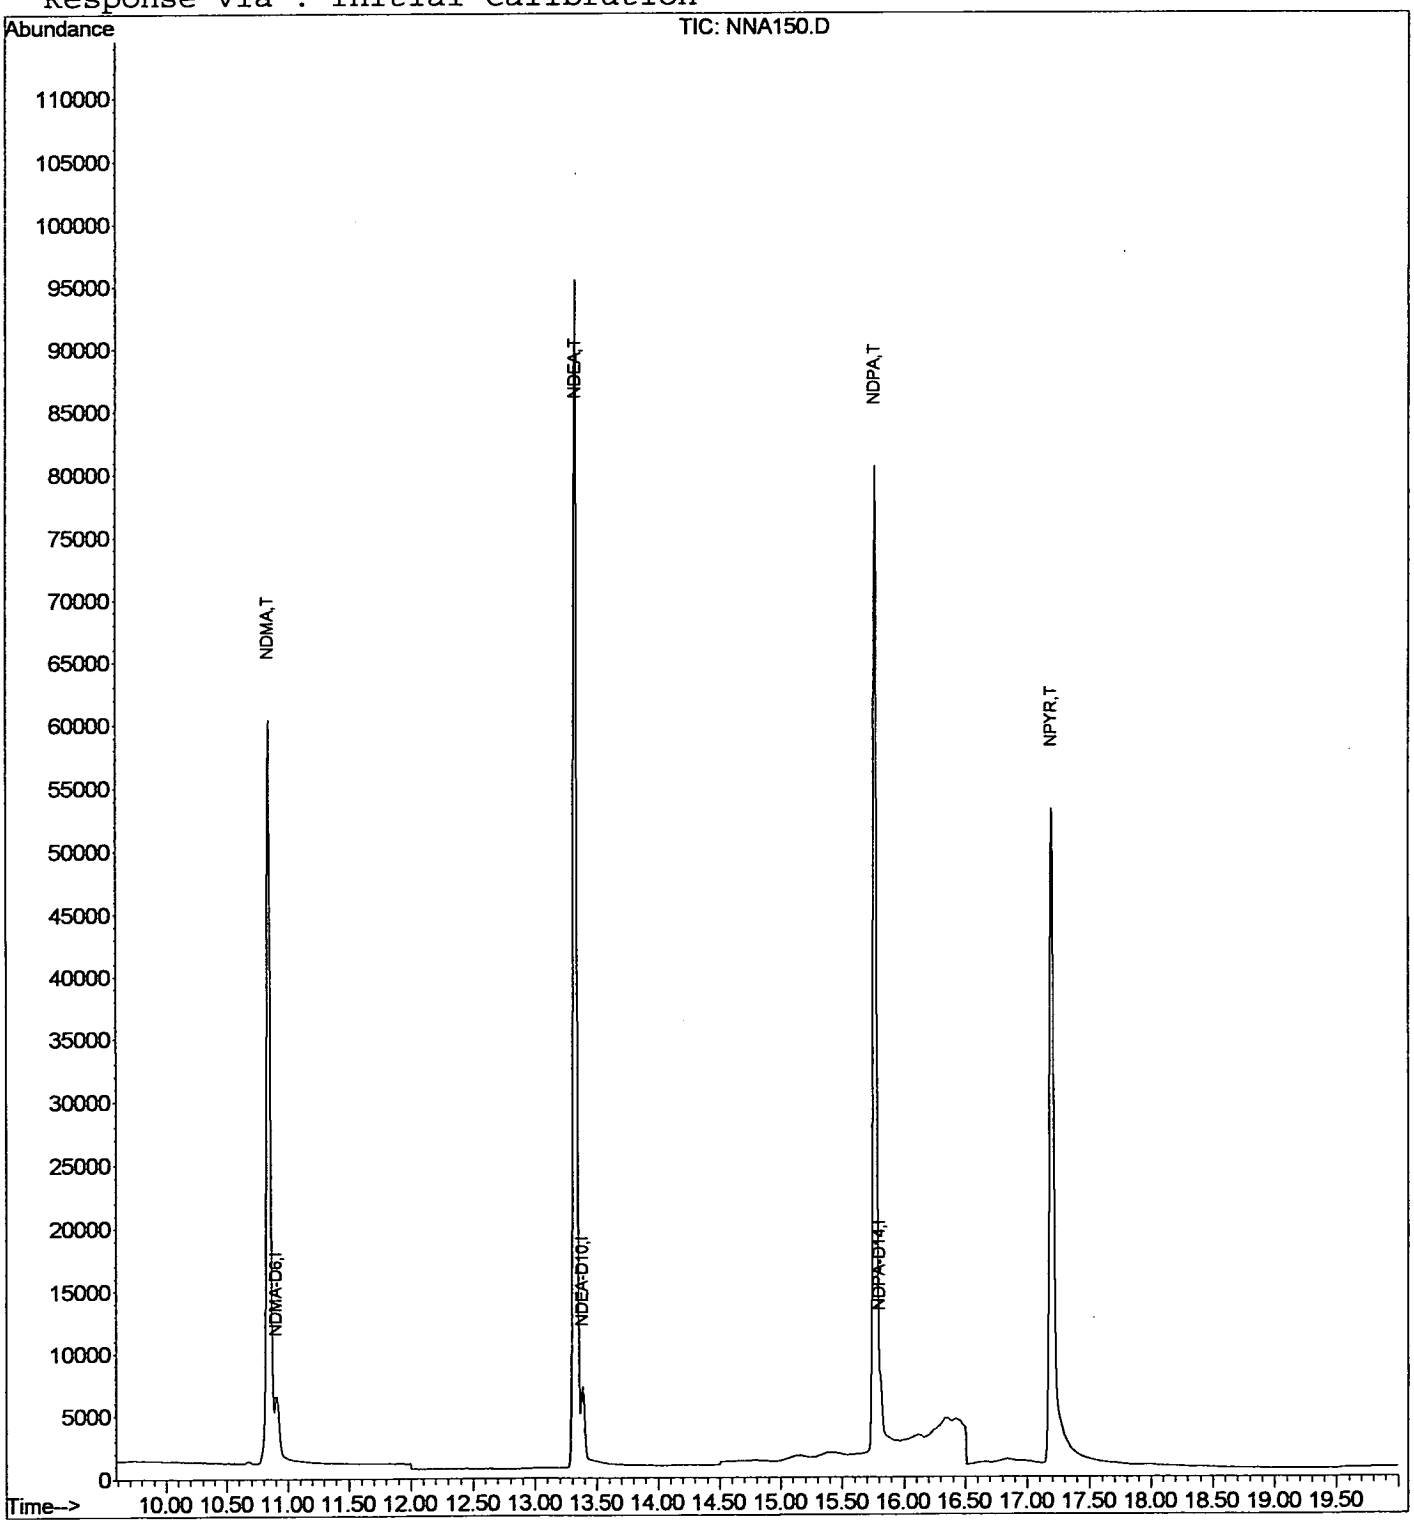

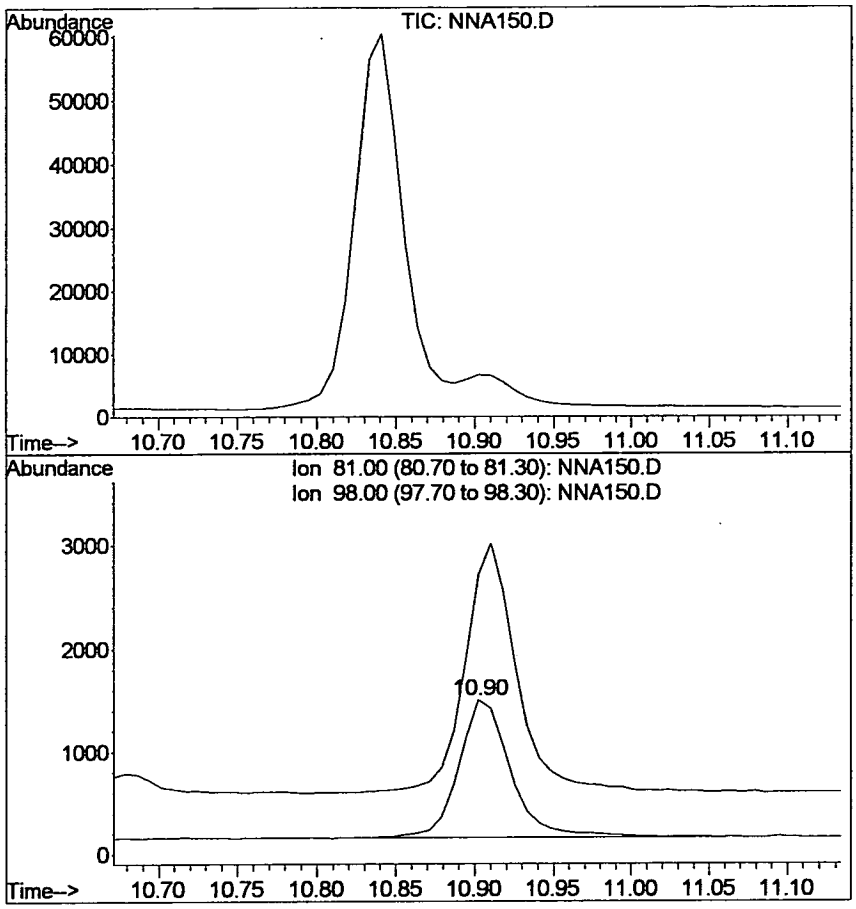

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.90 min Scan# 172
Delta R.T. 0.00 min
Lab File: NNA150.D
Acq: 14 Jun 2007 11:34 am

Tgt Ion: 81 Resp: 3079

Ion	Ratio	Lower	Upper
81	100		
98	178.5	144.1	224.1

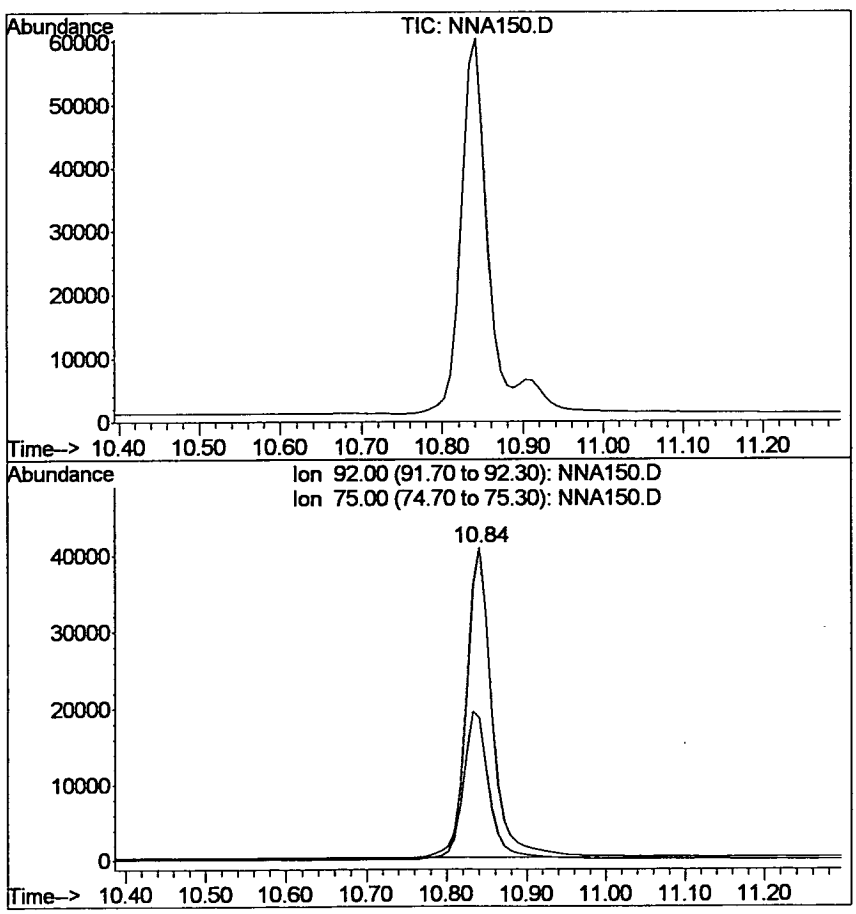

#2
NDMA
Concen: 146.20 PPB
RT: 10.84 min Scan# 164
Delta R.T. 0.01 min
Lab File: NNA150.D
Acq: 14 Jun 2007 11:34 am

Tgt Ion: 92 Resp: 90278

Ion	Ratio	Lower	Upper
92	100		
75	48.5	31.8	66.0

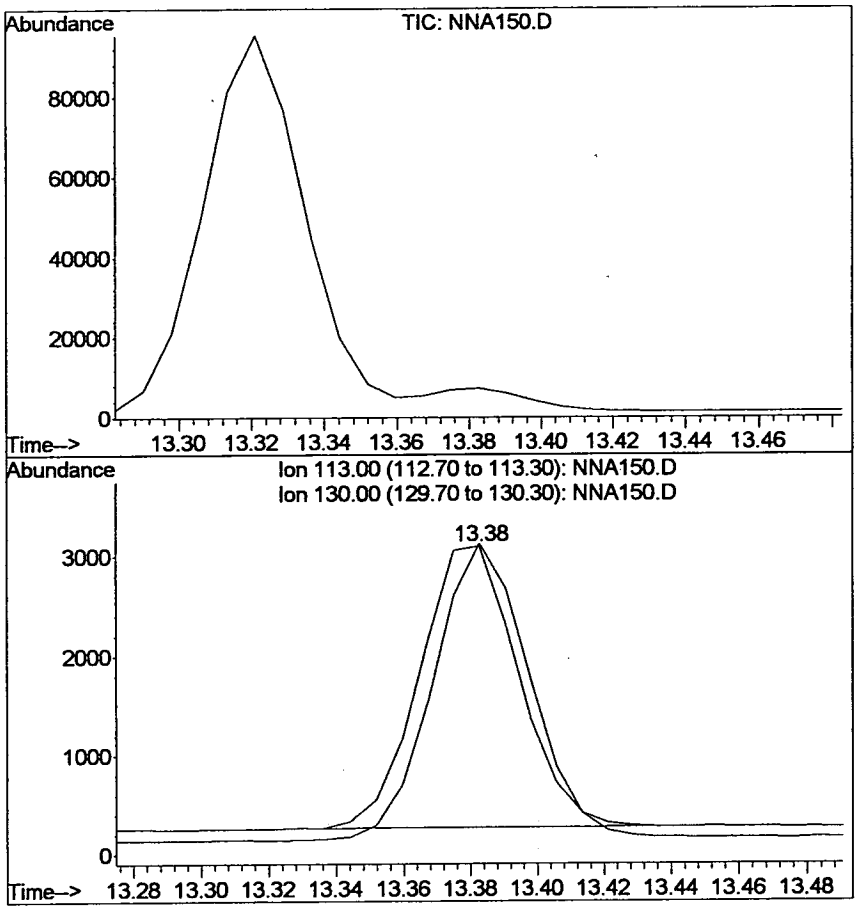

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.38 min Scan# 494
Delta R.T. 0.01 min
Lab File: NNA150.D
Acq: 14 Jun 2007 11:34 am

Tgt Ion:113 Resp: 5791

Ion	Ratio	Lower	Upper
113	100		
130	101.4	67.1	137.1

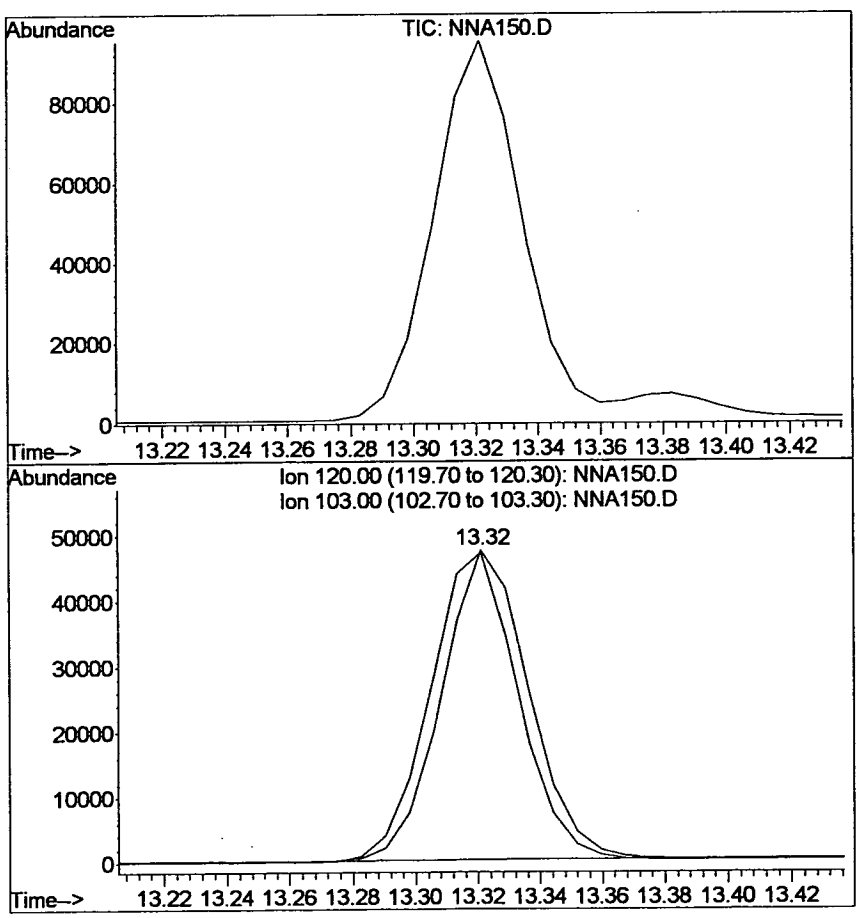

#4
NDEA
Concen: 148.05 PPB
RT: 13.32 min Scan# 486
Delta R.T. 0.00 min
Lab File: NNA150.D
Acq: 14 Jun 2007 11:34 am

Tgt Ion:120 Resp: 91277

Ion	Ratio	Lower	Upper
120	100		
103	101.2	65.3	135.5

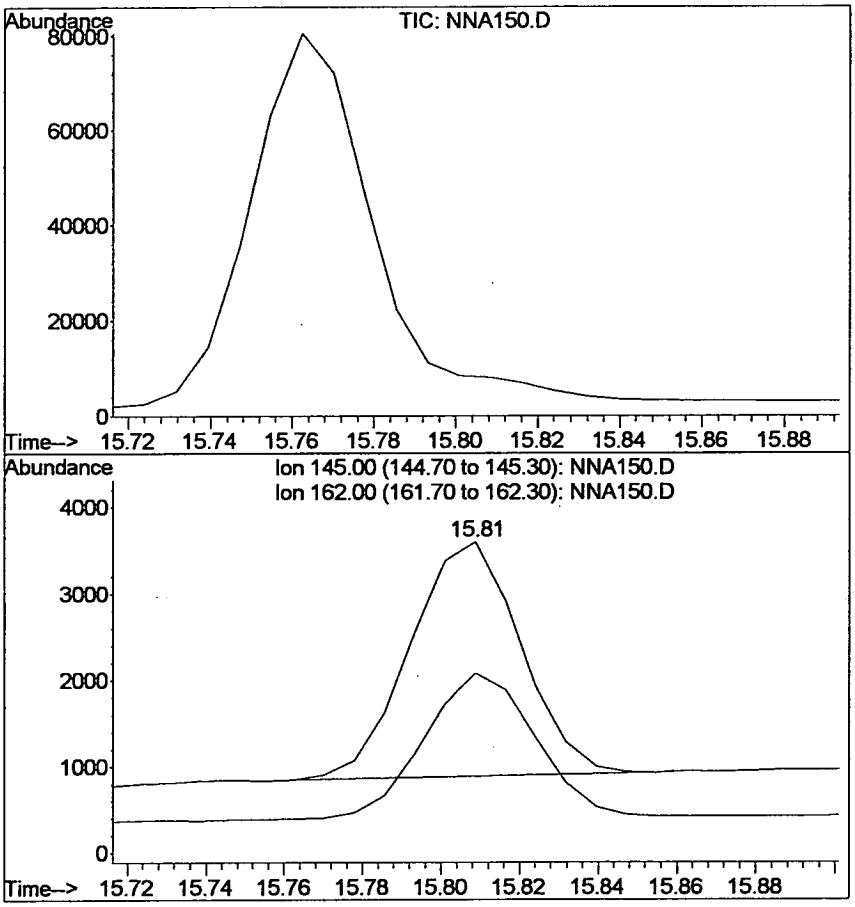

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.81 min Scan# 809
Delta R.T. 0.00 min
Lab File: NNA150.D
Acq: 14 Jun 2007 11:34 am

Tgt Ion:145 Resp: 5290

Ion	Ratio	Lower	Upper
145	100		
162	62.2	22.4	102.4

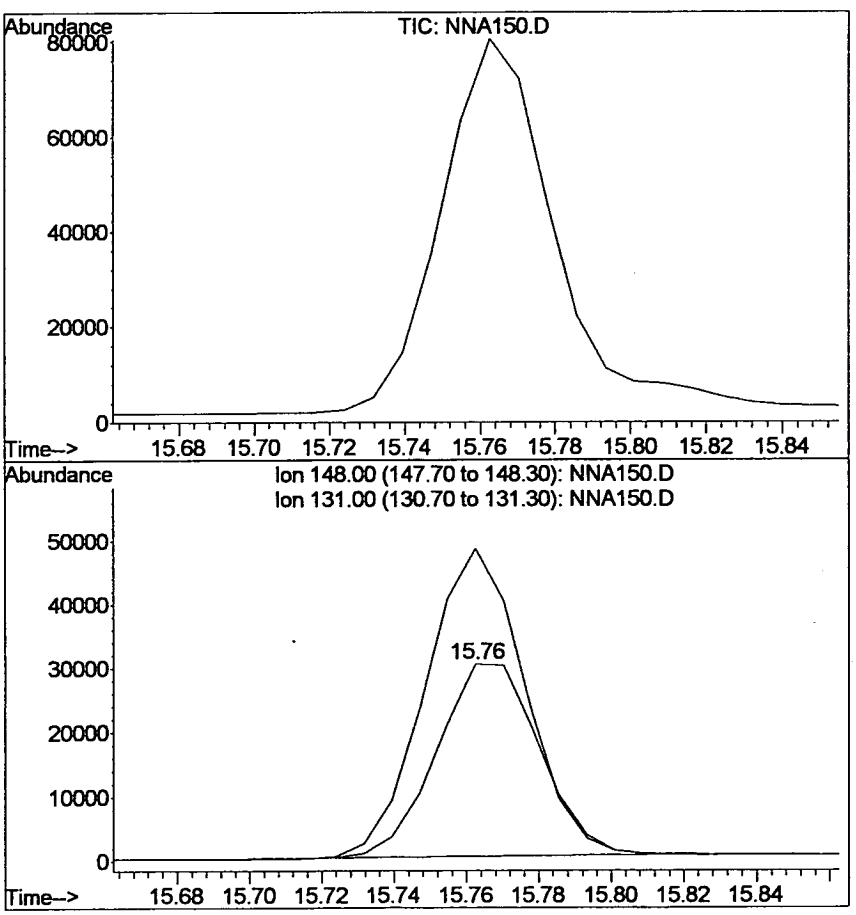

#6
NDPA
Concen: 132.37 PPB
RT: 15.76 min Scan# 803
Delta R.T. -0.01 min
Lab File: NNA150.D
Acq: 14 Jun 2007 11:34 am

Tgt Ion:148 Resp: 58976

Ion	Ratio	Lower	Upper
148	100		
131	154.7	99.8	207.2

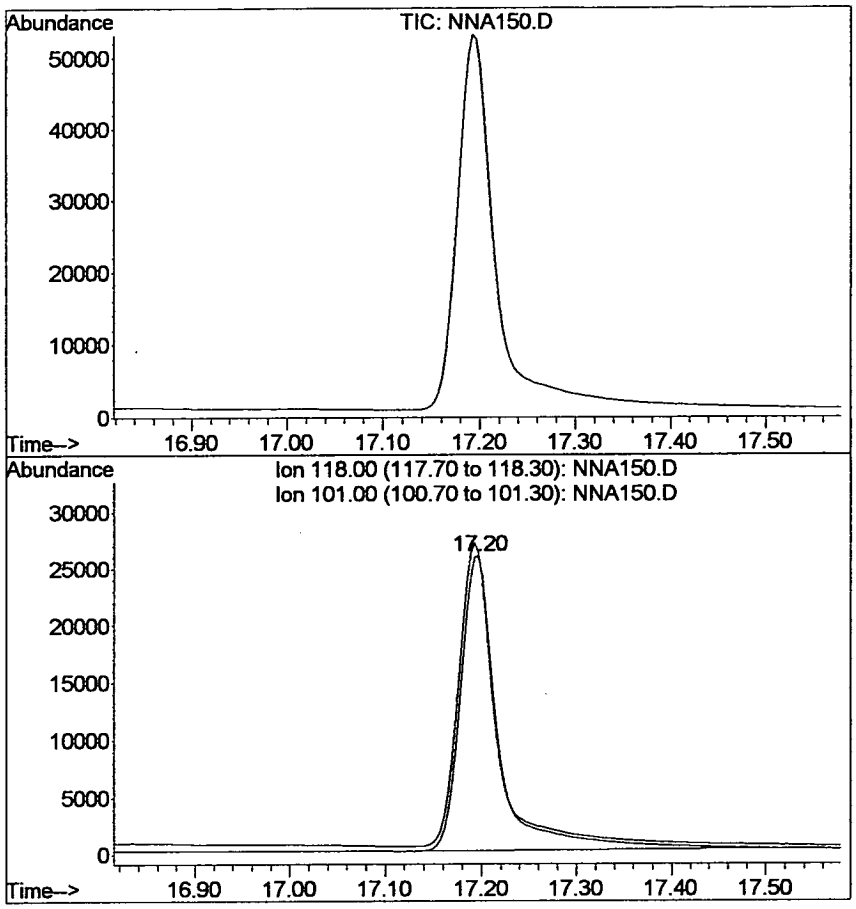

#7
NPYR
Concen: 167.07 PPB
RT: 17.20 min Scan# 1076
Delta R.T. 0.00 min
Lab File: NNA150.D
Acq: 14 Jun 2007 11:34 am

Tgt Ion:118 Resp: 71527

Ion	Ratio	Lower	Upper
118	100		
101	100.2	62.6	130.0

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA200.D Vial: 9
Acq On : 14 Jun 2007 11:58 am Operator: DF/AI
Sample : 200ppb Std.# 7060226 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:27 2007 Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration
DataAcq Meth : C7E29NWA

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) NDMA-D6	10.90	81	3031	10.00 PPB	0.00
3) NDEA-D10	13.38	113	5900	10.00 PPB	0.00
5) NDPA-D14	15.81	145	5851	10.00 PPB	0.00
Target Compounds					**Qvalue**
2) NDMA	10.84	92	123053	202.44 PPB	99
4) NDEA	13.32	120	126080	200.72 PPB	99
6) NDPA	15.76	148	86380	175.29 PPB	100
7) NPYR	17.19	118	101631	214.63 PPB	96

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA200.D Vial: 9
Acq On : 14 Jun 2007 11:58 am Operator: DF/AI
Sample : 200ppb Std.# 7060226 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:27 2007 Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration

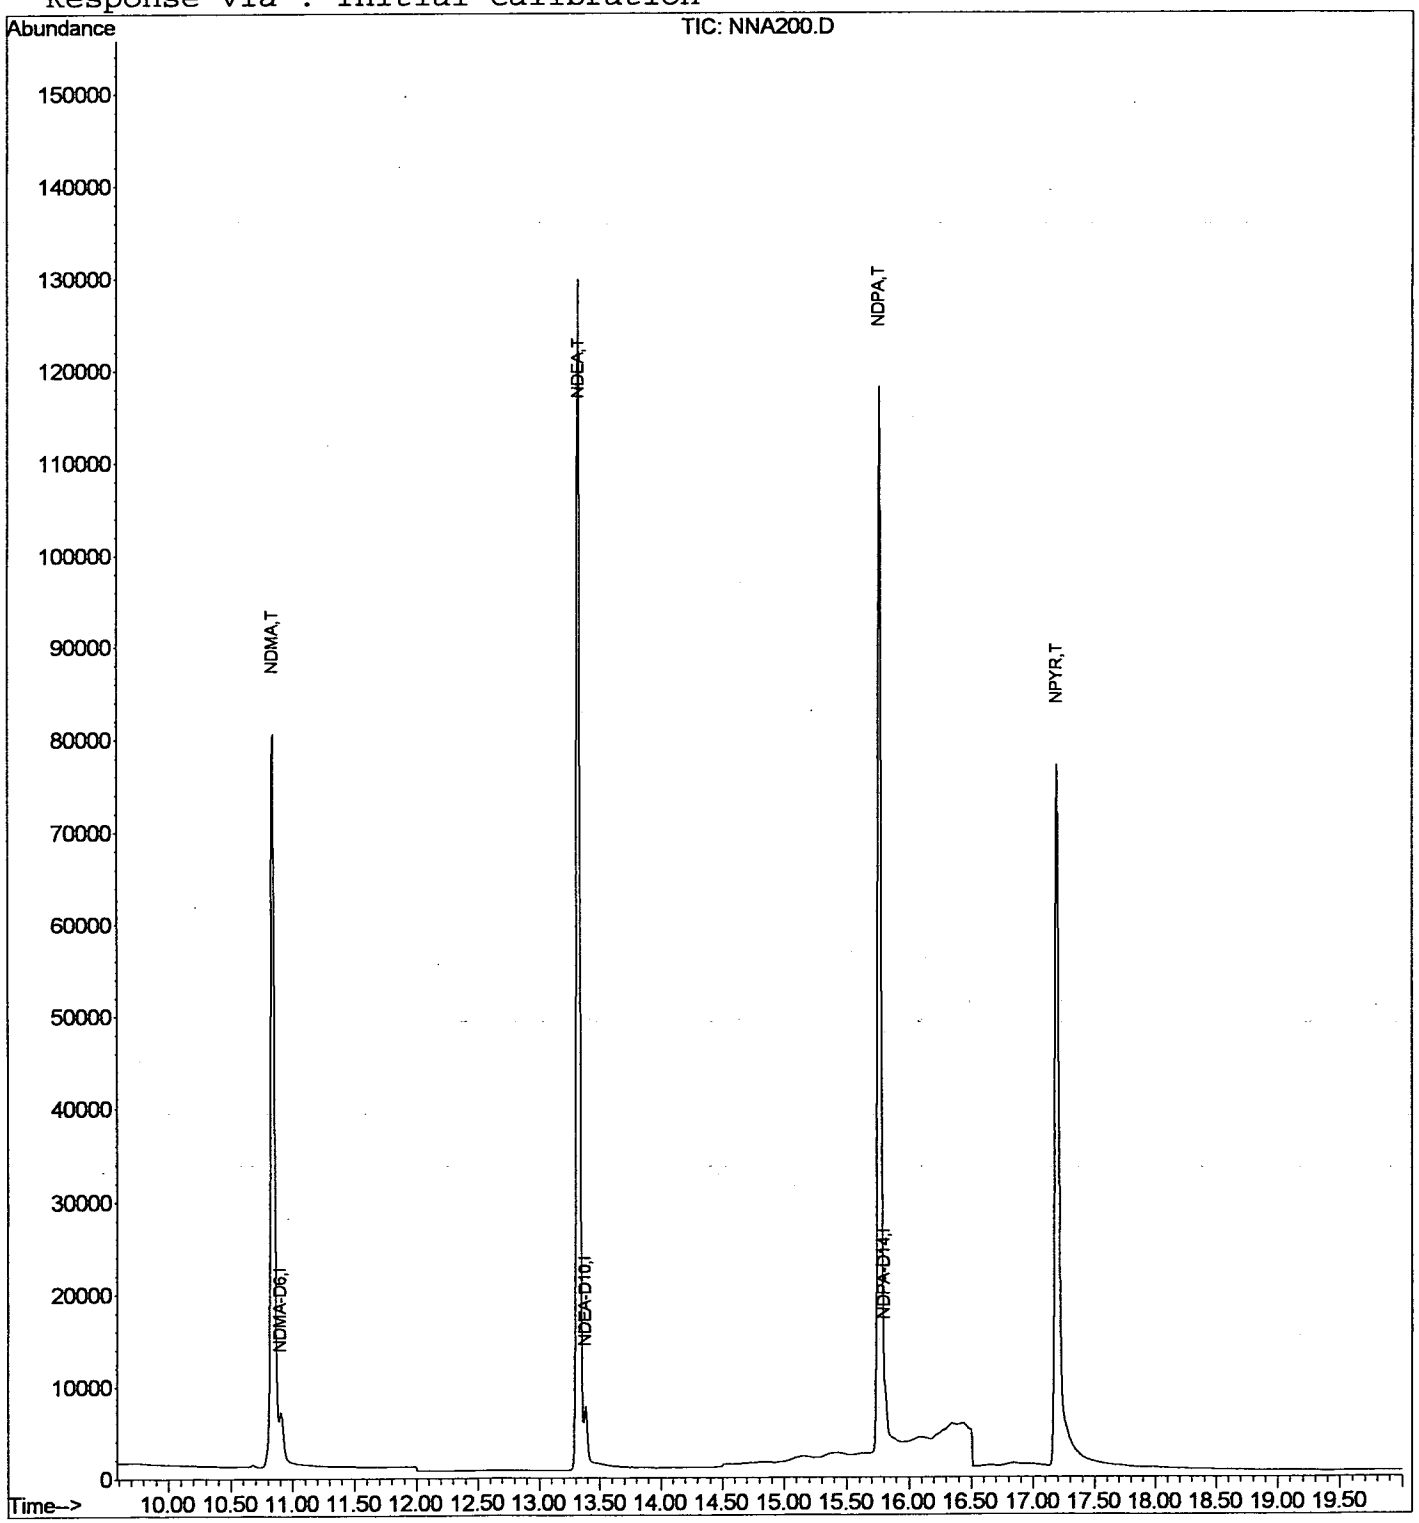

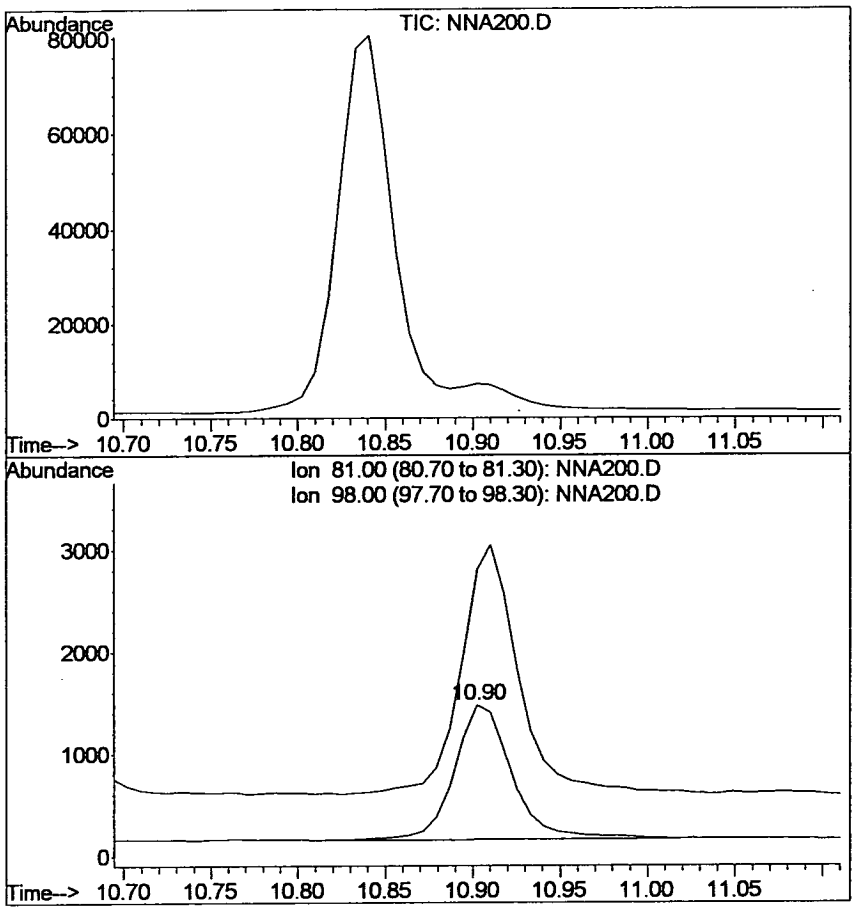

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.90 min Scan# 172
Delta R.T. 0.00 min
Lab File: NNA200.D
Acq: 14 Jun 2007 11:58 am

Tgt Ion: 81 Resp: 3031

Ion	Ratio	Lower	Upper
81	100		
98	183.9	144.1	224.1

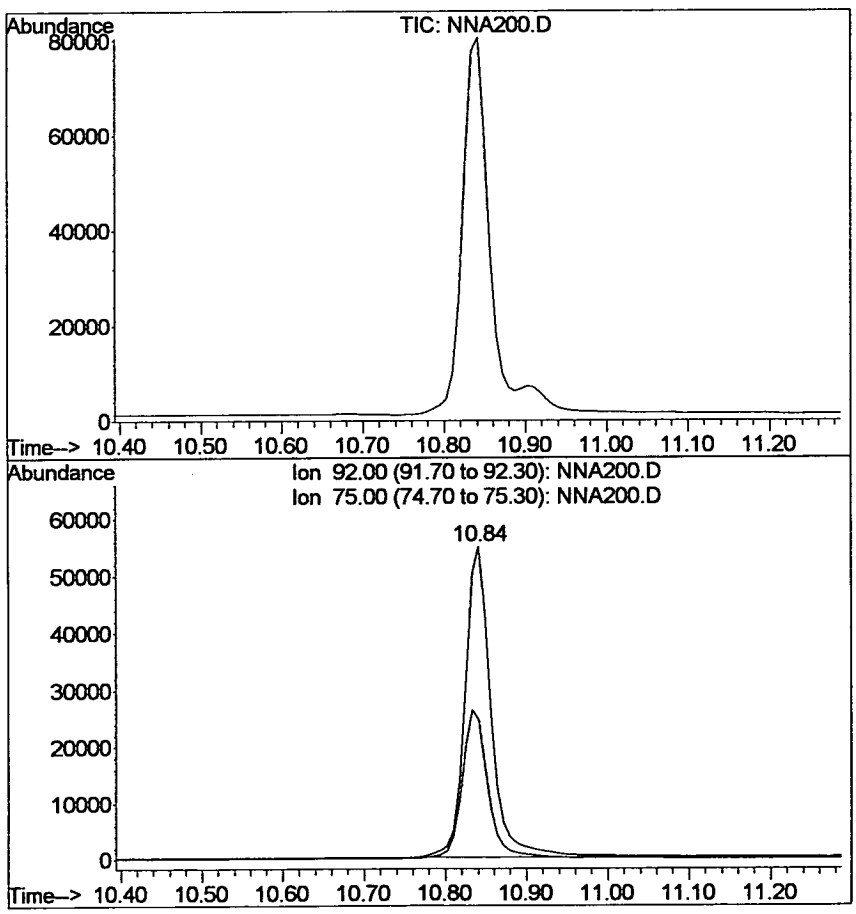

#2
NDMA
Concen: 202.44 PPB
RT: 10.84 min Scan# 164
Delta R.T. 0.01 min
Lab File: NNA200.D
Acq: 14 Jun 2007 11:58 am

Tgt Ion: 92 Resp: 123053

Ion	Ratio	Lower	Upper
92	100		
75	48.5	31.8	66.0

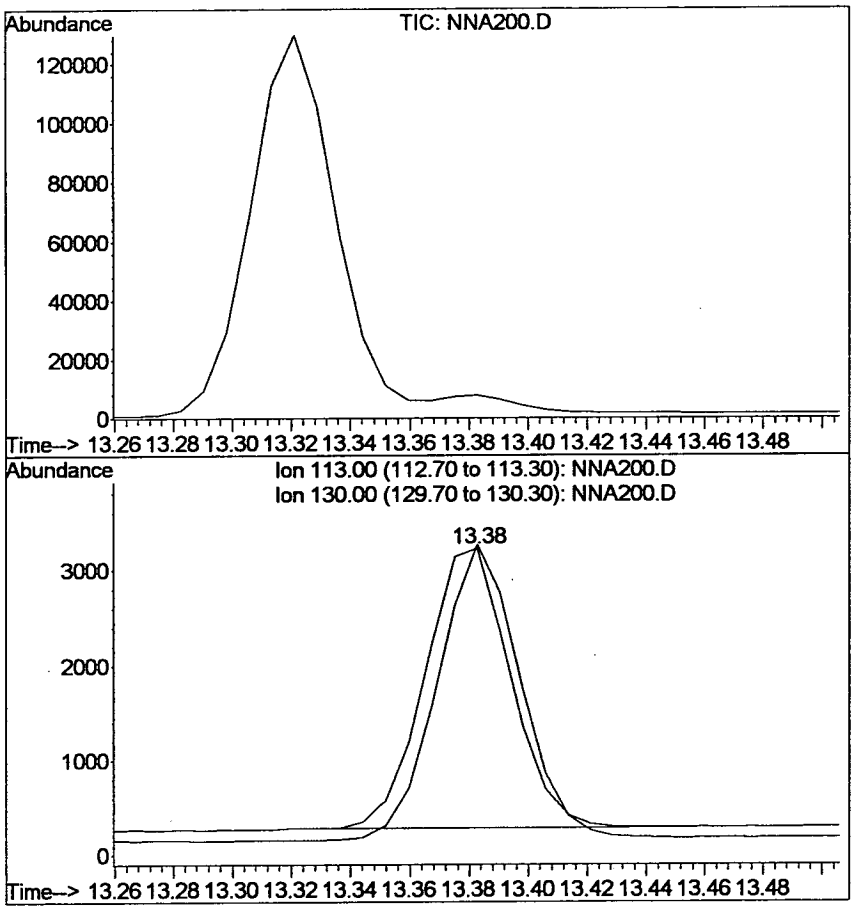

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.38 min Scan# 494
Delta R.T. 0.01 min
Lab File: NNA200.D
Acq: 14 Jun 2007 11:58 am

Tgt Ion:113 Resp: 5900

Ion	Ratio	Lower	Upper
113	100		
130	101.2	67.1	137.1

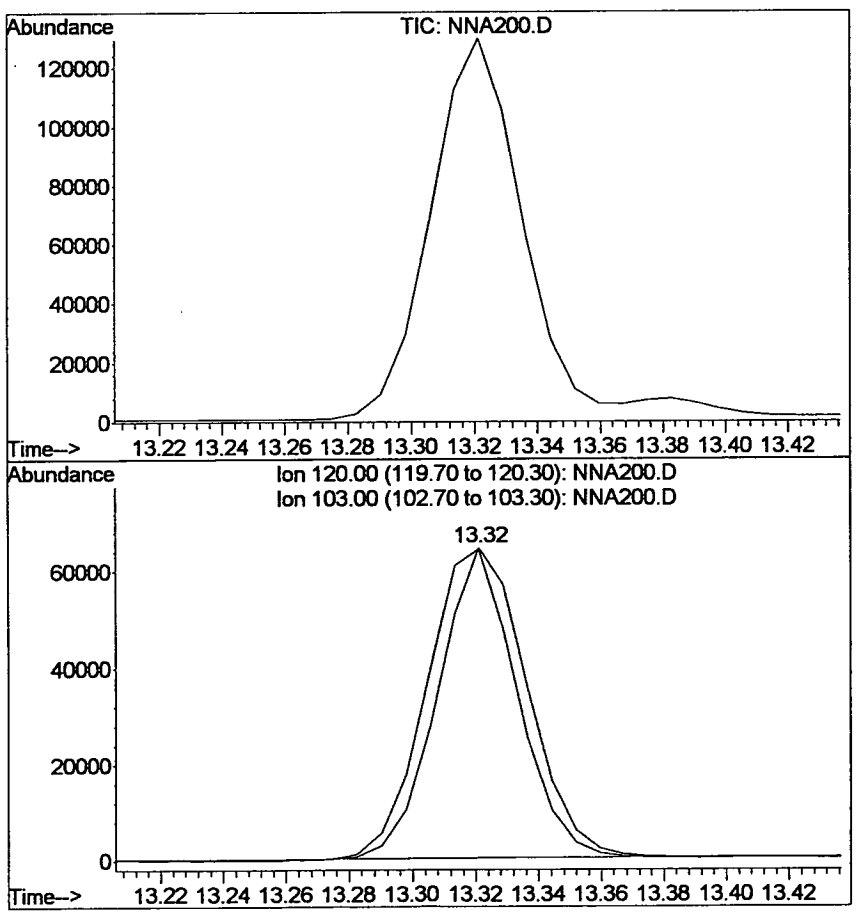

#4
NDEA
Concen: 200.72 PPB
RT: 13.32 min Scan# 486
Delta R.T. 0.00 min
Lab File: NNA200.D
Acq: 14 Jun 2007 11:58 am

Tgt Ion:120 Resp: 126080

Ion	Ratio	Lower	Upper
120	100		
103	101.7	65.3	135.5

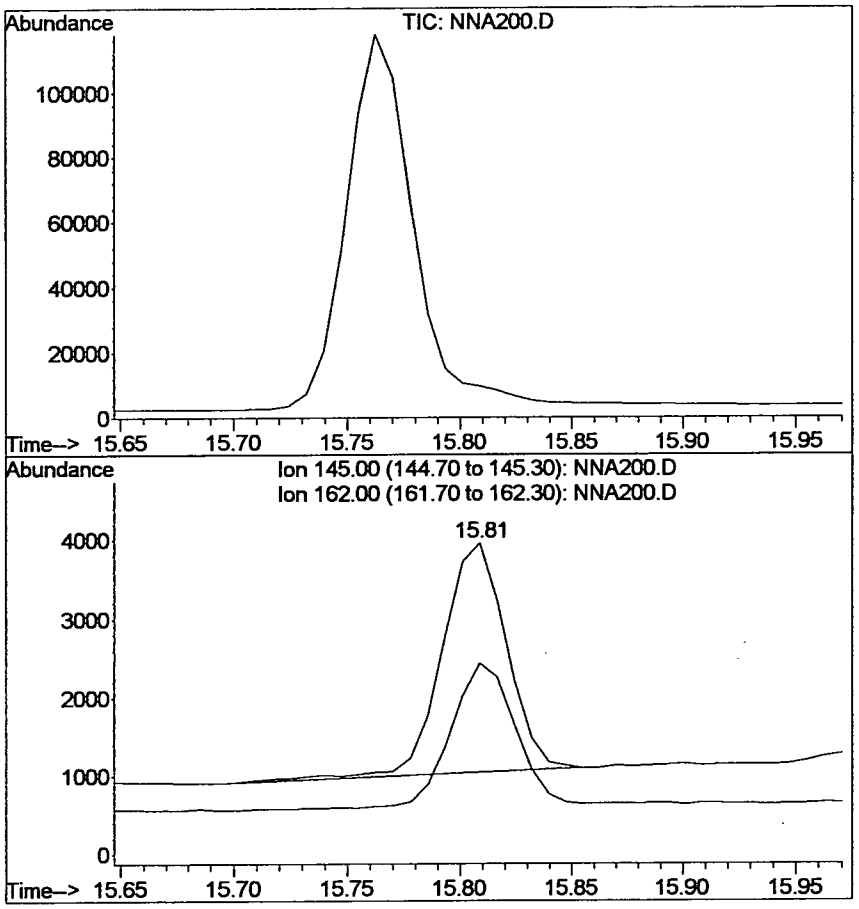

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.81 min Scan# 809
Delta R.T. 0.00 min
Lab File: NNA200.D
Acq: 14 Jun 2007 11:58 am

Tgt Ion:145 Resp: 5851

Ion	Ratio	Lower	Upper
145	100		
162	59.9	22.4	102.4

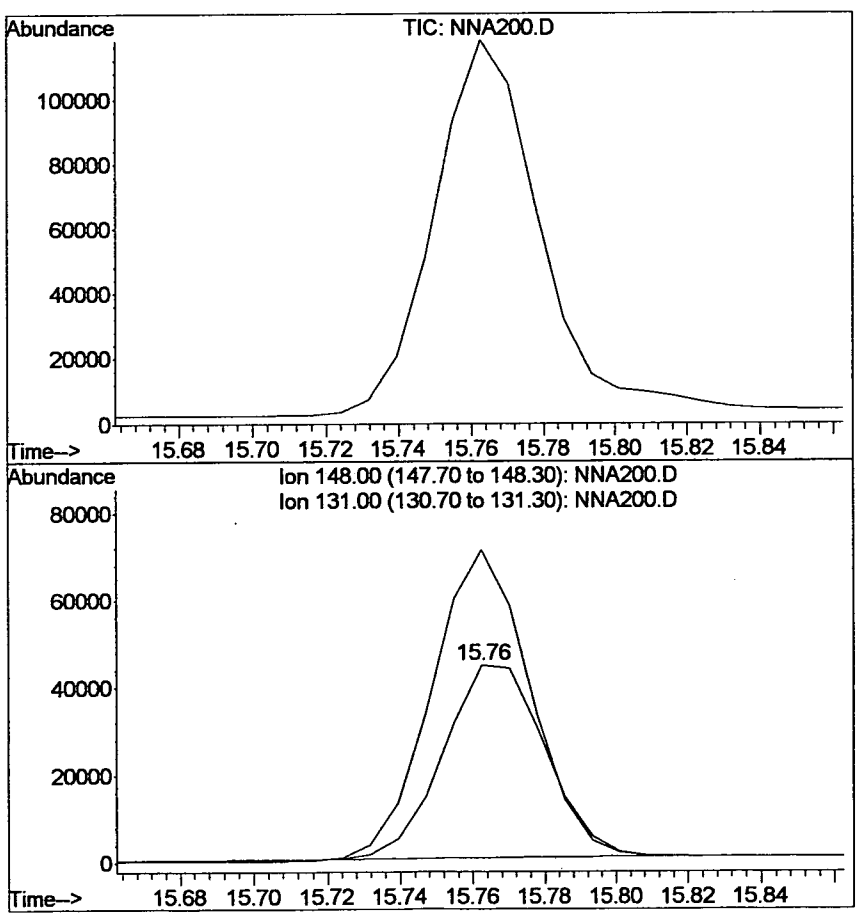

#6
NDPA
Concen: 175.29 PPB
RT: 15.76 min Scan# 803
Delta R.T. -0.01 min
Lab File: NNA200.D
Acq: 14 Jun 2007 11:58 am

Tgt Ion:148 Resp: 86380

Ion	Ratio	Lower	Upper
148	100		
131	154.1	99.8	207.2

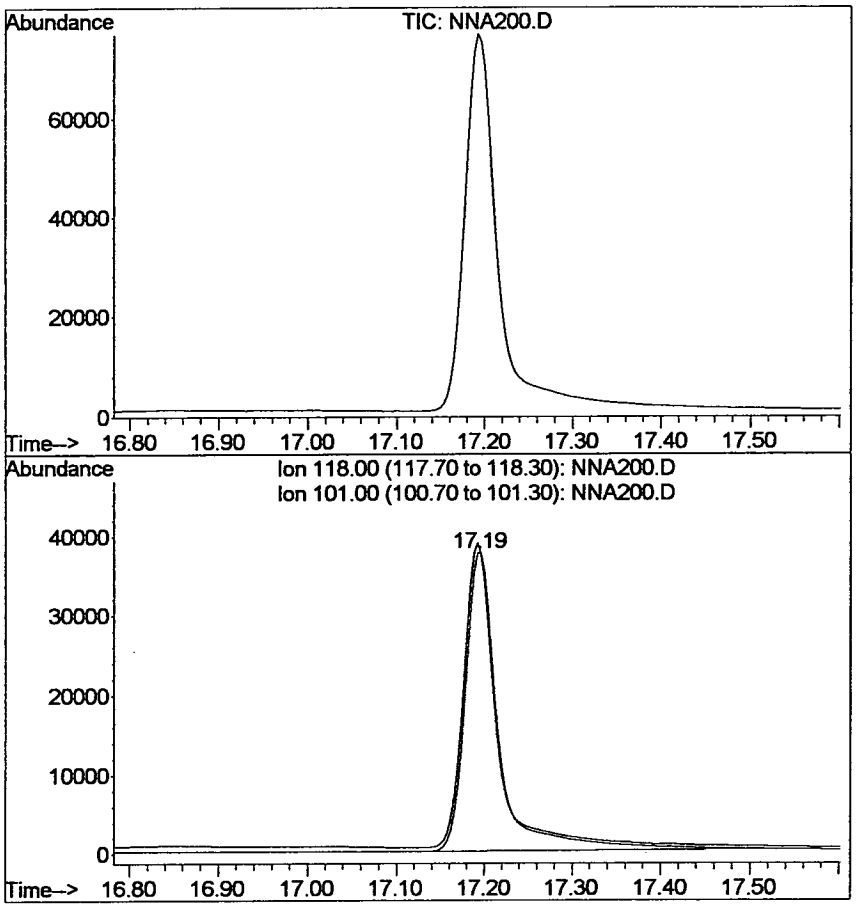

#7
NPYR
Concen: 214.63 PPB
RT: 17.19 min Scan# 1075
Delta R.T. -0.00 min
Lab File: NNA200.D
Acq: 14 Jun 2007 11:58 am

Tgt Ion:118 Resp: 101631

Ion	Ratio	Lower	Upper
118	100		
101	100.1	62.6	130.0

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA002B.D Vial: 3
Acq On : 14 Jun 2007 2:58 pm Operator: DF/AI
Sample : 2ppb Std.# 7060219 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:25 2007 Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration
DataAcq Meth : C7E29NWA

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) NDMA-D6	10.90	81	2696	10.00	PPB	0.00
3) NDEA-D10	13.37	113	5345	10.00	PPB	0.00
5) NDPA-D14	15.81	145	5002	10.00	PPB	0.00
Target Compounds						**Qvalue**
2) NDMA	10.84	92	1094	2.02	PPB	99
4) NDEA	13.32	120	1163	2.04	PPB	100
6) NDPA	15.76	148	905	2.15	PPB	96
7) NPYR	17.20	118	640	1.58	PPB	98

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NNA002B.D Vial: 3
Acq On : 14 Jun 2007 2:58 pm Operator: DF/AI
Sample : 2ppb Std.# 7060219 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:25 2007 Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 15:59:38 2007
Response via : Initial Calibration

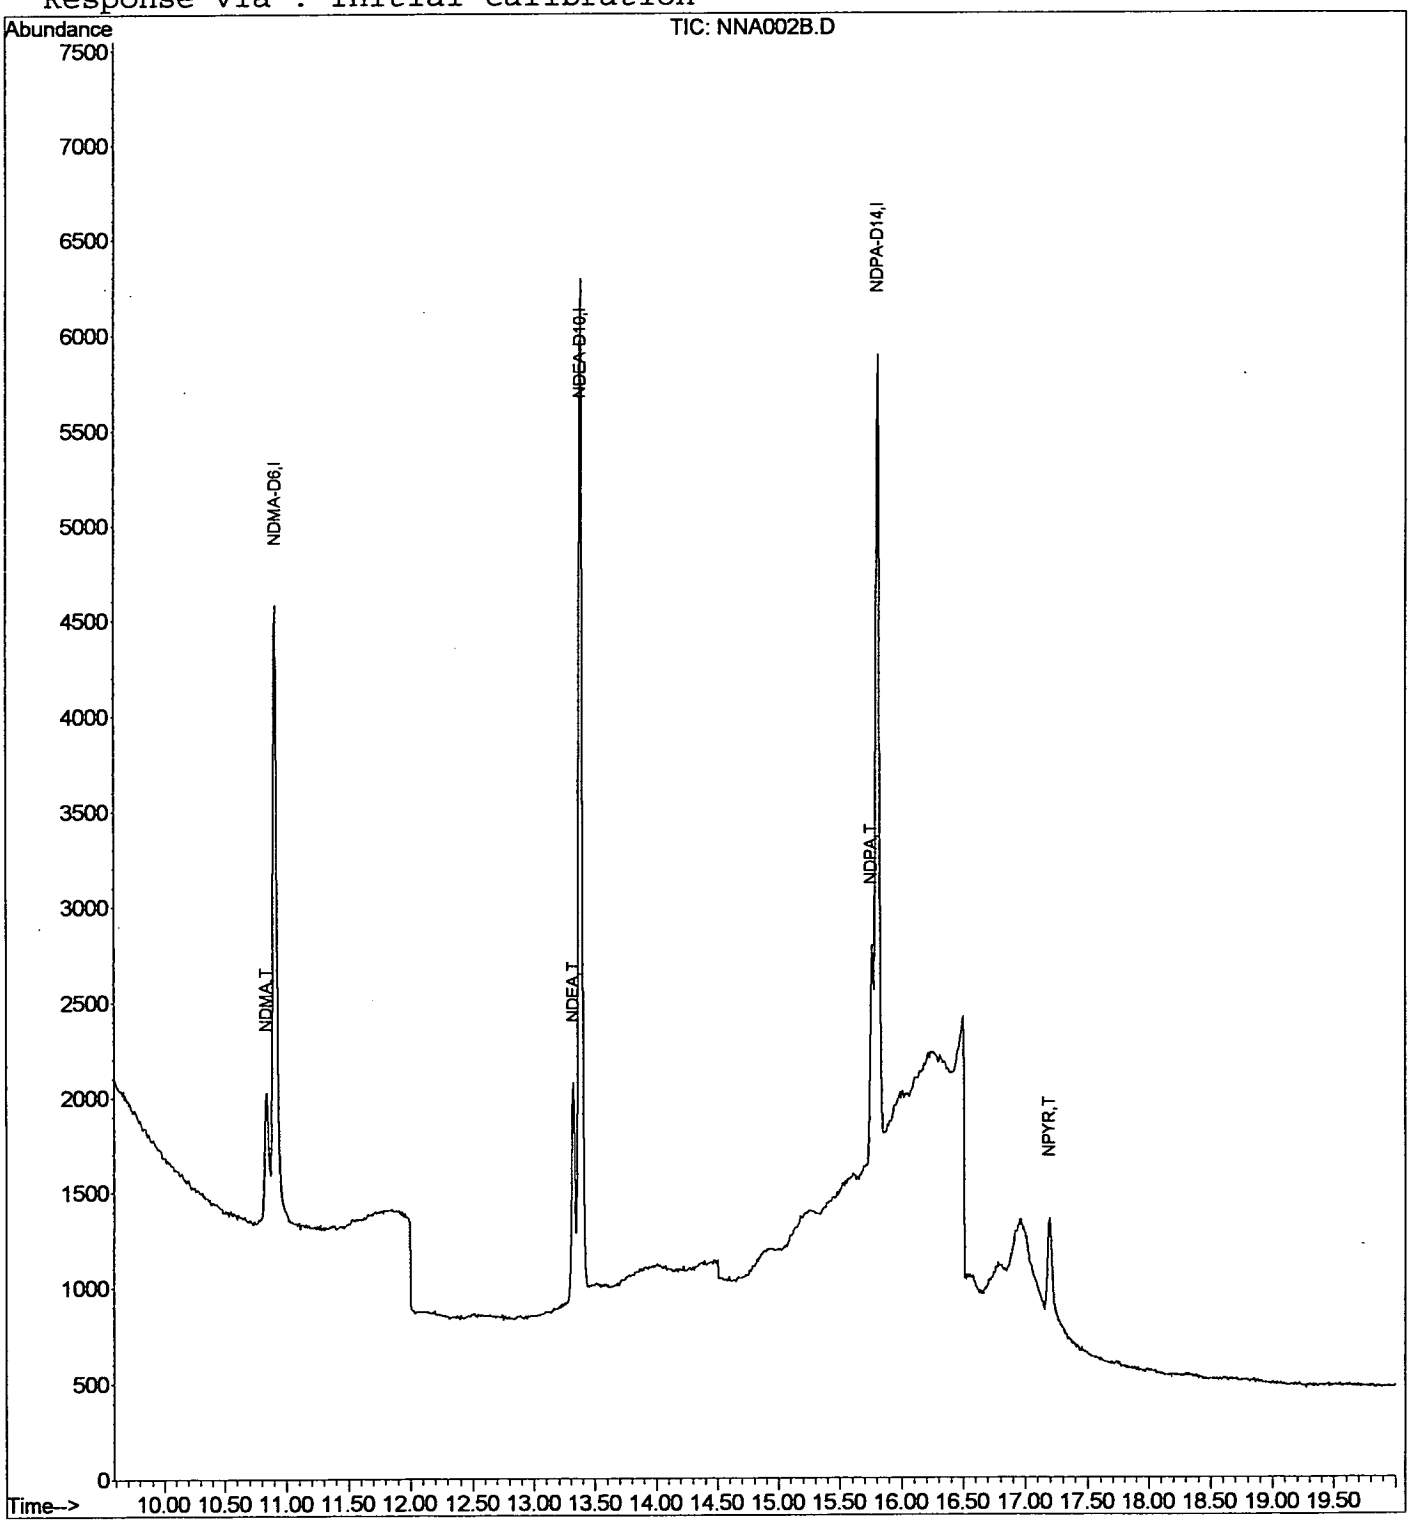

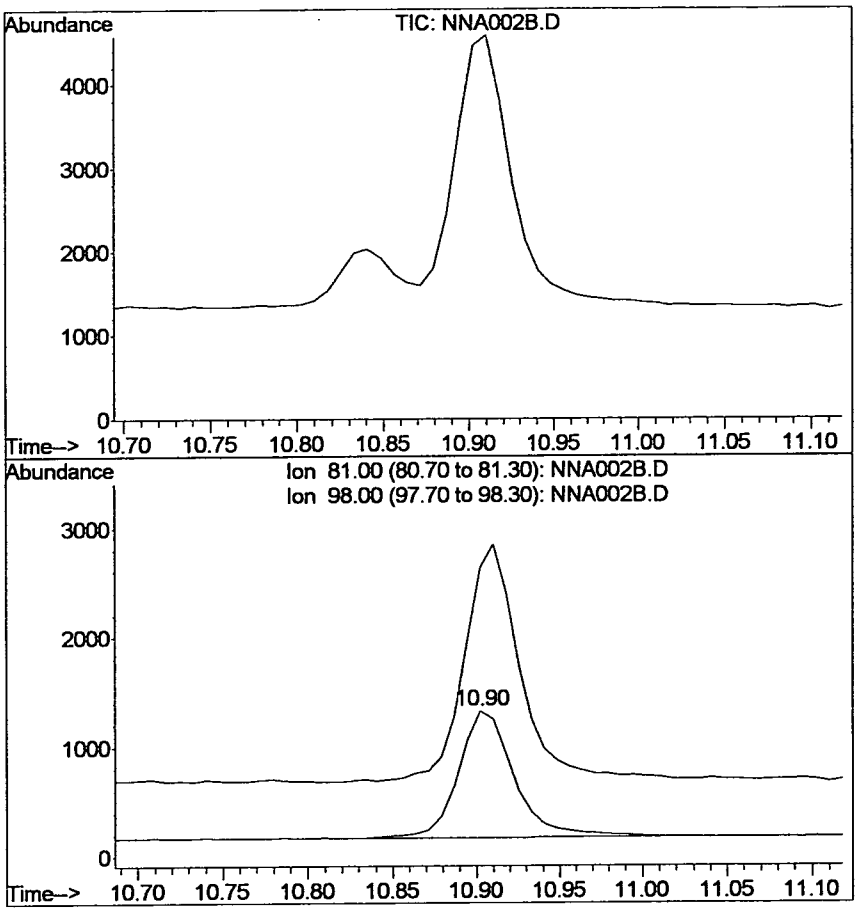

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.90 min Scan# 172
Delta R.T. 0.00 min
Lab File: NNA002B.D
Acq: 14 Jun 2007 2:58 pm

Tgt Ion: 81 Resp: 2696

Ion	Ratio	Lower	Upper
81	100		
98	182.3	144.1	224.1

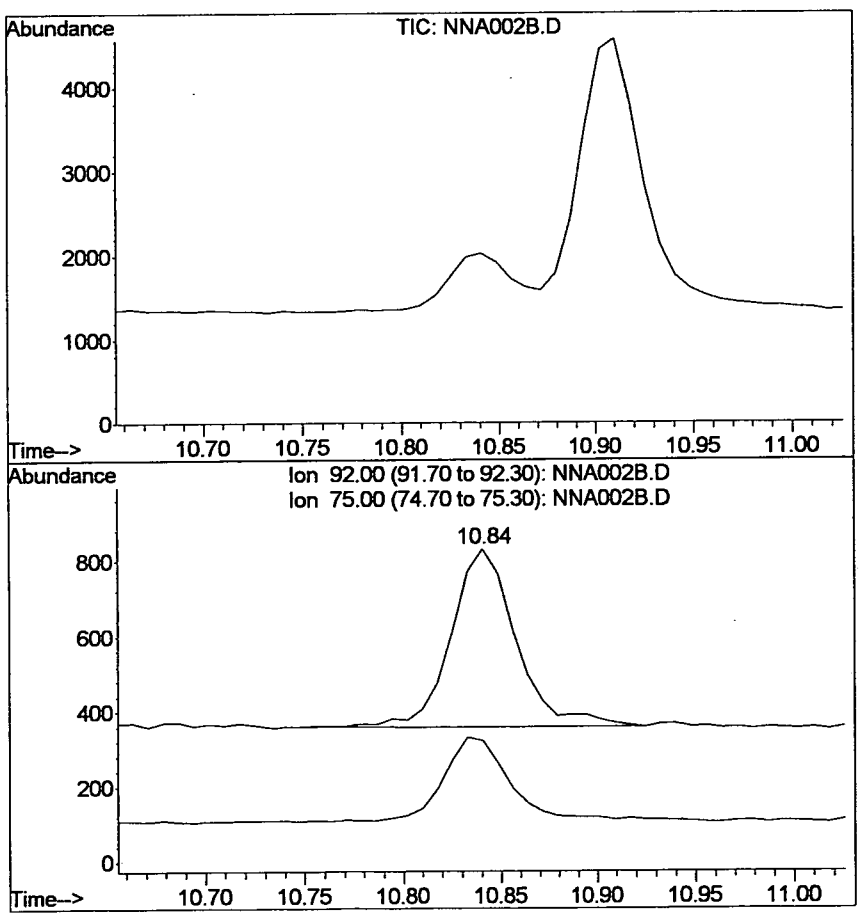

#2
NDMA
Concen: 2.02 PPB
RT: 10.84 min Scan# 164
Delta R.T. 0.01 min
Lab File: NNA002B.D
Acq: 14 Jun 2007 2:58 pm

Tgt Ion: 92 Resp: 1094

Ion	Ratio	Lower	Upper
92	100		
75	48.0	31.8	66.0

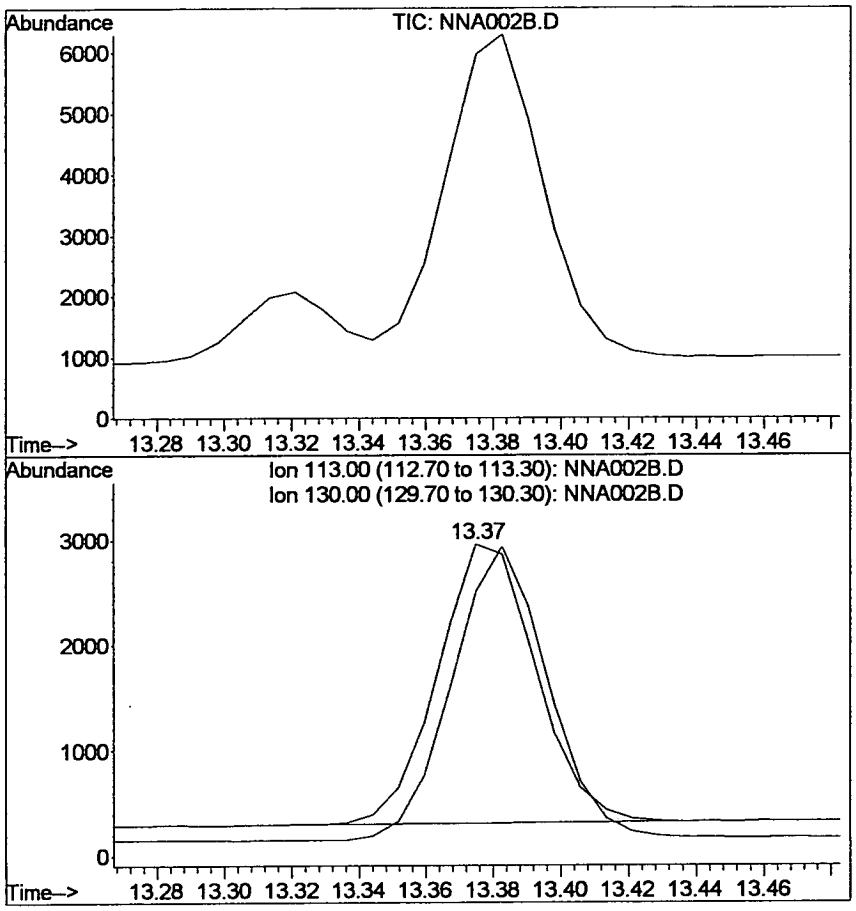

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.37 min Scan# 493
Delta R.T. 0.00 min
Lab File: NNA002B.D
Acq: 14 Jun 2007 2:58 pm

Tgt Ion:113 Resp: 5345

Ion	Ratio	Lower	Upper
113	100		
130	101.3	67.1	137.1

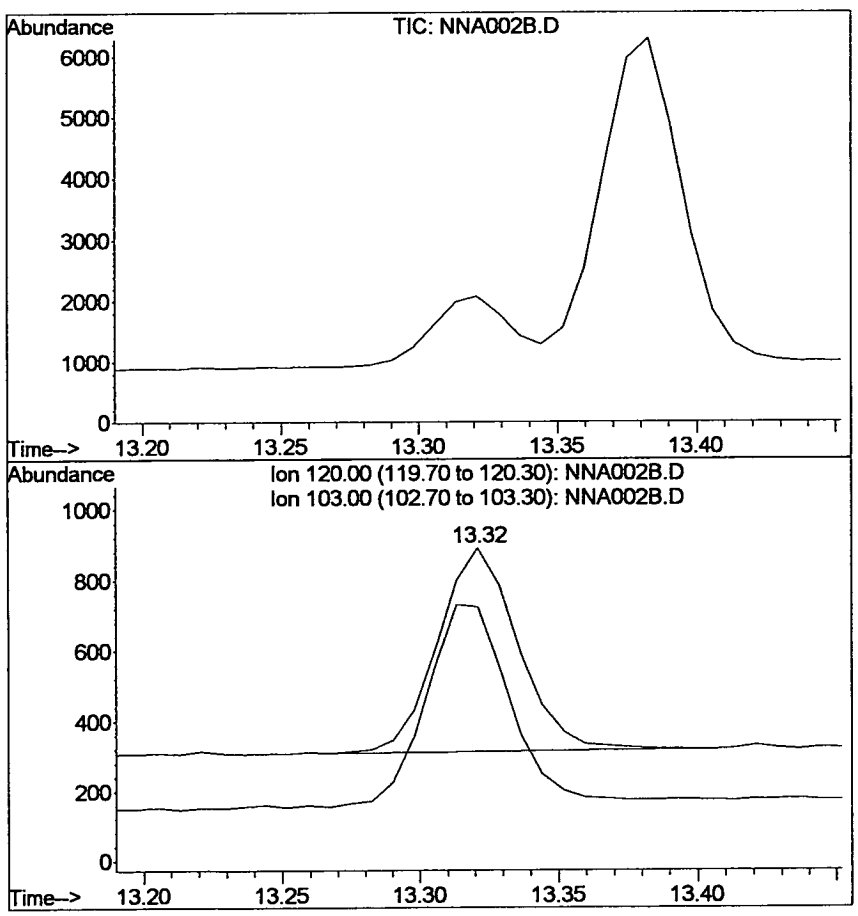

#4
NDEA
Concen: 2.04 PPB
RT: 13.32 min Scan# 486
Delta R.T. 0.00 min
Lab File: NNA002B.D
Acq: 14 Jun 2007 2:58 pm

Tgt Ion:120 Resp: 1163

Ion	Ratio	Lower	Upper
120	100		
103	100.8	65.3	135.5

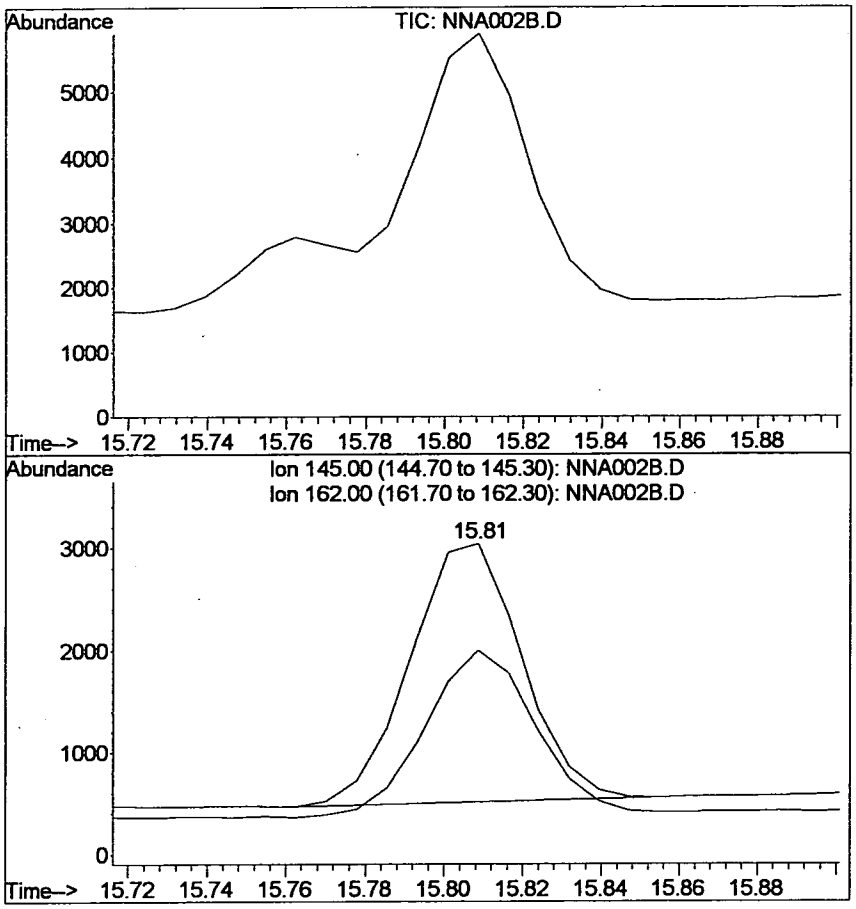

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.81 min Scan# 809
Delta R.T. 0.00 min
Lab File: NNA002B.D
Acq: 14 Jun 2007 2:58 pm

Tgt Ion:145 Resp: 5002

Ion	Ratio	Lower	Upper
145	100		
162	62.0	22.4	102.4

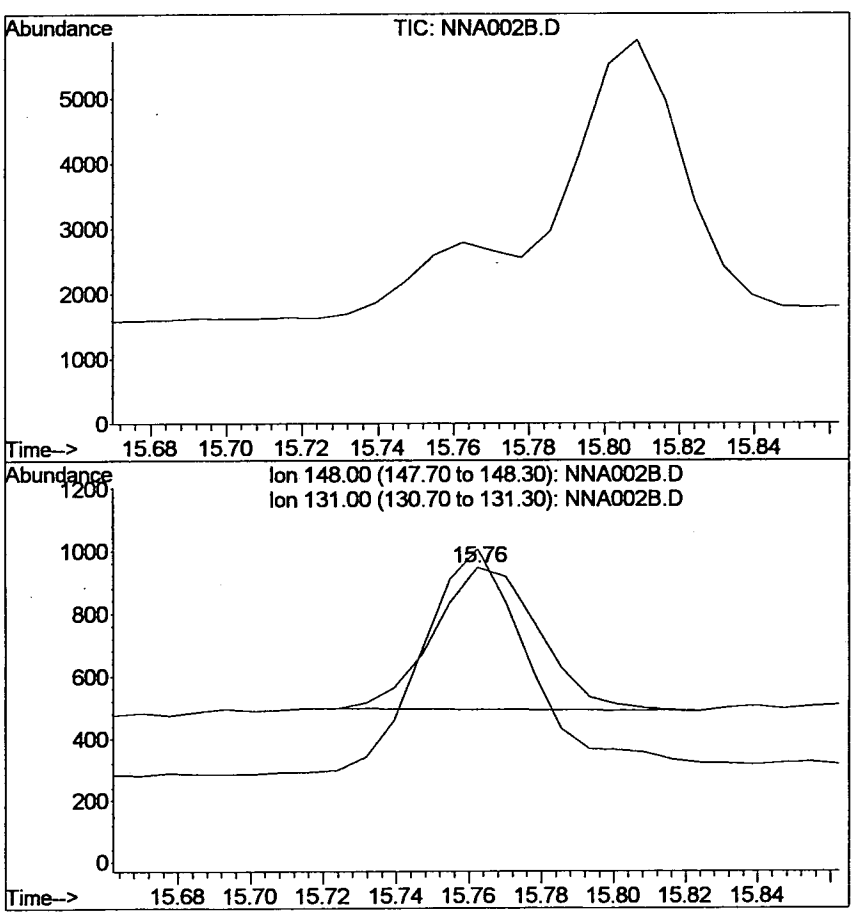

#6
NDPA
Concen: 2.15 PPB
RT: 15.76 min Scan# 803
Delta R.T. -0.01 min
Lab File: NNA002B.D
Acq: 14 Jun 2007 2:58 pm

Tgt Ion:148 Resp: 905

Ion	Ratio	Lower	Upper
148	100		
131	159.1	99.8	207.2

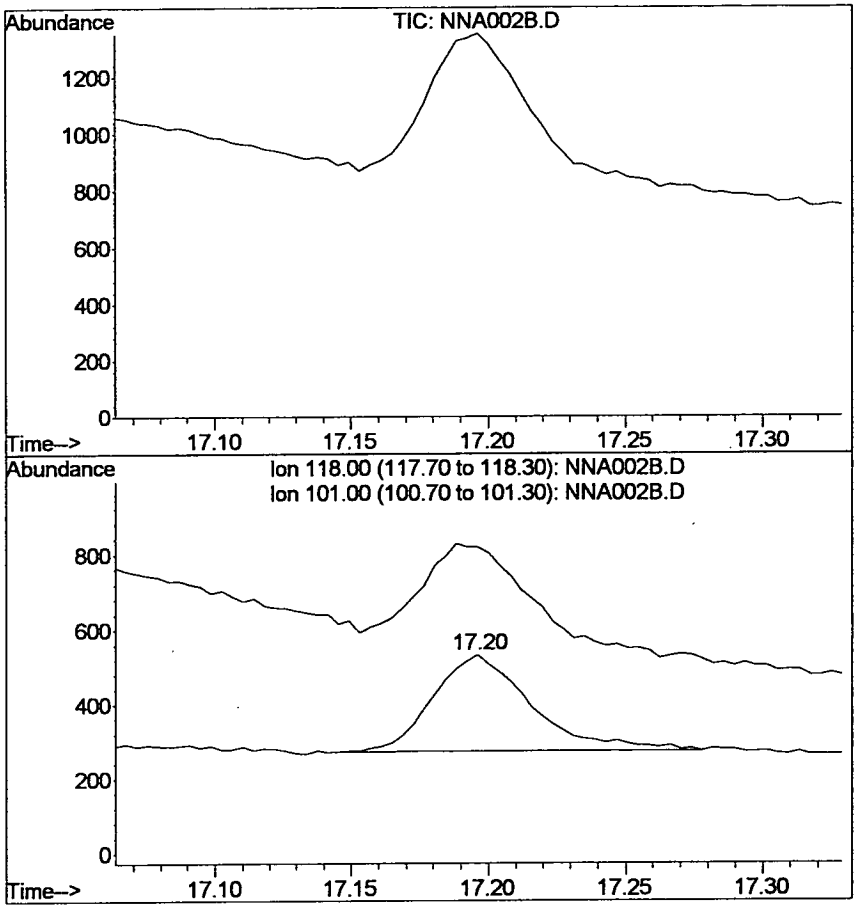

#7
NPYR
Concen: 1.58 PPB
RT: 17.20 min Scan# 1076
Delta R.T. 0.00 min
Lab File: NNA002B.D
Acq: 14 Jun 2007 2:58 pm

Tgt Ion:118 Resp: 640

Ion	Ratio	Lower	Upper
118	100		
101	97.8	62.6	130.0

Daily Midpoint Check
Nitrosamines by Method 1625C (Mod.)
Water Method
(Preextraction IS)

Data File: NLCS010.D Instrument: gcms37
Method File: ~~C7E29NWA~~ C7F14NW Date: 6/14/2007 12:21

Rev 7/31/07

Name	Conc.	Response	% Rec.	QC Limits
NDMA	10.00	9.93	99.3	(80-120)
NDEA	10.00	9.90	99.0	(80-120)
NDPA	10.00	11.50	115.0	(80-120)
NPYR	10.00	11.17	111.7	(80-120)

*Denotes value out of acceptance limit.

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NLCS010.D Vial: 10
Acq On : 14 Jun 2007 12:21 pm Operator: DF/AI
Sample : 10ppb LCS # 7060264 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:31 2007 Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration
DataAcq Meth : C7E29NWA

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) NDMA-D6	10.91	81	2820	10.00 PPB	0.00
3) NDEA-D10	13.38	113	5489	10.00 PPB	0.00
5) NDPA-D14	15.81	145	4947	10.00 PPB	0.00
Target Compounds					**Qvalue**
2) NDMA	10.84	92	5604	9.93 PPB	100
4) NDEA	13.32	120	5824	9.90 PPB	99
6) NDPA	15.76	148	4572	11.50 PPB	97
7) NPYR	17.20	118	4422	11.17 PPB	79

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUN14\NLCS010.D Vial: 10
Acq On : 14 Jun 2007 12:21 pm Operator: DF/AI
Sample : 10ppb LCS # 7060264 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P
Quant Time: Jun 14 16:31 2007 Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration

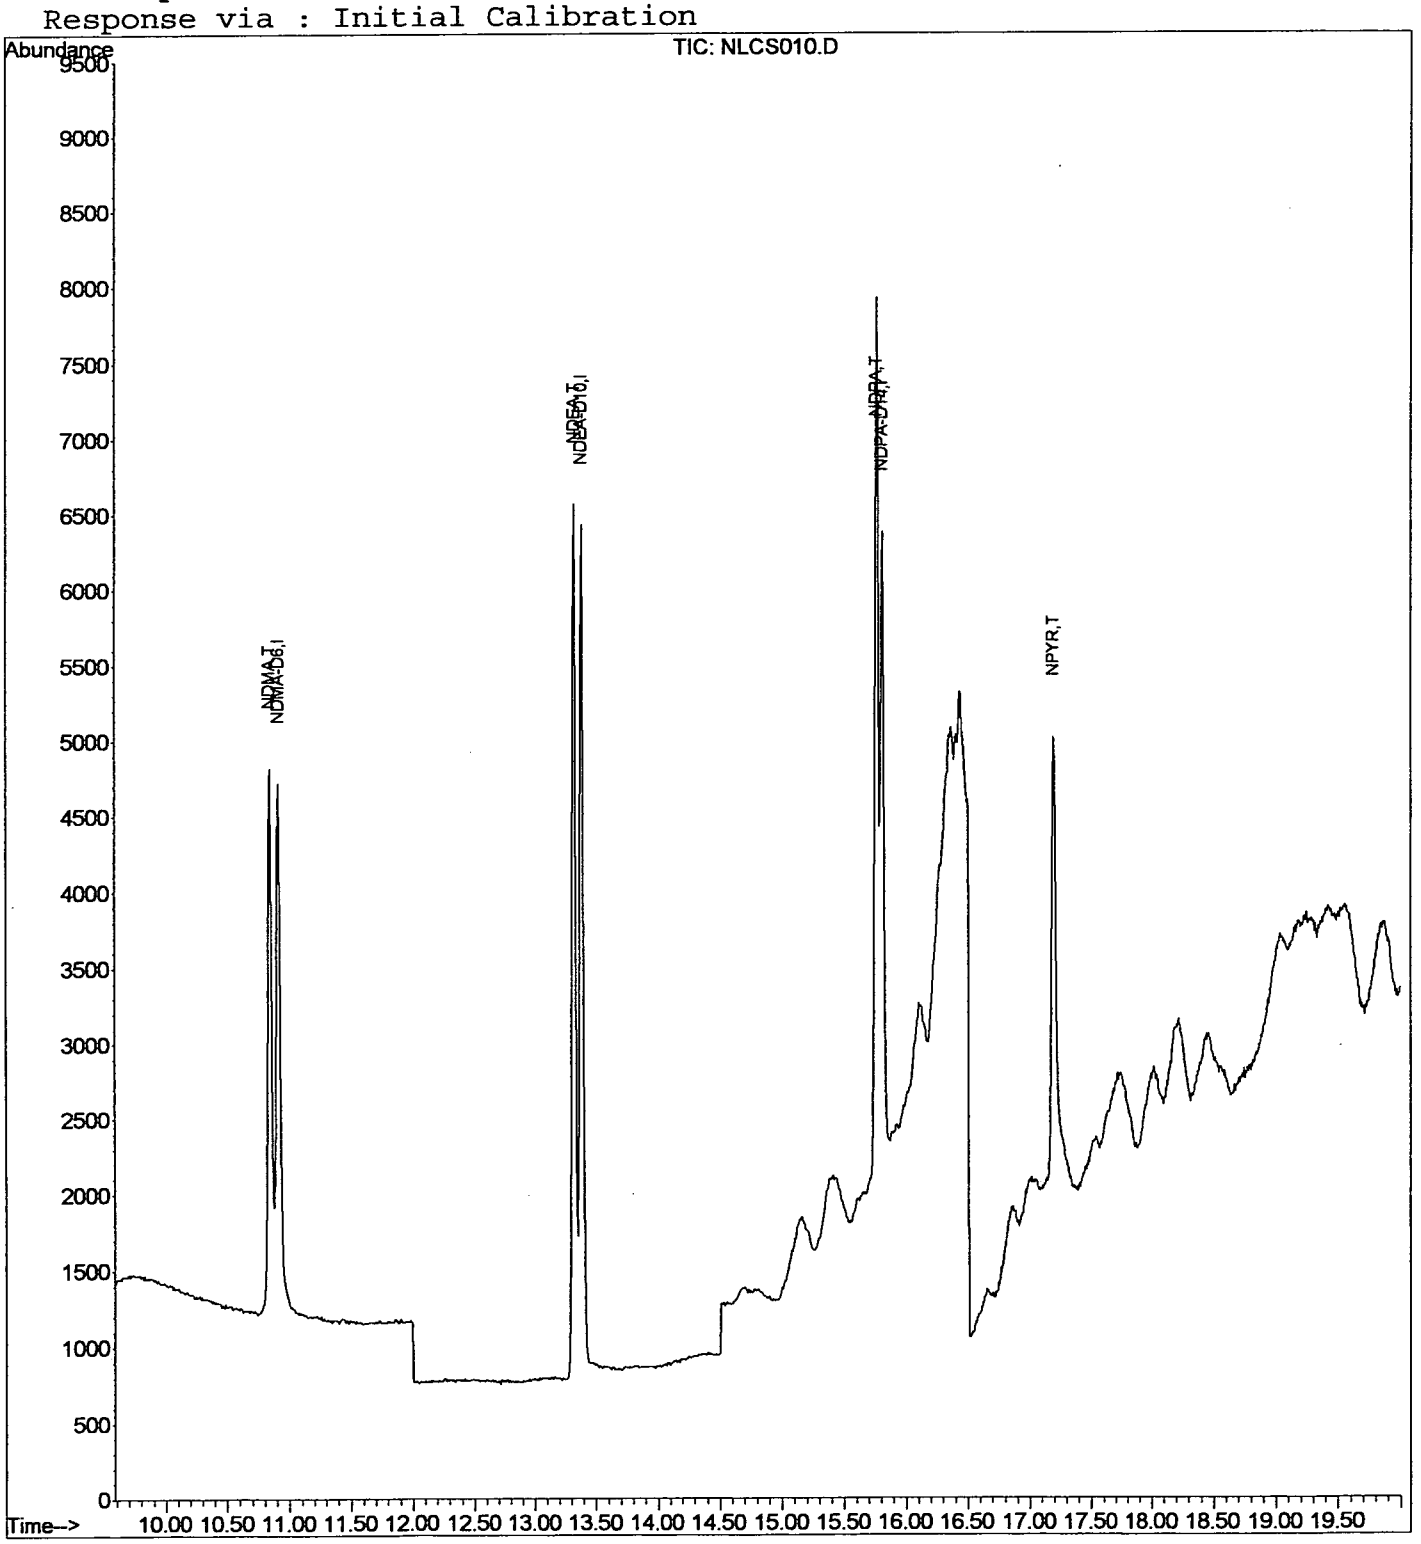

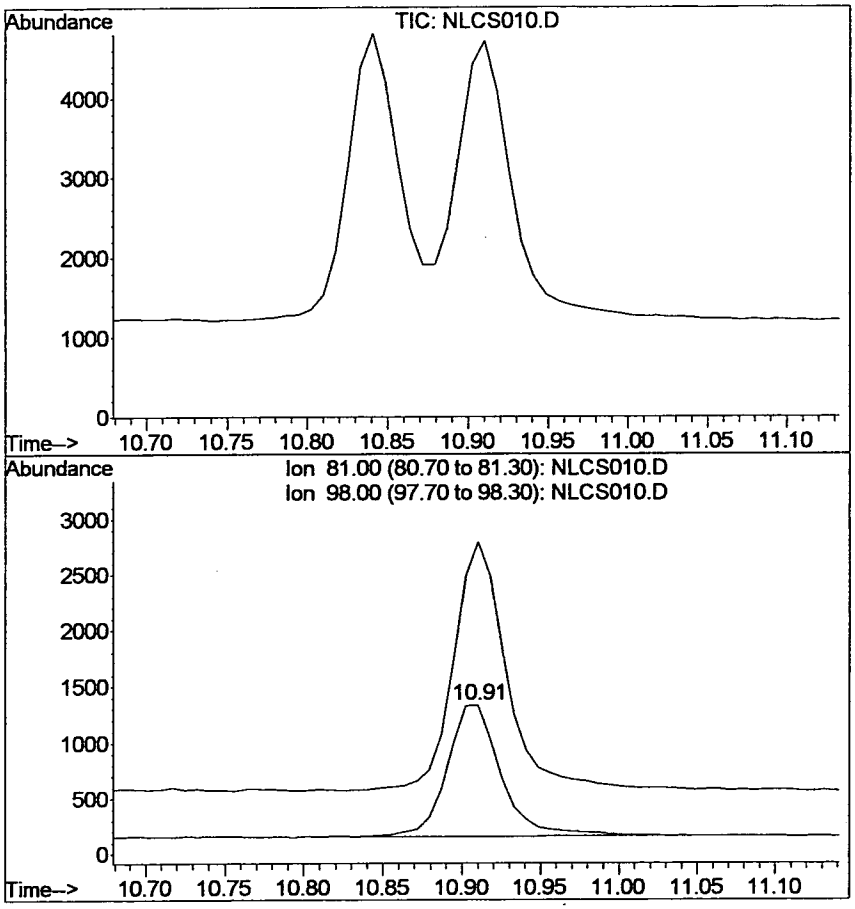

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.91 min Scan# 173
Delta R.T. 0.01 min
Lab File: NLCS010.D
Acq: 14 Jun 2007 12:21 pm

Tgt Ion: 81 Resp: 2820

Ion	Ratio	Lower	Upper
81	100		
98	185.3	144.1	224.1

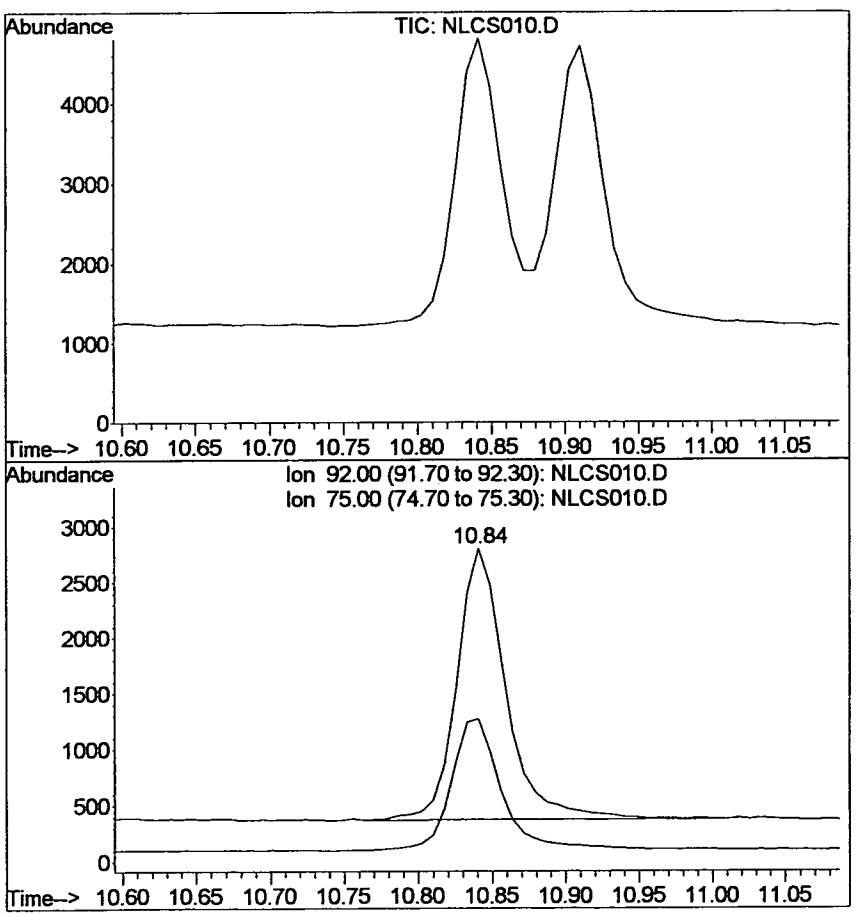

#2
NDMA
Concen: 9.93 PPB
RT: 10.84 min Scan# 164
Delta R.T. 0.01 min
Lab File: NLCS010.D
Acq: 14 Jun 2007 12:21 pm

Tgt Ion: 92 Resp: 5604

Ion	Ratio	Lower	Upper
92	100		
75	49.2	31.8	66.0

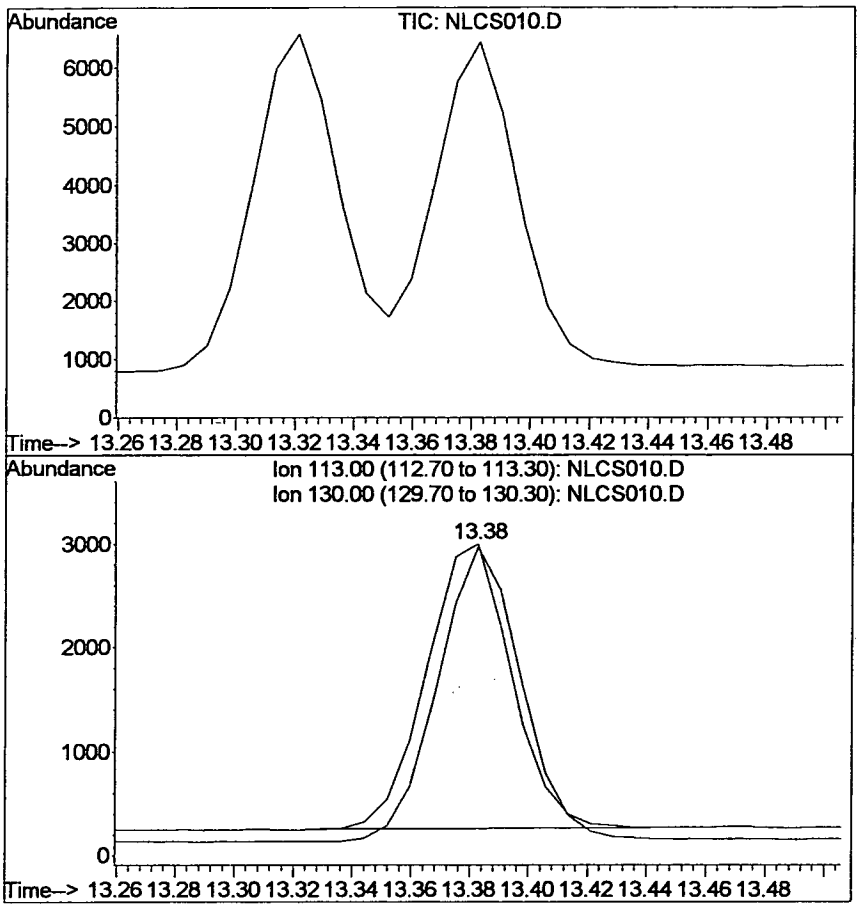

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.38 min Scan# 494
Delta R.T. 0.01 min
Lab File: NLCS010.D
Acq: 14 Jun 2007 12:21 pm

Tgt Ion:113 Resp: 5489

Ion	Ratio	Lower	Upper
113	100		
130	101.4	67.1	137.1

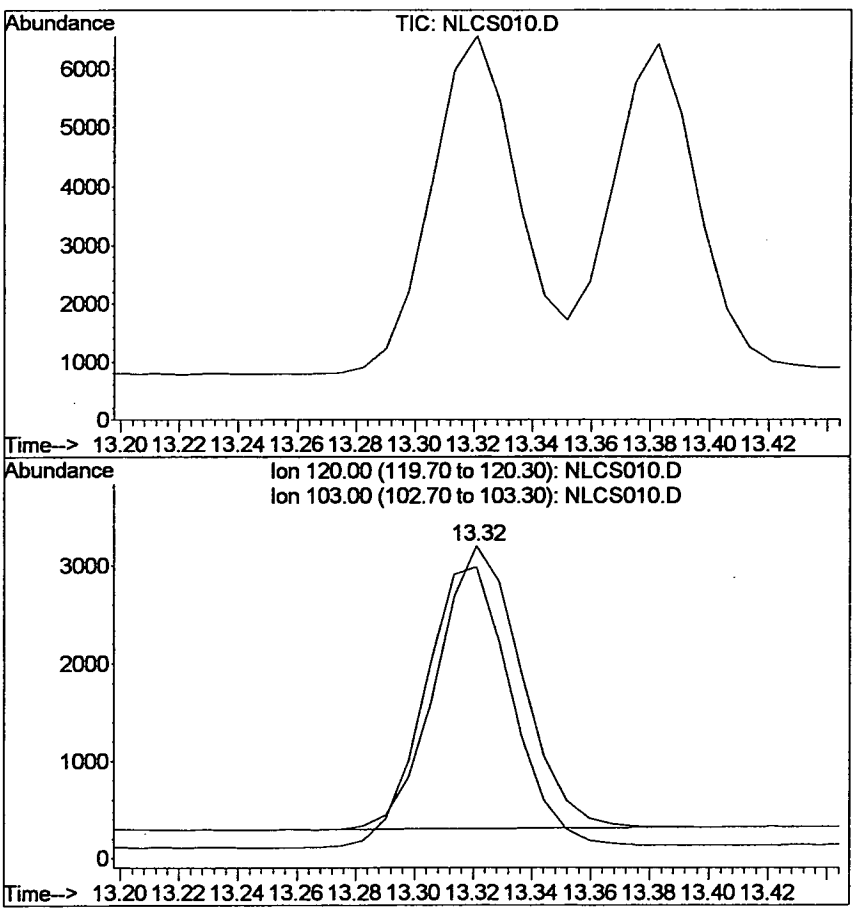

#4
NDEA
Concen: 9.90 PPB
RT: 13.32 min Scan# 486
Delta R.T. 0.00 min
Lab File: NLCS010.D
Acq: 14 Jun 2007 12:21 pm

Tgt Ion:120 Resp: 5824

Ion	Ratio	Lower	Upper
120	100		
103	101.3	65.3	135.5

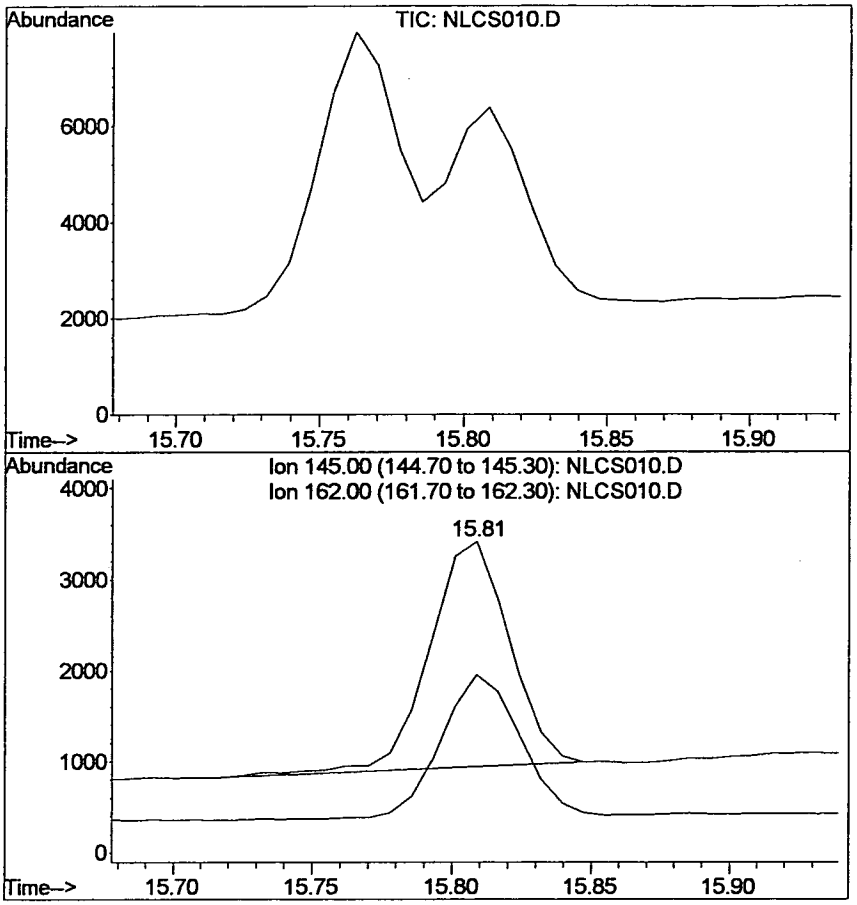

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.81 min Scan# 809
Delta R.T. -0.00 min
Lab File: NLCS010.D
Acq: 14 Jun 2007 12:21 pm

Tgt Ion:145 Resp: 4947

Ion	Ratio	Lower	Upper
145	100		
162	60.8	22.4	102.4

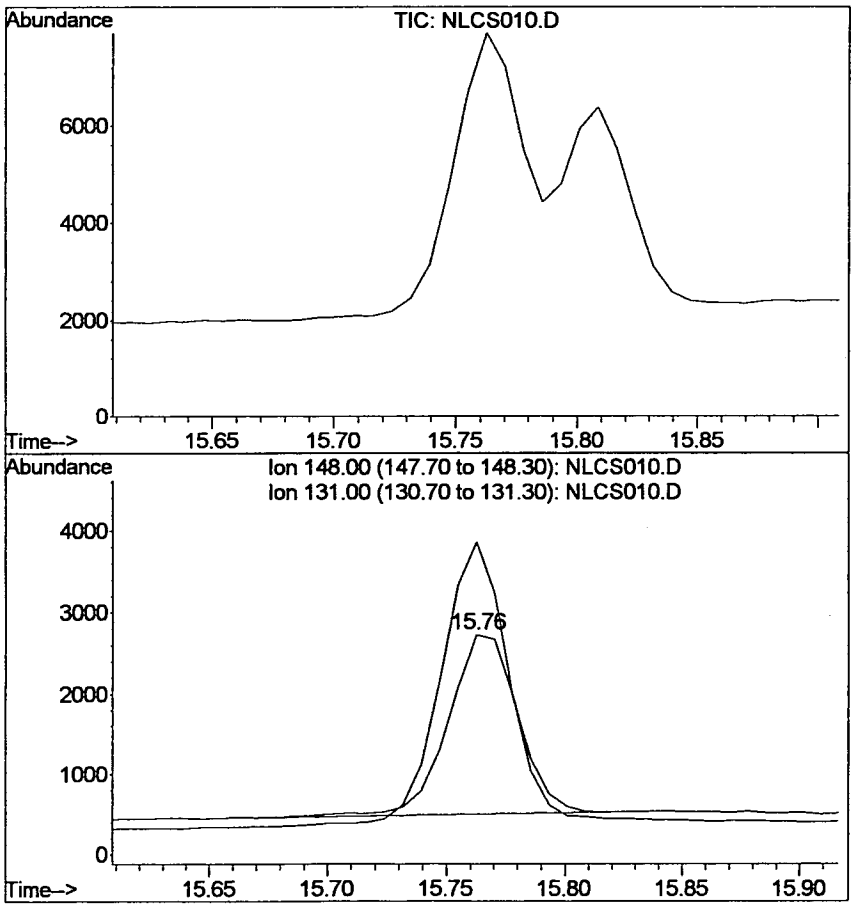

#6
NDPA
Concen: 11.50 PPB
RT: 15.76 min Scan# 803
Delta R.T. -0.01 min
Lab File: NLCS010.D
Acq: 14 Jun 2007 12:21 pm

Tgt Ion:148 Resp: 4572

Ion	Ratio	Lower	Upper
148	100		
131	149.1	99.8	207.2

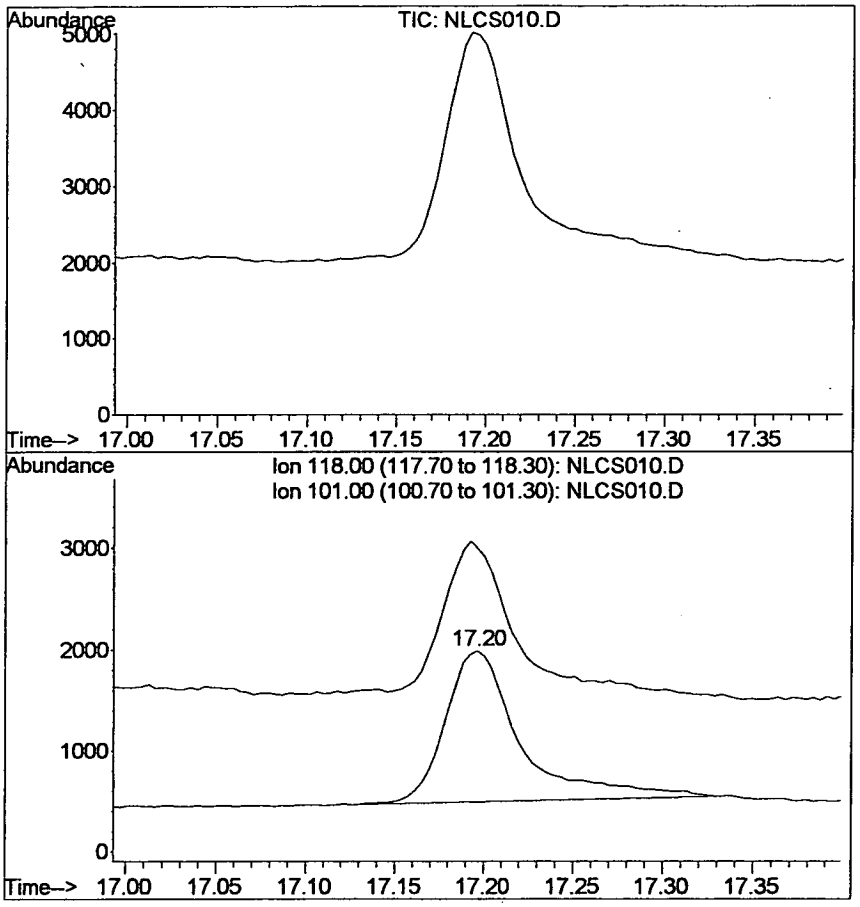

#7
NPYR
Concen: 11.17 PPB
RT: 17.20 min Scan# 1076
Delta R.T. 0.00 min
Lab File: NLCS010.D
Acq: 14 Jun 2007 12:21 pm

Tgt Ion:118 Resp: 4422

Ion	Ratio	Lower	Upper
118	100		
101	75.9	62.6	130.0

Evaluate Continuing Calibration Report

Data File : C:\MSDCHEM\1\DATA\07JUN14\NLCS010.D Vial: 10
Acq On : 14 Jun 2007 12:21 pm Operator: DF/AI
Sample : 10ppb LCS # 7060264 Inst : gcms37
Misc : n-Nitrosamines Water ICV Multiplr: 1.00
MS Integration Params: RTEINT2.P

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Multiple Level Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 200%

		Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1	I	NDMA-D6	1.000	1.000	0.0	100	0.00
2	T	NDMA	2.002	1.987	0.7	94	0.00
3	I	NDEA-D10	1.000	1.000	0.0	102	0.00
4	T	NDEA	1.072	1.061	1.0	96	0.00
5	I	NDPA-D14	1.000	1.000	0.0	101	0.00
6	T	NDPA	0.804	0.924	-14.9	100	0.00
7	T	NPYR	0.800	0.894	-11.7	110	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 0
NLCS010.D C7F14NW.M Thu Jun 14 16:31:45 2007 Page 1

GC/MS DAILY LOG SUMMARY

DATE: 07/20/07 DATAFILE C:\MSDCHEM\1 \DATA\07JUL20

ANALYST: LB/KS GCM # 37 EPA METHOD: n-Nitrosamines-1625

#	SAMPLE NAME	Dil	FILENAME	S/W	CLIENT	Prep	Batch #	Posted	Rev'd	Comments
1	ICV STANDARD	***	NNA010	***	*****	IS area:	2628			
2	7619061-BLK1	-	00720001	W	-	KS	19061	LB 07-21-07	7/23/07	
3	-BS1	-	02		-					
4	-BS2	-	03		-					
5	-BSD1	-	04		-					
6	1Q61101-01	-	05							
7	1Q61357-06	-	06							
8	-07	-	07							
9	1Q61437-01	-	08							
10	1Q61460-01	-	09							
11	-02	-	10							
12	-03	-	11							
13	-04	-	12							
14	-05	-	13							
15	-06	-	14							
16	1Q61646-01	-	15							
17										
18										
19										
20										
21										
22										
23										
24										
25										
26										
27										
28										
29										
30										

Standard Code: 7060221

Methylene Chloride Lot#: 072167

PREPARATION BENCH SHEET

7G19061

TestAmerica - Irvine, CA

Printed: 7/20/2007 12:39:29PM

Matrix: Water **Prepared using: Extractions - EPA 3520C** **Surrogate used: 7060499**

Lab Number	C	Analysis	Prepared	Initial (ml)	Final (ml)	Source ID	Spike 1	ul Spike	Spike 2	ul Spike	ul Surrogate	Initials			Extraction Comments
7G19061-BLK1		QC	07/19/07 09:42	1000	1			0		0	100				HPLC water fisher 064074
7G19061-BS1		QC	07/19/07 09:42	1000	1		7030370	250	7040159	50	100				HPLC water fisher 064074
7G19061-BS2		QC	07/19/07 09:42	1000	1		7030370	50			100				HPLC water fisher 064074
7G19061-BSD1		QC	07/19/07 09:42	1000	1		7030370	250	7040159	50	100				HPLC water fisher 064074
IQG1101-01	O	NDMA-1625C Mod	07/19/07 09:42	1050	1						100				J flag pH=7
IQG1150-05RE1	E	8270C-1,4-Dioxane	07/19/07 09:42	1020	1						100				Re-extract added7/18/2007 by LBSurrogate low pH=7
IQG1357-06	H	NDMA-1625C Mod	07/19/07 09:42	1050	1						100				pH=7
IQG1357-07	H	NDMA-1625C Mod	07/19/07 09:42	1050	1						100				pH=7
IQG1437-01	K	NDMA-1625C Mod	07/19/07 09:42	1055	1						100				rl=2ng/l pH=7
IQG1451-10	A	8270C-1,4-Dioxane	07/19/07 09:42	960	1						100				Irvine pH=7
IQG1460-01	G	NDMA-1625C Mod	07/19/07 09:42	1020	1						100				pH=7
IQG1460-02	G	NDMA-1625C Mod	07/19/07 09:42	1035	1						100				pH=7
IQG1460-03	G	NDMA-1625C Mod	07/19/07 09:42	1050	1						100				pH=7
IQG1460-04	G	NDMA-1625C Mod	07/19/07 09:42	1035	1						100				pH=7
IQG1460-05	G	NDMA-1625C Mod	07/19/07 09:42	1050	1						100				pH=7
IQG1460-06	G	NDMA-1625C Mod	07/19/07 09:42	1060	1						100				pH=7
IQG1574-04	D	8270C-1,4-Dioxane	07/19/07 09:42	1045	1						100				pH=7
IQG1574-08	E	8270C-1,4-Dioxane	07/19/07 09:42	1050	1						100				pH=7
IQG1574-10	E	8270C-1,4-Dioxane	07/19/07 09:42	1040	1						100				pH=5
IQG1578-04	A	8270C-1,4-Dioxane	07/19/07 09:42	960	1						100				Irvine pH=7

Spiking Witnessed By Date

JMH 07/20/07
Preparation Reviewed By Date

Am 7/23/07
Extracts Received By Date

PREPARATION BENCH SHEET

7G19061

TestAmerica - Irvine, CA

Printed: 7/20/2007 12:39:29PM

Matrix: Water **Prepared using: Extractions - EPA 3520C** **Surrogate used: 7060499**

Lab Number	C	Analysis	Prepared	Initial (ml)	Final (ml)	Source ID	Spike 1	ul Spike	Spike 2	ul Spike	ul Surrogate	Initials			Extraction Comments
IQG1625-02	I	8270C-1,4-Dioxane	07/19/07 09:42	1030	1						100				pH=7
IQG1625-03	I	8270C-1,4-Dioxane	07/19/07 09:42	1050	1						100				pH=7
IQG1625-04	I	8270C-1,4-Dioxane	07/19/07 09:42	1035	1						100				pH=7
IQG1646-01	B	NDMA-1625C Mod	07/19/07 09:42	1050	1						100				J Flag pH=7

Reagents used in Batch

Reagent	Description	Solvent

Base heat start 7/19/07 @ 1745
stop 7/20/07 @ 1145
MeCl2 fisher 067660
H2SO4 jtb C50055
NaOH jtb C11676
Na2SO4 emd 46361707
NDMA surrogate 7060499
1,4 diox. surrogate 7060473

Spiking Witnessed By Date

Preparation Reviewed By Date

Extracts Received By Date

PREPARATION BENCH SHEET

7G19061

TestAmerica - Irvine, CA

Printed: 7/19/2007 9:49:26AM

Matrix: Water 24

Prepared using: Extractions - EPA 3520C

7060499
7060473 ~~(No Surrogate)~~

Lab Number	C	Analysis	Prepared	Initial (ml)	Final (ml)	Source ID	Spike 1	ul Spike	Spike 2	ul Spike	ul Surrogate	Initials			Extraction Comments
7G19061-BLK1		QC	07/19/07 09:42	1000	1			0		0	100	JMH			HPLC WATER FISHER 064074
7G19061-BS1		QC	07/19/07 09:42	1000	1		7030370	250 ~~100~~	7040159 ~~7060473~~	50 ~~100~~					
7G19061-BS2		QC	07/19/07 09:42	1000	1			50 ~~100~~		~~100~~					
7G19061-BSD1		QC	07/19/07 09:42	1000	1			250 ~~100~~	7040159 ~~7060473~~	50 ~~100~~					
IQG1101-01	O	NDMA-1625C Mod	07/19/07 09:42	1050 ~~1000~~	1										J flag PH = 7
IQG1150-05RE1	E	8270C-1,4-Dioxane	07/19/07 09:42	1020 ~~1000~~	1										Re-extract added 7/18/2007 by LB, Surrogate low PH = 7
IQG1357-06	H	NDMA-1625C Mod	07/19/07 09:42	1050 ~~1000~~	1										PH = 7
IQG1357-07	H	NDMA-1625C Mod	07/19/07 09:42	1050 ~~1000~~	1										PH = 7
IQG1437-01	K	NDMA-1625C Mod	07/19/07 09:42	1055 ~~1000~~	1										rl=2ng/l PH = 7
IQG1451-10	A	8270C-1,4-Dioxane	07/19/07 09:42	960 ~~1000~~	1										Irvine PH = 7
IQG1460-01	G	NDMA-1625C Mod	07/19/07 09:42	1020 ~~1000~~	1										PH = 7
IQG1460-02	G	NDMA-1625C Mod	07/19/07 09:42	1035 ~~1000~~	1										PH = 7
IQG1460-03	G	NDMA-1625C Mod	07/19/07 09:42	1050 ~~1000~~	1										PH = 7
IQG1460-04	G	NDMA-1625C Mod	07/19/07 09:42	1035 ~~1000~~	1										PH = 7
IQG1460-05	G	NDMA-1625C Mod	07/19/07 09:42	1050 ~~1000~~	1										PH = 7
IQG1460-06	G	NDMA-1625C Mod	07/19/07 09:42	1080 ~~1000~~	1										PH = 7
IQG1574-04	D	8270C-1,4-Dioxane	07/19/07 09:42	1045 ~~1000~~	1										PH = 7
IQG1574-08	E	8270C-1,4-Dioxane	07/19/07 09:42	1050 ~~1000~~	1										PH = 7
IQG1574-10	E	8270C-1,4-Dioxane	07/19/07 09:42	1010 ~~1000~~	1										PH = 5
IQG1578-04	A	8270C-1,4-Dioxane	07/19/07 09:42	960 ~~1000~~	1										Irvine PH = 7

JMH 7/19/07

Spiking Witnessed By Date

Preparation Reviewed By Date

Extracts Received By Date

PREPARATION BENCH SHEET

7G19061

TestAmerica - Irvine, CA

Printed: 7/19/2007 9:49:26AM

Matrix: Water

Prepared using: Extractions - EPA 3520C

(No Surrogate)

Lab Number	C	Analysis	Prepared	Initial (ml)	Final (ml)	Source ID	Spike 1	ul Spike	Spike 2	ul Spike	ul Surrogate	Initials			Extraction Comments
IQG1625-02	I	8270C-1,4-Dioxane	07/19/07 09:42	1 ~~1000~~ 930	1						100	JMH			PH=7
IQG1625-03	I	8270C-1,4-Dioxane	07/19/07 09:42	1 ~~1000~~ 950	1						↓	↓			PH=7
IQG1625-04	I	8270C-1,4-Dioxane	07/19/07 09:42	1 ~~1000~~ 935	1						↓	↓			PH=7
IQG1646-01	B	NDMA-1625C Mod	07/19/07 09:42	1 ~~1000~~ 950	1						↓	↓			J Flag PH=7

$MeCl_2$ fisher 067CCO

H_2SO_4 JTB C50055

NaOH JTB C11676

Na_2SO_4 EMD 46365707

Base Heat start 7/19/07 @ 1745

Stop 7/20/07 @ 1145

Spiking Witnessed By Date

Preparation Reviewed By Date

Extracts Received By Date

87

GC/MS QA-QC Check Report

Tune File : C:\MSDCHEM\1\DATA\07JUL20\NNA010.D
Tune Time : 20 Jul 2007 4:30 pm

Daily Calibration File : C:\MSDCHEM\1\DATA\07JUL20\NNA010.D

File	Sample	2628	5142	5188
		Internal Standard Responses		
C0720001.D	7G19061-BLK1	2341	5008	5209
C0720002.D	7G19061-BS1	2280	4776	5300
C0720003.D	7G19061-BS2	2372	5096	5248
C0720004.D	7G19061-BSD1	2448	5249	5480
C0720005.D	IQG1101-01	2166	14362*	7104
C0720006.D	IQG1357-06	2468	5271	7470
C0720007.D	IQG1357-07	2066	4609	6681
C0720008.D	IQG1437-01	1619	3689	155485*
C0720009.D	IQG1460-01	1728	4066	4559
C0720010.D	IQG1460-02	1906	3994	4115
C0720011.D	IQG1460-03	2042	4776	5087
C0720012.D	IQG1460-04	2197	4738	5317
C0720013.D	IQG1460-05	1815	4190	4492
C0720014.D	IQG1460-06	2028	4335	4669
C0720015.D	IQG1646-01	2188	4644	5630

- fails 12hr time check * - fails criteria

Created: Fri Aug 10 15:48:39 2007 gcms37

Daily Midpoint Check
Nitrosamines by Method 1625C (Mod.)
Water Method
(Preextraction IS)

Data File: NNA010.D
Method File: C7F14NW

Instrument: gcms37
Date: 7/20/2007 16:30

Name	Conc.	Response	% Rec.	QC Limits
NDMA	10.00	10.58	105.8	(80-120)
NDEA	10.00	10.58	105.8	(80-120)
NDPA	10.00	9.95	99.5	(80-120)
NPYR	10.00	9.56	95.6	(80-120)

*Denotes value out of acceptance limit.

GCMS DATA CHECK LIST
EPA 1625C MOD - N-NITROSODIMETHYLAMINE Analysis

2nd Level Review:		Analyst:	LB
Date:	7/23/07	Analysis Date:	07-20-07
QC Batches:	7619061	GCMS #:	37

2nd Level Rev	Analyst Rev	
		CH4 CI-Autotune :
✓	✓	• At least weekly
✓	✓	• Peak shape: well defined at mass 41, 267 and 599
✓	✓	• Peak width: 0.45 to 0.54
✓	✓	• Sufficient abundance: 400,000 to 700,000 counts
		Calibration :
✓	✓	• Minimum 5-point calibration – lowest standard at RL
✓	✓	• RSD of RF <=20%
		Mid-point verification (ICV/CCV @ 10 ug/l) :
✓	✓	• 2nd source after initial calibration. %Recovery : <= ±20
✓	✓	• Daily: Every 12-hour shift. % Difference : <= ±20 (relative to initial calibration)
✓	✓	• IS areas : -50% to +100% (relative to initial calibration m-p. std)
✓	✓	**Method blank :** every extraction batch of 20 samples (< 0.5 ng/L or flag accordingly)
✓	✓	**LCS :** every extraction batch of 20 samples or less . % Rec <= ±30 (or in-house limits)
✓	✓	**MS/MSD :** every extraction batch of 20 samples or less (checked against in-house limits)
		All samples check for :
✓	✓	• Unit, Dilution Factor
✓	✓	• Manual Integration, Transcription Errors, Calculations
✓	✓	• Spectra Match
✓	✓	• IS area and retention time
✓	✓	• All samples analyzed within tuning period (12hr)
✓	✓	GCMS Initial Calibration Criteria Form attached (if averaged calibration RFs used)
✓	✓	Mint Miner Check
✓	✓	Corrective Action Report attached (if applicable)

Comments:

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\NNA010.D
Acq On : 20 Jul 2007 4:30 pm
Sample : 10ppb Std.# 7060221
Misc : n-Nitrosamines water
MS Integration Params: RTEINT2.P
Quant Time: Jul 20 17:14 2007

Vial: 1
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration
DataAcq Meth : C7F14NW

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) NDMA-D6	10.91	81	2628	10.00	PPB	0.00
3) NDEA-D10	13.39	113	5142	10.00	PPB	0.02
5) NDPA-D14	15.82	145	5188	10.00	PPB	0.00
Target Compounds						**Qvalue**
2) NDMA	10.85	92	5566	10.58	PPB	96
4) NDEA	13.33	120	5832	10.58	PPB	94
6) NDPA	15.78	148	4150	9.95	PPB	89
7) NPYR	17.20	118	3969	9.56	PPB	87

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\NNA010.D
Acq On : 20 Jul 2007 4:30 pm
Sample : 10ppb Std.# 7060221
Misc : n-Nitrosamines water
MS Integration Params: RTEINT2.P
Quant Time: Jul 20 17:14 2007

Vial: 1
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00

Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration

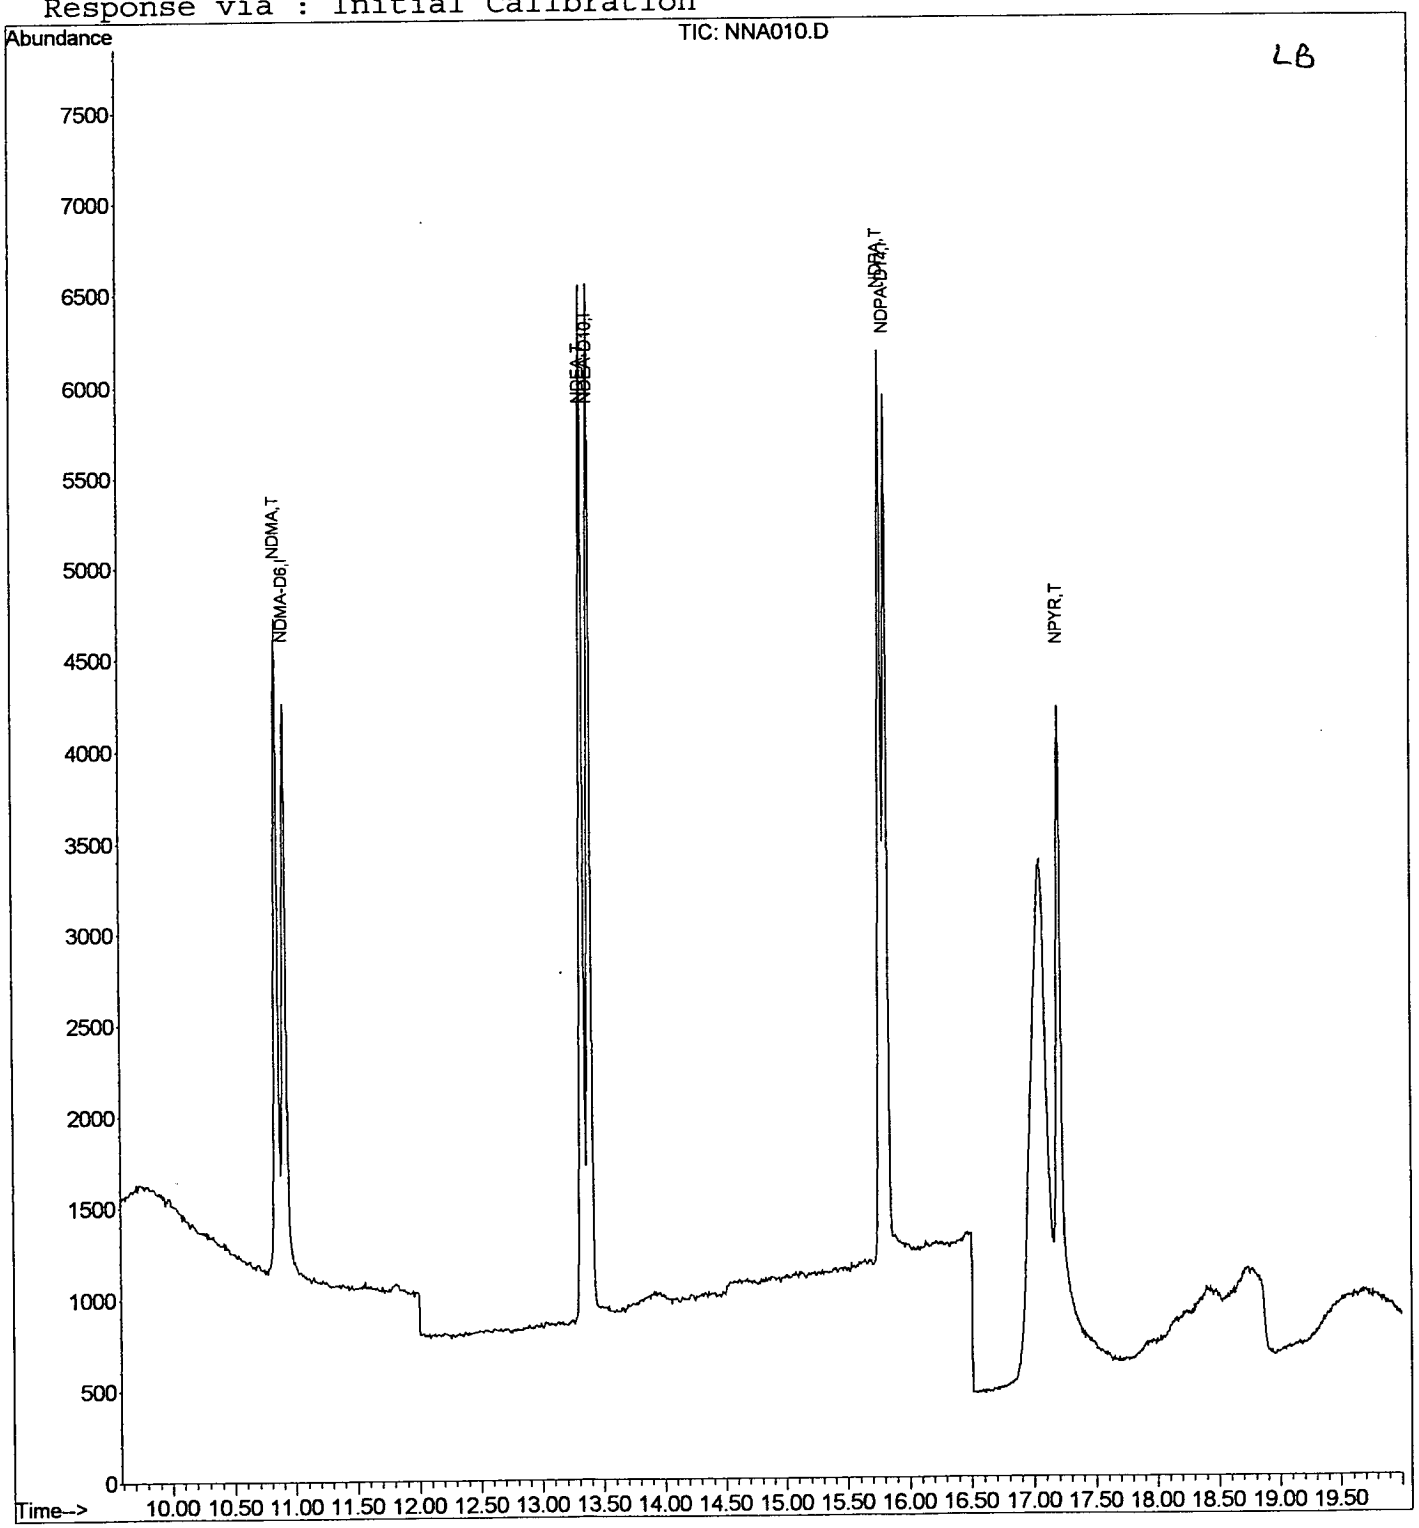

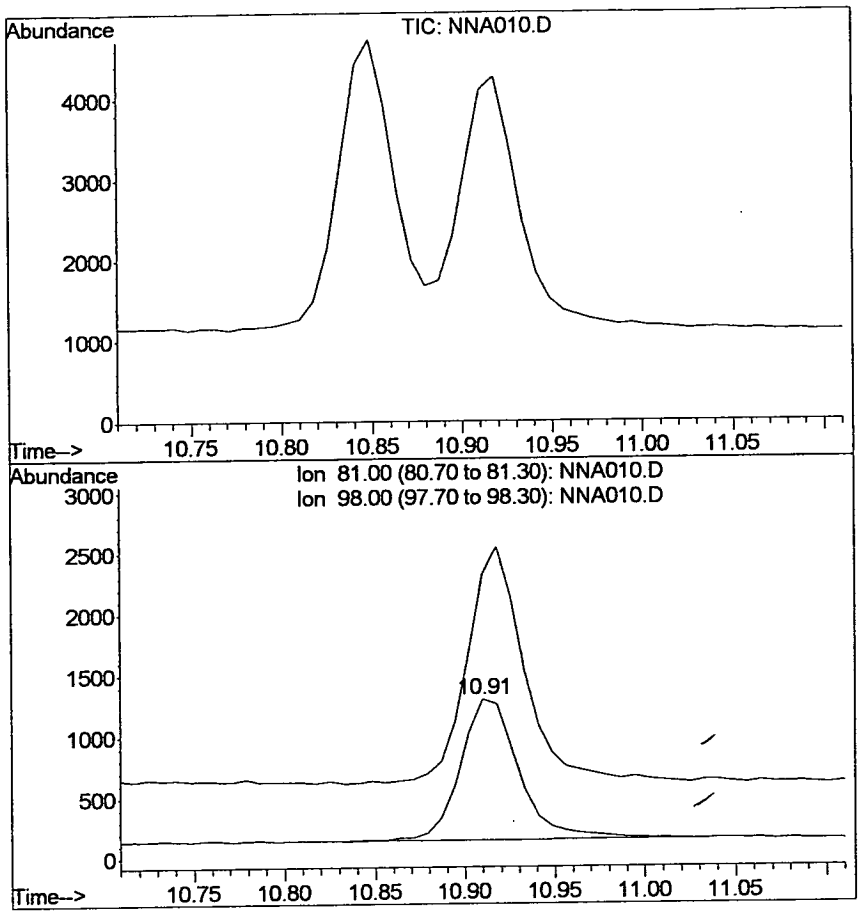

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.91 min Scan# 173
Delta R.T. 0.01 min
Lab File: NNA010.D
Acq: 20 Jul 2007 4:30 pm

Tgt Ion: 81 Resp: 2628

Ion	Ratio	Lower	Upper
81	100		
98	161.9	144.1	224.1

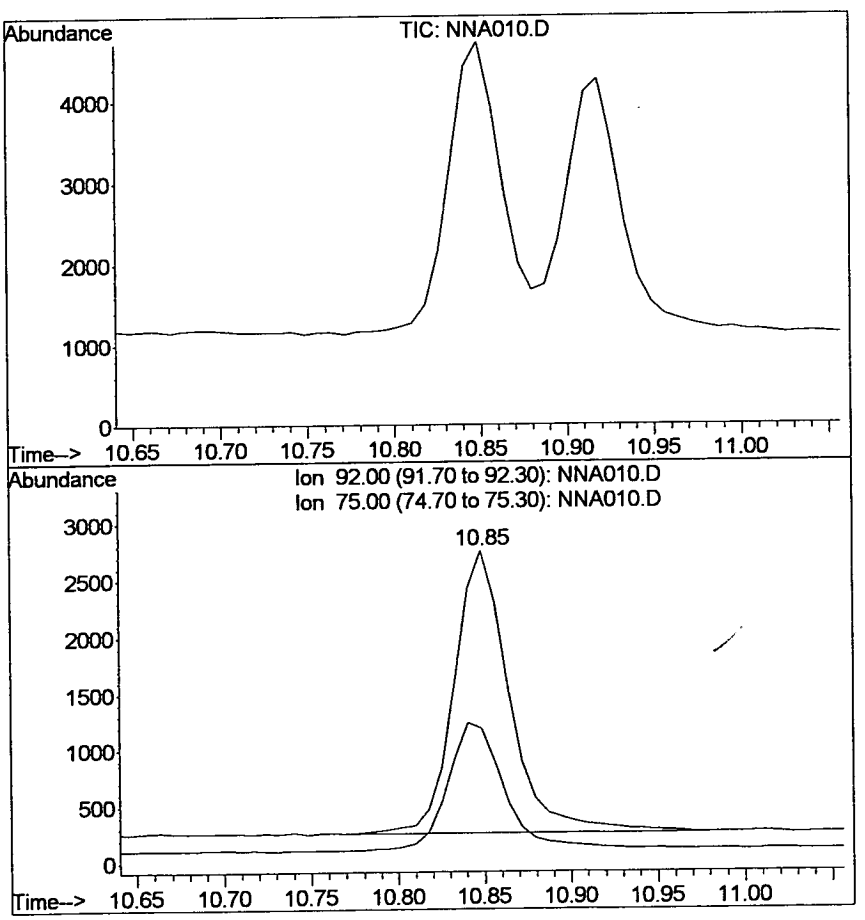

#2
NDMA
Concen: 10.58 PPB
RT: 10.85 min Scan# 165
Delta R.T. 0.02 min
Lab File: NNA010.D
Acq: 20 Jul 2007 4:30 pm

Tgt Ion: 92 Resp: 5566

Ion	Ratio	Lower	Upper
92	100		
75	46.3	31.8	66.0

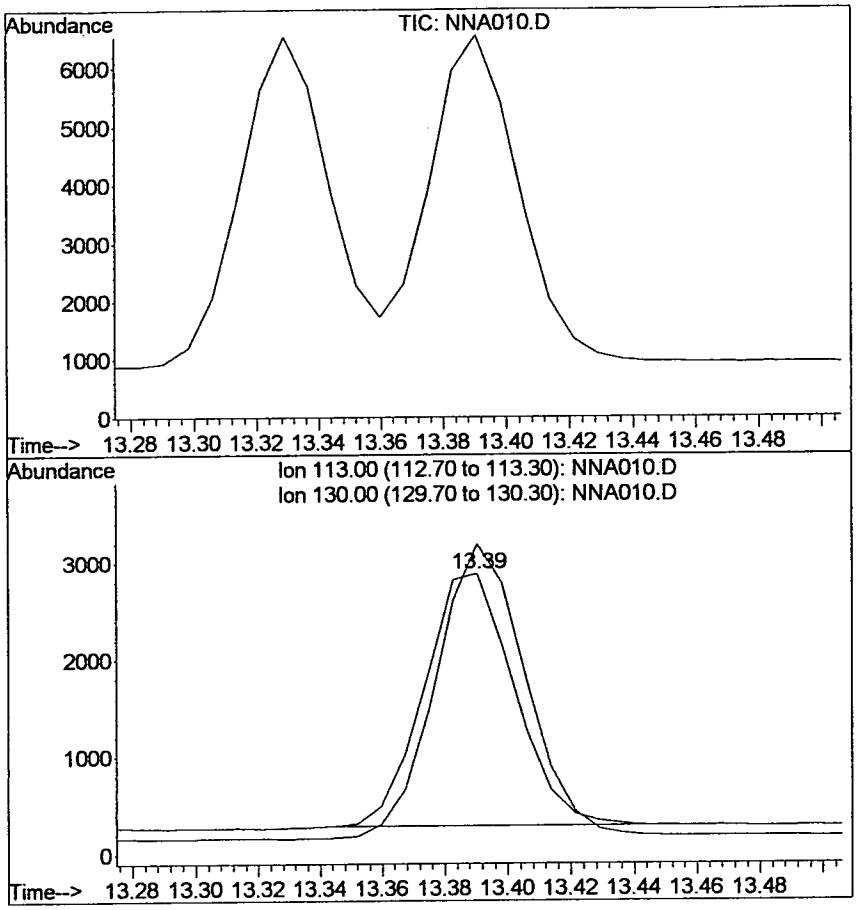

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.39 min Scan# 495
Delta R.T. 0.02 min
Lab File: NNA010.D
Acq: 20 Jul 2007 4:30 pm

Tgt Ion:113 Resp: 5142

Ion	Ratio	Lower	Upper
113	100		
130	114.4	67.1	137.1

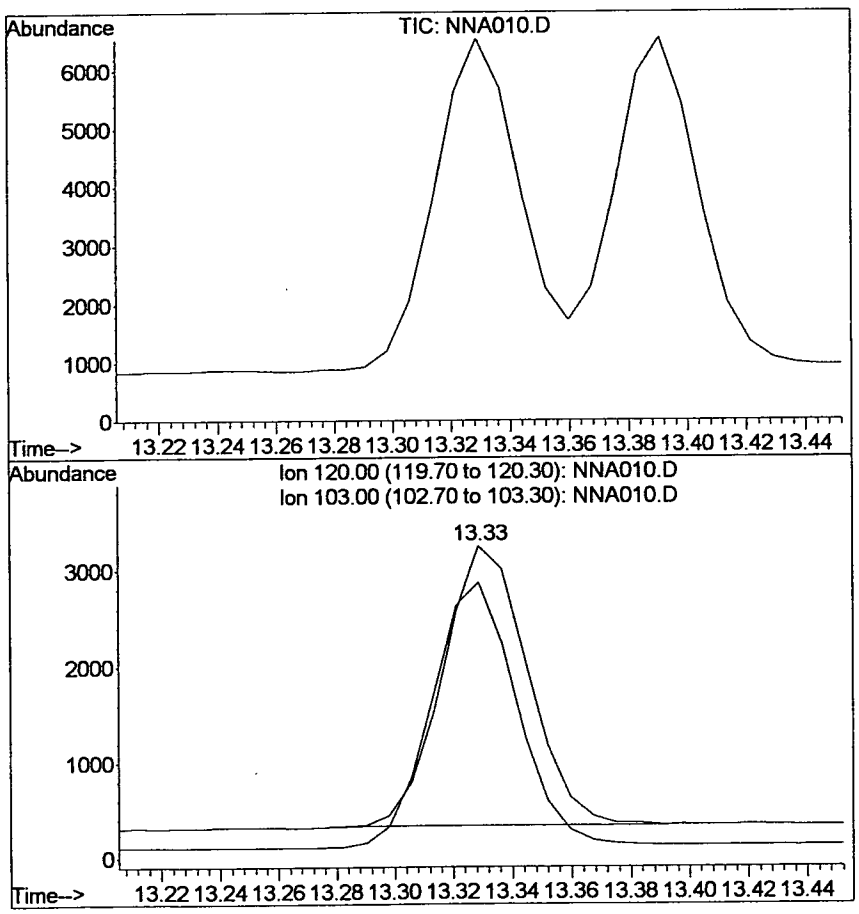

#4
NDEA
Concen: 10.58 PPB
RT: 13.33 min Scan# 487
Delta R.T. 0.01 min
Lab File: NNA010.D
Acq: 20 Jul 2007 4:30 pm

Tgt Ion:120 Resp: 5832

Ion	Ratio	Lower	Upper
120	100		
103	94.3	65.3	135.5

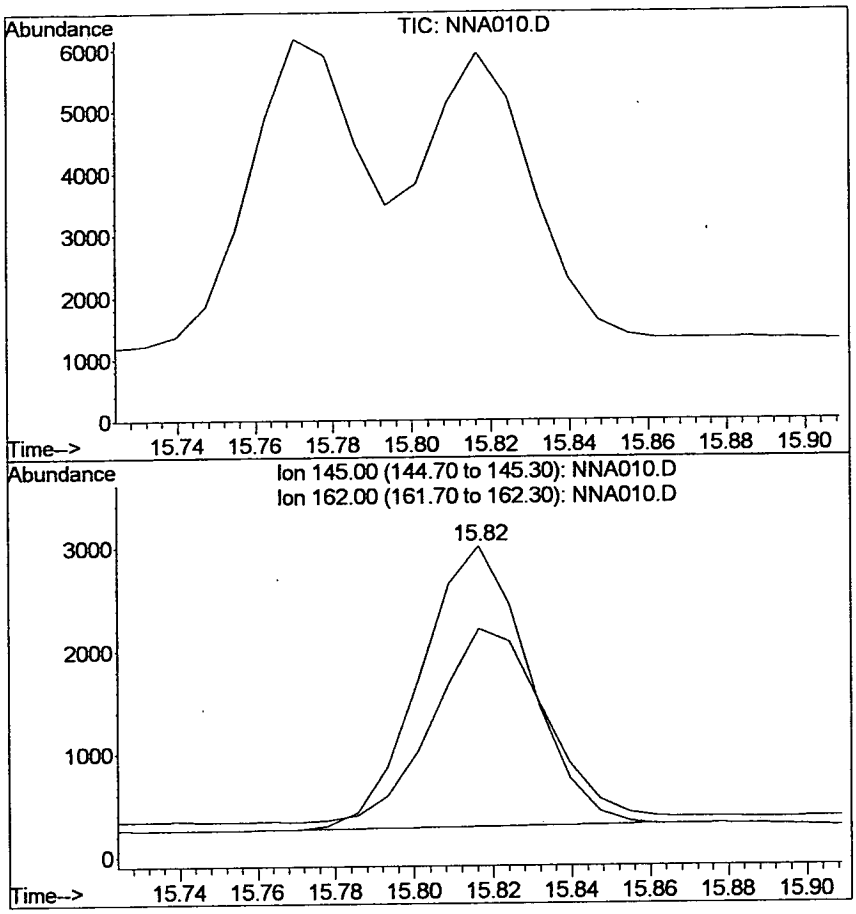

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.82 min Scan# 810
Delta R.T. 0.01 min
Lab File: NNA010.D
Acq: 20 Jul 2007 4:30 pm

Tgt Ion:145 Resp: 5188

Ion	Ratio	Lower	Upper
145	100		
162	69.5	22.4	102.4

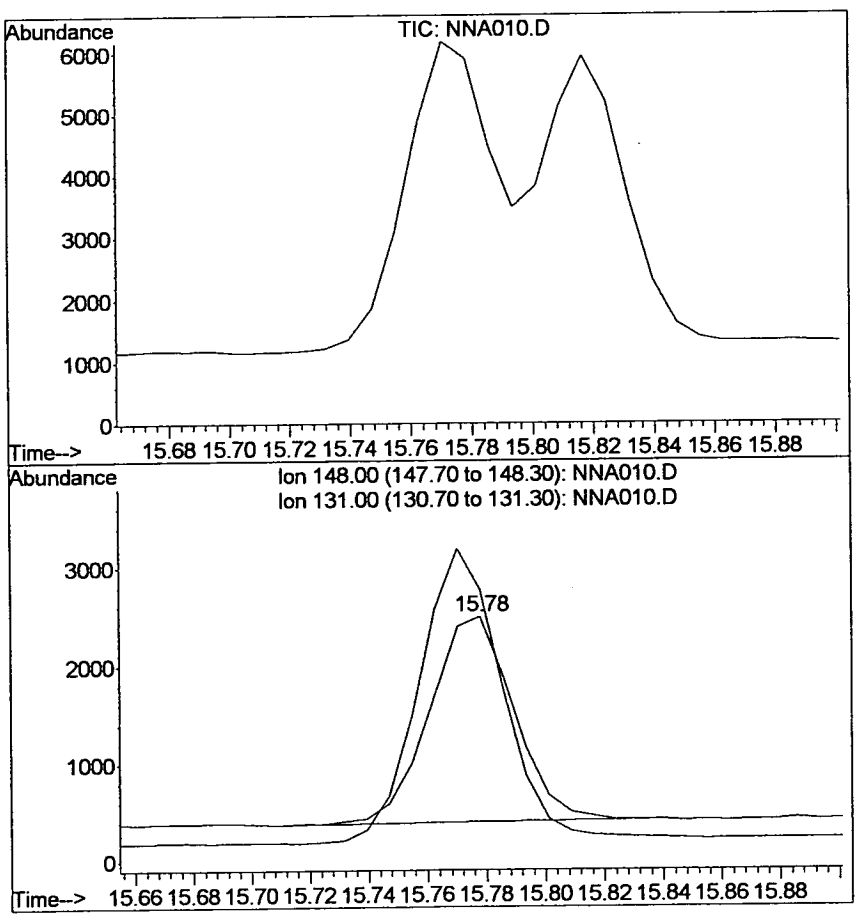

#6
NDPA
Concen: 9.95 PPB
RT: 15.78 min Scan# 805
Delta R.T. 0.01 min
Lab File: NNA010.D
Acq: 20 Jul 2007 4:30 pm

Tgt Ion:148 Resp: 4150

Ion	Ratio	Lower	Upper
148	100		
131	139.1	99.8	207.2

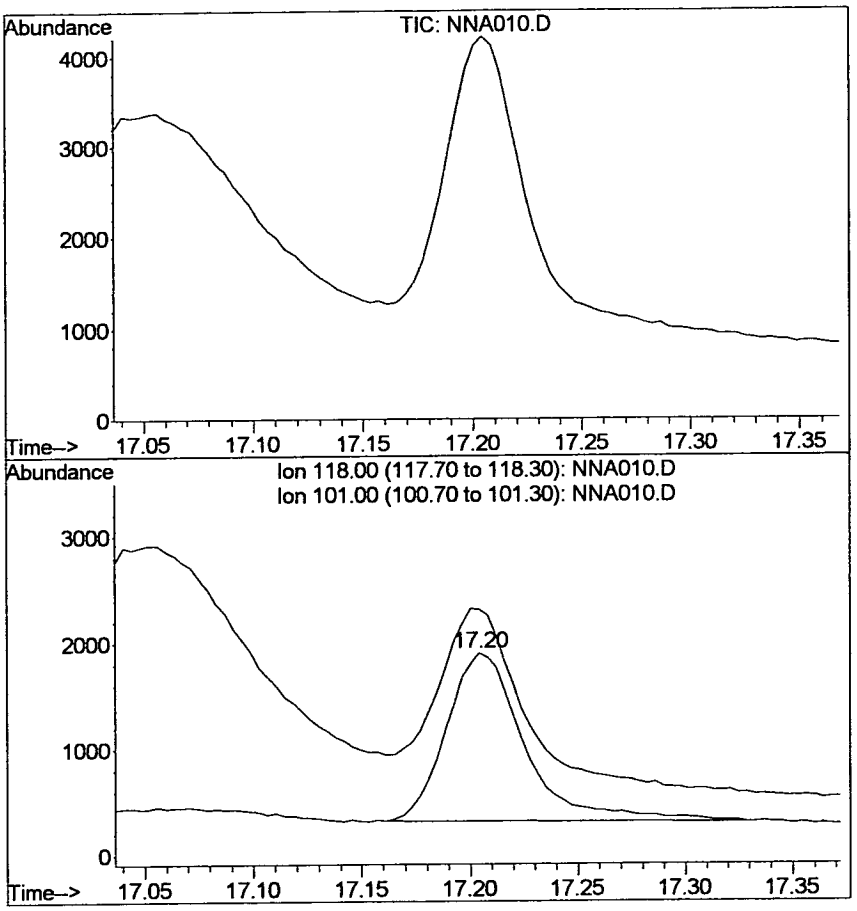

#7
NPYR
Concen: 9.56 PPB
RT: 17.20 min Scan# 1078
Delta R.T. 0.01 min
Lab File: NNA010.D
Acq: 20 Jul 2007 4:30 pm

Tgt Ion:118 Resp: 3969

Ion	Ratio	Lower	Upper
118	100		
101	83.4	62.6	130.0

Evaluate Continuing Calibration Report

Data File : C:\MSDCHEM\1\DATA\07JUL20\NNA010.D Vial: 1
Acq On : 20 Jul 2007 4:30 pm Operator: DF/AI
Sample : 10ppb Std.# 7060221 Inst : gcms37
Misc : n-Nitrosamines water Multiplr: 1.00
MS Integration Params: RTEINT2.P

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Multiple Level Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 200%

		Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1	I	NDMA-D6	1.000	1.000	0.0	93	0.00
2	T	NDMA	2.002	2.118	-5.8	94	0.02
3	I	NDEA-D10	1.000	1.000	0.0	95	0.02
4	T	NDEA	1.072	1.134	-5.8	96	0.00
5	I	NDPA-D14	1.000	1.000	0.0	106	0.00
6	T	NDPA	0.804	0.800	0.5	91	0.00
7	T	NPYR	0.800	0.765	4.4	99	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 0

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720001.D
Acq On : 20 Jul 2007 4:53 pm
Sample : 7G19061-BLK1
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 20 17:15 2007

Vial: 2
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration
DataAcq Meth : C7F14NW

Internal Standards	R.T.	QIon	Response	Conc	Units		LB Dev(Min)
1) NDMA-D6	10.91	81	2341	10.00	PPB		0.00
3) NDEA-D10	13.39	113	5008	10.00	PPB		0.02
5) NDPA-D14	15.82	145	5209	10.00	PPB		0.00
Target Compounds							Qvalue
2) NDMA	10.84	92	60	0.13	PPB		79
4) NDEA	13.33	120	121	0.23	PPB		86
6) NDPA	15.76	148	349	0.83	PPB	#	1
7) NPYR	17.19	118	6	0.01	PPB	#	2

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720001.D
Acq On : 20 Jul 2007 4:53 pm
Sample : 7G19061-BLK1
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 20 17:15 2007

Vial: 2
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration

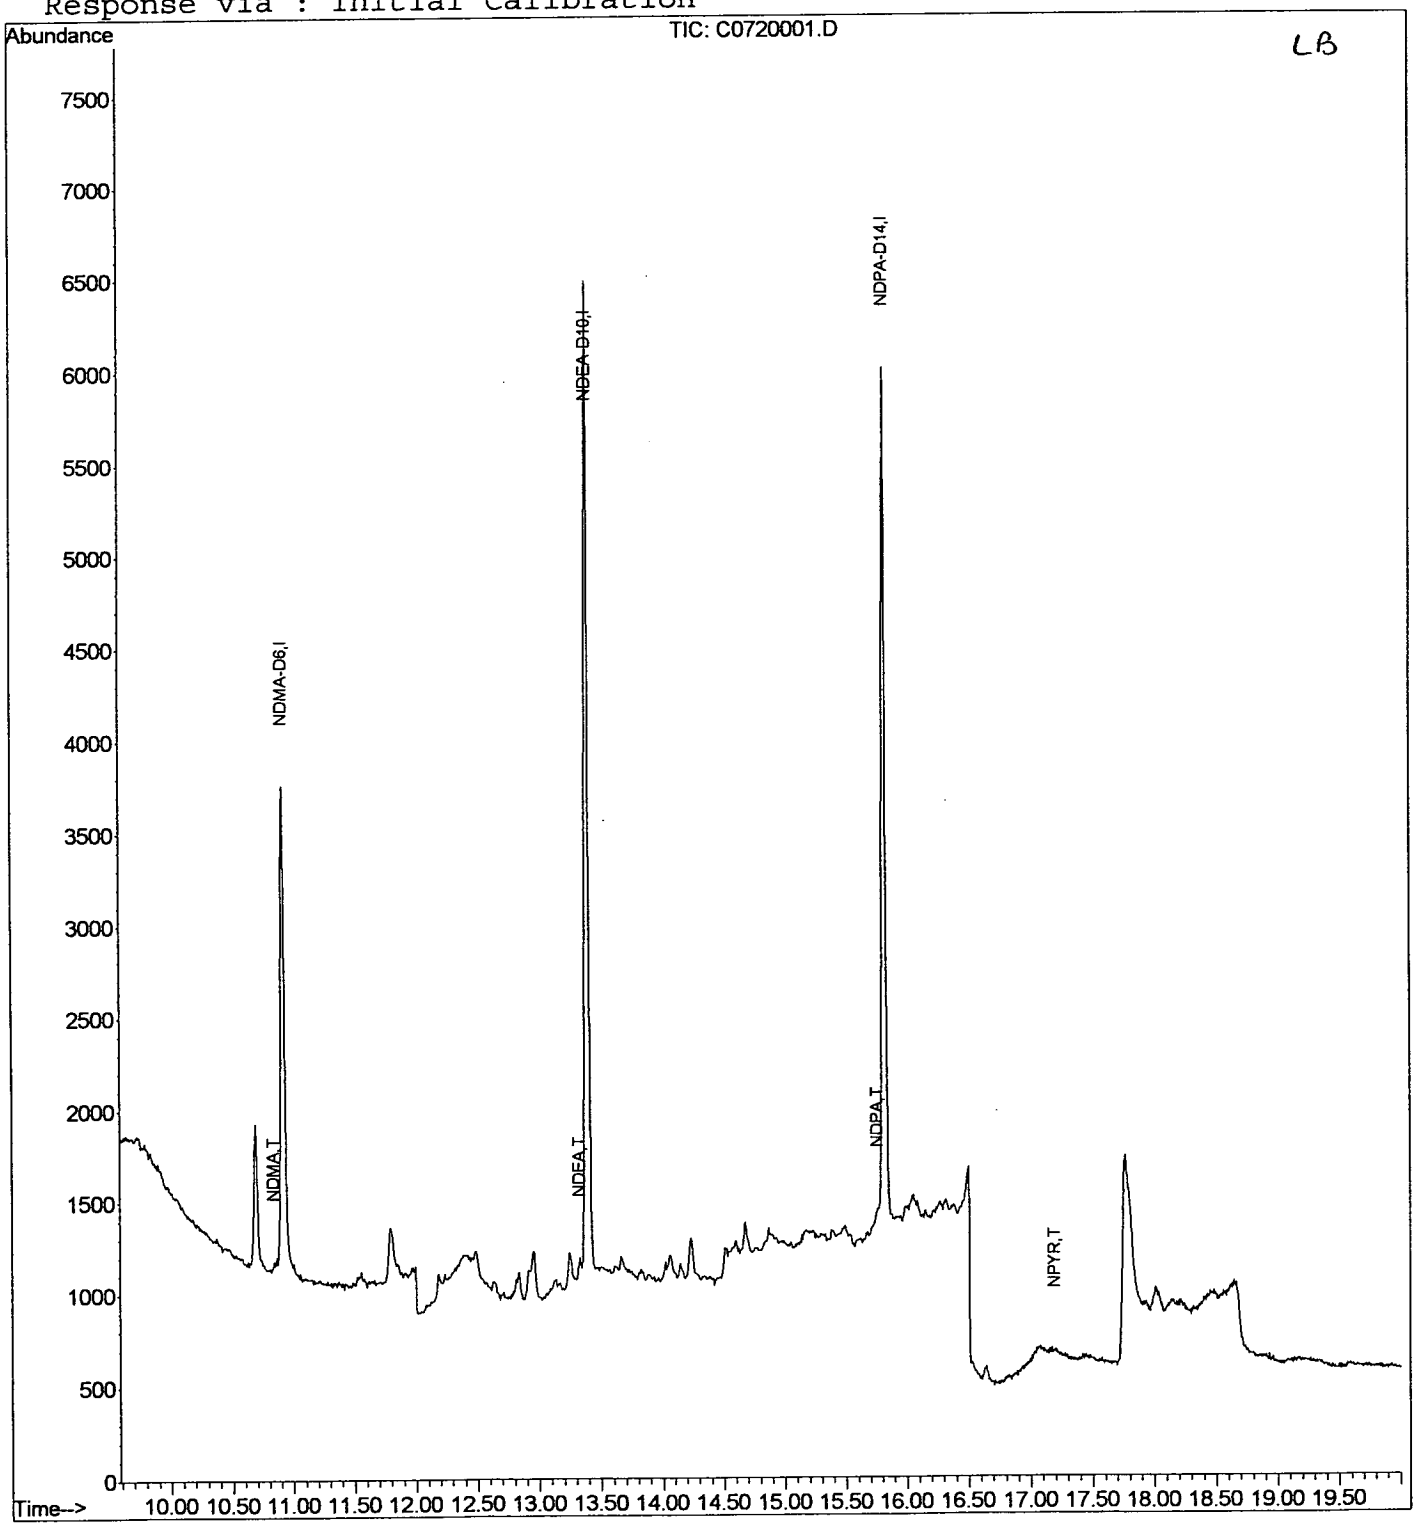

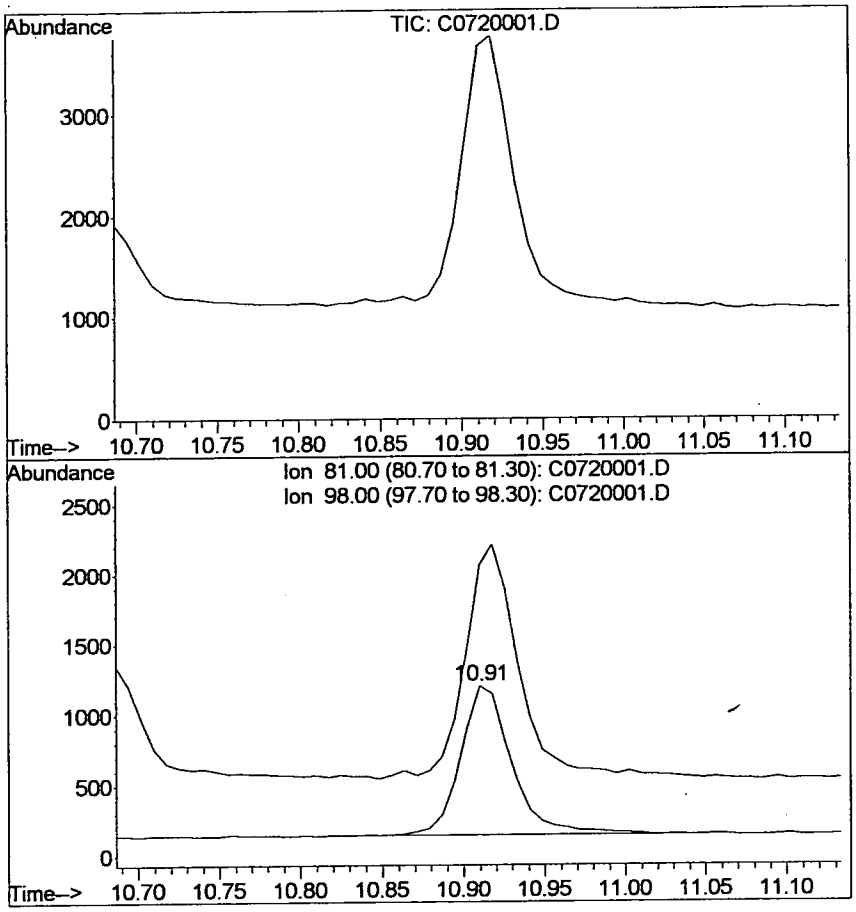

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.91 min Scan# 173
Delta R.T. 0.01 min
Lab File: C0720001.D
Acq: 20 Jul 2007 4:53 pm

Tgt Ion: 81 Resp: 2341

Ion	Ratio	Lower	Upper
81	100		
98	156.8	144.1	224.1

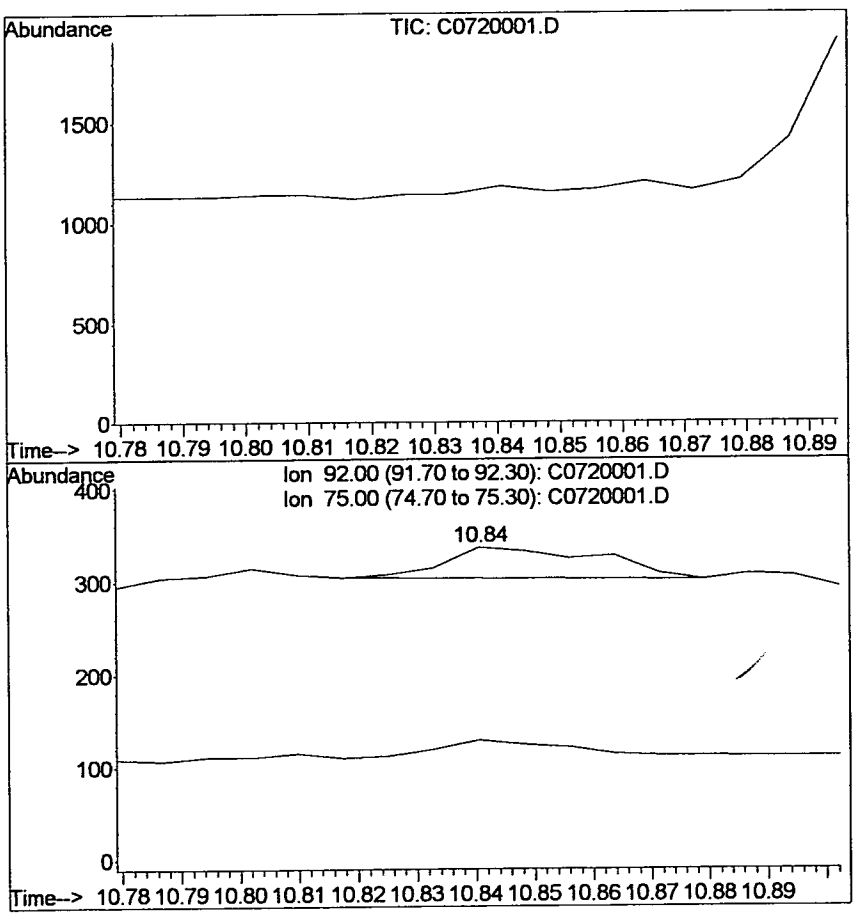

#2
NDMA
Concen: 0.13 PPB
RT: 10.84 min Scan# 164
Delta R.T. 0.01 min
Lab File: C0720001.D
Acq: 20 Jul 2007 4:53 pm

Tgt Ion: 92 Resp: 60

Ion	Ratio	Lower	Upper
92	100		
75	63.3	31.8	66.0

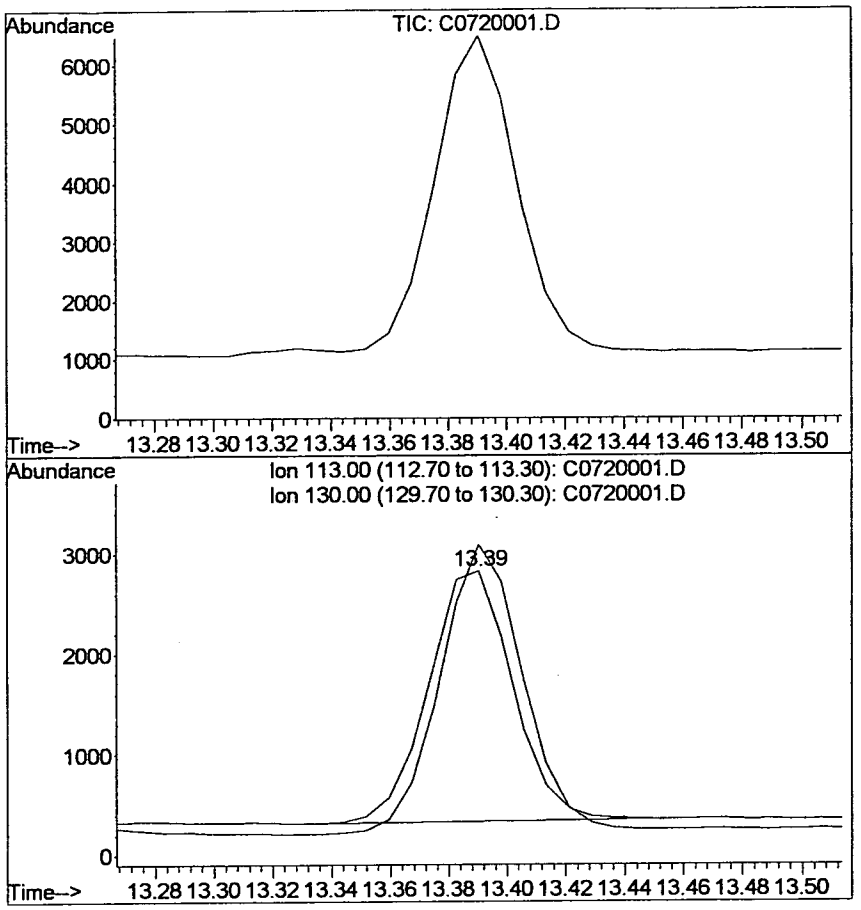

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.39 min Scan# 495
Delta R.T. 0.02 min
Lab File: C0720001.D
Acq: 20 Jul 2007 4:53 pm

Tgt Ion:113 Resp: 5008

Ion	Ratio	Lower	Upper
113	100		
130	110.7	67.1	137.1

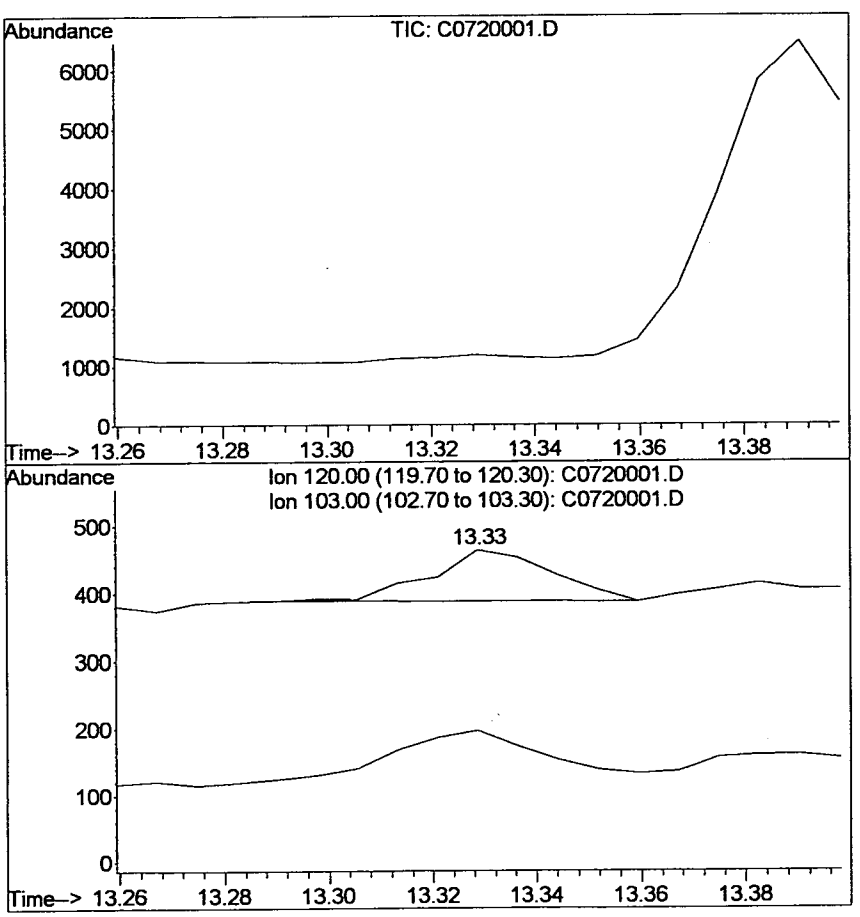

#4
NDEA
Concen: 0.23 PPB
RT: 13.33 min Scan# 487
Delta R.T. 0.01 min
Lab File: C0720001.D
Acq: 20 Jul 2007 4:53 pm

Tgt Ion:120 Resp: 121

Ion	Ratio	Lower	Upper
120	100		
103	114.9	65.3	135.5

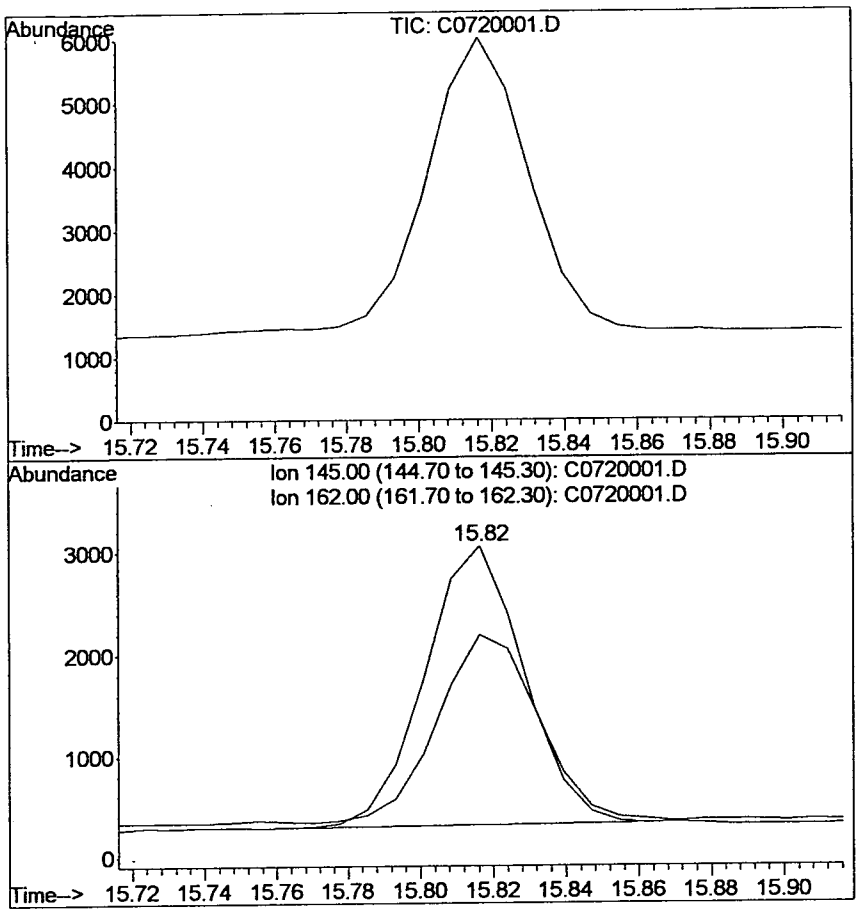

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.82 min Scan# 810
Delta R.T. 0.01 min
Lab File: C0720001.D
Acq: 20 Jul 2007 4:53 pm

Tgt Ion:145 Resp: 5209

Ion	Ratio	Lower	Upper
145	100		
162	68.9	22.4	102.4

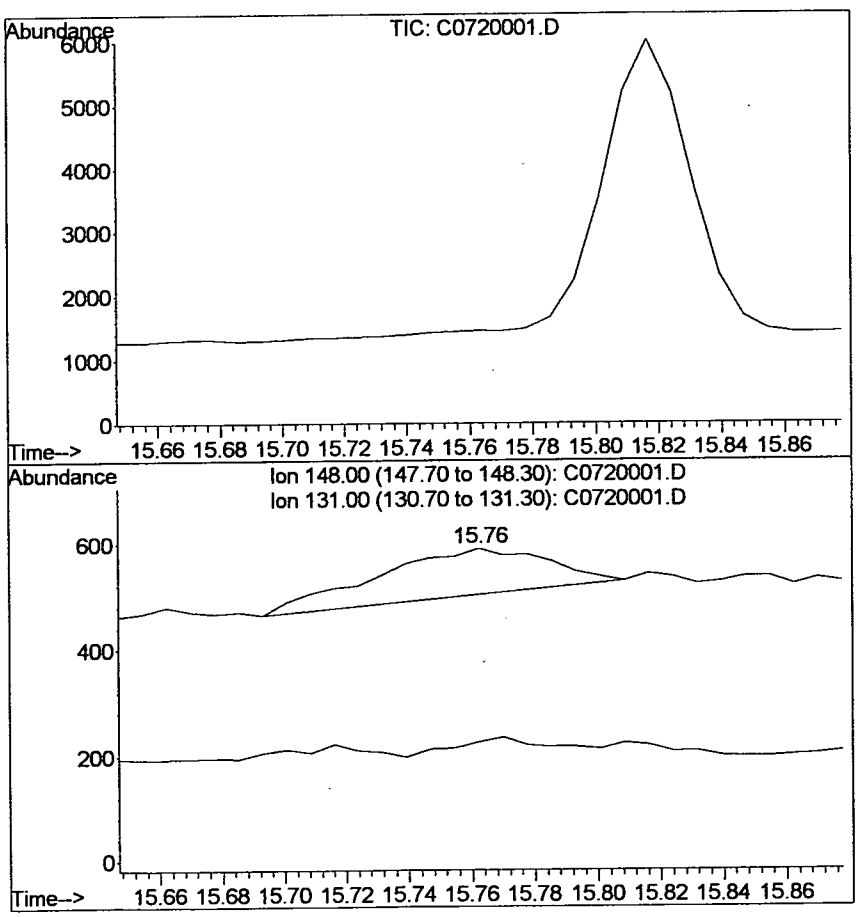

#6
NDPA
Concen: 0.83 PPB
RT: 15.76 min Scan# 803
Delta R.T. -0.01 min
Lab File: C0720001.D
Acq: 20 Jul 2007 4:53 pm

Tgt Ion:148 Resp: 349

Ion	Ratio	Lower	Upper
148	100		
131	10.6	99.8	207.2#

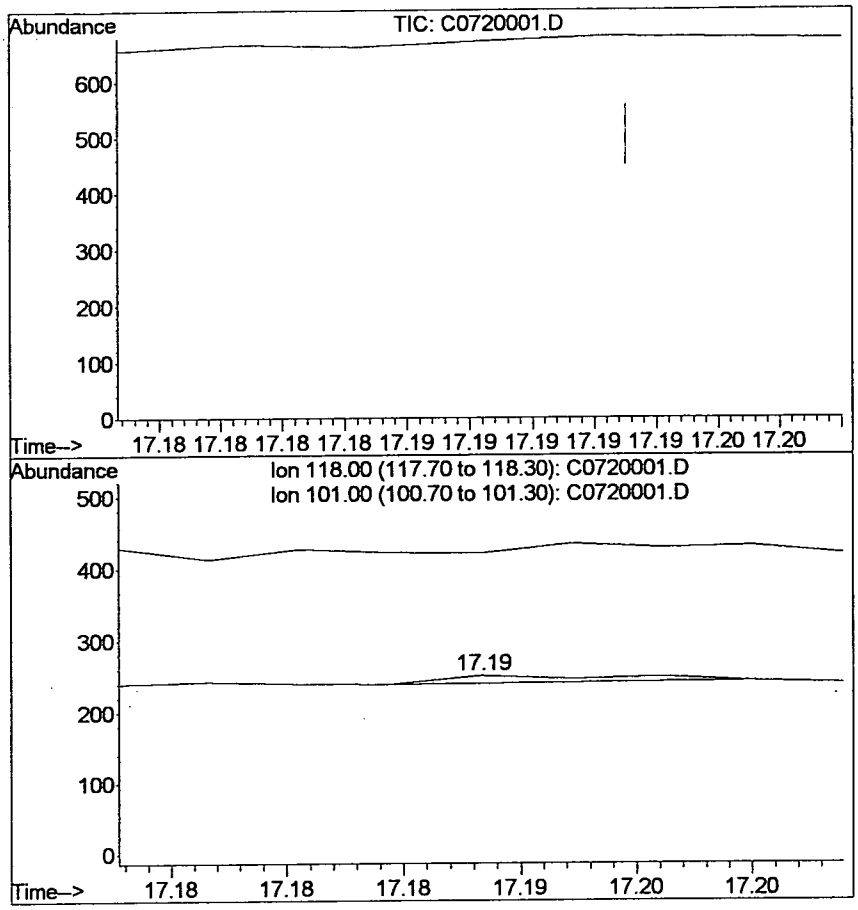

#7
NPYR
Concen: 0.01 PPB
RT: 17.19 min Scan# 1074
Delta R.T. -0.01 min
Lab File: C0720001.D
Acq: 20 Jul 2007 4:53 pm

Tgt Ion:118 Resp: 6

Ion	Ratio	Lower	Upper
118	100		
101	0.0	62.6	130.0#

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720002.D
Acq On : 20 Jul 2007 5:17 pm
Sample : 7G19061-BS1
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 20 17:43 2007

Vial: 3
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00

Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration
DataAcq Meth : C7F14NW

LB

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) NDMA-D6	10.92	81	2280	10.00 PPB	0.02
3) NDEA-D10	13.39	113	4776	10.00 PPB	0.02
5) NDPA-D14	15.82	145	5300	10.00 PPB	0.00

Target Compounds					Qvalue
2) NDMA	10.85	92	4310	9.44 PPB	96
4) NDEA	13.33	120	4697	9.17 PPB	93
6) NDPA	15.78	148	3863	9.07 PPB	86
7) NPYR	17.20	118	3999	9.43 PPB	99

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720002.D
Acq On : 20 Jul 2007 5:17 pm
Sample : 7G19061-BS1
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 20 17:43 2007

Vial: 3
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration

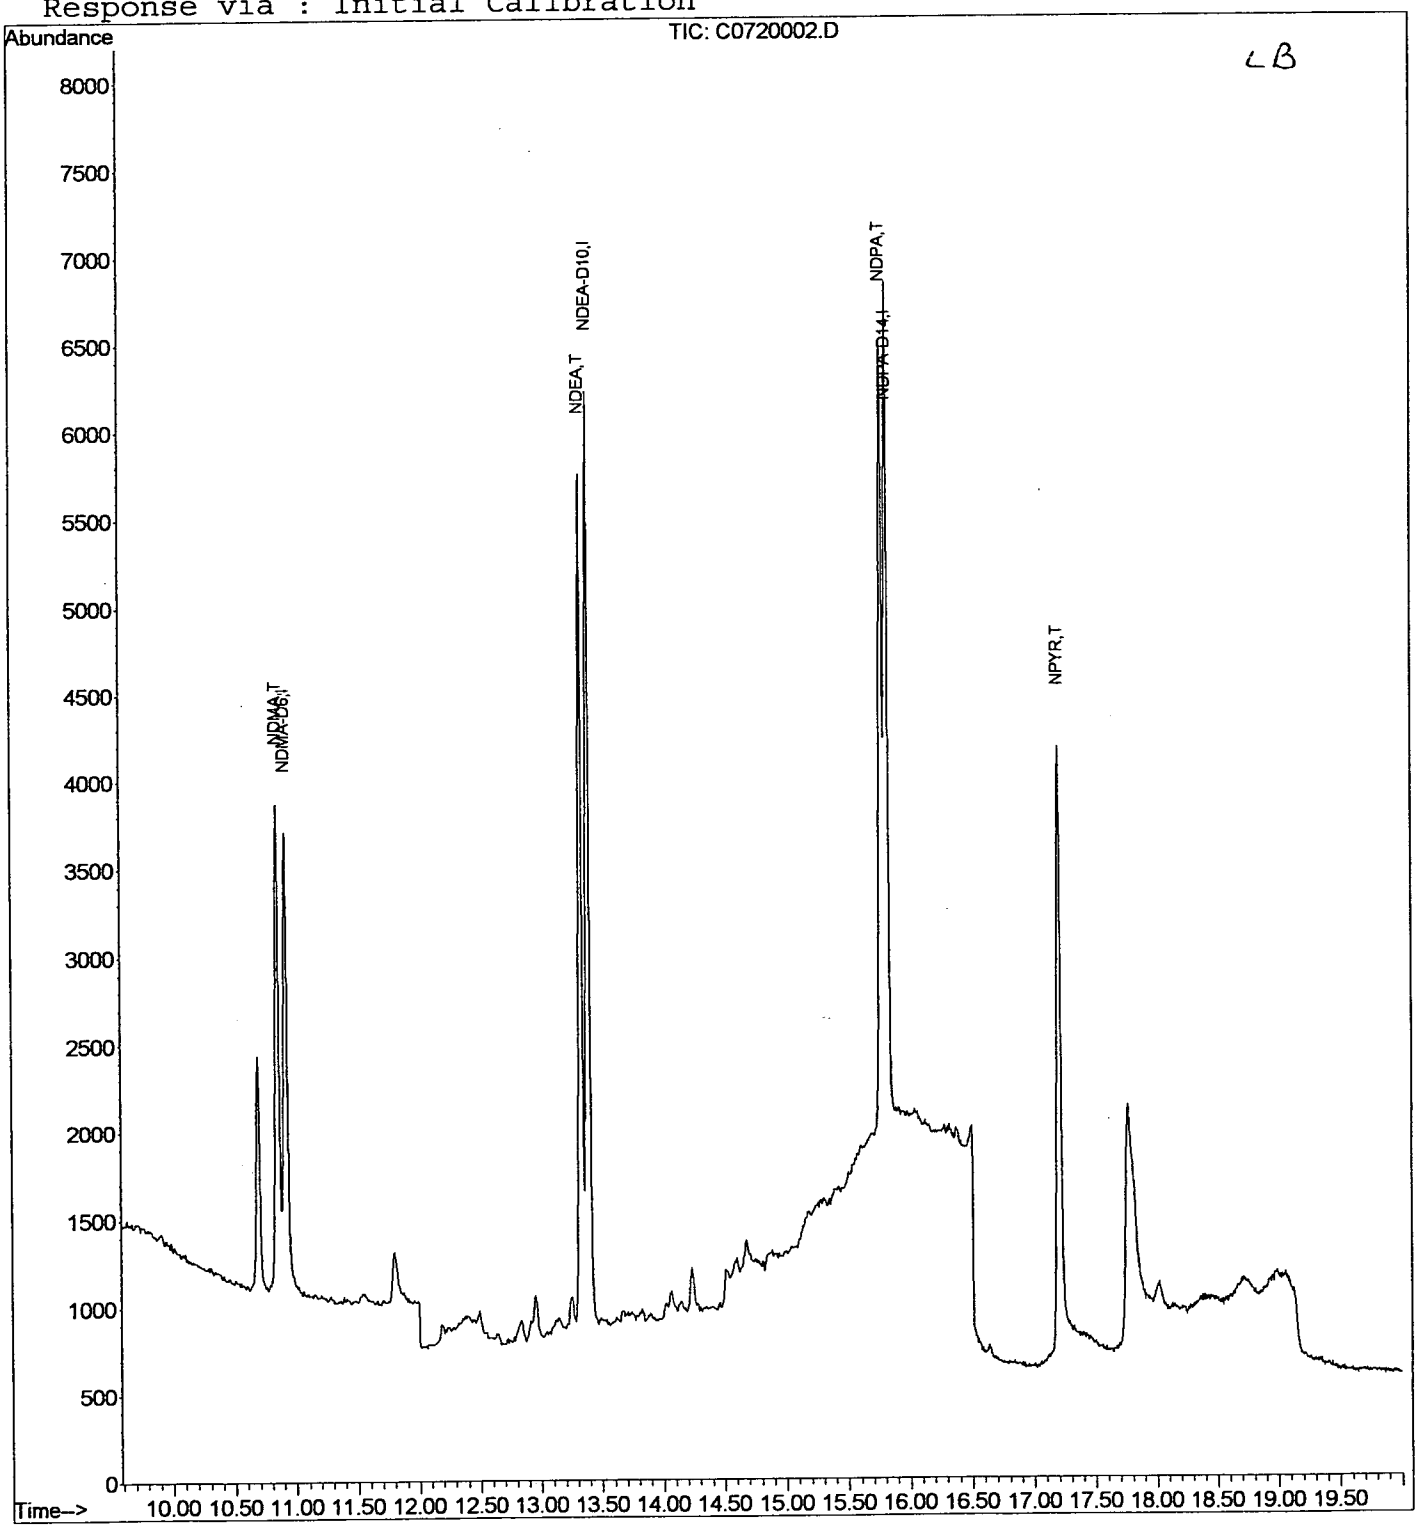

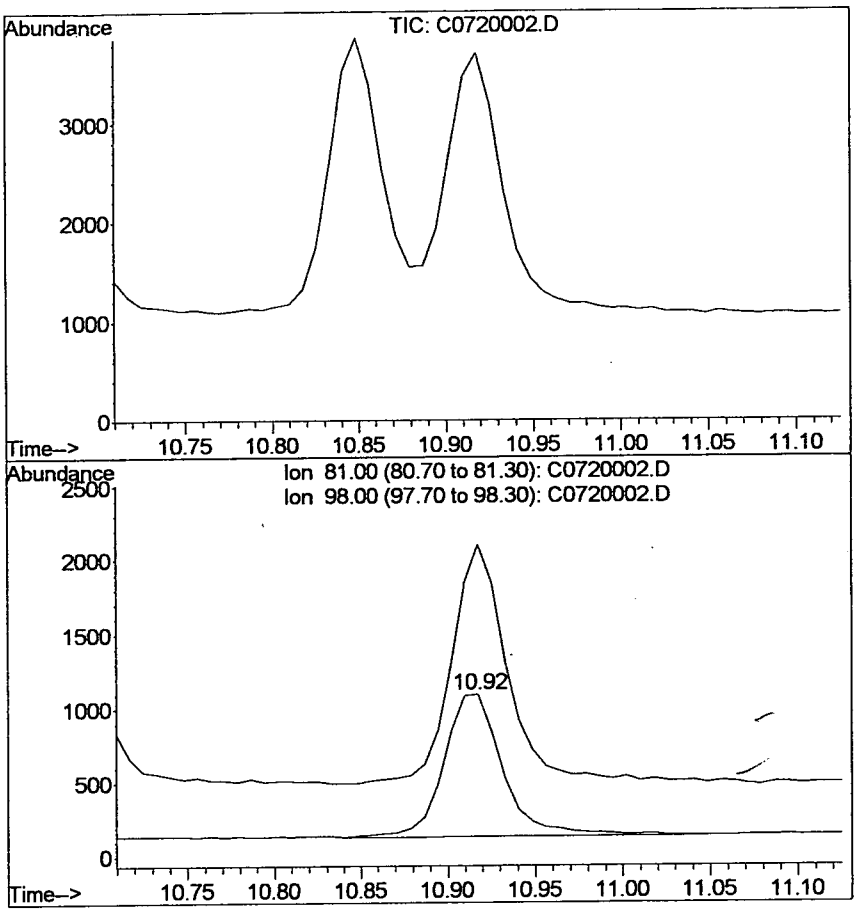

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.92 min Scan# 174
Delta R.T. 0.02 min
Lab File: C0720002.D
Acq: 20 Jul 2007 5:17 pm

Tgt Ion: 81 Resp: 2280

Ion	Ratio	Lower	Upper
81	100		
98	152.0	144.1	224.1

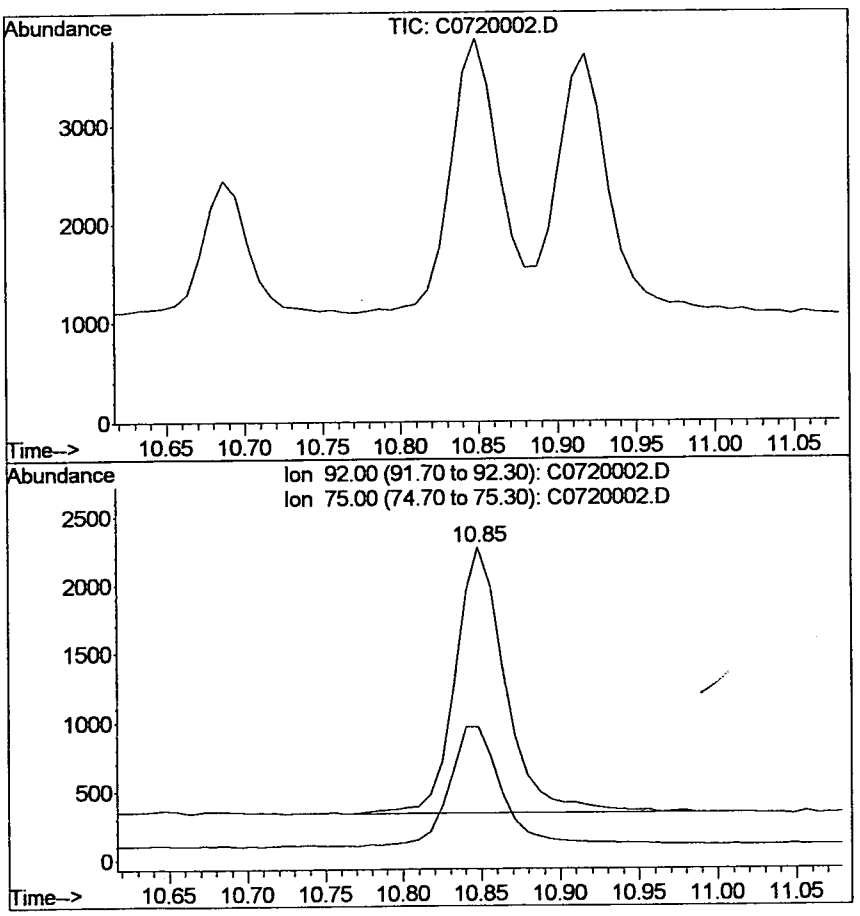

#2
NDMA
Concen: 9.44 PPB
RT: 10.85 min Scan# 165
Delta R.T. 0.02 min
Lab File: C0720002.D
Acq: 20 Jul 2007 5:17 pm

Tgt Ion: 92 Resp: 4310

Ion	Ratio	Lower	Upper
92	100		
75	46.5	31.8	66.0

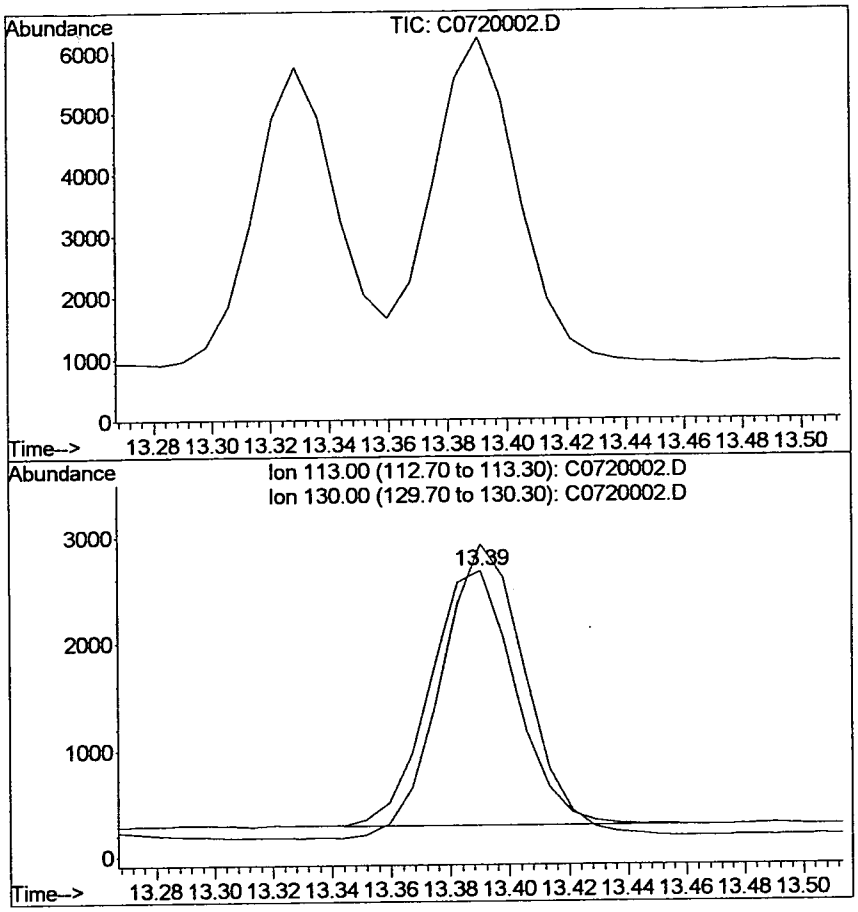

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.39 min Scan# 495
Delta R.T. 0.02 min
Lab File: C0720002.D
Acq: 20 Jul 2007 5:17 pm

Tgt Ion:113 Resp: 4776

Ion	Ratio	Lower	Upper
113	100		
130	114.2	67.1	137.1

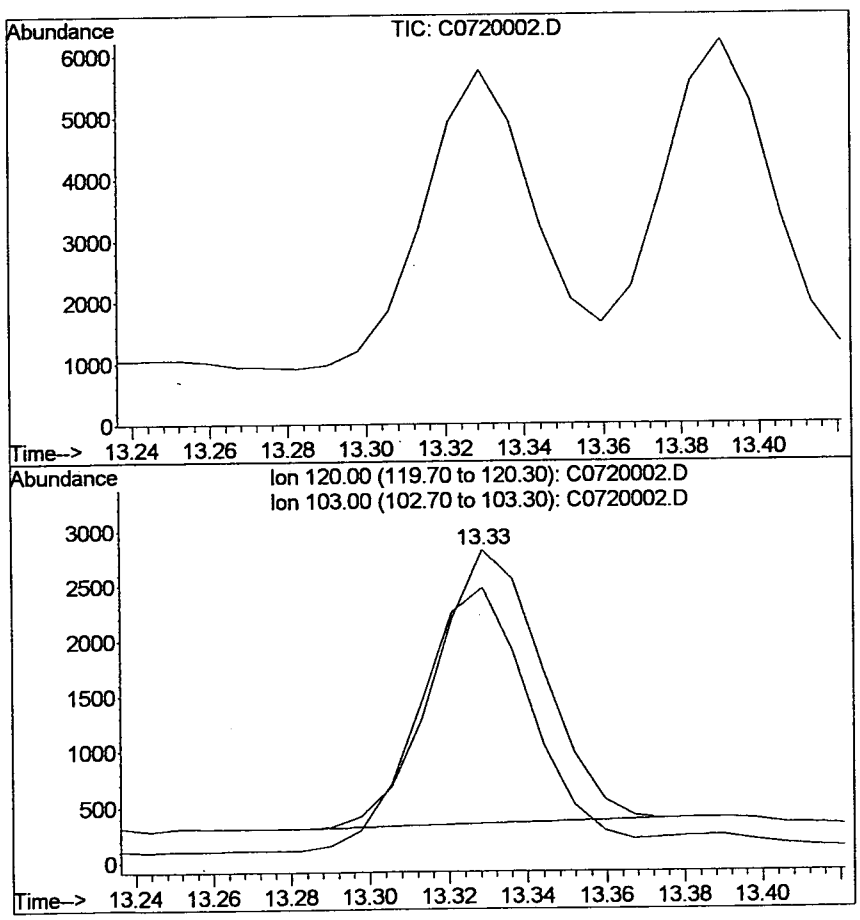

#4
NDEA
Concen: 9.17 PPB
RT: 13.33 min Scan# 487
Delta R.T. 0.01 min
Lab File: C0720002.D
Acq: 20 Jul 2007 5:17 pm

Tgt Ion:120 Resp: 4697

Ion	Ratio	Lower	Upper
120	100		
103	93.6	65.3	135.5

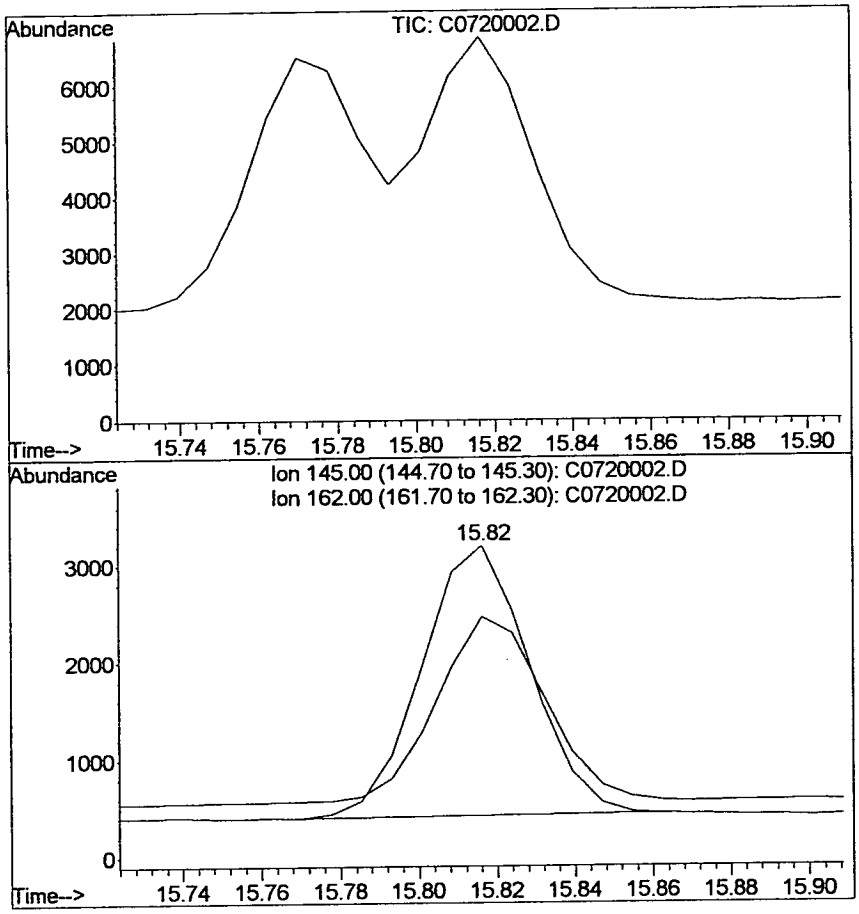

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.82 min Scan# 810
Delta R.T. 0.01 min
Lab File: C0720002.D
Acq: 20 Jul 2007 5:17 pm

Tgt Ion:145 Resp: 5300

Ion	Ratio	Lower	Upper
145	100		
162	68.4	22.4	102.4

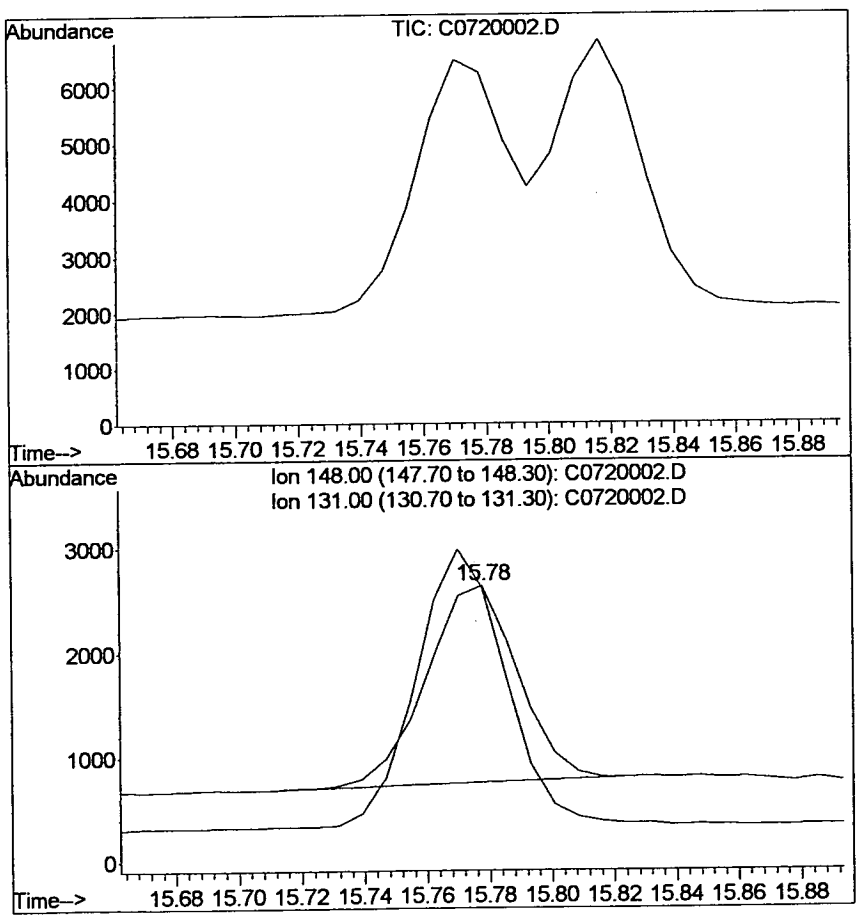

#6
NDPA
Concen: 9.07 PPB
RT: 15.78 min Scan# 805
Delta R.T. 0.01 min
Lab File: C0720002.D
Acq: 20 Jul 2007 5:17 pm

Tgt Ion:148 Resp: 3863

Ion	Ratio	Lower	Upper
148	100		
131	135.1	99.8	207.2

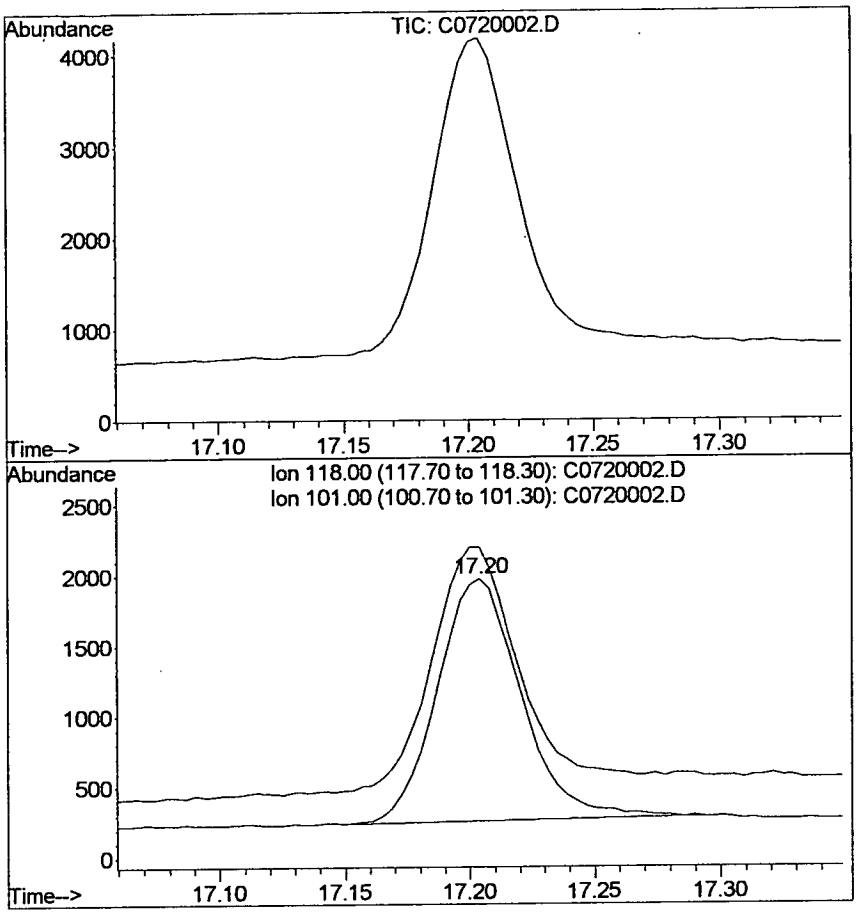

#7
NPYR
Concen: 9.43 PPB
RT: 17.20 min Scan# 1078
Delta R.T. 0.01 min
Lab File: C0720002.D
Acq: 20 Jul 2007 5:17 pm

Tgt Ion:118 Resp: 3999

Ion	Ratio	Lower	Upper
118	100		
101	97.0	62.6	130.0

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720003.D
Acq On : 20 Jul 2007 5:40 pm
Sample : 7G19061-BS2
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 20 18:03 2007

Vial: 4
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00

Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration
DataAcq Meth : C7F14NW

LB

Internal Standards	R.T.	QIon	Response	Conc	Units		Dev(Min)
1) NDMA-D6	10.91	81	2372	10.00	PPB		0.00
3) NDEA-D10	13.39	113	5096	10.00	PPB		0.02
5) NDPA-D14	15.82	145	5248	10.00	PPB		0.00

Target Compounds							Qvalue
2) NDMA	10.85	92	980	2.06	PPB		97
4) NDEA	13.33	120	1101	2.02	PPB		91
6) NDPA	15.77	148	1253	2.97	PPB	#	50
7) NPYR	17.20	118	795	1.89	PPB		95

(#) = qualifier out of range (m) = manual integration
C0720003.D C7F14NW.M Fri Jul 20 18:03:18 2007

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720003.D
Acq On : 20 Jul 2007 5:40 pm
Sample : 7G19061-BS2
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 20 18:03 2007

Vial: 4
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration

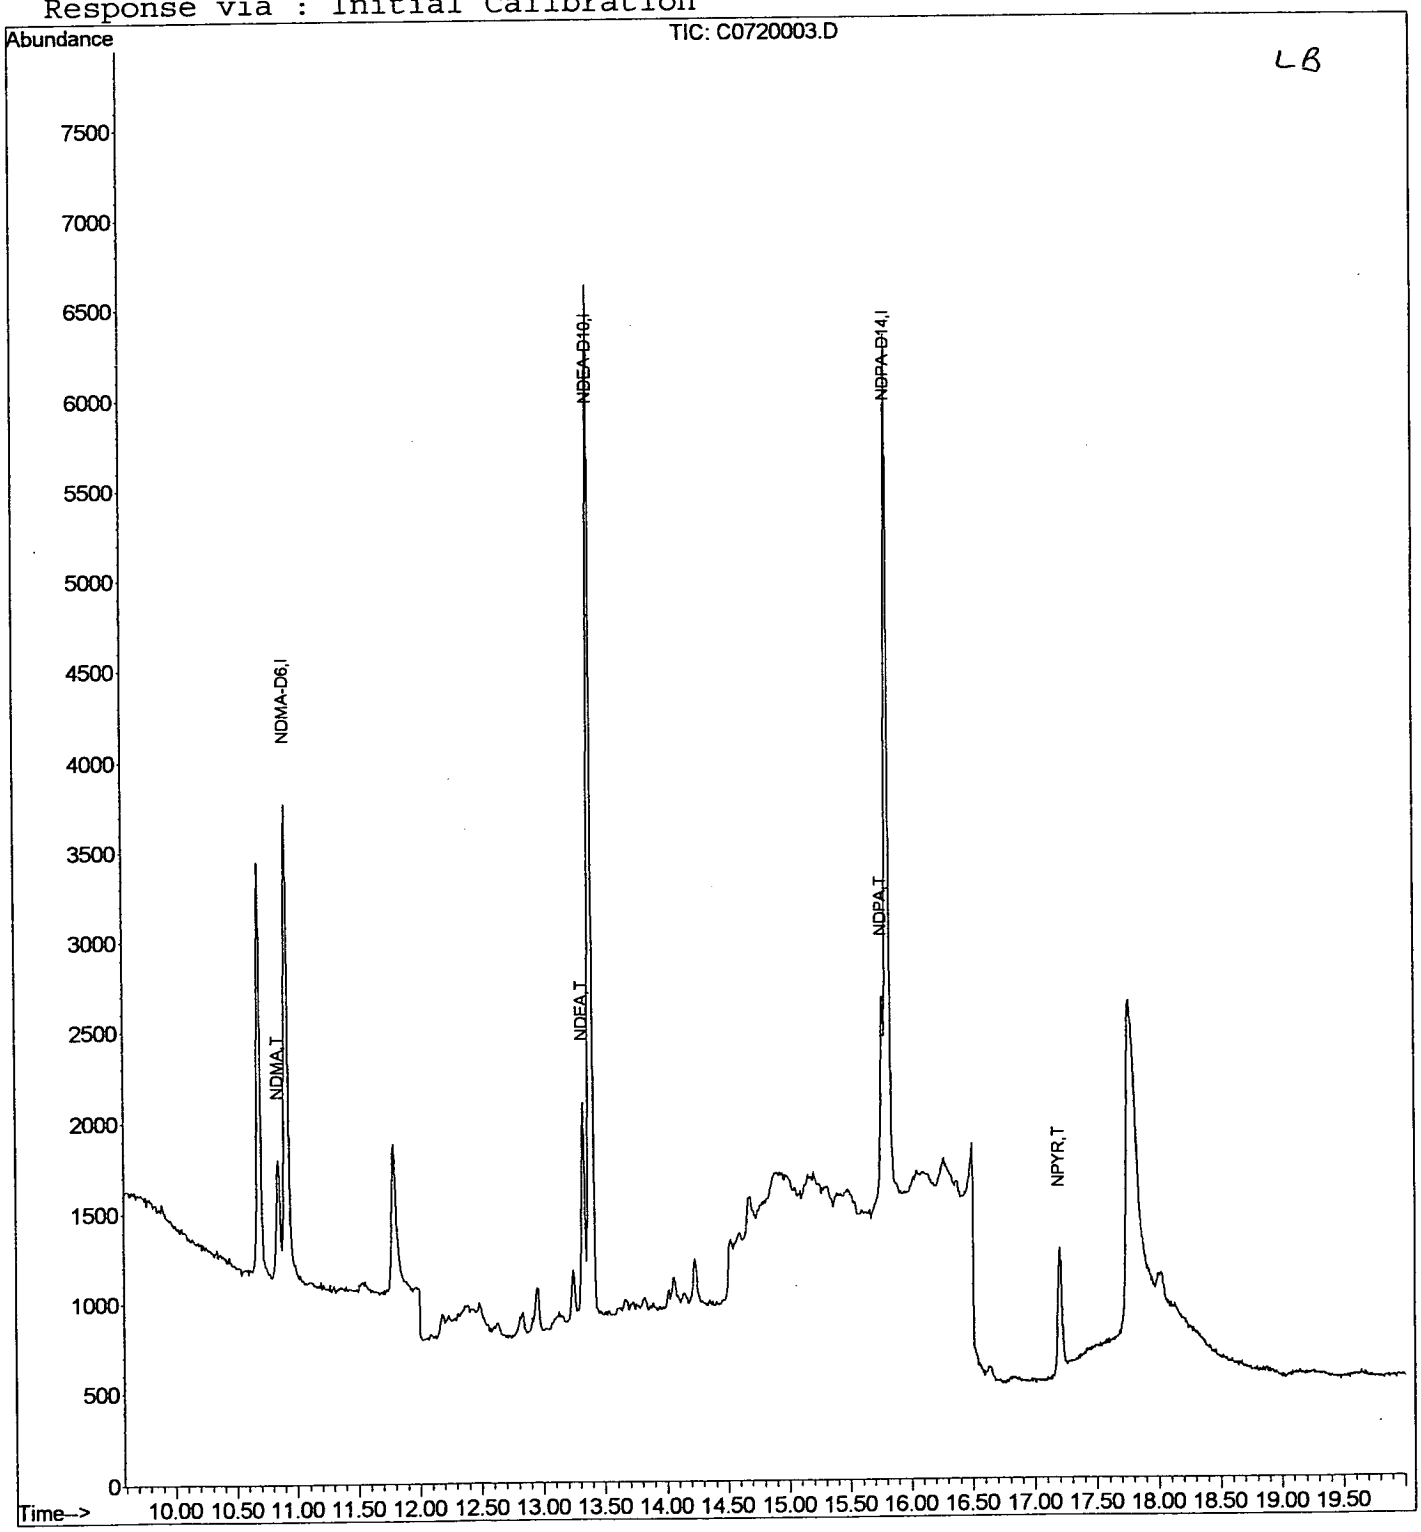

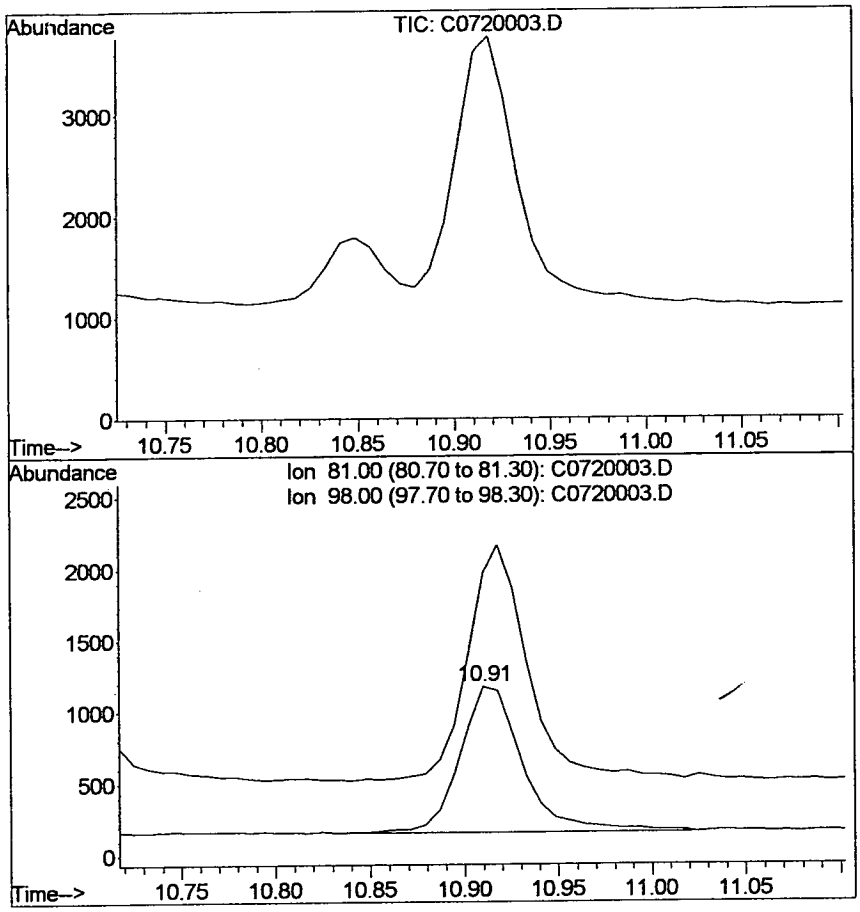

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.91 min Scan# 173
Delta R.T. 0.01 min
Lab File: C0720003.D
Acq: 20 Jul 2007 5:40 pm

Tgt Ion: 81 Resp: 2372

Ion	Ratio	Lower	Upper
81	100		
98	154.8	144.1	224.1

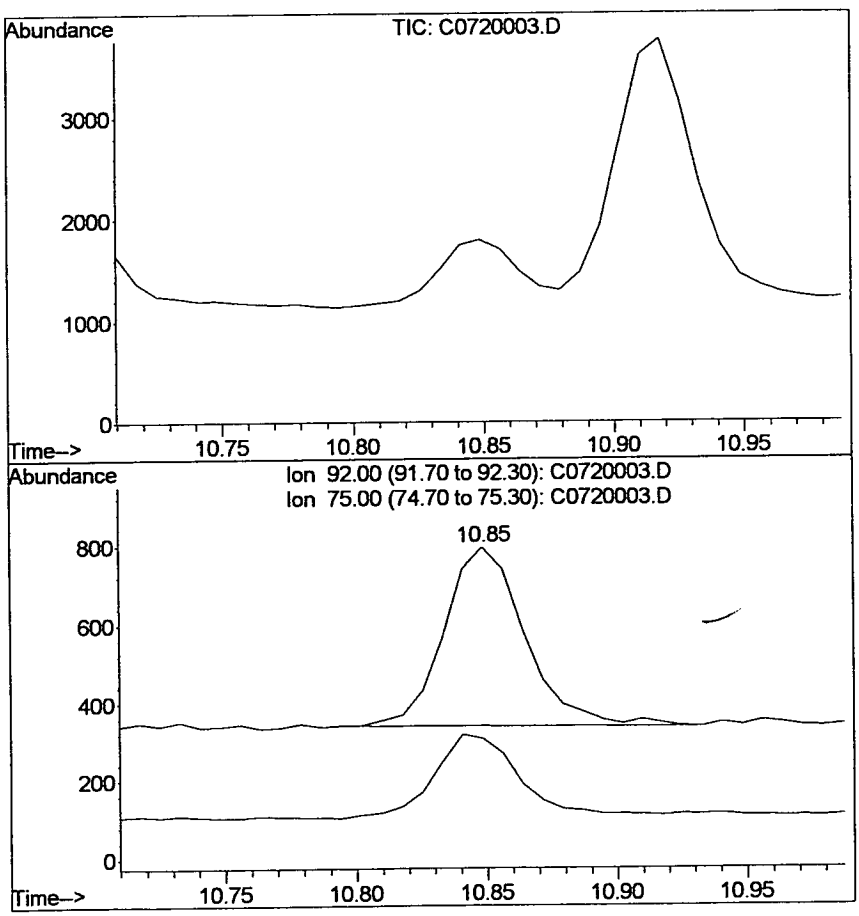

#2
NDMA
Concen: 2.06 PPB
RT: 10.85 min Scan# 165
Delta R.T. 0.02 min
Lab File: C0720003.D
Acq: 20 Jul 2007 5:40 pm

Tgt Ion: 92 Resp: 980

Ion	Ratio	Lower	Upper
92	100		
75	47.1	31.8	66.0

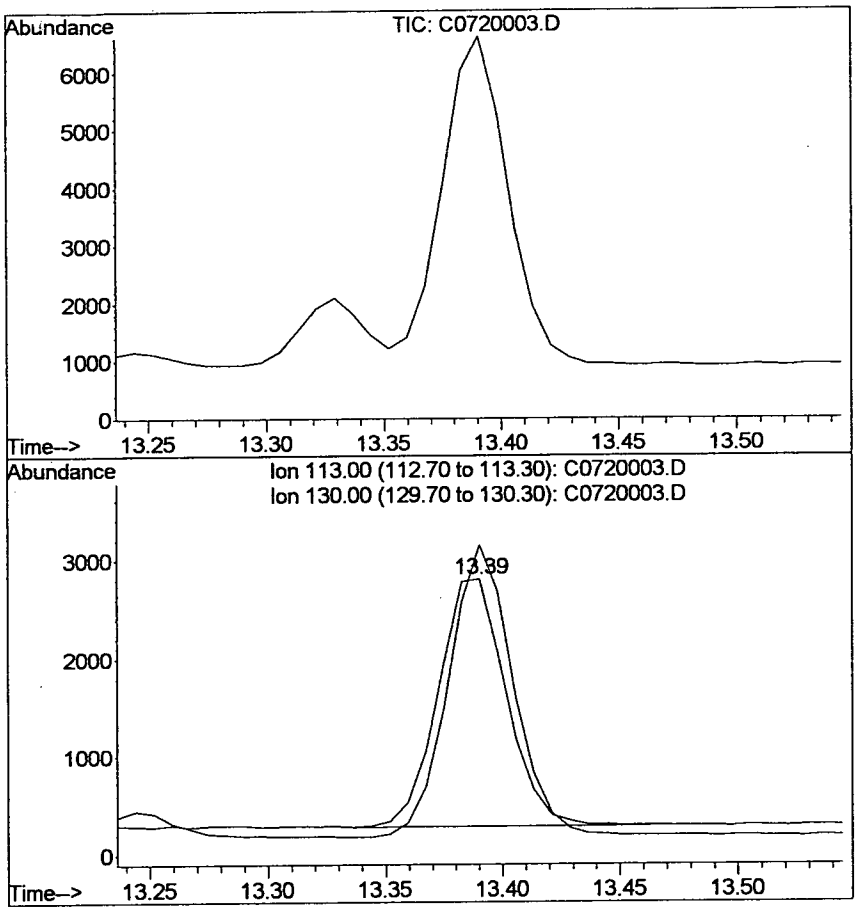

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.39 min Scan# 495
Delta R.T. 0.02 min
Lab File: C0720003.D
Acq: 20 Jul 2007 5:40 pm

Tgt Ion:113 Resp: 5096

Ion	Ratio	Lower	Upper
113	100		
130	110.7	67.1	137.1

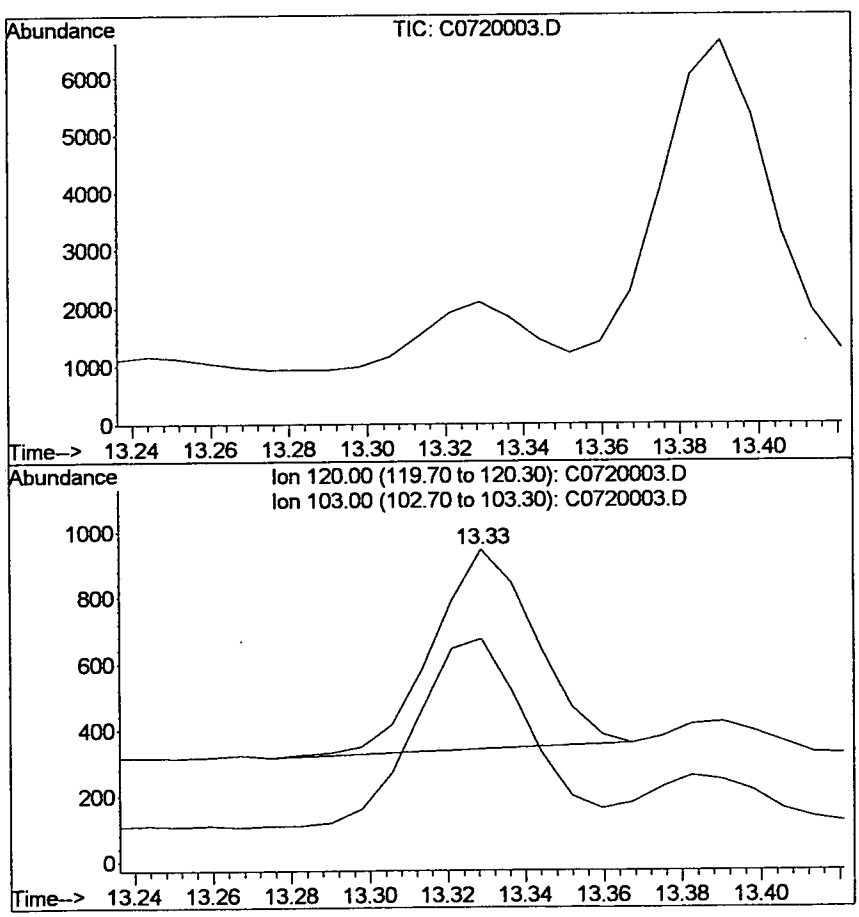

#4
NDEA
Concen: 2.02 PPB
RT: 13.33 min Scan# 487
Delta R.T. 0.01 min
Lab File: C0720003.D
Acq: 20 Jul 2007 5:40 pm

Tgt Ion:120 Resp: 1101

Ion	Ratio	Lower	Upper
120	100		
103	91.3	65.3	135.5

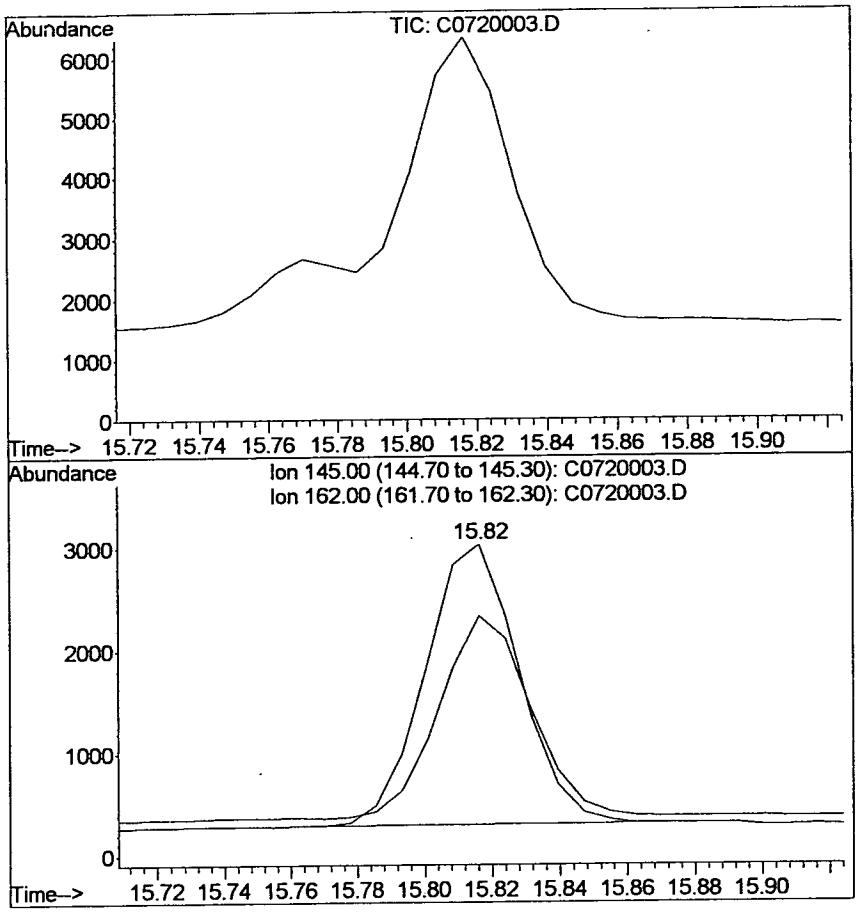

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.82 min Scan# 810
Delta R.T. 0.01 min
Lab File: C0720003.D
Acq: 20 Jul 2007 5:40 pm

Tgt Ion:145 Resp: 5248

Ion	Ratio	Lower	Upper
145	100		
162	70.2	22.4	102.4

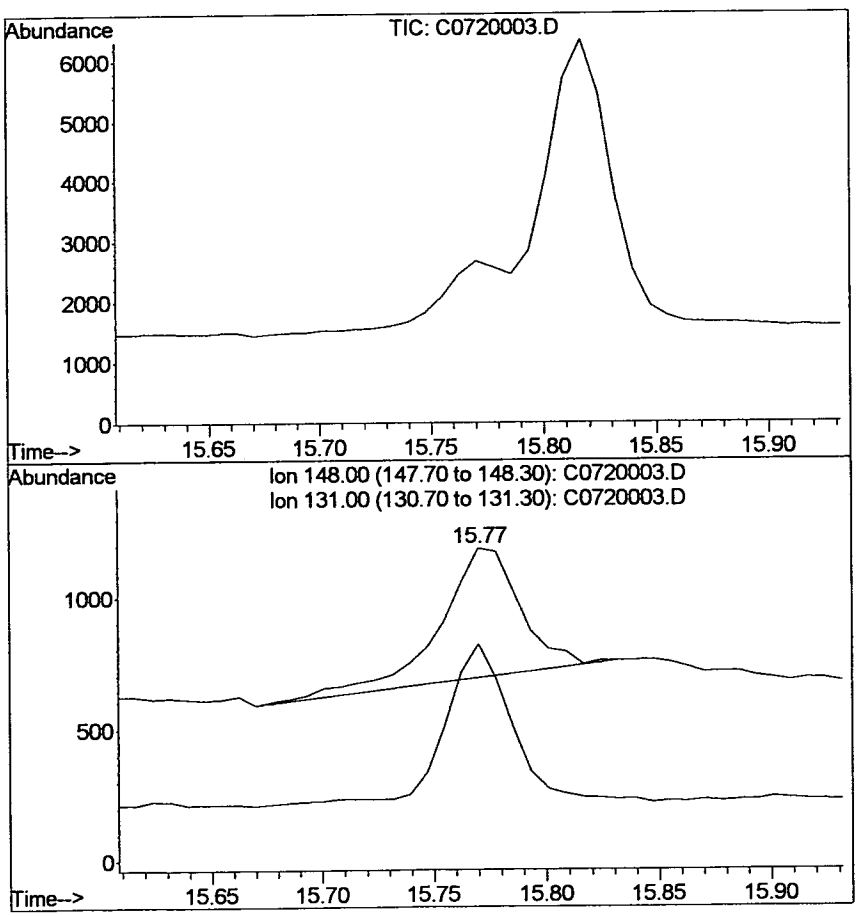

#6
NDPA
Concen: 2.97 PPB
RT: 15.77 min Scan# 804
Delta R.T. 0.00 min
Lab File: C0720003.D
Acq: 20 Jul 2007 5:40 pm

Tgt Ion:148 Resp: 1253

Ion	Ratio	Lower	Upper
148	100		
131	89.8	99.8	207.2#

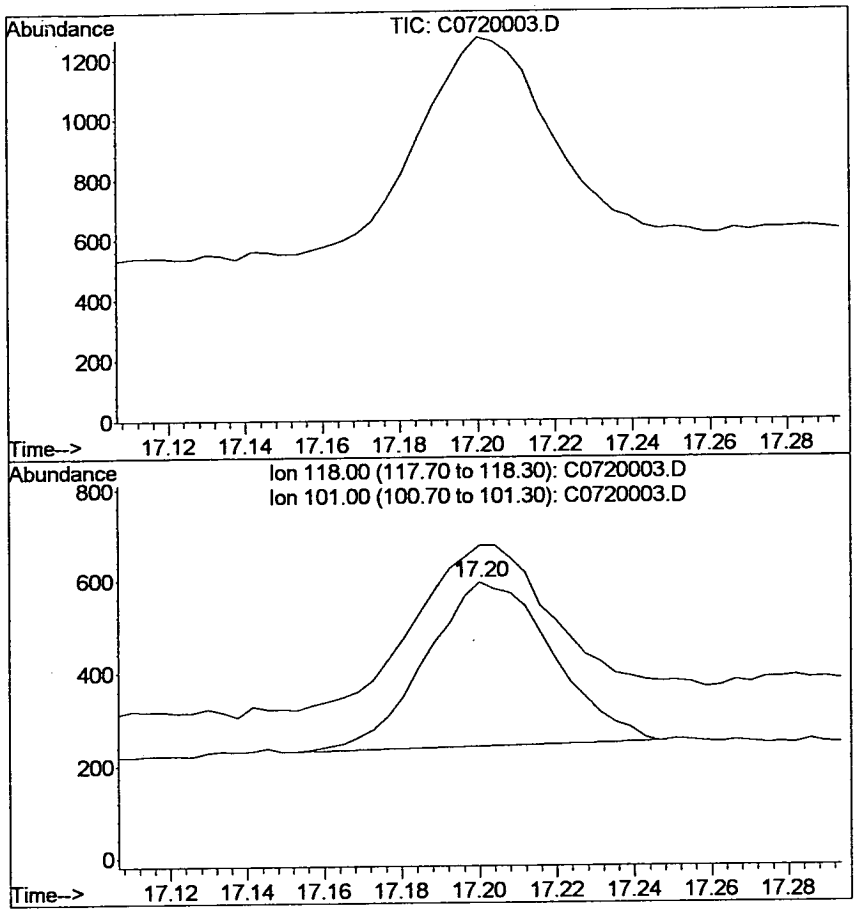

#7
NPYR
Concen: 1.89 PPB
RT: 17.20 min Scan# 1077
Delta R.T. 0.00 min
Lab File: C0720003.D
Acq: 20 Jul 2007 5:40 pm

Tgt Ion:118 Resp: 795

Ion	Ratio	Lower	Upper
118	100		
101	101.5	62.6	130.0

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720004.D
Acq On : 20 Jul 2007 6:04 pm
Sample : 7G19061-BSD1
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 20 18:31 2007

Vial: 5
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00

Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration
DataAcq Meth : C7F14NW

LB

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) NDMA-D6	10.91	81	2448	10.00	PPB	0.00
3) NDEA-D10	13.39	113	5249	10.00	PPB	0.02
5) NDPA-D14	15.82	145	5480	10.00	PPB	0.00

Target Compounds						Qvalue
2) NDMA	10.85	92	4706	9.60	PPB	96
4) NDEA	13.33	120	5116	9.09	PPB	97
6) NDPA	15.77	148	3889	8.83	PPB	88
7) NPYR	17.20	118	4203	9.58	PPB	100

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720004.D
Acq On : 20 Jul 2007 6:04 pm
Sample : 7G19061-BSD1
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 20 18:31 2007

Vial: 5
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration

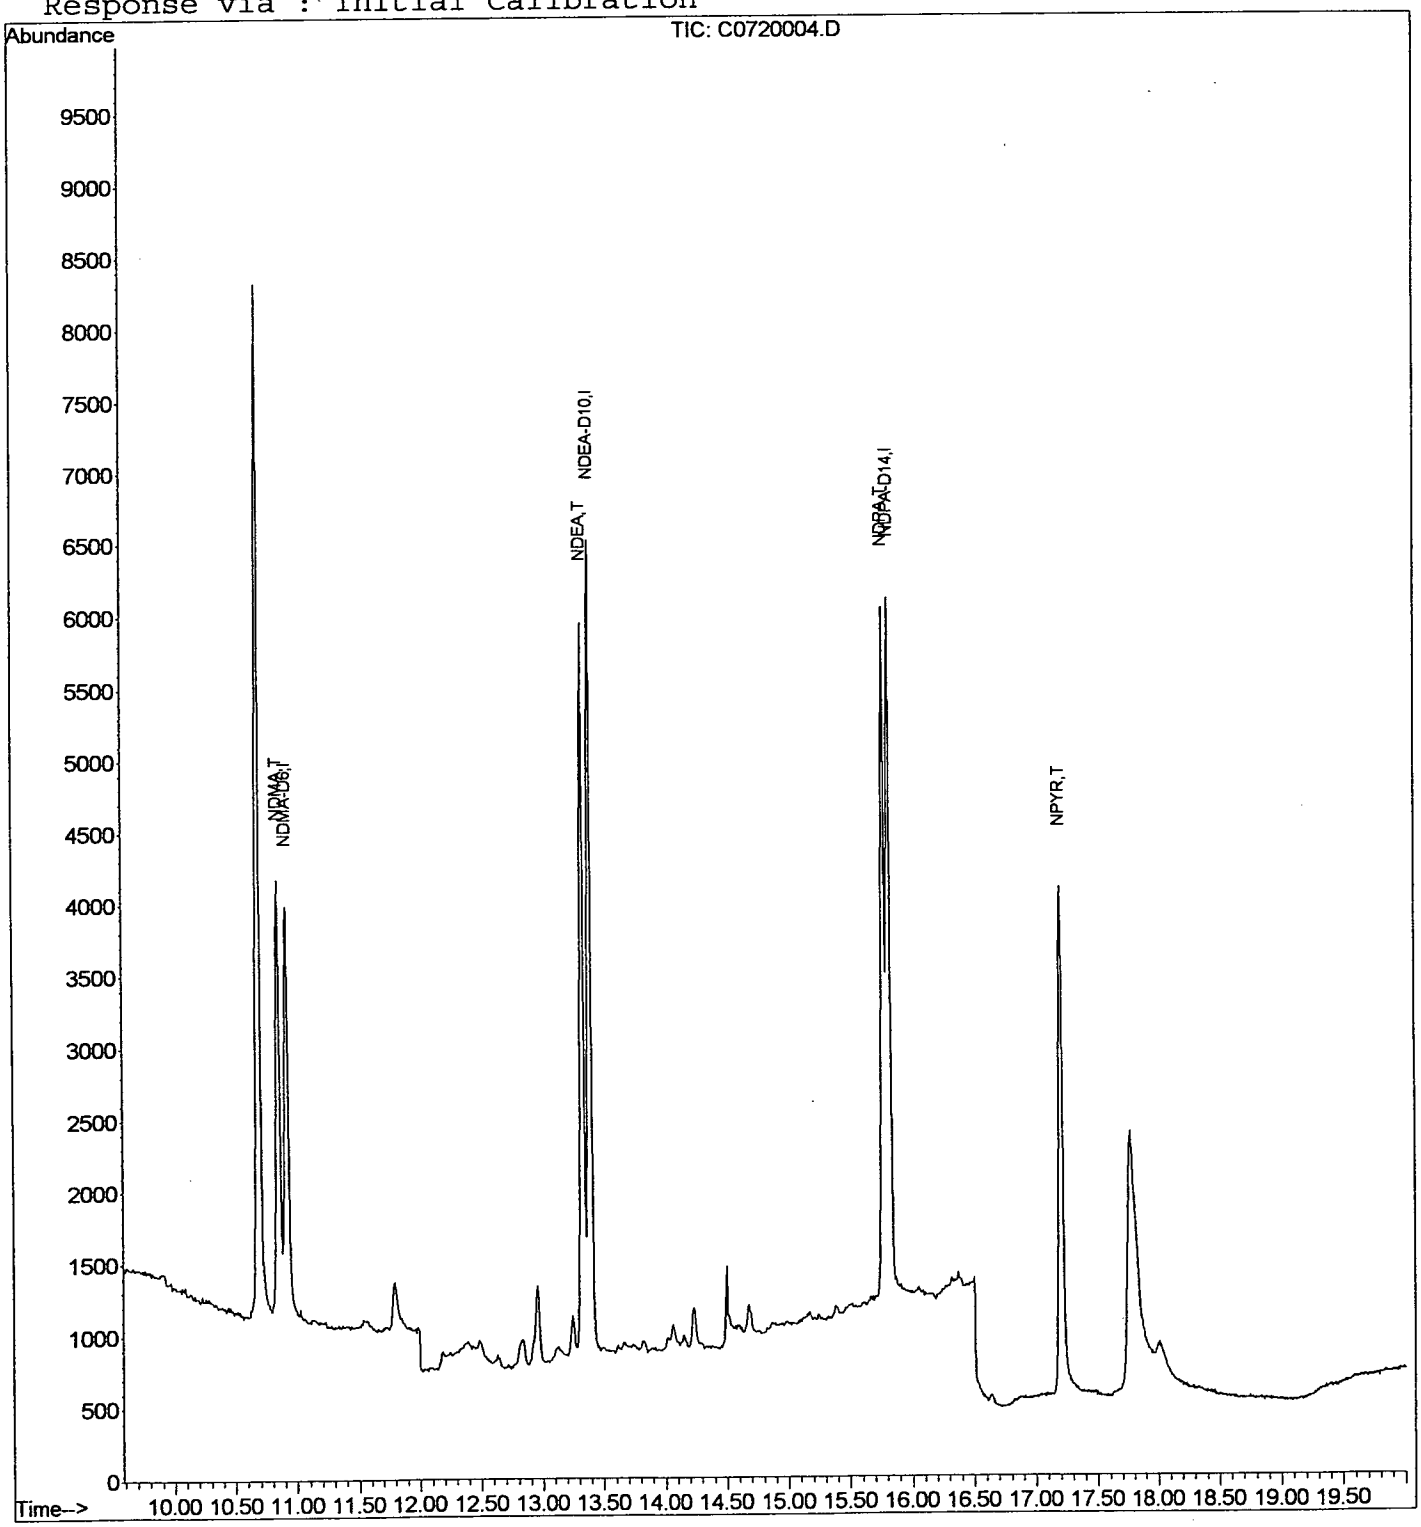

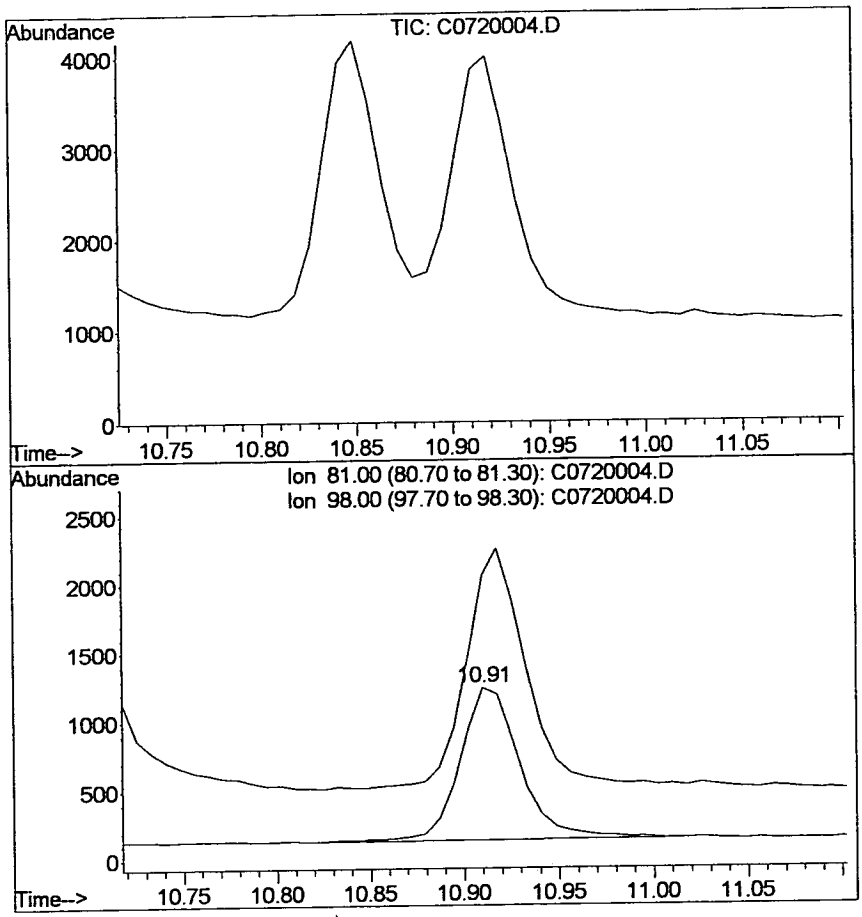

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.91 min Scan# 173
Delta R.T. 0.01 min
Lab File: C0720004.D
Acq: 20 Jul 2007 6:04 pm

Tgt Ion: 81 Resp: 2448

Ion	Ratio	Lower	Upper
81	100		
98	153.1	144.1	224.1

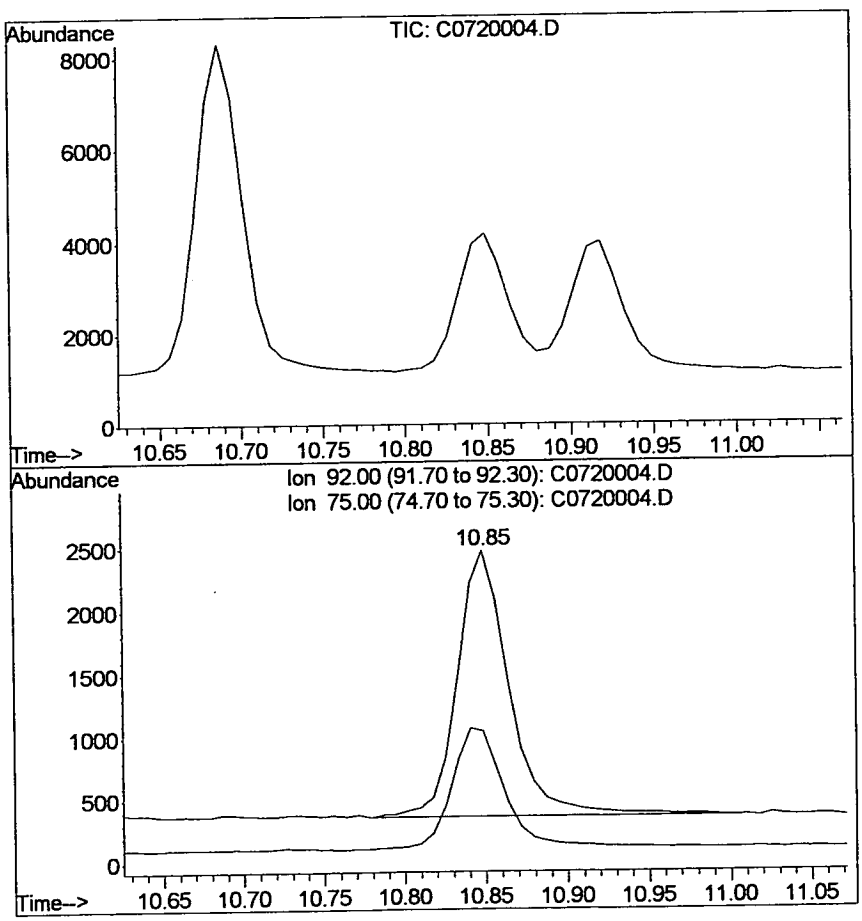

#2
NDMA
Concen: 9.60 PPB
RT: 10.85 min Scan# 165
Delta R.T. 0.02 min
Lab File: C0720004.D
Acq: 20 Jul 2007 6:04 pm

Tgt Ion: 92 Resp: 4706

Ion	Ratio	Lower	Upper
92	100		
75	46.4	31.8	66.0

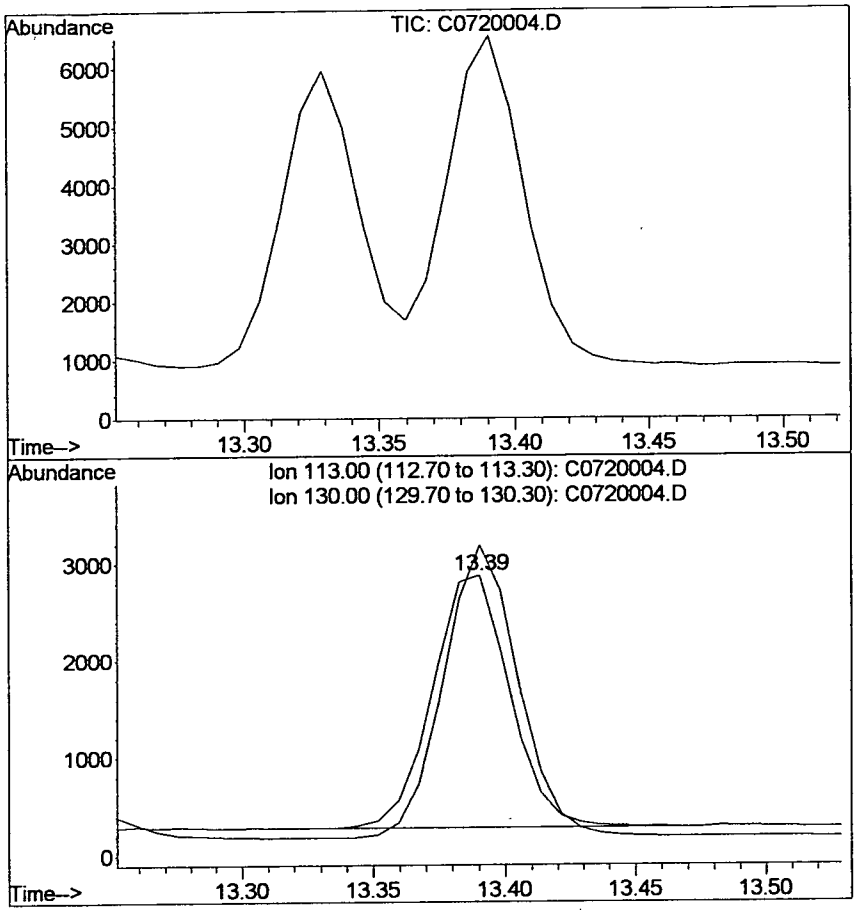

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.39 min Scan# 495
Delta R.T. 0.02 min
Lab File: C0720004.D
Acq: 20 Jul 2007 6:04 pm

Tgt Ion:113 Resp: 5249

Ion	Ratio	Lower	Upper
113	100		
130	111.2	67.1	137.1

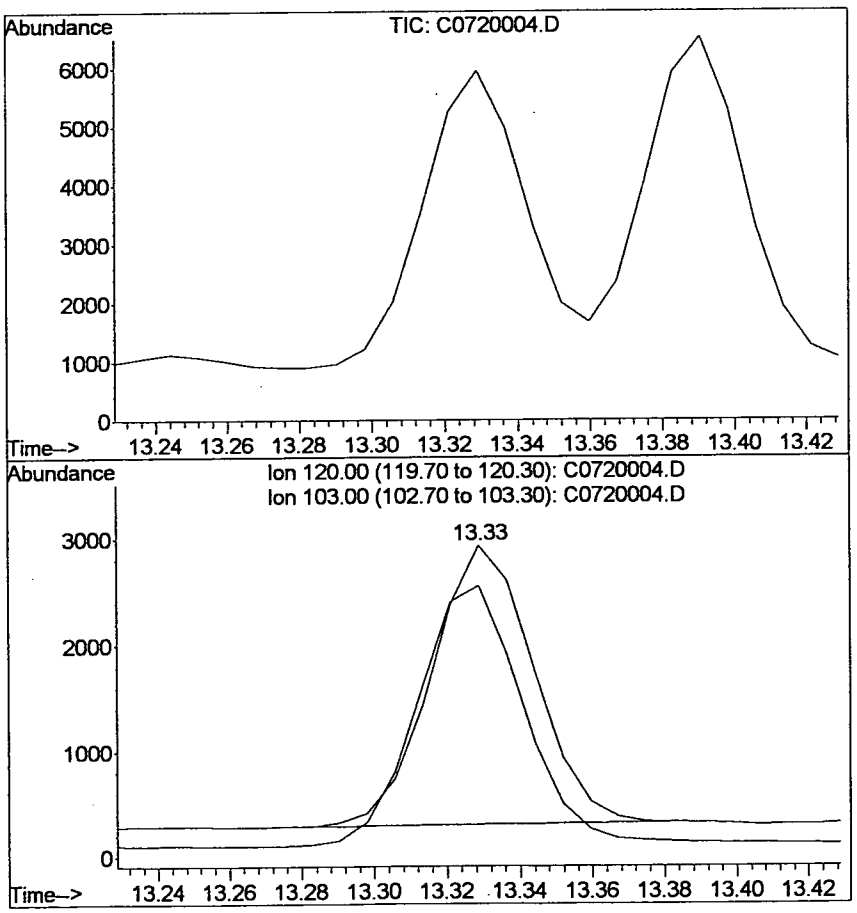

#4
NDEA
Concen: 9.09 PPB
RT: 13.33 min Scan# 487
Delta R.T. 0.01 min
Lab File: C0720004.D
Acq: 20 Jul 2007 6:04 pm

Tgt Ion:120 Resp: 5116

Ion	Ratio	Lower	Upper
120	100		
103	97.2	65.3	135.5

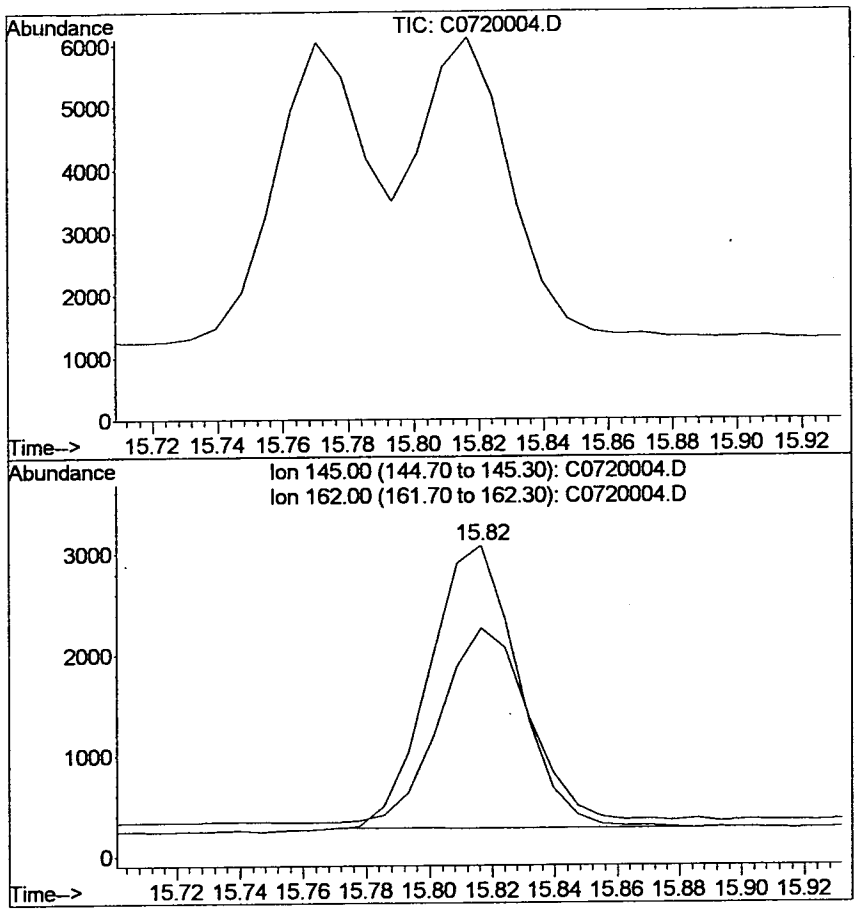

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.82 min Scan# 810
Delta R.T. 0.01 min
Lab File: C0720004.D
Acq: 20 Jul 2007 6:04 pm

Tgt Ion:145 Resp: 5480

Ion	Ratio	Lower	Upper
145	100		
162	67.7	22.4	102.4

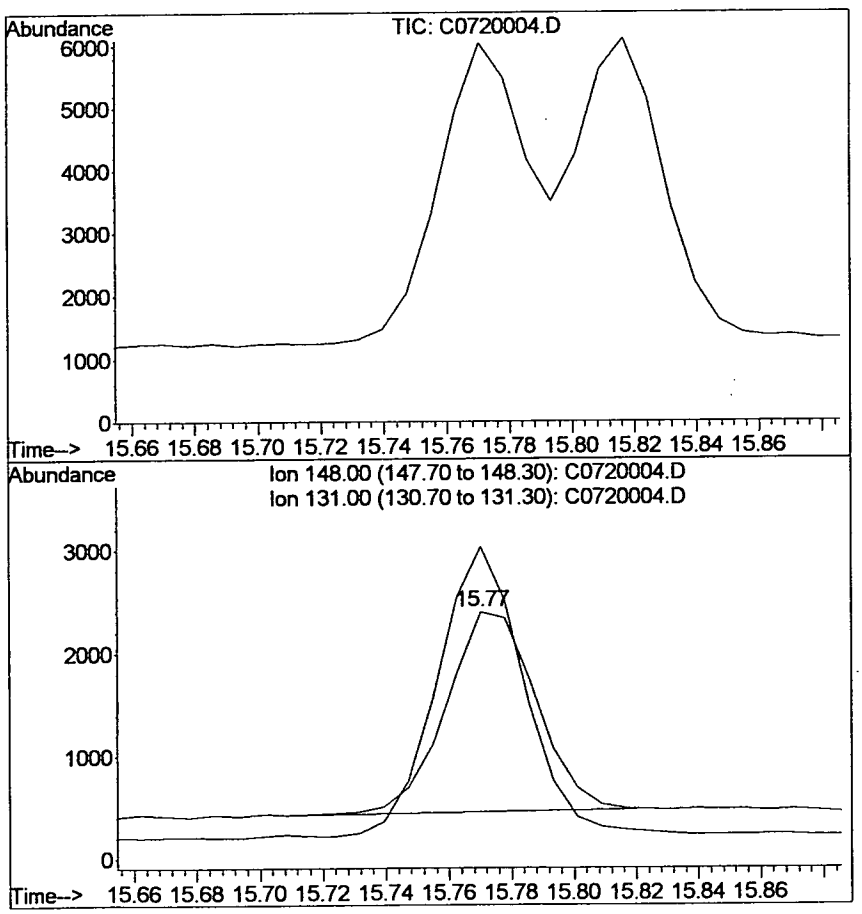

#6
NDPA
Concen: 8.83 PPB
RT: 15.77 min Scan# 804
Delta R.T. 0.00 min
Lab File: C0720004.D
Acq: 20 Jul 2007 6:04 pm

Tgt Ion:148 Resp: 3889

Ion	Ratio	Lower	Upper
148	100		
131	138.1	99.8	207.2

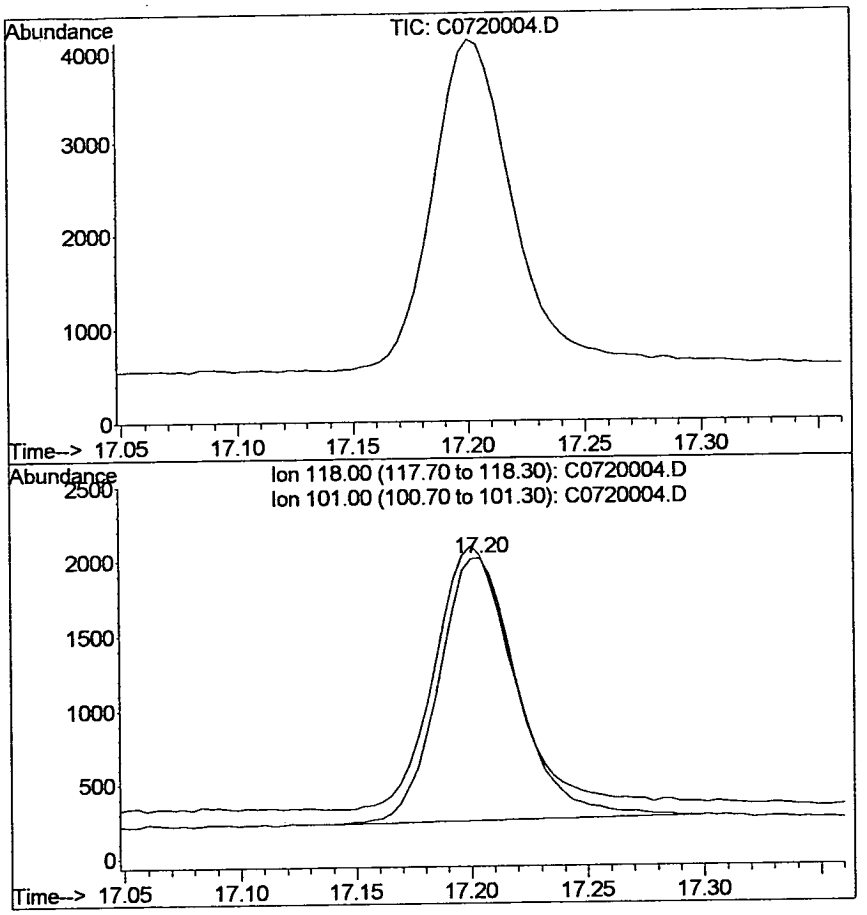

#7
NPYR
Concen: 9.58 PPB
RT: 17.20 min Scan# 1078
Delta R.T. 0.01 min
Lab File: C0720004.D
Acq: 20 Jul 2007 6:04 pm

Tgt Ion:118 Resp: 4203

Ion	Ratio	Lower	Upper
118	100		
101	96.6	62.6	130.0

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720009.D
Acq On : 20 Jul 2007 8:01 pm
Sample : IQG1460-01
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 21 6:34 2007

Vial: 10
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration
DataAcq Meth : C7F14NW

LB

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) NDMA-D6	10.91	81	1728	10.00 PPB	0.00
3) NDEA-D10	13.38	113	4066	10.00 PPB	0.00
5) NDPA-D14	15.82	145	4559	10.00 PPB	0.00
Target Compounds					**Qvalue**
2) NDMA	10.85	92	81	0.23 PPB	88
4) NDEA	13.33	120	111	0.25 PPB	72
6) NDPA	15.58	148	26	0.07 PPB	91
7) NPYR	17.26	118	10	0.03 PPB	94

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720009.D
Acq On : 20 Jul 2007 8:01 pm
Sample : IQG1460-01
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 21 6:34 2007

Vial: 10
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration

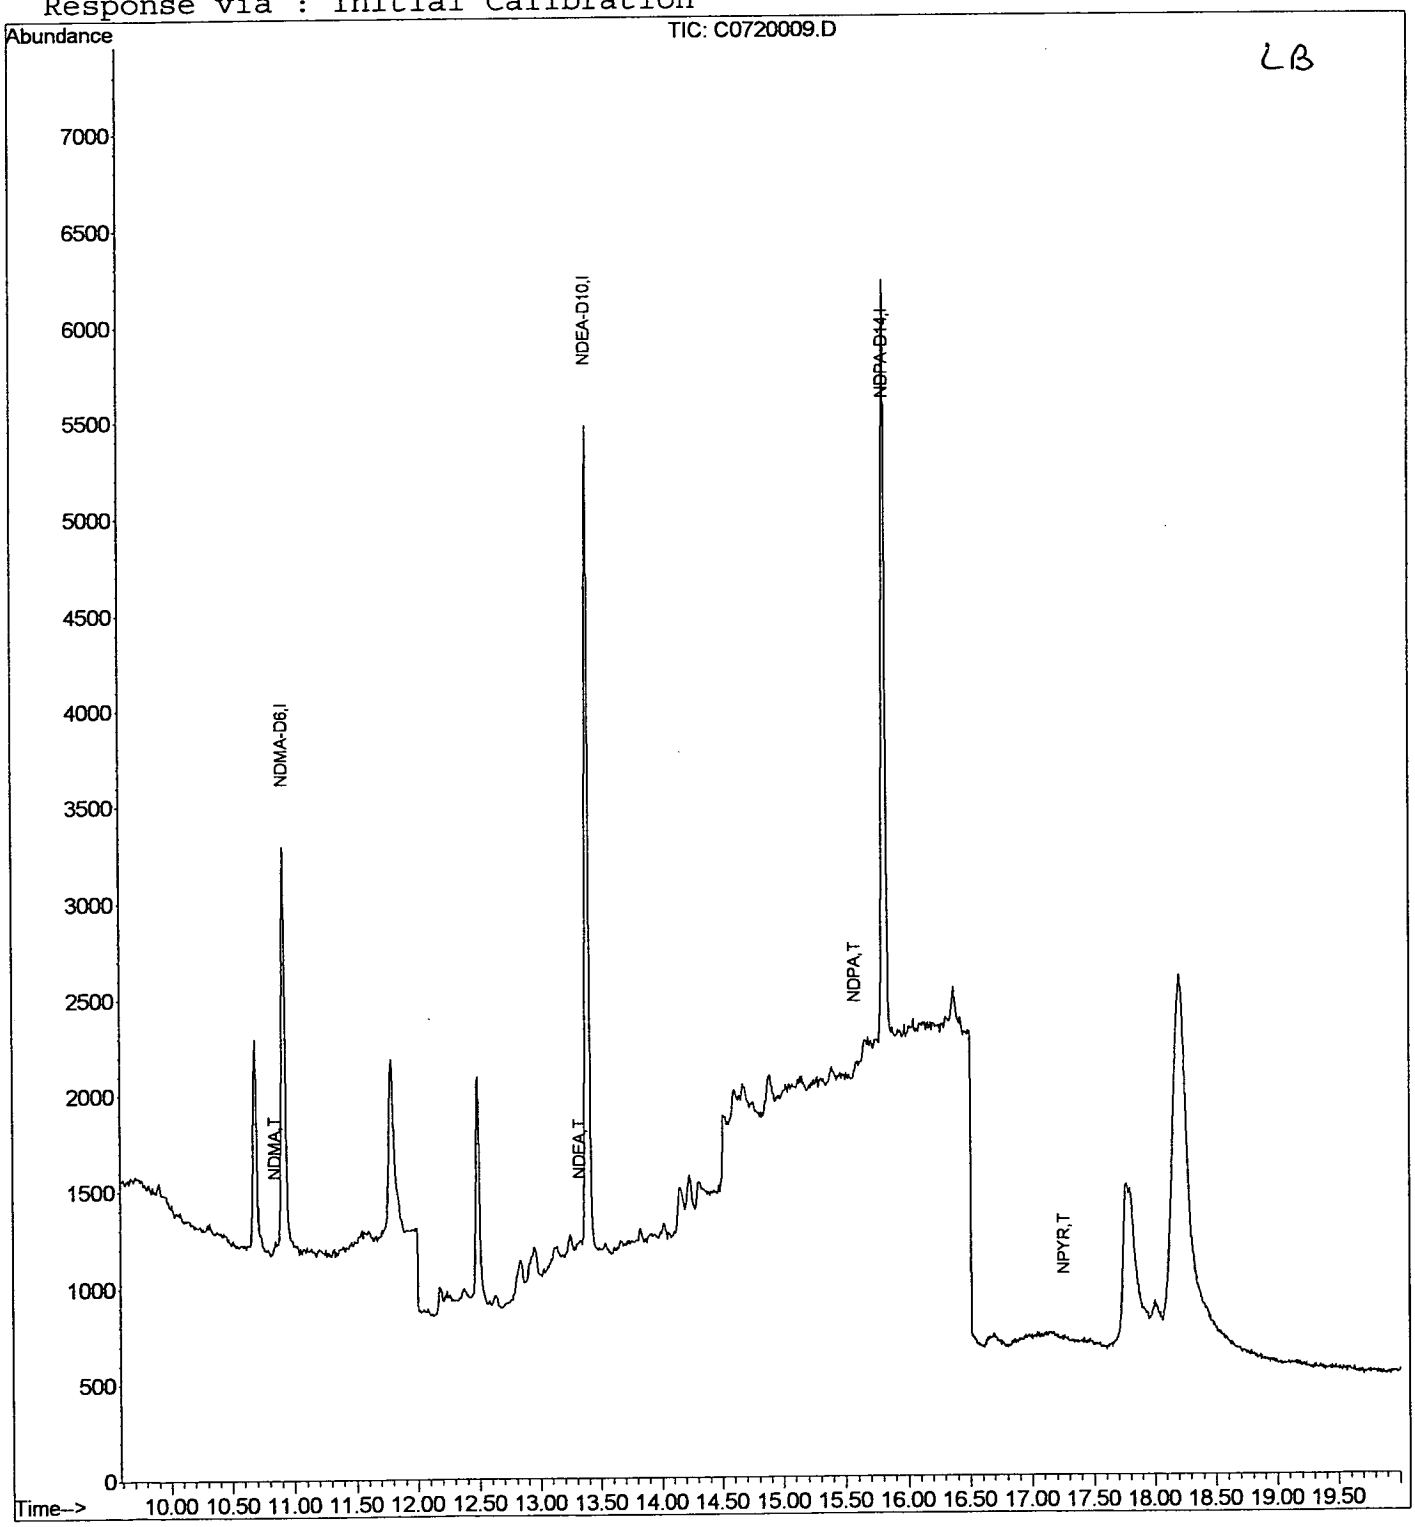

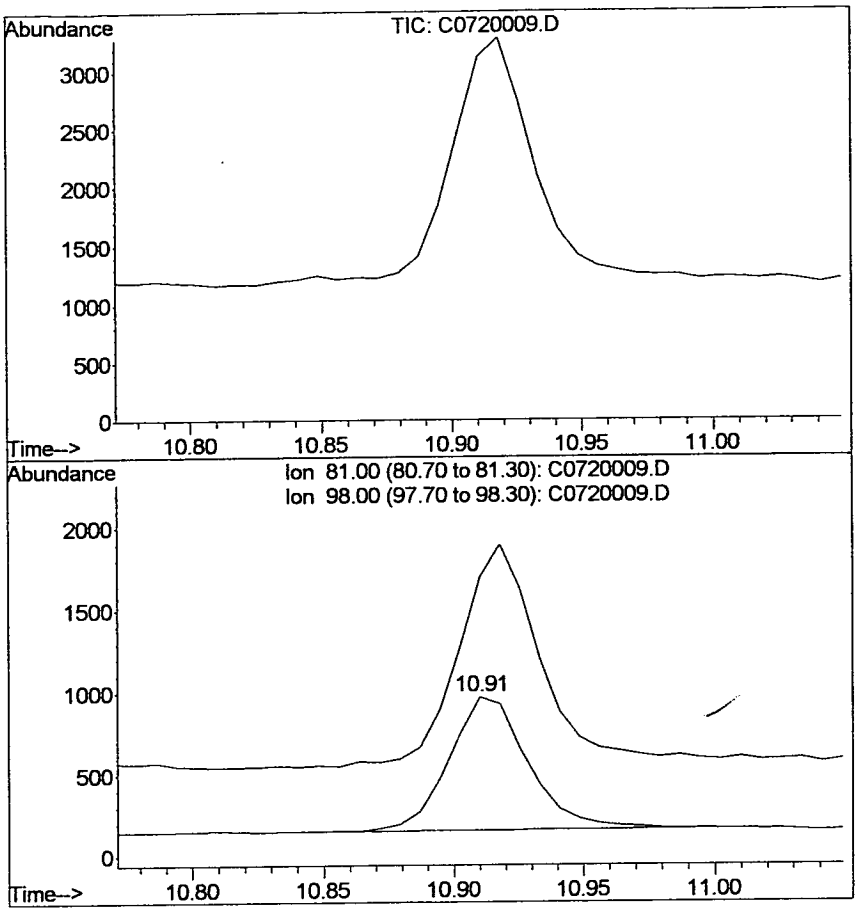

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.91 min Scan# 173
Delta R.T. 0.01 min
Lab File: C0720009.D
Acq: 20 Jul 2007 8:01 pm

Tgt Ion: 81 Resp: 1728

Ion	Ratio	Lower	Upper
81	100		
98	165.7	144.1	224.1

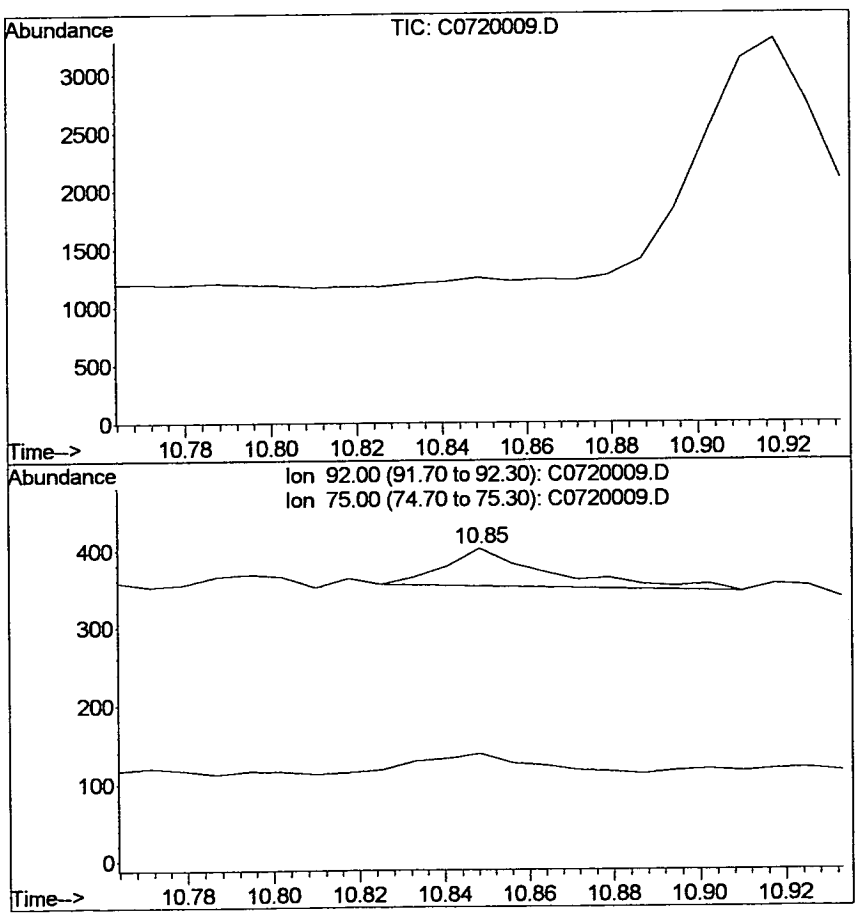

#2
NDMA
Concen: 0.23 PPB
RT: 10.85 min Scan# 165
Delta R.T. 0.02 min
Lab File: C0720009.D
Acq: 20 Jul 2007 8:01 pm

Tgt Ion: 92 Resp: 81

Ion	Ratio	Lower	Upper
92	100		
75	56.8	31.8	66.0

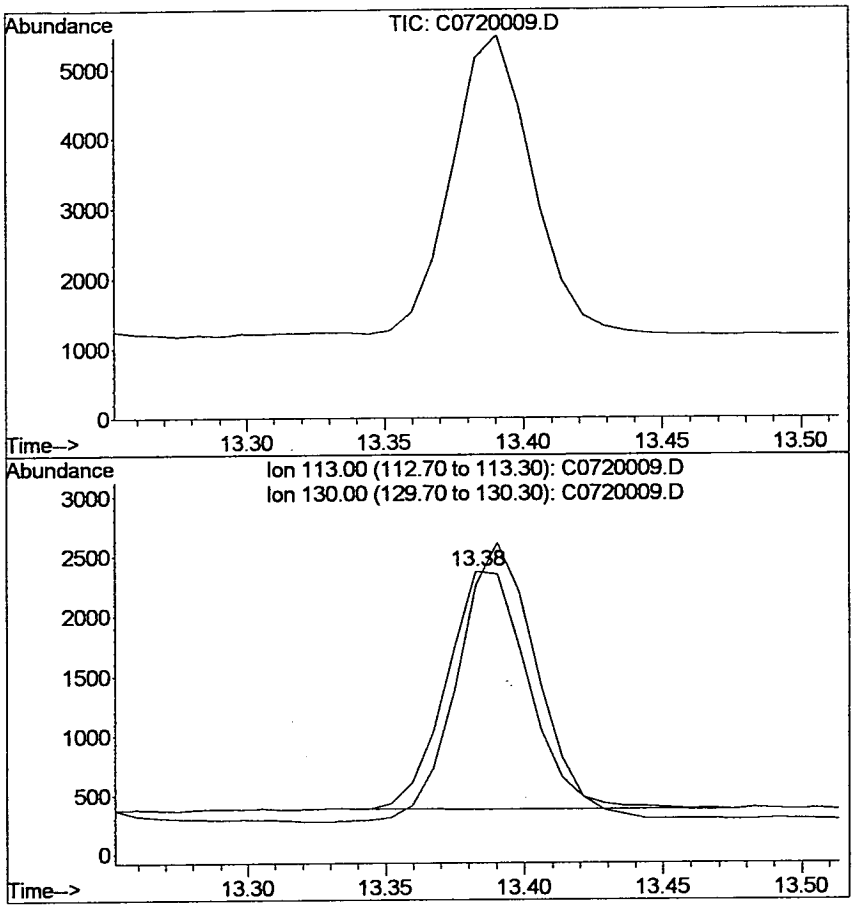

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.38 min Scan# 494
Delta R.T. 0.01 min
Lab File: C0720009.D
Acq: 20 Jul 2007 8:01 pm

Tgt Ion:113 Resp: 4066

Ion	Ratio	Lower	Upper
113	100		
130	111.5	67.1	137.1

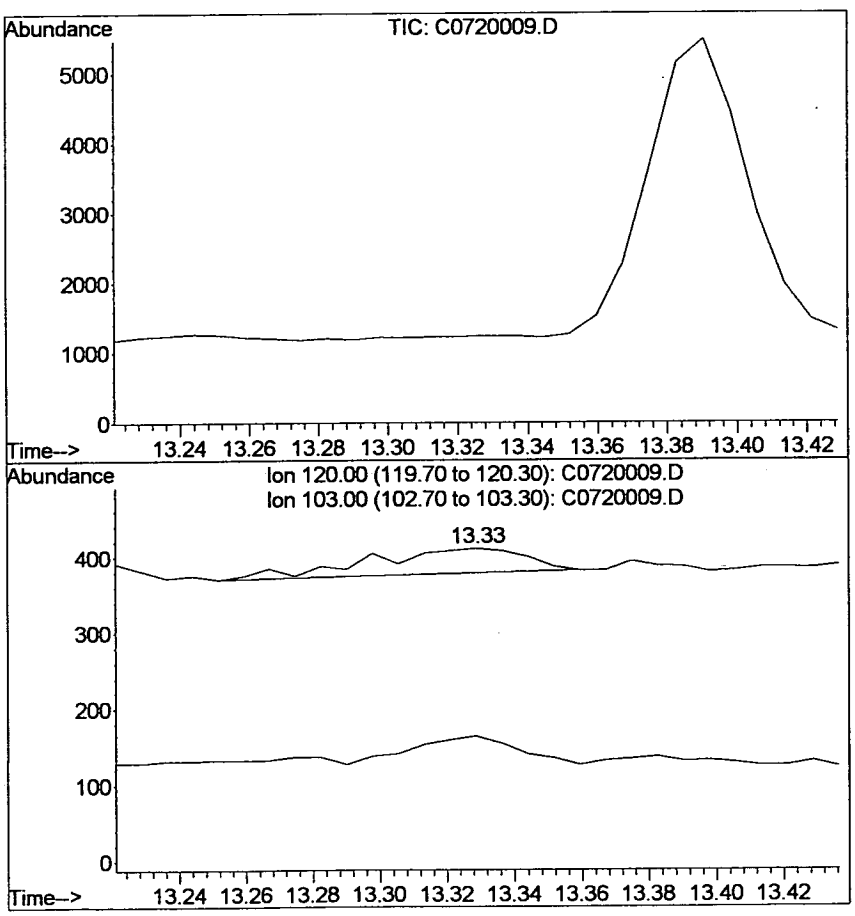

#4
NDEA
Concen: 0.25 PPB
RT: 13.33 min Scan# 487
Delta R.T. 0.01 min
Lab File: C0720009.D
Acq: 20 Jul 2007 8:01 pm

Tgt Ion:120 Resp: 111

Ion	Ratio	Lower	Upper
120	100		
103	72.1	65.3	135.5

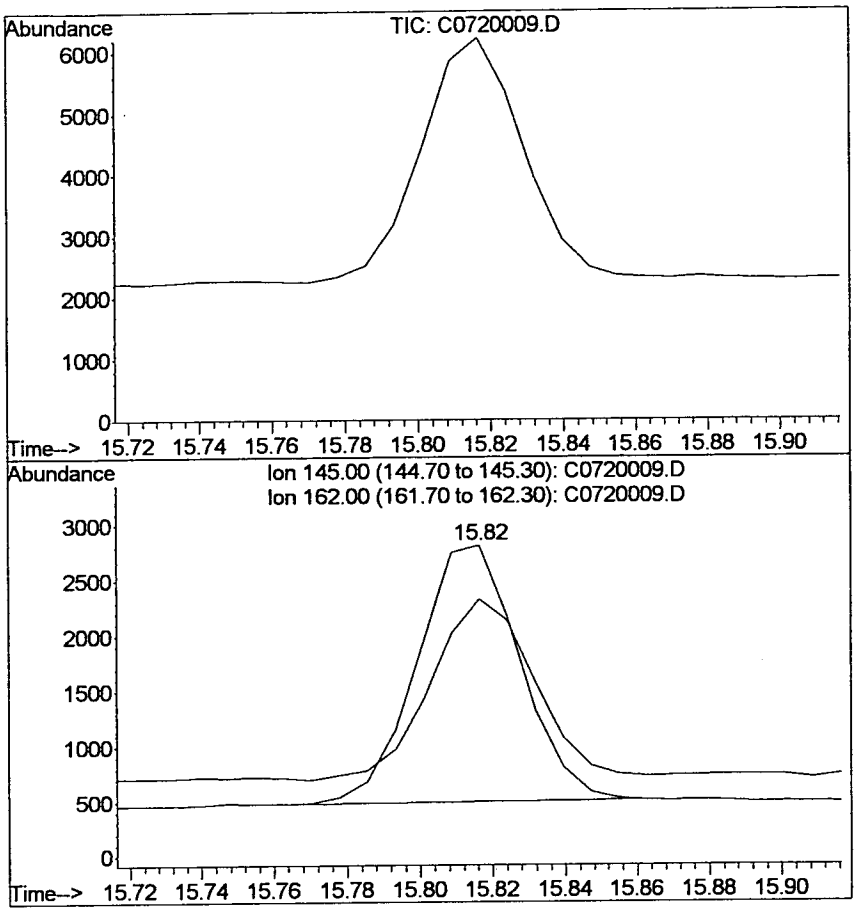

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.82 min Scan# 810
Delta R.T. 0.01 min
Lab File: C0720009.D
Acq: 20 Jul 2007 8:01 pm

Tgt Ion:145 Resp: 4559

Ion	Ratio	Lower	Upper
145	100		
162	68.6	22.4	102.4

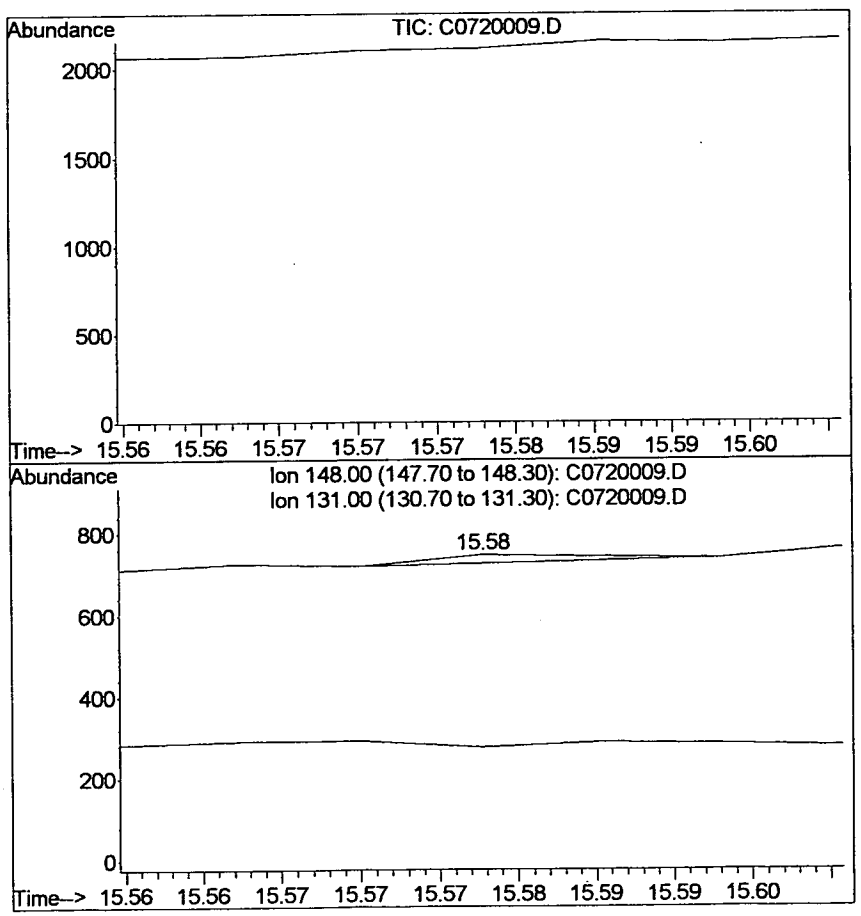

#6
NDPA
Concen: 0.07 PPB
RT: 15.58 min Scan# 779
Delta R.T. -0.19 min
Lab File: C0720009.D
Acq: 20 Jul 2007 8:01 pm

Tgt Ion:148 Resp: 26

Ion	Ratio	Lower	Upper
148	100		
131	142.3	99.8	207.2

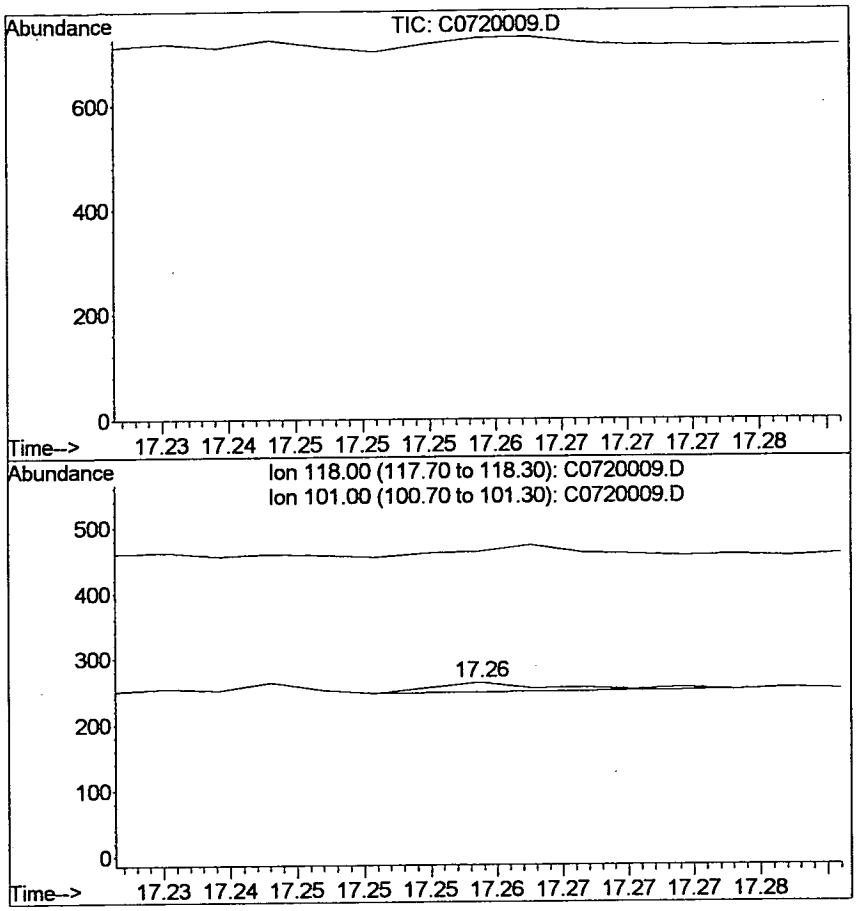

#7
NPYR
Concen: 0.03 PPB
RT: 17.26 min Scan# 1092
Delta R.T. 0.06 min
Lab File: C0720009.D
Acq: 20 Jul 2007 8:01 pm

Tgt Ion:118 Resp: 10

Ion	Ratio	Lower	Upper
118	100		
101	90.0	62.6	130.0

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720010.D
Acq On : 20 Jul 2007 8:24 pm
Sample : IQG1460-02
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 21 6:34 2007

Vial: 11
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration
DataAcq Meth : C7F14NW

LB

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) NDMA-D6	10.91	81	1906	10.00 PPB	0.00
3) NDEA-D10	13.39	113	3994	10.00 PPB	0.02
5) NDPA-D14	15.82	145	4115	10.00 PPB	0.00
Target Compounds					**Qvalue**
2) NDMA	10.86	92	120	0.31 PPB	95
4) NDEA	13.33	120	95	0.22 PPB	69
6) NDPA	15.49	148	15	0.05 PPB	100
7) NPYR	17.17	118	24	0.07 PPB	87

(#) = qualifier out of range (m) = manual integration
C0720010.D C7F14NW.M Sat Jul 21 06:34:44 2007

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720010.D
Acq On : 20 Jul 2007 8:24 pm
Sample : IQG1460-02
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 21 6:34 2007

Vial: 11
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration

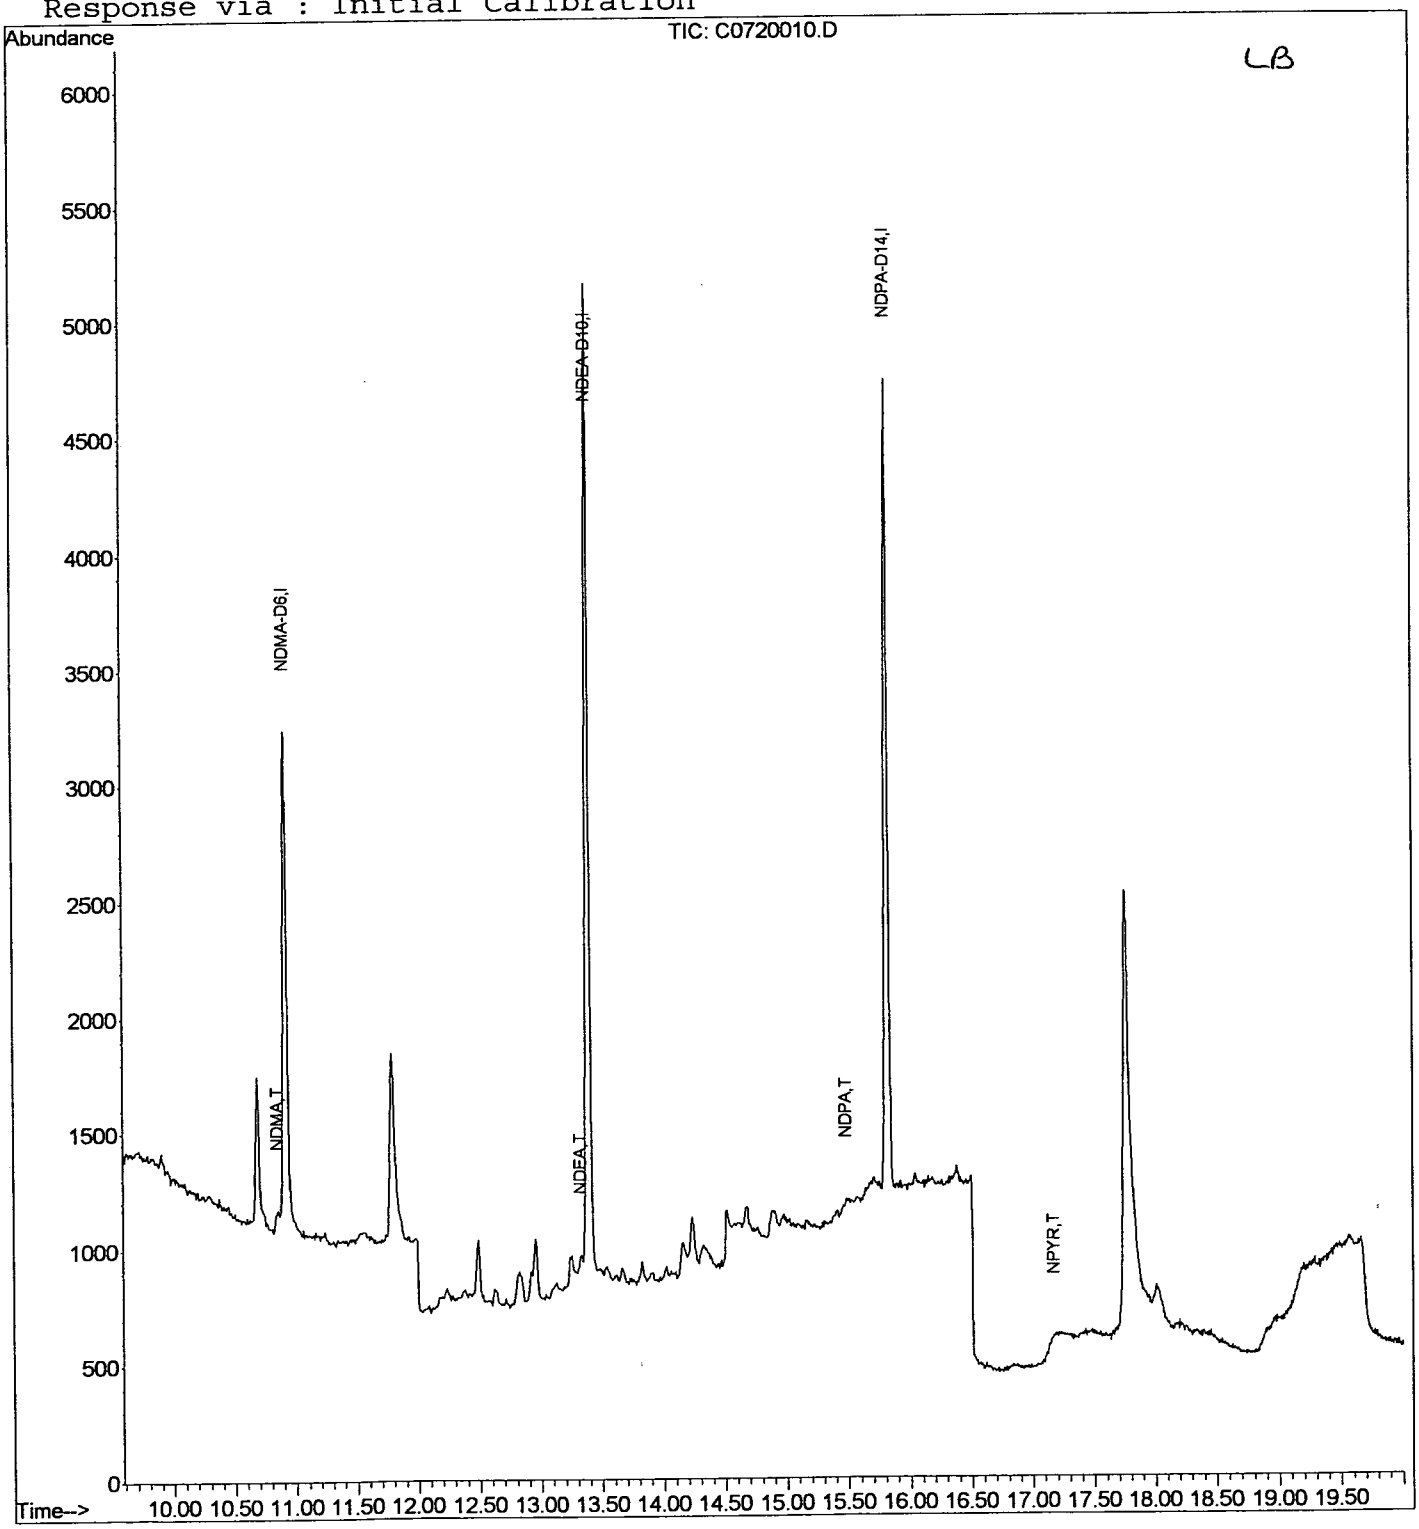

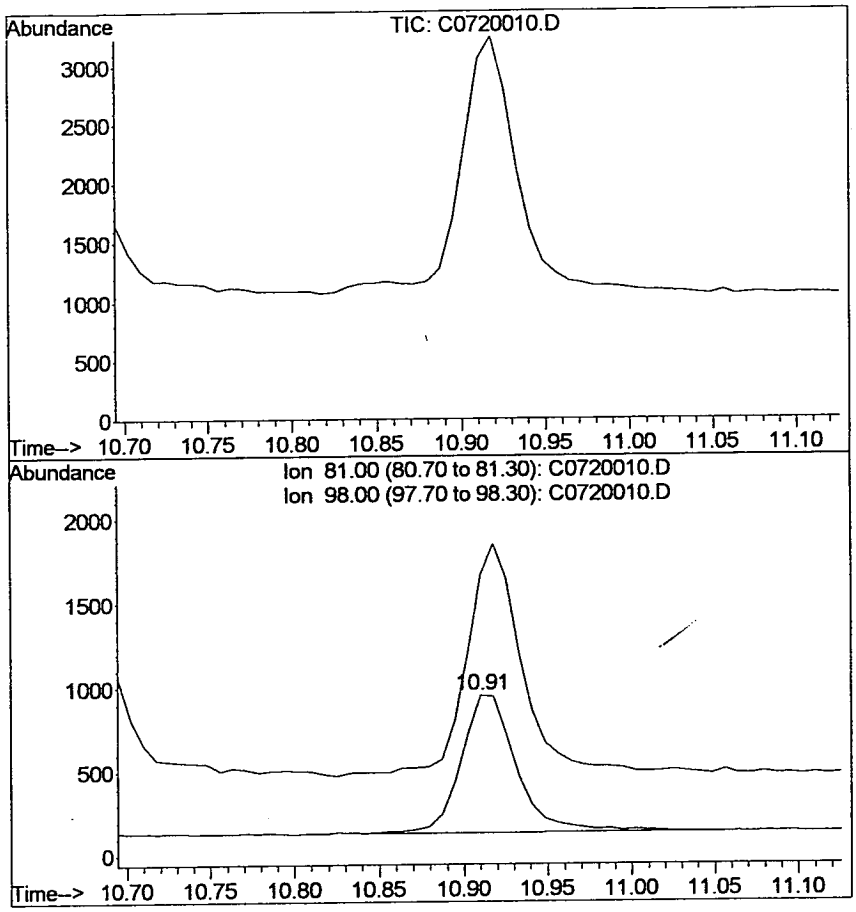

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.91 min Scan# 173
Delta R.T. 0.01 min
Lab File: C0720010.D
Acq: 20 Jul 2007 8:24 pm

Tgt Ion: 81 Resp: 1906

Ion	Ratio	Lower	Upper
81	100		
98	147.5	144.1	224.1

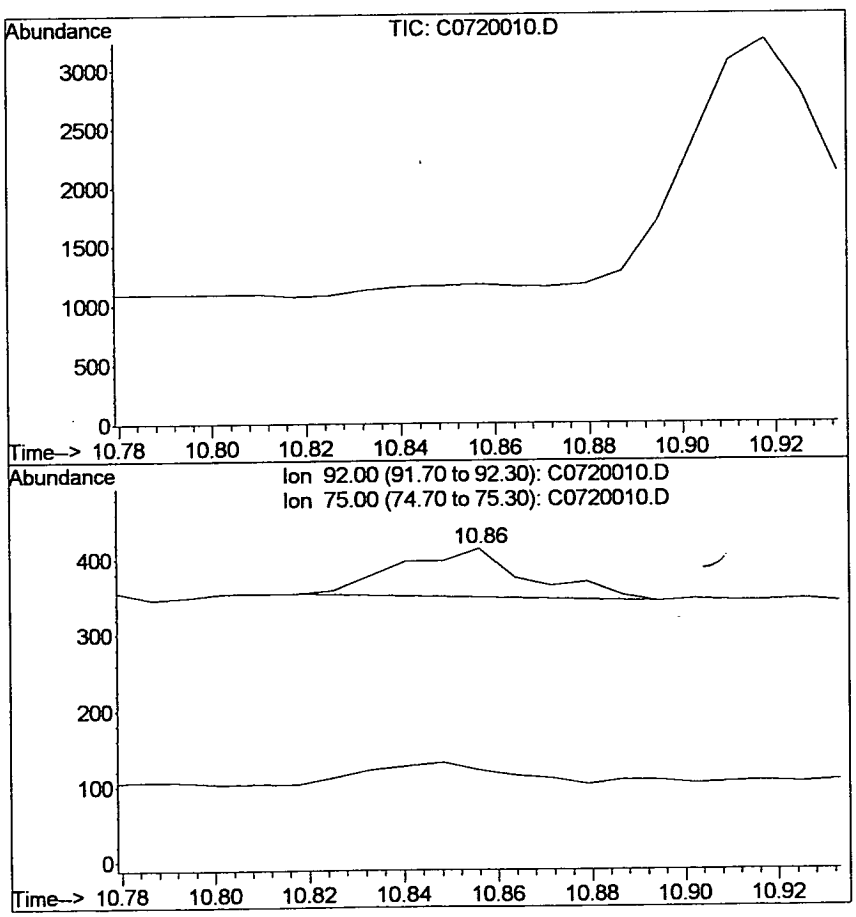

#2
NDMA
Concen: 0.31 PPB
RT: 10.86 min Scan# 166
Delta R.T. 0.02 min
Lab File: C0720010.D
Acq: 20 Jul 2007 8:24 pm

Tgt Ion: 92 Resp: 120

Ion	Ratio	Lower	Upper
92	100		
75	45.8	31.8	66.0

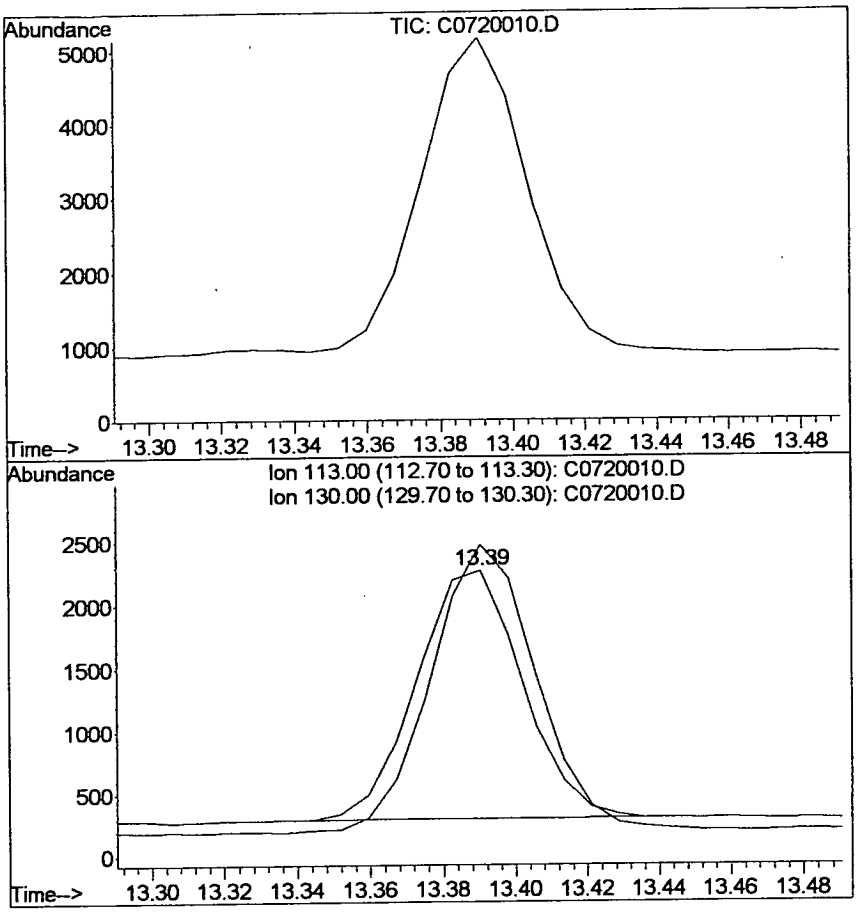

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.39 min Scan# 495
Delta R.T. 0.02 min
Lab File: C0720010.D
Acq: 20 Jul 2007 8:24 pm

Tgt Ion:113 Resp: 3994

Ion	Ratio	Lower	Upper
113	100		
130	113.5	67.1	137.1

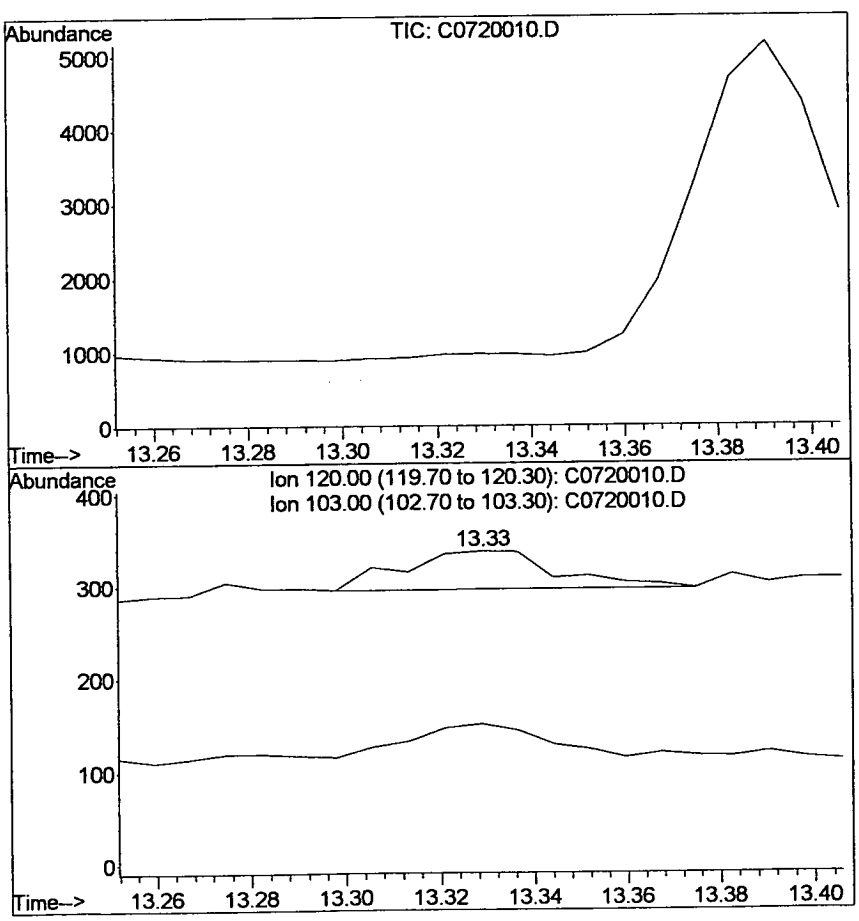

#4
NDEA
Concen: 0.22 PPB
RT: 13.33 min Scan# 487
Delta R.T. 0.01 min
Lab File: C0720010.D
Acq: 20 Jul 2007 8:24 pm

Tgt Ion:120 Resp: 95

Ion	Ratio	Lower	Upper
120	100		
103	69.5	65.3	135.5

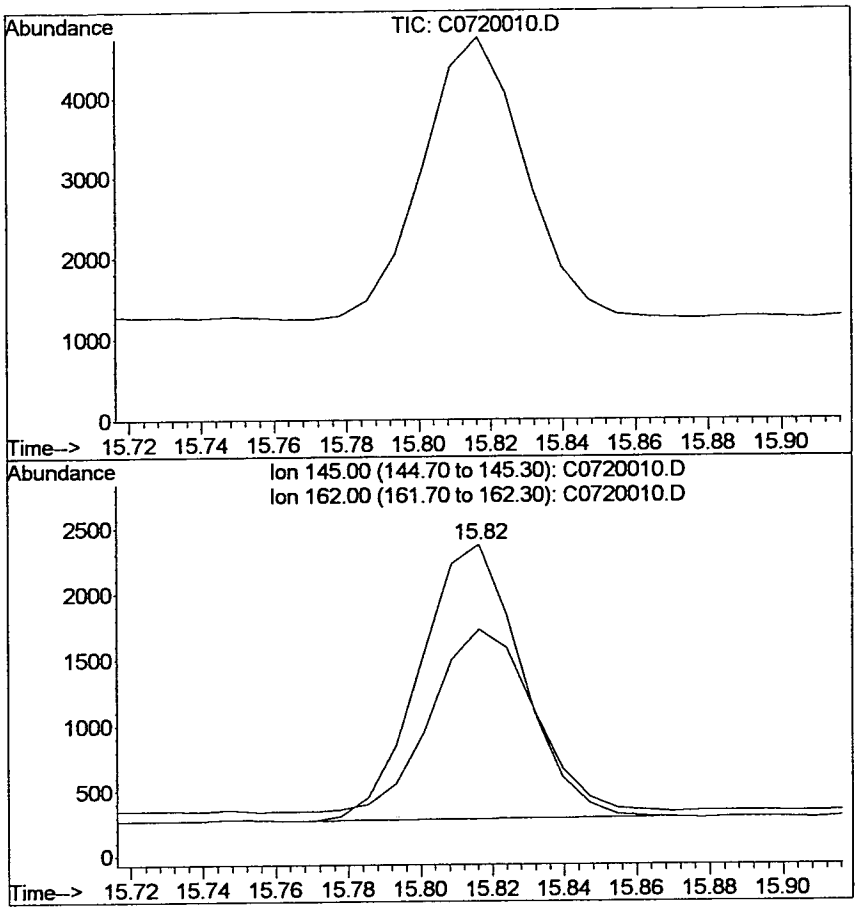

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.82 min Scan# 810
Delta R.T. 0.01 min
Lab File: C0720010.D
Acq: 20 Jul 2007 8:24 pm

Tgt Ion:145 Resp: 4115

Ion	Ratio	Lower	Upper
145	100		
162	66.7	22.4	102.4

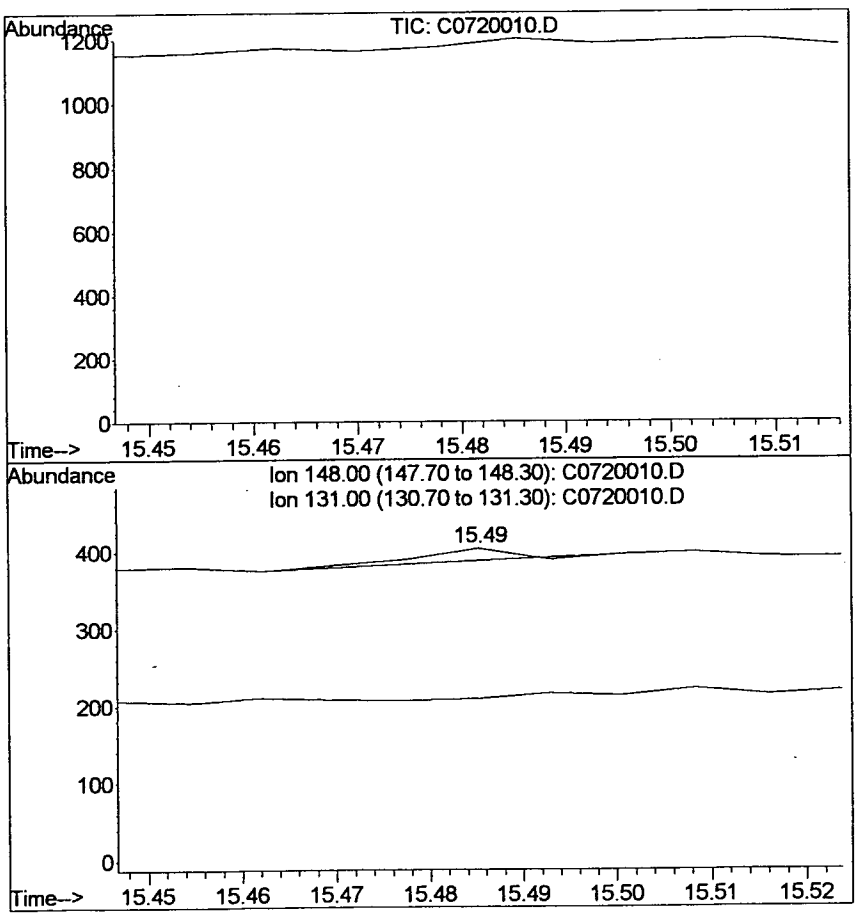

#6
NDPA
Concen: 0.05 PPB
RT: 15.49 min Scan# 767
Delta R.T. -0.28 min
Lab File: C0720010.D
Acq: 20 Jul 2007 8:24 pm

Tgt Ion:148 Resp: 15

Ion	Ratio	Lower	Upper
148	100		
131	153.3	99.8	207.2

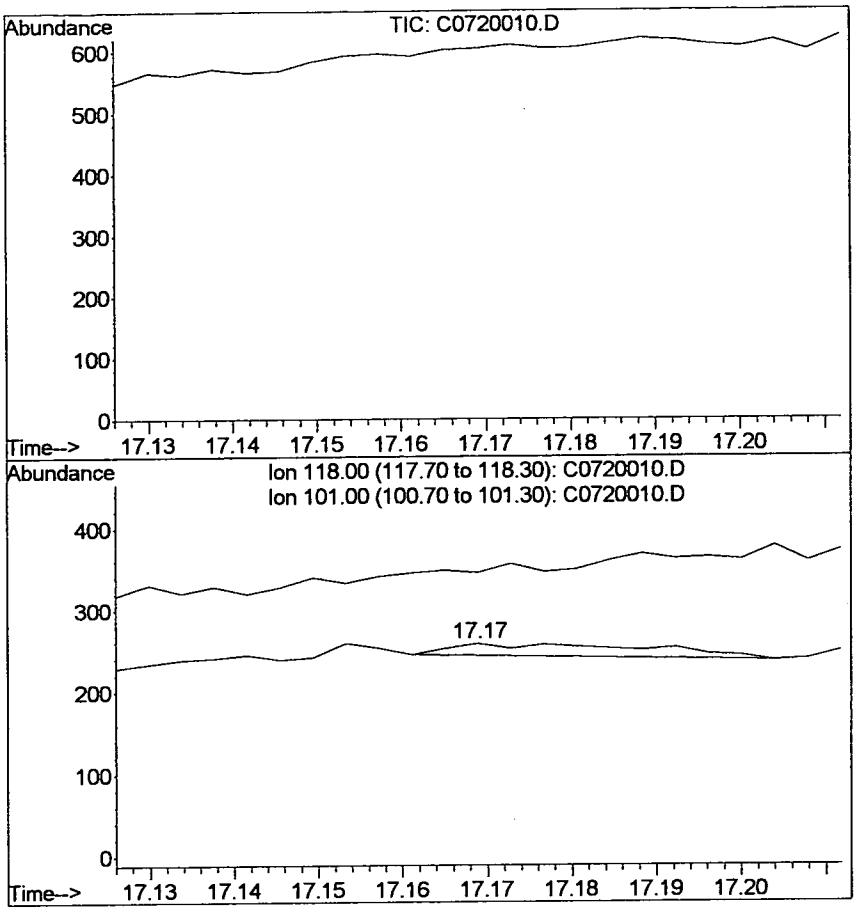

#7
NPYR
Concen: 0.07 PPB
RT: 17.17 min Scan# 1069
Delta R.T. -0.03 min
Lab File: C0720010.D
Acq: 20 Jul 2007 8:24 pm

Tgt Ion:118 Resp: 24

Ion	Ratio	Lower	Upper
118	100		
101	83.3	62.6	130.0

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720011.D
Acq On : 20 Jul 2007 8:48 pm
Sample : IQG1460-03
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 21 6:34 2007

Vial: 12
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00

Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration
DataAcq Meth : C7F14NW

LB

Internal Standards	R.T.	QIon	Response	Conc	Units		Dev(Min)
1) NDMA-D6	10.91	81	2042	10.00	PPB		0.00
3) NDEA-D10	13.38	113	4776	10.00	PPB		0.00
5) NDPA-D14	15.82	145	5087	10.00	PPB		0.00
Target Compounds							**Qvalue**
2) NDMA	10.85	92	81	0.20	PPB		88
4) NDEA	13.33	120	183	0.36	PPB		85
6) NDPA	15.75	148	73	0.18	PPB	#	37
7) NPYR	17.21	118	6	0.01	PPB	#	1

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720011.D
Acq On : 20 Jul 2007 8:48 pm
Sample : IQG1460-03
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 21 6:34 2007

Vial: 12
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration

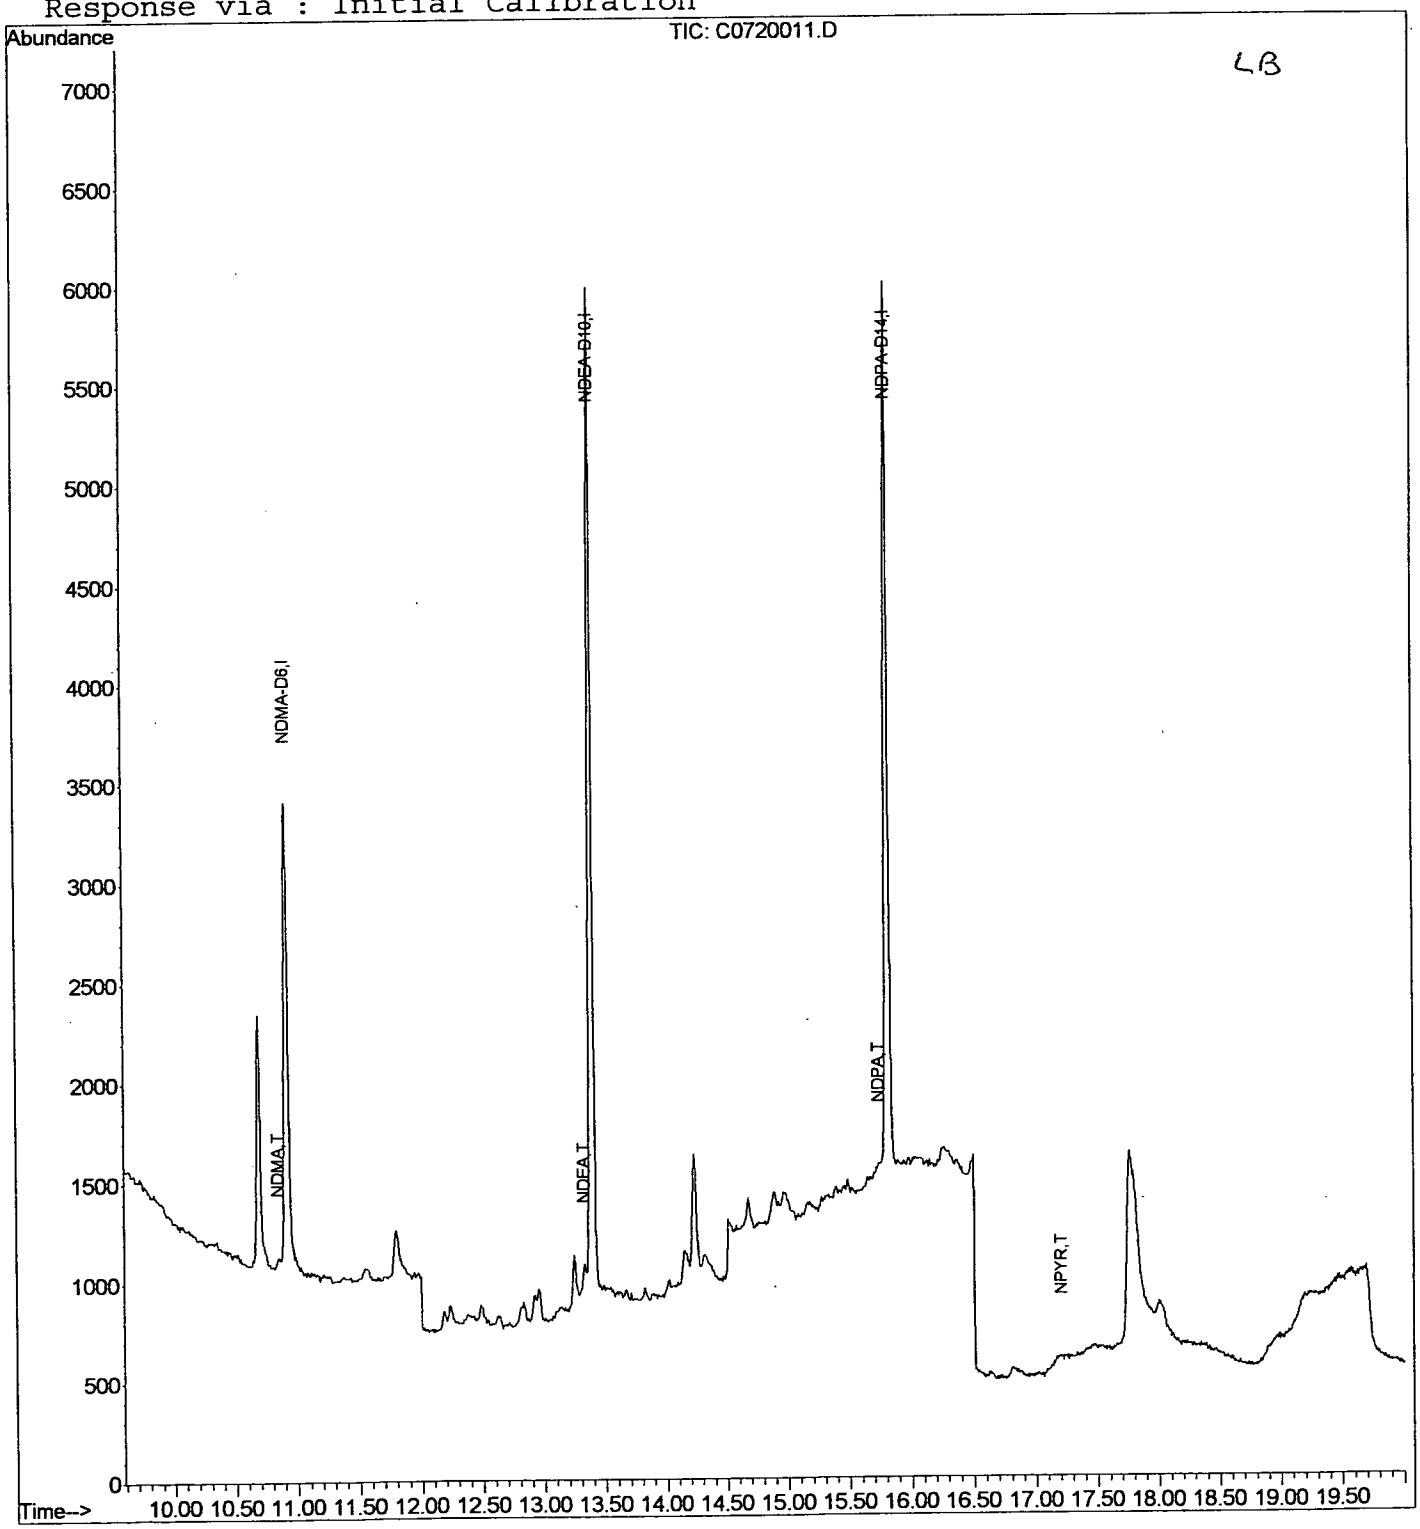

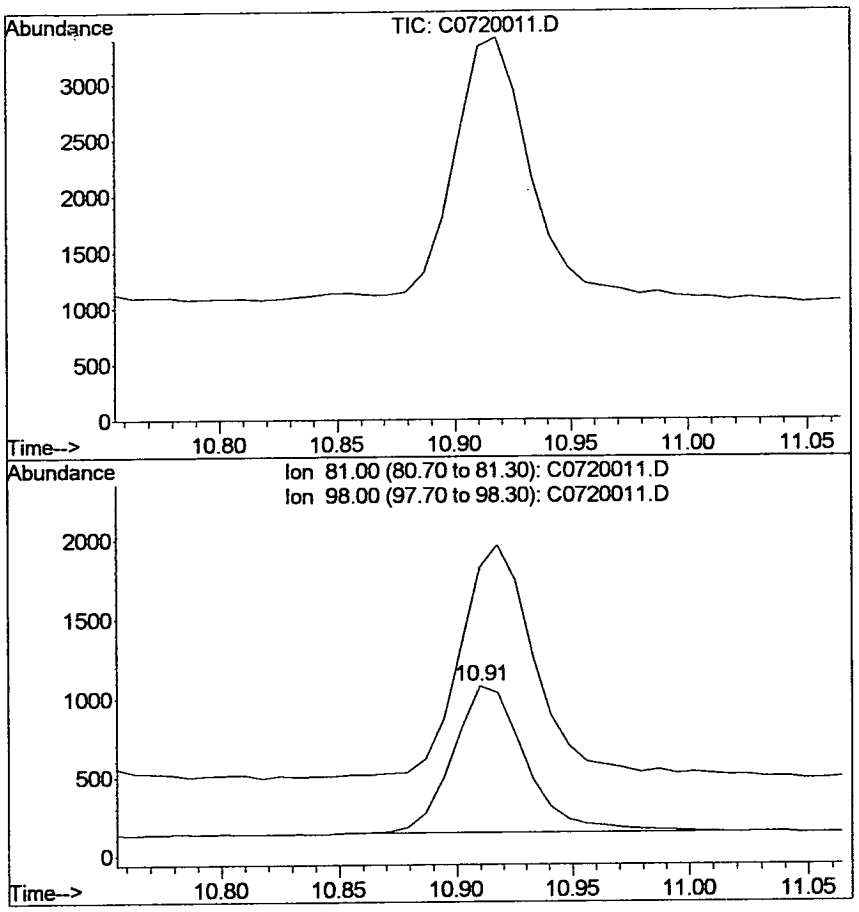

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.91 min Scan# 173
Delta R.T. 0.01 min
Lab File: C0720011.D
Acq: 20 Jul 2007 8:48 pm

Tgt Ion: 81 Resp: 2042

Ion	Ratio	Lower	Upper
81	100		
98	158.4	144.1	224.1

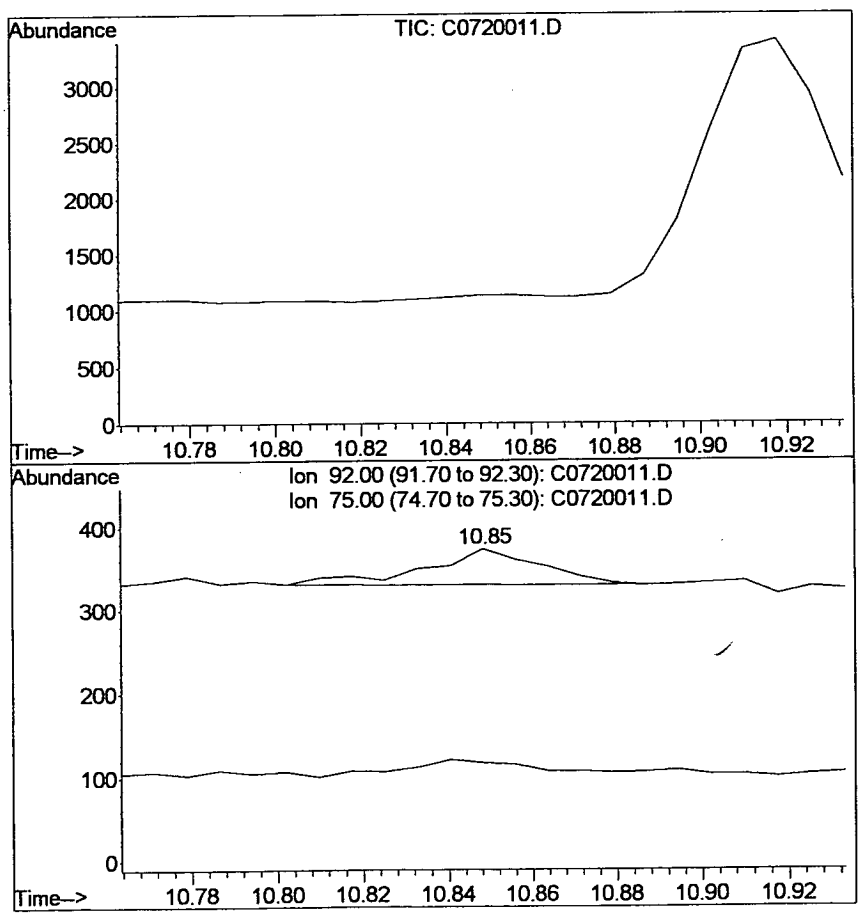

#2
NDMA
Concen: 0.20 PPB
RT: 10.85 min Scan# 165
Delta R.T. 0.02 min
Lab File: C0720011.D
Acq: 20 Jul 2007 8:48 pm

Tgt Ion: 92 Resp: 81

Ion	Ratio	Lower	Upper
92	100		
75	40.7	31.8	66.0

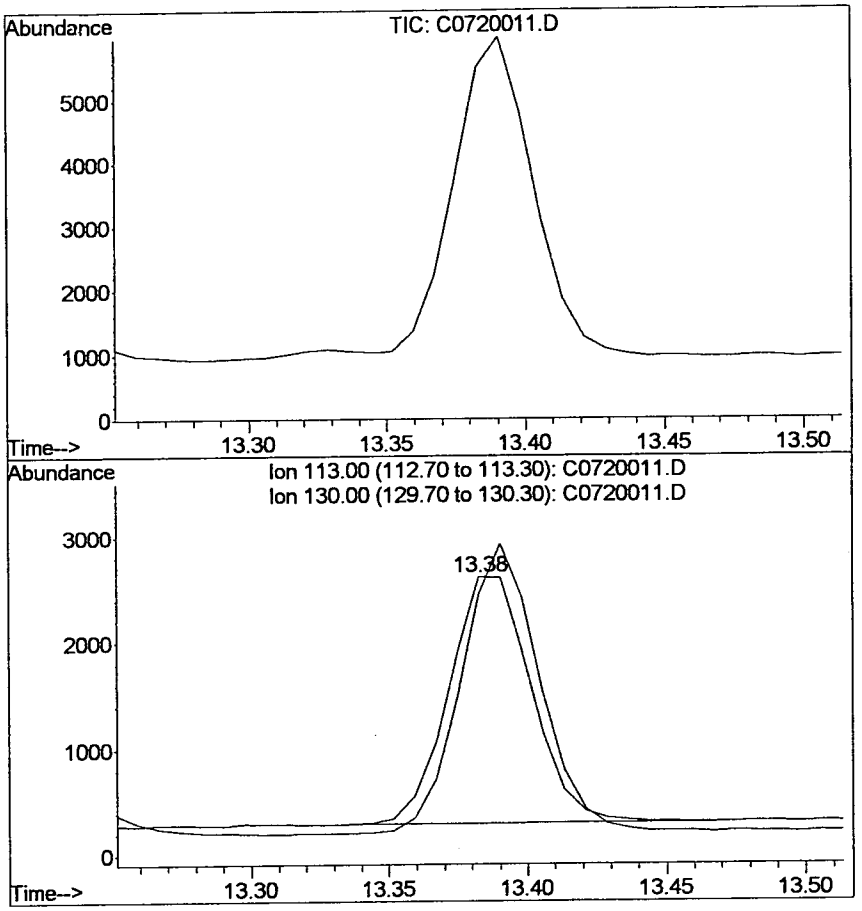

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.38 min Scan# 494
Delta R.T. 0.01 min
Lab File: C0720011.D
Acq: 20 Jul 2007 8:48 pm

Tgt Ion:113 Resp: 4776

Ion	Ratio	Lower	Upper
113	100		
130	110.2	67.1	137.1

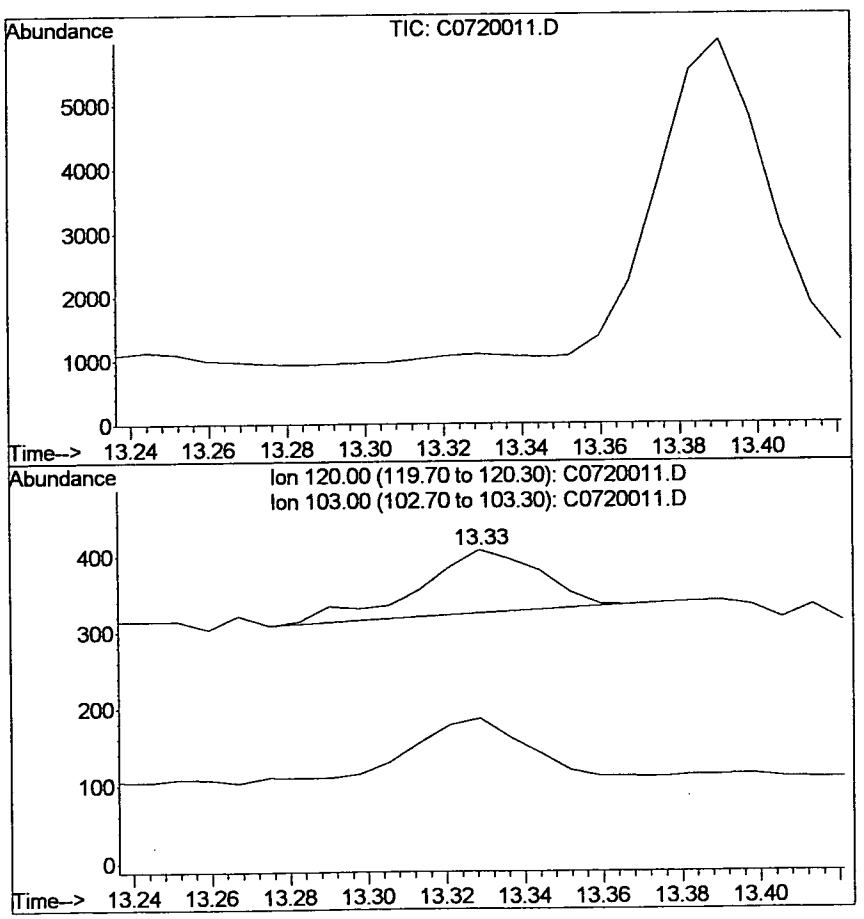

#4
NDEA
Concen: 0.36 PPB
RT: 13.33 min Scan# 487
Delta R.T. 0.01 min
Lab File: C0720011.D
Acq: 20 Jul 2007 8:48 pm

Tgt Ion:120 Resp: 183

Ion	Ratio	Lower	Upper
120	100		
103	85.2	65.3	135.5

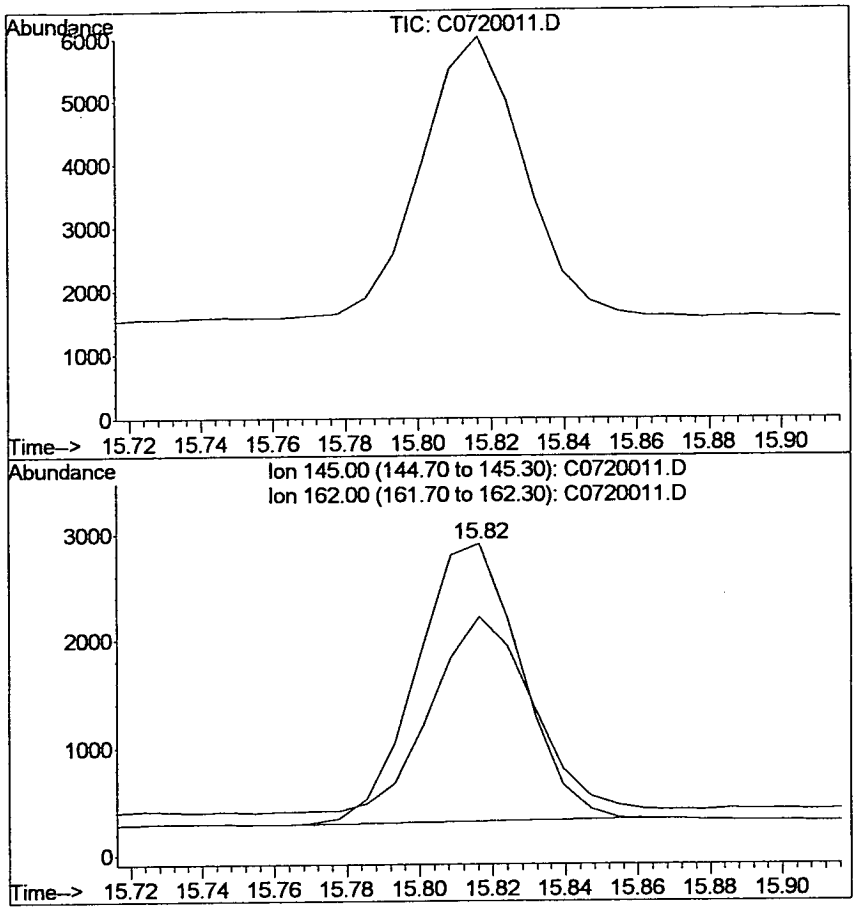

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.82 min Scan# 810
Delta R.T. 0.01 min
Lab File: C0720011.D
Acq: 20 Jul 2007 8:48 pm

Tgt Ion:145 Resp: 5087

Ion	Ratio	Lower	Upper
145	100		
162	66.9	22.4	102.4

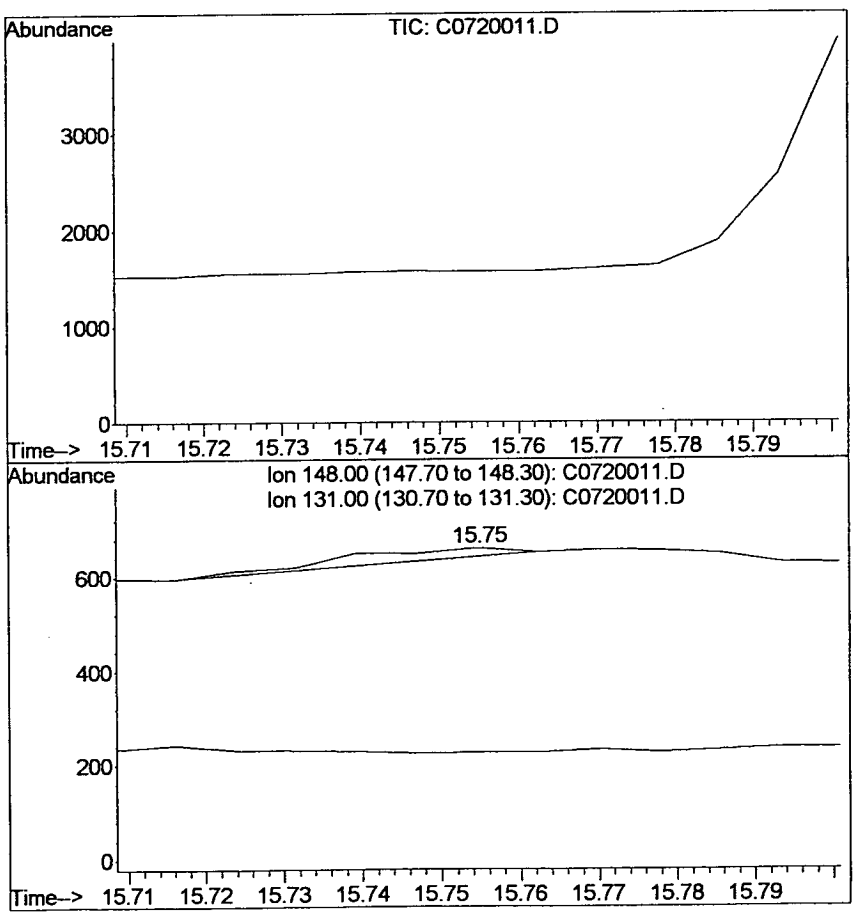

#6
NDPA
Concen: 0.18 PPB
RT: 15.75 min Scan# 802
Delta R.T. -0.02 min
Lab File: C0720011.D
Acq: 20 Jul 2007 8:48 pm

Tgt Ion:148 Resp: 73

Ion	Ratio	Lower	Upper
148	100		
131	72.6	99.8	207.2#

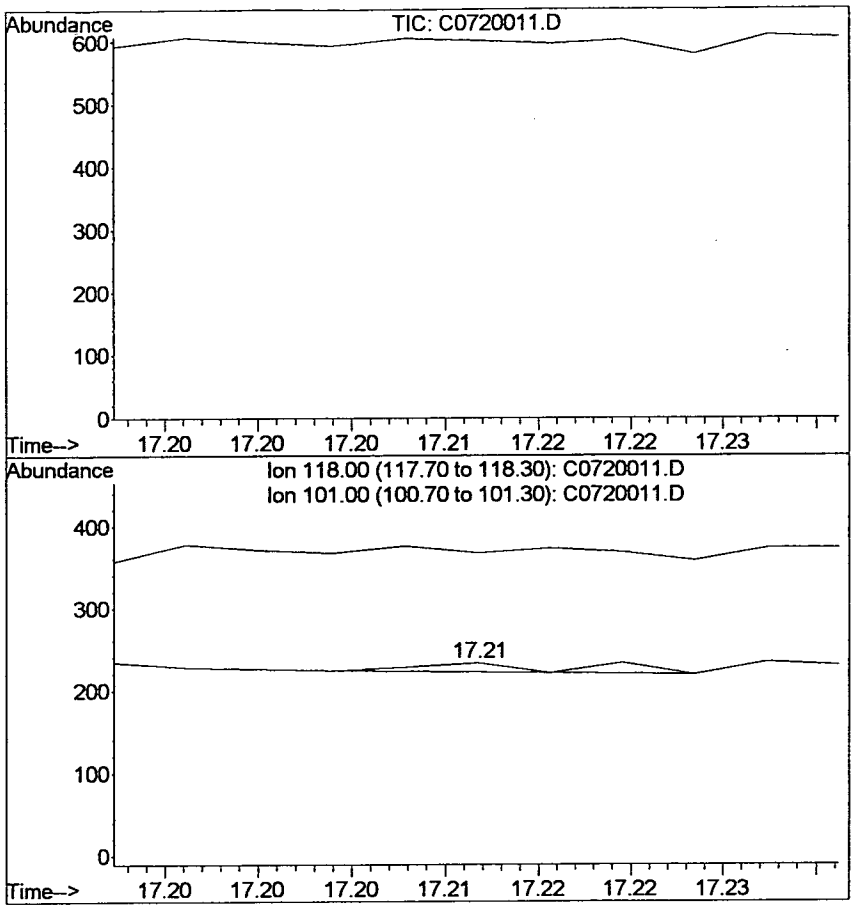

#7
NPYR
Concen: 0.01 PPB
RT: 17.21 min Scan# 1080
Delta R.T. 0.02 min
Lab File: C0720011.D
Acq: 20 Jul 2007 8:48 pm

Tgt Ion:118 Resp: 6

Ion	Ratio	Lower	Upper
118	100		
101	550.0	62.6	130.0#

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720012.D
Acq On : 20 Jul 2007 9:11 pm
Sample : IQG1460-04
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 21 6:35 2007

Vial: 13
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00

Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration
DataAcq Meth : C7F14NW

LB

Internal Standards	R.T.	QIon	Response	Conc	Units		Dev(Min)
1) NDMA-D6	10.91	81	2197	10.00	PPB		0.00
3) NDEA-D10	13.38	113	4738	10.00	PPB		0.00
5) NDPA-D14	15.81	145	5317	10.00	PPB		0.00
Target Compounds							**Qvalue**
2) NDMA	10.85	92	76	0.17	PPB		77
4) NDEA	13.33	120	53	0.10	PPB		78
6) NDPA	15.76	148	282	0.66	PPB	#	1
7) NPYR	17.09	118	10	0.02	PPB		96

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720012.D
Acq On : 20 Jul 2007 9:11 pm
Sample : IQG1460-04
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 21 6:35 2007

Vial: 13
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration

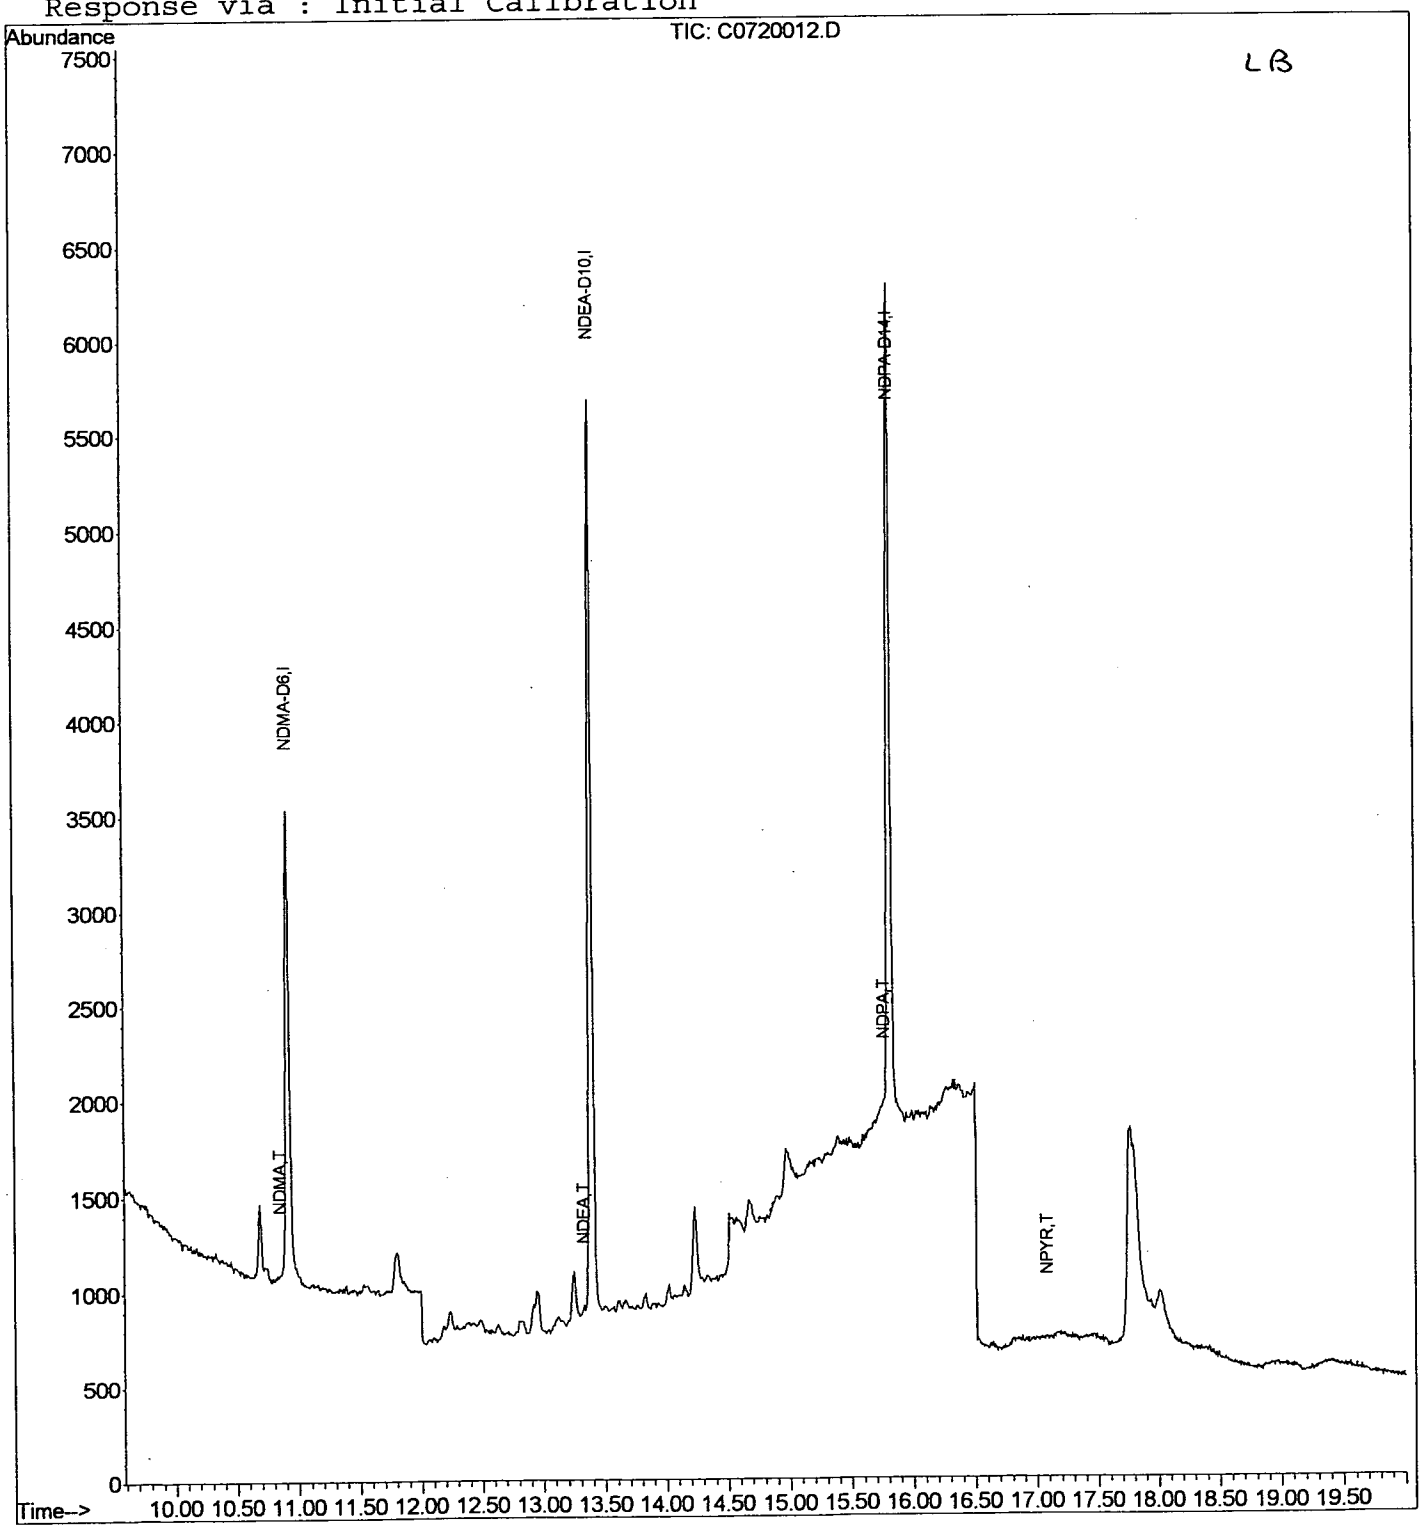

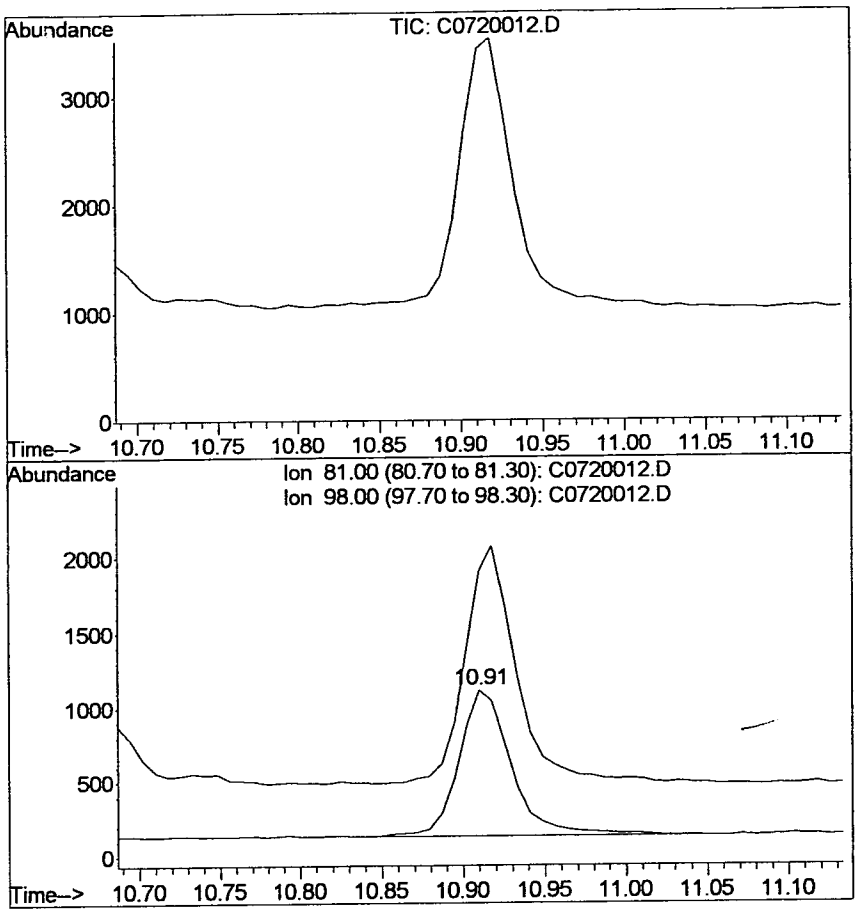

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.91 min Scan# 173
Delta R.T. 0.01 min
Lab File: C0720012.D
Acq: 20 Jul 2007 9:11 pm

Tgt Ion: 81 Resp: 2197

Ion	Ratio	Lower	Upper
81	100		
98	155.5	144.1	224.1

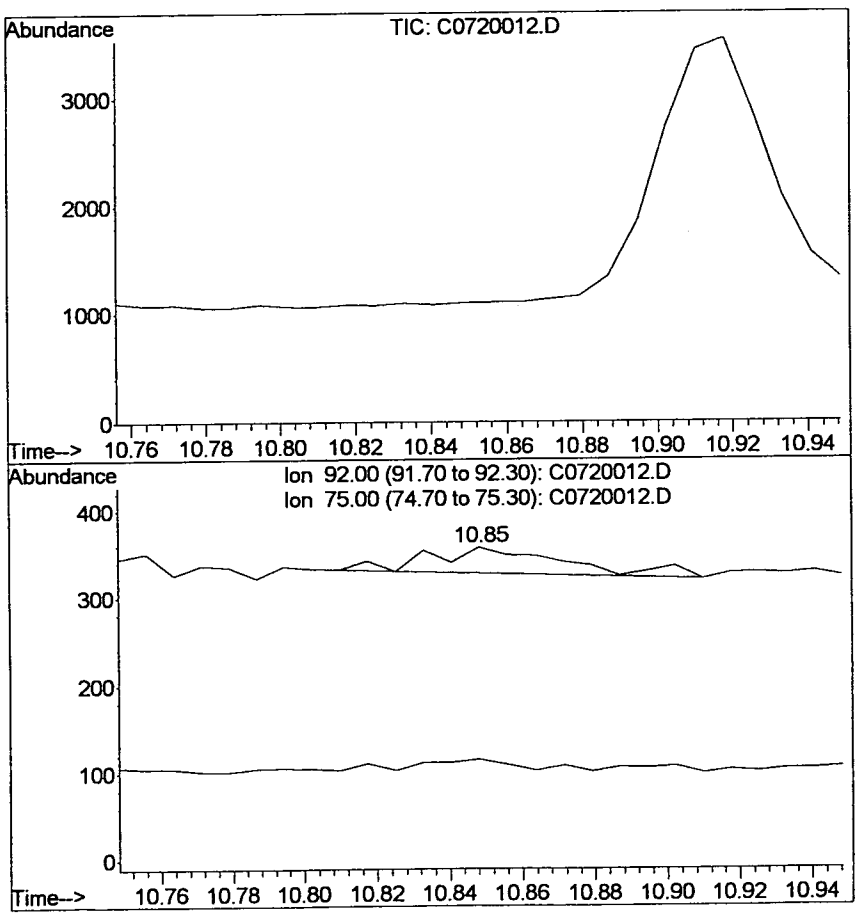

#2
NDMA
Concen: 0.17 PPB
RT: 10.85 min Scan# 165
Delta R.T. 0.02 min
Lab File: C0720012.D
Acq: 20 Jul 2007 9:11 pm

Tgt Ion: 92 Resp: 76

Ion	Ratio	Lower	Upper
92	100		
75	32.9	31.8	66.0

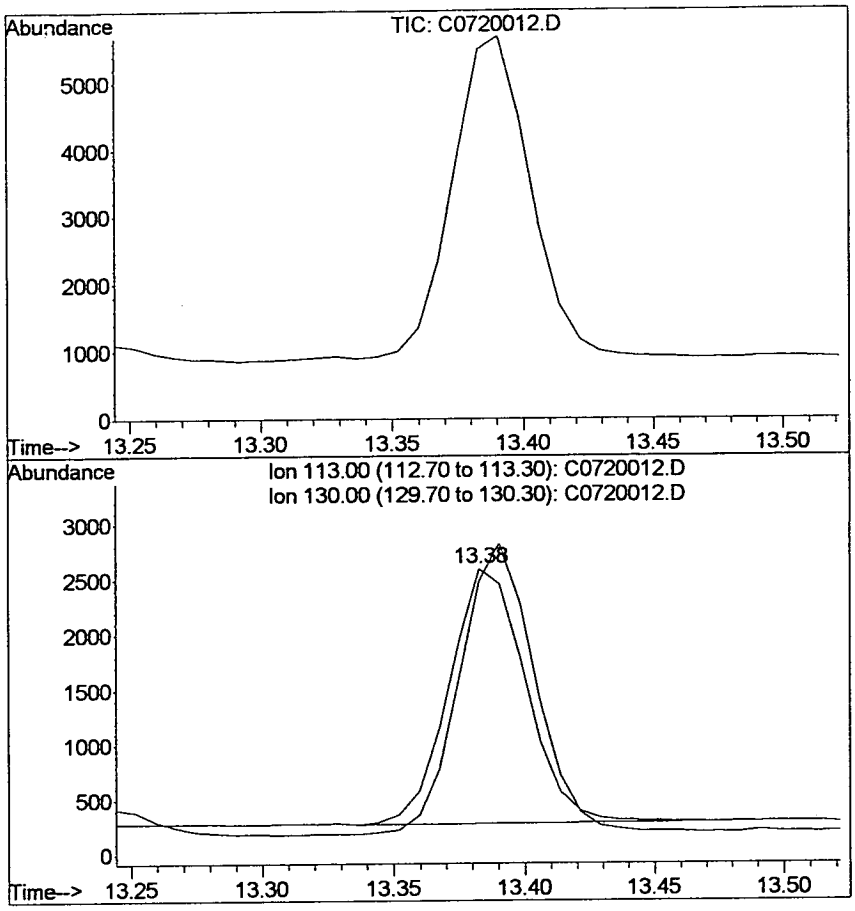

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.38 min Scan# 494
Delta R.T. 0.01 min
Lab File: C0720012.D
Acq: 20 Jul 2007 9:11 pm

Tgt Ion:113 Resp: 4738

Ion	Ratio	Lower	Upper
113	100		
130	109.0	67.1	137.1

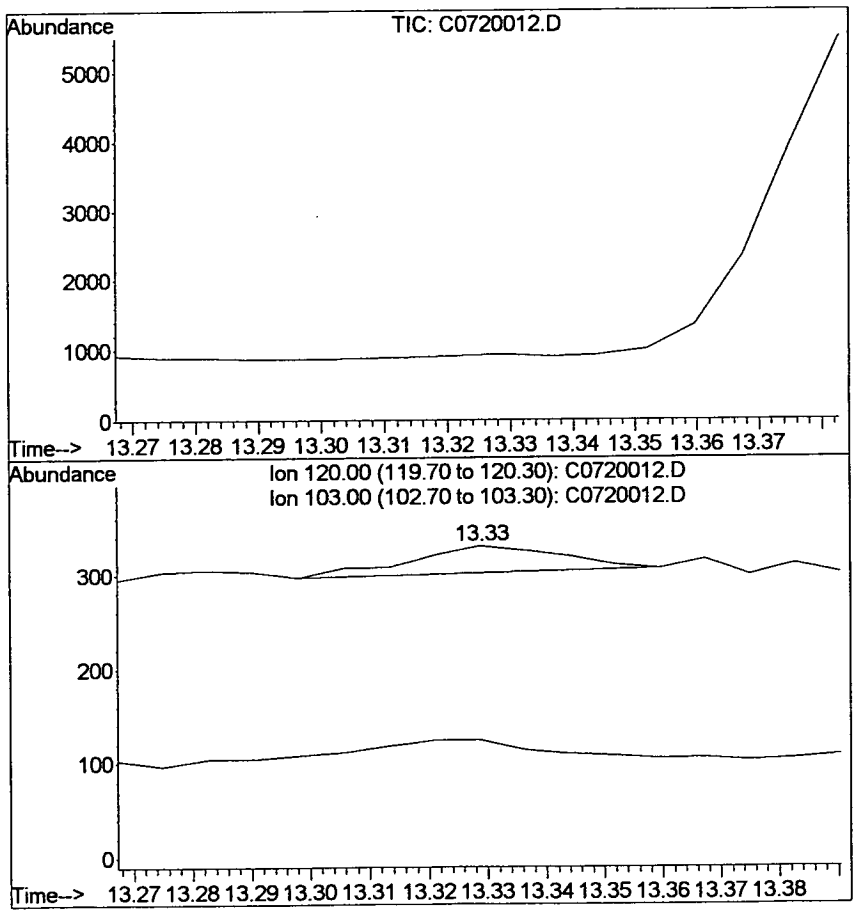

#4
NDEA
Concen: 0.10 PPB
RT: 13.33 min Scan# 487
Delta R.T. 0.01 min
Lab File: C0720012.D
Acq: 20 Jul 2007 9:11 pm

Tgt Ion:120 Resp: 53

Ion	Ratio	Lower	Upper
120	100		
103	122.6	65.3	135.5

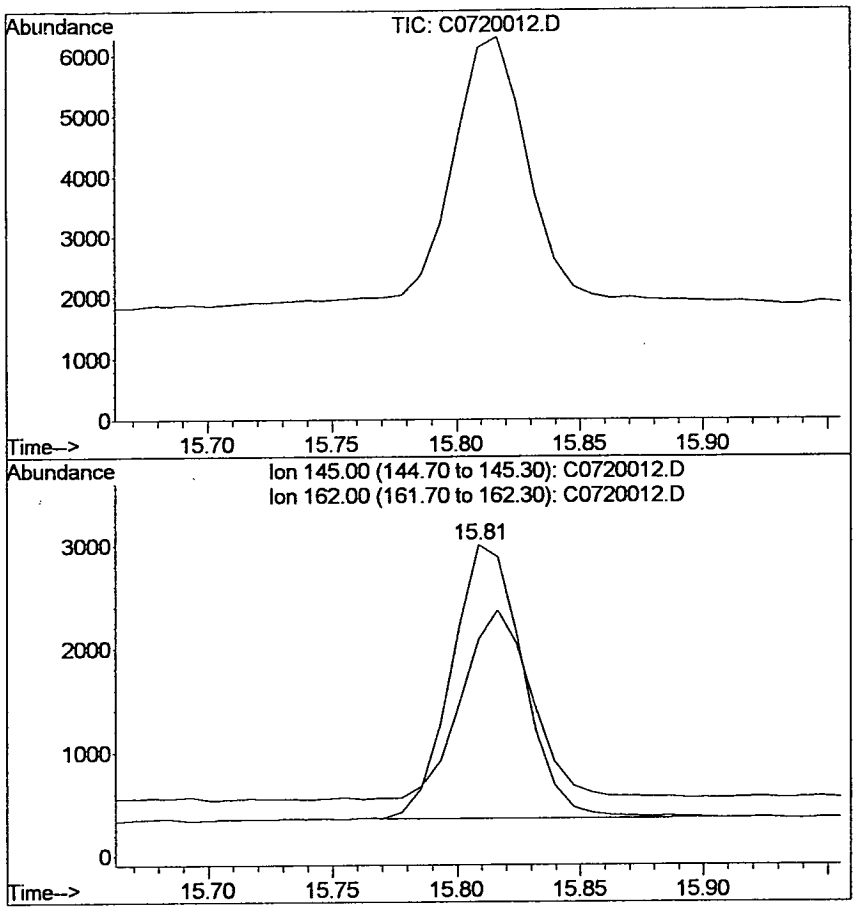

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.81 min Scan# 809
Delta R.T. 0.00 min
Lab File: C0720012.D
Acq: 20 Jul 2007 9:11 pm

Tgt Ion:145 Resp: 5317

Ion	Ratio	Lower	Upper
145	100		
162	66.4	22.4	102.4

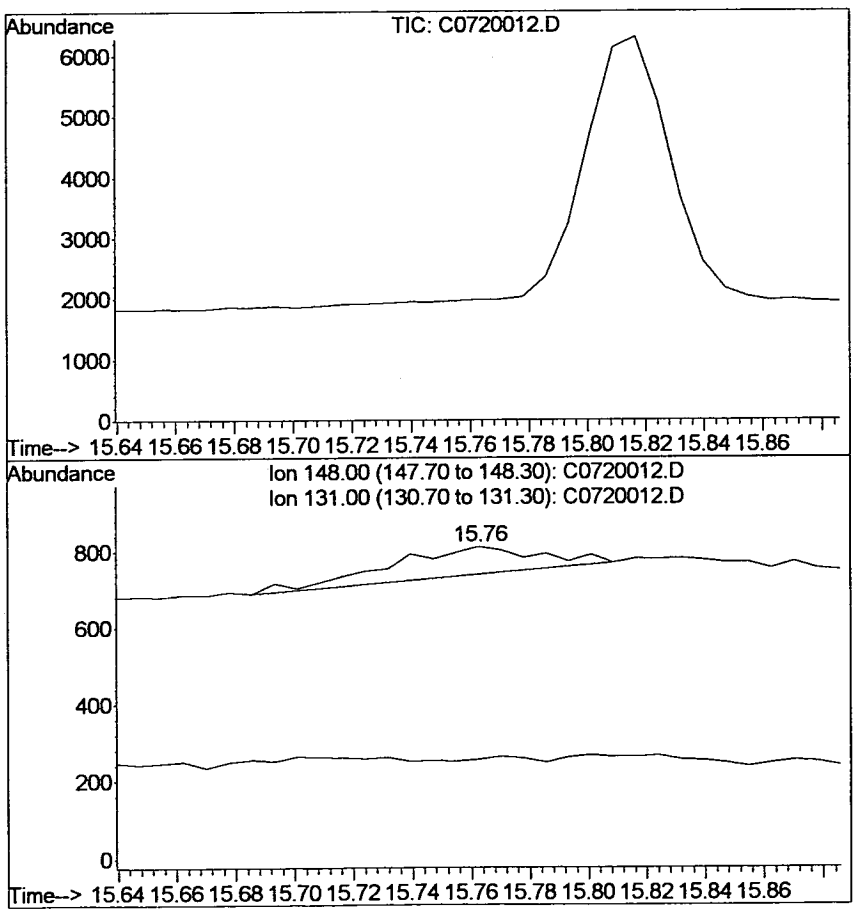

#6
NDPA
Concen: 0.66 PPB
RT: 15.76 min Scan# 803
Delta R.T. -0.01 min
Lab File: C0720012.D
Acq: 20 Jul 2007 9:11 pm

Tgt Ion:148 Resp: 282

Ion	Ratio	Lower	Upper
148	100		
131	4.6	99.8	207.2#

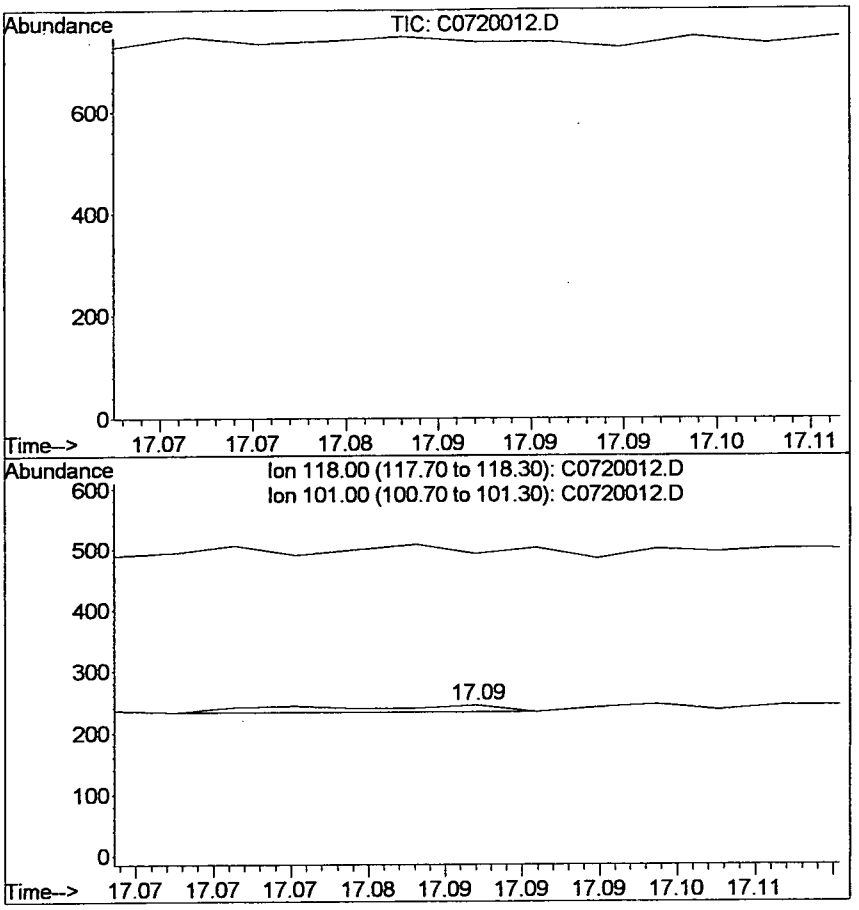

#7
NPYR
Concen: 0.02 PPB
RT: 17.09 min Scan# 1048
Delta R.T. -0.11 min
Lab File: C0720012.D
Acq: 20 Jul 2007 9:11 pm

Tgt Ion:118 Resp: 10

Ion	Ratio	Lower	Upper
118	100		
101	100.0	62.6	130.0

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720013.D
Acq On : 20 Jul 2007 9:35 pm
Sample : IQG1460-05
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 21 6:35 2007

Vial: 14
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00

Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration
DataAcq Meth : C7F14NW

LB

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) NDMA-D6	10.91	81	1815	10.00 PPB	0.00
3) NDEA-D10	13.38	113	4190	10.00 PPB	0.00
5) NDPA-D14	15.81	145	4492	10.00 PPB	0.00

Target Compounds					Qvalue
2) NDMA	10.85	92	858	2.36 PPB	98
4) NDEA	13.33	120	236	0.53 PPB	86
6) NDPA	15.77	148	319	0.88 PPB #	10
7) NPYR	0.00	118	0	N.D.	

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720013.D
Acq On : 20 Jul 2007 9:35 pm
Sample : IQG1460-05
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 21 6:35 2007

Vial: 14
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration

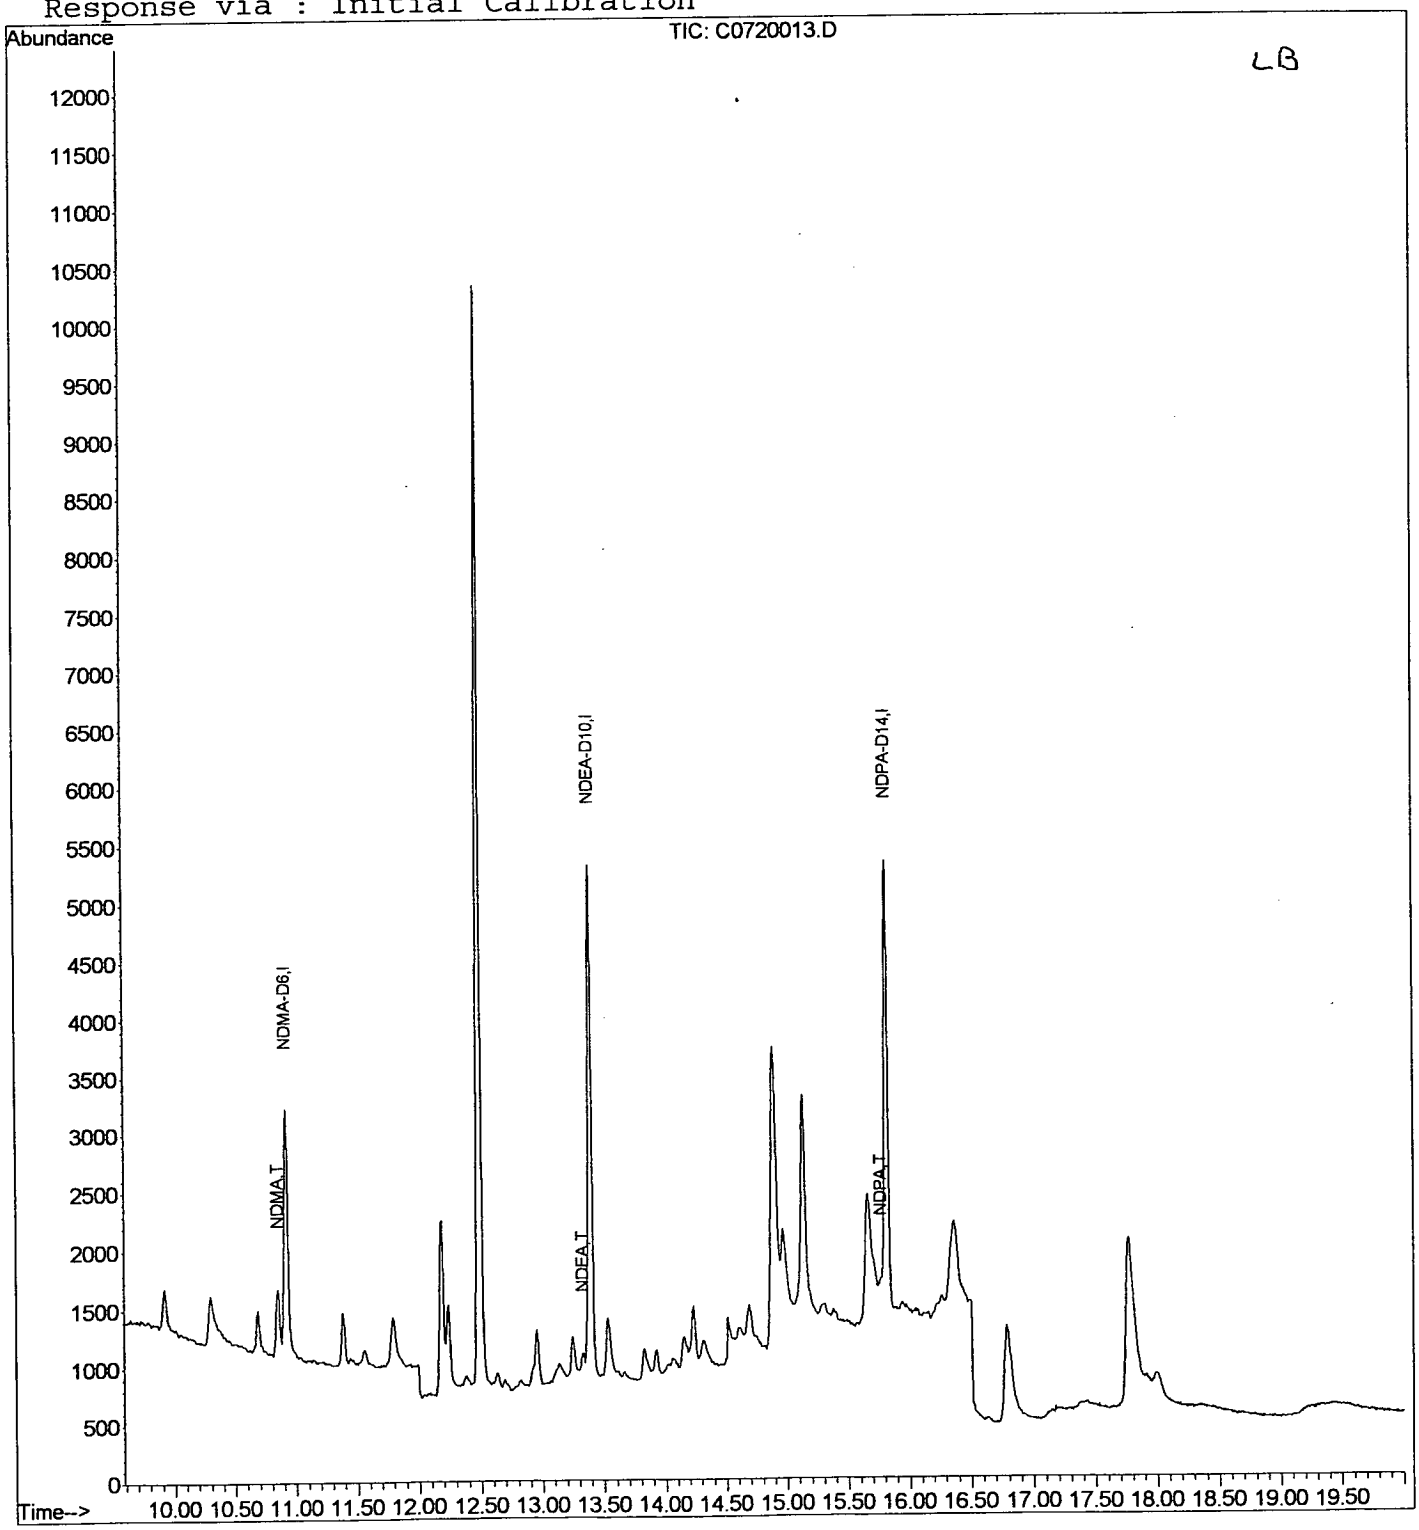

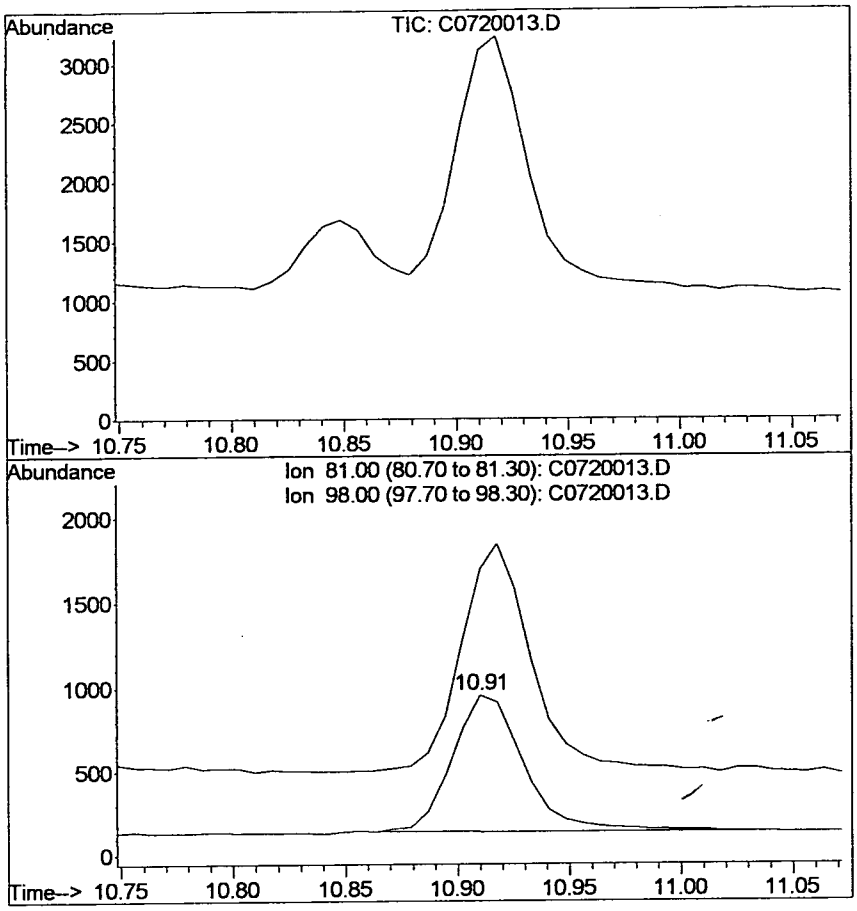

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.91 min Scan# 173
Delta R.T. 0.01 min
Lab File: C0720013.D
Acq: 20 Jul 2007 9:35 pm

Tgt Ion: 81 Resp: 1815

Ion	Ratio	Lower	Upper
81	100		
98	163.3	144.1	224.1

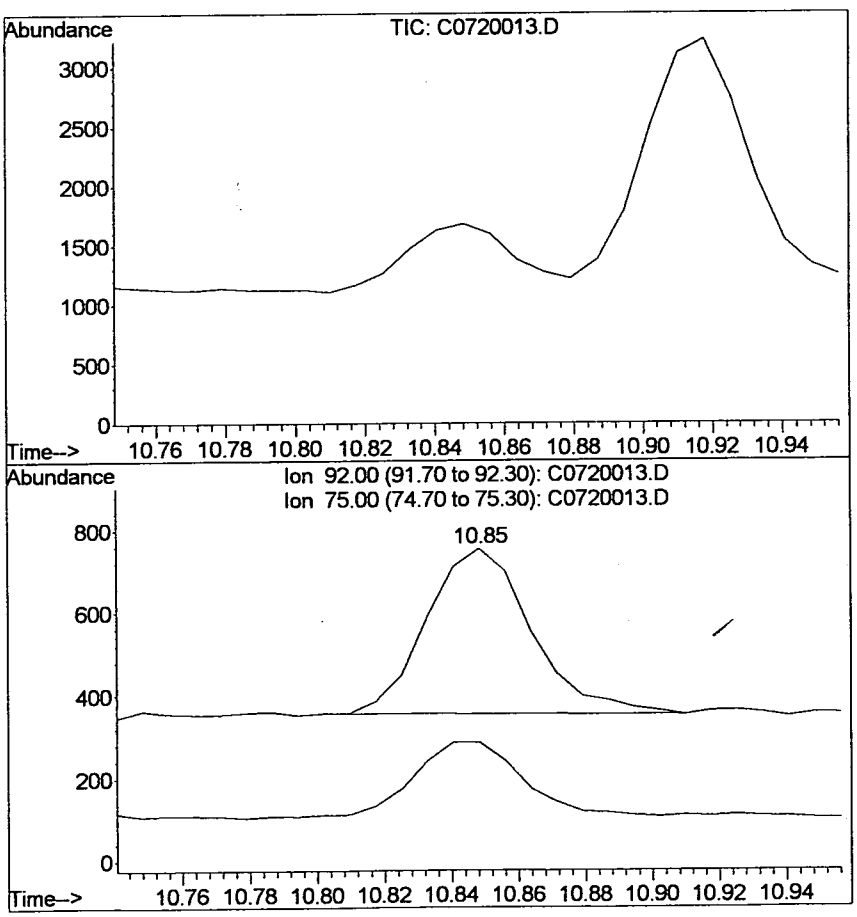

#2
NDMA
Concen: 2.36 PPB
RT: 10.85 min Scan# 165
Delta R.T. 0.02 min
Lab File: C0720013.D
Acq: 20 Jul 2007 9:35 pm

Tgt Ion: 92 Resp: 858

Ion	Ratio	Lower	Upper
92	100		
75	47.4	31.8	66.0

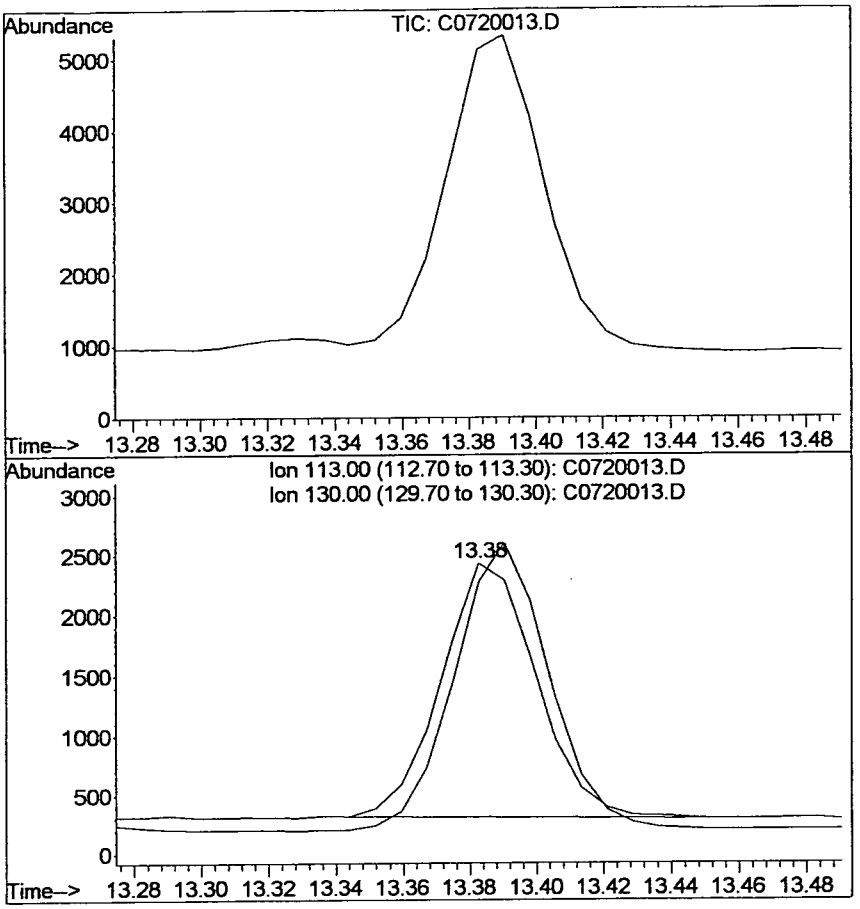

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.38 min Scan# 494
Delta R.T. 0.01 min
Lab File: C0720013.D
Acq: 20 Jul 2007 9:35 pm

Tgt Ion:113 Resp: 4190

Ion	Ratio	Lower	Upper
113	100		
130	112.2	67.1	137.1

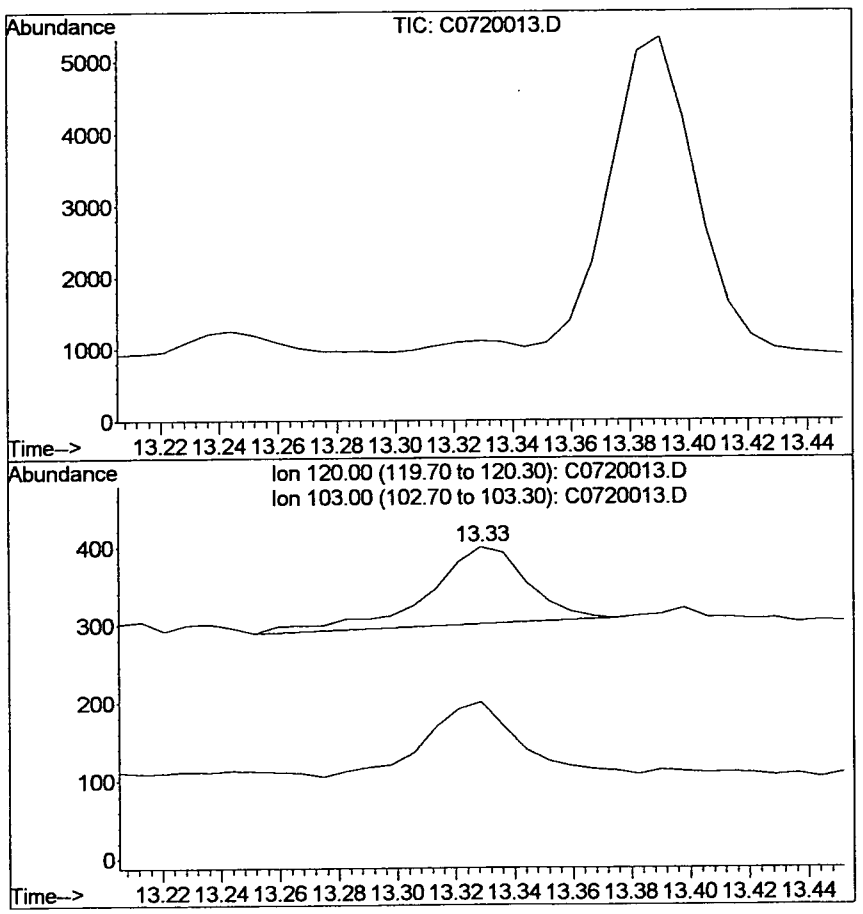

#4
NDEA
Concen: 0.53 PPB
RT: 13.33 min Scan# 487
Delta R.T. 0.01 min
Lab File: C0720013.D
Acq: 20 Jul 2007 9:35 pm

Tgt Ion:120 Resp: 236

Ion	Ratio	Lower	Upper
120	100		
103	86.9	65.3	135.5

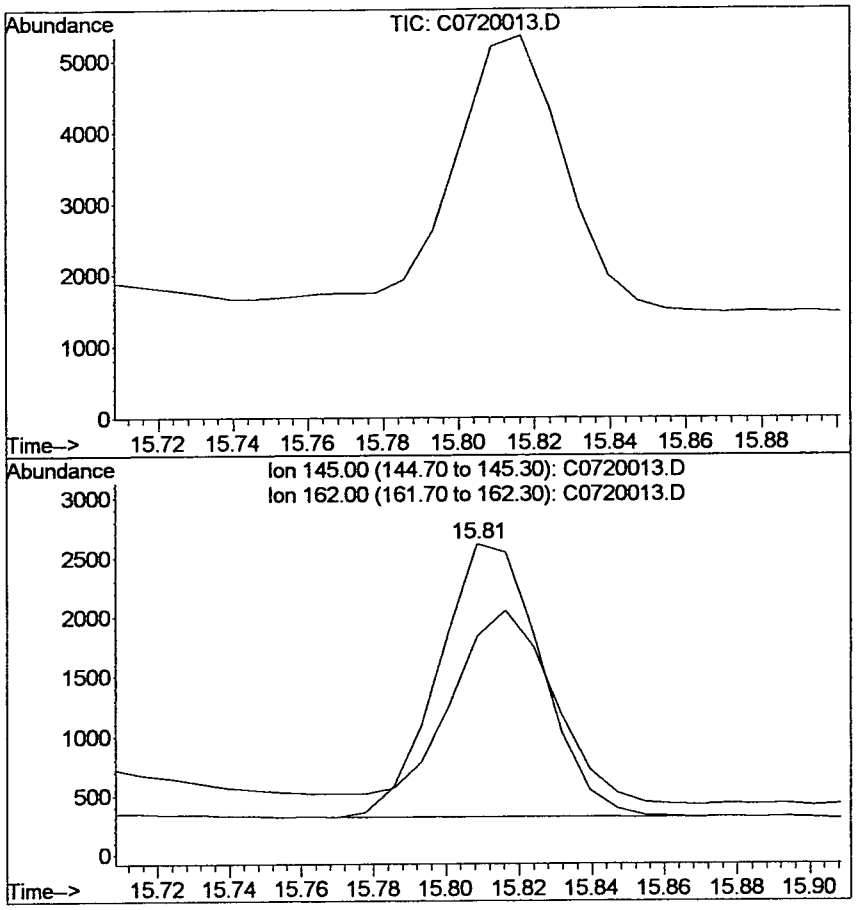

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.81 min Scan# 809
Delta R.T. -0.00 min
Lab File: C0720013.D
Acq: 20 Jul 2007 9:35 pm

Tgt Ion:145 Resp: 4492

Ion	Ratio	Lower	Upper
145	100		
162	65.5	22.4	102.4

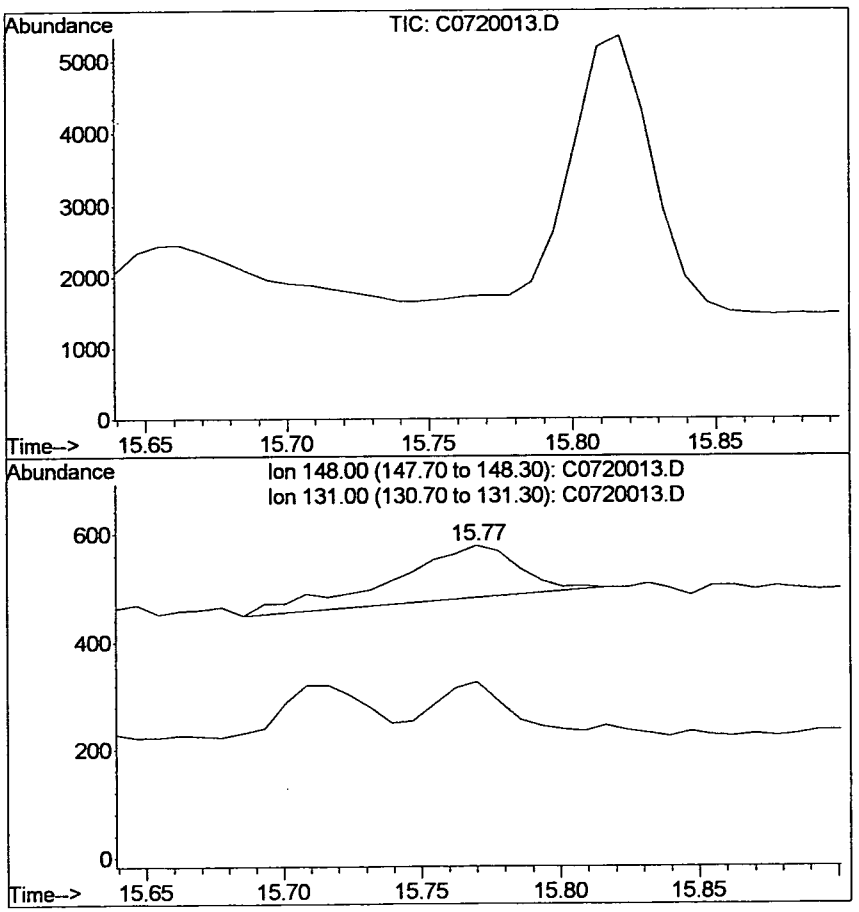

#6
NDPA
Concen: 0.88 PPB
RT: 15.77 min Scan# 804
Delta R.T. -0.00 min
Lab File: C0720013.D
Acq: 20 Jul 2007 9:35 pm

Tgt Ion:148 Resp: 319

Ion	Ratio	Lower	Upper
148	100		
131	38.2	99.8	207.2#

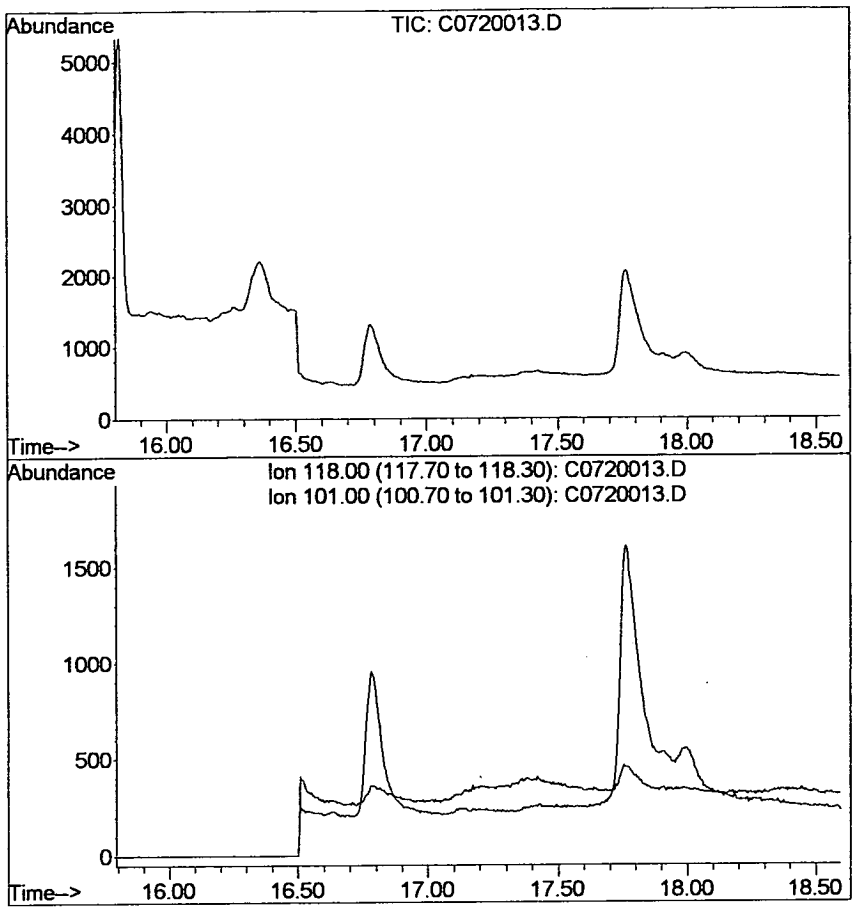

#7
NPYR
Concen: N.D.
Expected RT: 17.20 min

Lab File: C0720013.D
Acq: 20 Jul 2007 9:35 pm

Tgt Ion: 118

Sig	Exp Ratio
118	100
101	96.3

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720014.D
Acq On : 20 Jul 2007 9:58 pm
Sample : IQG1460-06
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 21 6:35 2007

Vial: 15
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00

Quant Results File: C7F14NW.RES

Quant Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration
DataAcq Meth : C7F14NW

LB

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) NDMA-D6	10.91	81	2028	10.00 PPB	0.00
3) NDEA-D10	13.38	113	4335	10.00 PPB	0.00
5) NDPA-D14	15.82	145	4669	10.00 PPB	0.00

Target Compounds					Qvalue
2) NDMA	10.85	92	189	0.47 PPB	94
4) NDEA	13.32	120	159	0.34 PPB	97
6) NDPA	15.74	148	93	0.25 PPB	71
7) NPYR	0.00	118	0	N.D.	

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : C:\MSDCHEM\1\DATA\07JUL20\C0720014.D
Acq On : 20 Jul 2007 9:58 pm
Sample : IQG1460-06
Misc : WATER 1L/1ml ----- Batch 7G19061
MS Integration Params: RTEINT2.P
Quant Time: Jul 21 6:35 2007

Vial: 15
Operator: DF/AI
Inst : gcms37
Multiplr: 1.00
Quant Results File: C7F14NW.RES

Method : C:\MSDCHEM\1\METHODS\C7F14NW.M (RTE Integrator)
Title : Nitrosamine Water ICAL
Last Update : Thu Jun 14 16:31:25 2007
Response via : Initial Calibration

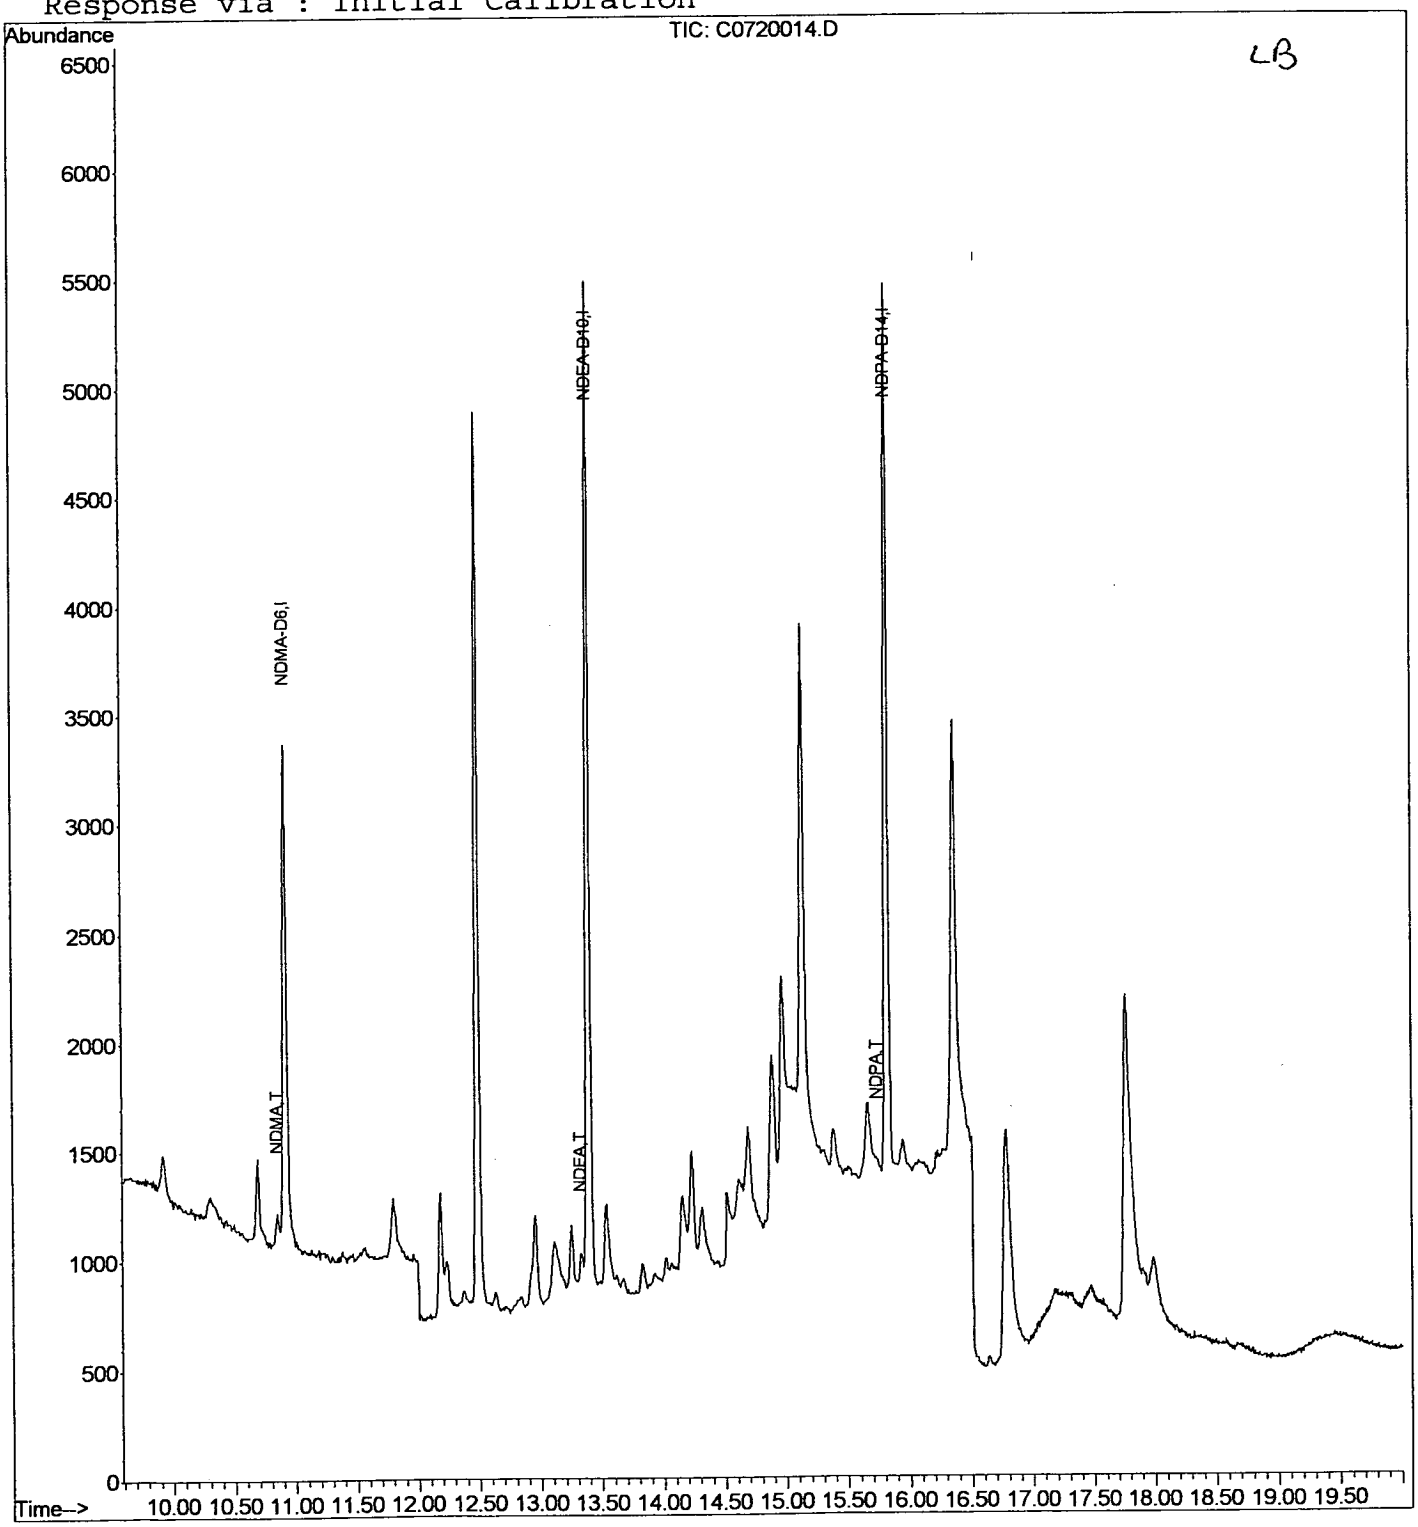

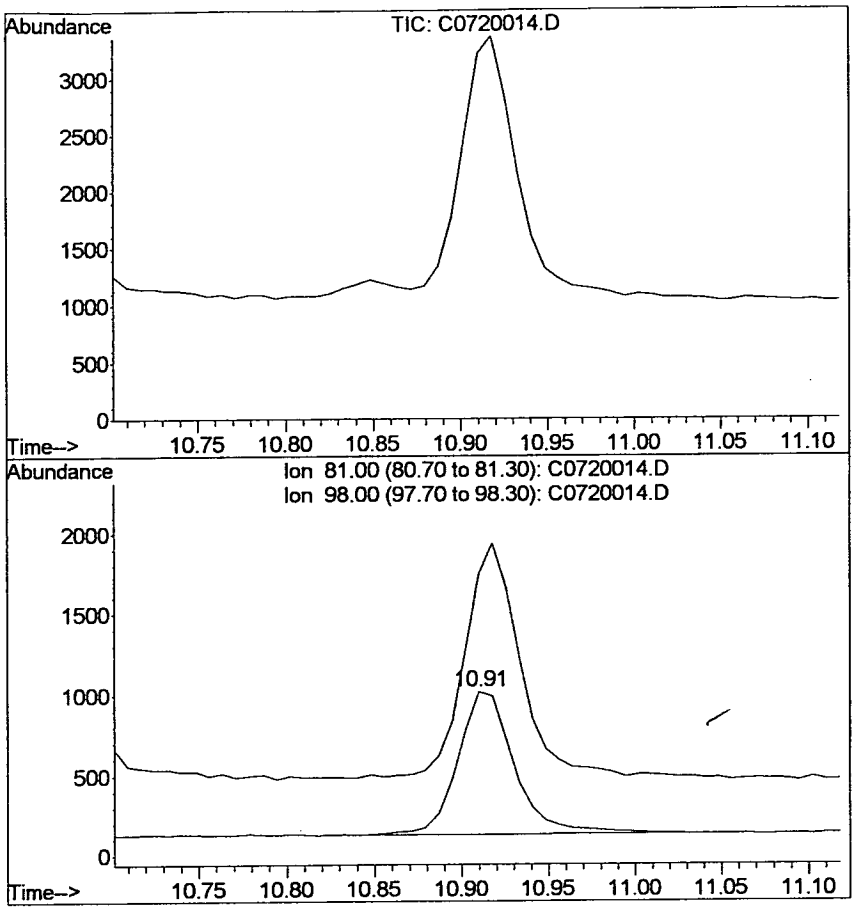

#1
NDMA-D6
Concen: 10.00 PPB
RT: 10.91 min Scan# 173
Delta R.T. 0.01 min
Lab File: C0720014.D
Acq: 20 Jul 2007 9:58 pm

Tgt Ion: 81 Resp: 2028

Ion	Ratio	Lower	Upper
81	100		
98	152.0	144.1	224.1

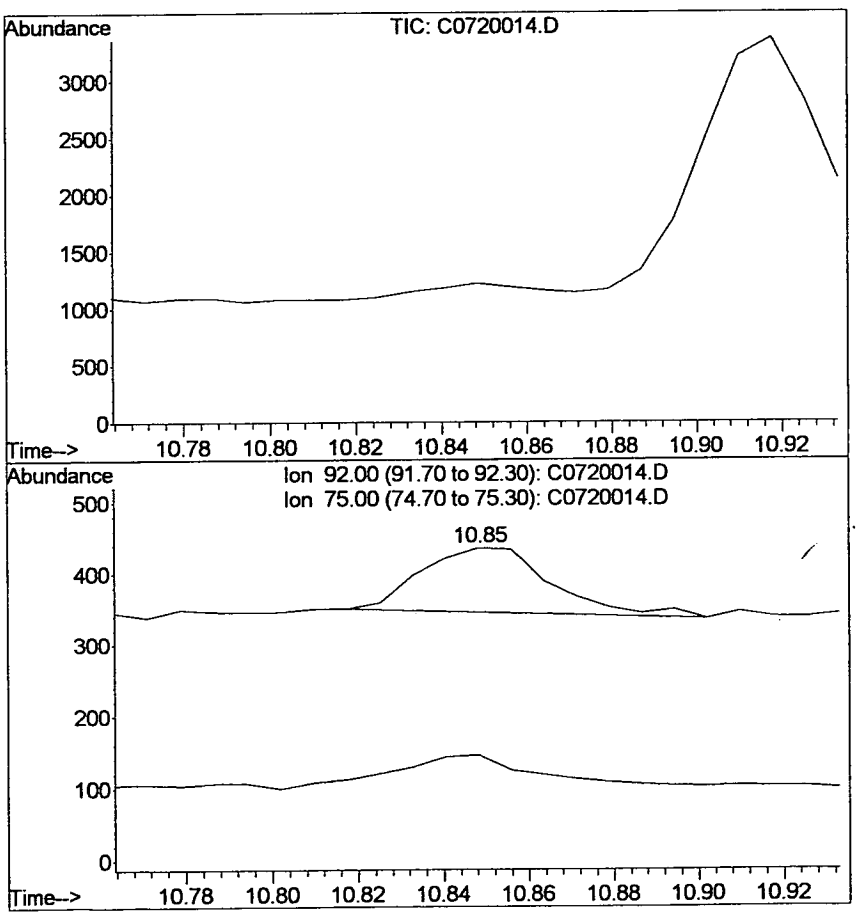

#2
NDMA
Concen: 0.47 PPB
RT: 10.85 min Scan# 165
Delta R.T. 0.02 min
Lab File: C0720014.D
Acq: 20 Jul 2007 9:58 pm

Tgt Ion: 92 Resp: 189

Ion	Ratio	Lower	Upper
92	100		
75	52.9	31.8	66.0

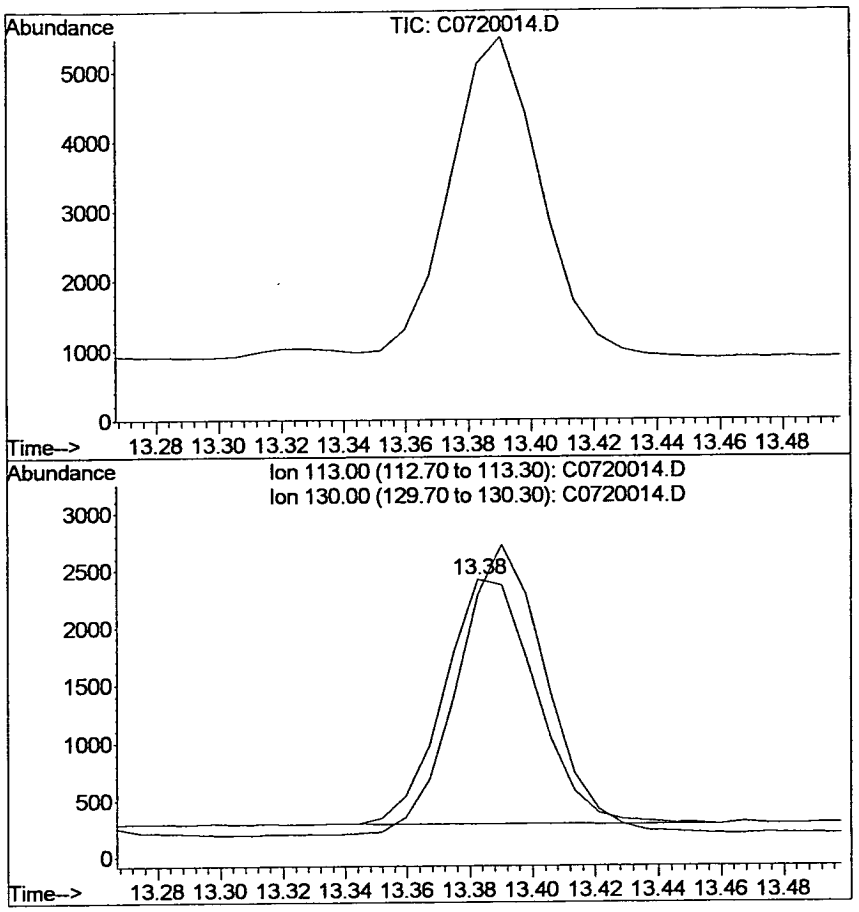

#3
NDEA-D10
Concen: 10.00 PPB
RT: 13.38 min Scan# 494
Delta R.T. 0.01 min
Lab File: C0720014.D
Acq: 20 Jul 2007 9:58 pm

Tgt Ion:113 Resp: 4335

Ion	Ratio	Lower	Upper
113	100		
130	113.1	67.1	137.1

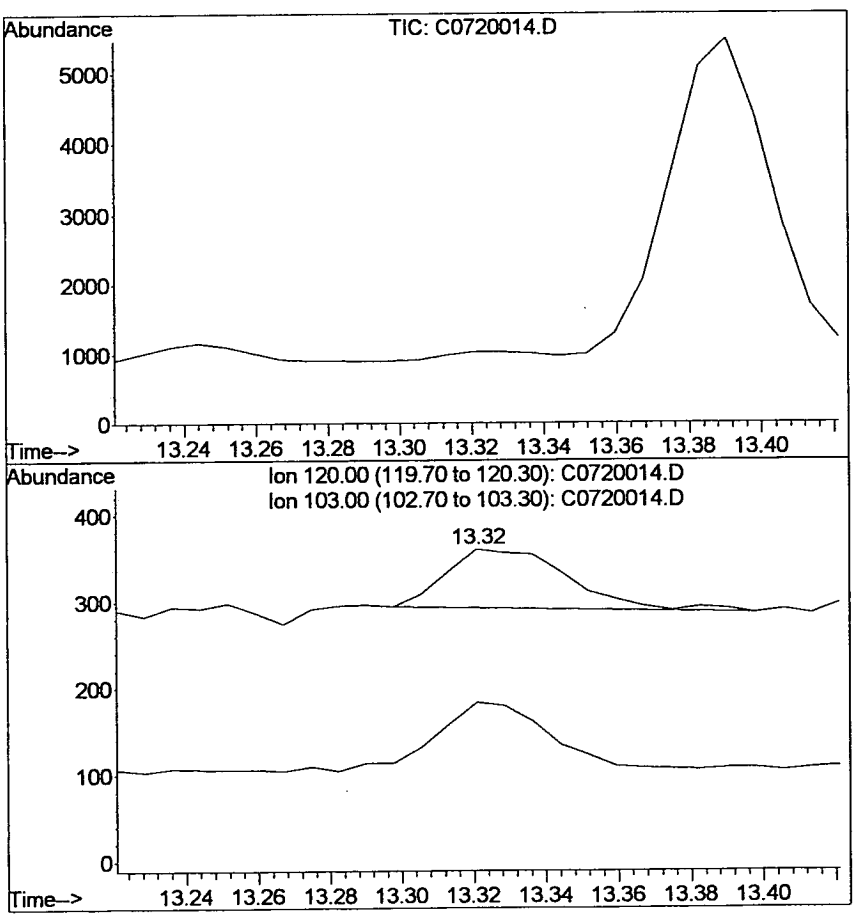

#4
NDEA
Concen: 0.34 PPB
RT: 13.32 min Scan# 486
Delta R.T. -0.00 min
Lab File: C0720014.D
Acq: 20 Jul 2007 9:58 pm

Tgt Ion:120 Resp: 159

Ion	Ratio	Lower	Upper
120	100		
103	103.8	65.3	135.5

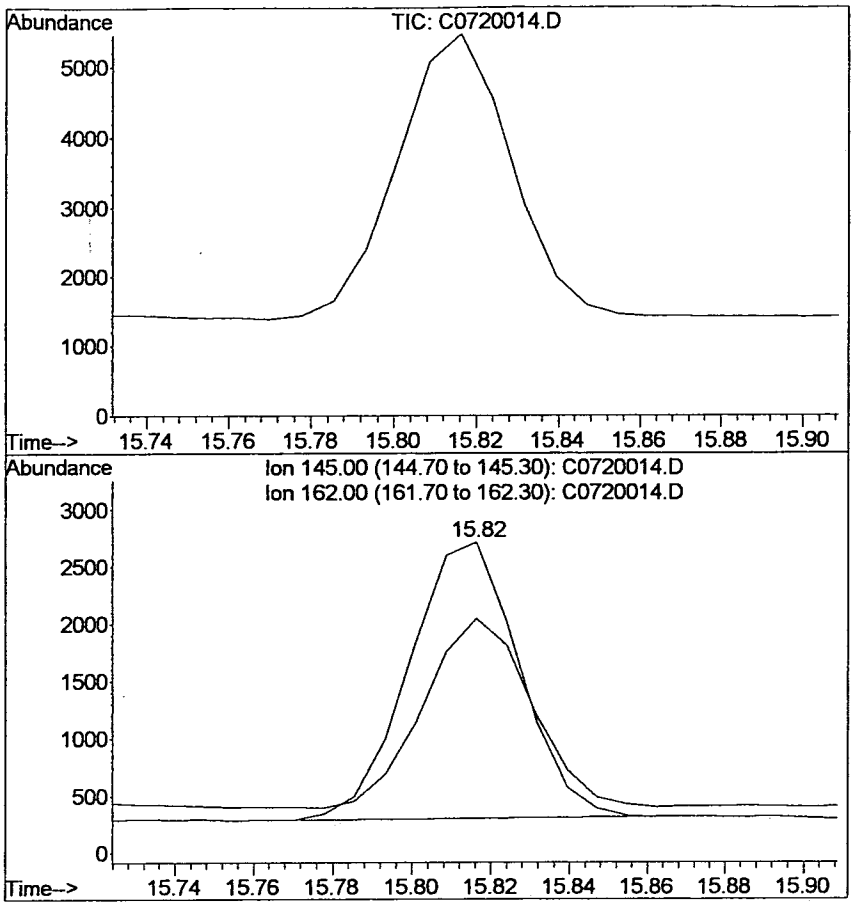

#5
NDPA-D14
Concen: 10.00 PPB
RT: 15.82 min Scan# 810
Delta R.T. 0.01 min
Lab File: C0720014.D
Acq: 20 Jul 2007 9:58 pm

Tgt Ion:145 Resp: 4669

Ion	Ratio	Lower	Upper
145	100		
162	66.8	22.4	102.4

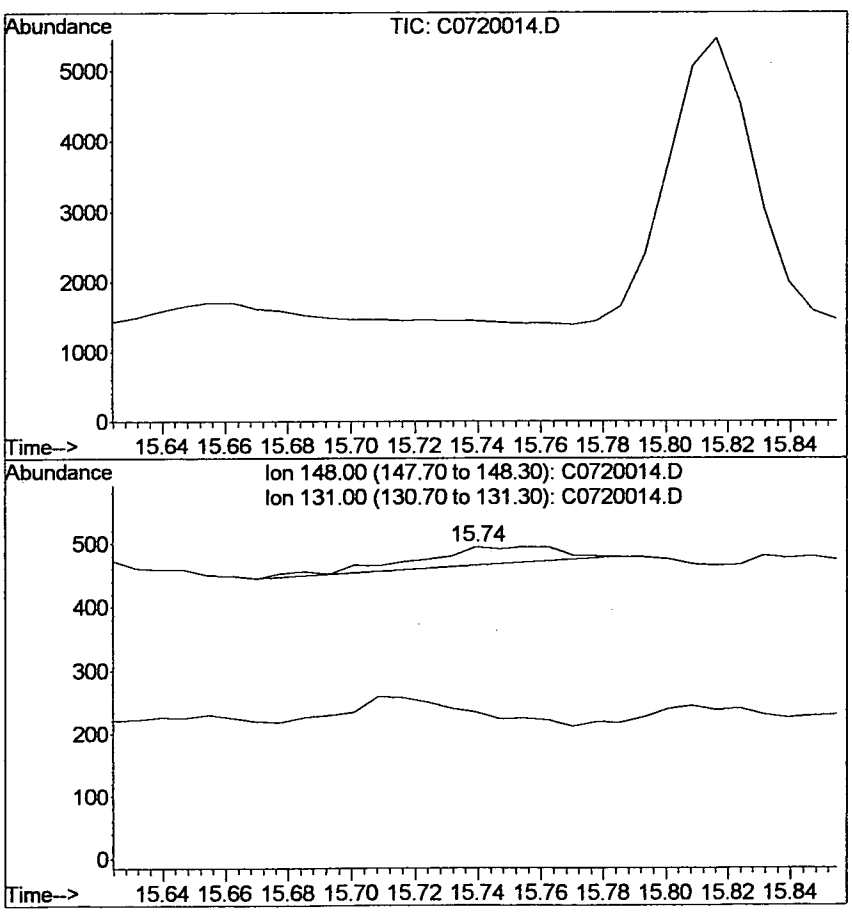

#6
NDPA
Concen: 0.25 PPB
RT: 15.74 min Scan# 800
Delta R.T. -0.03 min
Lab File: C0720014.D
Acq: 20 Jul 2007 9:58 pm

Tgt Ion:148 Resp: 93

Ion	Ratio	Lower	Upper
148	100		
131	116.1	99.8	207.2

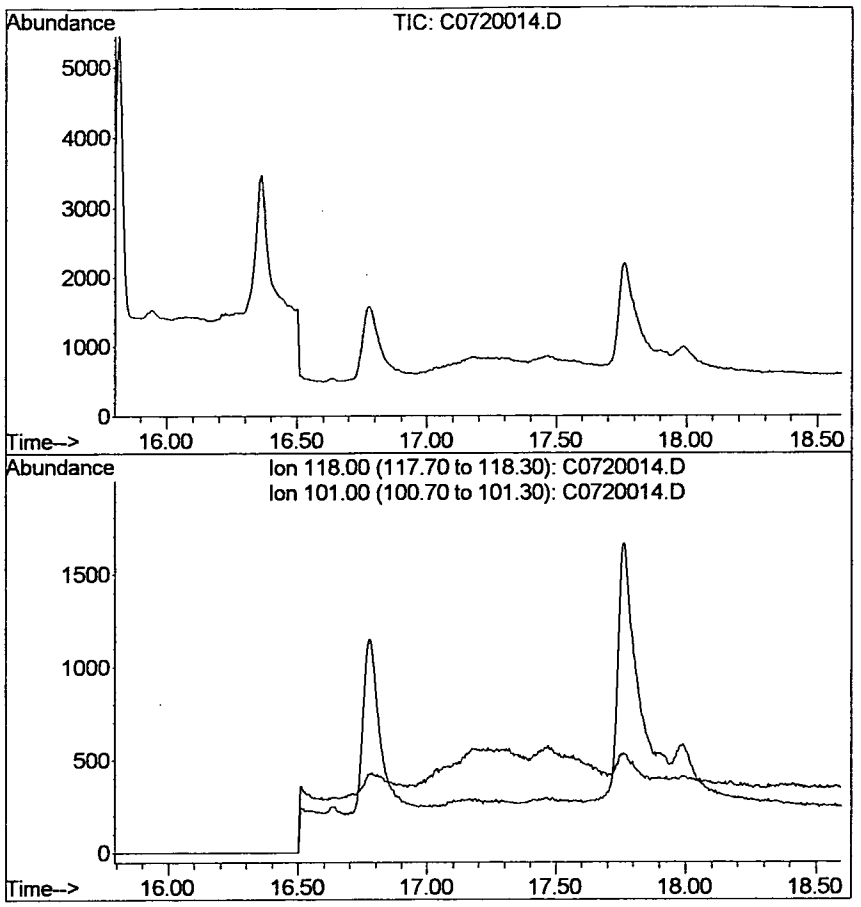

#7
NPYR
Concen: N.D.
Expected RT: 17.20 min

Lab File: C0720014.D
Acq: 20 Jul 2007 9:58 pm

Tgt Ion: 118

Sig	Exp Ratio
118	100
101	96.3

TestAmerica
ANALYTICAL TESTING CORPORATION
17461Derian Ave. Suite 100 Irvine CA 92614 (949) 261-1022 FAX (949) 260-3297

QA/QC PACKAGE: LEVEL IV
PREPARED FOR: GPL LABORATORIES
LABORATORY NUMBER: IQG1460
PROJECT: OMEGA CHEMICAL OU-2 SSID-BC
OMEGA CHEMICAL 335392.FI.01

EPA 218.6 LABORATORY RAW DATA

- INITIAL CALIBRATION
- CONTINUING CALIBRATION
- DIGESTION LOG
- RUN LOG
- QUANTITATION REPORTS

TotalChrom Method File H:\DATA\IC4\chr6qd30.mth
Printed by : inorg on: 4/30/2007 11:31:30 AM
Created by : inorg on: 4/30/2007 11:31:24 AM
Edited by : inorg on: 4/30/2007 11:31:24 AM
Number of Times Edited : 0
Number of Times Calibrated : 40
Description: CHANGED RT FROM 5.7 TO 5.3

Instrument Conditions

Instrument Control Method
Instrument Name : ICDNX-4
Instrument Type : 900 Series Intelligent Interface

Interface Parameters
Delay Time : 0.30 min
Run Time : 9.00 min
Sampling Rate : 20.0000 pts/s
Interface Type : 900 Series Intelligent Interface
Analog Voltage Input : 1000 mV
Data will be collected from channel A

Timed Events
RLY3 set to Off at 0.00 min
RLY3 set to On at 8.90 min

Real Time Plot Parameters

	Pages	Offset (mV)	Scale (mV)
Channel A	1	120.000	20.000

Processing Parameters
Bunch Factor : 40 points
Noise Threshold : 2 µV
Area Threshold : 14.00 µV

Peak Separation Criteria
Width Ratio : 0.200
Valley-to-Peak Ratio : 0.010

Exponential Skim Criteria
Peak Height Ratio : 5.000
Adjusted Height Ratio : 4.000
Valley Height Ratio : 3.000

Baseline Timed Events
Event #1 - Disable Peak Detection at 0.400
Event #2 - Enable Peak Detection at 4.383

Optional Reports
No report format files given

Optional Report Plot Parameters

Plot Number	1	2	3	4	5
Generate this plot	No	No	No	No	No
Start plot at end of delay time	Yes	Yes	Yes	Yes	Yes
Start Time					
End Time					
Scale Type	Vertical Scaling	Vertical Scaling	Vertical Scaling	Vertical Scaling	Vertical Scaling
Scale Factor	1.000	1.000	1.000	1.000	1.000
Full Scale					
Offset					

Annotated Replot Parameters
Offset & Scale set to absolute values
Draw baselines

Include timed event annotations

Plot Offset : 129.000 µV
Plot Scale : 7.500 µV
Number of Pages : 1
Plot Title : Chromatogram
X-Axis Label : Time [min]
Y-Axis Label : Response [mV]
Orientation : Landscape
Retention Labels : Top of Plot
Component Labels : Actual Time
Start Time : 0.00
End Time : 9.00

User Programs

No user programs will be executed

Global Sample Information

Default Sample Volume : 1.000 uL
Quantitation Units : ng
Void Time : 0.000 min
Correct amounts during calibration : Yes
Convert unknowns to concentration units : Yes
Reject outliers during calibration : No

An External Standard calibration will be used
Unknown peaks will be quantitated using a response factor of 1.000000e+06
First peak will be relative retention reference

Component Information

chrom6

Component Type : Single Peak Component
Retention Time : 7.007 min
Search Window : 2.00 s, 7.00 %
Reference Component :
Find largest peak in window
Calibrating Height versus Amount using a 1st Order Fit
Curve will ignore the origin
Amounts will not be scaled prior to the regression
Weighting factor for the regression: 1
Component standard purity percentage : 100.0000%

User Values

Label :
Value 1 : 0.000000
Value 2 : 0.000000
Value 3 : 0.000000
Value 4 : 0.000000
Value 5 : 0.000000

Calibration Level

Level Name	Amount	Area	Height	ISTD Amt.	ISTD Resp.	# Replicates
1	0.0001	0.00	0.00	————	————	0
2	0.3000	265.90	16.49	————	————	1
3	1.0000	779.65	37.92	————	————	1
4	5.0000	3317.80	166.71	————	————	1
5	10.0000	5521.80	312.29	————	————	1
6	25.0000	14074.45	786.15	————	————	1
7	50.0000	28618.20	1601.31	————	————	1
8	75.0000	42355.20	2395.19	————	————	1

Calibration Curve : y = (1.459791) + (31.896423)x + (0.000000)x^2 + (0.000000)x^3
R-squared : 0.999938

Calibration Replicate Lists

Component : chrom6
Level : 1
This level has no replicate injections

4/30/2007 11:31:30 AM Method: H:\DATA\IC4\chr6qd30.mth

Level : 2

Area	Height	Vol Adj Amt	ISTD Response	ISTD Amount	Date	Time	File
265.90	16.49	0.3000	———	———	4/30/2007	11:30:08 AM	H:\DATA\IC4\20070428\20070428004.rst

Level : 3

Area	Height	Vol Adj Amt	ISTD Response	ISTD Amount	Date	Time	File
779.65	37.92	1.0000	———	———	4/30/2007	11:30:08 AM	H:\DATA\IC4\20070428\20070428005.rst

Level : 4

Area	Height	Vol Adj Amt	ISTD Response	ISTD Amount	Date	Time	File
3317.80	166.71	5.0000	———	———	4/30/2007	11:30:09 AM	H:\DATA\IC4\20070428\20070428006.rst

Level : 5

Area	Height	Vol Adj Amt	ISTD Response	ISTD Amount	Date	Time	File
5521.80	312.29	10.0000	———	———	4/30/2007	11:30:09 AM	H:\DATA\IC4\20070428\20070428007.rst

Level : 6

Area	Height	Vol Adj Amt	ISTD Response	ISTD Amount	Date	Time	File
14074.45	786.15	25.0000	———	———	4/30/2007	11:30:09 AM	H:\DATA\IC4\20070428\20070428008.rst

Level : 7

Area	Height	Vol Adj Amt	ISTD Response	ISTD Amount	Date	Time	File
28618.20	1601.31	50.0000	———	———	4/30/2007	11:30:09 AM	H:\DATA\IC4\20070428\20070428009.rst

Level : 8

Area	Height	Vol Adj Amt	ISTD Response	ISTD Amount	Date	Time	File
42355.20	2395.19	75.0000	———	———	4/30/2007	11:30:10 AM	H:\DATA\IC4\20070428\20070428010.rst

TotalChrom Sequence File H:\DATA\IC4\20070428\20070428.seq
Printed by : inorg on: 4/30/2007 11:32:52 AM
Created by : inorg on: 4/28/2007 3:01:42 PM
Edited by : inorg on: 4/30/2007 11:32:46 AM
Number of Times Edited : 5
Description:

Sequence File Header Information:
Number of Rows : 176
Instrument Type : 900 Series Intelligent Interface
Injection Type : SINGLE
Raw tokens channel A :
Result tokens channel A :
Modified tokens channel A :
Raw tokens channel B :
Result tokens channel B :
Modified tokens channel B :

Sequence Sample Descriptions - Channel A

Row	Type	Name	Number	Study name	Sample Amt	Sample Vol	Dil Factor	Multiplier	Divisor	Addend	Norm Factor
1	Sample	IB	7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
2	Sample	7D28054-BS1	7D28054	7040301	1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
3	Sample	0ppb	7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
4	Sample	0.3ppb	7D28054	7040301	1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
5	Sample	1.0ppb	7D28054	7040301	1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
6	Sample	5.0ppb	7D28054	7040301	1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
7	Sample	10ppb	7D28054	7040301	1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
8	Sample	25ppb	7D28054	7040301	1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
9	Sample	50ppb	7D28054	7040301	1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
10	Sample	75ppb	7D28054	7040301	1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
11	Sample	ICV	7D28054	7040302	1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
12	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
13	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
14	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
15	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
16	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
17	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
18	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
19	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
20	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
21	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
22	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
23	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
24	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
25	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
26	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
27	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
28	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
29	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
30	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
31	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
32	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
33	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
34	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
35	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
36	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
37	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
38	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
39	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
40	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
41	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
42	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
43	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
44	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
45	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
46	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
47	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
48	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
49	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
50	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
51	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
52	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
53	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
54	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
55	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
56	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
57	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
58	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
59	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
60	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
61	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
62	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
63	Sample		7D28054		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000

CALIBRATION CHECKLIST

EPA 7199 & 218.6 – Hexavalent Chromium by IC

Analyst:	TM/EC	2nd Level Review:	[illegible]
Analysis Date:	4/30/07	Date:	5/25/07
IC #:	IC4	Original Calibration date:	4/19/07
Method used:	218.6 & 7199	Original Calibration file #:	Chrqd19.MTH Chrqd19a.MTH

Analyst Rev	2nd Level Rev	
✓	✓	6-point calibration, lowest point at RL, r >= 0.999
✓	✓	2nd ICV: %REC = 90-110% (immediately after calibration)
		Calibration date and file checked for completeness and accuracy:
✓	✓	• Correct date, analyst's name and calibration file
✓	✓	• Correct instrument parameters, retention time and window
✓	✓	• Chromatography peak shape and baseline acceptable
✓	✓	• Calibration summary and raw data match for calibration levels and area counts
		Instrument update for new calibration information:
✓	✓	• Calibration: Chrqd30.MTH
✓	✓	• Standard preparation: 7040301
✓	✓	• Supplier: ERA
✓	✓	• Standard Lot #: 100751.4
		• Calibration Chart:

Comments:

Cr6_cal.doc
Rev 09/15/04

Software Version	: 6.2.1.0.106:0106	Date	: 4/28/2007 3:57:04 PM
Reprocess Number	: ic2: 84758		
Operator	: inorg	Sample Name	: 0ppb
Sample Number	: 7D28054	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 4/28/2007 3:47:46 PM	Cycle	: 3

Raw Data File : h:\data\ic4\20070428\20070428003.raw
Result File : h:\data\ic4\20070428\20070428003.rst
Inst Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428003.raw
Proc Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428003.rst
Calib Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428003.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070428\20070428.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
-	7.037	chrom6	0.00	0.00000	0.0000	0.0000	
			0.00	0.00000	0.0000	0.0000	

Report stored in ASCII file: h:\data\ic4\20070428\20070428003.TX0

Chromatogram

Sample Name : 0ppb Sample #: 7D28054 Page 1 of 1
FileName : h:\data\ic4\20070428\20070428003.raw
Date : 4/28/2007 3:57:09 PM
Method : chr6qd19a.mth Time of Injection: 4/28/2007 3:47:46 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

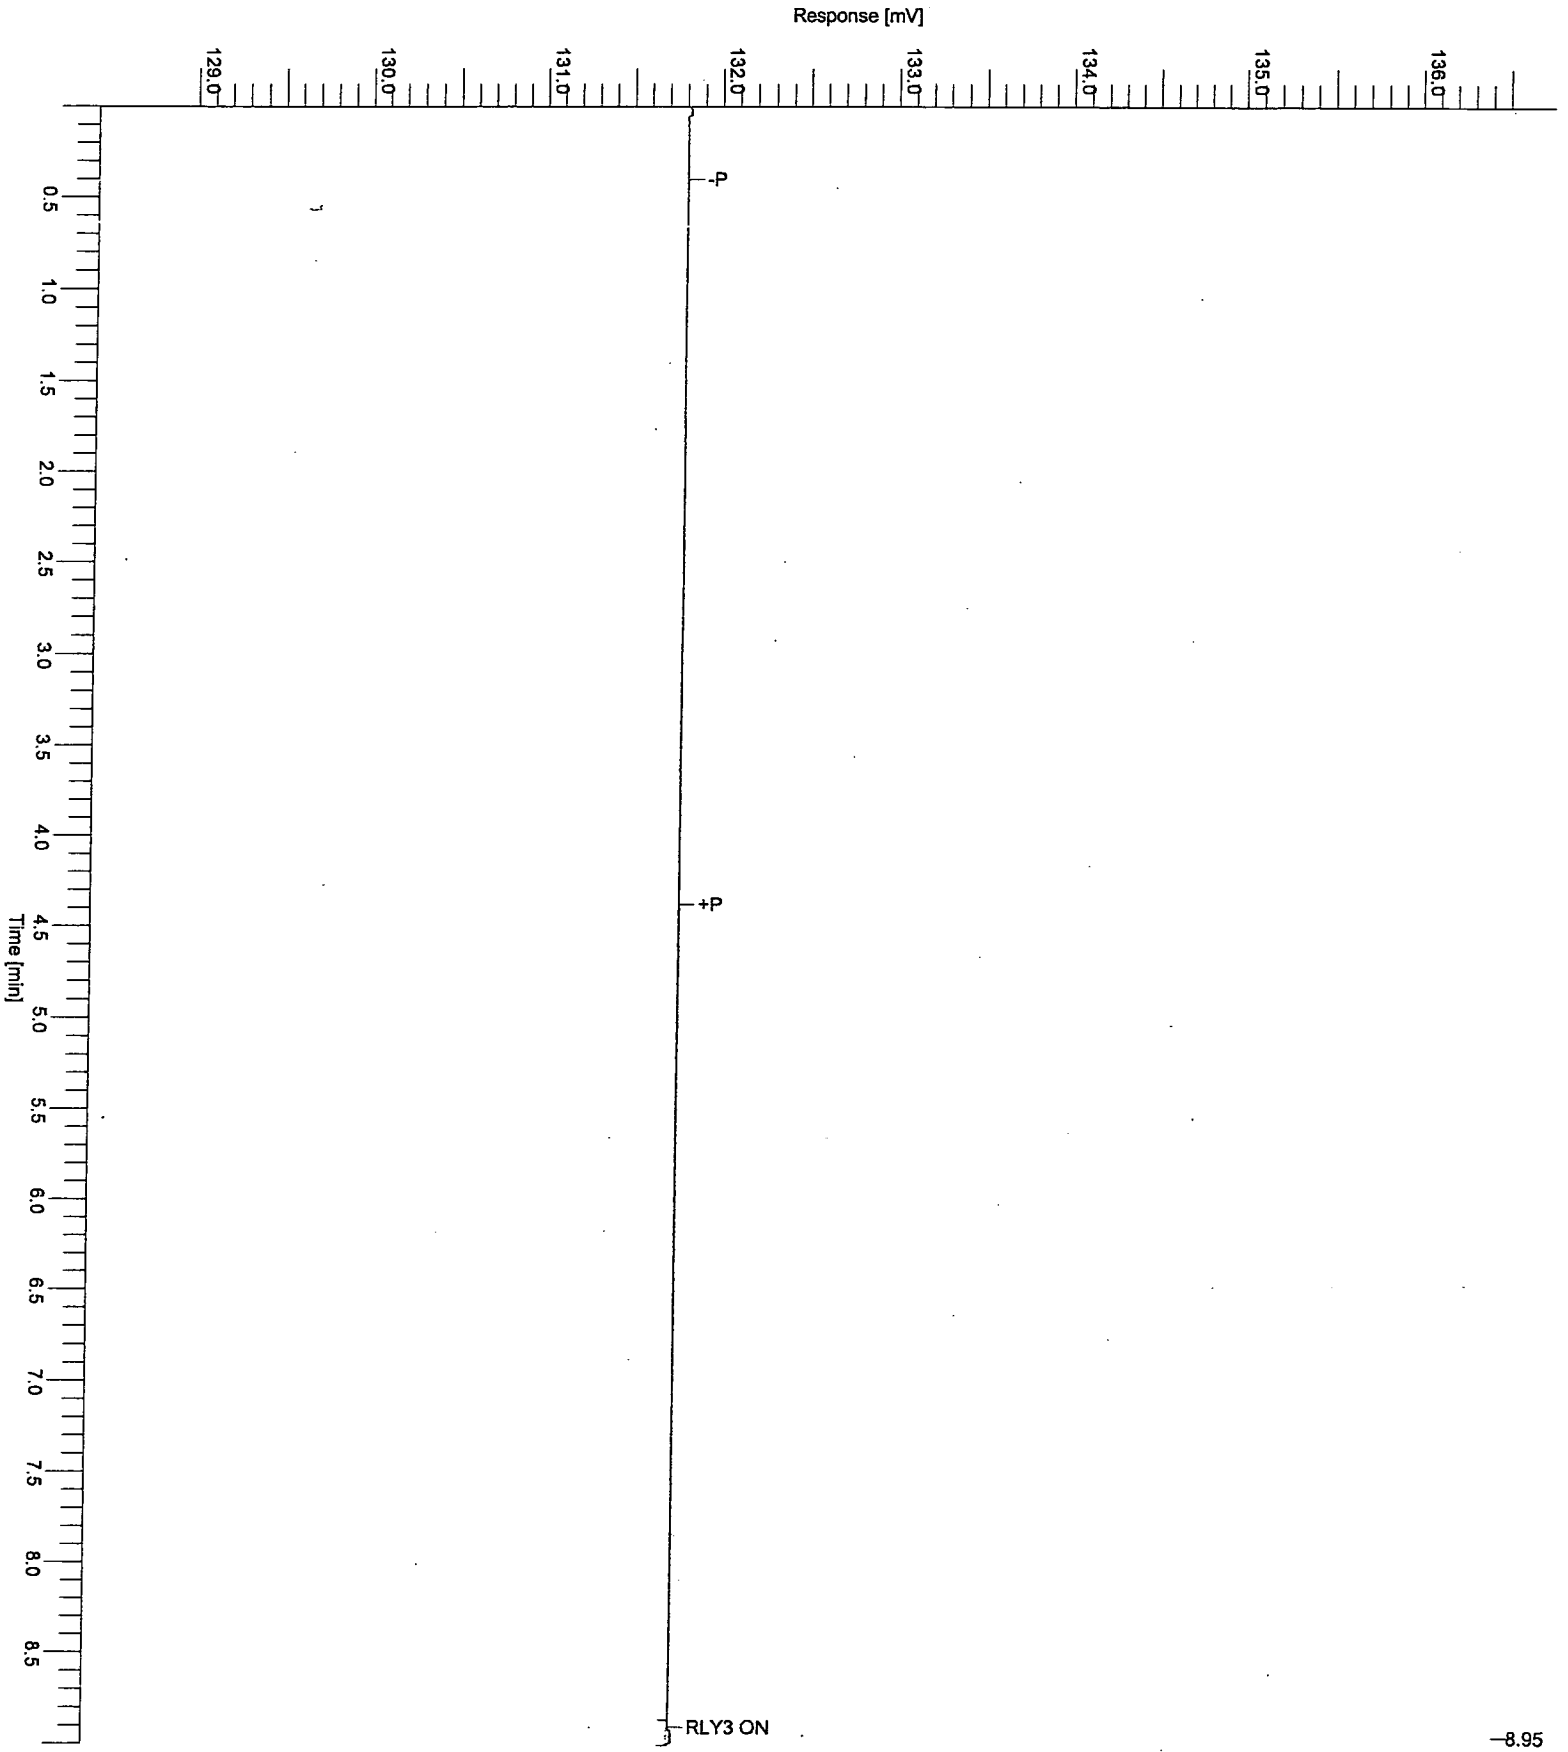

—8.95

Software Version	: 6.2.1.0.106:0106	Date	: 4/28/2007 4:08:10 PM
Reprocess Number	: ic2: 84759		
Operator	: inorg	Sample Name	: 0.3ppb
Sample Number	: 7D28054	Study	: 7040301
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 4/28/2007 3:58:53 PM	Cycle	: 4

Raw Data File : h:\data\ic4\20070428\20070428004.raw
Result File : h:\data\ic4\20070428\20070428004.rst
Inst Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428004.raw
Proc Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428004.rst
Calib Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428004.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070428\20070428.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.964	chrom6	265.90	16.48514	0.4643	0.4643	*
			265.90	16.48514	0.4643	0.4643	

* Warning – uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070428\20070428004.TX0

Chromatogram

Sample Name : 0.3ppb Sample #: 7D28054 Page 1 of 1
FileName : h:\data\ic4\20070428\20070428004.raw
Date : 4/28/2007 4:08:15 PM
Method : chr6qd19a.mth Time of Injection: 4/28/2007 3:58:53 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

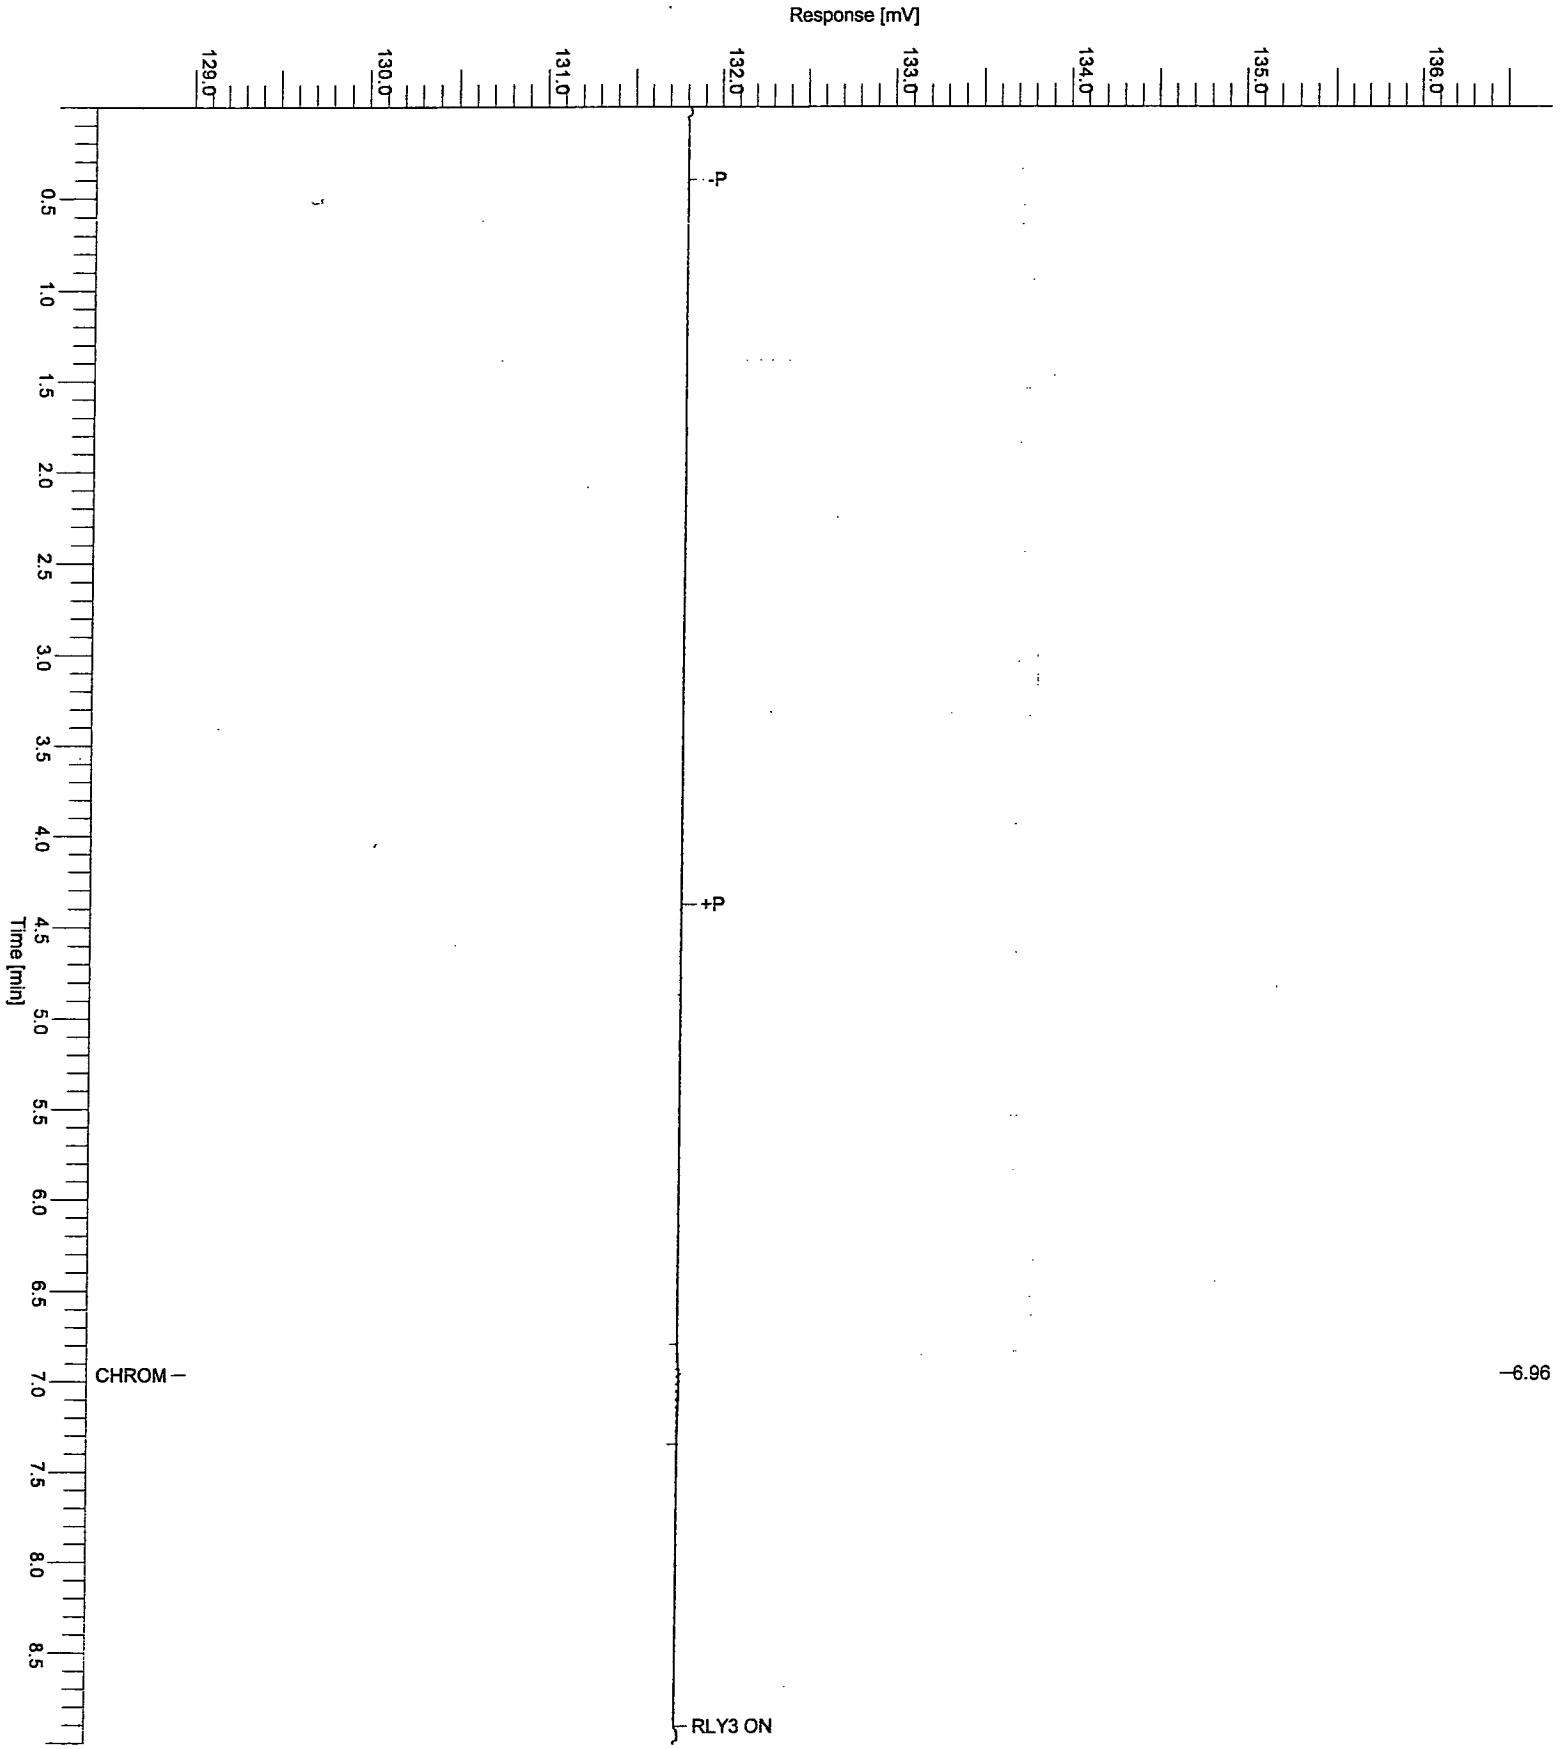

Software Version	: 6.2.1.0.106:0106	Date	: 4/28/2007 4:19:16 PM
Reprocess Number	: ic2: 84761		
Operator	: inorg	Sample Name	: 1.0ppb
Sample Number	: 7D28054	Study	: 7040301
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 4/28/2007 4:09:59 PM	Cycle	: 5

Raw Data File : h:\data\ic4\20070428\20070428005.raw
Result File : h:\data\ic4\20070428\20070428005.rst
Inst Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428005.raw
Proc Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428005.rst
Calib Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428005.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070428\20070428.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.989	chrom6	779.65	37.91797	1.2832	1.2832	*
			779.65	37.91797	1.2832	1.2832	

* Warning -- uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070428\20070428005.TX0

Chromatogram

Sample Name : 1.0ppb Sample #: 7D28054 Page 1 of 1
FileName : h:\data\ic4\20070428\20070428005.raw
Date : 4/28/2007 4:19:21 PM
Method : chr6qd19a.mth Time of Injection: 4/28/2007 4:09:59 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

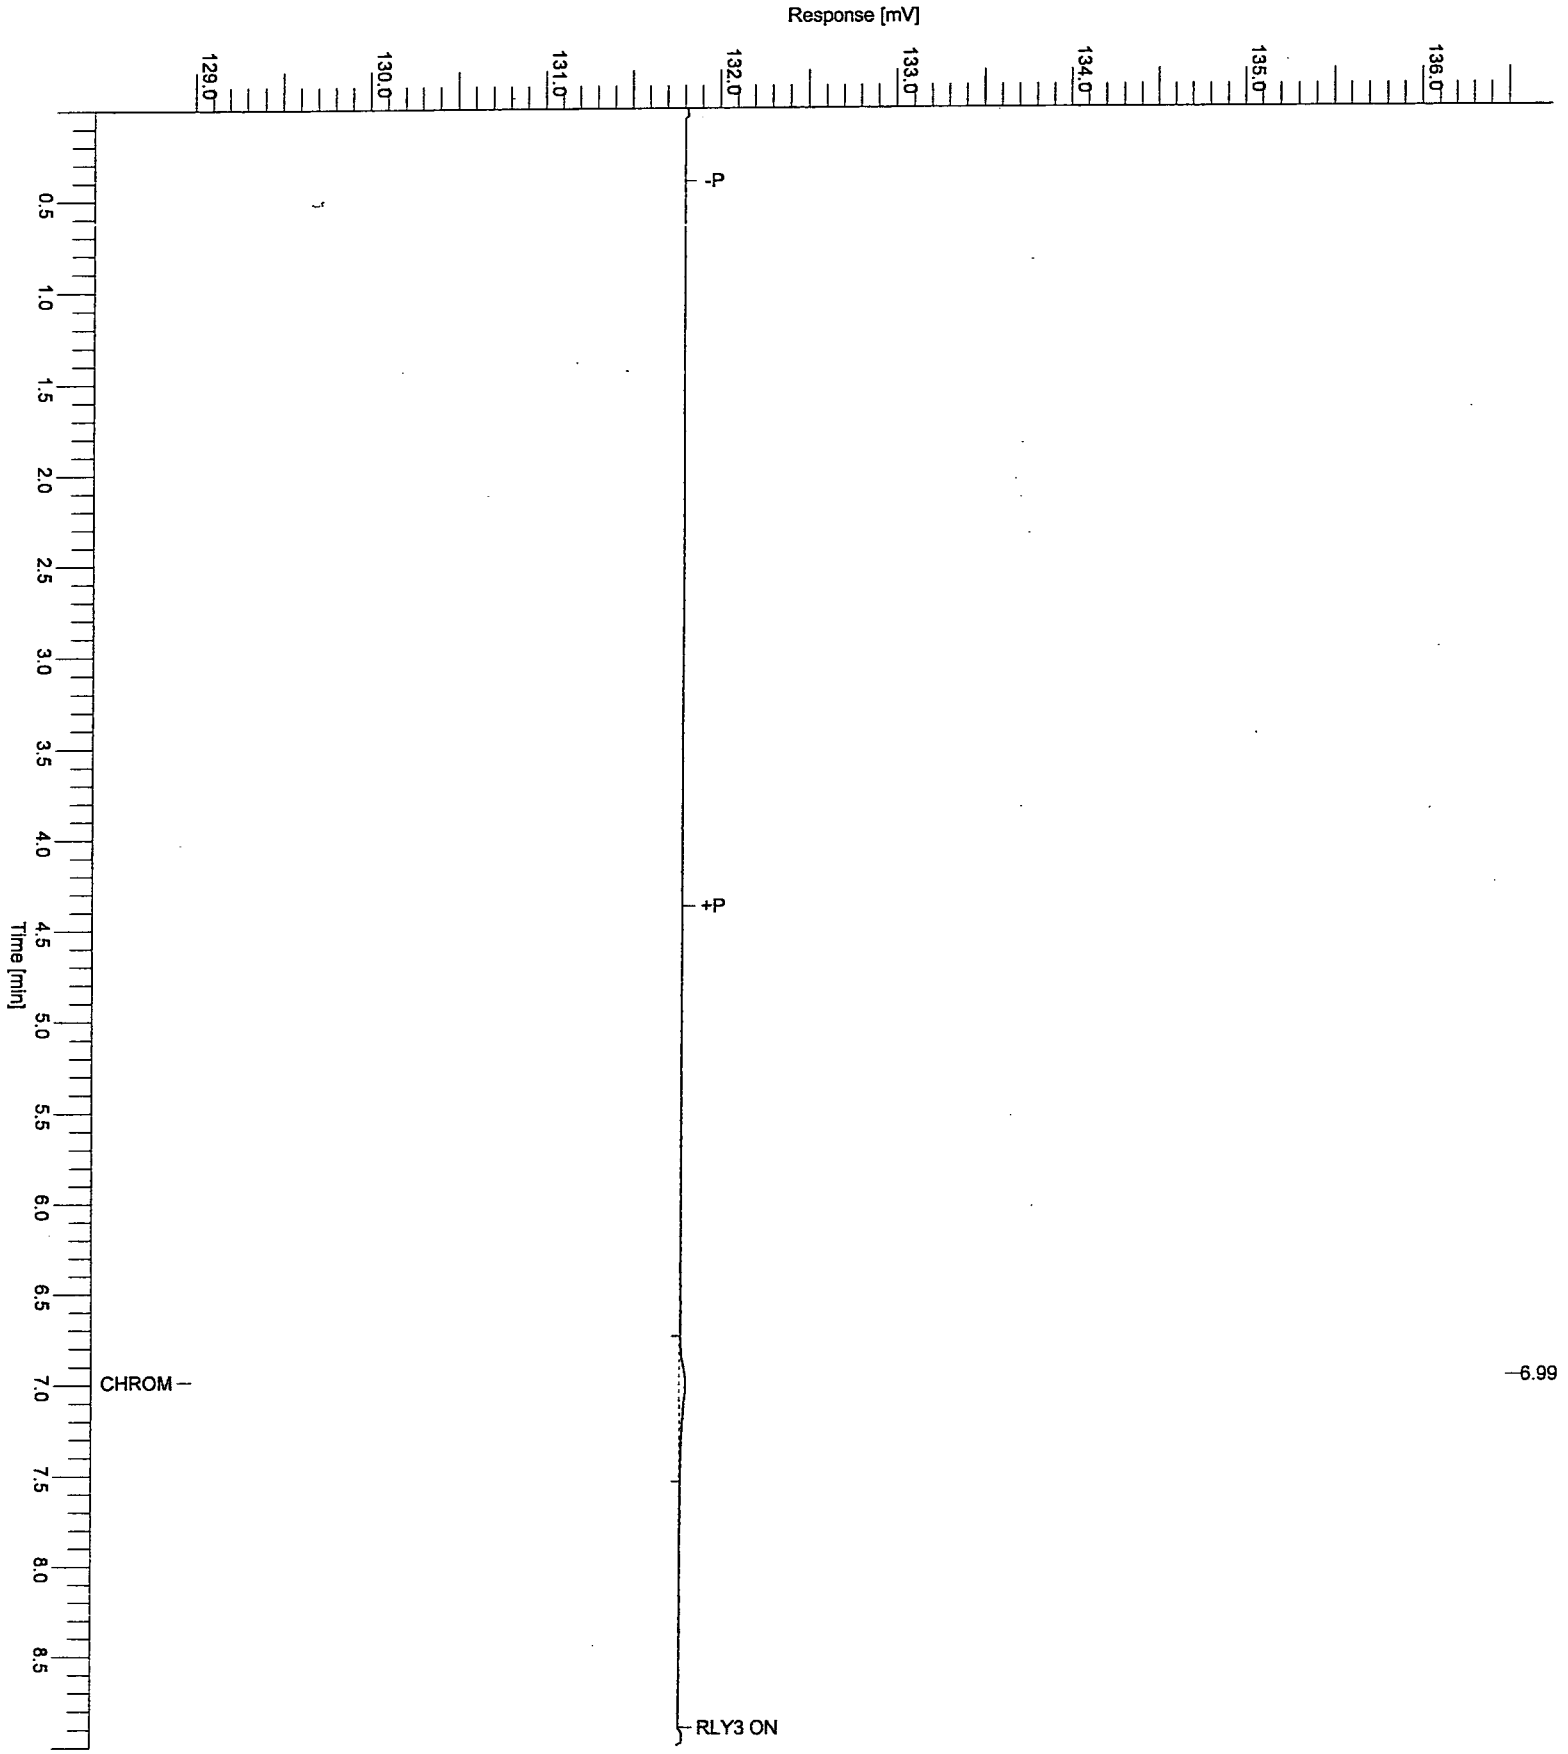

Software Version	: 6.2.1.0.106:0106	Date	: 4/28/2007 4:30:30 PM
Reprocess Number	: ic2: 84762		
Operator	: inorg	Sample Name	: 5.0ppb
Sample Number	: 7D28054	Study	: 7040301
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 4/28/2007 4:21:06 PM	Cycle	: 6

Raw Data File : h:\data\ic4\20070428\20070428006.raw
Result File : h:\data\ic4\20070428\20070428006.rst
Inst Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428006.raw
Proc Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428006.rst
Calib Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428006.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070428\20070428.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	7.010	chrom6	3317.80	166.70604	6.2035	6.2035	*
			3317.80	166.70604	6.2035	6.2035	

* Warning – uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070428\20070428006.TX0

Chromatogram

Sample Name : 5.0ppb
Sample #: 7D28054

FileName : h:\data\ic4\20070428\20070428006.raw
Date : 4/28/2007 4:30:36 PM
Method : chr6qd19a.mth
Time of Injection: 4/28/2007 4:21:06 PM
Start Time : 0.00 min
End Time : 9.00 min
Low Point : 129.00 mV
High Point : 136.50 mV
Plot Offset: 129.00 mV
Plot Scale: 7.5 mV

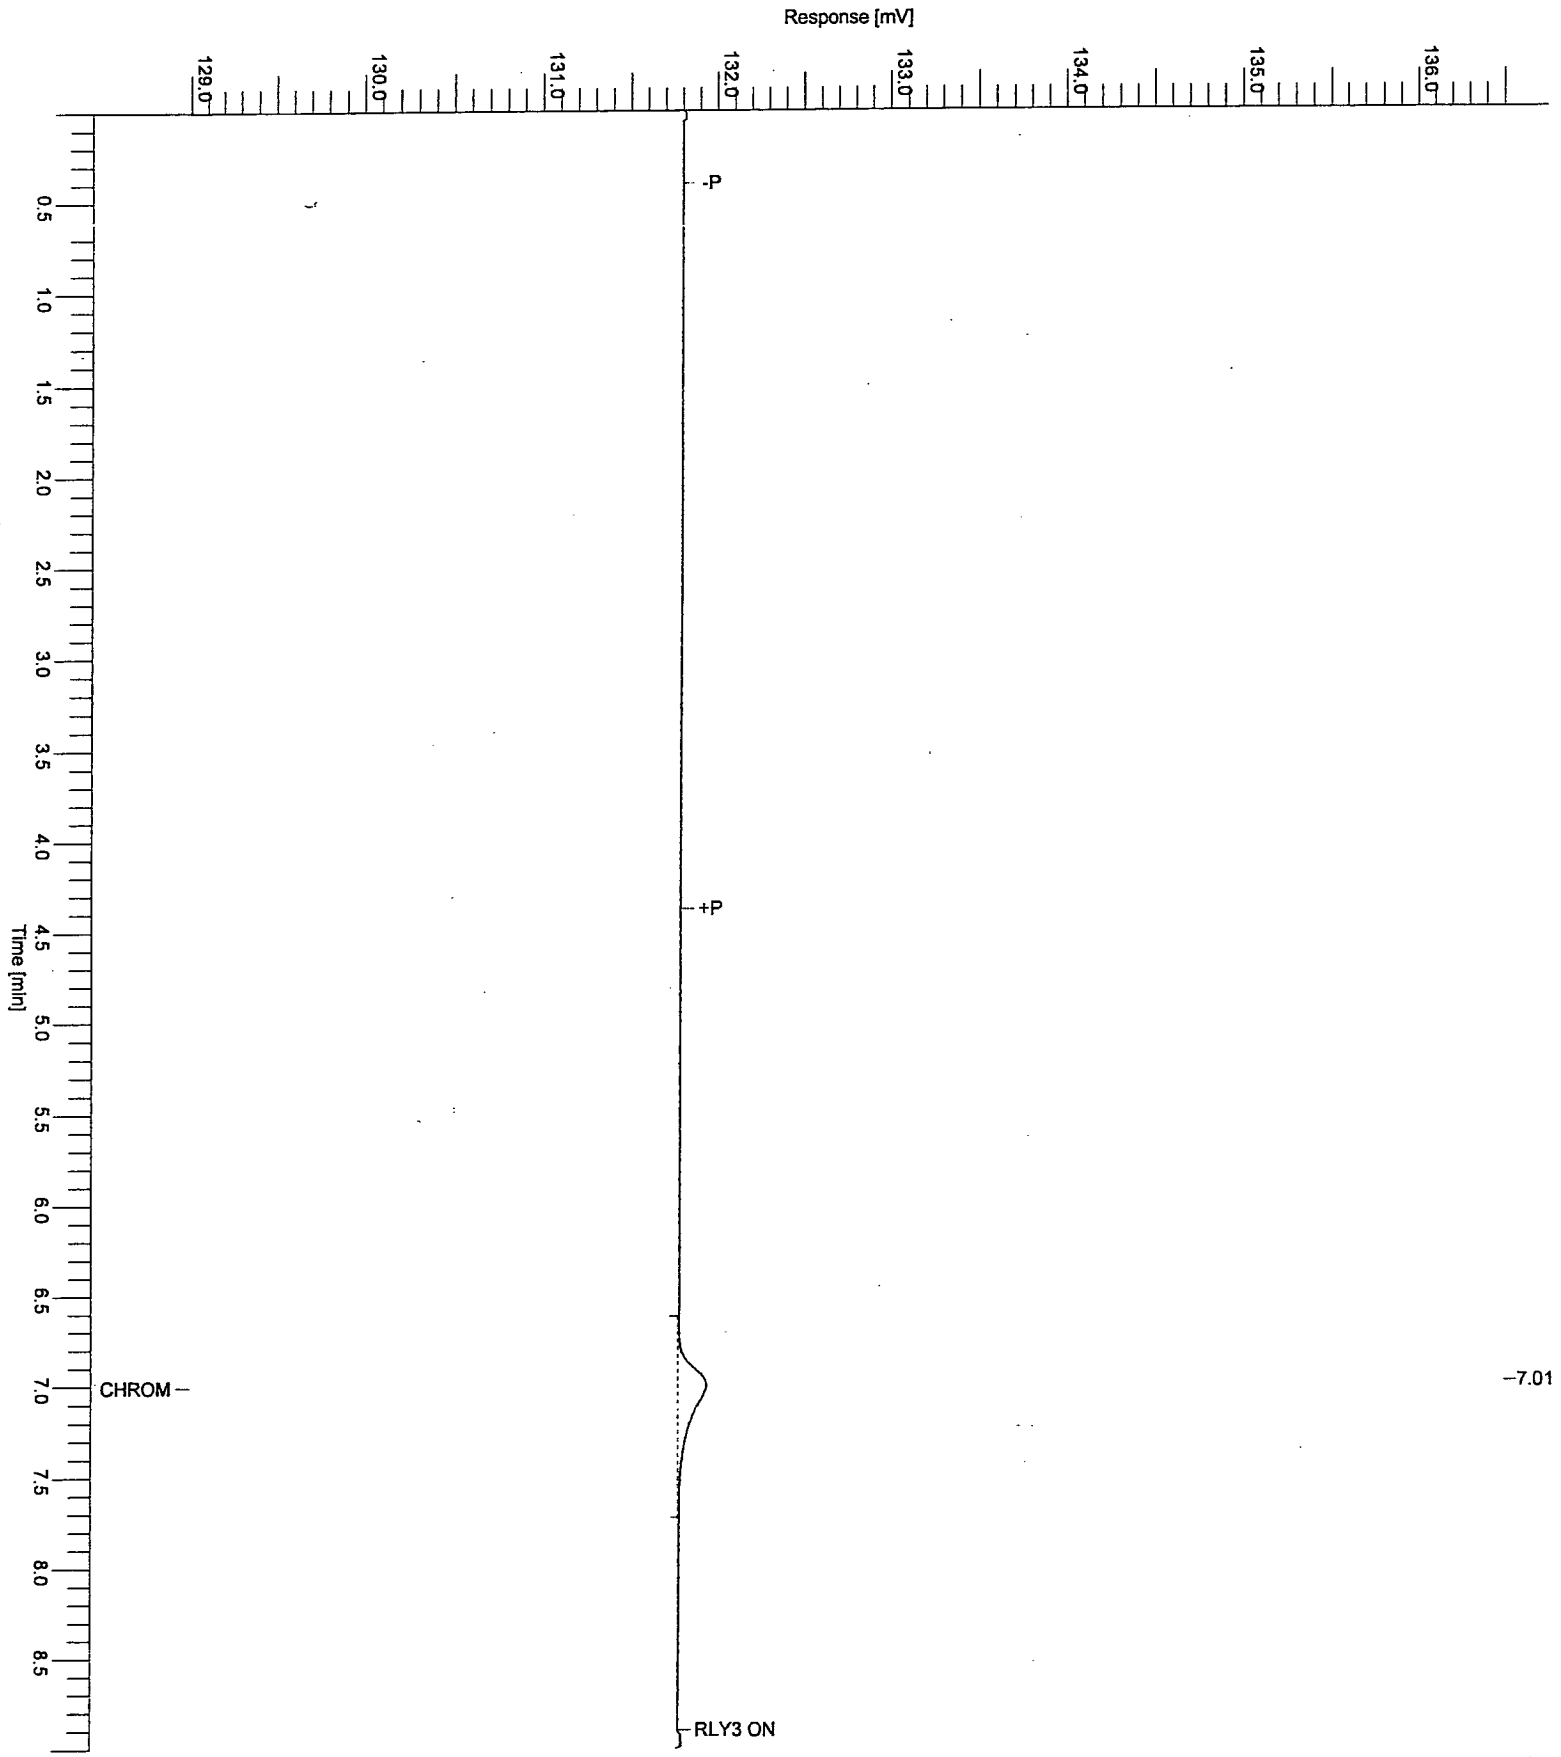

Software Version	: 6.2.1.0.106:0106	Date	: 4/28/2007 4:41:27 PM
Reprocess Number	: ic2: 84764		
Operator	: inorg	Sample Name	: 10ppb
Sample Number	: 7D28054	Study	: 7040301
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 4/28/2007 4:32:12 PM	Cycle	: 7

Raw Data File : h:\data\ic4\20070428\20070428007.raw
Result File : h:\data\ic4\20070428\20070428007.rst
Inst Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428007.raw
Proc Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428007.rst
Calib Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428007.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070428\20070428.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	7.021	chrom6	5521.80	312.29167	11.7655	11.7655	*
			5521.80	312.29167	11.7655	11.7655	

* Warning – uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070428\20070428007.TX0

Chromatogram

Sample Name : 10ppb Sample #: 7D28054 Page 1 of 1
FileName : h:\data\ic4\20070428\20070428007.raw
Date : 4/28/2007 4:41:33 PM
Method : chr6qd19a.mth Time of Injection: 4/28/2007 4:32:12 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

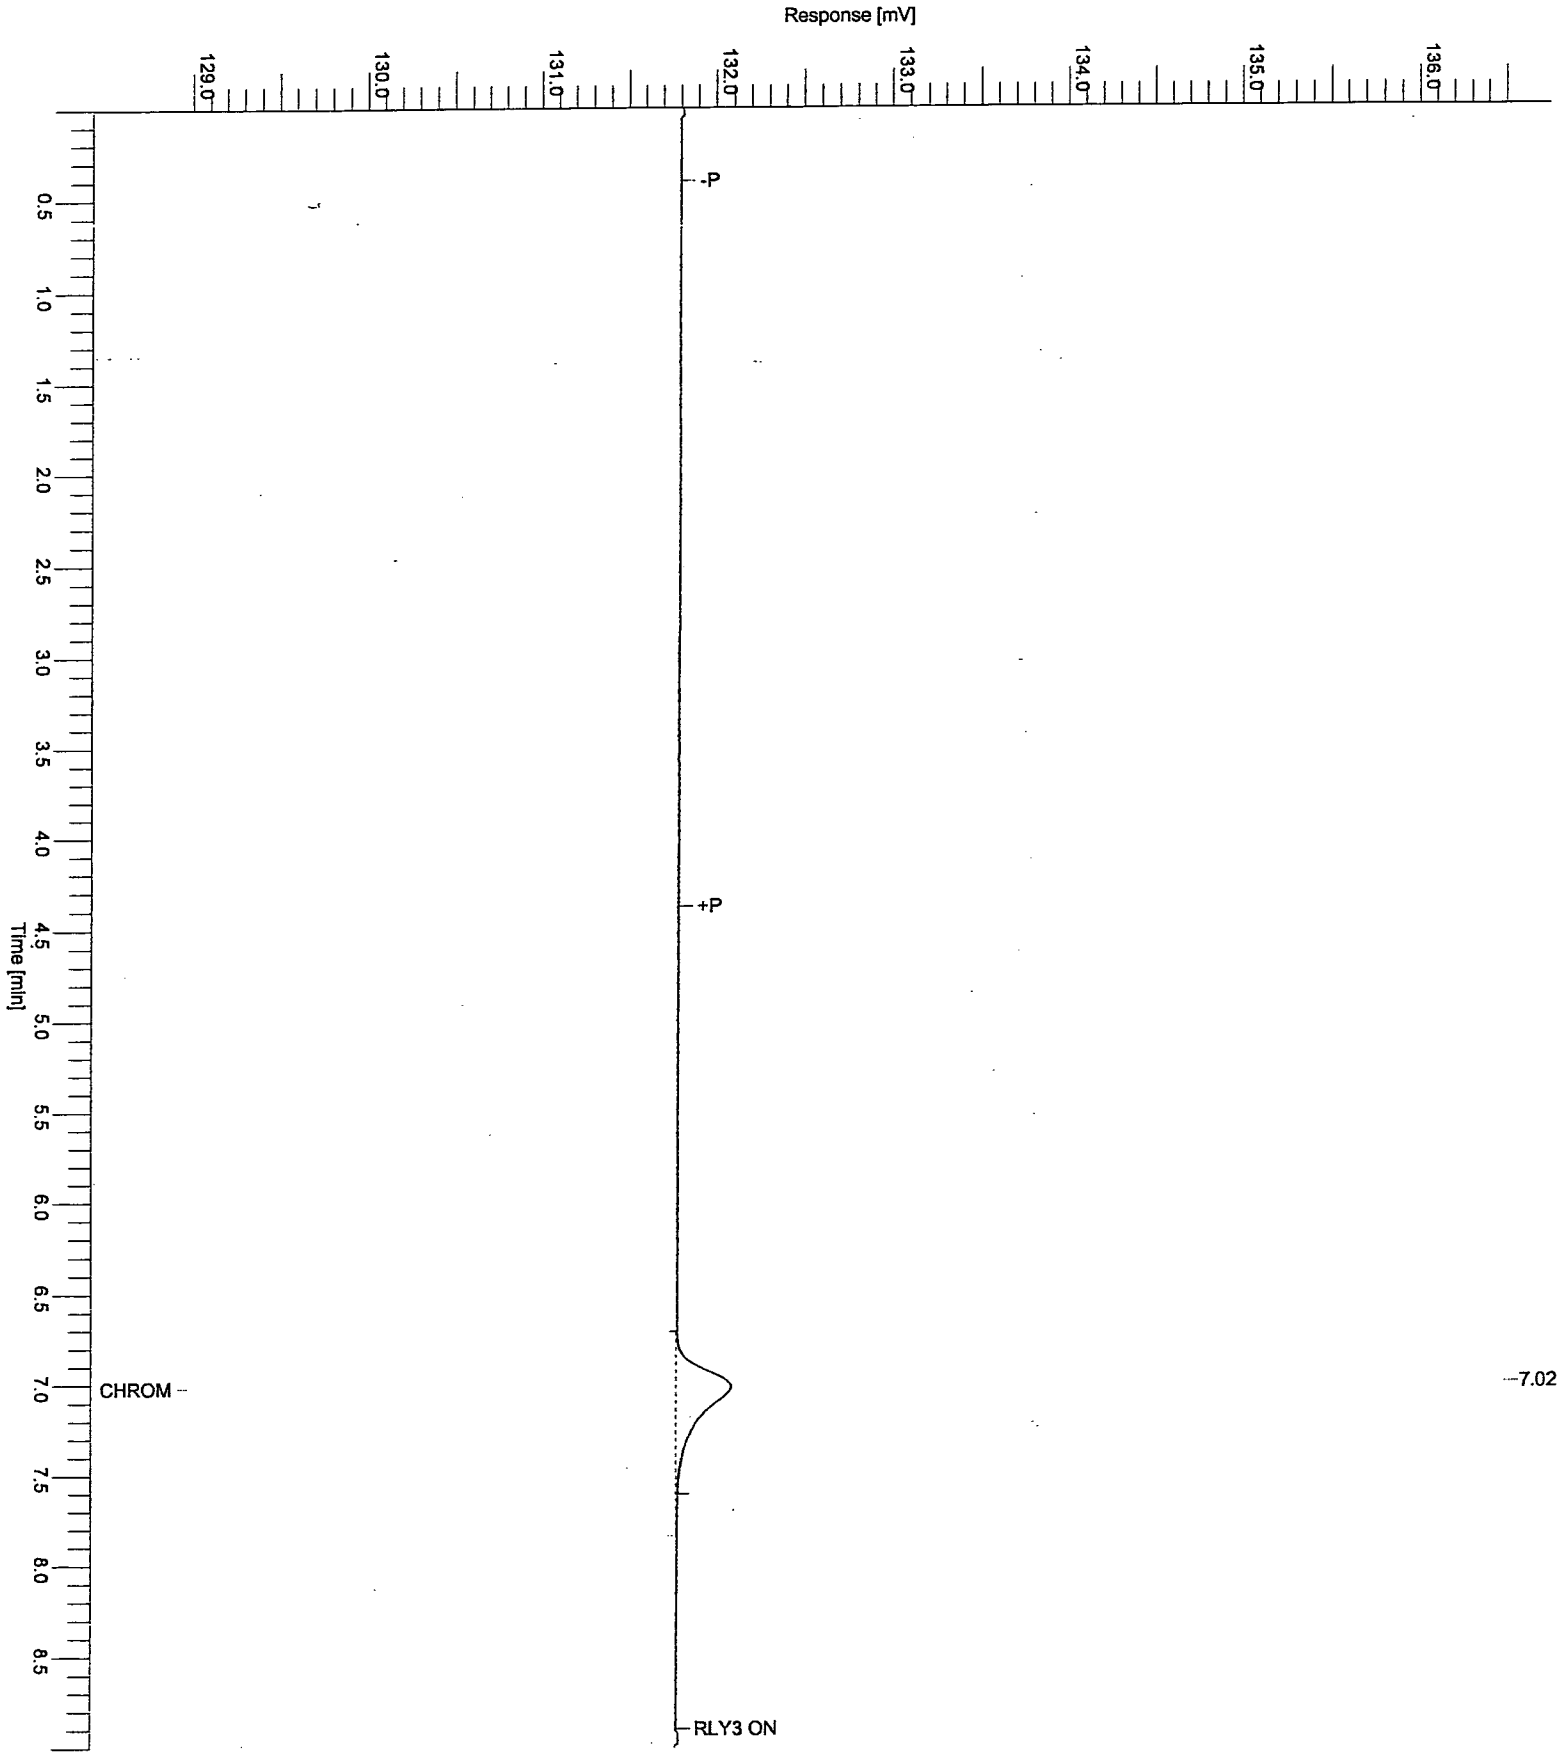

Software Version	: 6.2.1.0.106:0106	Date	: 4/28/2007 4:52:33 PM
Reprocess Number	: ic2: 84765		
Operator	: inorg	Sample Name	: 25ppb
Sample Number	: 7D28054	Study	: 7040301
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 4/28/2007 4:43:17 PM	Cycle	: 8

Raw Data File : h:\data\ic4\20070428\20070428008.raw
Result File : h:\data\ic4\20070428\20070428008.rst
Inst Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428008.raw
Proc Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428008.rst
Calib Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428008.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070428\20070428.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	7.034	chrom6	14074.45	786.14700	29.8689	29.8689	*
			14074.45	786.14700	29.8689	29.8689	

* Warning -- uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070428\20070428008.TX0

Chromatogram

Sample Name : 25ppb
Sample #: 7D28054

FileName : h:\data\ic4\20070428\20070428008.raw
Date : 4/28/2007 4:52:38 PM
Method : chr6qd19a.mth
Time of Injection: 4/28/2007 4:43:17 PM
Start Time : 0.00 min
End Time : 9.00 min
Low Point : 129.00 mV
High Point : 136.50 mV
Plot Offset: 129.00 mV
Plot Scale: 7.5 mV

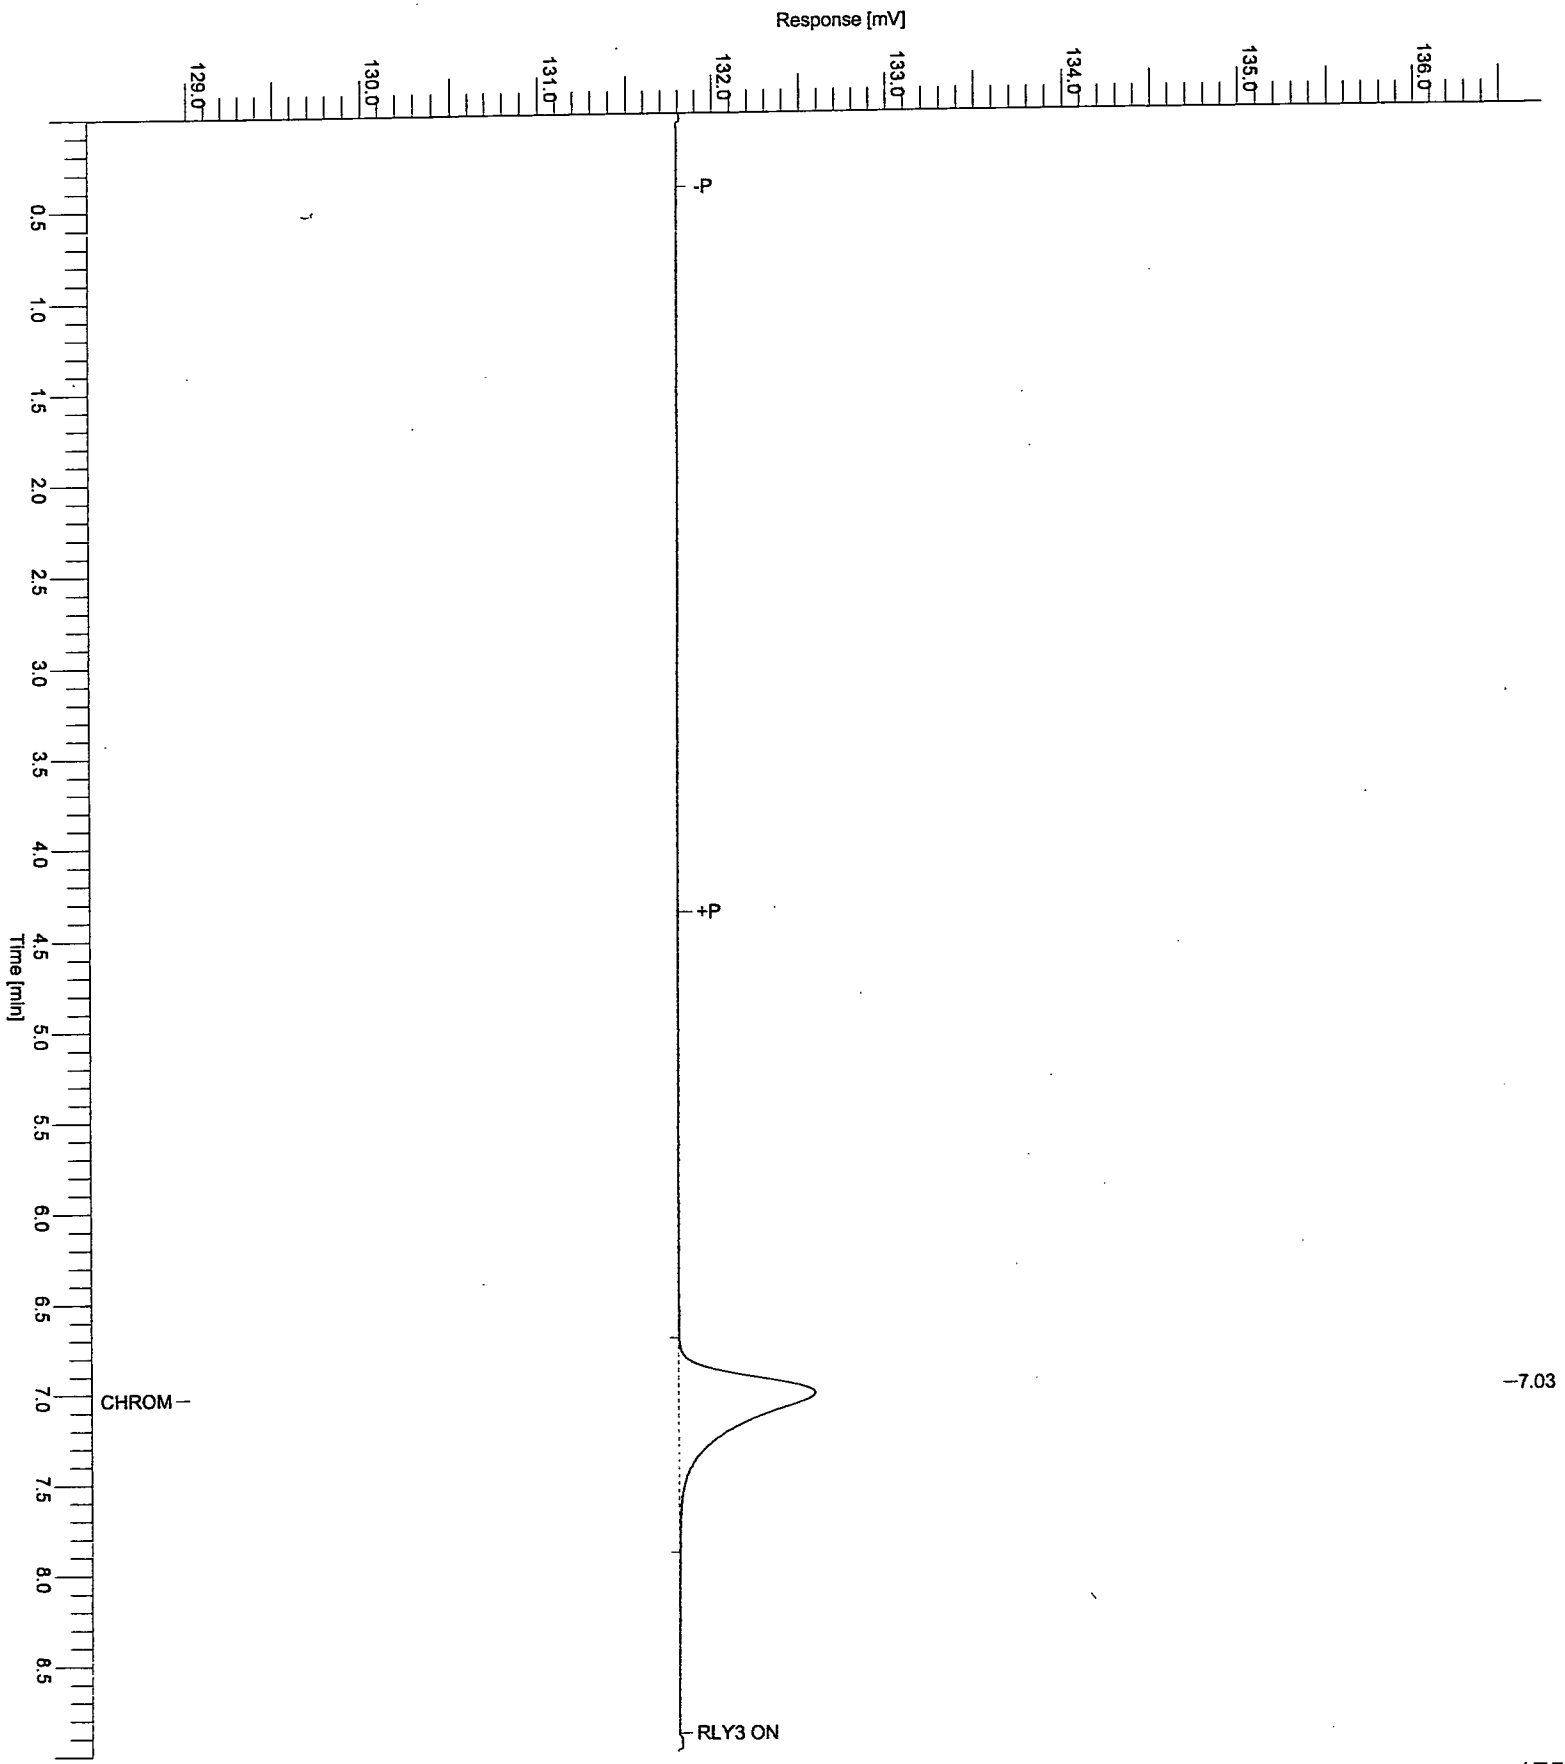

Software Version	: 6.2.1.0.106:0106	Date	: 4/28/2007 5:03:42 PM
Reprocess Number	: ic2: 84767		
Operator	: inorg	Sample Name	: 50ppb
Sample Number	: 7D28054	Study	: 7040301
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 4/28/2007 4:54:24 PM	Cycle	: 9

Raw Data File : h:\data\ic4\20070428\20070428009.raw
Result File : h:\data\ic4\20070428\20070428009.rst
Inst Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428009.raw
Proc Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428009.rst
Calib Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428009.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070428\20070428.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	7.014	chrom6	28618.20	1.601e+03	61.0121	61.0121	*
			28618.20	1.601e+03	61.0121	61.0121	

* Warning -- uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070428\20070428009.TX0

Chromatogram

Sample Name : 50ppb
Sample #: 7D28054

FileName : h:\data\ic4\20070428\20070428009.raw
Date : 4/28/2007 5:03:47 PM
Method : chr6qd19a.mth
Time of Injection: 4/28/2007 4:54:24 PM
Start Time : 0.00 min
End Time : 9.00 min
Low Point : 129.00 mV
High Point : 136.50 mV
Plot Offset: 129.00 mV
Plot Scale: 7.5 mV

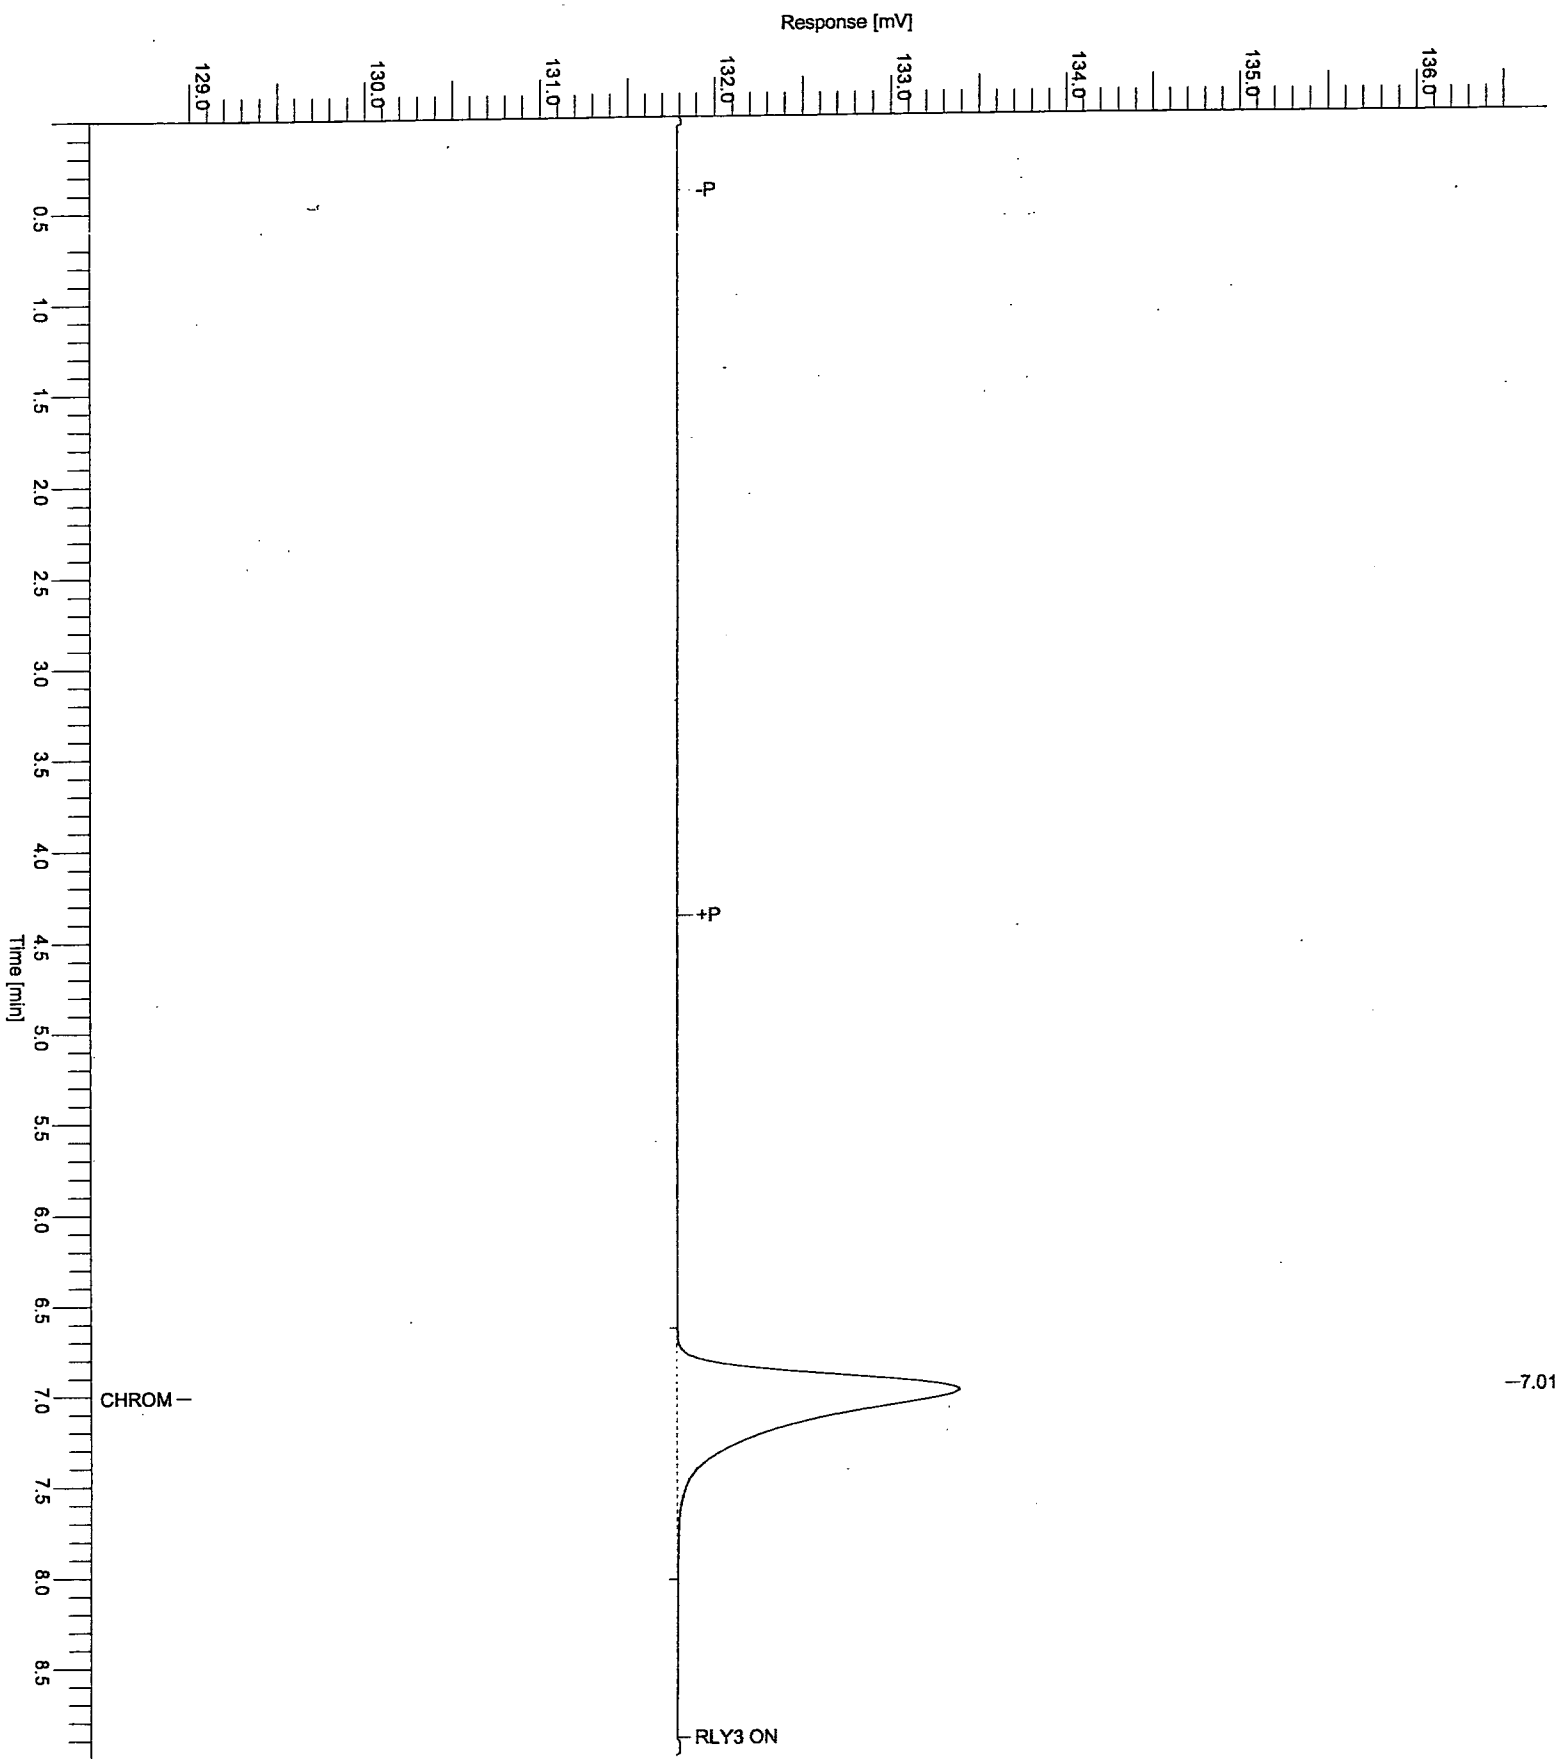

Software Version	: 6.2.1.0.106:0106	Date	: 4/28/2007 5:14:45 PM
Reprocess Number	: ic2: 84769		
Operator	: inorg	Sample Name	: 75ppb
Sample Number	: 7D28054	Study	: 7040301
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 4/28/2007 5:05:31 PM	Cycle	: 10

Raw Data File : h:\data\ic4\20070428\20070428010.raw
Result File : h:\data\ic4\20070428\20070428010.rst
Inst Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428010.raw
Proc Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428010.rst
Calib Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428010.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070428\20070428.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	7.019	chrom6	42355.20	2.395e+03	91.3419	91.3419	*
			42355.20	2.395e+03	91.3419	91.3419	

* Warning – uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070428\20070428010.TX0

Chromatogram

Sample Name : 75ppb
Sample #: 7D28054

FileName : h:\data\ic4\20070428\20070428010.raw
Date : 4/28/2007 5:14:50 PM
Method : chr6qd19a.mth
Time of Injection: 4/28/2007 5:05:31 PM
Start Time : 0.00 min
End Time : 9.00 min
Low Point : 129.00 mV
High Point : 136.50 mV
Plot Offset: 129.00 mV
Plot Scale: 7.5 mV

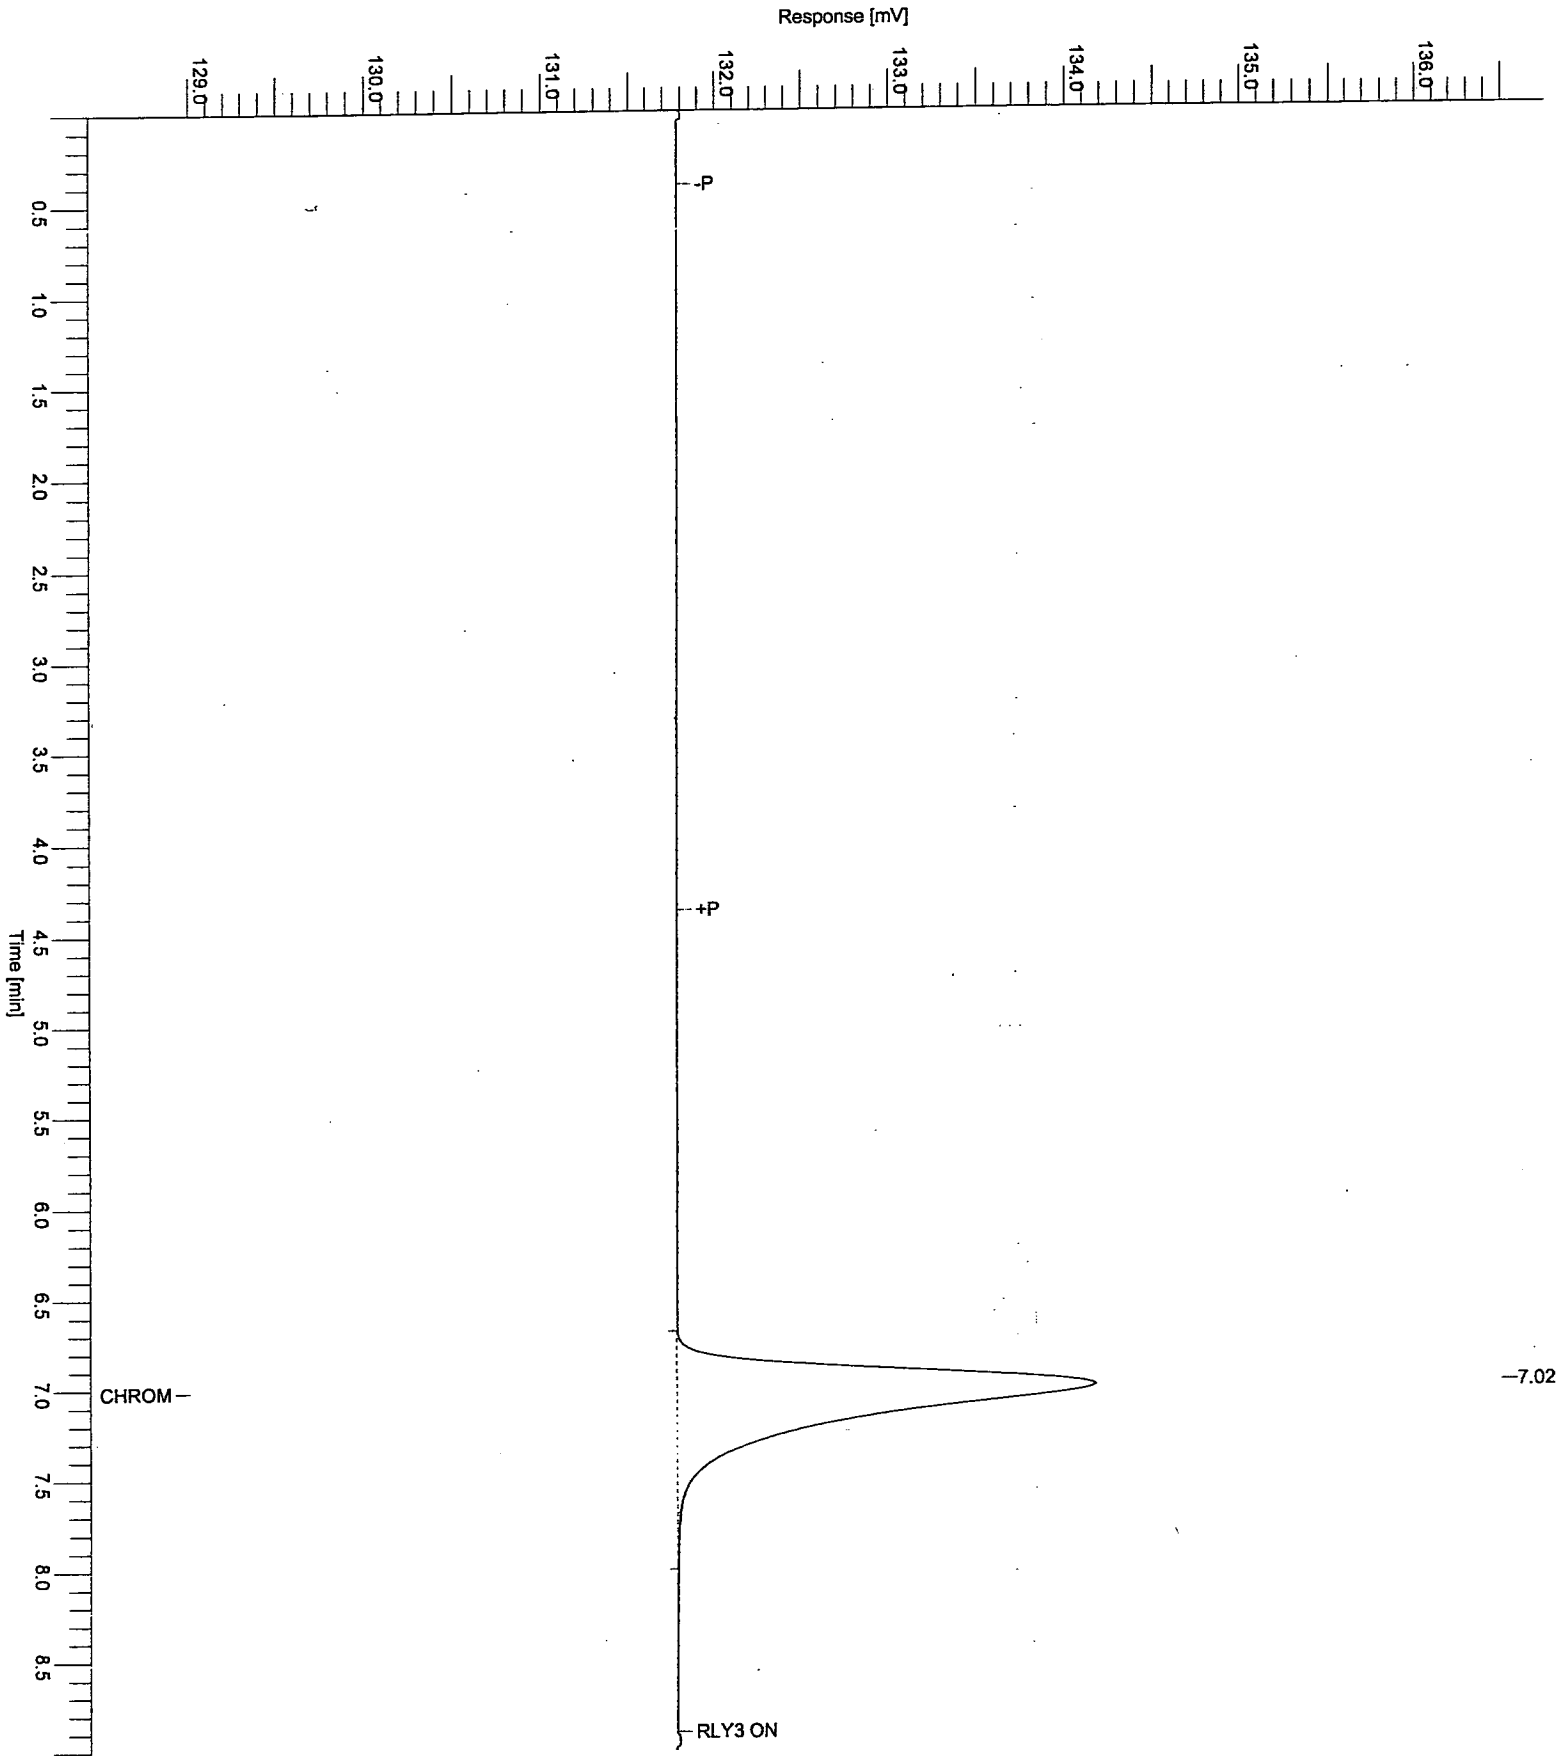

Software Version	: 6.2.1.0.106:0106	Date	: 4/30/2007 11:35:11 AM
Reprocess Number	: irv-inorgwet4: 4719		
Operator	: inorg	Sample Name	: ICV
Sample Number	: 7D28054	Study	: 7040302
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 4/28/2007 5:16:37 PM	Cycle	: 1

Raw Data File : h:\data\ic4\20070428\20070428011.raw <Modified>
Result File : h:\data\ic4\20070428\20070428011.rst
Inst Method : h:\data\ic4\chr6qd19a from h:\data\ic4\20070428\20070428011.raw
Proc Method : h:\data\ic4\chr6qd30.mth from h:\data\ic4\20070428\20070428011.rst
Calib Method : h:\data\ic4\chr6qd30.mth from h:\data\ic4\20070428\20070428011.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070428\20070428.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	7.049	chrom6	27618.00	1.572e+03	49.2492	49.2492	*
			27618.00	1.572e+03	49.2492	49.2492	

* Warning – uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070428\20070428011.TX0

Chromatogram

Sample Name : ICV Sample #: 7D28054 Page 1 of 1
FileName : h:\data\ic4\20070428\20070428011.raw
Date : 4/30/2007 11:35:12 AM
Method : chr6qd19a Time of Injection: 4/28/2007 5:16:37 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

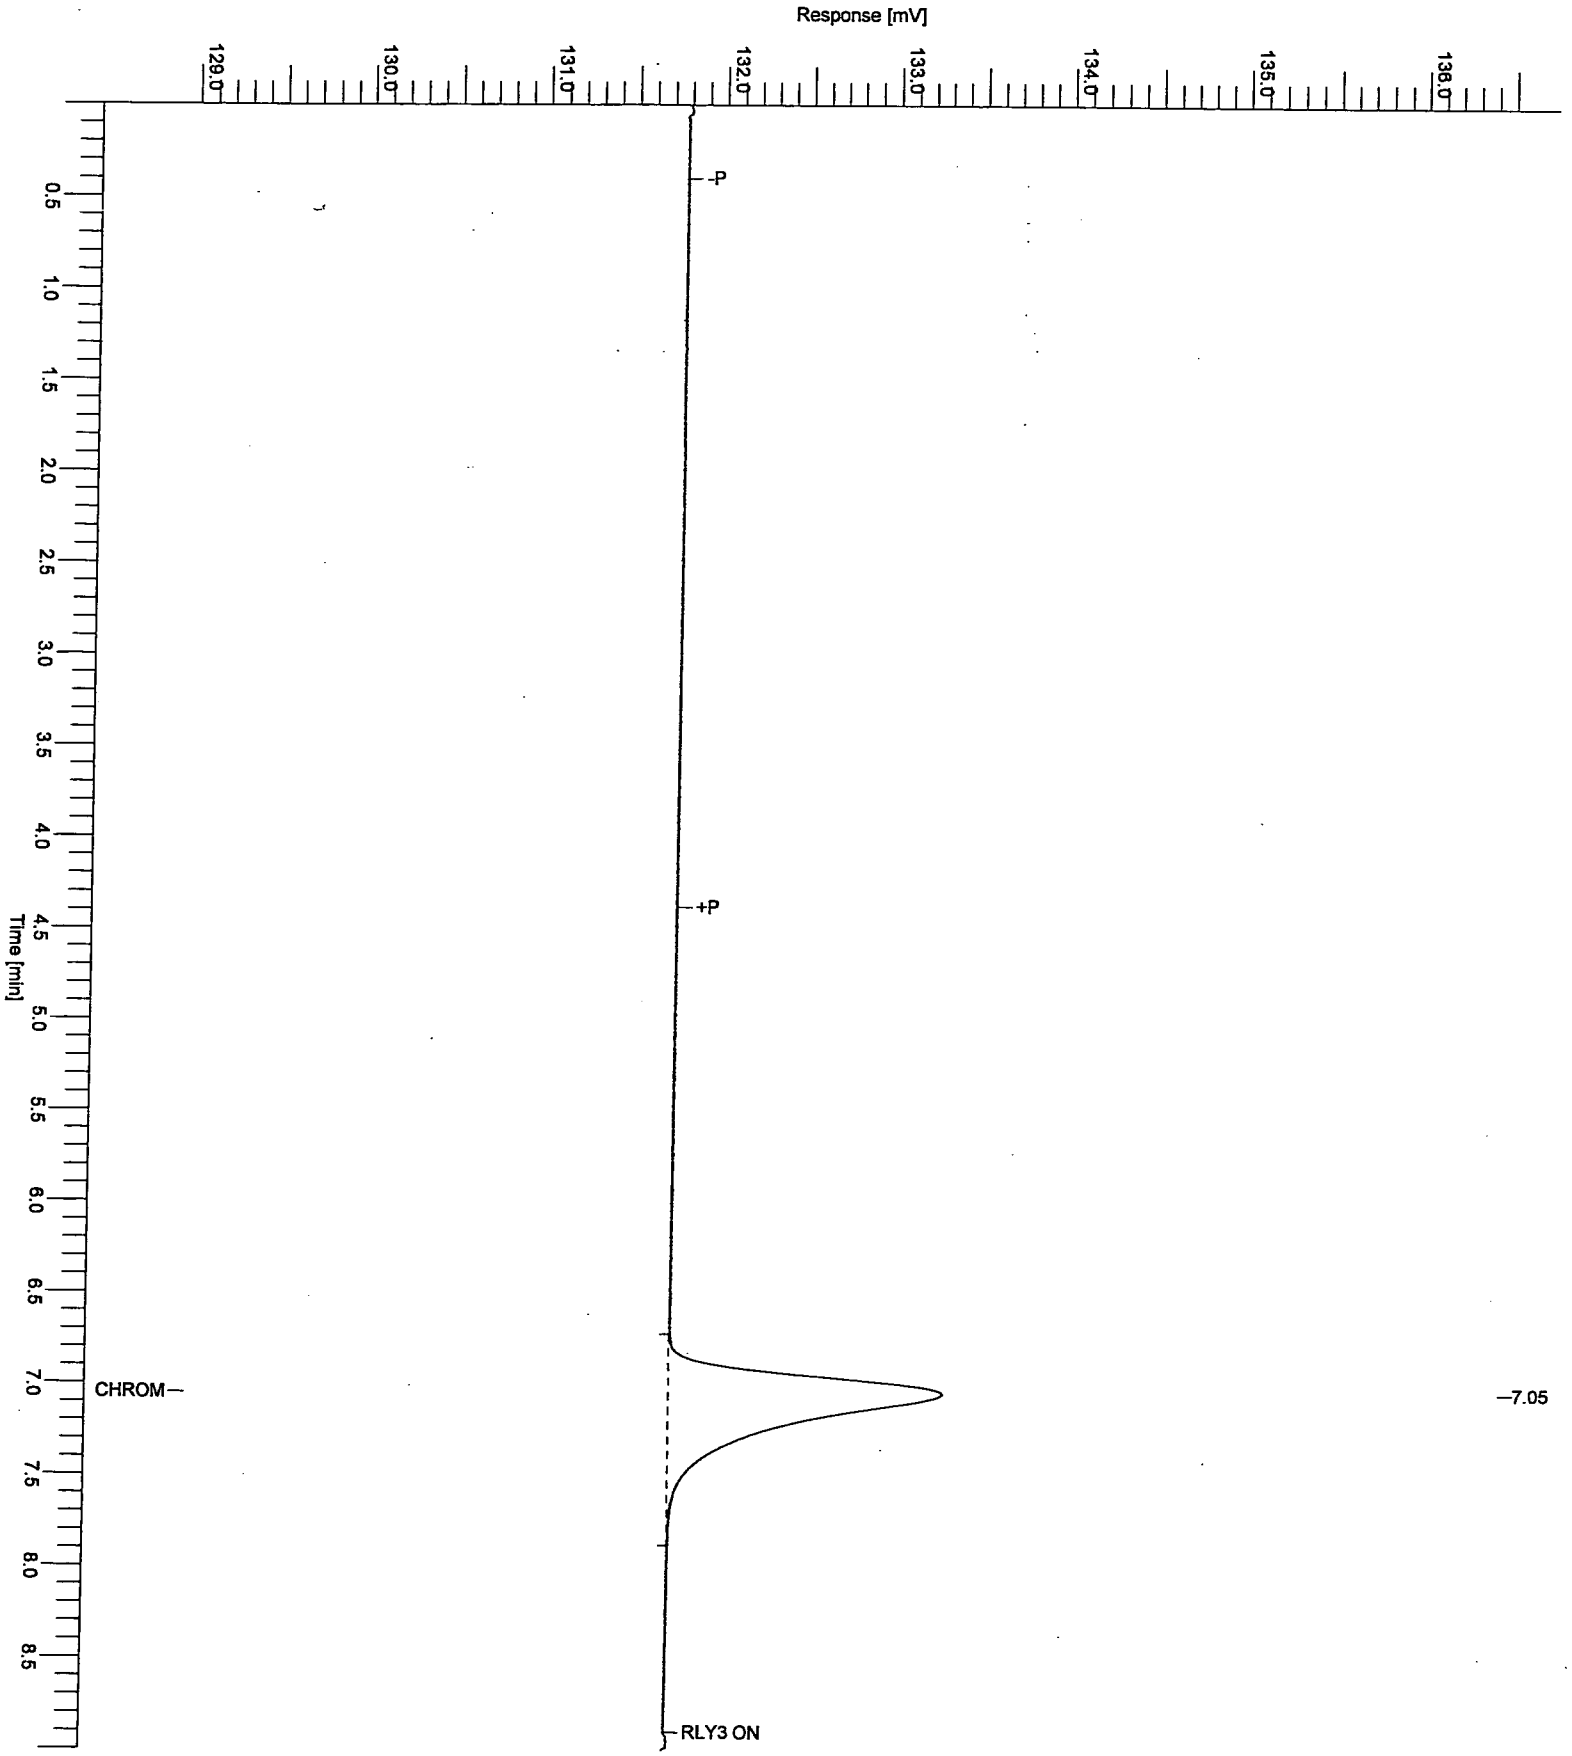

DAILY DATA CHECKLIST

EPA 7199 & 218.6 – Hexavalent Chromium by IC

Analyst:	IM/SLa	2nd Level Review:	W
Analysis Date:	7/17/07	Date:	7/25/07
IC #:	IC4	Original Calibration date:	4/30/07
Method used:	218.6 & 7199	Original Calibration file #:	Chrgd 30.MTH
QC Batches:	7G17075, 7G16086		

Analyst Rev	2nd Level Rev	
✓	✓	New sequence file created for each day of analysis
✓	✓	Daily IPC: %REC = 90 - 110 for EPA 7199
✓	✓	%REC = 95 - 105 for EPA 218.6
✓	✓	ICB/CCB: After IPC/CCB and < RL
✓	✓	CCV: Every 10 samples and at end of run. %REC = 90 - 110 for EPA7199
✓	✓	%REC = 95 - 105 for EPA 218.6
✓	✓	Method Blank: Every batch of 20 samples or less and < RL
✓	✓	LCS: Every batch of 20 samples or less
✓	✓	• Water samples (EPA 7199 & 218.6): %REC = 90-110 % or in-house limits
✓		• Soil samples (EPA 7199): in-house limits
✓	✓	**MS/MSD**: EPA 7199 : every 20 samples or less
✓		EPA 218.6: 1MS every 10 samples and 1MSD every 20 samples or less
✓		• EPA 7199: %REC (soluble Cr6) = 75-125% or in-house limits
✓	✓	• EPA 7199: %REC (insoluble Cr6, soil samples) = 75-125% or in-house limits
✓		• EPA 218.6: %REC = 90-110% or in-house limits
✓	✓	All samples adusted to proper pH (9.0-9.5), dilution factors, retention time, integration, peak shape, linear range, transcription errors and frequency between compliant CCV/CCB

Comments:

TotalChrom Sequence File H:\DATA\IC4\20070717\20070717.seq
Printed by : inorg on: 7/18/2007 1:35:42 PM
Created by : inorg on: 7/17/2007 11:38:49 AM
Edited by : inorg on: 7/18/2007 12:01:06 AM
Number of Times Edited : 15
Description:

Sequence File Header Information:

Number of Rows : 189
Instrument Type : 900 Series Intelligent Interface
Injection Type : SINGLE
Raw tokens channel A :
Result tokens channel A :
Modified tokens channel A :
Raw tokens channel B :
Result tokens channel B :
Modified tokens channel B :

Sequence Sample Descriptions - Channel A

Row	Type	Name	Number	Study name	Sample Amt	Sample Vol	Dil Factor	Multiplier	Divisor	Addend	Norm Factor
1	Sample	IB	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
2	Sample	7G17075-BS1	7G17075	7060052	1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
3	Sample	7G17075-BLK1	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
4	Sample	IQG1425-03	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
5	Sample	IQG1425-05	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
6	Sample	IQG1425-06	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
7	Sample	7G17075-MS1	7G17075	IQG1425-03	1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
8	Sample	7G17075-MSD1	7G17075	IQG1425-03	1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
9	Sample	CCV	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
10	Sample	CCB	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
11	Sample	CCV	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
~~12~~	~~Sample~~	~~CCB~~	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
13	Sample	CCB	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
14	Sample	IQG1460-01	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
15	Sample	IQG1460-02	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
16	Sample	IQG1460-03	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
17	Sample	~~IQG1460-04~~	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
18	Sample	IQG1460-05	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
19	Sample	IQG1460-06	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
20	Sample	IQG1460-04	7G17075		1.000000	1.000	10.000000	1.000000	1.000000	0.000000	100.000
21	Sample	CCV	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
22	Sample	CCB	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
23	Sample	7G16086-BS1	7G16086		1.000000	1.000	1.000000	10.000000	1.000000	0.000000	100.000
24	Sample	7G16086-BLK1	7G16086		1.000000	1.000	1.000000	10.000000	1.000000	0.000000	100.000
25	Sample	IQG0958-05	7G16086		1.000000	1.000	1.000000	10.000000	1.000000	0.000000	100.000
26	Sample	7G16086-MS1	7G16086	IQG0958-05	1.000000	1.000	1.000000	10.000000	1.000000	0.000000	100.000
27	Sample	7G16086-MSD1	7G16086	IQG0958-05	1.000000	1.000	1.000000	10.000000	1.000000	0.000000	100.000
28	Sample	IQG0958-06	7G16086		1.000000	1.000	1.000000	10.000000	1.000000	0.000000	100.000
29	Sample	IQG0958-07	7G16086		1.000000	1.000	1.000000	10.000000	1.000000	0.000000	100.000
30	Sample	IQG0958-08	7G16086		1.000000	1.000	1.000000	10.000000	1.000000	0.000000	100.000
31	Sample	IQG0958-14	7G16086		1.000000	1.000	5.000000	10.000000	1.000000	0.000000	100.000
32	Sample	IQG0958-15	7G16086		1.000000	1.000	1.000000	10.000000	1.000000	0.000000	100.000
33	Sample	IQG0958-16	7G16086		1.000000	1.000	10.000000	10.000000	1.000000	0.000000	100.000
34	Sample	CCV	7G16086		1.000000	1.000	1.000000	10.000000	1.000000	0.000000	100.000
35	Sample	CCB	7G16086		1.000000	1.000	1.000000	10.000000	1.000000	0.000000	100.000
36	Sample	IQG0958-17	7G16086		1.000000	1.000	1.000000	10.000000	1.000000	0.000000	100.000
37	Sample	IQG0958-18	7G16086		1.000000	1.000	1.000000	10.000000	1.000000	0.000000	100.000
38	Sample	IQG0958-19	7G16086		1.000000	1.000	5.000000	10.000000	1.000000	0.000000	100.000
39	Sample	IQG0958-19	7G16086		1.000000	1.000	50.000000	10.000000	1.000000	0.000000	100.000
40	Sample	CCV	7G16086		1.000000	1.000	1.000000	10.000000	1.000000	0.000000	100.000
41	Sample	CCB	7G16086		1.000000	1.000	1.000000	10.000000	1.000000	0.000000	100.000
42	Sample	IQG1538-01	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
43	Sample	CCV	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
44	Sample	CCB	7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
45	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
46	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
47	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
48	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
49	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
50	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
51	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
52	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
53	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
54	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
55	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
56	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
57	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
58	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
59	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
60	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
61	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000
62	Sample		7G17075		1.000000	1.000	1.000000	1.000000	1.000000	0.000000	100.000

PREPARATION BENCH SHEET

7G17075

TestAmerica - Irvine, CA

Printed: 7/24/2007 6:57:32PM

Matrix: Water **Prepared using: Wet Chemistry - General Prep** **(No Surrogate)**

Lab Number	C	Analysis	Prepared	Initial (ml)	Final (ml)	Source ID	Spike 1	ul Spike	Spike 2	ul Spike	ul Surrogate	Initials			Extraction Comments
7G17075-BLK1		QC	07/17/07 12:00	10	10			0		0					
7G17075-BS1		QC	07/17/07 12:00	10	10		7060052	100		100					
7G17075-MS1		QC	07/17/07 12:00	10	10	IQG1425-03	7060052	100		100					
7G17075-MSD1		QC	07/17/07 12:00	10	10	IQG1425-03	7060052	100		100					
IQG1425-03	A	Chromium VI-7199, 1p	07/17/07 12:00	10	10										
IQG1425-03	A	Chromium VI-218.6 (0	07/17/07 12:00	10	10										Added for BatchQC in: 7G17075
IQG1425-03	A	Chromium VI-218.6 C	07/17/07 12:00	10	10										Added for BatchQC in: 7G17075
IQG1425-05	A	Chromium VI-7199, 1p	07/17/07 12:00	10	10										
IQG1425-06	A	Chromium VI-7199, 1p	07/17/07 12:00	10	10										
IQG1460-01	E	Chromium VI-218.6 (0	07/17/07 16:40	10	10										
IQG1460-02	E	Chromium VI-218.6 (0	07/17/07 16:40	10	10										
IQG1460-03	E	Chromium VI-218.6 (0	07/17/07 16:40	10	10										
IQG1460-04	E	Chromium VI-218.6 (0	07/17/07 16:40	10	10										
IQG1460-05	E	Chromium VI-218.6 (0	07/17/07 16:40	10	10										
IQG1460-06	E	Chromium VI-218.6 (0	07/17/07 16:40	10	10										
IQG1538-01	C	Chromium VI-218.6 C	07/17/07 23:30	10	10										

Reagents used in Batch

Reagent	Description	Solvent

Spiking Witnessed By Date

Preparation Reviewed By Date 7/25/07

Extracts Received By Date

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 12:00:23 PM
Reprocess Number	: ic2: 90535		
Operator	: inorg	Sample Name	: IB
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 11:51:08 AM	Cycle	: 1

Raw Data File : h:\data\ic4\20070717\20070717001.raw
Result File : h:\data\ic4\20070717\20070717001.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717001.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717001.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717001.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
-	7.007	chrom6	0.00	0.00000	0.0000	0.0000	
			0.00	0.00000	0.0000	0.0000	

Report stored in ASCII file: h:\data\ic4\20070717\20070717001.TX0

Chromatogram

Sample Name : IB Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717001.raw
Date : 7/17/2007 12:00:25 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 11:51:08 AM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

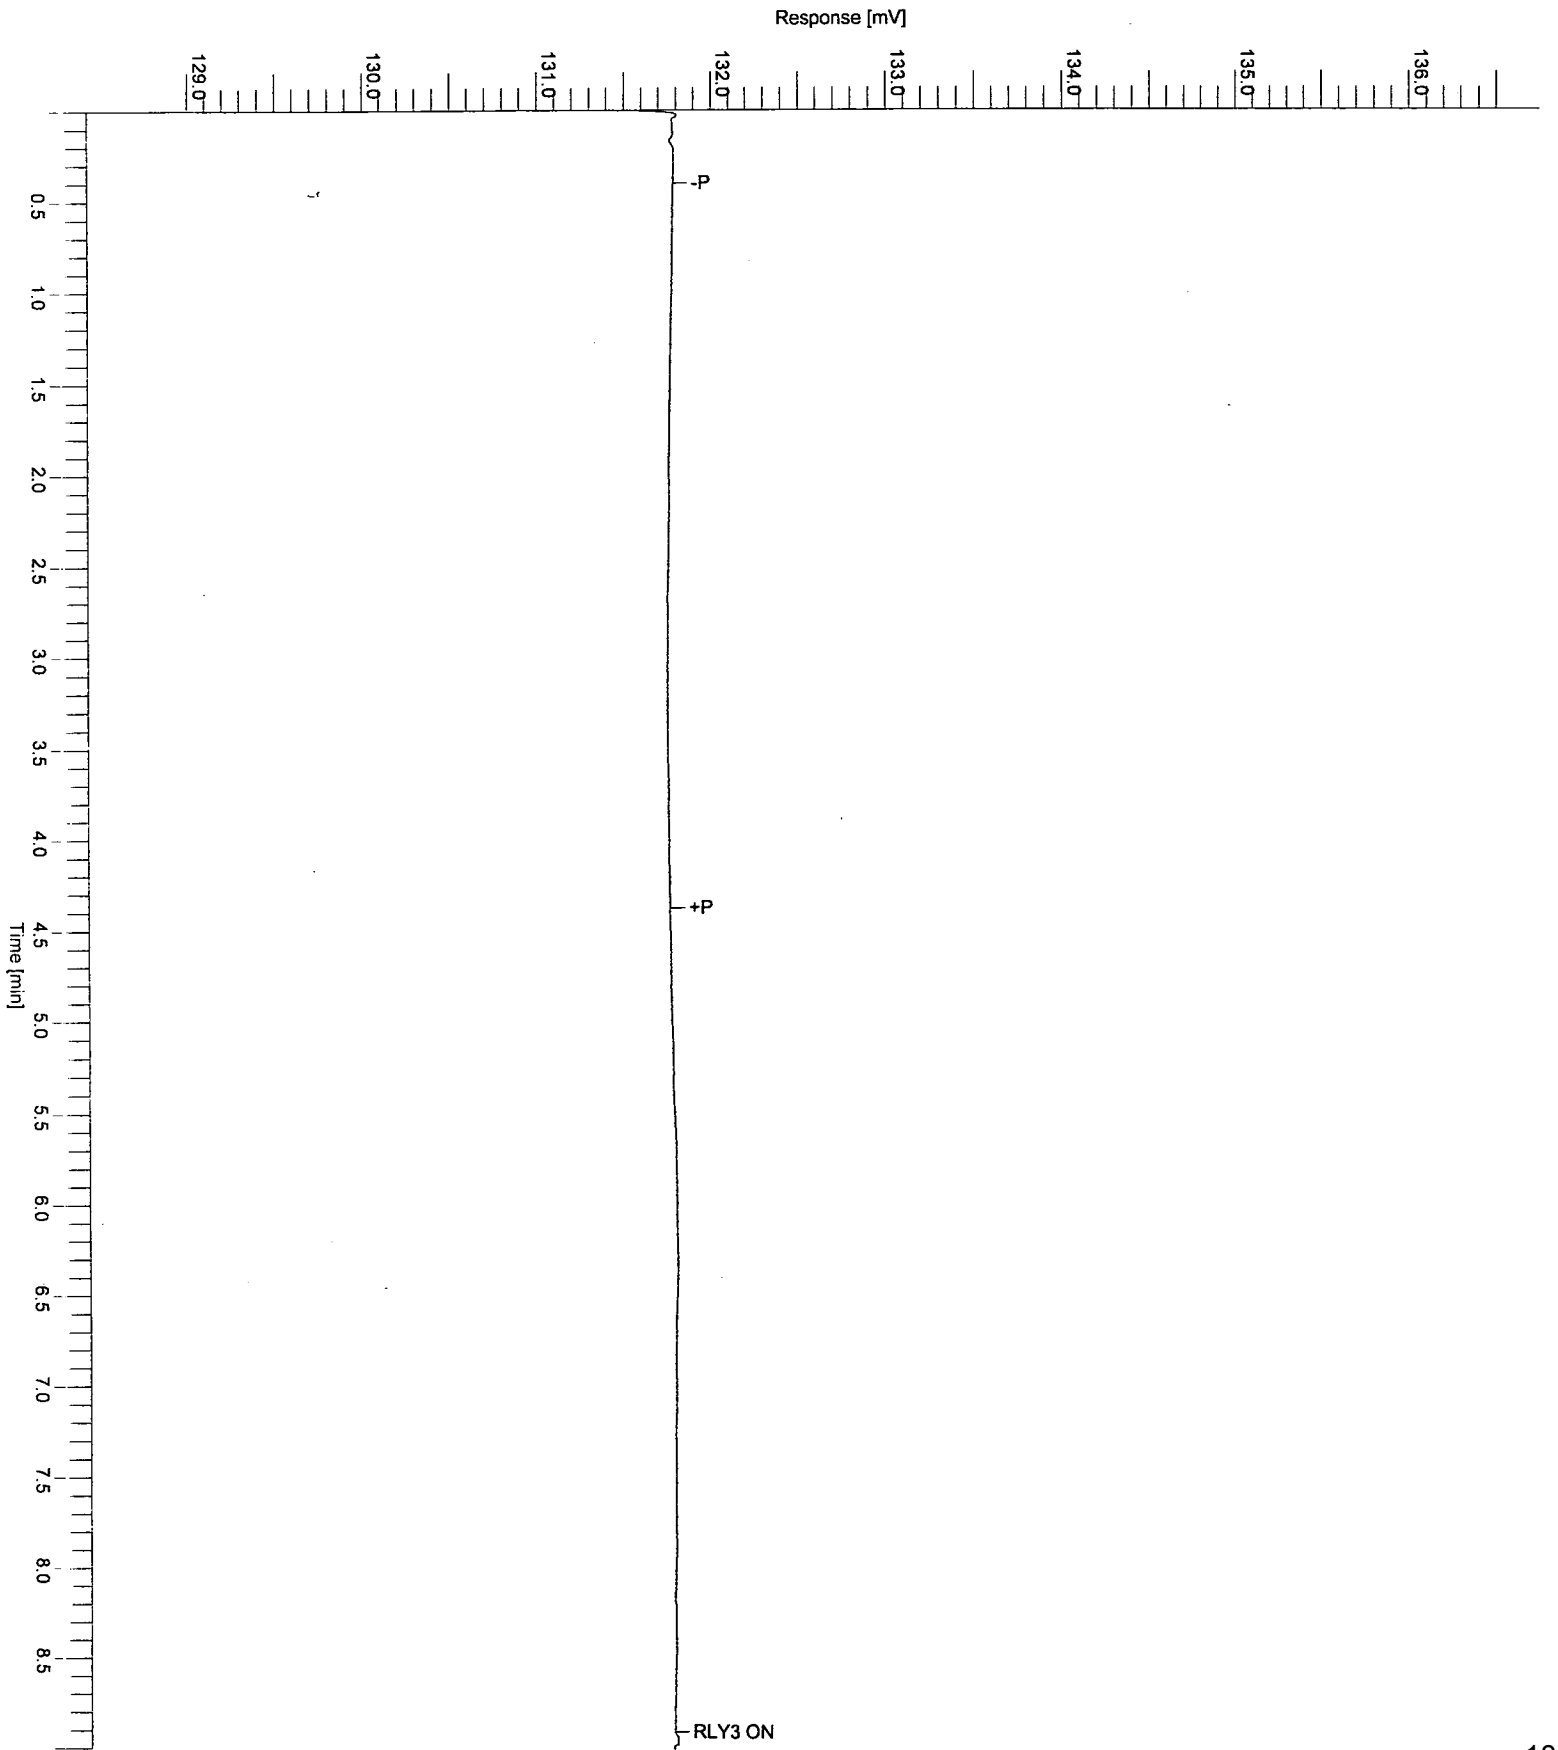

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 12:11:31 PM
Reprocess Number	: ic2: 90538		
Operator	: inorg	Sample Name	: 7G17075-BS1
Sample Number	: 7G17075	Study	: 7060052
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 12:02:17 PM	Cycle	: 2

Raw Data File : h:\data\ic4\20070717\20070717002.raw
Result File : h:\data\ic4\20070717\20070717002.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717002.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717002.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717002.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.536	chrom6	26562.25	1.461e+03	45.7714	45.7714	*
			26562.25	1.461e+03	45.7714	45.7714	

* Warning – uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070717\20070717002.TX0

Chromatogram

Sample Name : 7G17075-BS1 Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717002.raw
Date : 7/17/2007 12:11:32 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 12:02:17 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

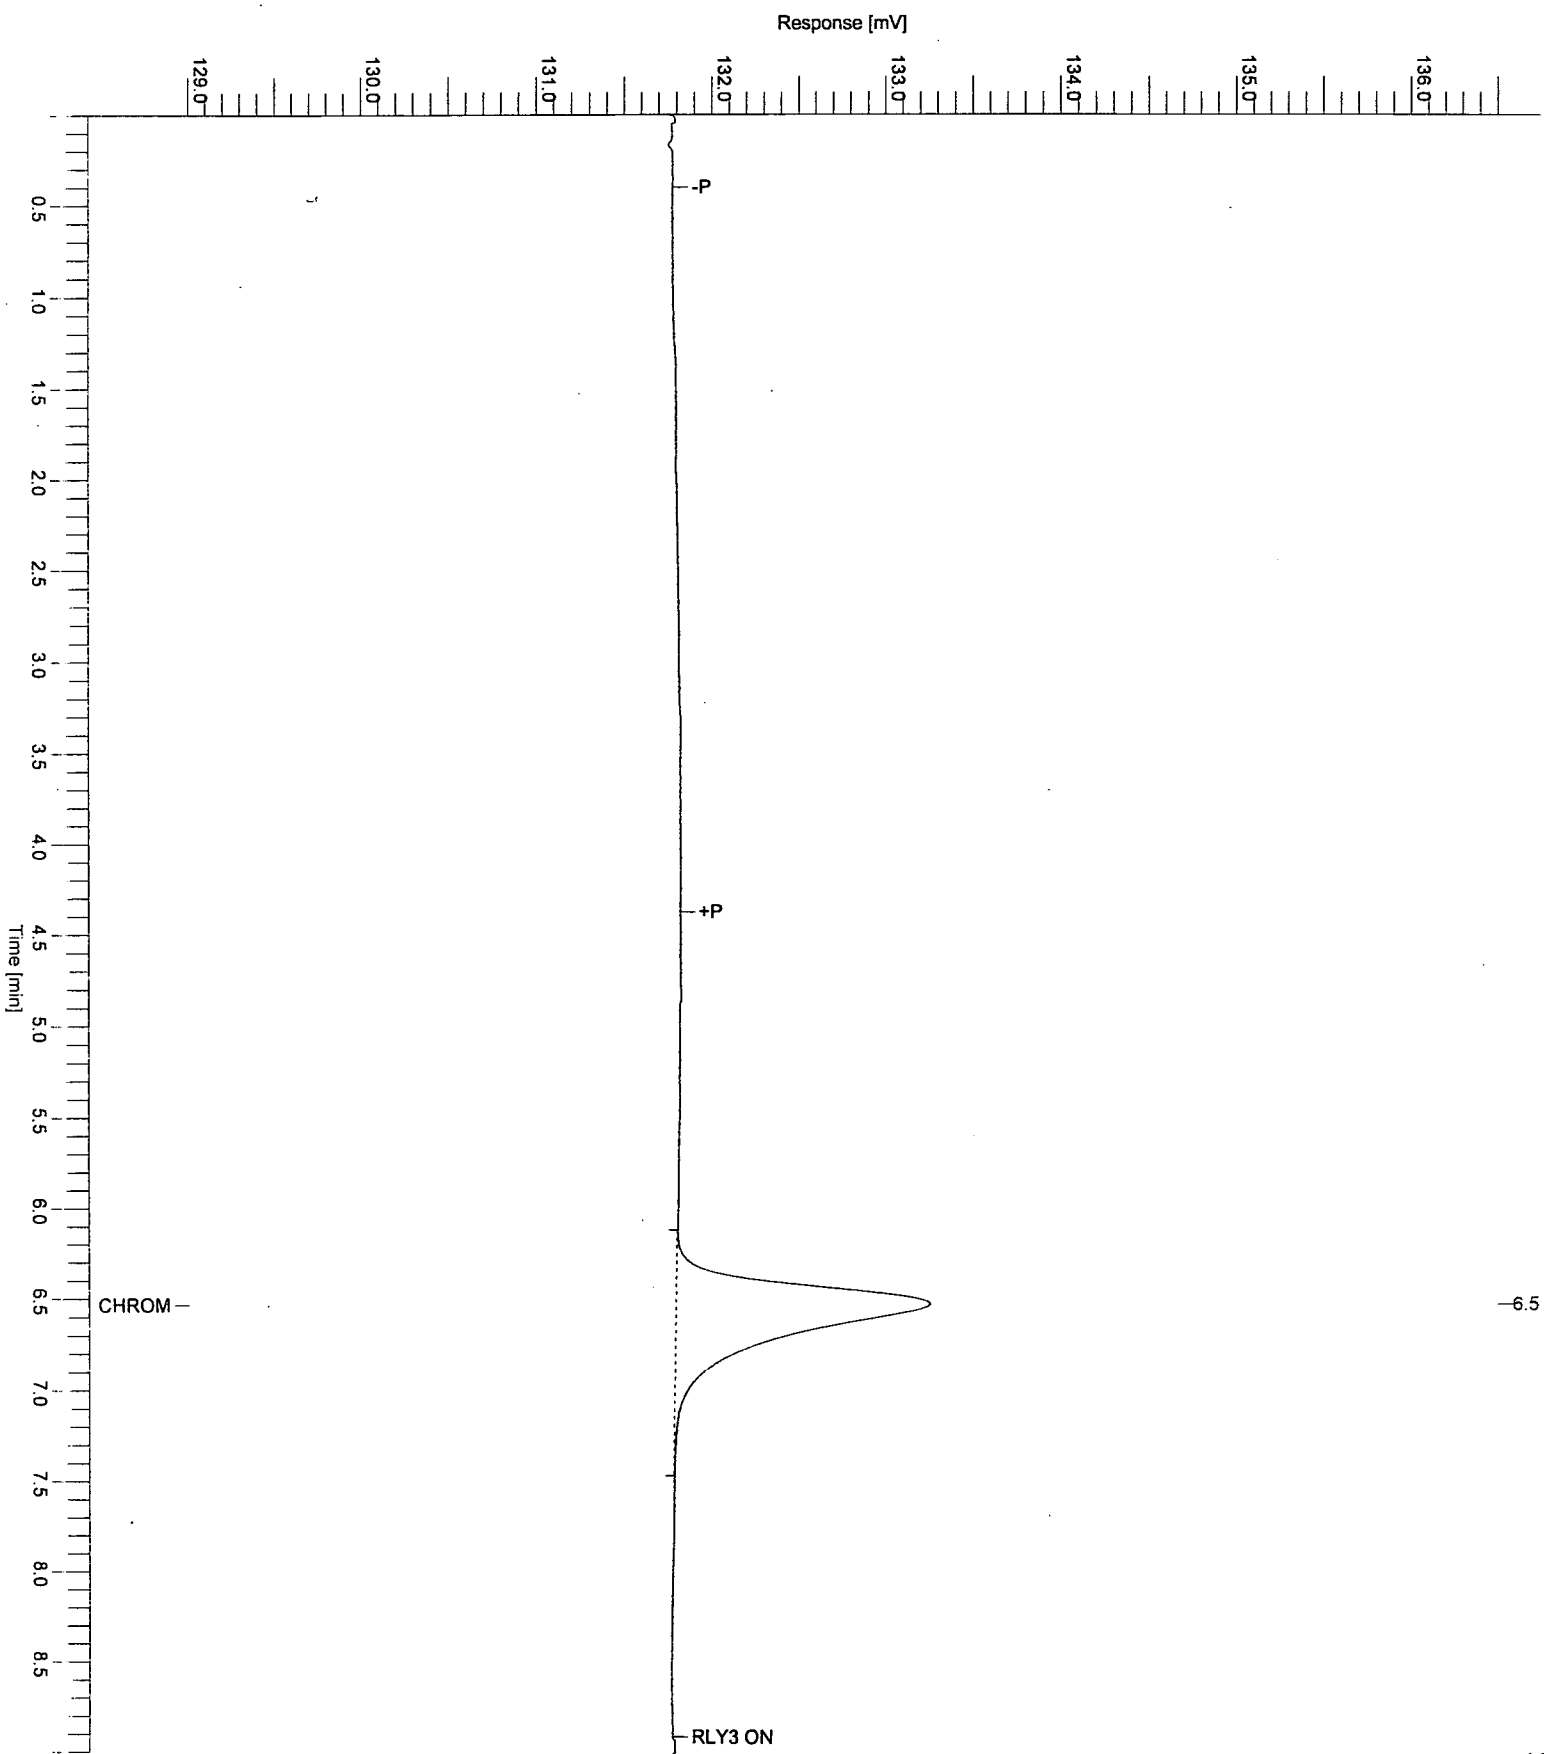

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 12:22:37 PM
Reprocess Number	: ic2: 90539		
Operator	: inorg	Sample Name	: 7G17075-BLK1
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 12:13:26 PM	Cycle	: 3

Raw Data File : h:\data\ic4\20070717\20070717003.raw
Result File : h:\data\ic4\20070717\20070717003.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717003.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717003.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717003.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
-	7.007	chrom6	0.00	0.00000	0.0000	0.0000	
			0.00	0.00000	0.0000	0.0000	

Report stored in ASCII file: h:\data\ic4\20070717\20070717003.TX0

Chromatogram

Sample Name : 7G17075-BLK1 Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717003.raw
Date : 7/17/2007 12:22:39 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 12:13:26 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

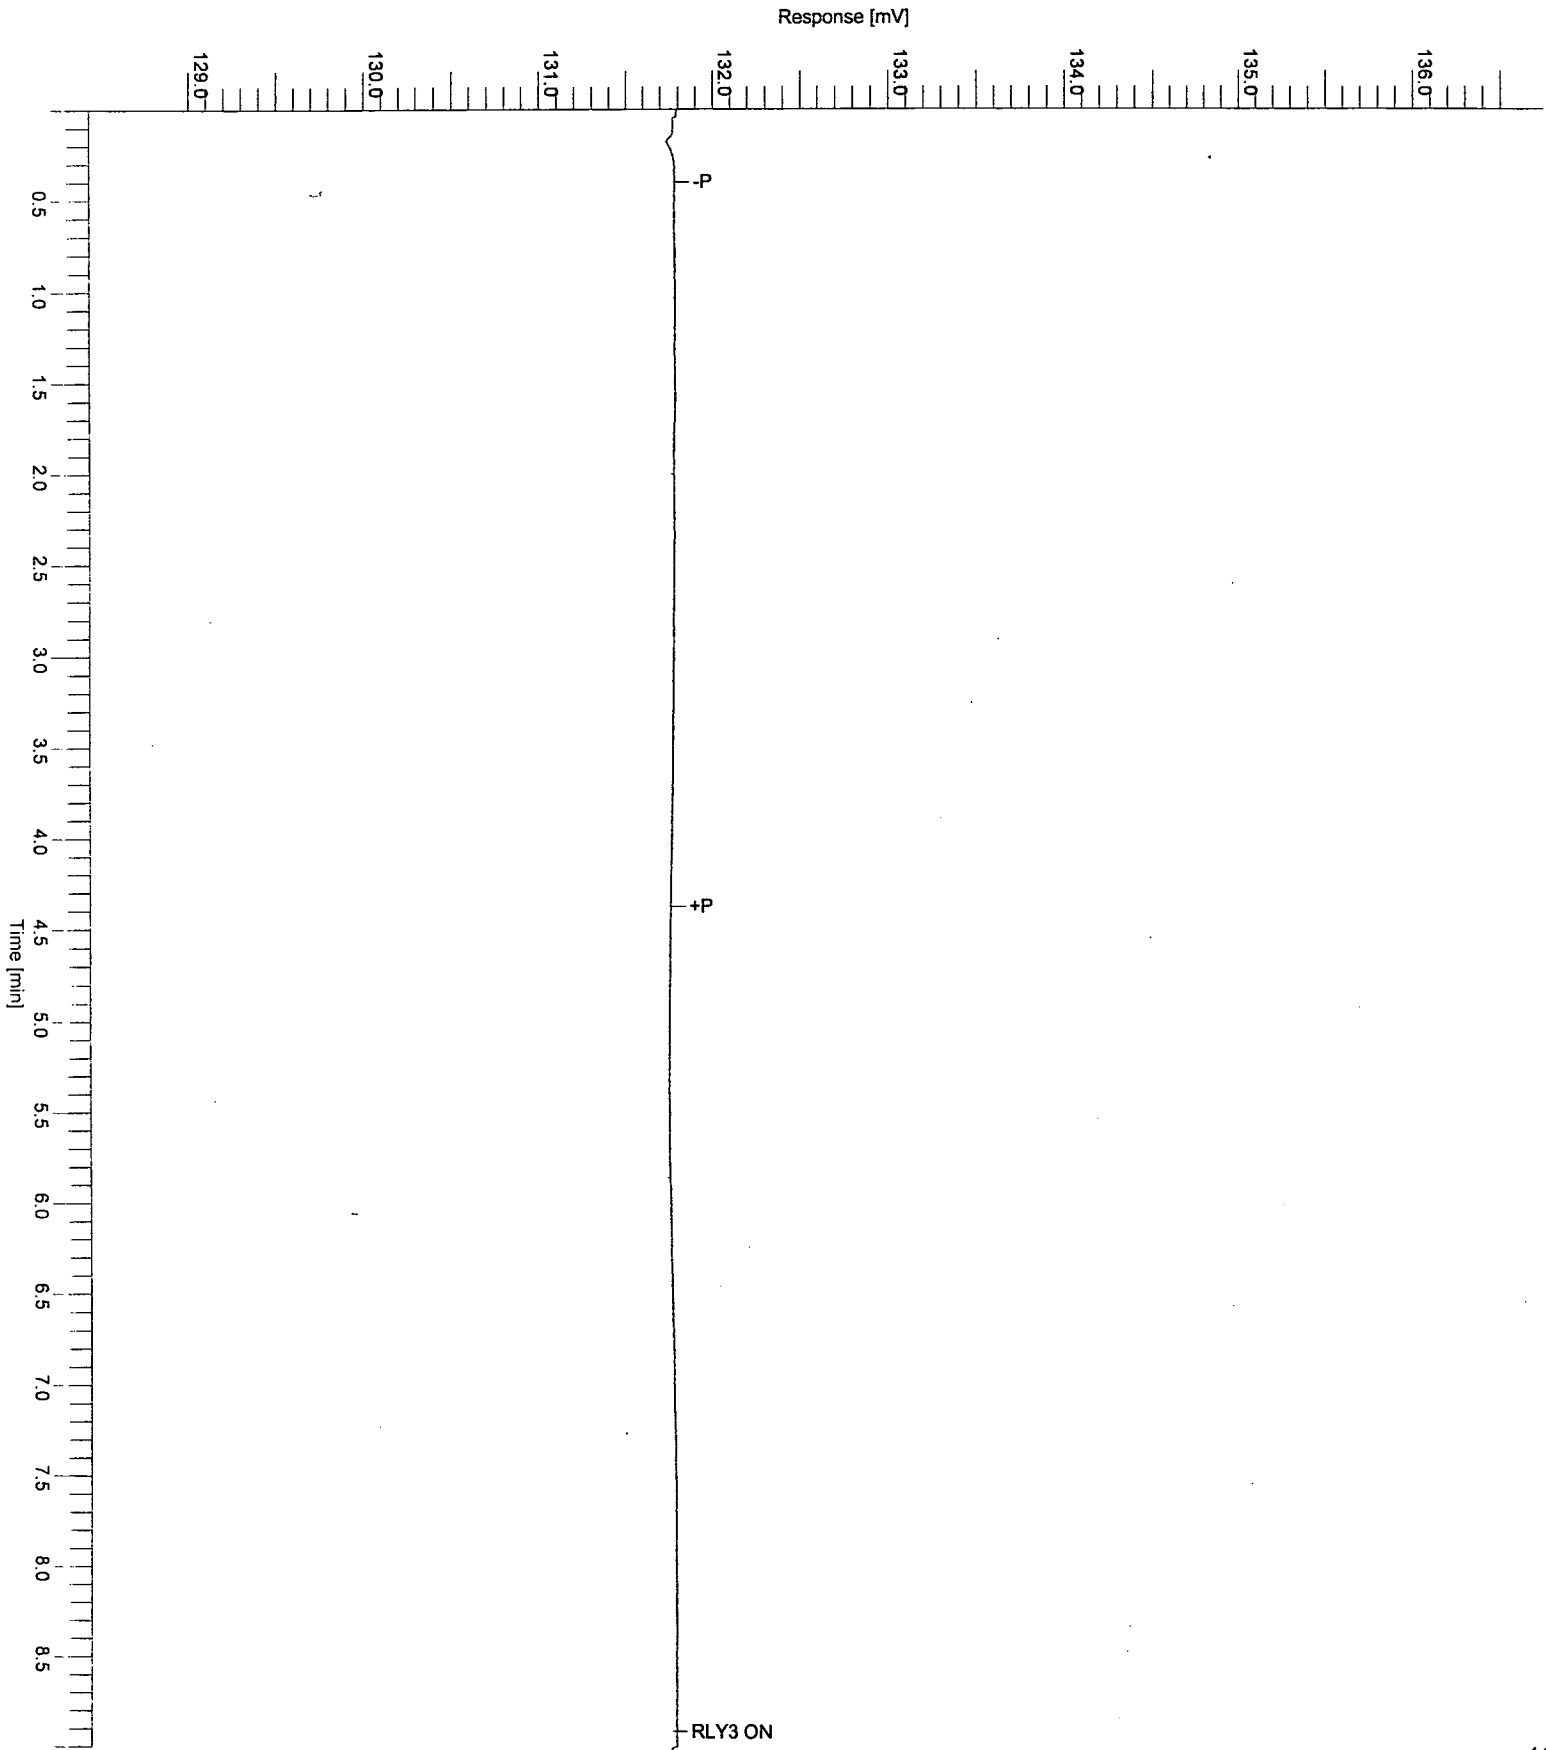

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 12:33:48 PM
Reprocess Number	: ic2: 90542		
Operator	: inorg	Sample Name	: IQG1425-03
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 12:24:34 PM	Cycle	: 4

Raw Data File : h:\data\ic4\20070717\20070717004.raw
Result File : h:\data\ic4\20070717\20070717004.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717004.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717004.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717004.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
-	7.007	chrom6	0.00	0.00000	0.0000	0.0000	
			0.00	0.00000	0.0000	0.0000	

Report stored in ASCII file: h:\data\ic4\20070717\20070717004.TX0

Chromatogram

Sample Name : IQG1425-03 Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717004.raw
Date : 7/17/2007 12:33:49 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 12:24:34 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

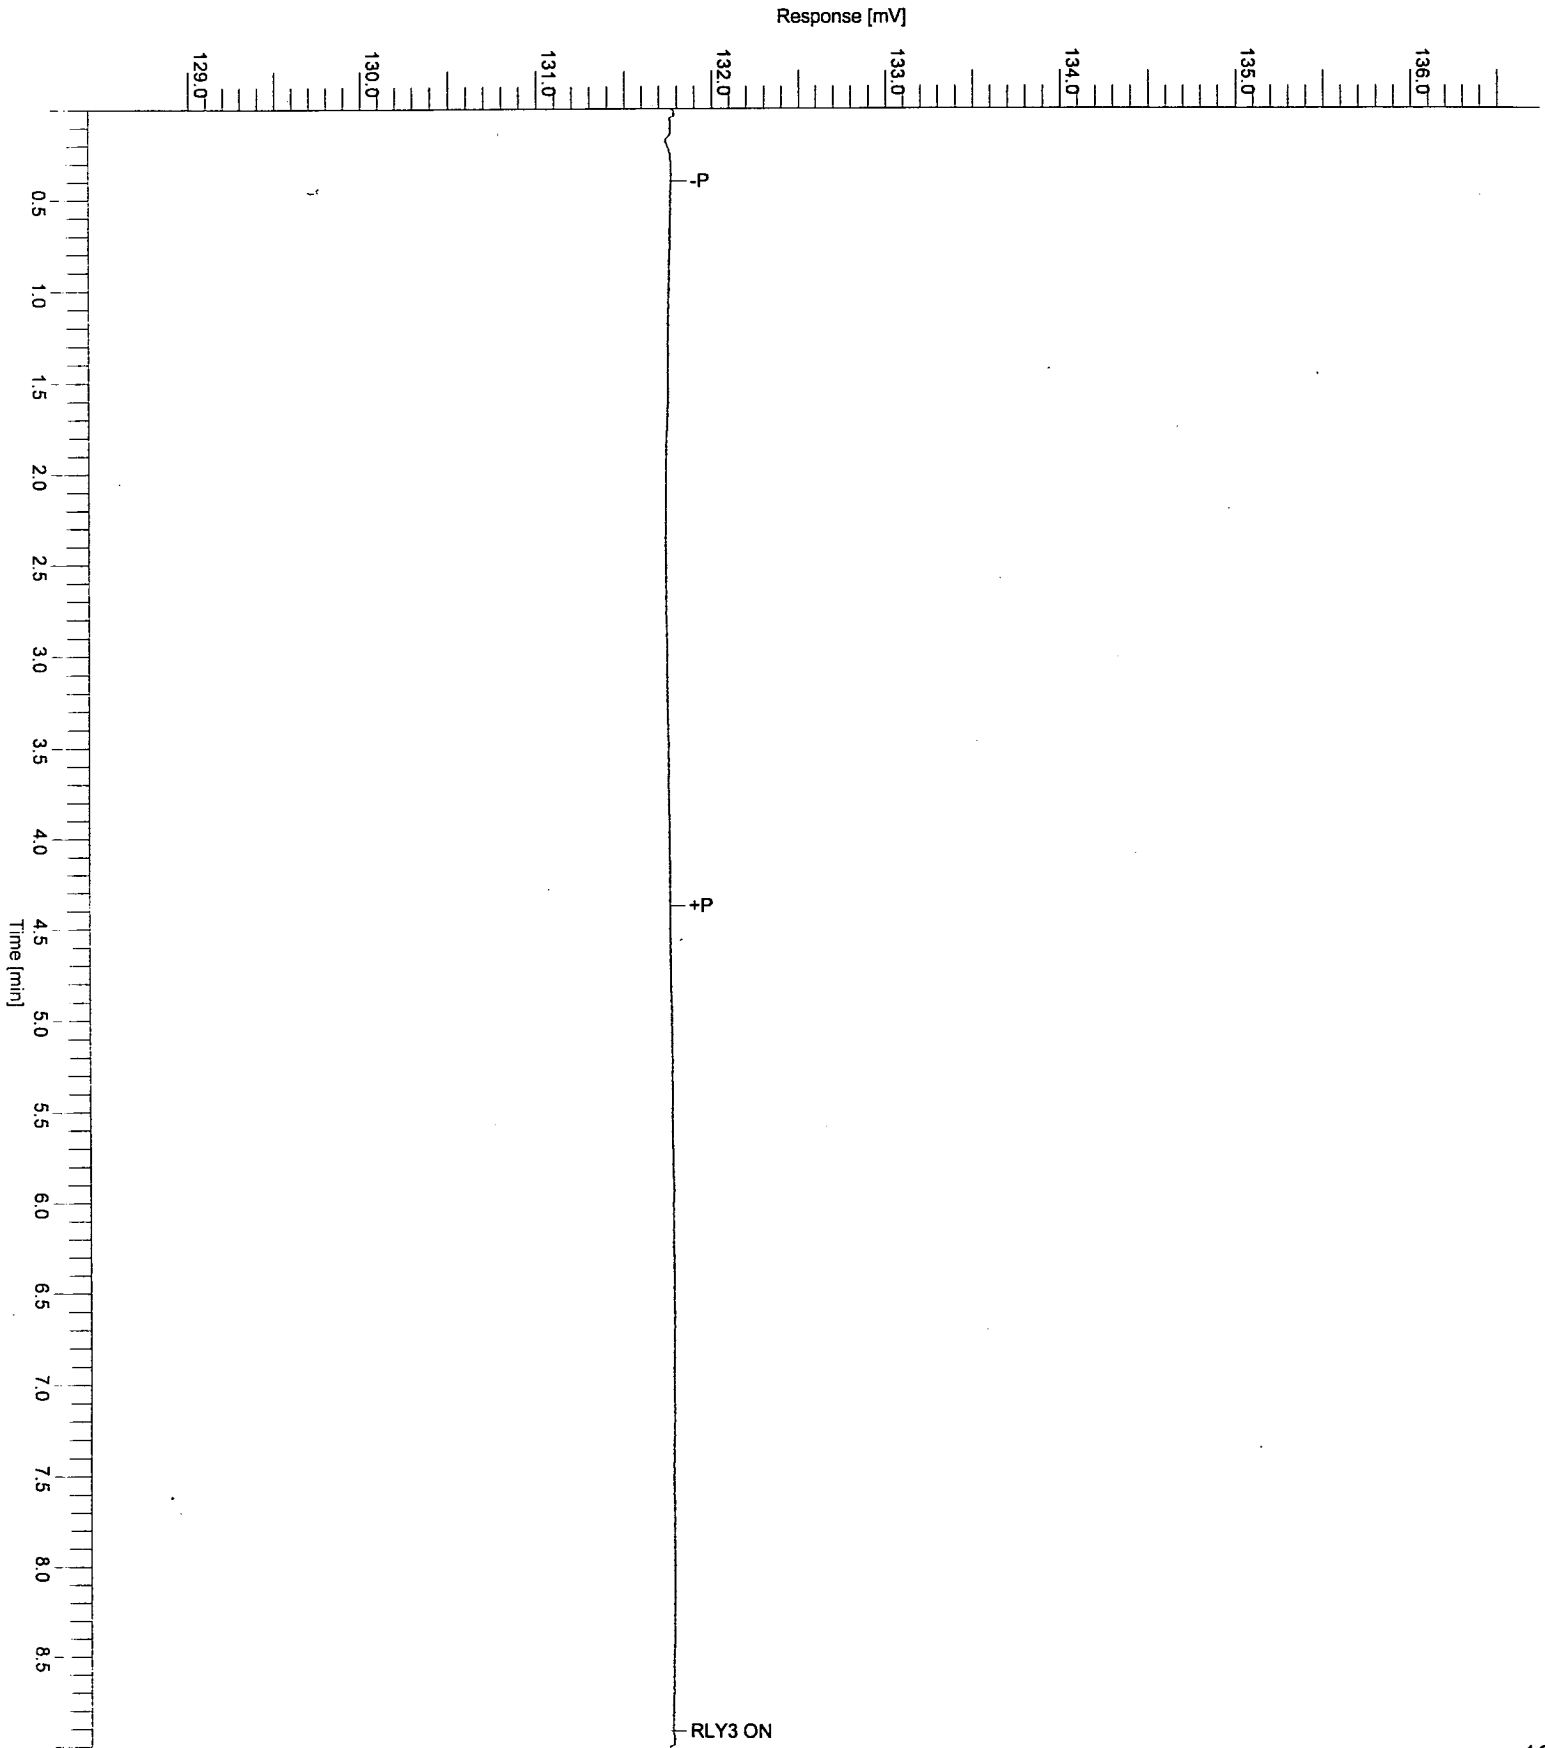

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 1:13:10 PM
Reprocess Number	: ic2: 90547		
Operator	: inorg	Sample Name	: 7G17075-MS1
Sample Number	: 7G17075	Study	: IQG1425-03
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 1:03:55 PM	Cycle	: 7

Raw Data File : h:\data\ic4\20070717\20070717007.raw
Result File : h:\data\ic4\20070717\20070717007.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717007.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717007.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717007.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.629	chrom6	27402.85	1.661e+03	52.0323	52.0323	*
			27402.85	1.661e+03	52.0323	52.0323	

* Warning -- uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070717\20070717007.TX0

Chromatogram

Sample Name : 7G17075-MS1 Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717007.raw
Date : 7/17/2007 1:13:12 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 1:03:55 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

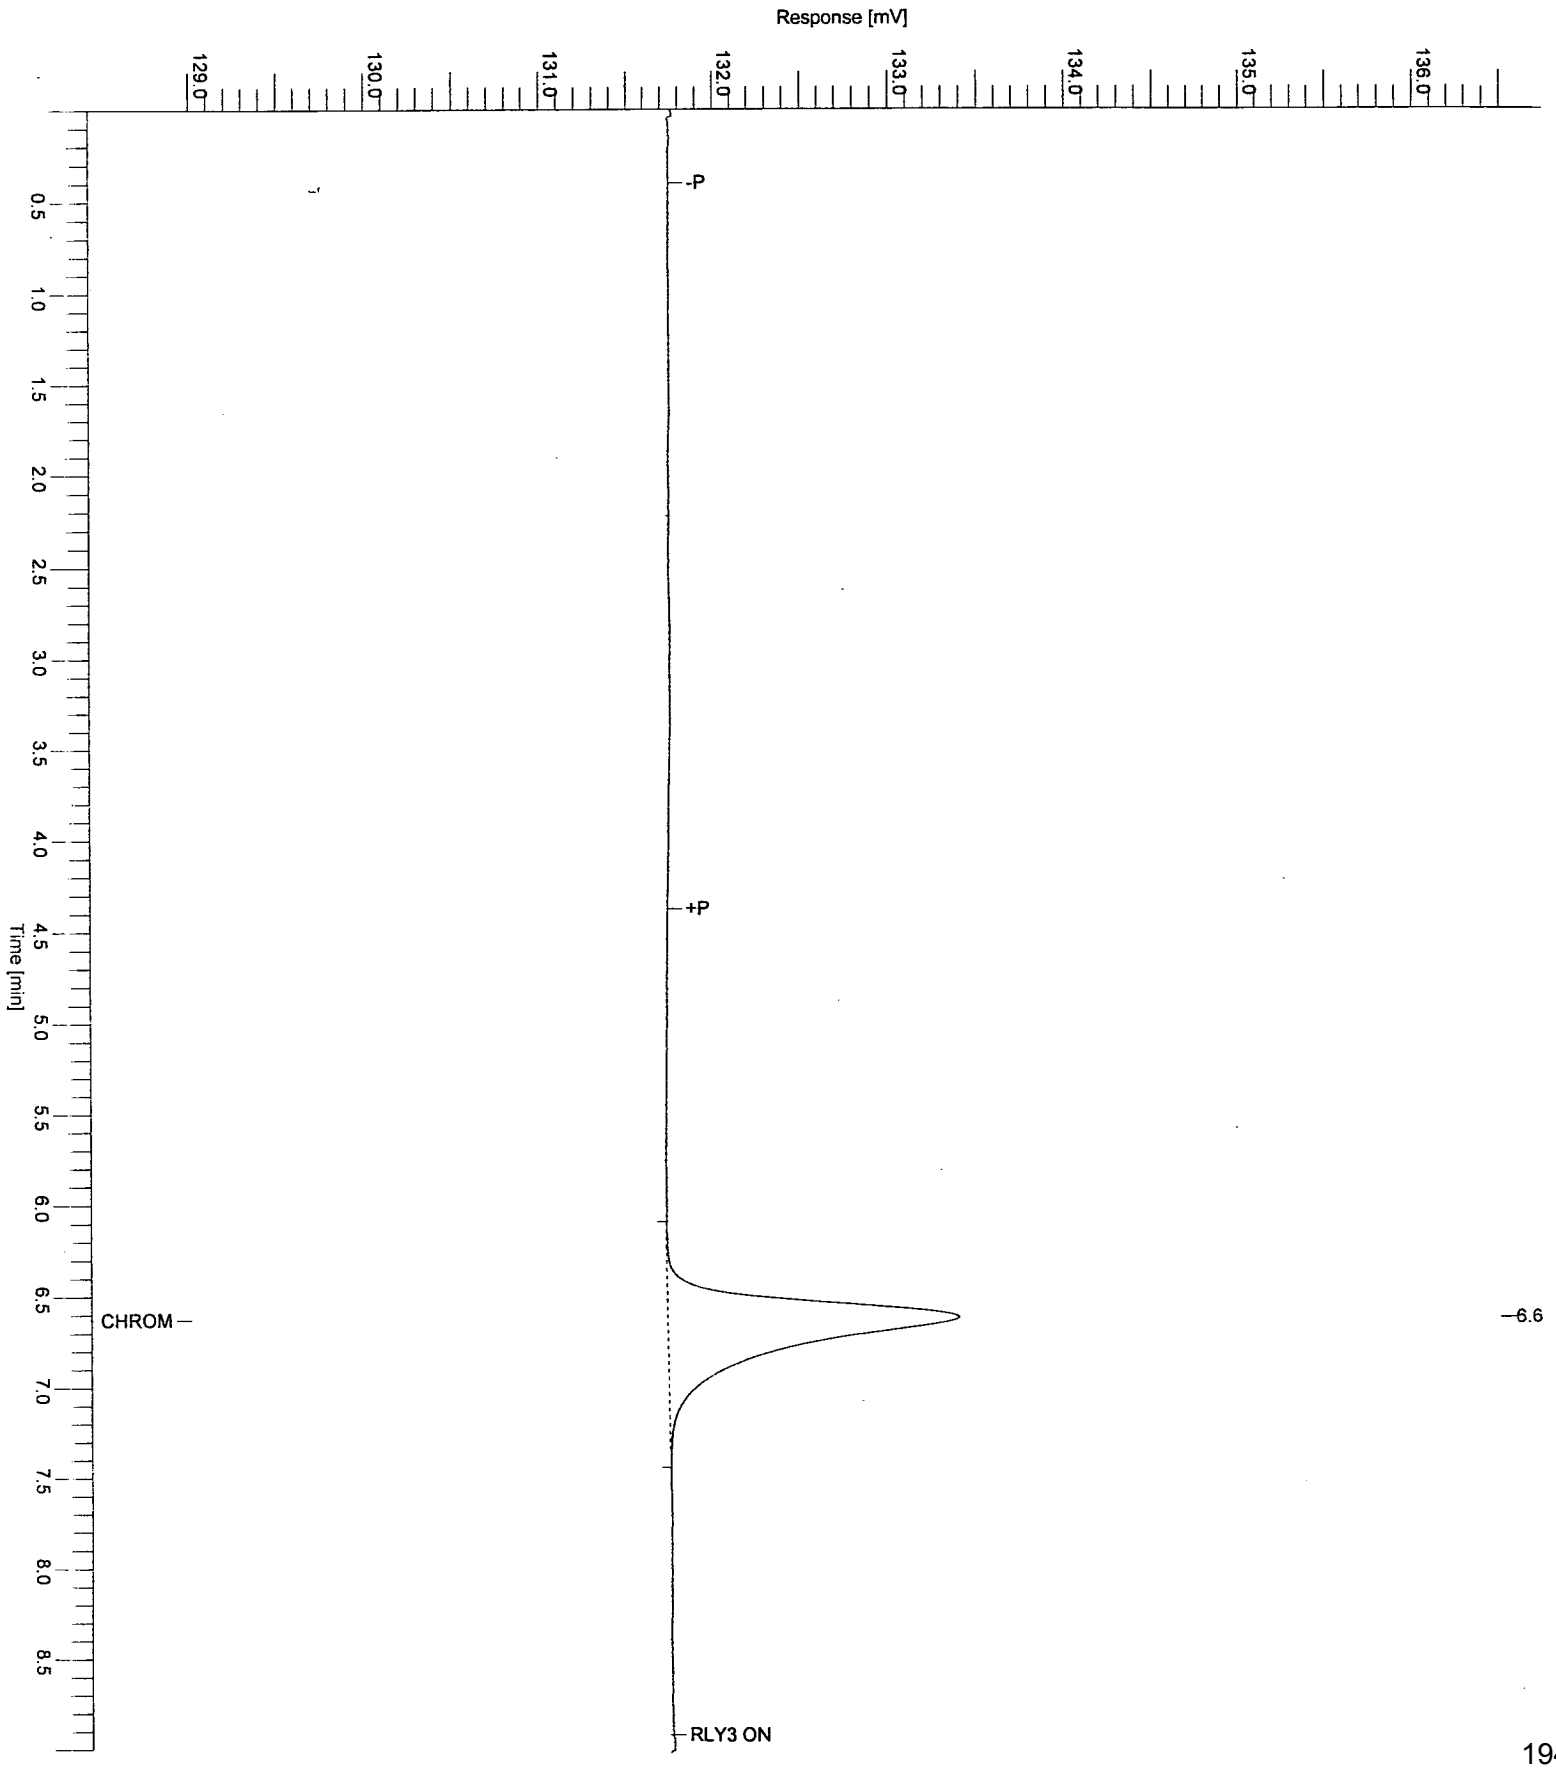

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 1:33:33 PM
Operator	: inorg	Sample Name	: 7G17075-MSD1
Sample Number	: 7G17075	Study	: IQG1425-03
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 1:22:48 PM	Cycle	: 8

Raw Data File : h:\data\ic4\20070717\20070717008.raw
Result File : H:\DATA\IC4\20070717\20070717008A.rst [Editing in Progress]
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717008.raw
Proc Method : h:\data\ic4\chr6qd30 from H:\DATA\IC4\20070717\20070717008A.rst [Editing in Progress]
Calib Method : h:\data\ic4\chr6qd30 from H:\DATA\IC4\20070717\20070717008A.rst [Editing in Progress]
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

after

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.590	chrom6	27220.84	1.657e+03	51.8907	51.8907	*
			27220.84	1.657e+03	51.8907	51.8907	

* Warning -- uncalibrated levels encountered

Report stored in ASCII file: H:\DATA\IC4\20070717\20070717008A.TX0

Chromatogram

Sample Name : 7G17075-MSD1 Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717008.raw
Date : 7/17/2007 1:33:36 PM
Method : Time of Injection: 7/17/2007 1:22:48 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

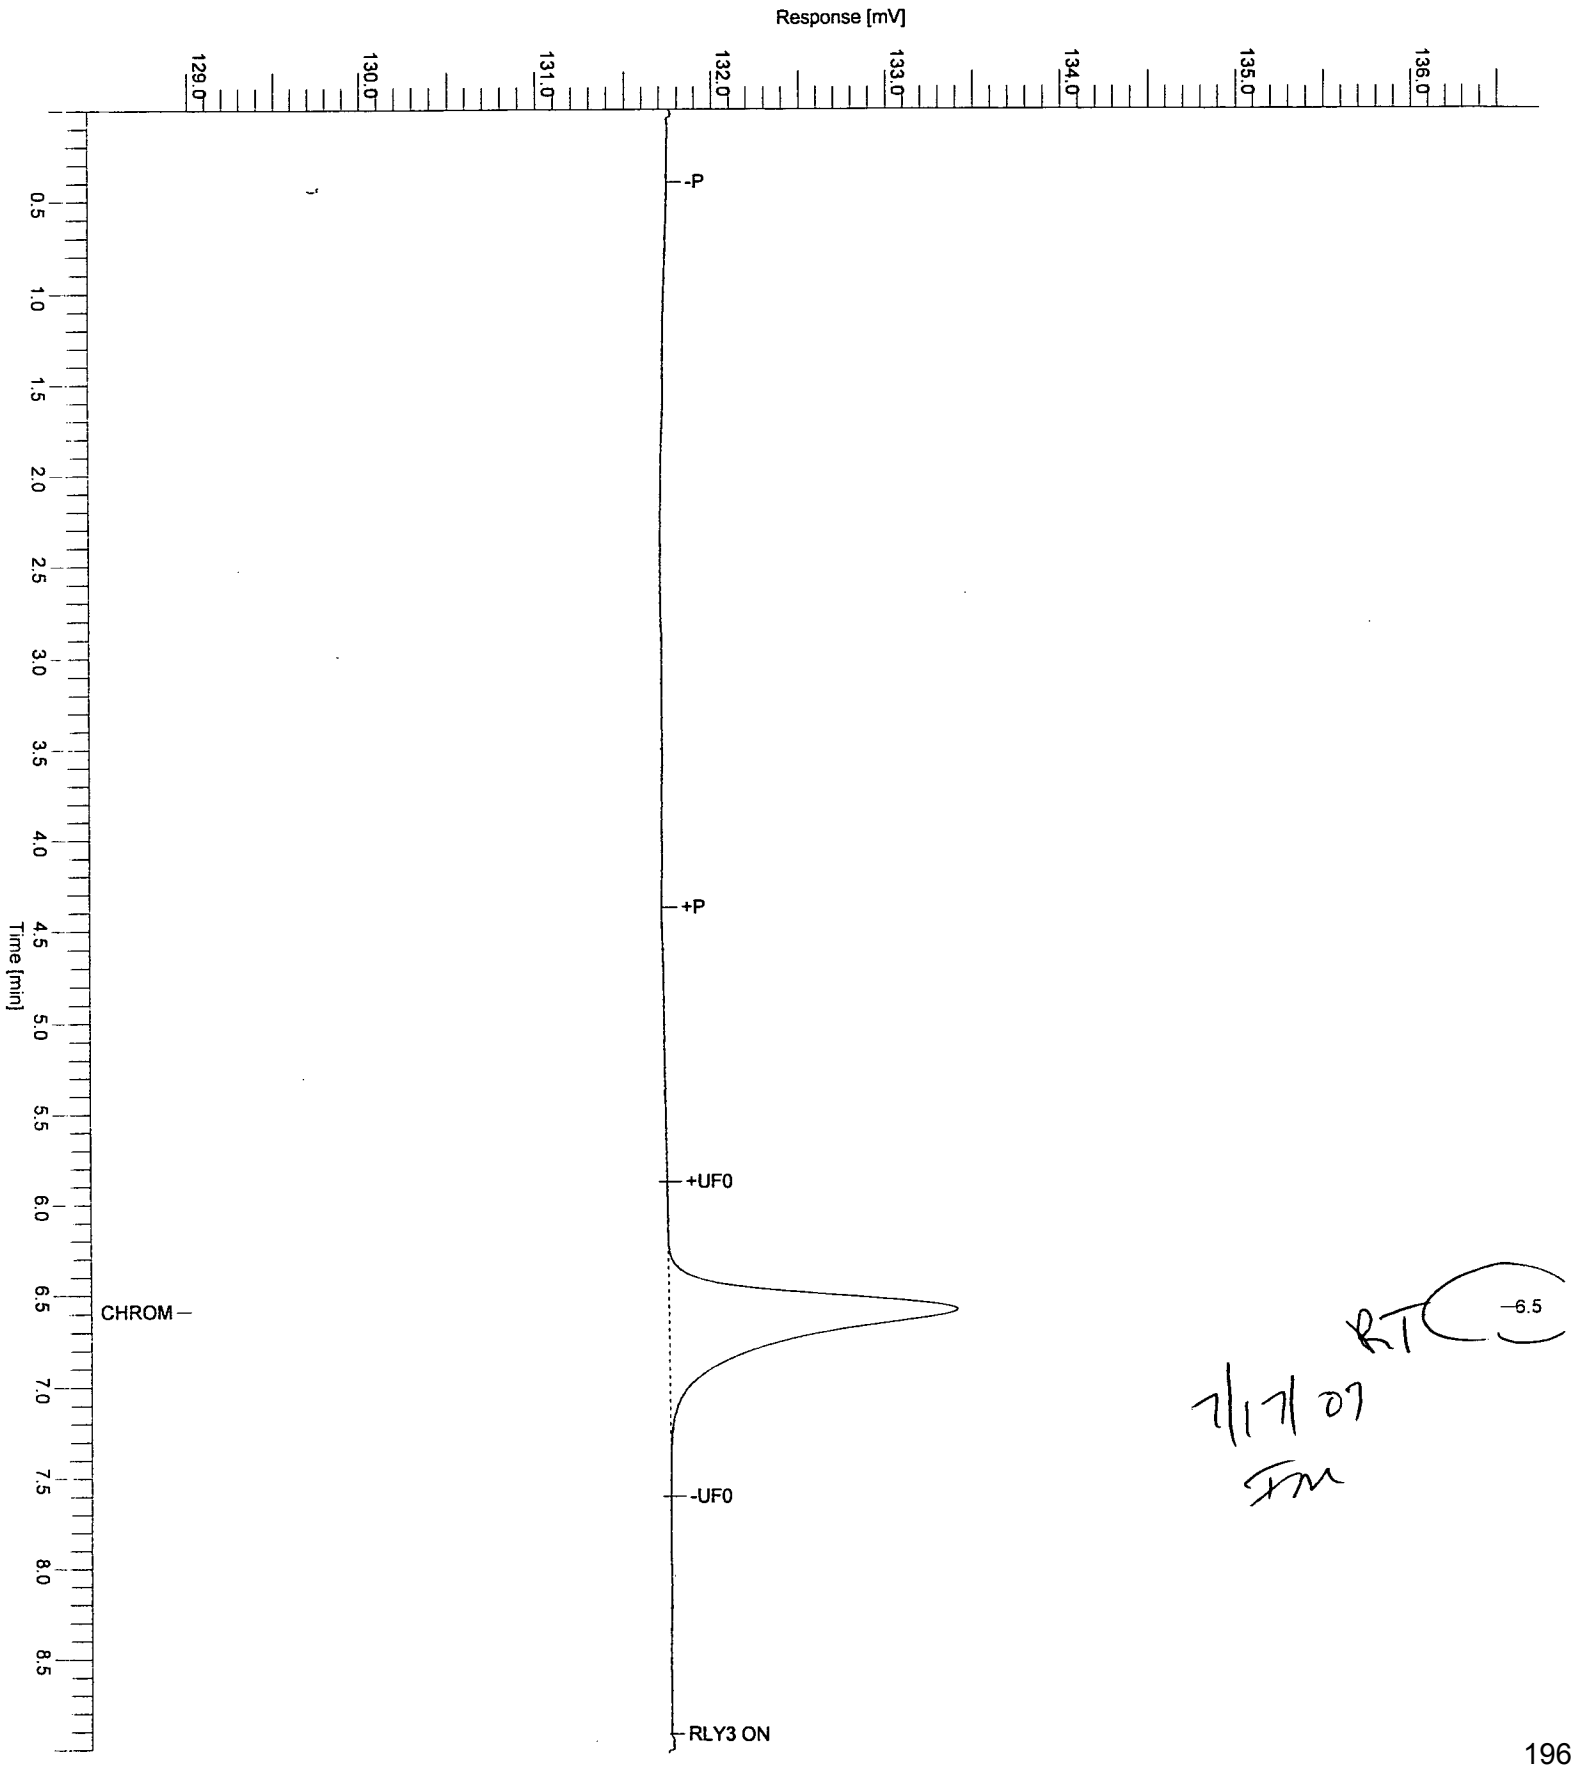

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 1:32:04 PM
Reprocess Number	: ic2: 90549		
Operator	: inorg	Sample Name	: 7G17075-MSD1
Sample Number	: 7G17075	Study	: IQG1425-03
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 1:22:48 PM	Cycle	: 8

Raw Data File : h:\data\ic4\20070717\20070717008.raw
Result File : h:\data\ic4\20070717\20070717008.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717008.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717008.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717008.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.657	chrom6	27559.75	1.310e+03	41.0160	41.0160	*
			27559.75	1.310e+03	41.0160	41.0160	

before

* Warning -- uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070717\20070717008.TX0

Chromatogram

Sample Name : 7G17075-MSD1 Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717008.raw
Date : 7/17/2007 1:32:06 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 1:22:48 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

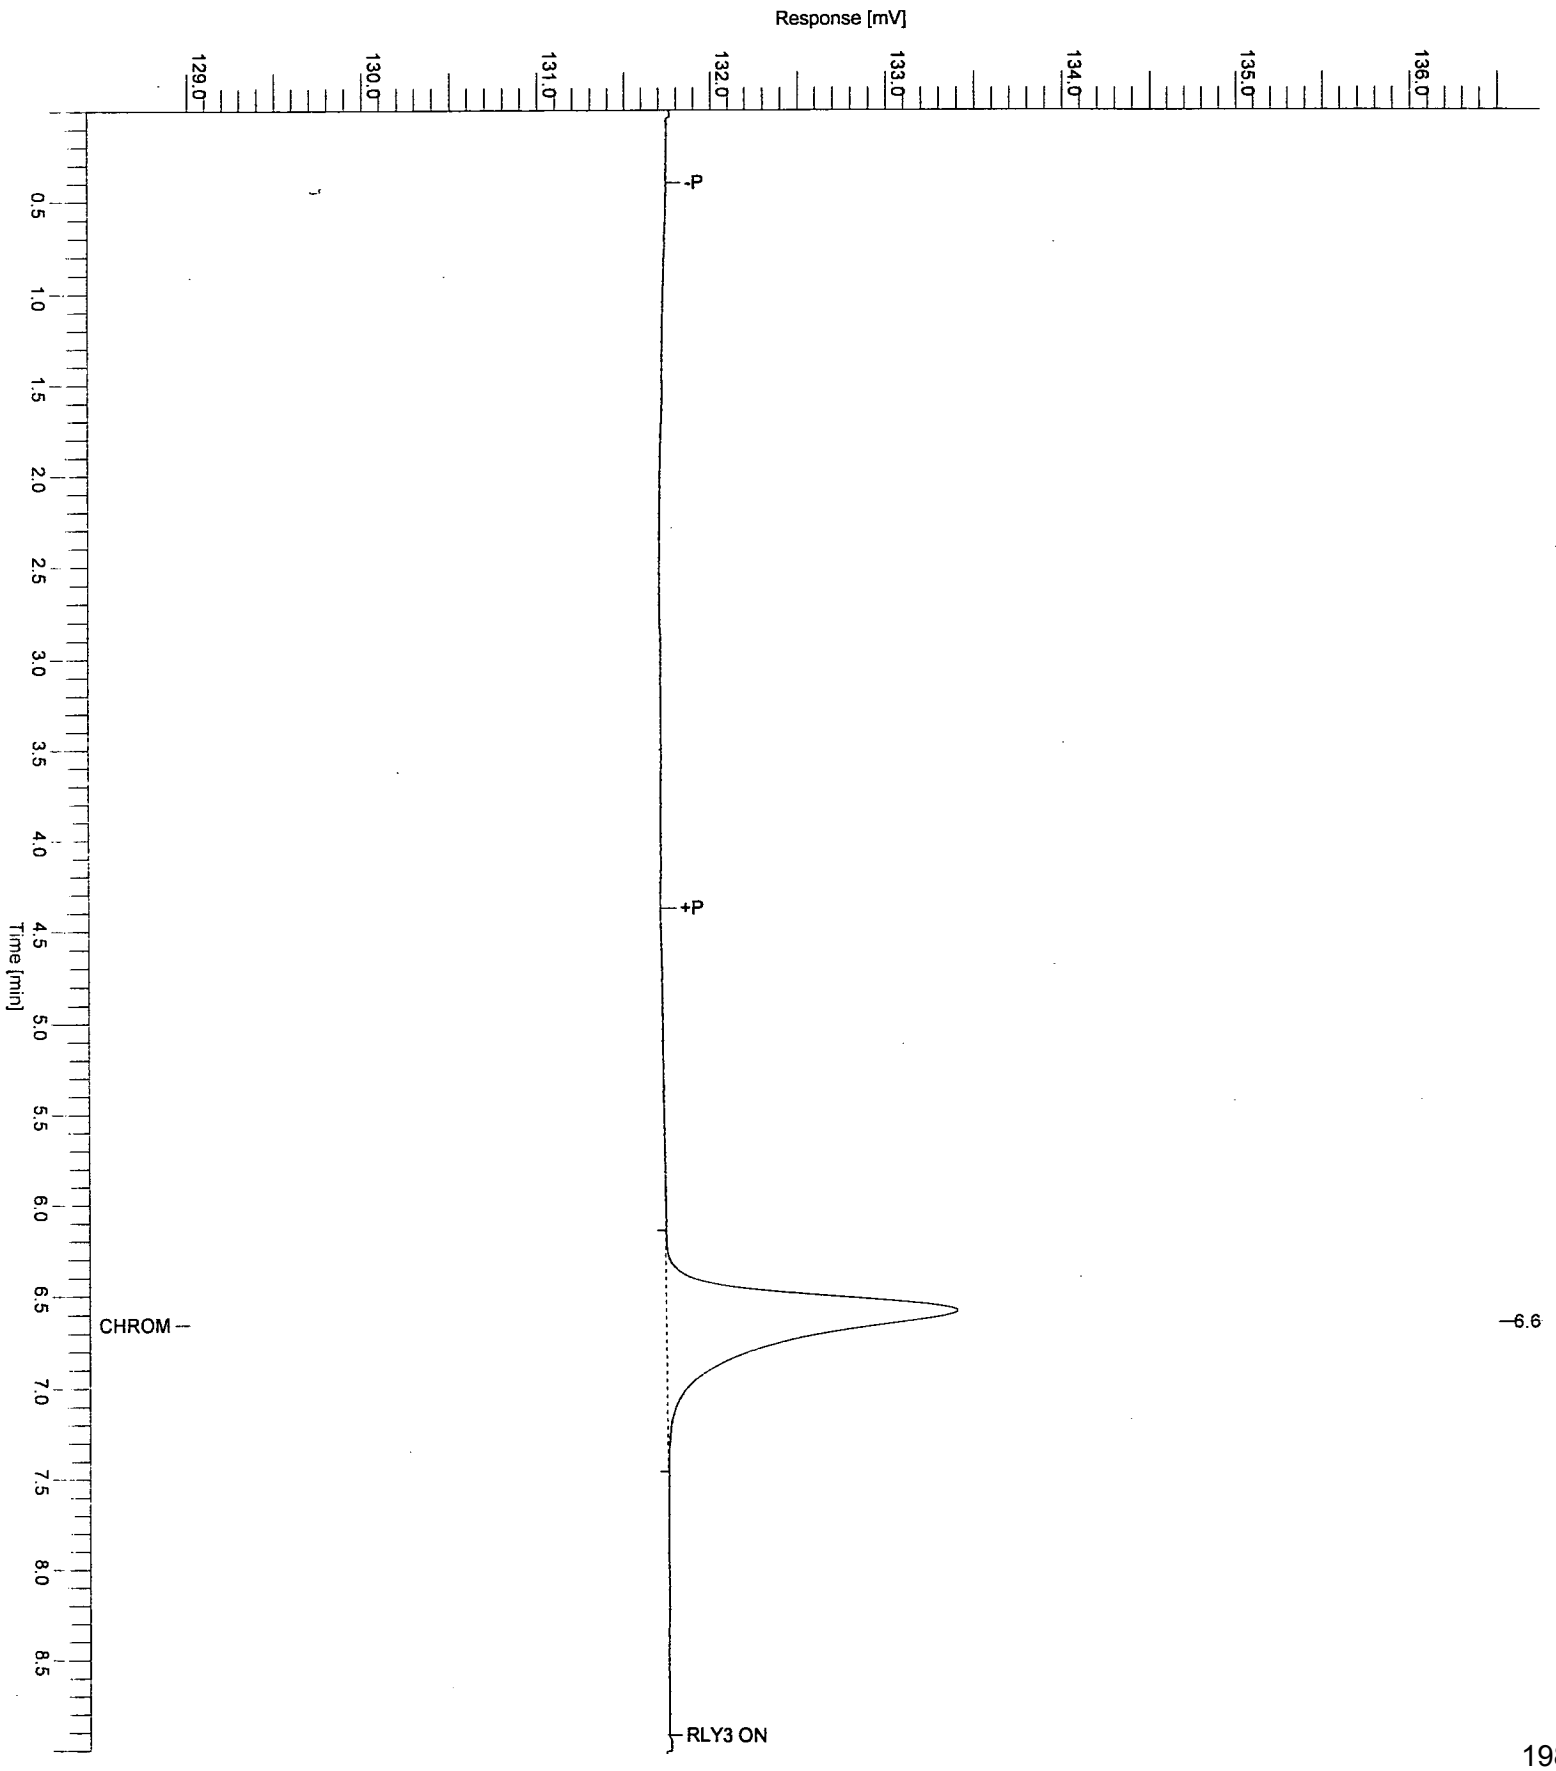

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 1:43:33 PM
Reprocess Number	: ic2: 90551		
Operator	: inorg	Sample Name	: CCV
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 1:34:16 PM	Cycle	: 9

Raw Data File : h:\data\ic4\20070717\20070717009.raw
Result File : h:\data\ic4\20070717\20070717009.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717009.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717009.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717009.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.668	chrom6	27819.70	1.650e+03	51.6998	51.6998	*
			27819.70	1.650e+03	51.6998	51.6998	

* Warning -- uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070717\20070717009.TX0

Chromatogram

Sample Name : CCV Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717009.raw
Date : 7/17/2007 1:43:34 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 1:34:16 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

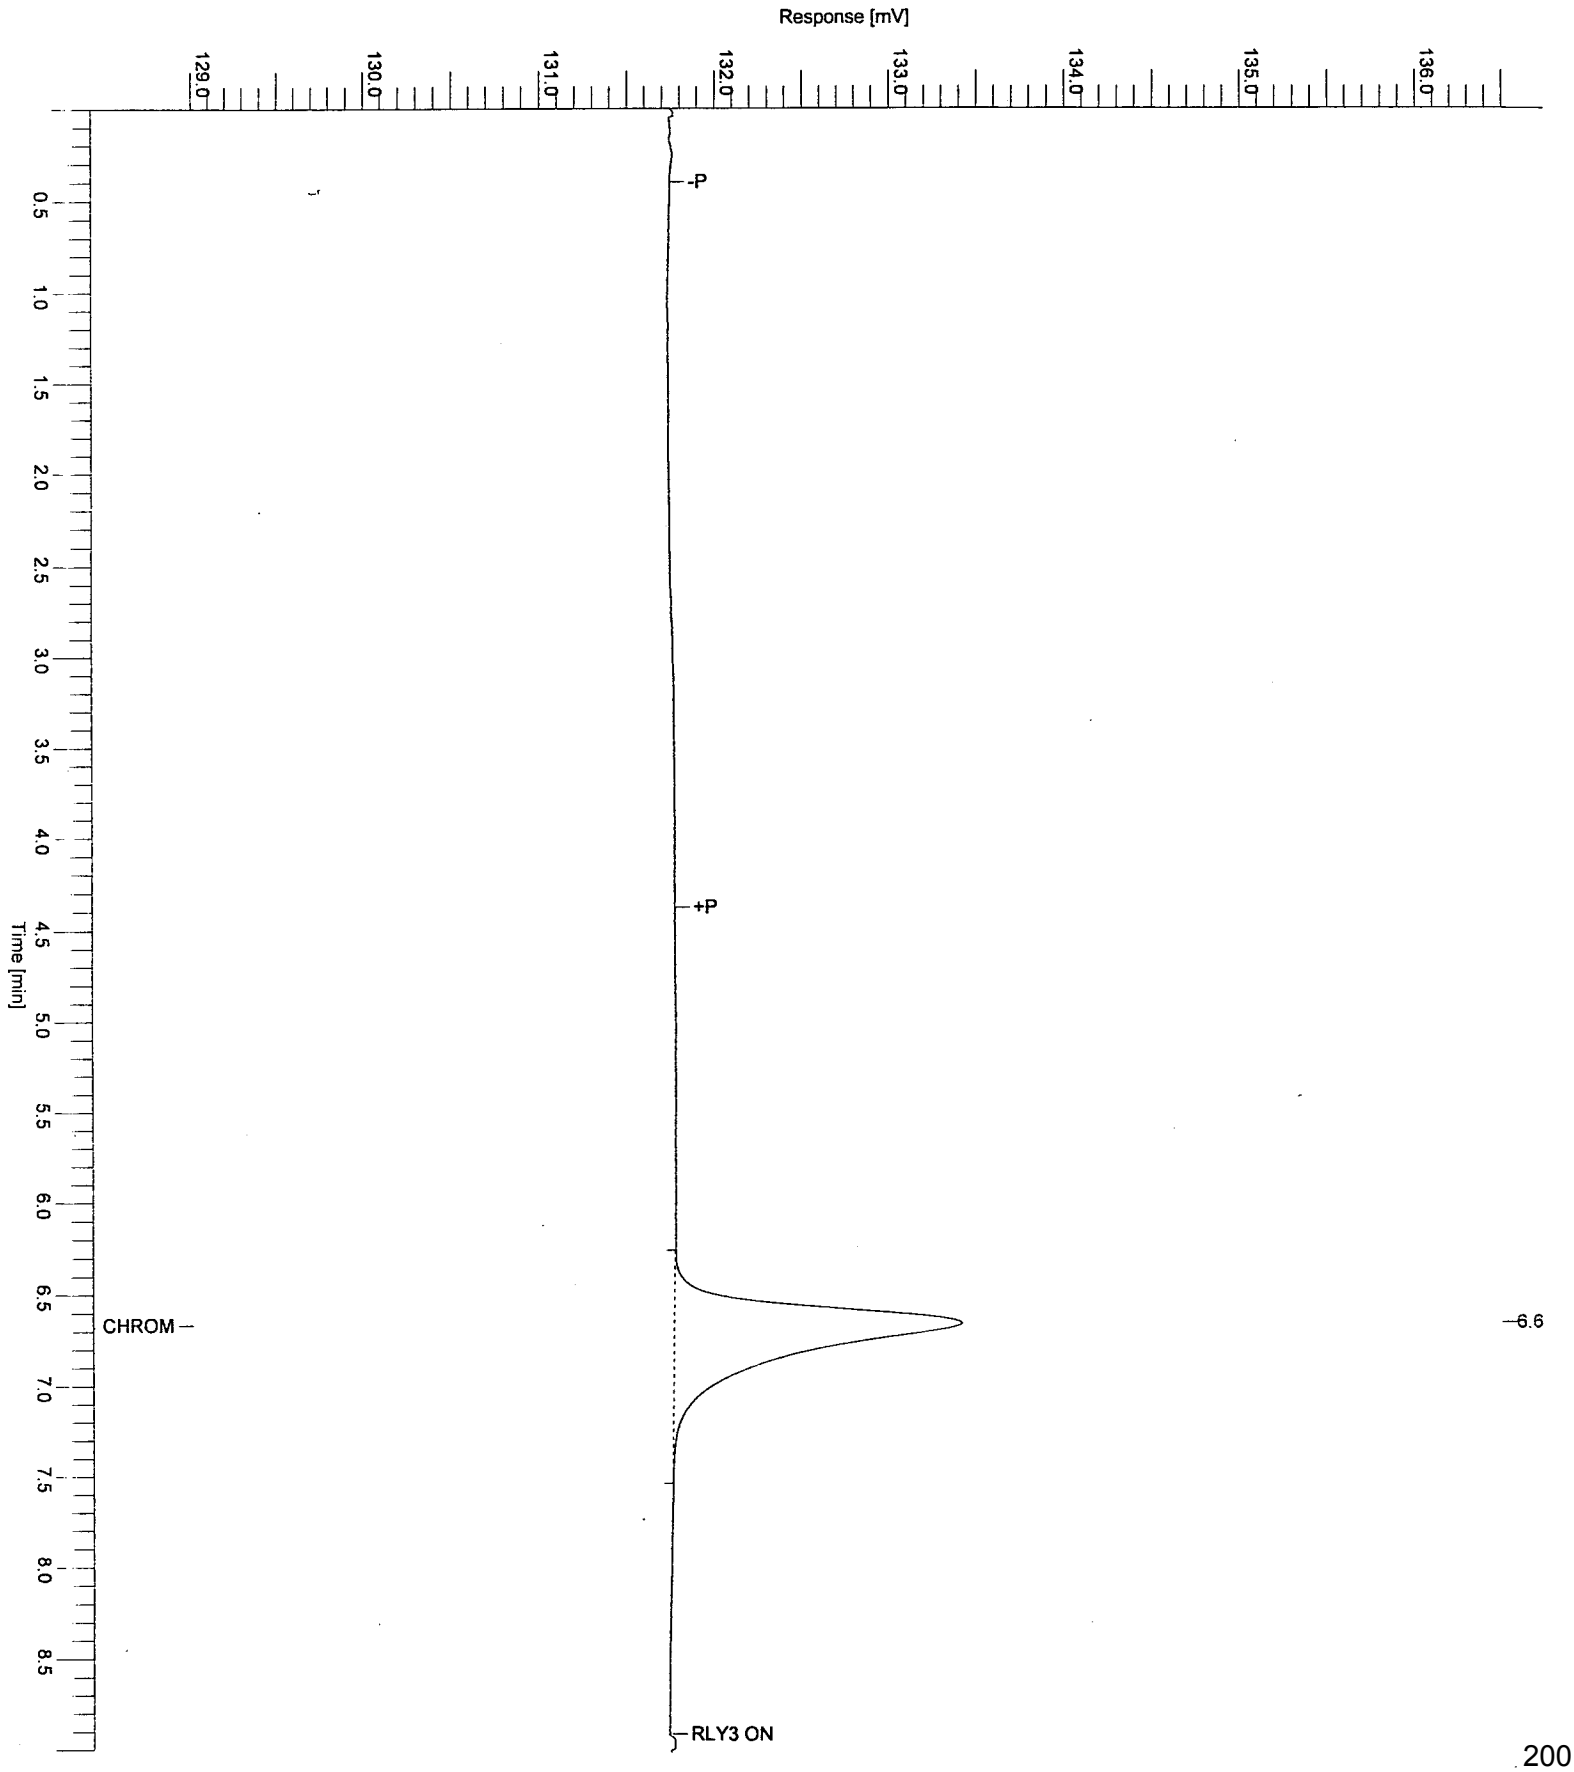

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 1:54:40 PM
Reprocess Number	: ic2: 90553		
Operator	: inorg	Sample Name	: CCB
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 1:45:25 PM	Cycle	: 10

Raw Data File : h:\data\ic4\20070717\20070717010.raw
Result File : h:\data\ic4\20070717\20070717010.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717010.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717010.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717010.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
-	7.007	chrom6	0.00	0.00000	0.0000	0.0000	
			0.00	0.00000	0.0000	0.0000	

Report stored in ASCII file: h:\data\ic4\20070717\20070717010.TX0

Chromatogram

Sample Name : CCB Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717010.raw
Date : 7/17/2007 1:54:41 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 1:45:25 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

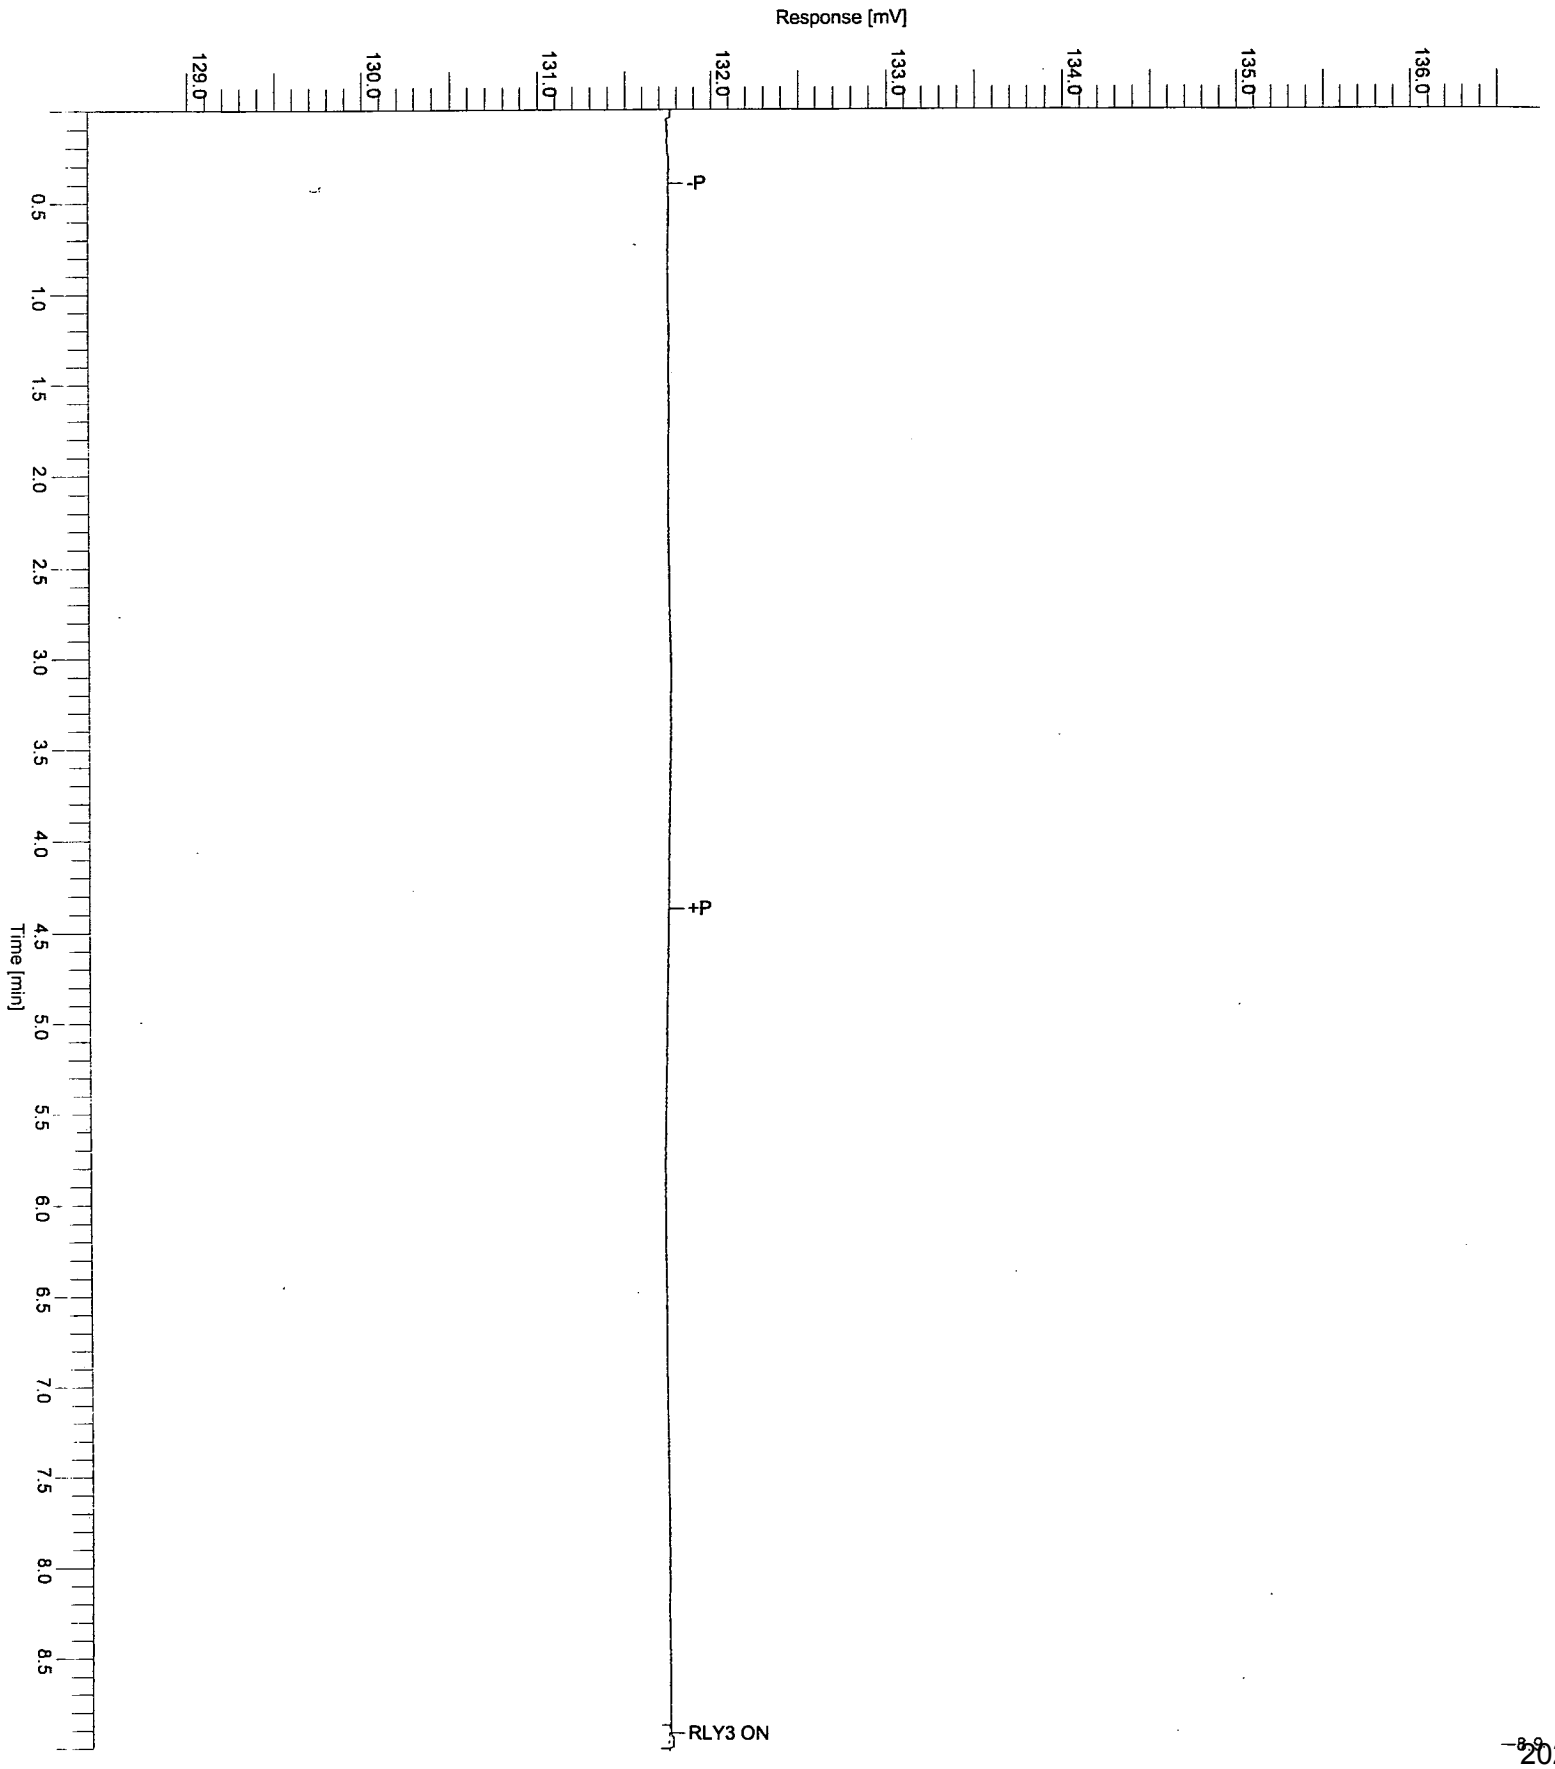

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 4:55:13 PM
Reprocess Number	: ic2: 90569		
Operator	: inorg	Sample Name	: CCV
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 4:46:02 PM	Cycle	: 11

Raw Data File : h:\data\ic4\20070717\20070717011.raw
Result File : h:\data\ic4\20070717\20070717011.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717011.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717011.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717011.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.719	chrom6	26713.25	1.581e+03	49.5286	49.5286	*
			26713.25	1.581e+03	49.5286	49.5286	

* Warning – uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070717\20070717011.TX0

Chromatogram

Sample Name : CCV Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717011.raw
Date : 7/17/2007 4:55:15 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 4:46:02 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

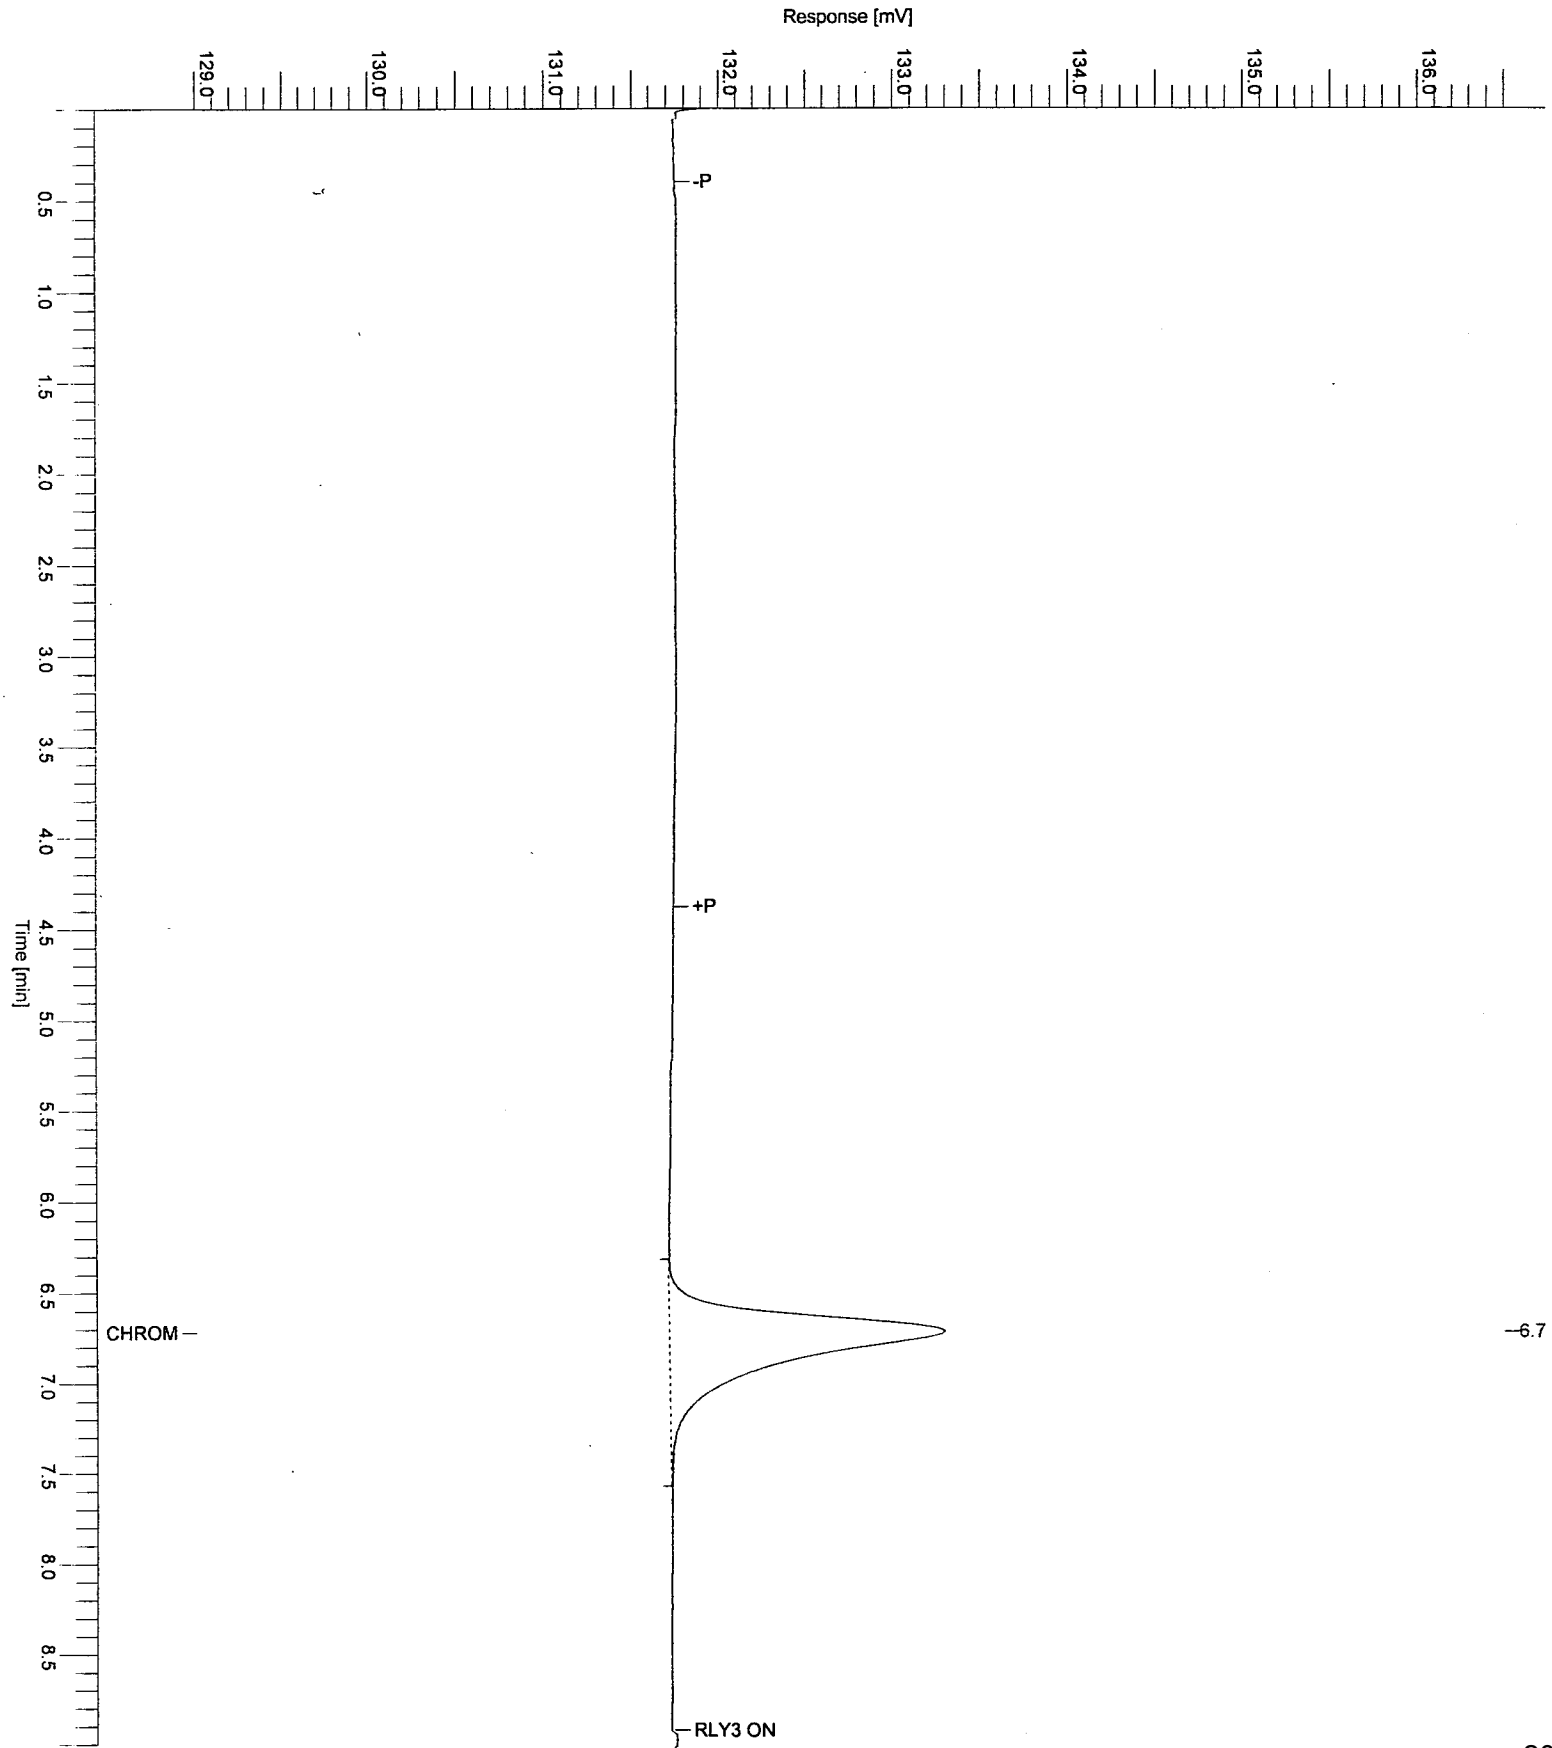

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 5:06:24 PM
Reprocess Number	: ic2: 90571		
Operator	: inorg	Sample Name	: CCB
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 4:57:11 PM	Cycle	: 12

Raw Data File : h:\data\ic4\20070717\20070717012.raw
Result File : h:\data\ic4\20070717\20070717012.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717012.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717012.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717012.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.686	chrom6	88.00	13.23895	0.3693	0.3693	*
			88.00	13.23895	0.3693	0.3693	

* Warning -- uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070717\20070717012.TX0

Chromatogram

Sample Name : CCB Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717012.raw
Date : 7/17/2007 5:06:25 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 4:57:11 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

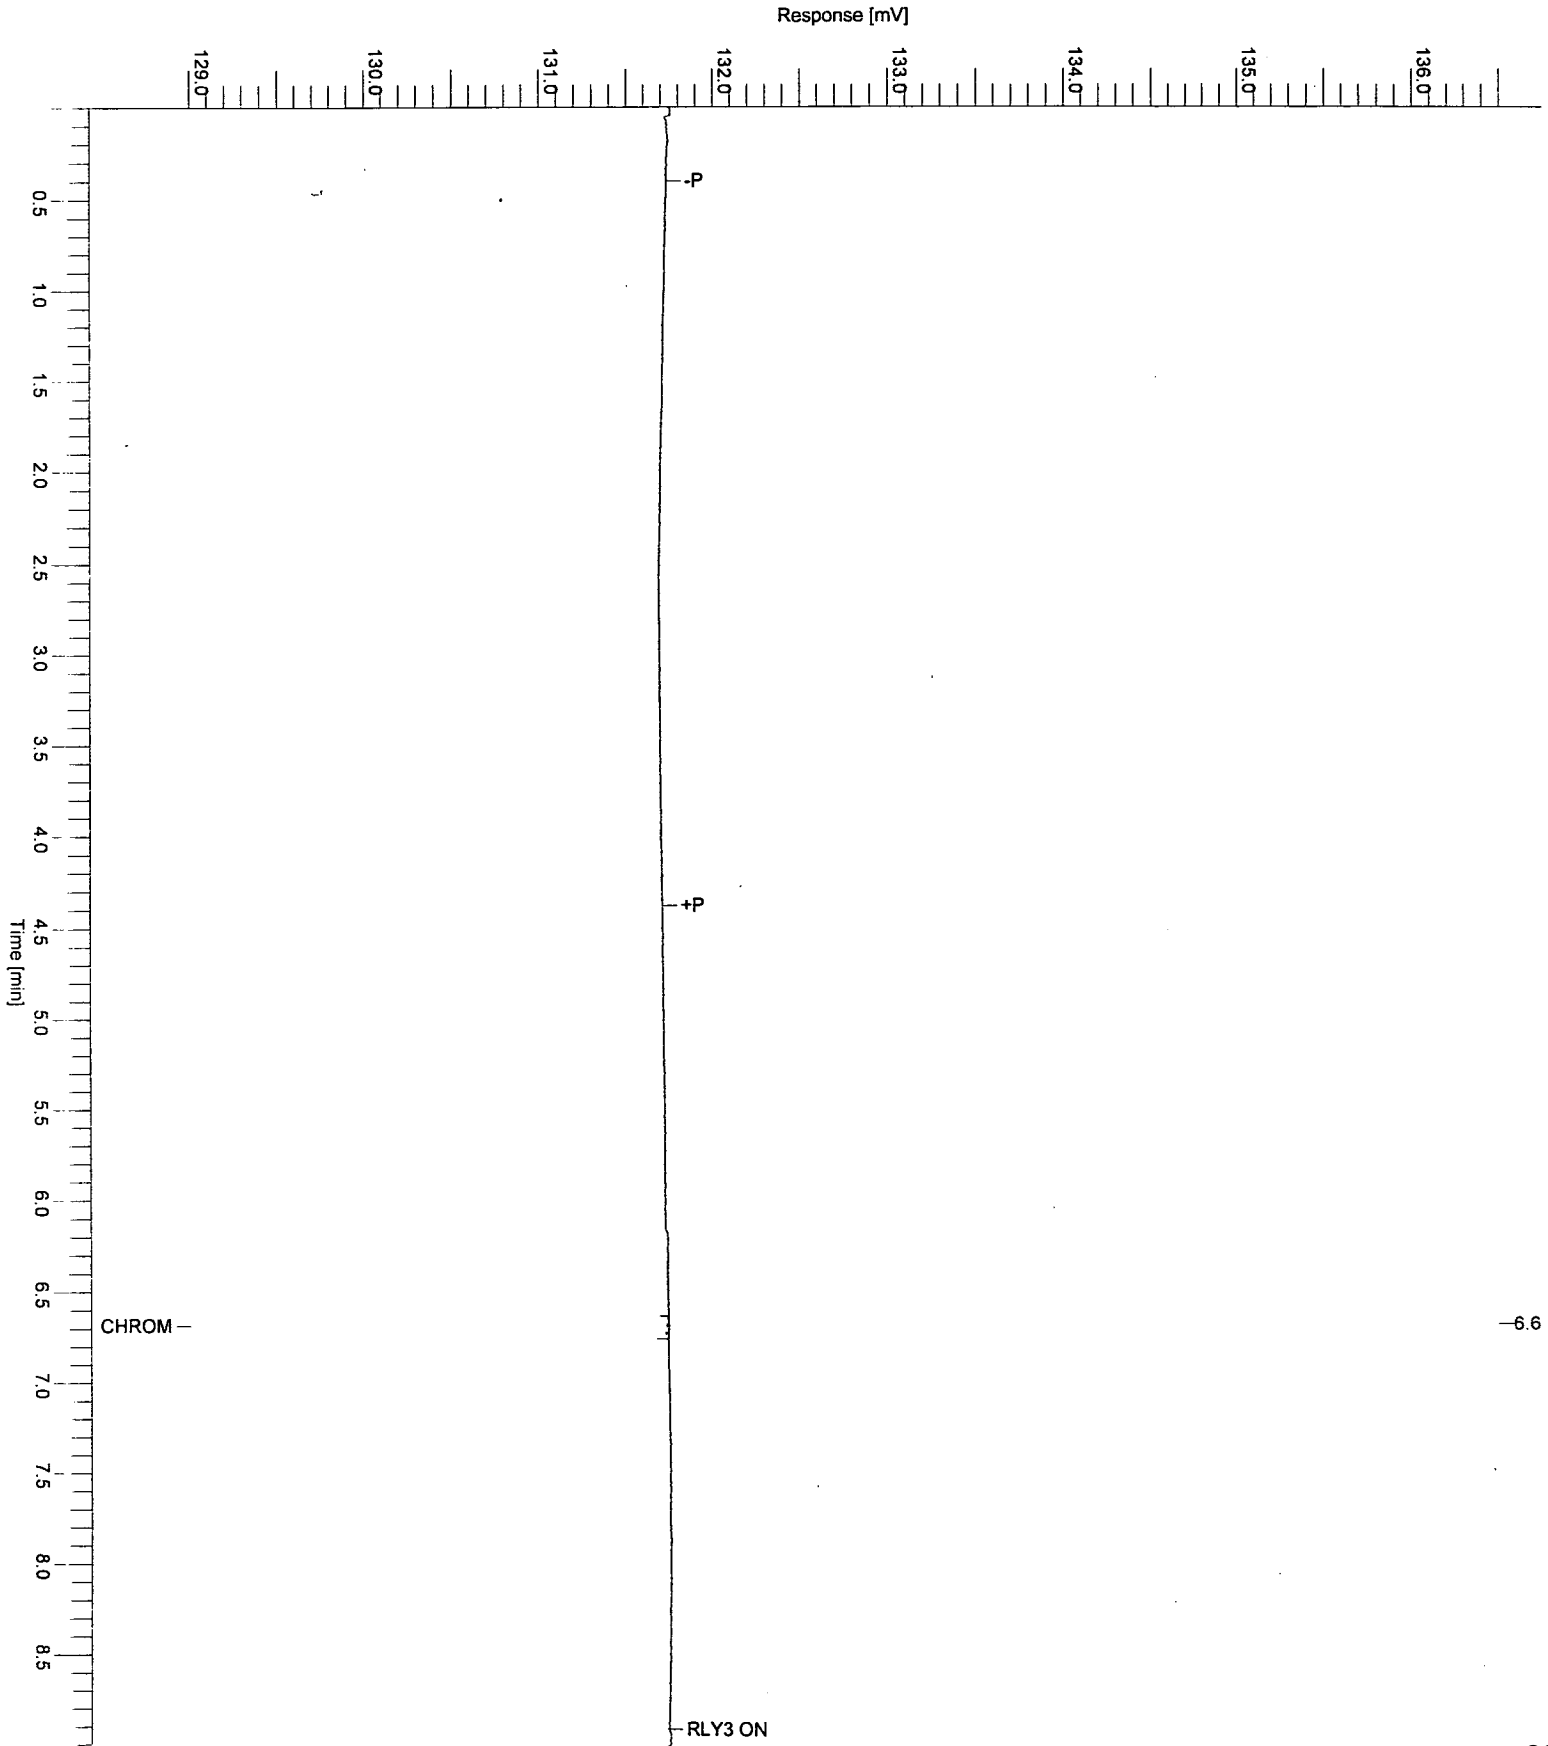

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 5:23:41 PM
Reprocess Number	: ic2: 90574		
Operator	: inorg	Sample Name	: CCB
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 5:14:25 PM	Cycle	: 13

Raw Data File : h:\data\ic4\20070717\20070717013.raw
Result File : h:\data\ic4\20070717\20070717013.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717013.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717013.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717013.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
-	7.007	chrom6	0.00	0.00000	0.0000	0.0000	
			0.00	0.00000	0.0000	0.0000	

Report stored in ASCII file: h:\data\ic4\20070717\20070717013.TX0

Chromatogram

Sample Name : CCB Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717013.raw
Date : 7/17/2007 5:23:43 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 5:14:25 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

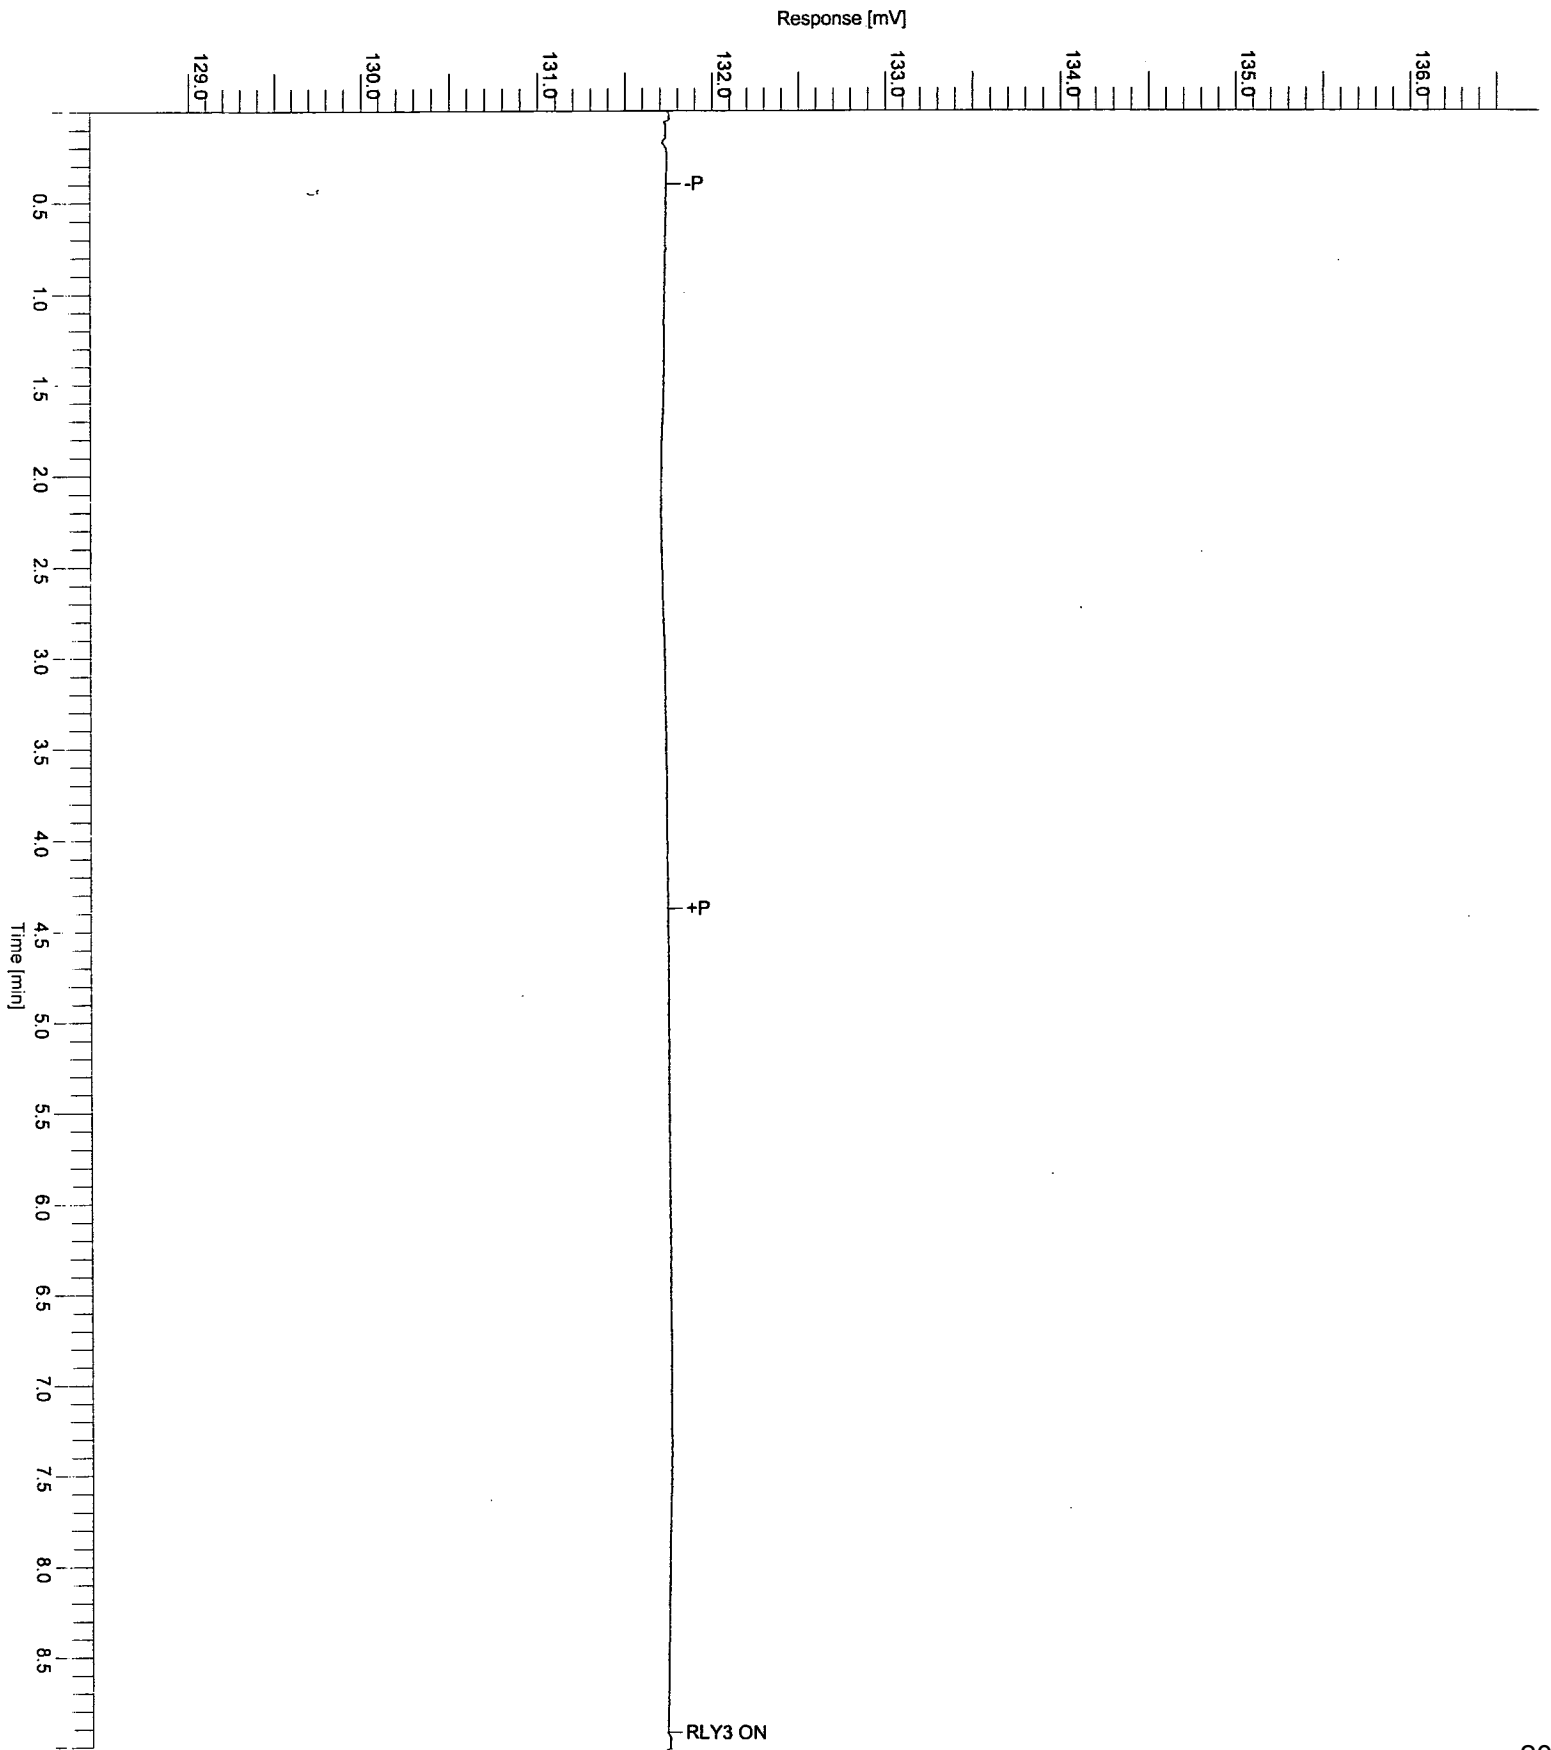

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 5:34:51 PM
Reprocess Number	: ic2: 90575		
Operator	: inorg	Sample Name	: IQG1460-01
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 5:25:35 PM	Cycle	: 14

Raw Data File : h:\data\ic4\20070717\20070717014.raw
Result File : h:\data\ic4\20070717\20070717014.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717014.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717014.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717014.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.520	chrom6	1365.00	64.89658	1.9888	1.9888	*
			1365.00	64.89658	1.9888	1.9888	

* Warning -- uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070717\20070717014.TX0

Chromatogram

Sample Name : IQG1460-01 Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717014.raw
Date : 7/17/2007 5:34:53 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 5:25:35 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

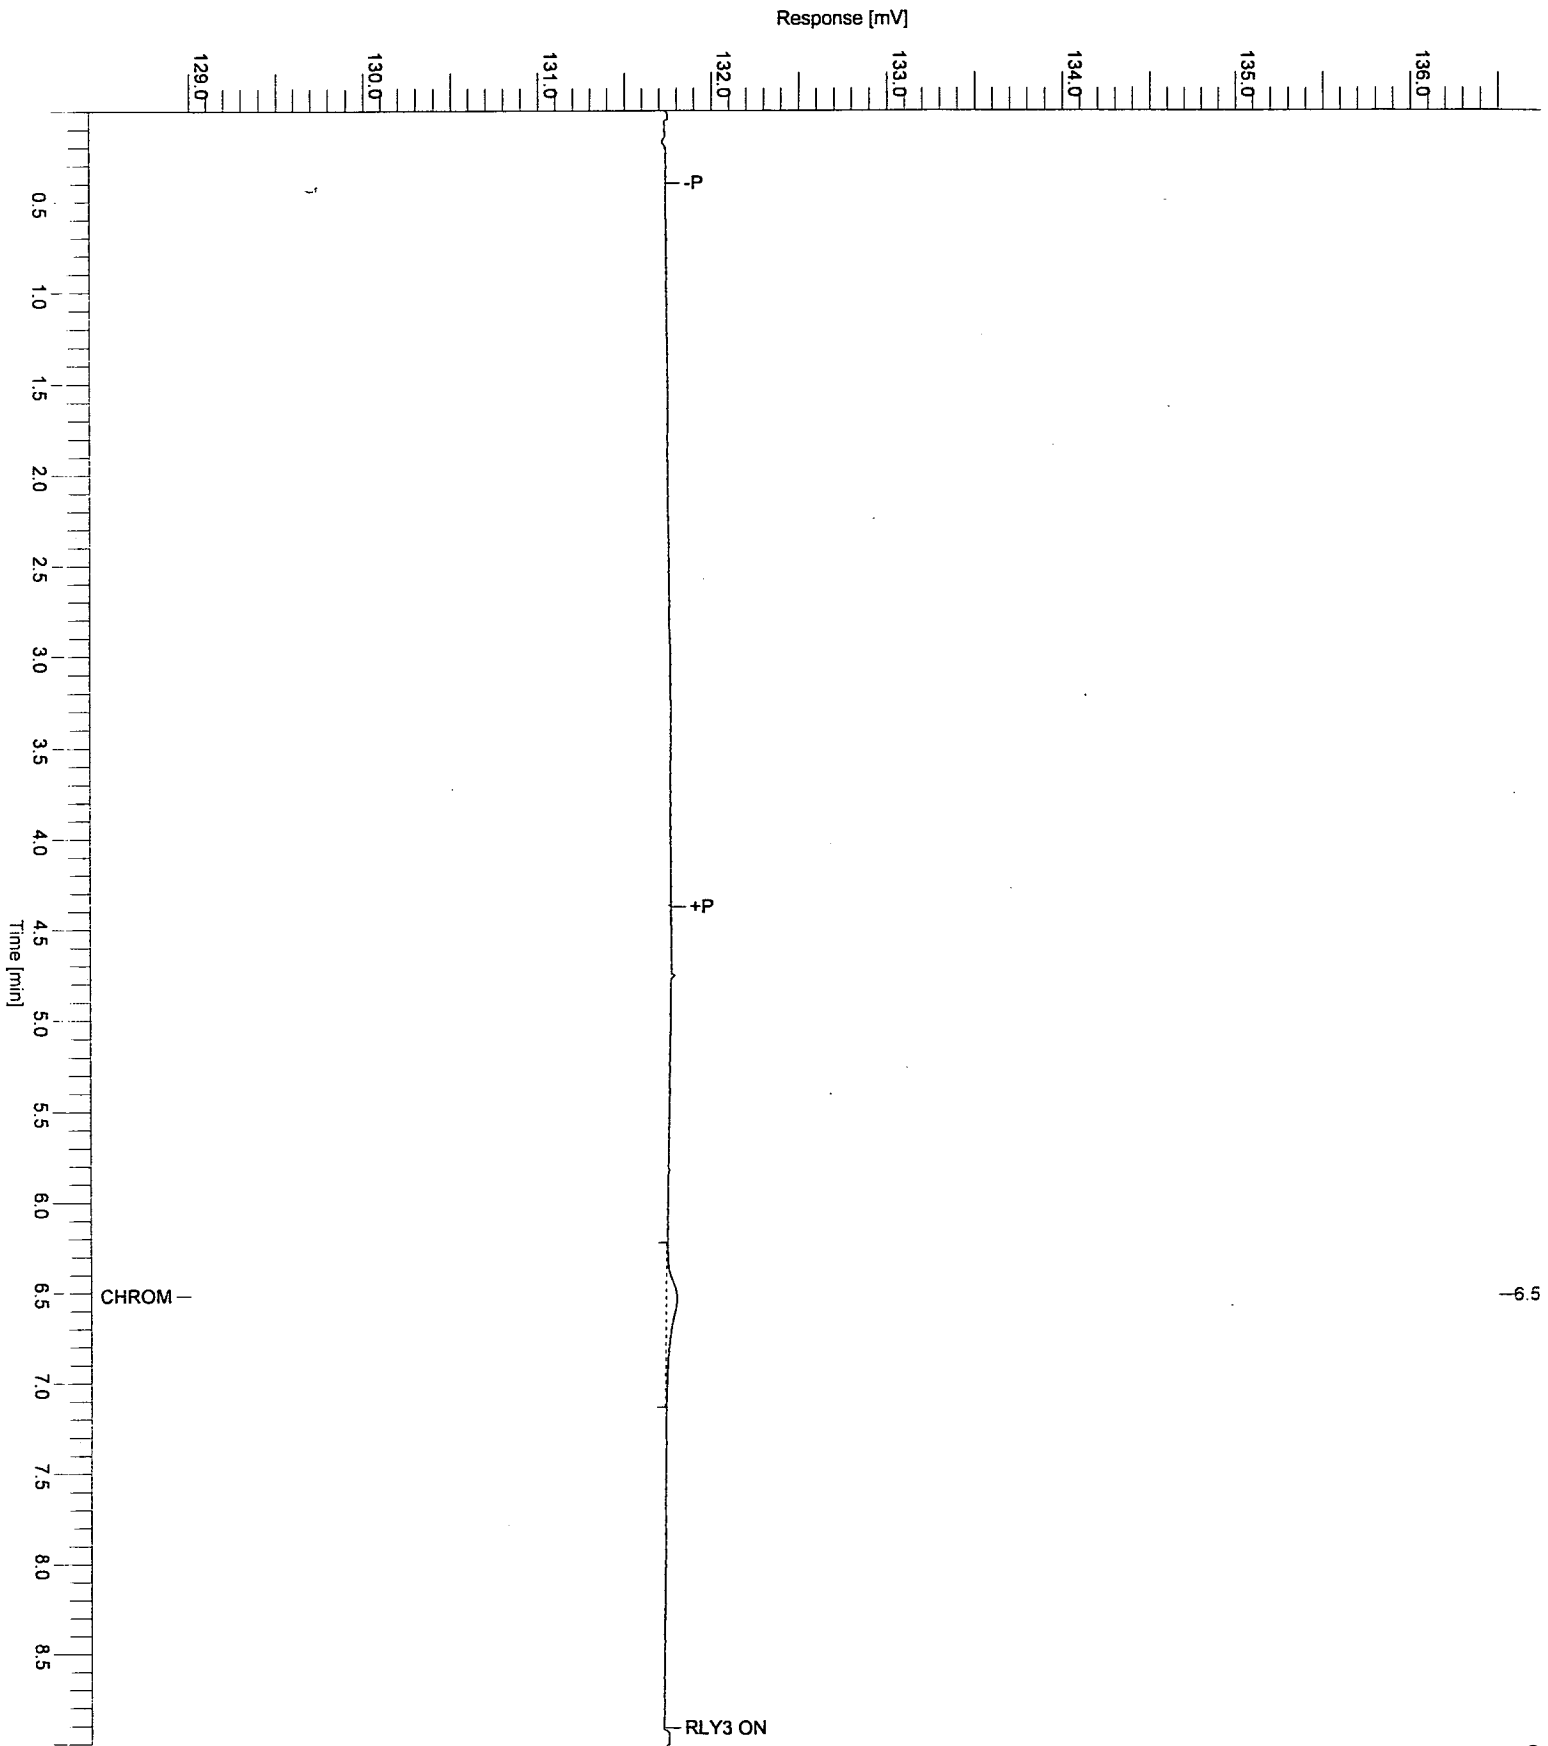

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 5:46:00 PM
Reprocess Number	: ic2: 90578		
Operator	: inorg	Sample Name	: IQG1460-02
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 5:36:44 PM	Cycle	: 15

Raw Data File : h:\data\ic4\20070717\20070717015.raw
Result File : h:\data\ic4\20070717\20070717015.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717015.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717015.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717015.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.598	chrom6	3514.50	181.20950	5.6354	5.6354	*
			3514.50	181.20950	5.6354	5.6354	

* Warning -- uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070717\20070717015.TX0

Chromatogram

Sample Name : IQG1460-02 Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717015.raw
Date : 7/17/2007 5:46:02 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 5:36:44 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

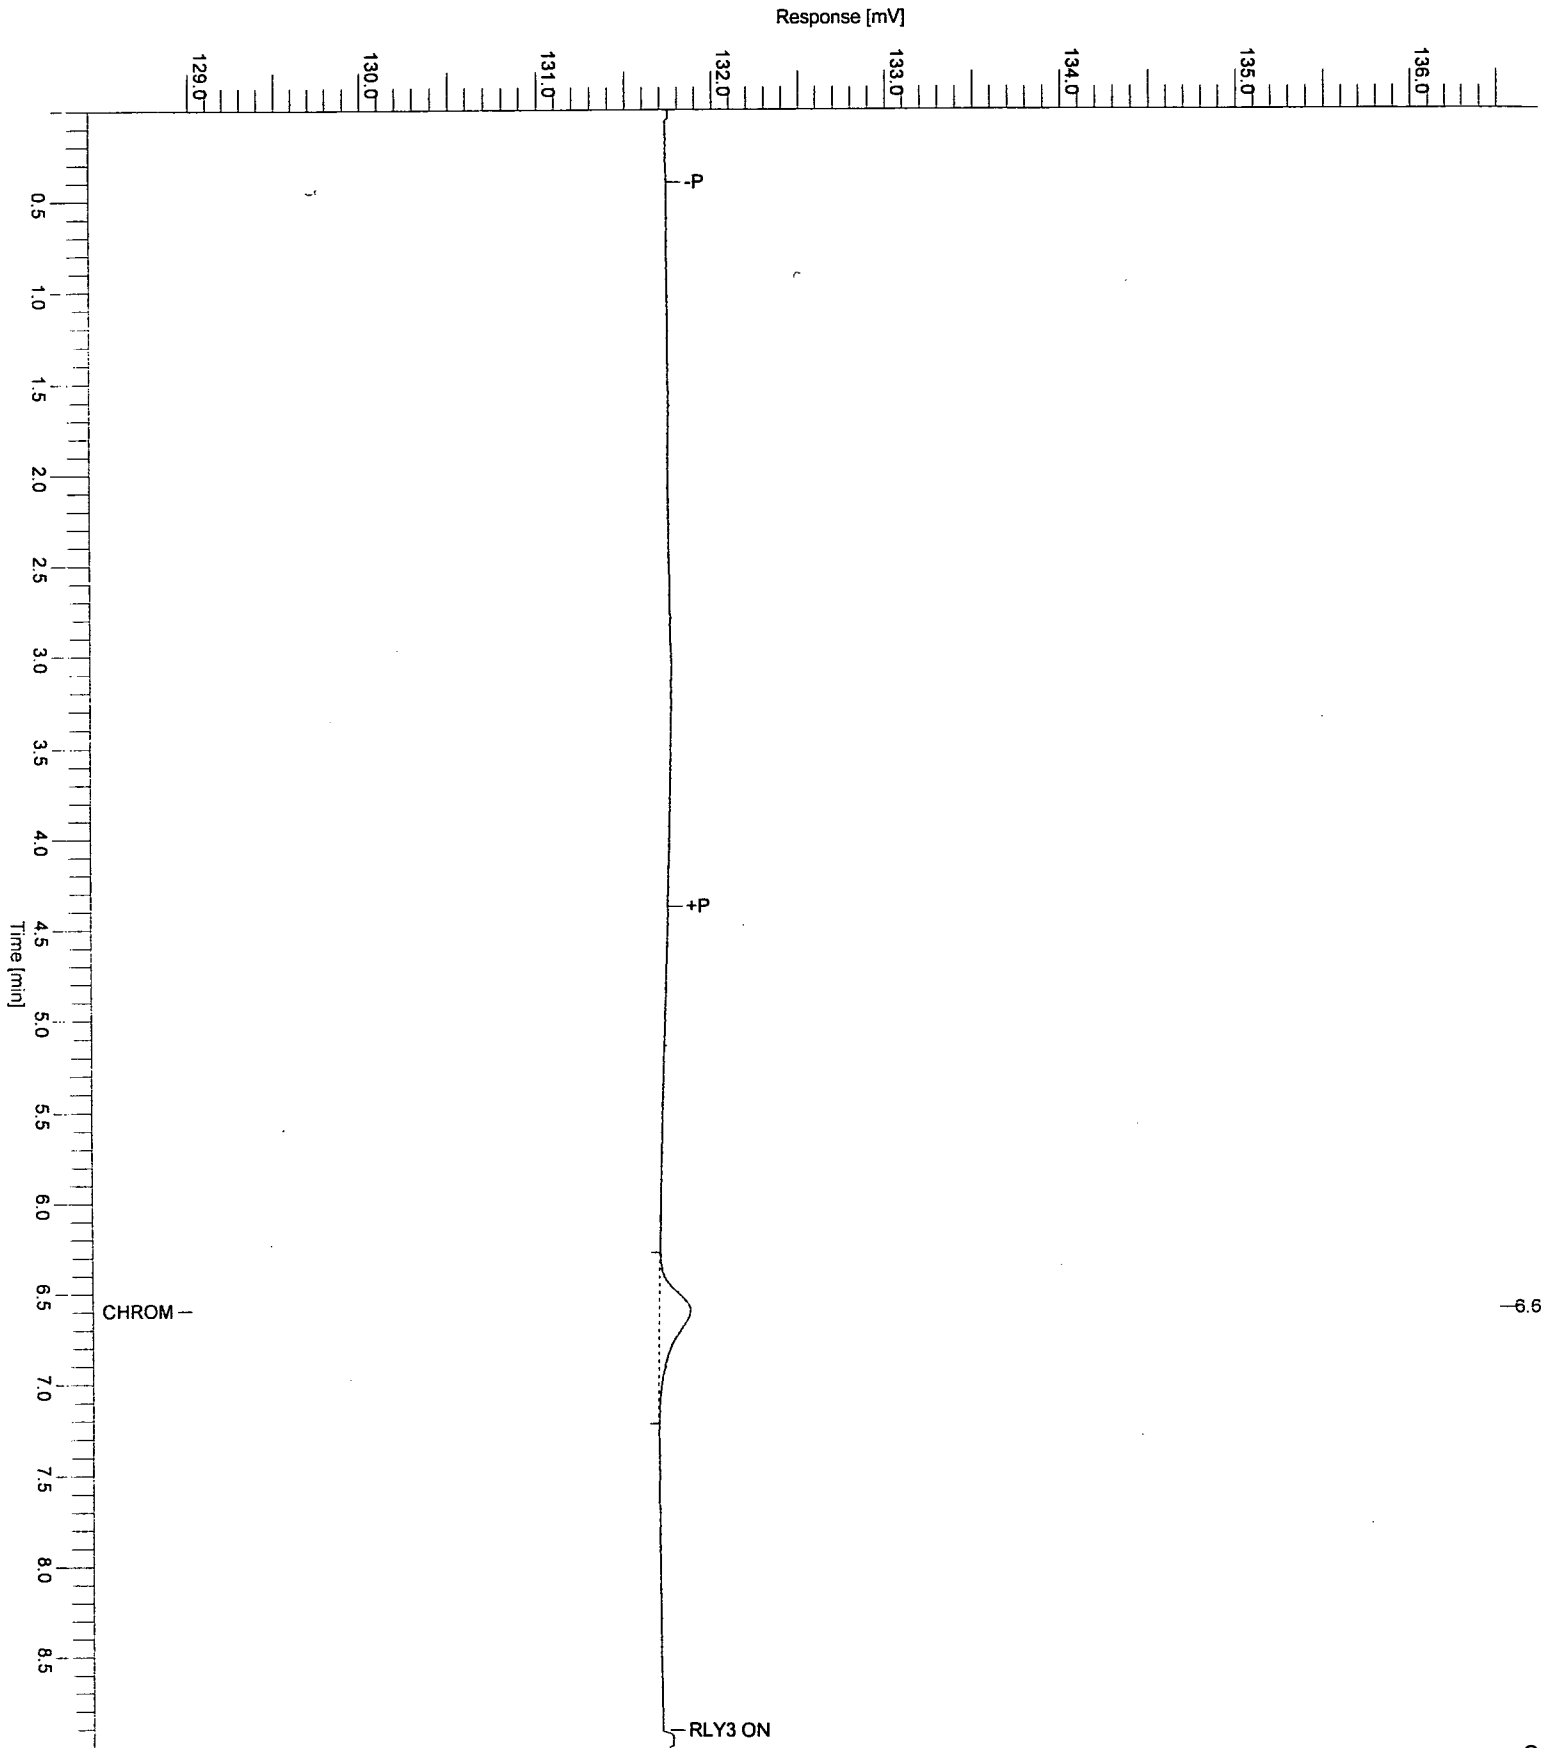

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 5:57:07 PM
Reprocess Number	: ic2: 90579		
Operator	: inorg	Sample Name	: IQG1460-03
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 5:47:53 PM	Cycle	: 16

Raw Data File : h:\data\ic4\20070717\20070717016.raw
Result File : h:\data\ic4\20070717\20070717016.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717016.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717016.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717016.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.624	chrom6	5123.75	263.12758	8.2037	8.2037	*
			5123.75	263.12758	8.2037	8.2037	

* Warning -- uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070717\20070717016.TX0

Chromatogram

Sample Name : IQG1460-03 Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717016.raw
Date : 7/17/2007 5:57:08 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 5:47:53 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

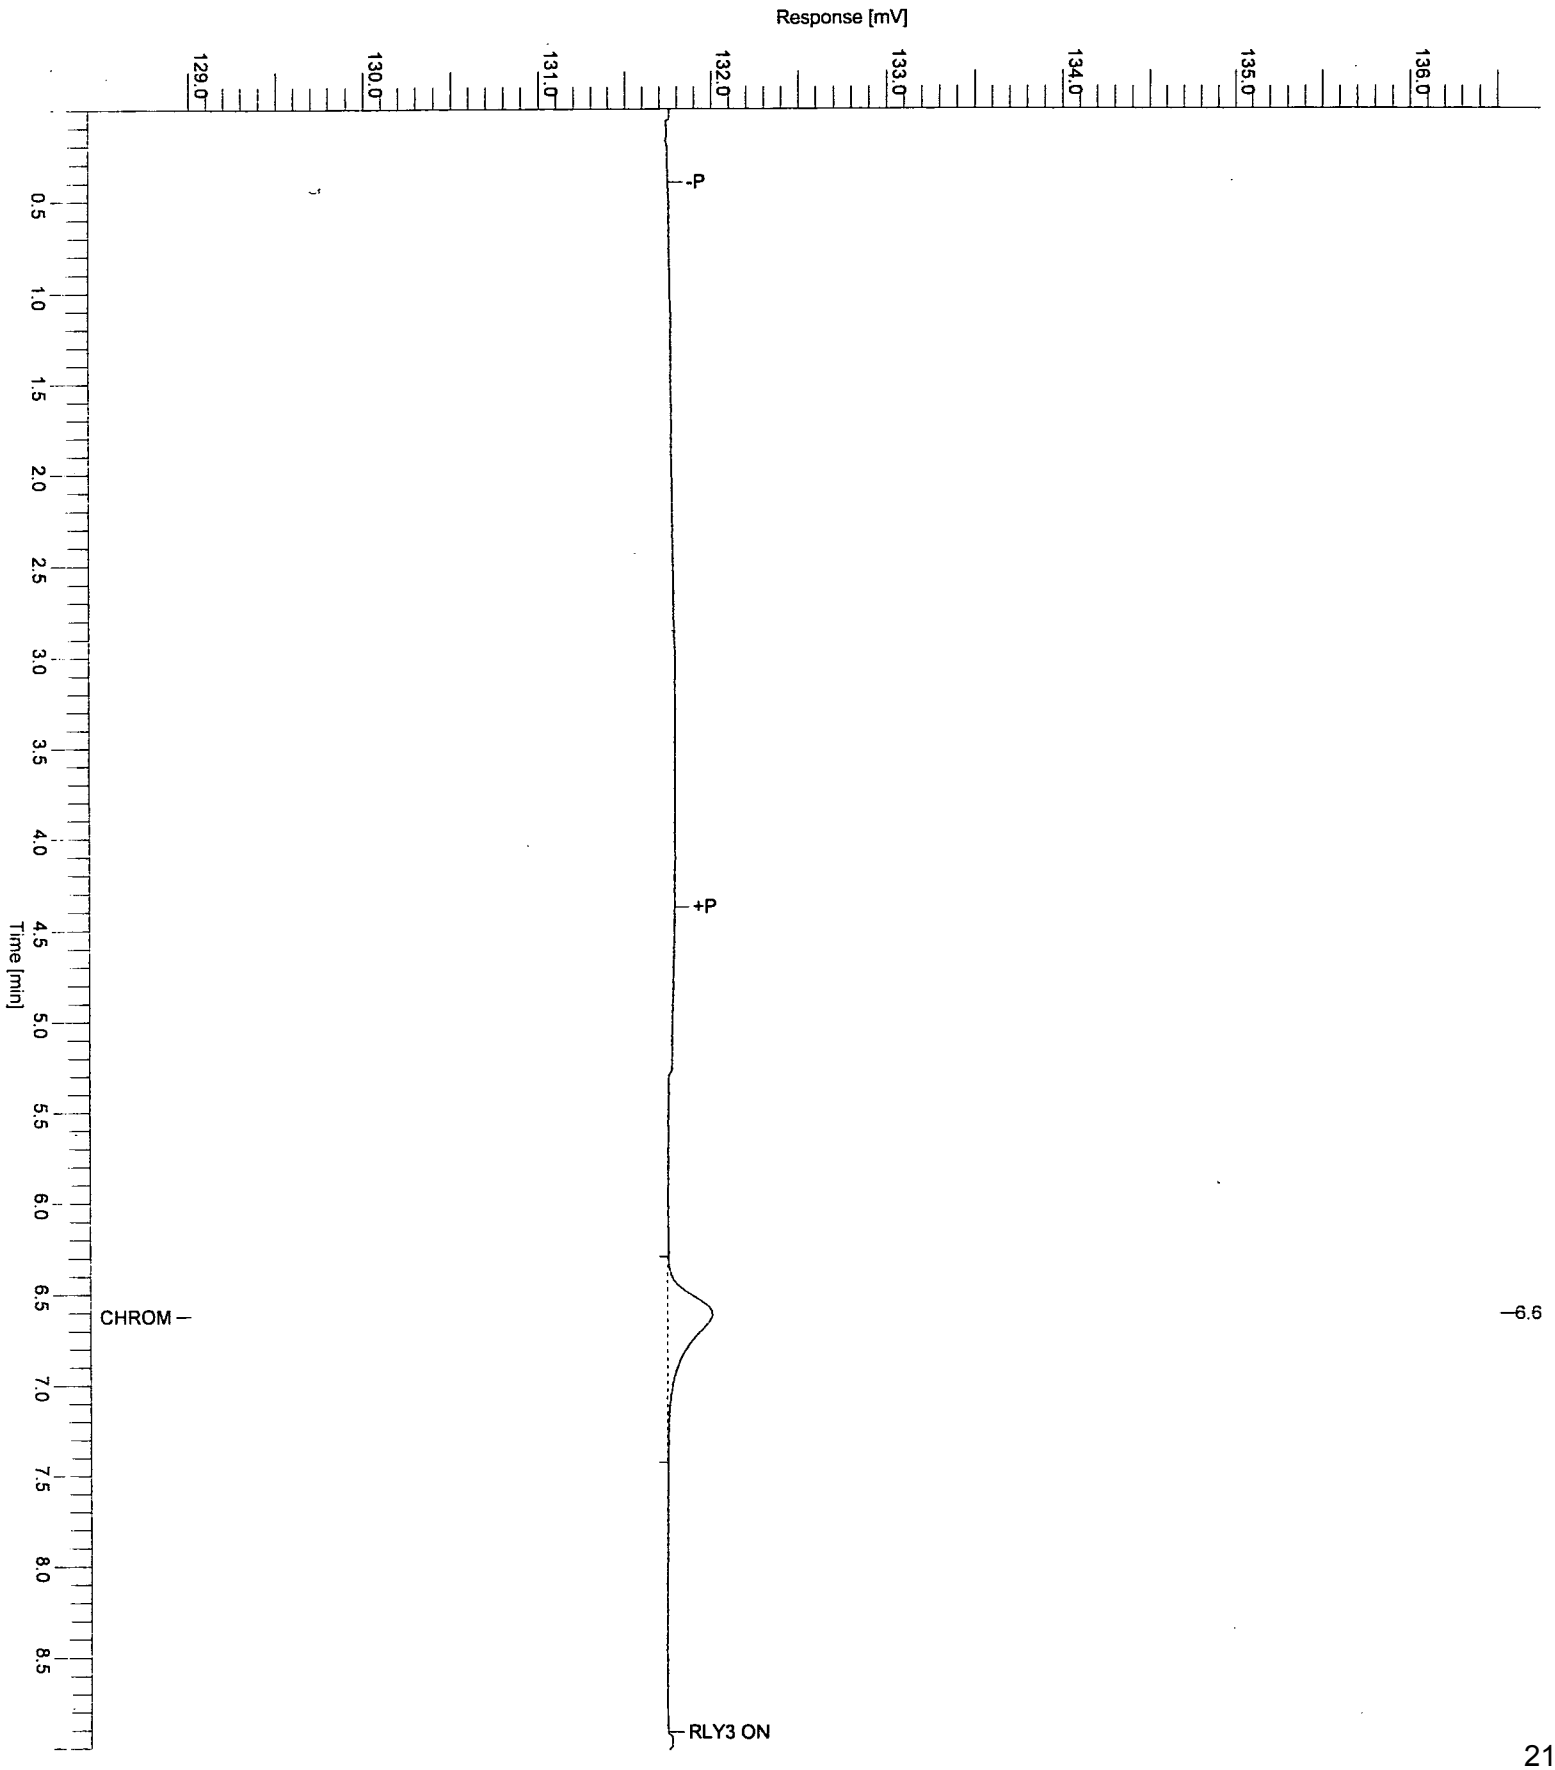

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 6:08:15 PM
Reprocess Number	: ic2: 90582		
Operator	: inorg	Sample Name	: IQG1460-04
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 5:59:02 PM	Cycle	: 17

Raw Data File : h:\data\ic4\20070717\20070717017.raw
Result File : h:\data\ic4\20070717\20070717017.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717017.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717017.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717017.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

over range

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.526	chrom6	97243.80	5.305e+03	166.2627	166.2627	*
			97243.80	5.305e+03	166.2627	166.2627	

* Warning -- uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070717\20070717017.TX0

Chromatogram

Sample Name : IQG1460-04 Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717017.raw
Date : 7/17/2007 6:08:17 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 5:59:02 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

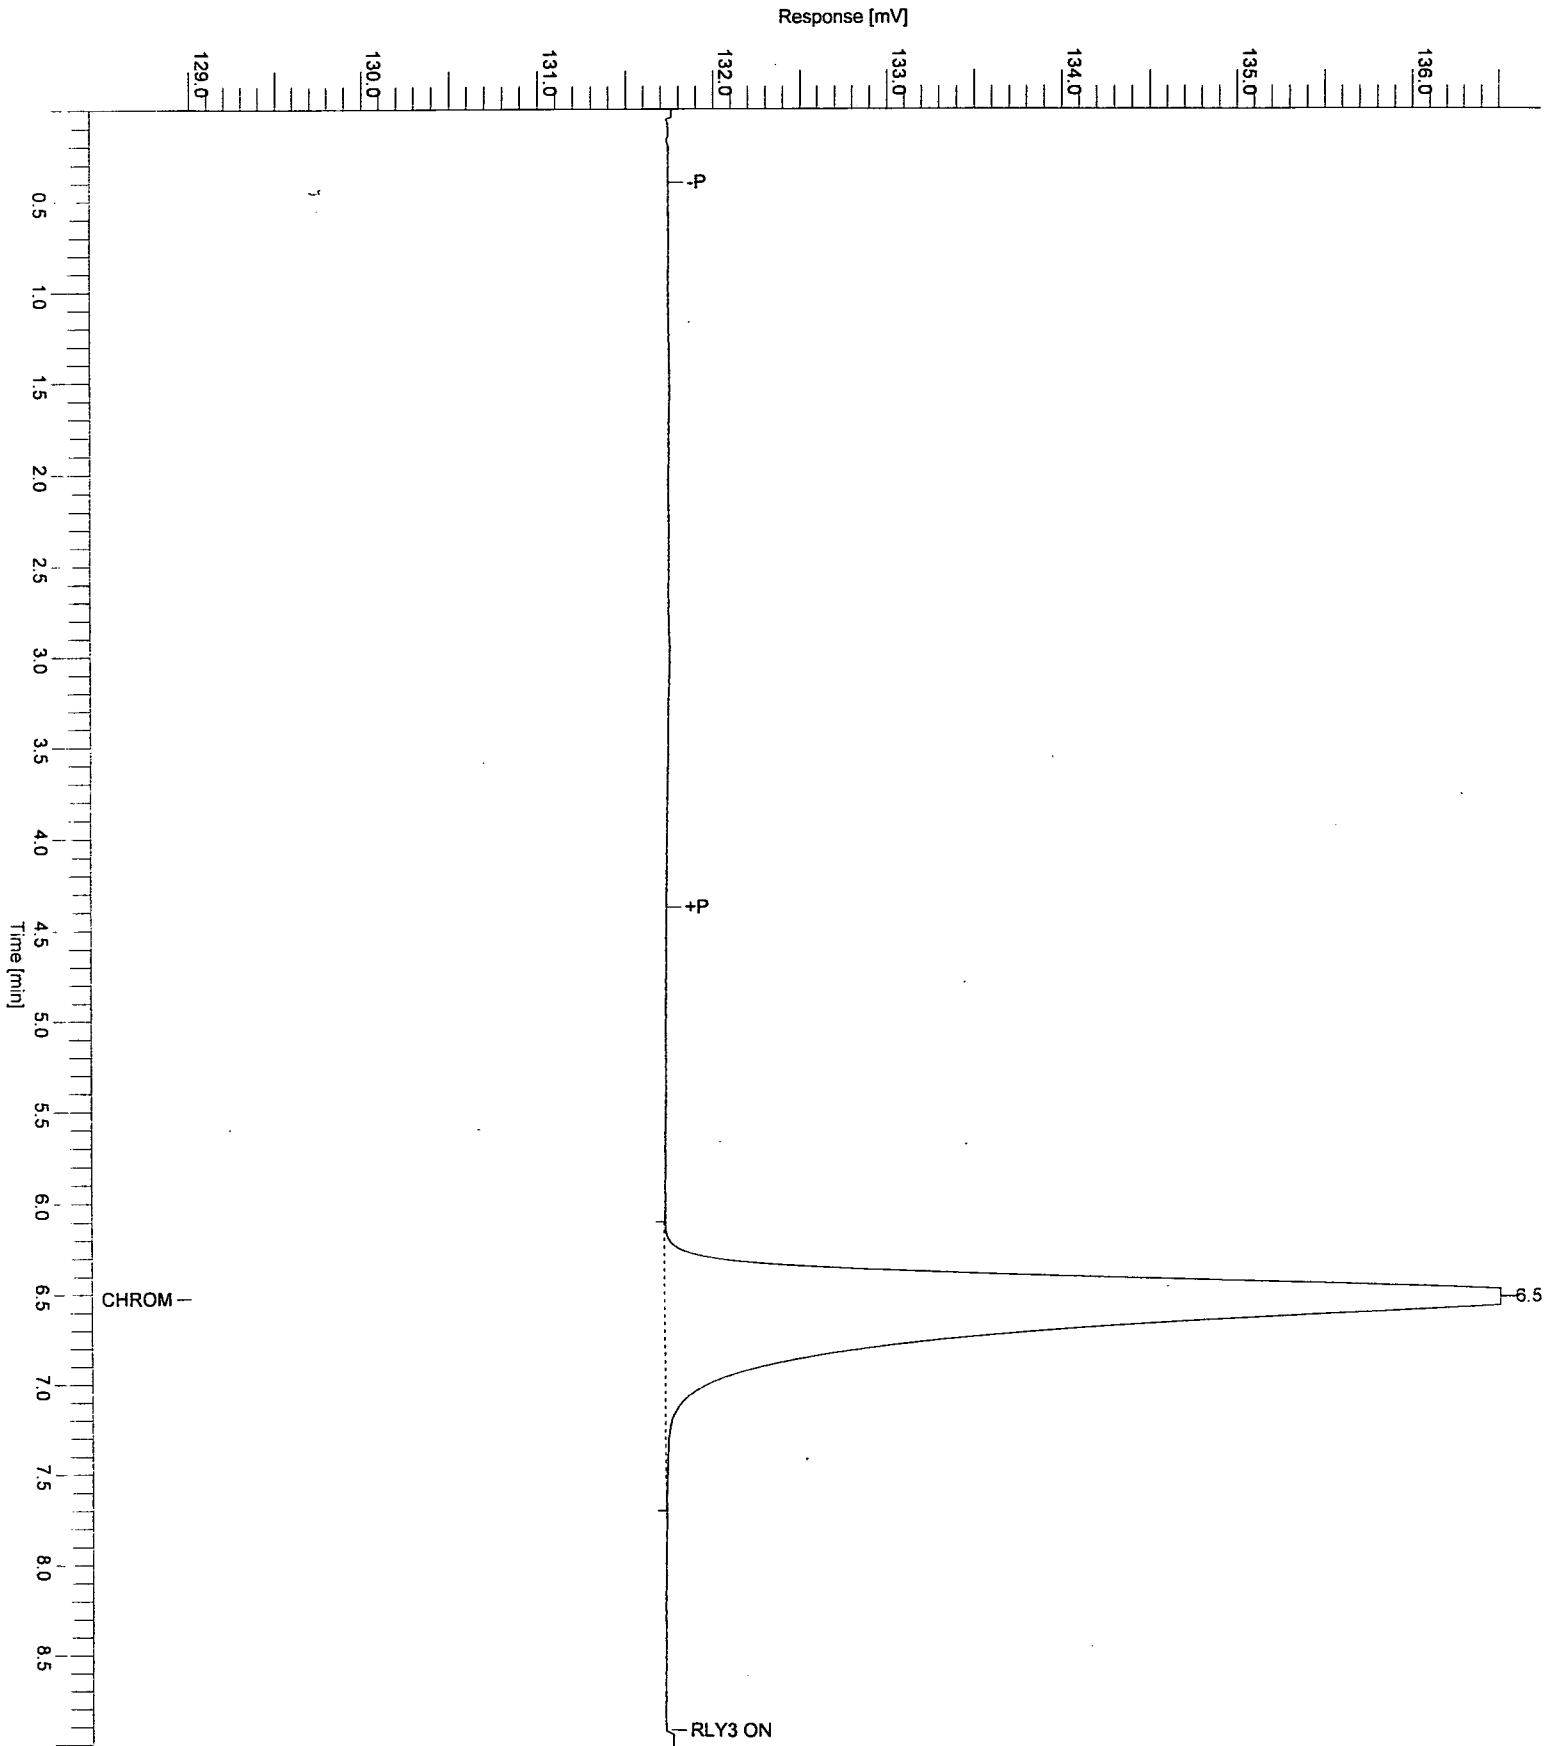

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 6:19:29 PM
Reprocess Number	: ic2: 90584		
Operator	: inorg	Sample Name	: IQG1460-05
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 6:10:11 PM	Cycle	: 18

Raw Data File : h:\data\ic4\20070717\20070717018.raw
Result File : h:\data\ic4\20070717\20070717018.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717018.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717018.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717018.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.603	chrom6	792.30	32.97160	0.9879	0.9879	*
			792.30	32.97160	0.9879	0.9879	

* Warning -- uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070717\20070717018.TX0

Chromatogram

Sample Name : IQG1460-05 Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717018.raw
Date : 7/17/2007 6:19:30 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 6:10:11 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

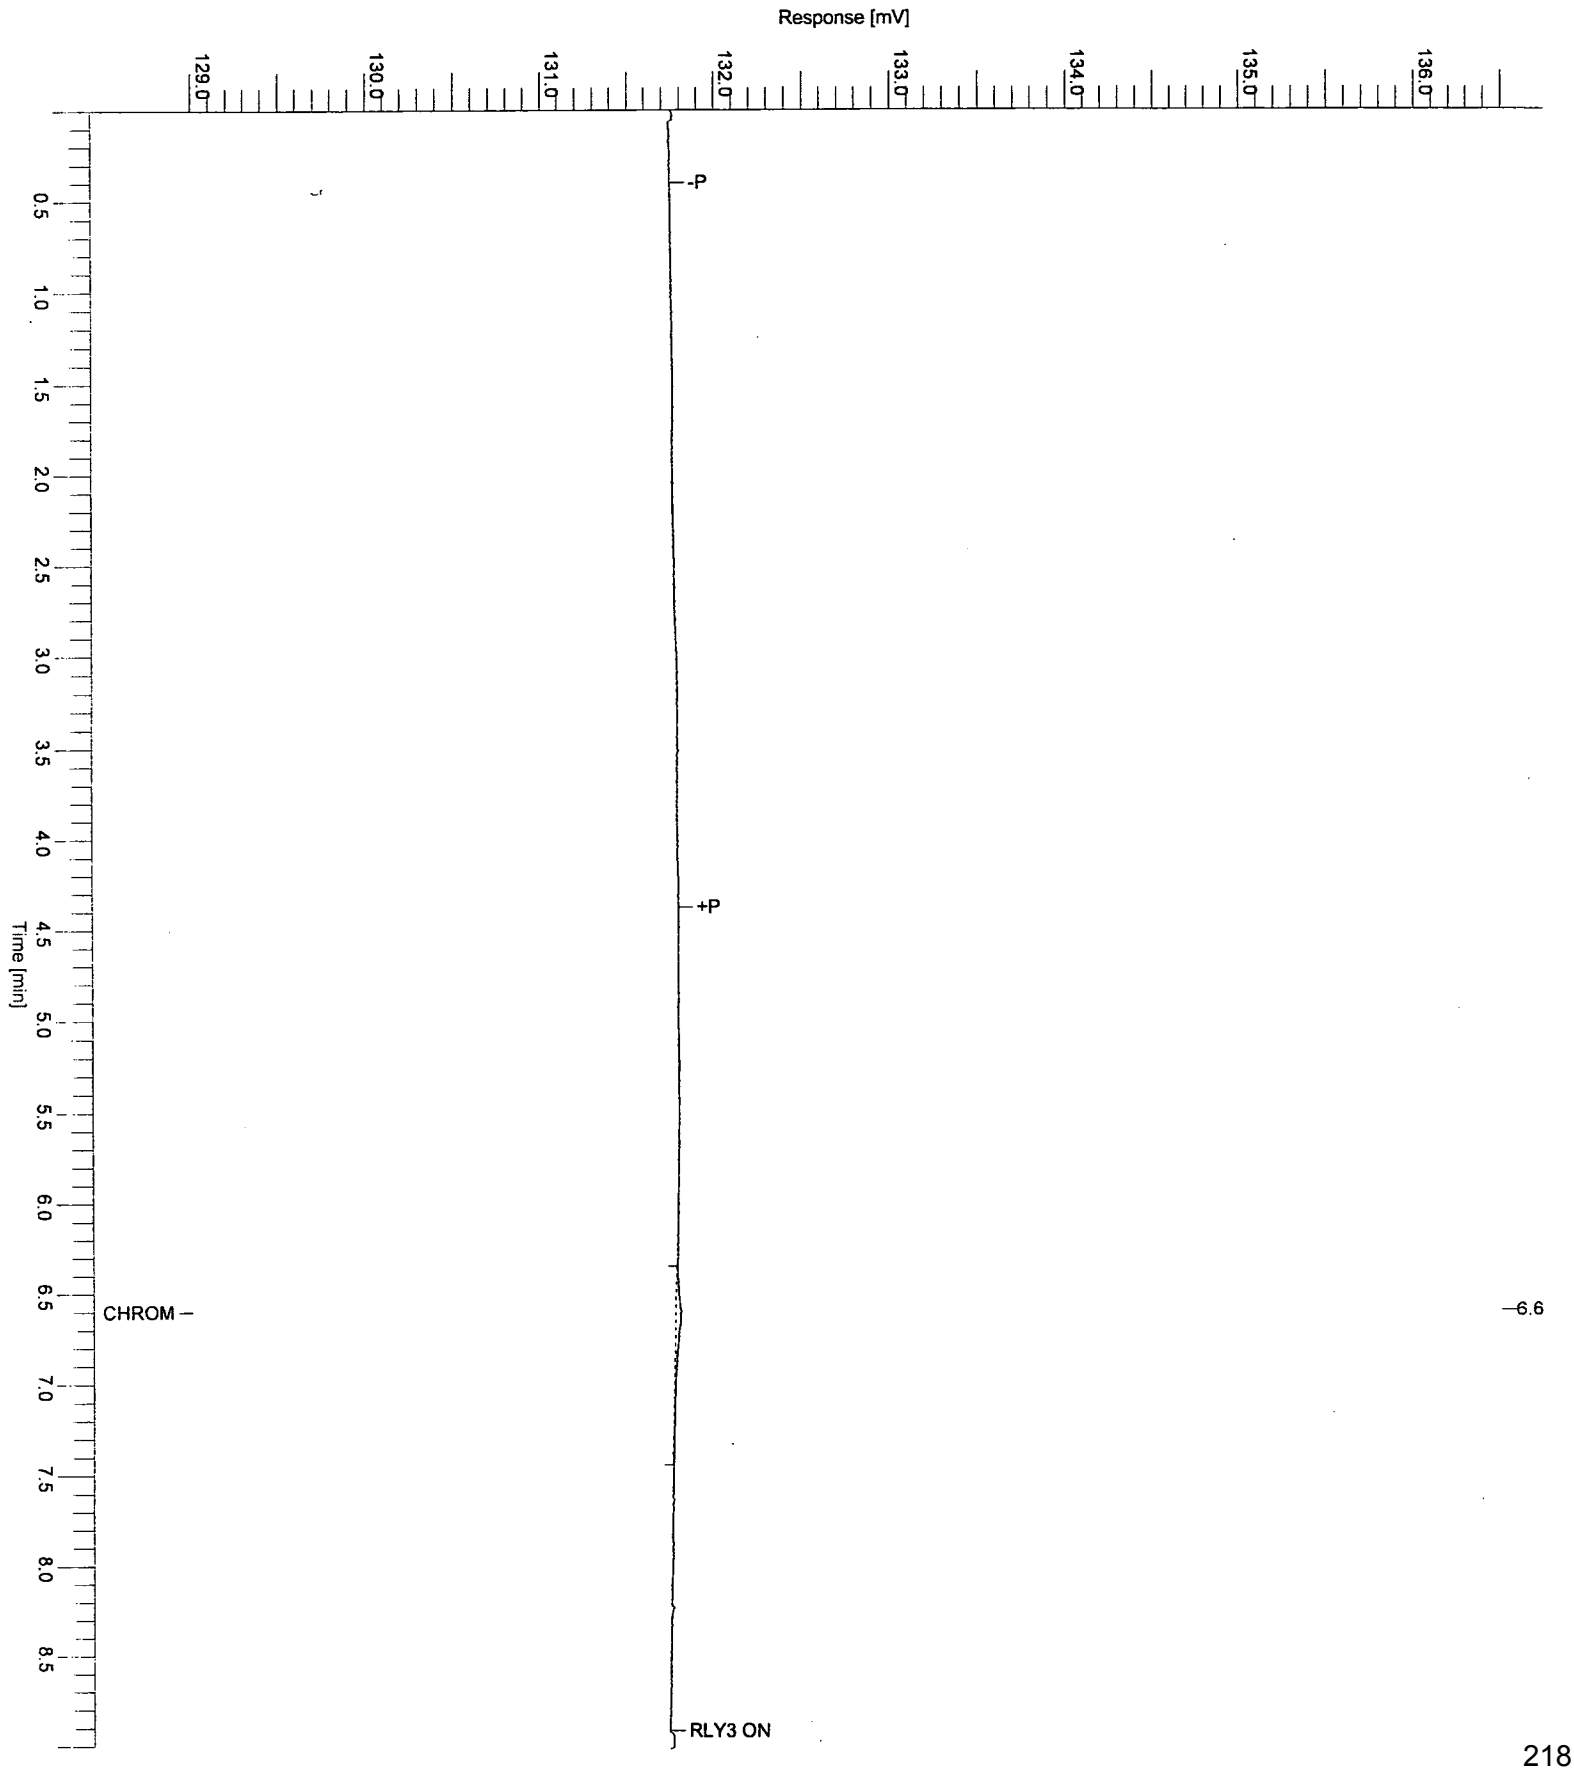

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 6:30:39 PM
Reprocess Number	: ic2: 90586		
Operator	: inorg	Sample Name	: IQG1460-06
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 6:21:20 PM	Cycle	: 19

Raw Data File : h:\data\ic4\20070717\20070717019.raw
Result File : h:\data\ic4\20070717\20070717019.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717019.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717019.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717019.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.599	chrom6	1181.50	54.71751	1.6697	1.6697	*
			1181.50	54.71751	1.6697	1.6697	

* Warning -- uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070717\20070717019.TX0

Chromatogram

Sample Name : IQG1460-06 Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717019.raw
Date : 7/17/2007 6:30:41 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 6:21:20 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

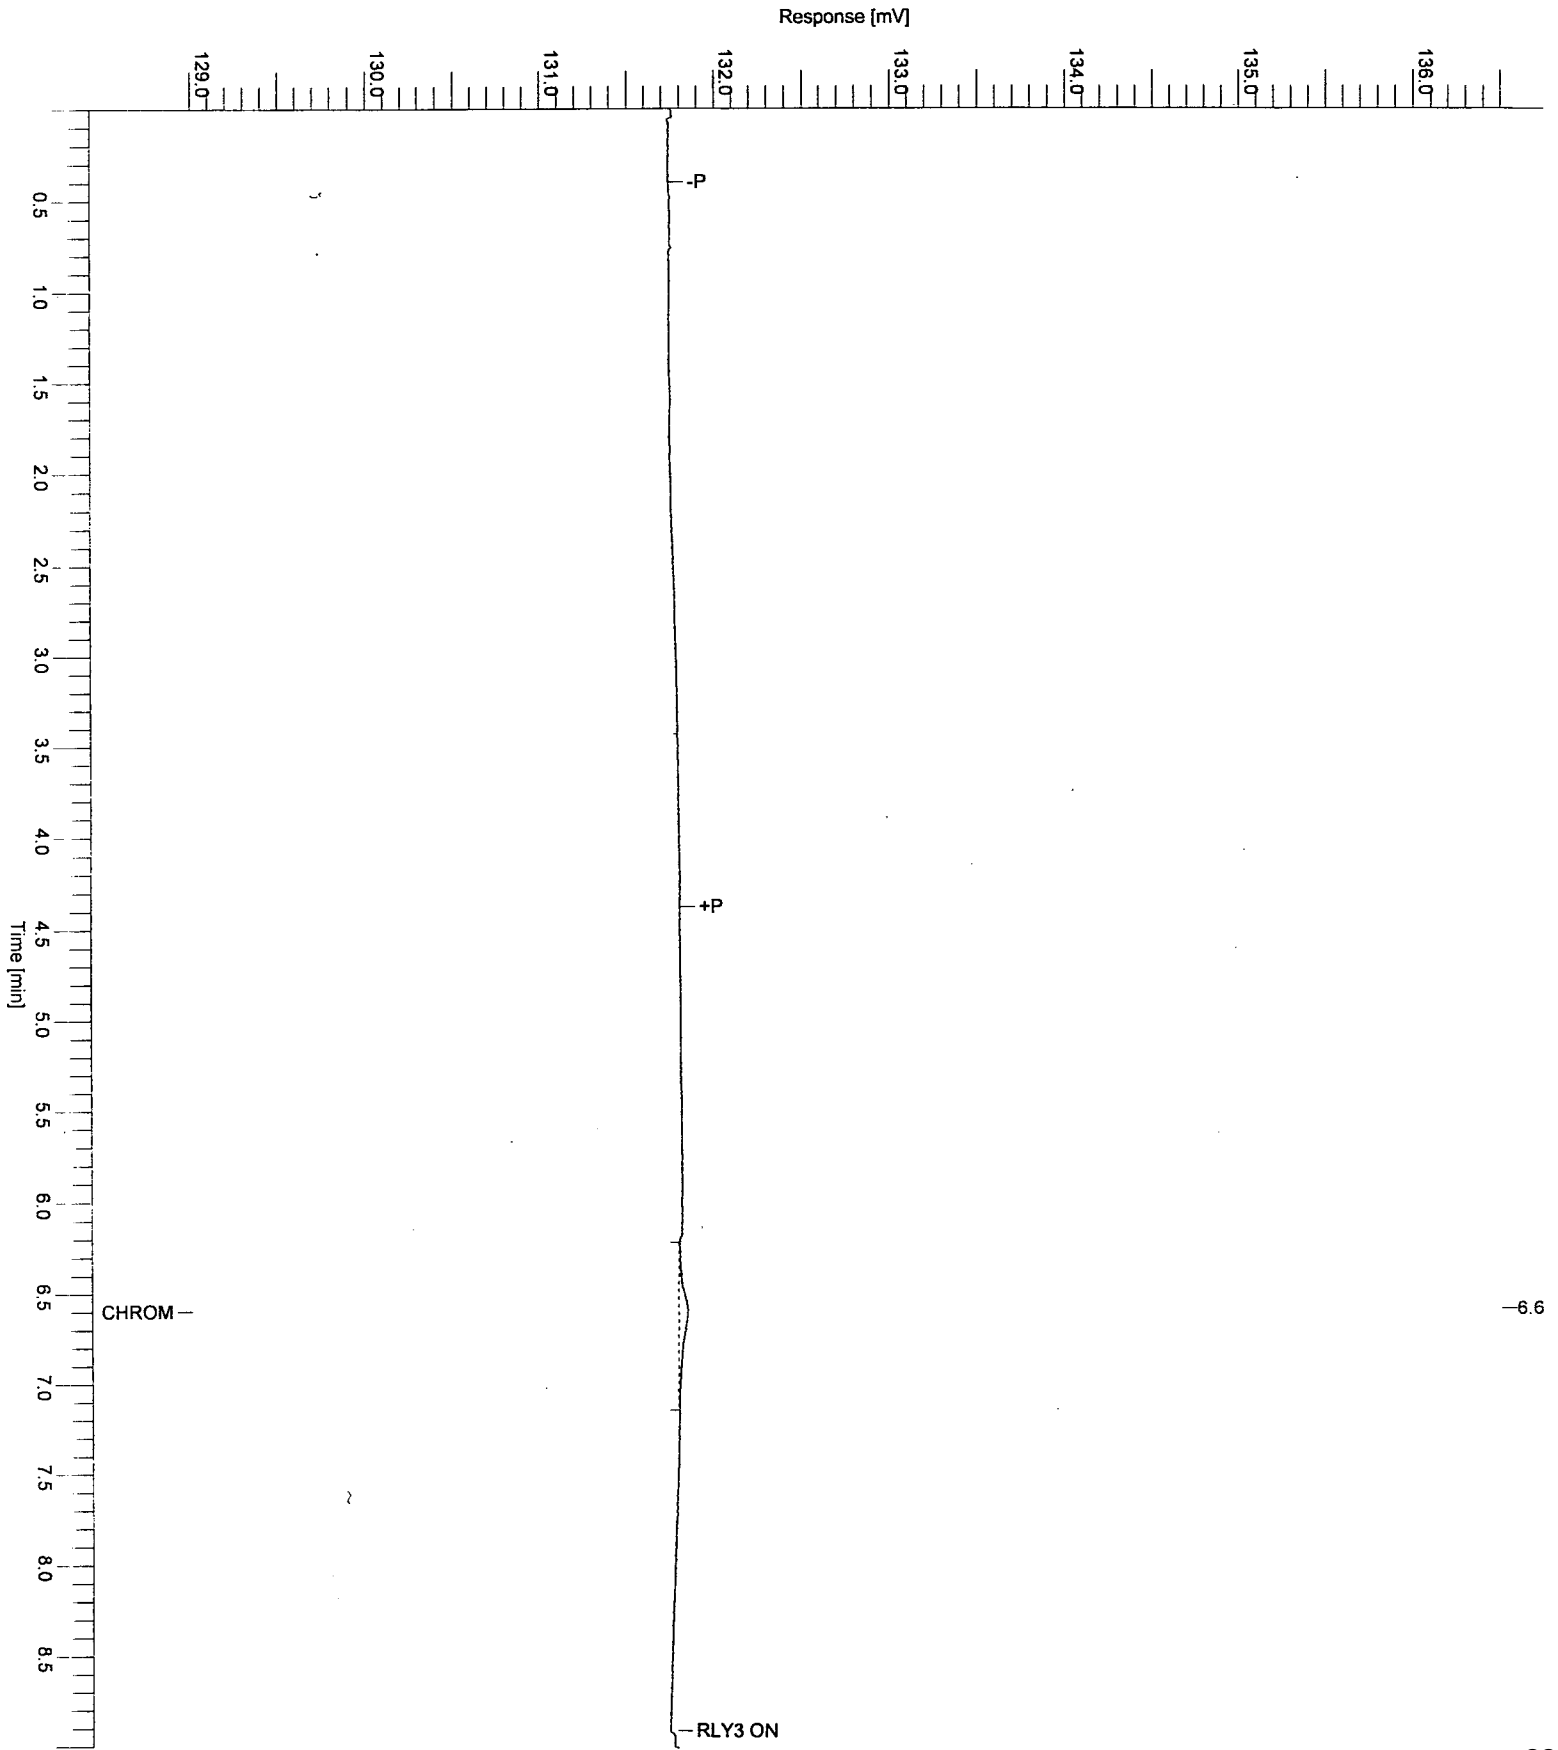

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 6:41:44 PM
Reprocess Number	: ic2: 90588		
Operator	: inorg	Sample Name	: IQG1460-04
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 10.00
Data Acquisition Time	: 7/17/2007 6:32:28 PM	Cycle	: 20

Raw Data File : h:\data\ic4\20070717\20070717020.raw
Result File : h:\data\ic4\20070717\20070717020.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717020.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717020.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717020.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.638	chrom6	11525.70	651.87601	20.3915	203.9151	*
			11525.70	651.87601	20.3915	203.9151	

* Warning -- uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070717\20070717020.TX0

Chromatogram

Sample Name : IQG1460-04 Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717020.raw
Date : 7/17/2007 6:41:45 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 6:32:28 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

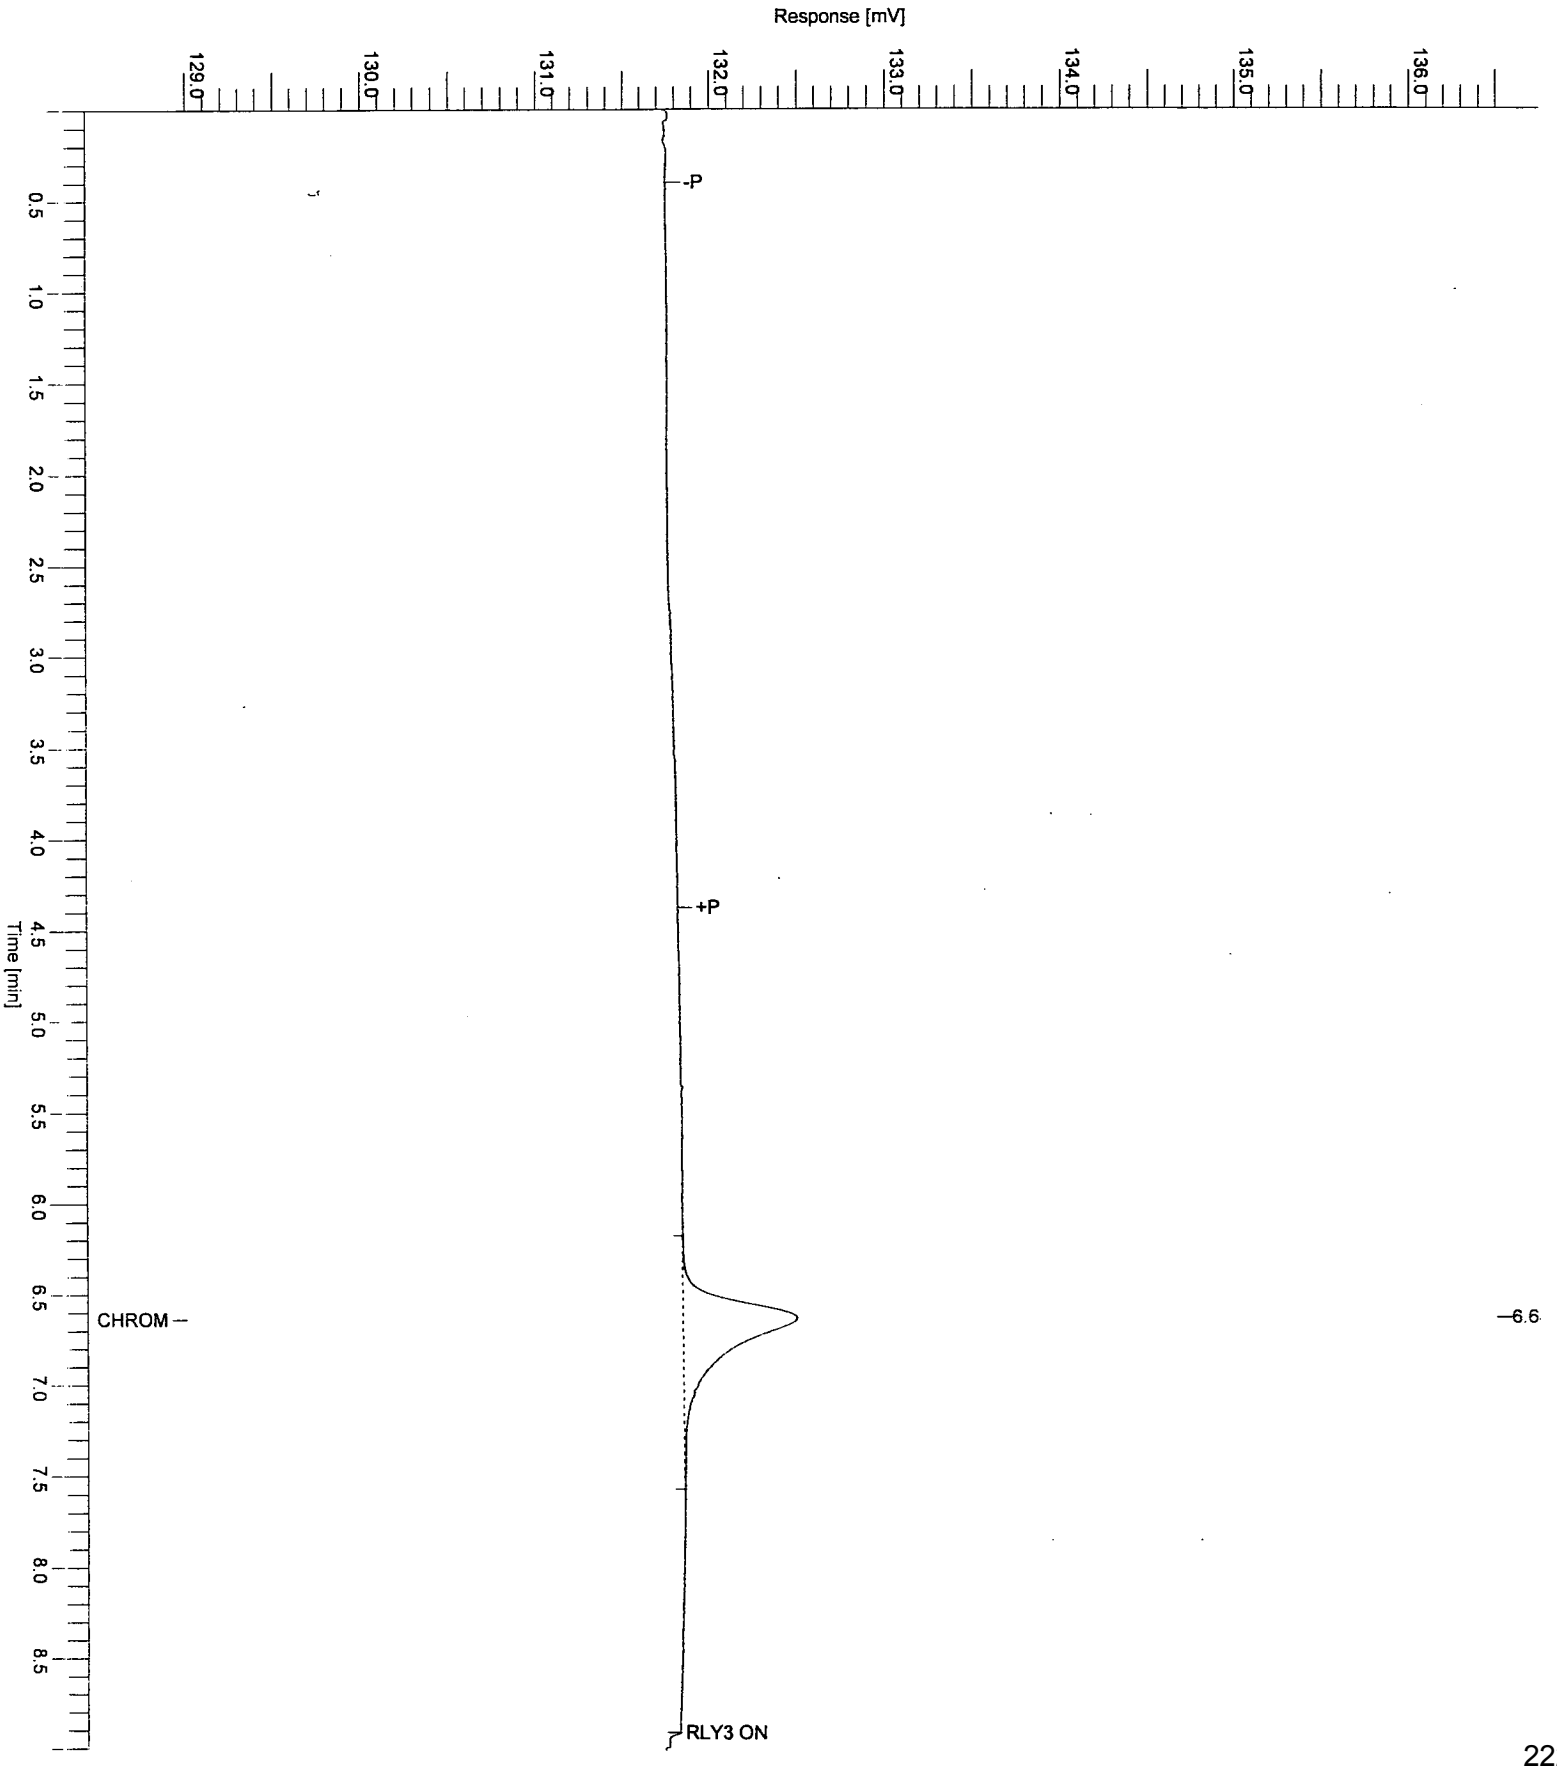

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 7:07:02 PM
Reprocess Number	: ic2: 90592		
Operator	: inorg	Sample Name	: CCV
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 6:57:50 PM	Cycle	: 21

Raw Data File : h:\data\ic4\20070717\20070717021.raw
Result File : h:\data\ic4\20070717\20070717021.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717021.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717021.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717021.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
1	6.931	chrom6	28363.60	1.641e+03	51.4114	51.4114	*
			28363.60	1.641e+03	51.4114	51.4114	

* Warning – uncalibrated levels encountered

Report stored in ASCII file: h:\data\ic4\20070717\20070717021.TX0

Chromatogram

Sample Name : CCV Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717021.raw
Date : 7/17/2007 7:07:04 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 6:57:50 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

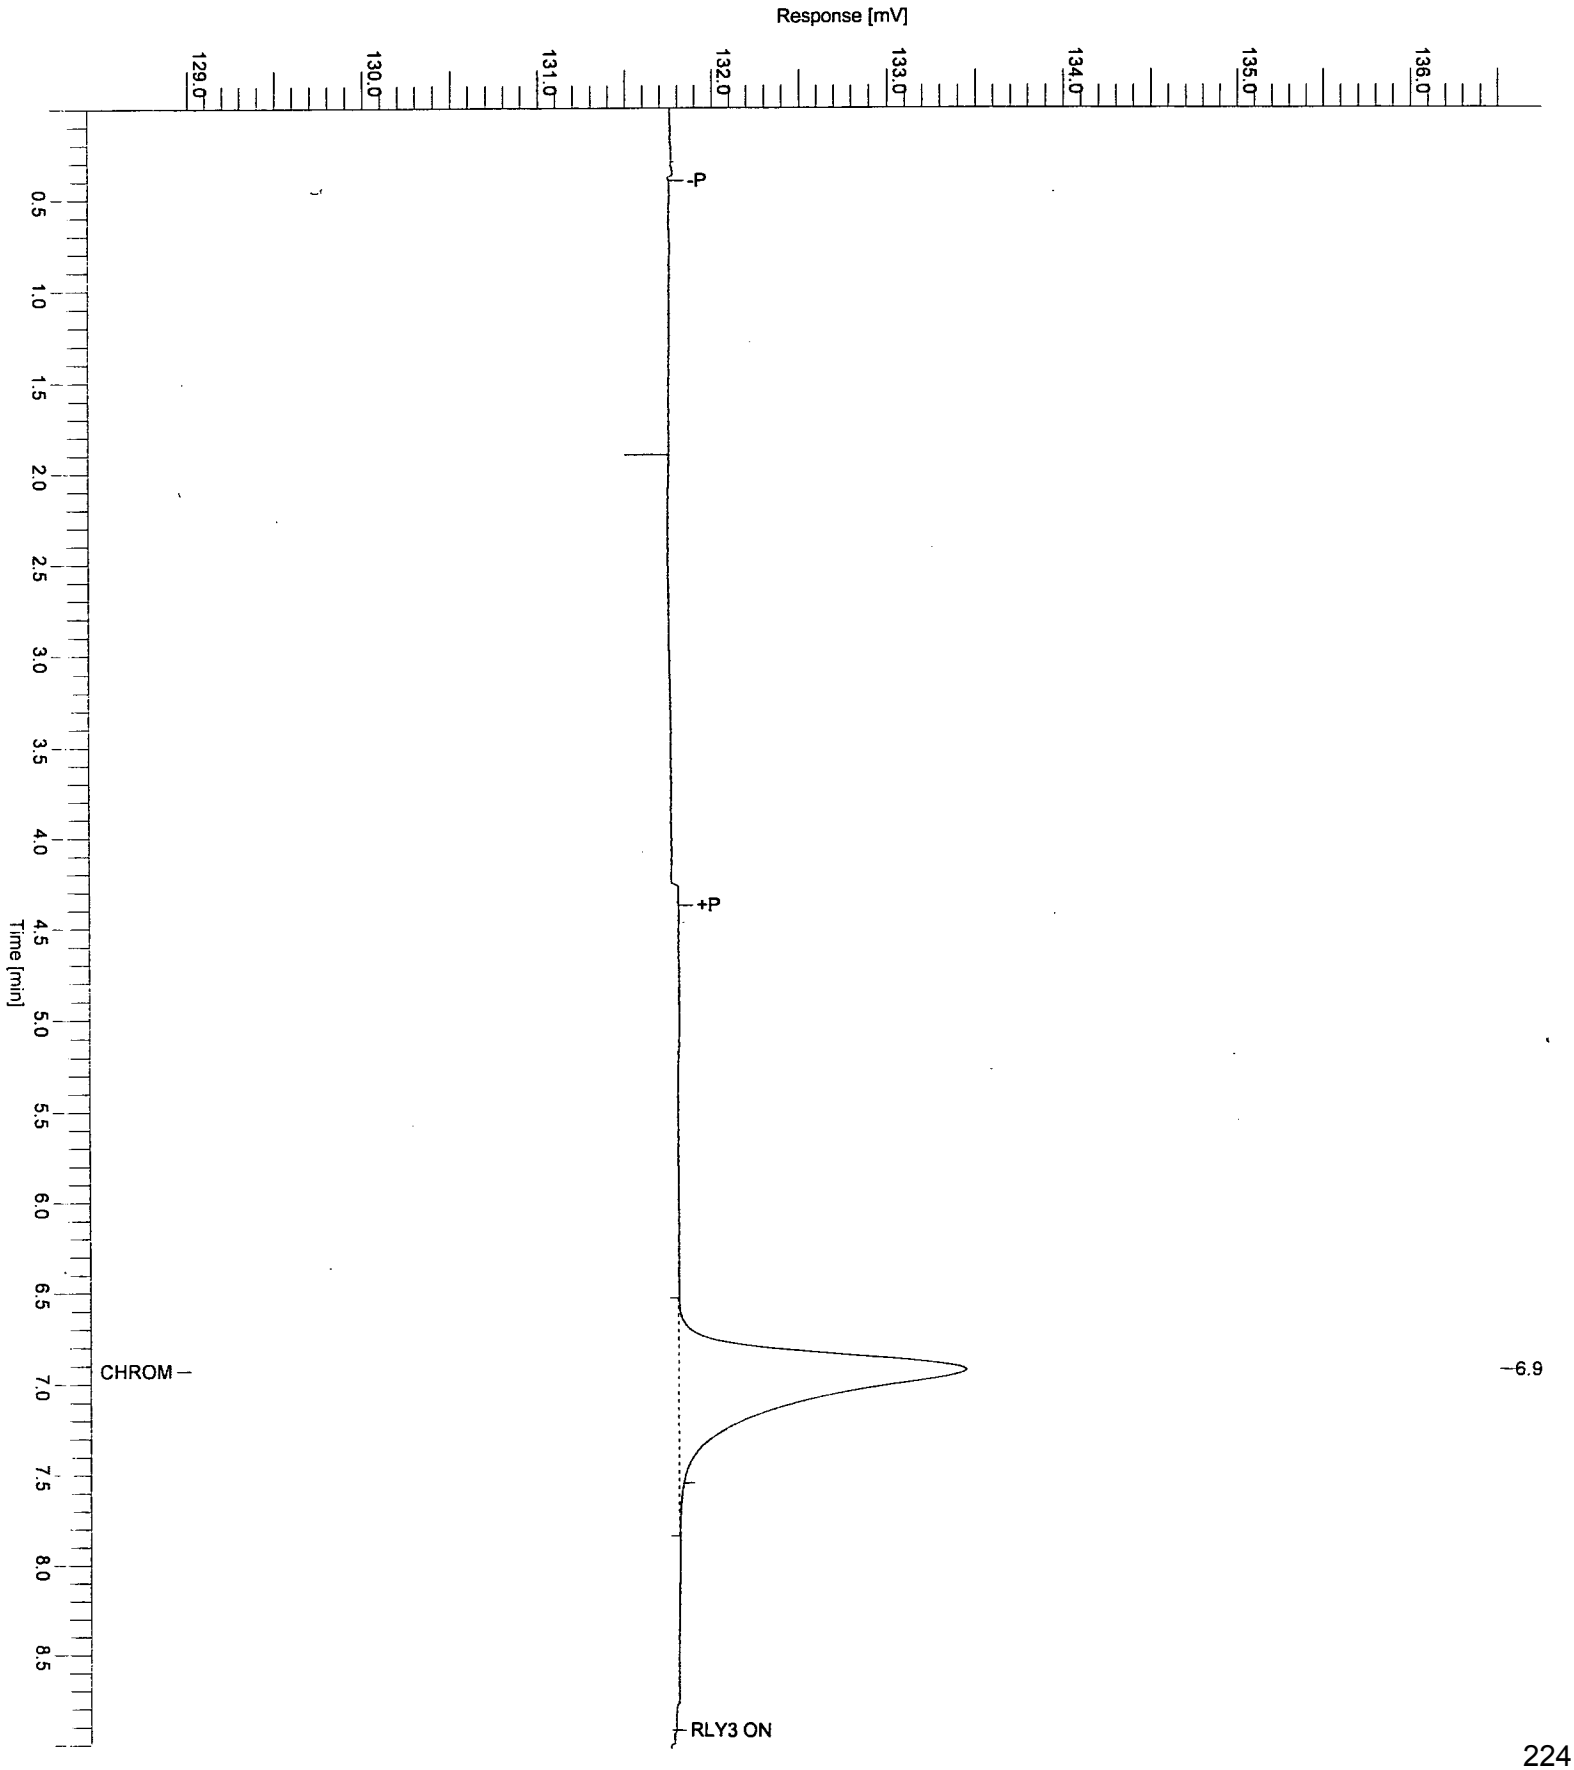

Software Version	: 6.2.1.0.106:0106	Date	: 7/17/2007 7:18:14 PM
Reprocess Number	: ic2: 90594		
Operator	: inorg	Sample Name	: CCB
Sample Number	: 7G17075	Study	:
AutoSampler	: NONE	Rack/Vial	: 0/0
Instrument Name	: ICDNX4	Channel	: A
Interface Serial #	: 2100574712	A/D mV Range	: 1000
Delay Time	: 0.30 min	End Time	: 9.00 min
Sampling Rate	: 20.0000 pts/s		
Sample Volume	: 1.000000 uL	Area Reject	: 0.000000
Sample Amount	: 1.0000	Dilution Factor	: 1.00
Data Acquisition Time	: 7/17/2007 7:08:59 PM	Cycle	: 22

Raw Data File : h:\data\ic4\20070717\20070717022.raw
Result File : h:\data\ic4\20070717\20070717022.rst
Inst Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717022.raw
Proc Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717022.rst
Calib Method : h:\data\ic4\chr6qd30 from h:\data\ic4\20070717\20070717022.rst
Report Format File: h:\data\ic4\chrom6w.rpt
Sequence File : H:\DATA\IC4\20070717\20070717.seq

CHROM6

Peak #	Time [min]	Component Name	Area [µV·s]	Height [µV]	Raw Amount	Adjusted Amount	Cal. Range
-	7.007	chrom6	0.00	0.00000	0.0000	0.0000	
			0.00	0.00000	0.0000	0.0000	

Report stored in ASCII file: h:\data\ic4\20070717\20070717022.TX0

Chromatogram

Sample Name : CCB Sample #: 7G17075 Page 1 of 1
FileName : h:\data\ic4\20070717\20070717022.raw
Date : 7/17/2007 7:18:15 PM
Method : chr6qd30.mth Time of Injection: 7/17/2007 7:08:59 PM
Start Time : 0.00 min End Time : 9.00 min Low Point : 129.00 mV High Point : 136.50 mV
Plot Offset: 129.00 mV Plot Scale: 7.5 mV

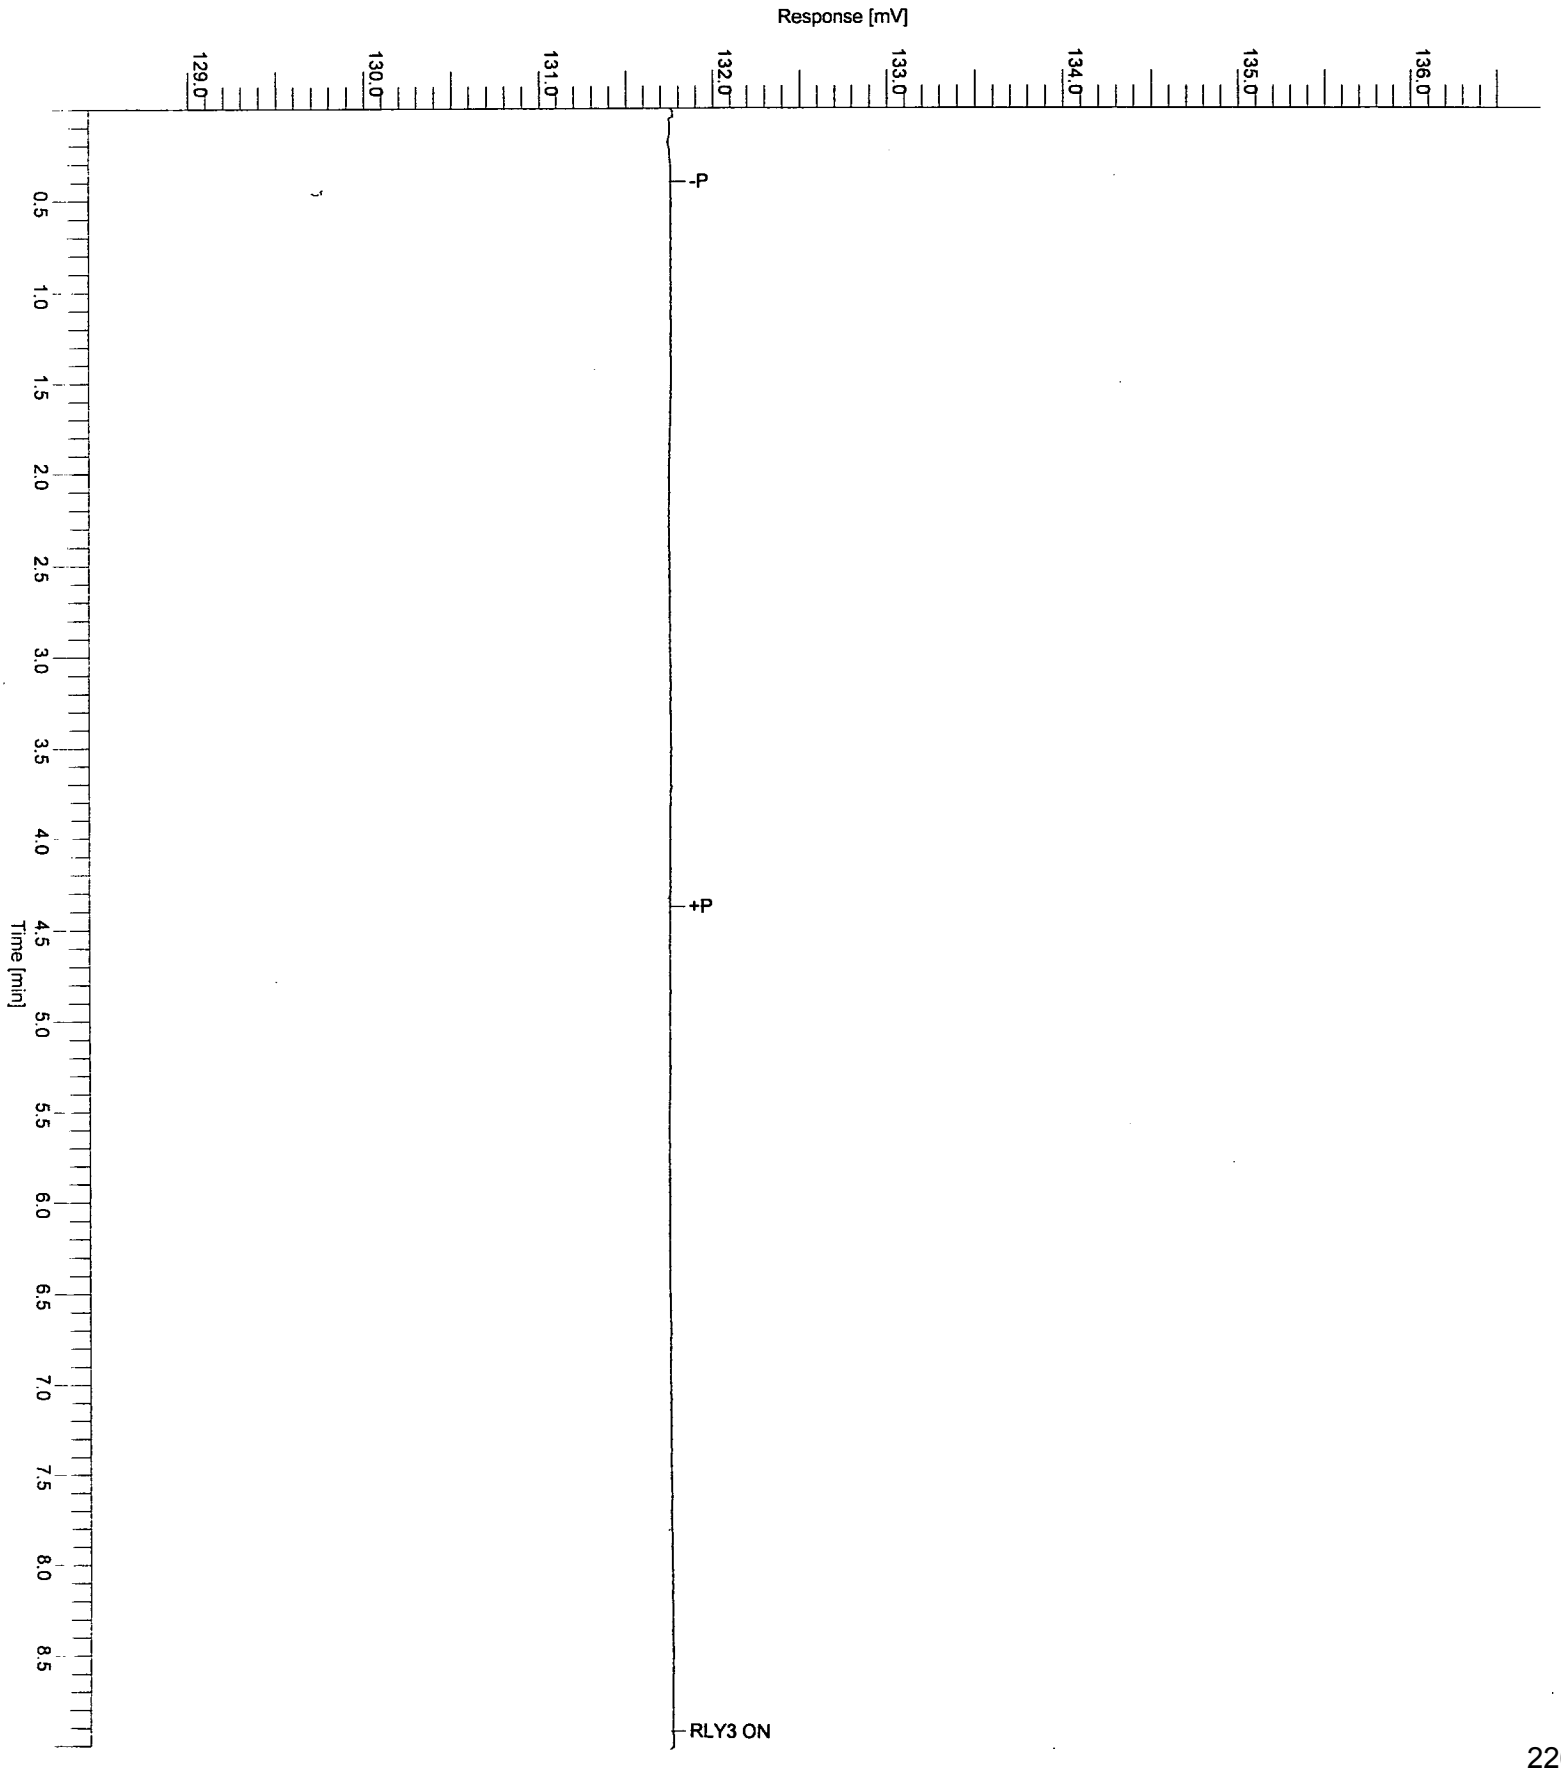

TestAmerica
ANALYTICAL TESTING CORPORATION
17461Derian Ave. Suite 100 Irvine CA 92614 (949) 261-1022 FAX (949) 260-3297

QA/QC PACKAGE: LEVEL IV
PREPARED FOR: GPL LABORATORIES
LABORATORY NUMBER: IQG1460
PROJECT: OMEGA CHEMICAL OU-2 SSID-BC
OMEGA CHEMICAL 335392.FI.01

EPA 524.2 & EPA 524M-TCP
SUBCONTRACTED LABORATORY RAW DATA
(TESTAMERICA – ONTARIO, CA)

- INITIAL CALIBRATION
- CONTINUING CALIBRATION
- RUN LOG
- TUNE REPORT
- QUANTITATION REPORTS
- CHROMATOGRAMS

IQG1460 / CQG0634
LEVEL IV DATA PACKAGE

CHAIN OF CUSTODY

SUBCONTRACT ORDER

TestAmerica - Irvine, CA

IQG1460

SENDING LABORATORY:

TestAmerica - Irvine, CA
17461 Derian Avenue. Suite 100
Irvine, CA 92614
Phone: (949) 261-1022
Fax: (949) 260-3297
Project Manager: Trevor Brenner
Client: GPL Laboratories

RECEIVING LABORATORY:

TestAmerica - Ontario, CA
1014 E. Cooley Drive, Suite AB
Colton, CA 92324
Phone :(909) 370-4667
Fax: (909) 370-1046
Project Location: California
Receipt Temperature: 6 °C Ice: (Y) / N

CQG0634

Analysis	Due	Expires	Interlab	Surch	Comments
Sample ID: IQG1460-01 Water		Sampled: 07/17/07 08:12			
524.2 CA 123-TCP (SIM)	DN07/26/07 12:00	07/31/07 08:12	$110.00	0%	
Level 4 + EDD-Colton - Out	07/26/07 12:00	08/14/07 08:12	$0.00	0%	
Containers Supplied:					
40 mL VOA w/Ascorbic acid (A)	40 mL VOA w/Ascorbic acid (B)	40 mL VOA w/Ascorbic acid (C)			
Sample ID: IQG1460-02 Water		Sampled: 07/17/07 09:00			
524.2 CA 123-TCP (SIM)	DN07/26/07 12:00	07/31/07 09:00	$110.00	0%	
Level 4 + EDD-Colton - Out	07/26/07 12:00	08/14/07 09:00	$0.00	0%	
Containers Supplied:					
40 mL VOA w/Ascorbic acid (A)	40 mL VOA w/Ascorbic acid (B)	40 mL VOA w/Ascorbic acid (C)			
Sample ID: IQG1460-03 Water		Sampled: 07/17/07 09:35			
524.2 CA 123-TCP (SIM)	DN07/26/07 12:00	07/31/07 09:35	$110.00	0%	
Level 4 + EDD-Colton - Out	07/26/07 12:00	08/14/07 09:35	$0.00	0%	
Containers Supplied:					
40 mL VOA w/Ascorbic acid (A)	40 mL VOA w/Ascorbic acid (B)	40 mL VOA w/Ascorbic acid (C)			
Sample ID: IQG1460-04 Water		Sampled: 07/17/07 10:20			
524.2 CA 123-TCP (SIM)	DN07/26/07 12:00	07/31/07 10:20	$110.00	0%	
Level 4 + EDD-Colton - Out	07/26/07 12:00	08/14/07 10:20	$0.00	0%	
Containers Supplied:					
40 mL VOA w/Ascorbic acid (A)	40 mL VOA w/Ascorbic acid (B)	40 mL VOA w/Ascorbic acid (C)			
Sample ID: IQG1460-05 Water		Sampled: 07/17/07 11:30			
524.2 CA 123-TCP (SIM)	DN07/26/07 12:00	07/31/07 11:30	$110.00	0%	
Level 4 + EDD-Colton - Out	07/26/07 12:00	08/14/07 11:30	$0.00	0%	
Containers Supplied:					
40 mL VOA w/Ascorbic acid (A)	40 mL VOA w/Ascorbic acid (B)	40 mL VOA w/Ascorbic acid (C)			

Released By	Date/Time	Received By	Date/Time
Released By	Date/Time	Received By	Date/Time 7/18/07 815

SUBCONTRACT ORDER

TestAmerica - Irvine, CA

IQG1460

Analysis	Due	Expires	Interlab	Surch	Comments
Sample ID: IQG1460-06	**Water**		Sampled: 07/17/07 12:00		
524.2 CA 123-TCP (SIM) DN	07/26/07 12:00	07/31/07 12:00	$110.00	0%	
Level 4 + EDD-Colton - Out	07/26/07 12:00	08/14/07 12:00	$0.00	0%	
Containers Supplied:					
40 mL VOA w/Ascorbic acid (A)	40 mL VOA w/Ascorbic acid (B)	40 mL VOA w/Ascorbic acid (C)			

IQG1460 / CQG0634
LEVEL IV DATA PACKAGE

ANALYTICAL REPORT

TestAmerica
ANALYTICAL TESTING CORPORATION

1014 E. Cooley Dr, Ste A, Colton, CA 92324 (909) 370-4667 Fax:(909) 370-1046

LABORATORY REPORT

Prepared For: TestAmerica - Irvine, CA
17461 Derian Avenue. Suite 100
Irvine, CA 92614
Attention: Trevor Brenner

Project: Omega Chemical OU-2 SSID-BC
IQG1460

Sampled: 07/17/07
Received: 07/18/07
Issued: 07/27/07 11:05

The results listed within this Laboratory Report pertain only to the samples tested in the laboratory. The analyses contained in this report were performed in accordance with the applicable certifications as noted. All soil samples are reported on a wet weight basis unless otherwise noted in the report. This Laboratory Report is confidential and is intended for the sole use of TestAmerica and its client. This report shall not be reproduced, except in full, without written permission from TestAmerica. The Chain(s) of Custody, 2 pages, are included and are an integral part of this report.
This entire report was reviewed and approved for release.

CASE NARRATIVE

SAMPLE RECEIPT: Samples were received intact, at 6°C, on ice and with chain of custody documentation.

HOLDING TIMES: All samples were analyzed within prescribed holding times and/or in accordance with the TestAmerica Sample Acceptance Policy unless otherwise noted in the report.

PRESERVATION: Samples requiring preservation were verified prior to sample analysis.

QA/QC CRITERIA: All analyses met method criteria, except as noted in the report with data qualifiers.

COMMENTS: Results that fall between the MDL and RL are 'J' flagged.

SUBCONTRACTED: No analyses were subcontracted to an outside laboratory.

LABORATORY ID	CLIENT ID	MATRIX
CQG0634-01	IQG1460-01 (OC2-MW8D-W-0-603)	Water
CQG0634-02	IQG1460-02 (OC2-MW8C-W-0-604)	Water
CQG0634-03	IQG1460-03 (OC2-MW8B-W-0-605)	Water
CQG0634-04	IQG1460-04 (OC2-MW8A-W-0-606)	Water
CQG0634-05	IQG1460-05 (OC2-MW12-W-0-607)	Water
CQG0634-06	IQG1460-06 (OC2-MW12-W-1-608)	Water

Reviewed By:

TestAmerica - Ontario, CA

John Stuart Styles
Project Manager

TestAmerica
ANALYTICAL TESTING CORPORATION
1014 E. Cooley Dr, Ste A, Colton, CA 92324 (909) 370-4667 Fax:(909) 370-1046

TestAmerica - Irvine, CA
17461 Derian Avenue. Suite 100
Irvine, CA 92614
Attention: Trevor Brenner

Project ID: Omega Chemical OU-2 SSID-BC
IQG1460
Report Number: CQG0634

Sampled: 07/17/07
Received: 07/18/07

CDHS SRL 524 MODIFIED METHOD FOR 1,2,3-TRICHLOROPROPANE PT/GCMS

Analyte	Method	Batch	MDL Limit	Reporting Limit	Sample Result	Dilution Factor	Date Extracted	Date Analyzed	Data Qualifiers
Sample ID: CQG0634-01 (IQG1460-01 (OC2-MW8D-W-0-603) - Water)									
Reporting Units: ng/L									
1,2,3-Trichloropropane (123-TCP)	SRL 524M-123TCP	C7G1807	N/A	5.0	ND	1	07/18/07	07/18/07	
Sample ID: CQG0634-02 (IQG1460-02 (OC2-MW8C-W-0-604) - Water)									
Reporting Units: ng/L									
1,2,3-Trichloropropane (123-TCP)	SRL 524M-123TCP	C7G1807	N/A	5.0	ND	1	07/18/07	07/18/07	
Sample ID: CQG0634-03 (IQG1460-03 (OC2-MW8B-W-0-605) - Water)									
Reporting Units: ng/L									
1,2,3-Trichloropropane (123-TCP)	SRL 524M-123TCP	C7G1807	N/A	5.0	ND	1	07/18/07	07/18/07	
Sample ID: CQG0634-04 (IQG1460-04 (OC2-MW8A-W-0-606) - Water)									
Reporting Units: ng/L									
1,2,3-Trichloropropane (123-TCP)	SRL 524M-123TCP	C7G1807	N/A	5.0	ND	1	07/18/07	07/18/07	
Sample ID: CQG0634-05 (IQG1460-05 (OC2-MW12-W-0-607) - Water)									
Reporting Units: ng/L									
1,2,3-Trichloropropane (123-TCP)	SRL 524M-123TCP	C7G2611	N/A	5.0	ND	1	07/26/07	07/26/07	
Sample ID: CQG0634-06 (IQG1460-06 (OC2-MW12-W-1-608) - Water)									
Reporting Units: ng/L									
1,2,3-Trichloropropane (123-TCP)	SRL 524M-123TCP	C7G2611	N/A	5.0	ND	1	07/26/07	07/26/07	

TestAmerica - Ontario, CA

John Stuart Styles
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

TestAmerica
ANALYTICAL TESTING CORPORATION
1014 E. Cooley Dr, Ste A, Colton, CA 92324 (909) 370-4667 Fax:(909) 370-1046

TestAmerica - Irvine, CA
17461 Derian Avenue. Suite 100
Irvine, CA 92614
Attention: Trevor Brenner

Project ID: Omega Chemical OU-2 SSID-BC
IQG1460
Report Number: CQG0634

Sampled: 07/17/07
Received: 07/18/07

METHOD BLANK/QC DATA

CDHS SRL 524 MODIFIED METHOD FOR 1,2,3-TRICHLOROPROPANE PT/GCMS

Analyte	Result	Reporting Limit	MDL	Units	Spike Level	Source Result	%REC	%REC Limits	RPD	RPD Limit	Data Qualifiers
Batch: C7G1807 Extracted: 07/18/07											
Blank Analyzed: 07/18/2007 (C7G1807-BLK1)											
1,2,3-Trichloropropane (123-TCP)	ND	5.0	N/A	ng/L							
LCS Analyzed: 07/18/2007 (C7G1807-BS1)											
1,2,3-Trichloropropane (123-TCP)	5.02	5.0	N/A	ng/L	5.00		100	80-120			
Matrix Spike Analyzed: 07/18/2007 (C7G1807-MS1)						**Source: CQG0466-01RE1**					
1,2,3-Trichloropropane (123-TCP)	42.9	5.0	N/A	ng/L	50.0	ND	86	52-135			
Matrix Spike Dup Analyzed: 07/18/2007 (C7G1807-MSD1)						**Source: CQG0466-01RE1**					
1,2,3-Trichloropropane (123-TCP)	53.0	5.0	N/A	ng/L	50.0	ND	106	52-135	21	27	
Batch: C7G2611 Extracted: 07/26/07											
Blank Analyzed: 07/26/2007 (C7G2611-BLK1)											
1,2,3-Trichloropropane (123-TCP)	ND	5.0	N/A	ng/L							
LCS Analyzed: 07/26/2007 (C7G2611-BS1)											
1,2,3-Trichloropropane (123-TCP)	4.08	5.0	N/A	ng/L	5.00		82	80-120			
Matrix Spike Analyzed: 07/26/2007 (C7G2611-MS1)						**Source: CQG0702-01**					
1,2,3-Trichloropropane (123-TCP)	49.8	5.0	N/A	ng/L	50.0	ND	100	52-135			
Matrix Spike Dup Analyzed: 07/26/2007 (C7G2611-MSD1)						**Source: CQG0702-01**					
1,2,3-Trichloropropane (123-TCP)	48.0	5.0	N/A	ng/L	50.0	ND	96	52-135	4	27	

TestAmerica - Ontario, CA

John Stuart Styles
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

TestAmerica
ANALYTICAL TESTING CORPORATION
1014 E. Cooley Dr, Ste A, Colton, CA 92324 (909) 370-4667 Fax:(909) 370-1046

TestAmerica - Irvine, CA 17461 Derian Avenue. Suite 100 Irvine, CA 92614 Attention: Trevor Brenner	Project ID: Omega Chemical OU-2 SSID-BC IQG1460 Report Number: CQG0634	Sampled: 07/17/07 Received: 07/18/07

DATA QUALIFIERS AND DEFINITIONS

ND Analyte NOT DETECTED at or above the reporting limit or MDL, if MDL is specified.

RPD Relative Percent Difference

TestAmerica - Ontario, CA

John Stuart Styles
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

TestAmerica
ANALYTICAL TESTING CORPORATION
1014 E. Cooley Dr, Ste A, Colton, CA 92324 (909) 370-4667 Fax:(909) 370-1046

TestAmerica - Irvine, CA 17461 Derian Avenue. Suite 100 Irvine, CA 92614 Attention: Trevor Brenner	Project ID: Omega Chemical OU-2 SSID-BC IQG1460 Report Number: CQG0634	Sampled: 07/17/07 Received: 07/18/07

Certification Summary

TestAmerica - Ontario, CA

Method	Matrix	Nelac	California
SRL 524M-123TCP	Water		

TestAmerica - Ontario, CA

John Stuart Styles
Project Manager

The results pertain only to the samples tested in the laboratory. This report shall not be reproduced, except in full, without written permission from TestAmerica.

IQG1460 / CQG0634
LEVEL IV DATA PACKAGE

SRL 524M-123 TCP
INITIAL CALIBRATION SUMMARY

1,2,3-Trichloropropane Initial Calibration Verification Checklist

Instrument: GCMS 39

Standard: 7060083 @ 0.25 ng/µL

Internal stds: 7060081 @ 0.25 ng/µL

Analyst: PM

Date: 7/11/07

Method: 123-TCP071107.M

Reviewed by: DA (Initials) 7-13-07 (Date)

Calibration Requirements

	Required RSD	Actual RSD	Initials
2) 1,2,3-Trichloropropane	< 20%	9.75	PM

		Criteria	Initials
Retention time o-Xylene (from most recent 524.2 calibration):	17.22		
Retention time 1,2,3-tcp-d5:	17.31		
Difference:	0.09	>0.08minutes	PM

		Meets Criteria	Initials	Date Analyzed	Date Due
Quality Control Sample (QCS):	Meets CCV criteria	Pass	PM	7/11/07	10/11/07

Response Factor Report GCMS39

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration

Calibration File
5 =G11002.D 10 =G11003.D 20 =G11004.D 50 =G11005.D
100 =G11006.D 200 =G11007.D 500 =G11008.D = =

Compound	5	10	20	50	100	200	500	Avg	%RSD
1) I 1,2,3-TCP-d5 (IS)	ISTD								
2) CPM 1,2,3-Trichloropropane	1.024	0.990	0.762	0.900	0.939	0.871	0.853	0.906	9.75

(#) = Out of Range

123-TCP071107.M Thu Jul 12 16:39:48 2007

Quantitation Report (Qedit)

Data File : C:\DATA\07JUL11\G11009.D
Acq On : 11 Jul 2007 6:55 pm
Sample : Xylene RT
Misc : 25mL w/ #7070019
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:40 2007

Vial: 9
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: temp.res

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Multiple Level Calibration

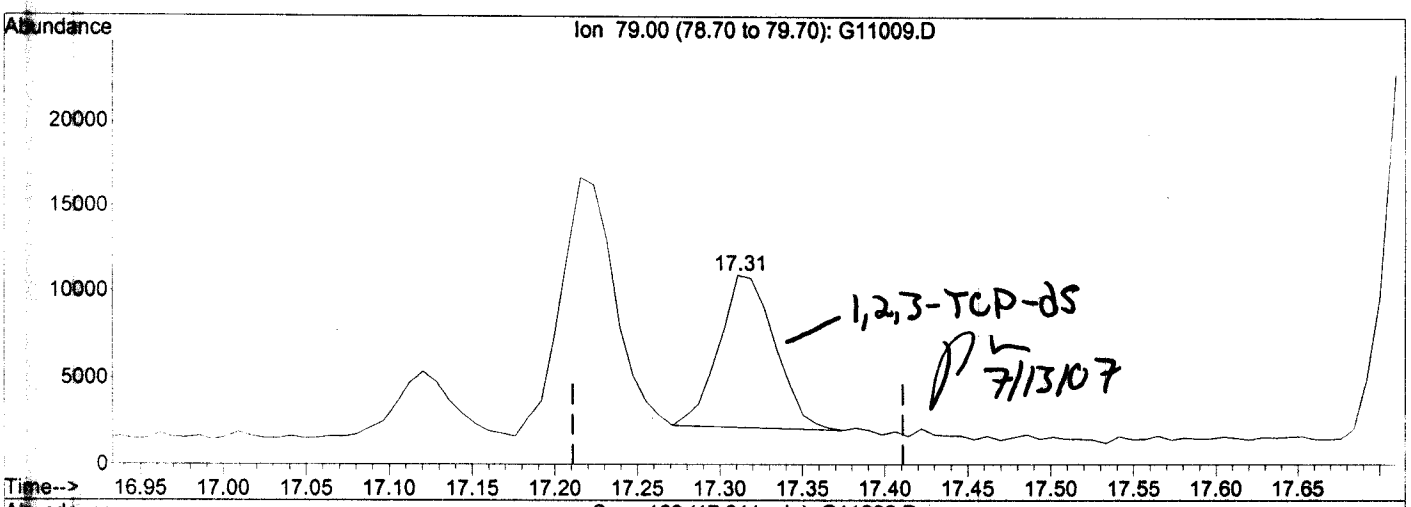

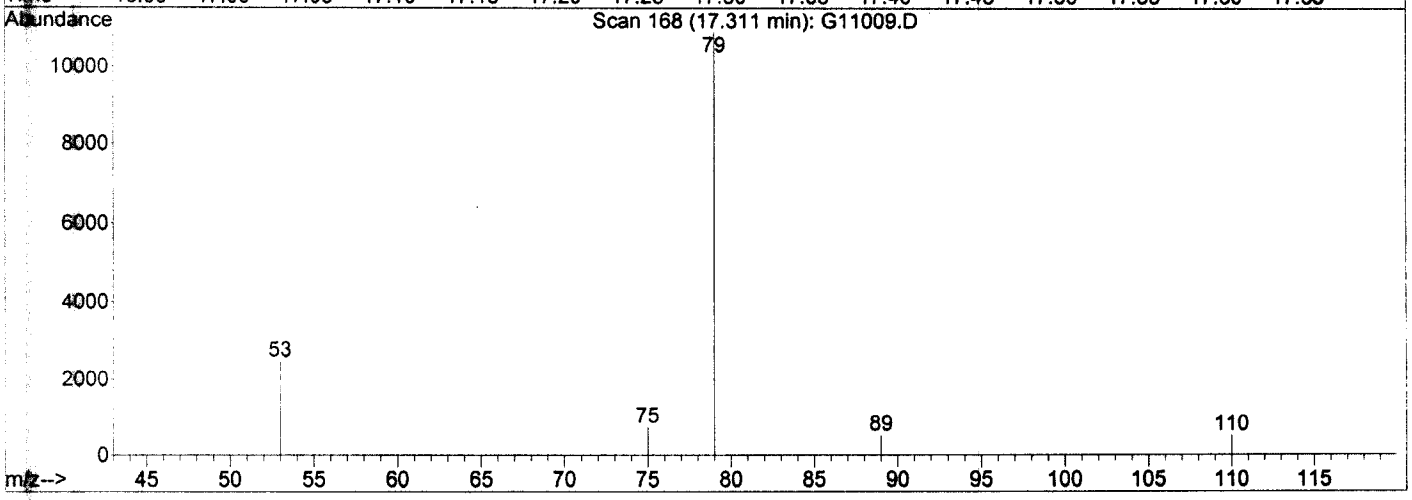

TIC: G11009.D

(1) 1,2,3-TCP-d5 (IS) (I)

17.31min 50.00ng/L

response 20461

Ion	Exp%	Act%
79.00	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

G11009.D 123-TCP071107.M Thu Jul 12 16:40:16 2007

Quantitation Report (Qedit)

Data File : C:\DATA\07JUL11\G11009.D
Acq On : 11 Jul 2007 6:55 pm
Sample : Xylene RT
Misc : 25mL w/ #7070019
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:40 2007

Vial: 9
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: temp.res

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Multiple Level Calibration

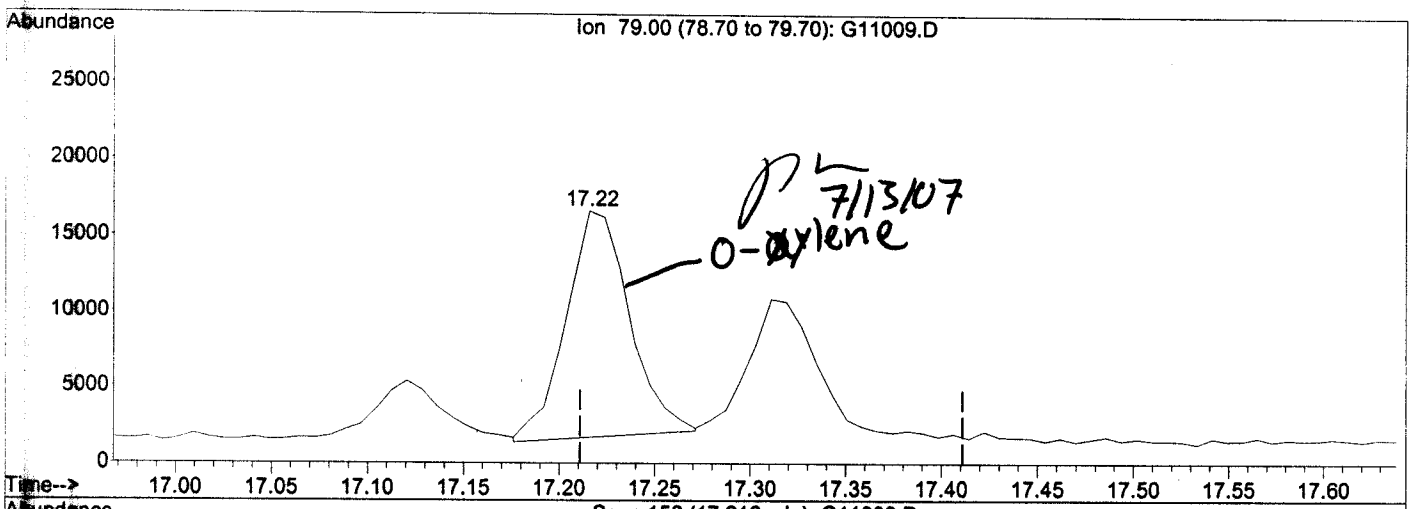

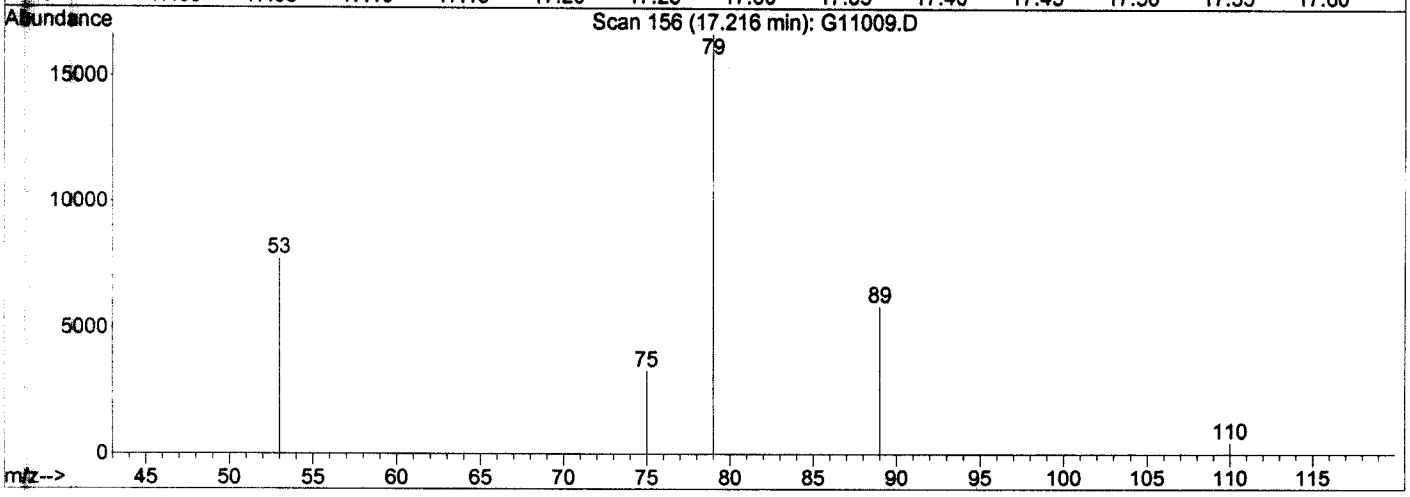

TIC: G11009.D

(1) 1,2,3-TCP-d5 (IS) (I)

17.22min 50.00ng/L m

response 34627

Ion	Exp%	Act%
79.00	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

1,2,3-Trichloropropane by GC/MS Calibration Verification Check

7/13/07

File:	G11011.D	**Instrument:**	GCMS39
Operator:	PM		
Date:	11 Jul 2007 8:00 pm	**QC BATCH # :**	CCV - Second Source

	Source	Response	% Recovery	Control Limits
2) 1,2,3-Trichloropropane	50	44.22	88.4	80-120

* Denotes values out of expected range

Evaluate Continuing Calibration Report

Data File : C:\DATA\07JUL11\G11011.D Vial: 11
Acq On : 11 Jul 2007 8:00 pm Operator: PM
Sample : CCV - Second Source Inst : GCMS39
Misc : 25mL w/ QCS #7060085 Multiplr: 1.00
MS Integration Params: RTEINT.P

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Multiple Level Calibration

Min. RRF : 0.000 Min. Rel. Area : 80% Max. R.T. Dev 0.50min
Max. RRF Dev : 20% Max. Rel. Area : 200%

		Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1	I	1,2,3-TCP-d5 (IS)	1.000	1.000	0.0	105	0.00
2	CPM	1,2,3-Trichloropropane	0.906	0.801	11.6	94	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 0

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11011.D
Acq On : 11 Jul 2007 8:00 pm
Sample : CCV - Second Source
Misc : 25mL w/ QCS #7060085
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35:27 2007

Vial: 11
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	21224	50.00 ng/L	0.00
Target Compounds					Qvalue
2) 1,2,3-Trichloropropane	17.41	75	16997	44.22 ng/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11011.D
Acq On : 11 Jul 2007 8:00 pm
Sample : CCV - Second Source
Misc : 25mL w/ QCS #7060085
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35 2007

Vial: 11
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration

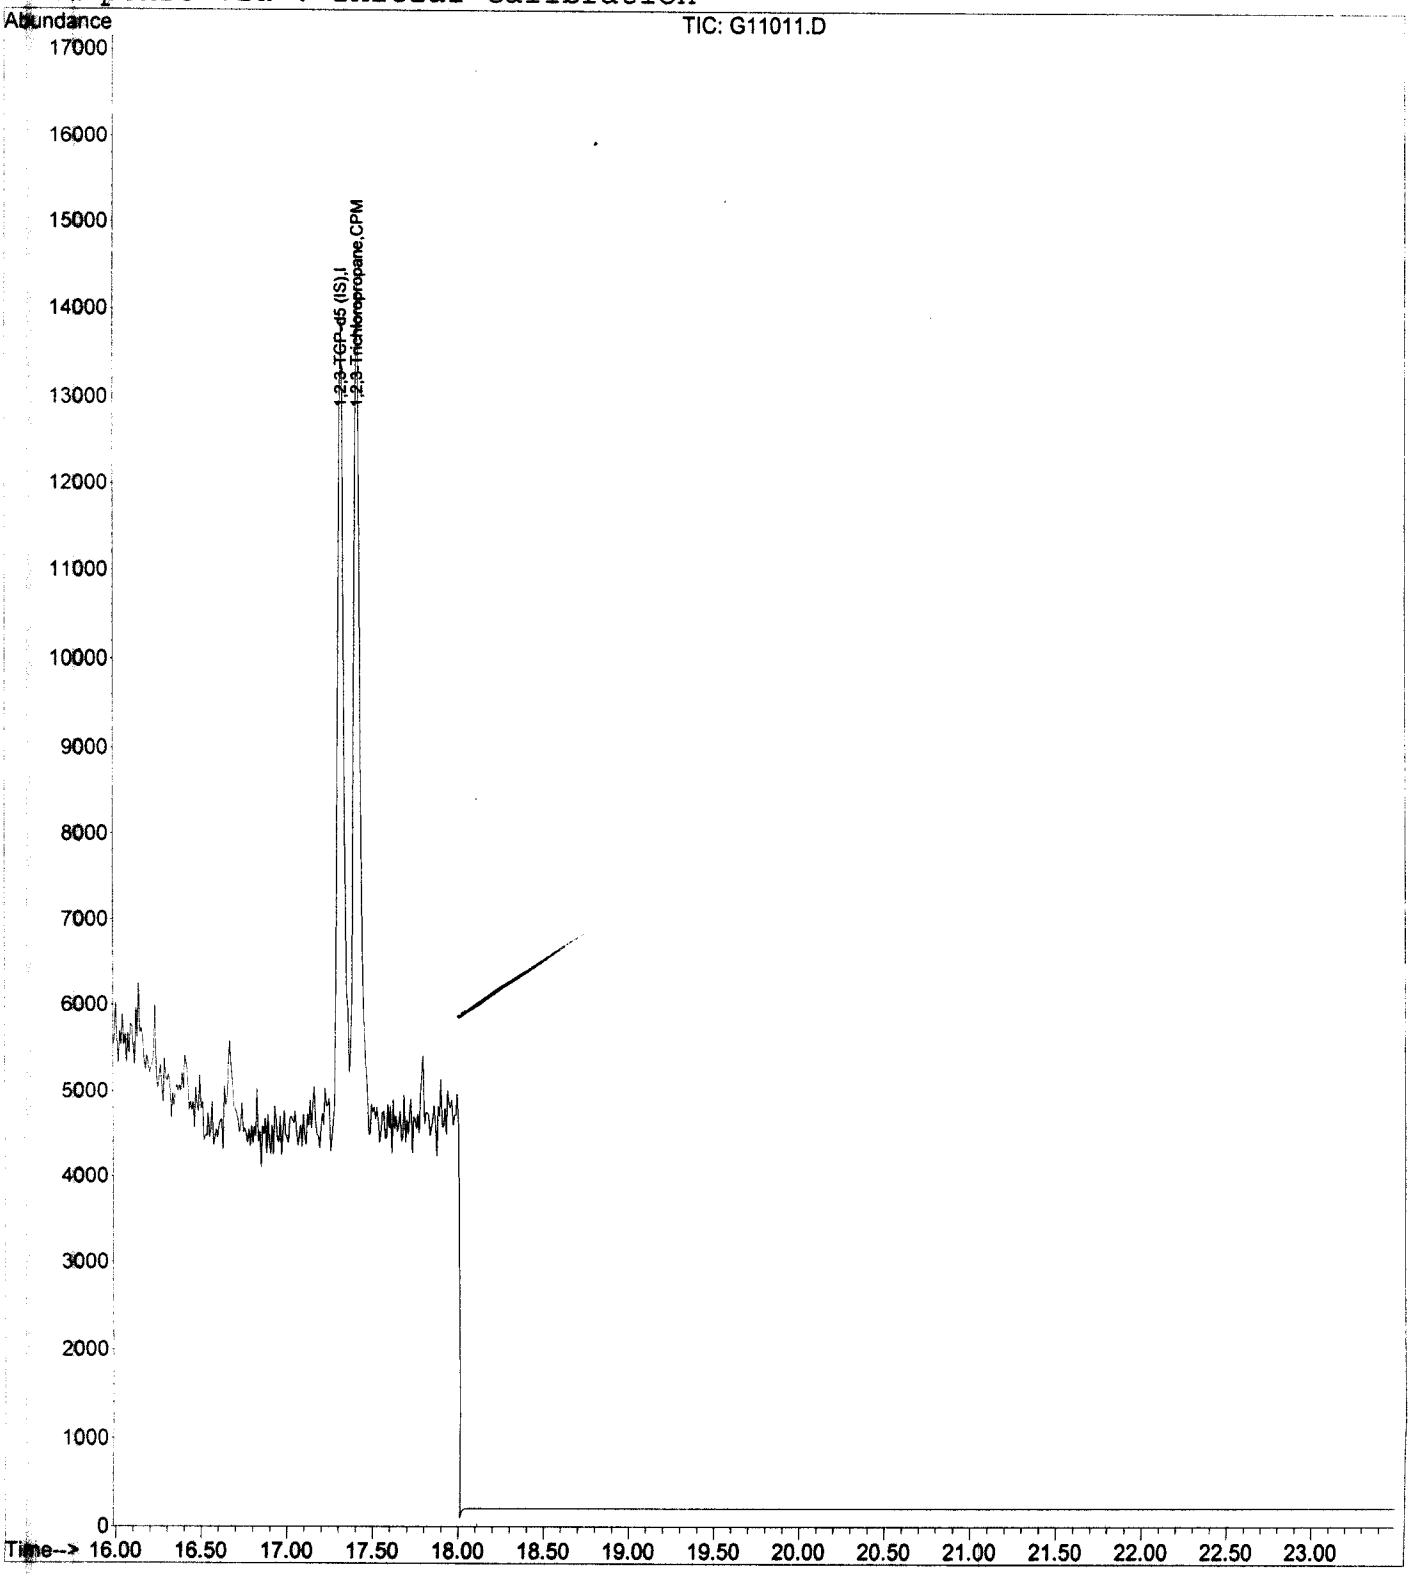

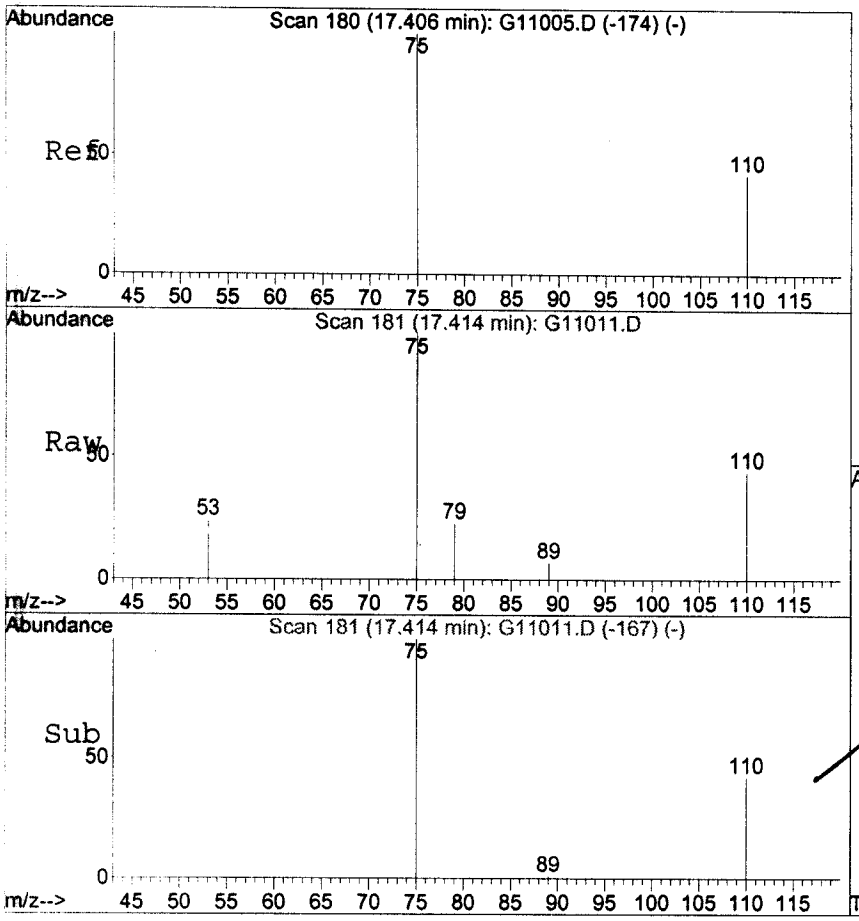

#2
1,2,3-Trichloropropane
Concen: 44.22 ng/L
RT: 17.41 min Scan# 181
Delta R.T. 0.01 min
Lab File: G11011.D
Acq: 11 Jul 2007 8:00 pm

Tgt Ion: 75 Resp: 16997

Ion	Ratio	Lower	Upper
75	100		
110	41.5	11.2	71.2
53	1.7	0.0	30.0
89	1.1	0.0	30.8

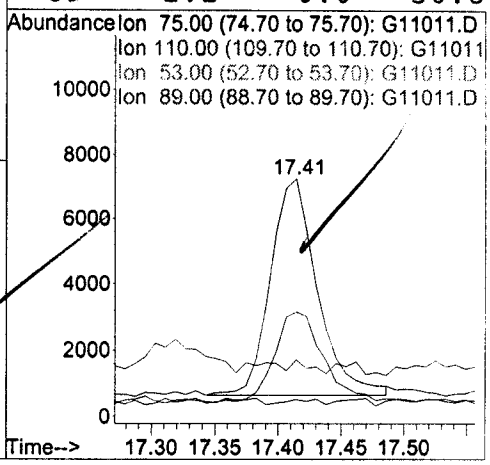

IQG1460 / CQG0634
LEVEL IV DATA PACKAGE

SRL 524M-123 TCP
INITIAL CALIBRATION RAW DATA

Injection Log

Directory: C:\DATA\07JUL11

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	1	G11001.d	1.	Blank	25mL w/ #7060081	11 Jul 2007 14:34
2	2	G11002.d	1.	5ppt #7060083	25mL Initial Cal	11 Jul 2007 15:07
3	3	G11003.d	1.	10ppt #7060083	25mL Initial Cal	11 Jul 2007 15:39
4	4	G11004.d	1.	20ppt #7060083	25mL Initial Cal	11 Jul 2007 16:12
5	5	G11005.d	1.	50ppt #7060083	25mL Initial Cal	11 Jul 2007 16:44
6	6	G11006.d	1.	100ppt #7060083	25mL Initial Cal	11 Jul 2007 17:17
7	7	G11007.d	1.	200ppt #7060083	25mL Initial Cal	11 Jul 2007 17:50
8	8	G11008.d	1.	500ppt #7060083	25mL Initial Cal	11 Jul 2007 18:22
9	9	G11009.d	1.	Xylene RT	25mL w/ #7070019	11 Jul 2007 18:55
10	10	G11010.d	1.	Rinse	25mL	11 Jul 2007 19:27
11	11	G11011.d	1.	CCV - Second Source	25mL w/ QCS #7060085	11 Jul 2007 20:00

Mint Miner 2.02 (70108) Directory Scan: x:\07JUL11

13 Jul 2007 15:11

Level	Status	Code	Operator	Instrument	Sample ID
Scan File Path: x:\07JUL11\G11001.D					
Original Path: C:\DATA\07JUL11\G11001.D					
0	Scanned		PM	GCMS39	Blank (25mL w/ #7060081)
Scan File Path: x:\07JUL11\G11002.D					
Original Path: C:\DATA\07JUL11\G11002.D					
5	Scanned	QD(1)	PM	GCMS39	5ppt #7060083 (25mL Initial Cal)
Scan File Path: x:\07JUL11\G11003.D					
Original Path: C:\DATA\07JUL11\G11003.D					
0	Scanned		PM	GCMS39	10ppt #7060083 (25mL Initial Cal)
Scan File Path: x:\07JUL11\G11004.D					
Original Path: C:\DATA\07JUL11\G11004.D					
0	Scanned		PM	GCMS39	20ppt #7060083 (25mL Initial Cal)
Scan File Path: x:\07JUL11\G11005.D					
Original Path: C:\DATA\07JUL11\G11005.D					
5	Scanned	QD(1)	PM	GCMS39	50ppt #7060083 (25mL Initial Cal)
Scan File Path: x:\07JUL11\G11006.D					
Original Path: C:\DATA\07JUL11\G11006.D					
0	Scanned		PM	GCMS39	100ppt #7060083 (25mL Initial Cal)
Scan File Path: x:\07JUL11\G11007.D					
Original Path: C:\DATA\07JUL11\G11007.D					
0	Scanned		PM	GCMS39	200ppt #7060083 (25mL Initial Cal)
Scan File Path: x:\07JUL11\G11008.D					
Original Path: C:\DATA\07JUL11\G11008.D					
0	Scanned		PM	GCMS39	500ppt #7060083 (25mL Initial Cal)
Scan File Path: x:\07JUL11\G11009.D					
Original Path: C:\DATA\07JUL11\G11009.D					
0	Scanned		PM	GCMS39	Xylene RT (25mL w/ #7070019)
Scan File Path: x:\07JUL11\G11010.D					
Original Path: x:\07JUL11\G11010.D					
0	No Audit				
Scan File Path: x:\07JUL11\G11011.D					
Original Path: C:\DATA\07JUL11\G11011.D					
5	Scanned	QD(1)	PM	GCMS39	CCV - Second Source (25mL w/ QCS #7060085

QD = Method Last Update date after Quantitation date

No Time Travel computer error 7-13-07

Level	Status	Code	Operator	Instrument	Sample ID

ScanSummary.rpt

Total Files Scanned	Beginning Analyzed Date
Methods	Ending Analyzed Date
Samples	Analyzed Range
Tunes	Greatest Time Between Tunes
CCCs	Greatest Time Between CCCs

Distinct Method Last Updated count
Operators Intruments

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11001.D
Acq On : 11 Jul 2007 2:34 pm
Sample : Blank
Misc : 25mL w/ #7060081
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35:13 2007

Vial: 1
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	16854	50.00 ng/L	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11001.D
Acq On : 11 Jul 2007 2:34 pm
Sample : Blank
Misc : 25mL w/ #7060081
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35 2007

Vial: 1
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration

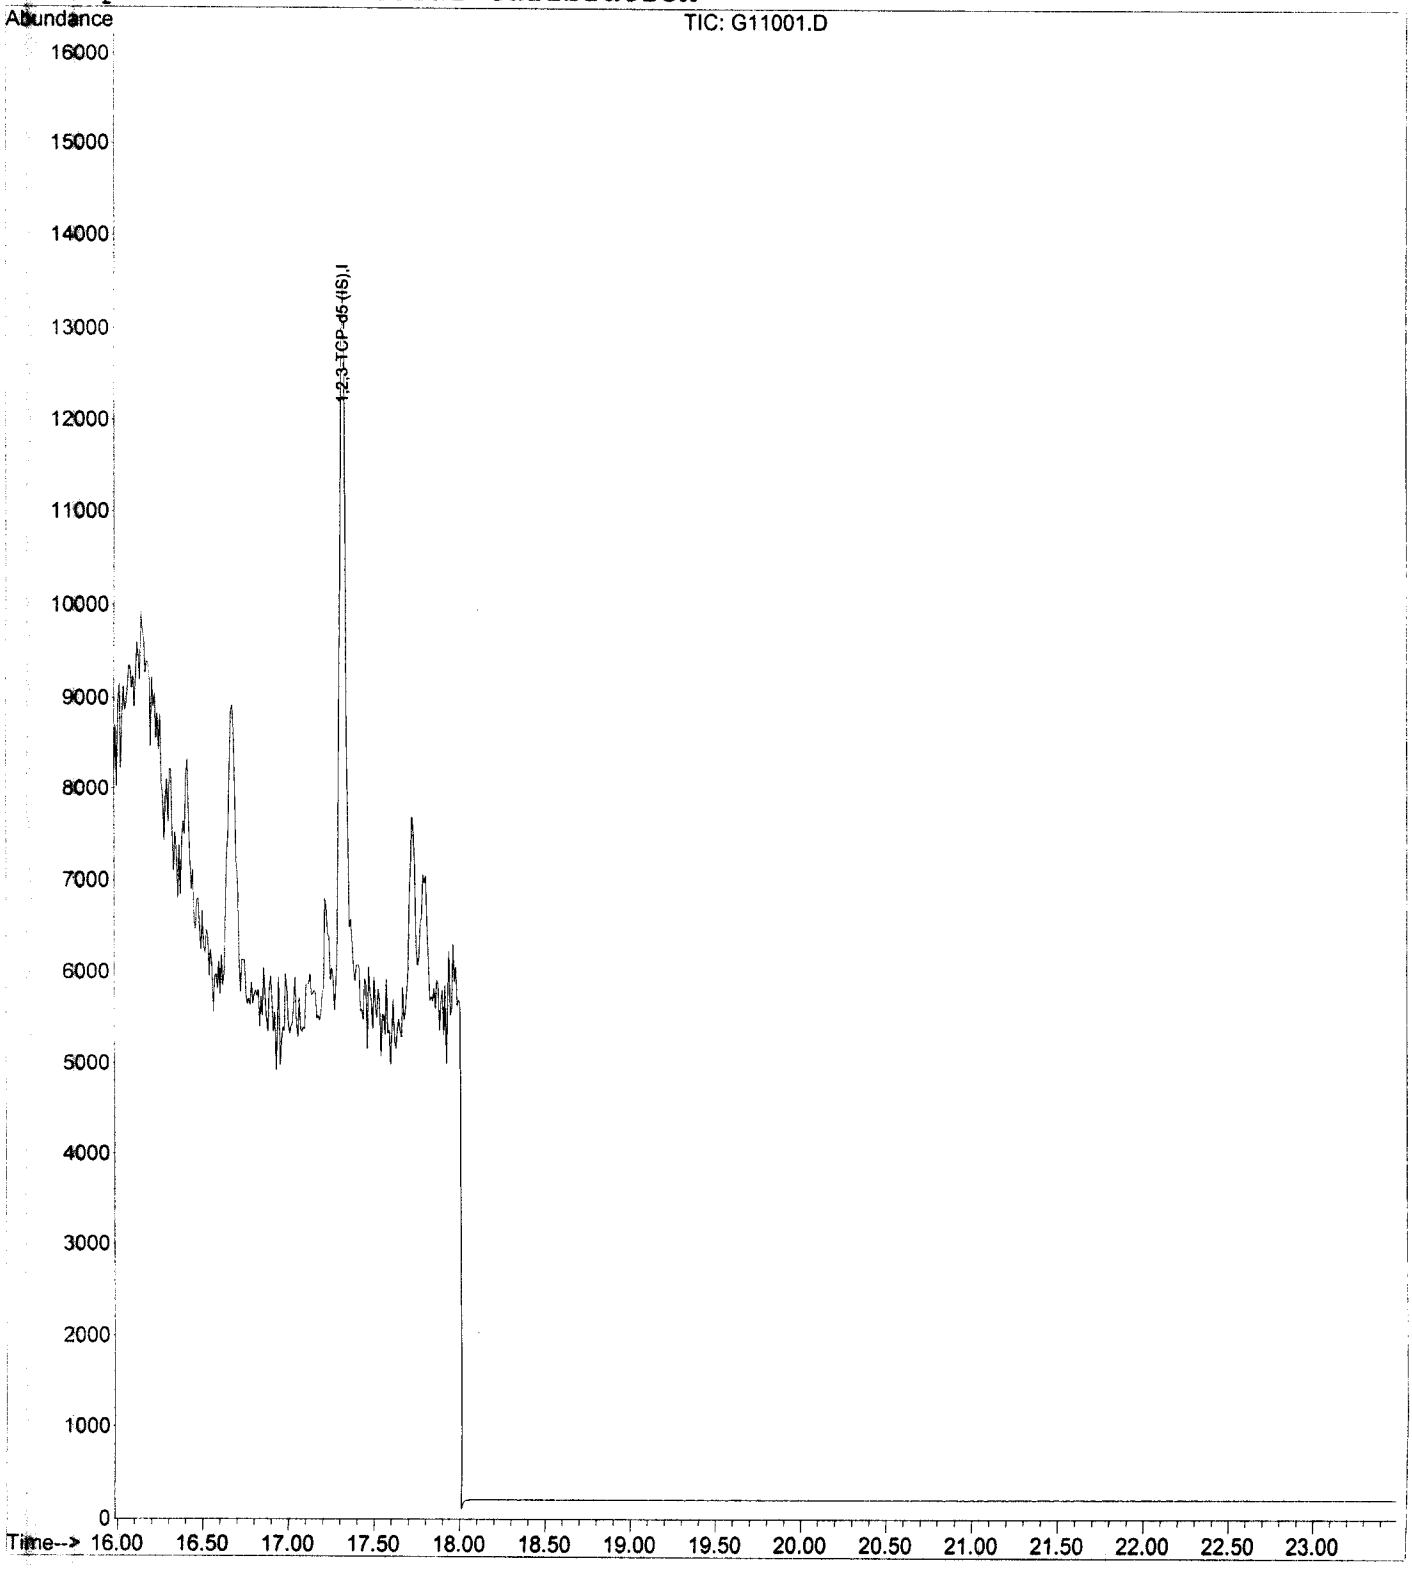

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11002.D
Acq On : 11 Jul 2007 3:07 pm
Sample : 5ppt #7060083
Misc : 25mL Initial Cal
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35:14 2007

Vial: 2
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	17996	50.00 ng/L	0.00
Target Compounds					Qvalue
2) 1,2,3-Trichloropropane	17.41	75	1842	5.65 ng/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11002.D
Acq On : 11 Jul 2007 3:07 pm
Sample : 5ppt #7060083
Misc : 25mL Initial Cal
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35 2007

Vial: 2
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration

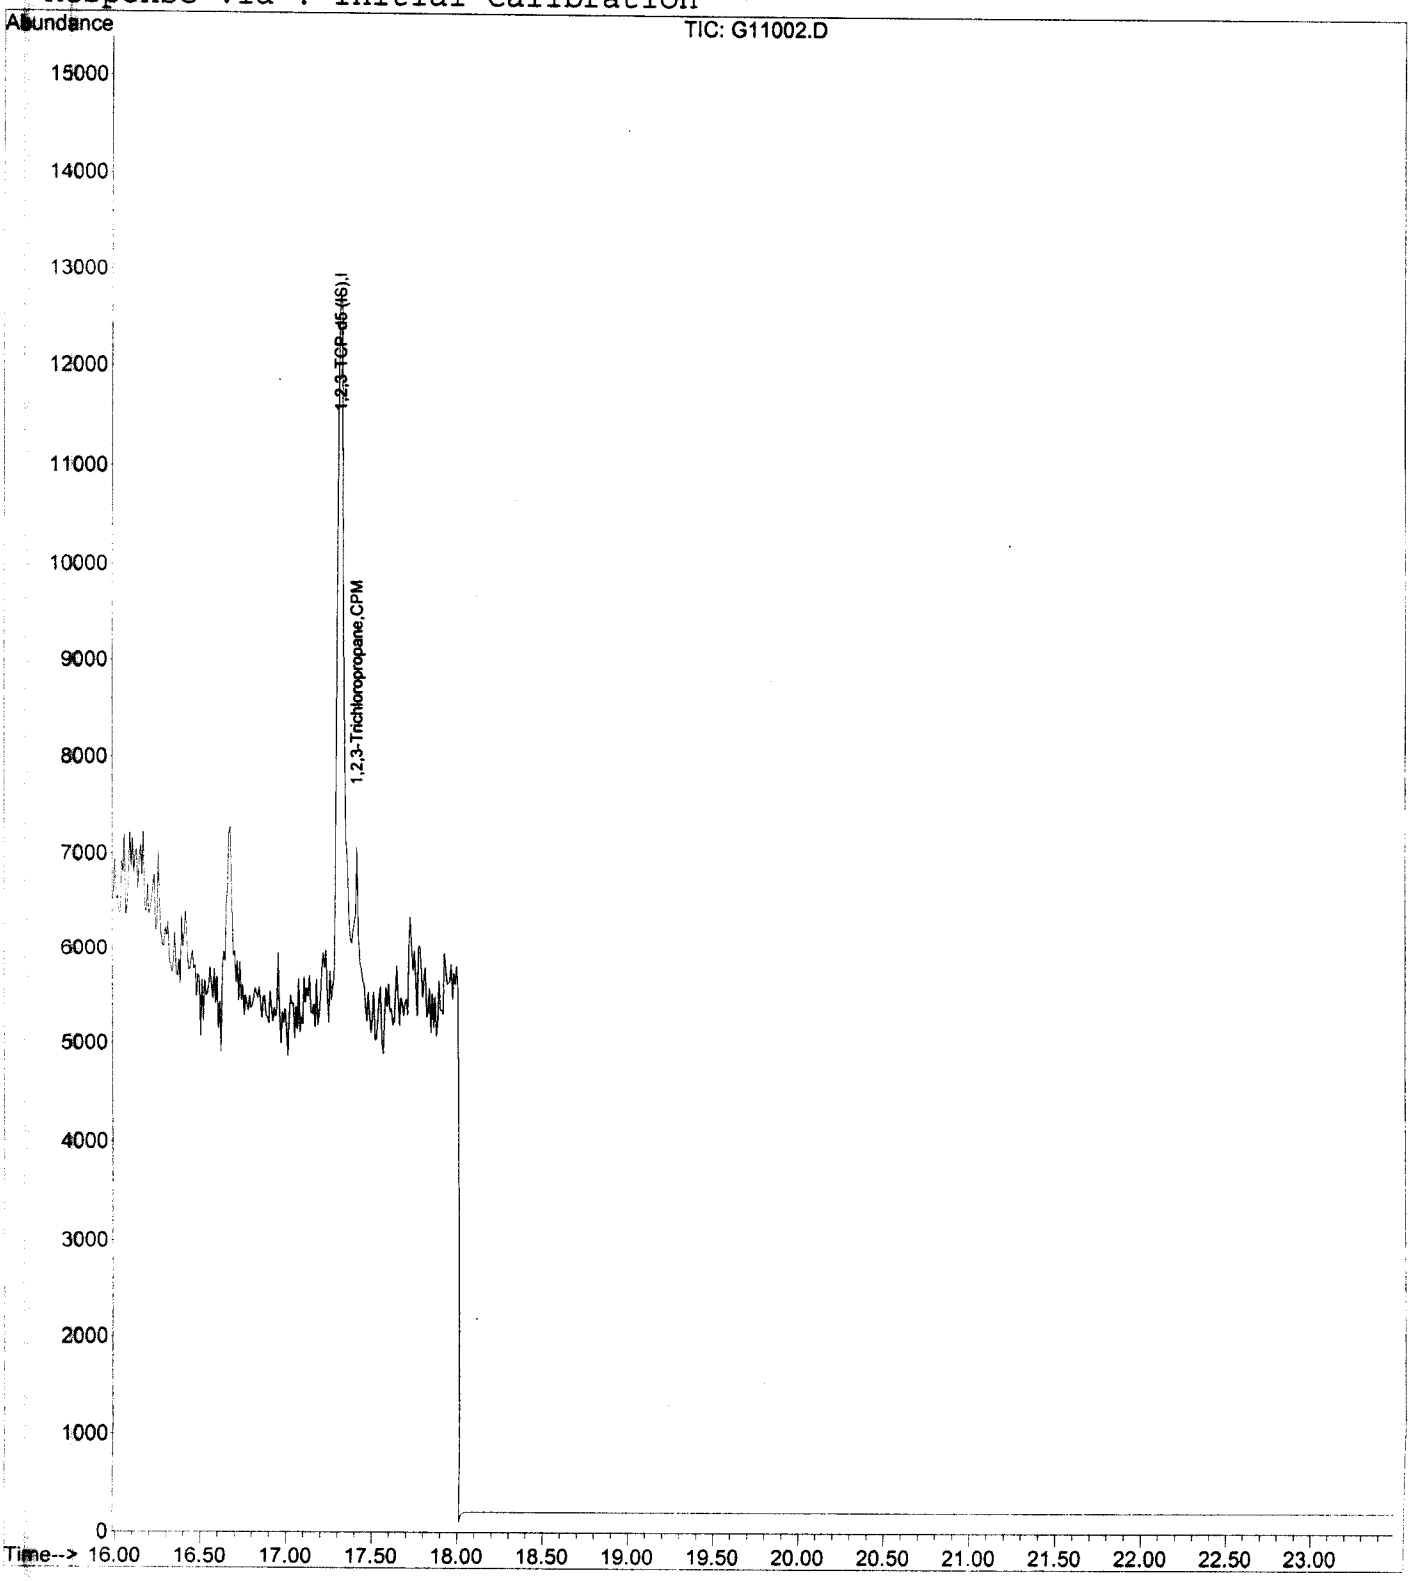

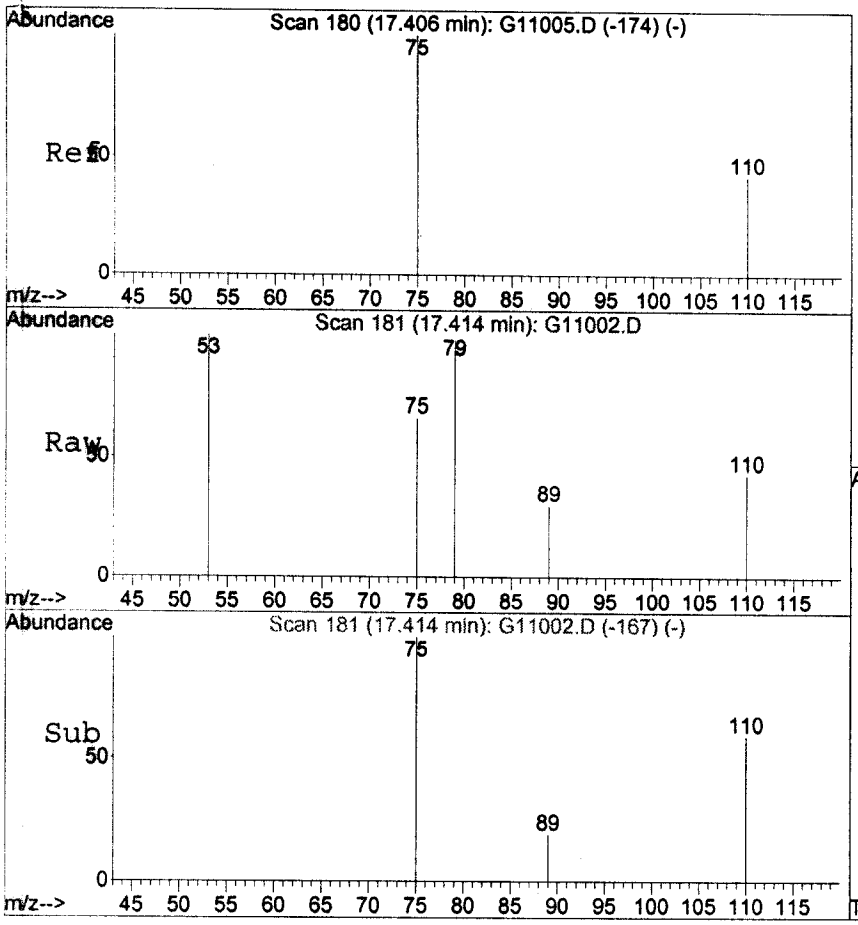

#2
1,2,3-Trichloropropane
Concen: 5.65 ng/L
RT: 17.41 min Scan# 181
Delta R.T. 0.01 min
Lab File: G11002.D
Acq: 11 Jul 2007 3:07 pm

Tgt Ion: 75 Resp: 1842

Ion	Ratio	Lower	Upper
75	100		
110	48.5	11.2	71.2
53	13.2	0.0	30.0
89	7.3	0.0	30.8

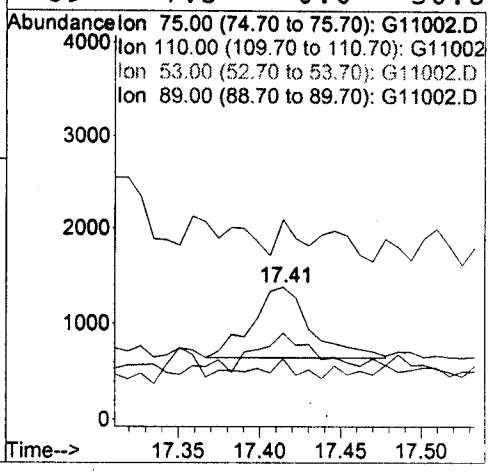

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11003.D
Acq On : 11 Jul 2007 3:39 pm
Sample : 10ppt #7060083
Misc : 25mL Initial Cal
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35:16 2007

Vial: 3
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	16353	50.00 ng/L	0.00
Target Compounds					Qvalue
2) 1,2,3-Trichloropropane	17.41	75	3239	10.94 ng/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11003.D
Acq On : 11 Jul 2007 3:39 pm
Sample : 10ppt #7060083
Misc : 25mL Initial Cal
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35 2007

Vial: 3
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration

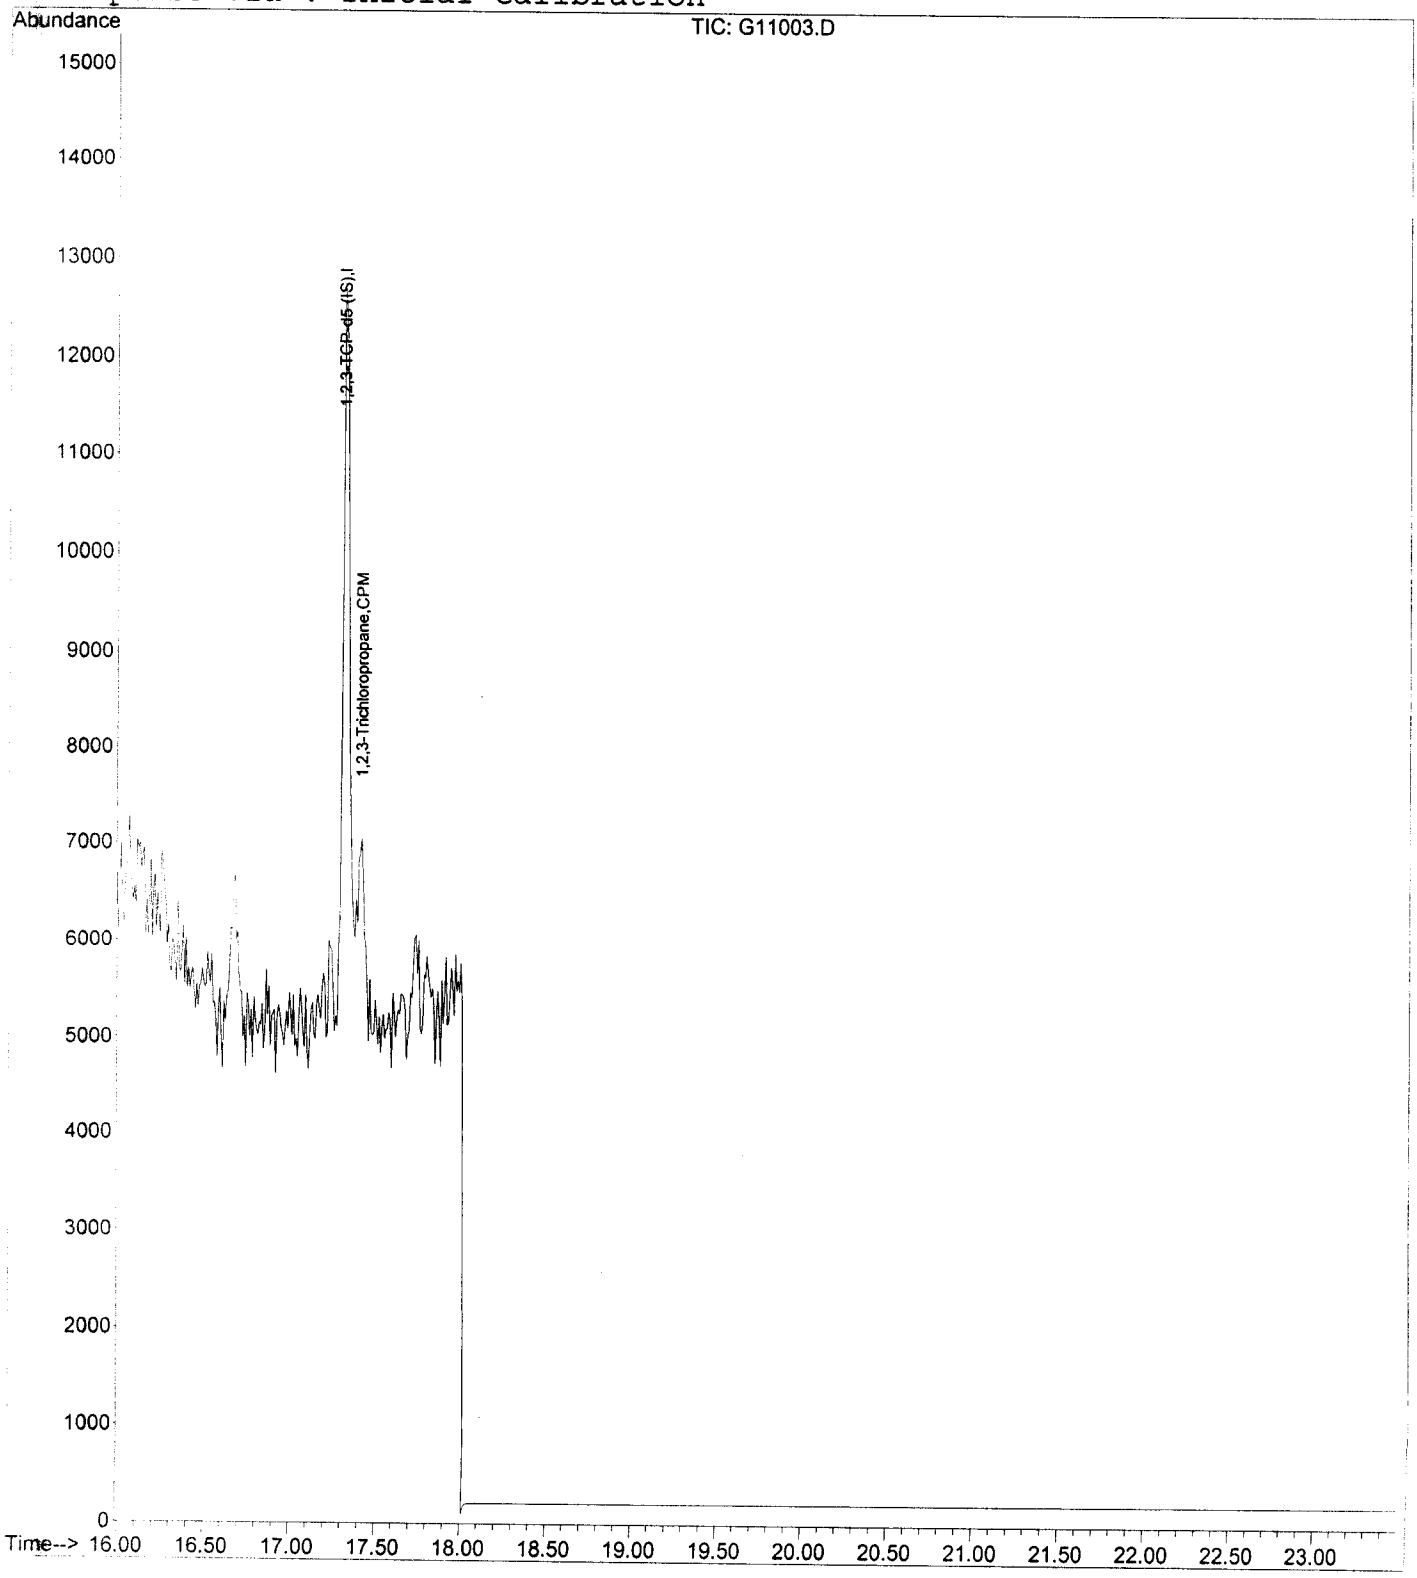

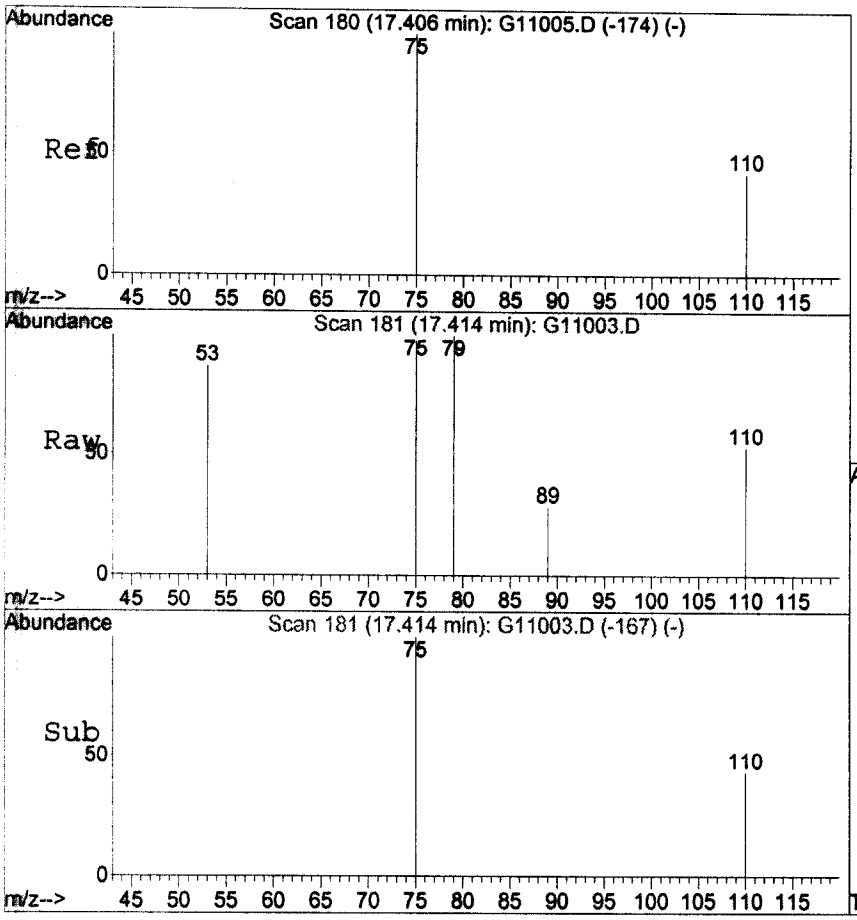

#2
1,2,3-Trichloropropane
Concen: 10.94 ng/L
RT: 17.41 min Scan# 181
Delta R.T. 0.01 min
Lab File: G11003.D
Acq: 11 Jul 2007 3:39 pm

Tgt Ion: 75 Resp: 3239

Ion	Ratio	Lower	Upper
75	100		
110	46.9	11.2	71.2
53	3.8	0.0	30.0
89	9.9	0.0	30.8

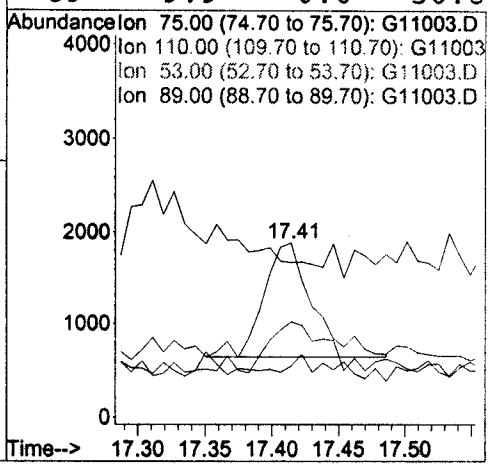

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11004.D
Acq On : 11 Jul 2007 4:12 pm
Sample : 20ppt #7060083
Misc : 25mL Initial Cal
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35:18 2007

Vial: 4
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	18685	50.00 ng/L	0.00
Target Compounds					Qvalue
2) 1,2,3-Trichloropropane	17.41	75	5698	16.84 ng/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11004.D
Acq On : 11 Jul 2007 4:12 pm
Sample : 20ppt #7060083
Misc : 25mL Initial Cal
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35 2007

Vial: 4
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration

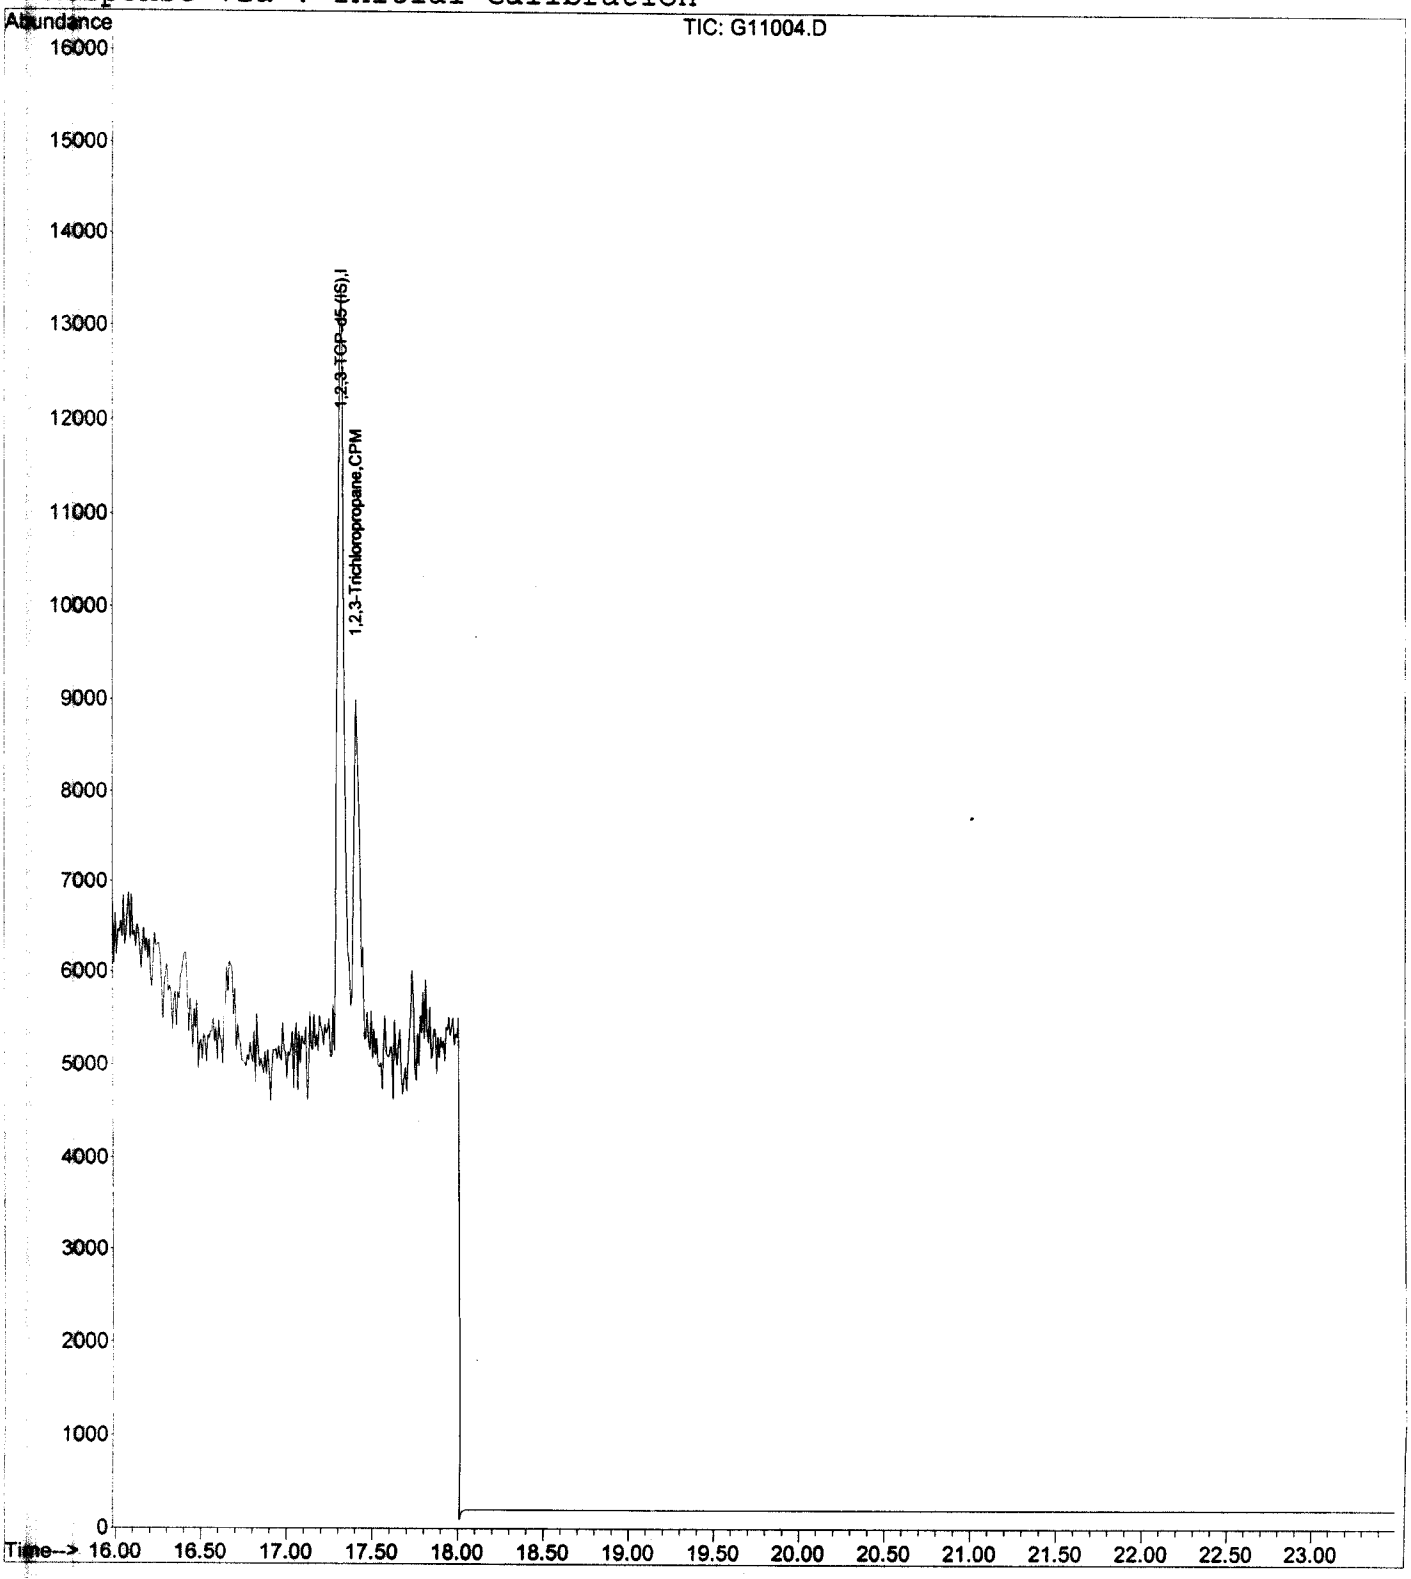

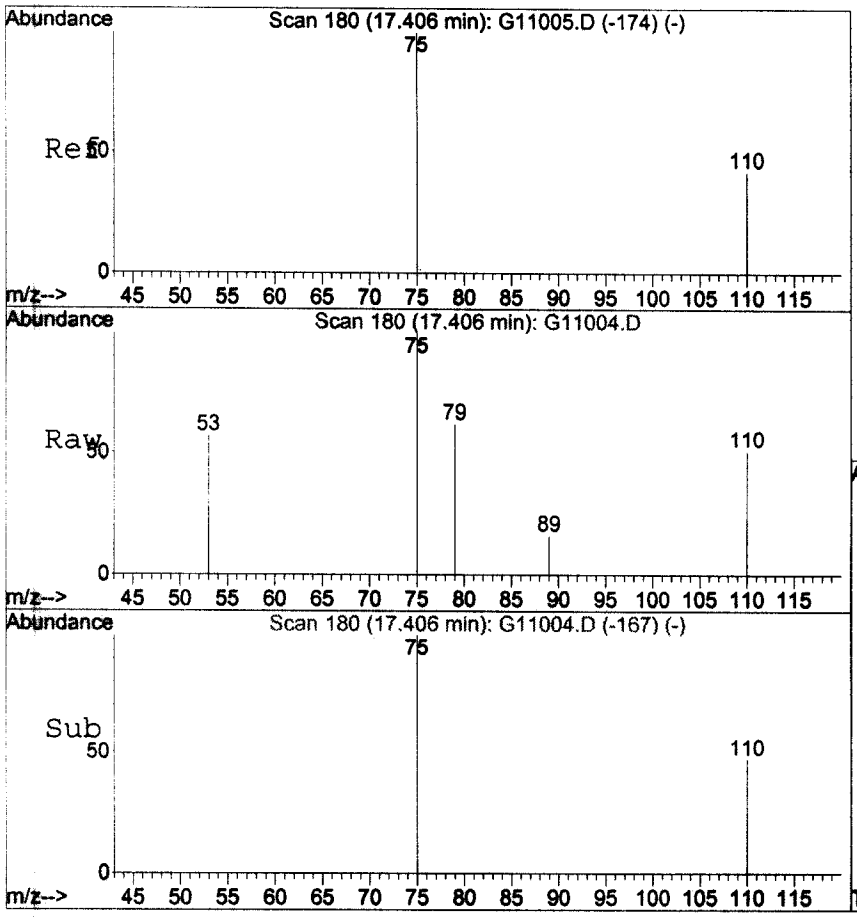

#2
1,2,3-Trichloropropane
Concen: 16.84 ng/L
RT: 17.41 min Scan# 180
Delta R.T. 0.00 min
Lab File: G11004.D
Acq: 11 Jul 2007 4:12 pm

Tgt Ion: 75 Resp: 5698

Ion	Ratio	Lower	Upper
75	100		
110	44.9	11.2	71.2
53	3.6	0.0	30.0
89	2.0	0.0	30.8

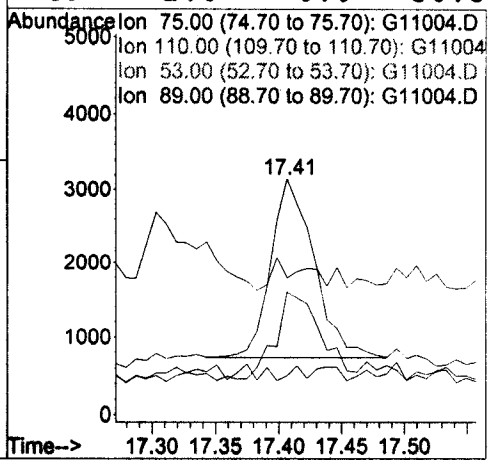

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11005.D
Acq On : 11 Jul 2007 4:44 pm
Sample : 50ppt #7060083
Misc : 25mL Initial Cal
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35:20 2007

Vial: 5
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.31	79	20175	50.00 ng/L	0.00
Target Compounds					Qvalue
2) 1,2,3-Trichloropropane	17.41	75	18153	49.68 ng/L #	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11005.D
Acq On : 11 Jul 2007 4:44 pm
Sample : 50ppt #7060083
Misc : 25mL Initial Cal
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35 2007

Vial: 5
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration

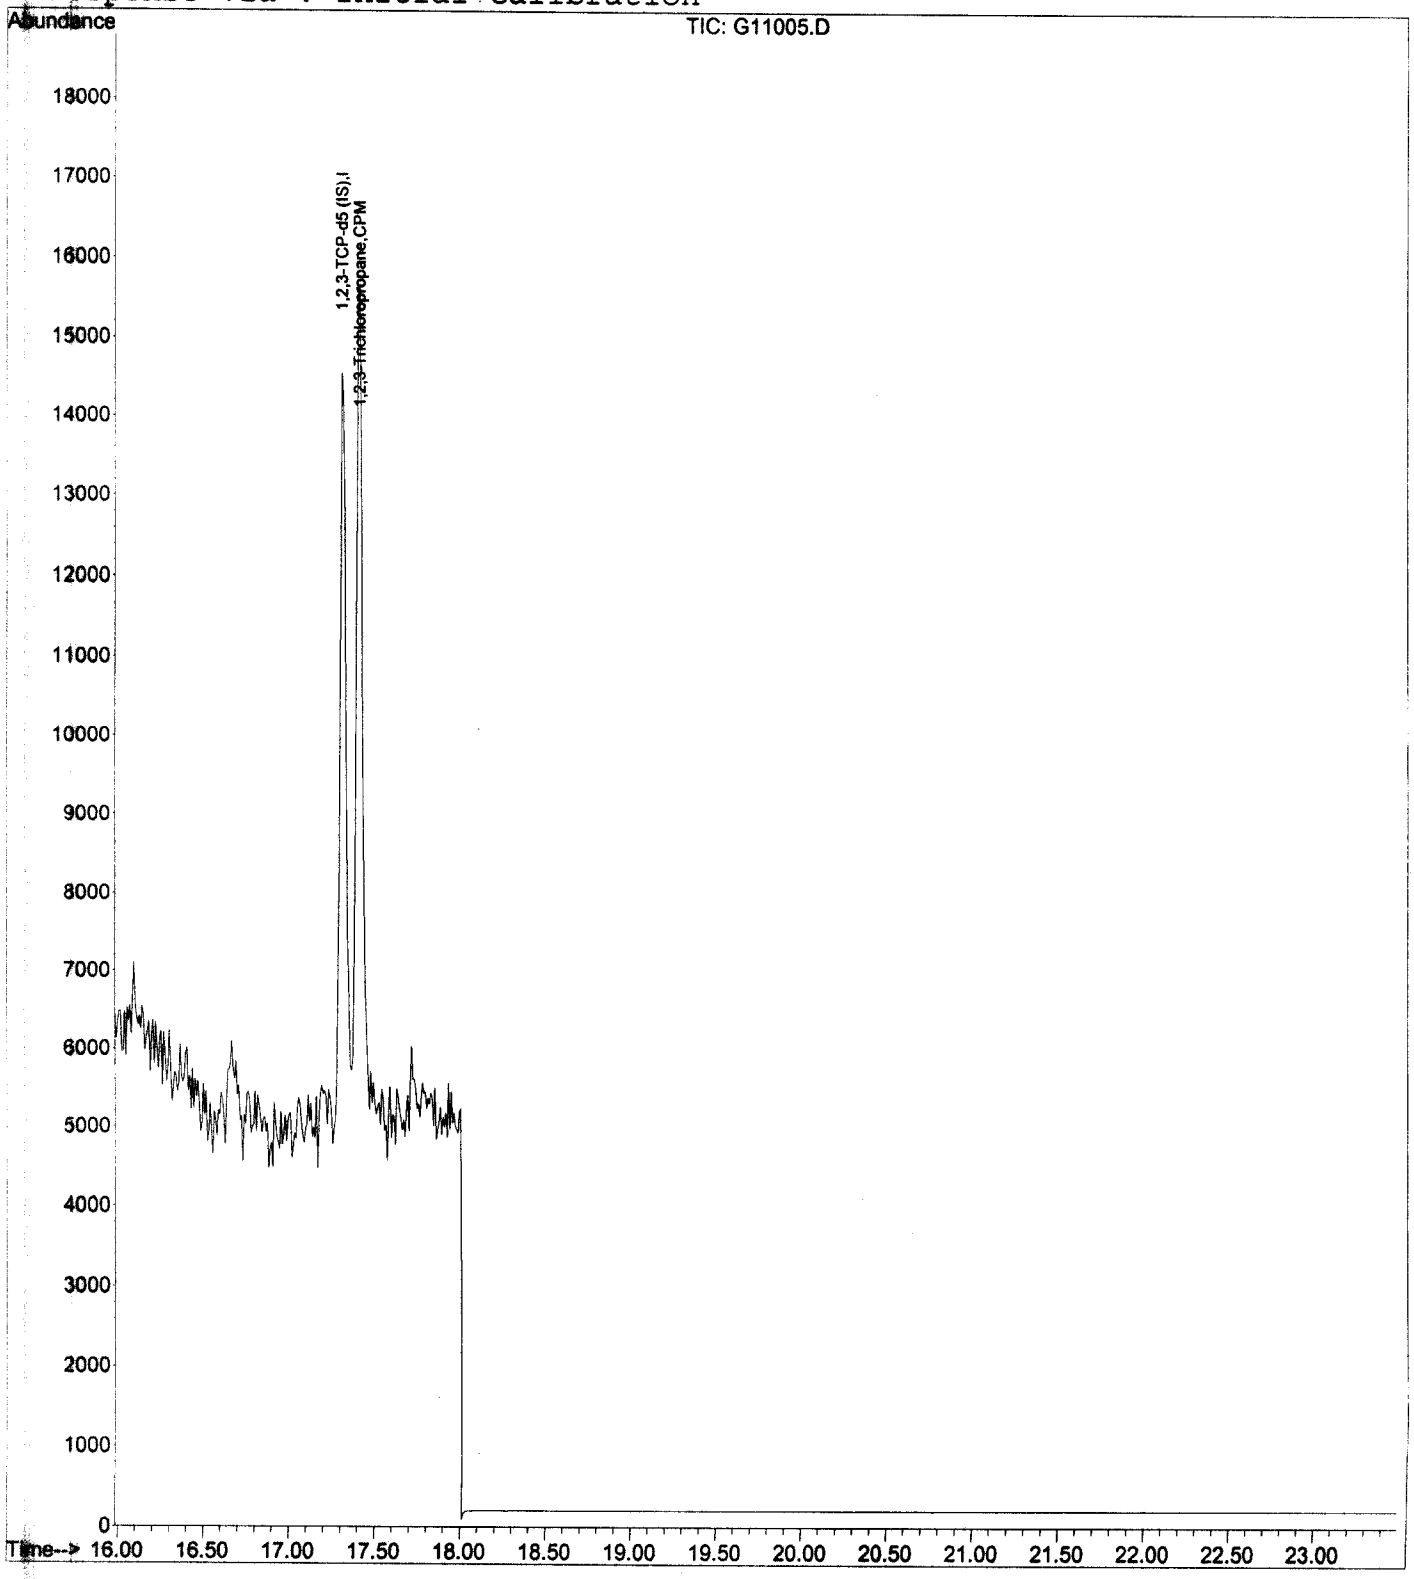

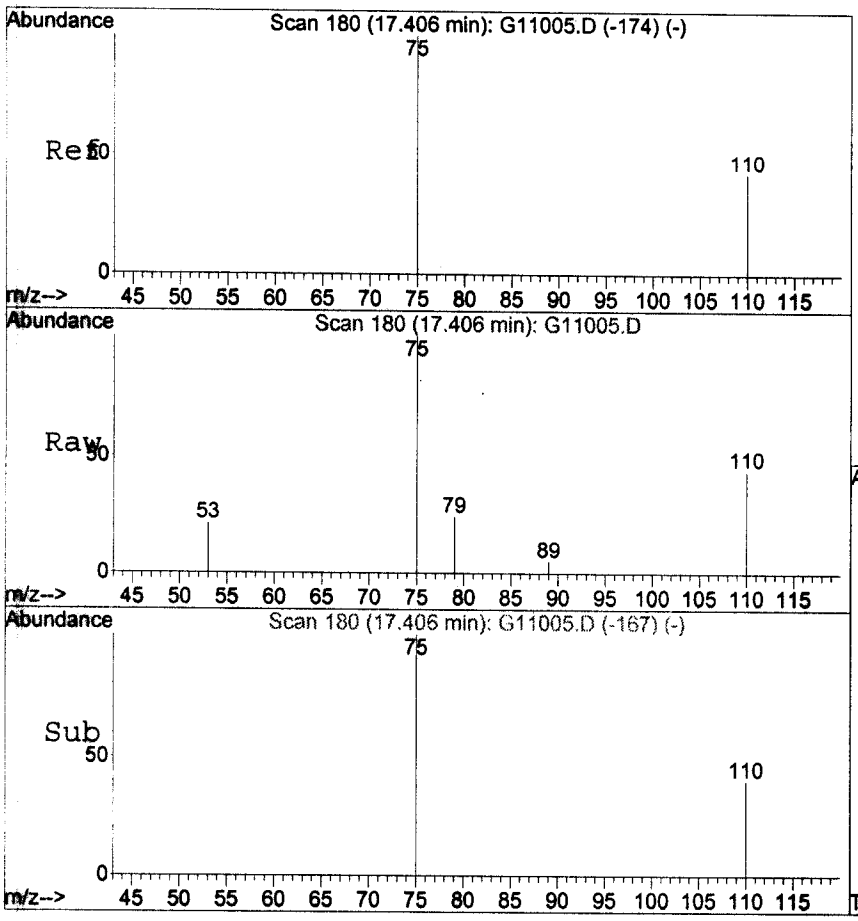

#2
1,2,3-Trichloropropane
Concen: 49.68 ng/L
RT: 17.41 min Scan# 180
Delta R.T. 0.00 min
Lab File: G11005.D
Acq: 11 Jul 2007 4:44 pm

Tgt Ion: 75 Resp: 18153

Ion	Ratio	Lower	Upper
75	100		
110	42.8	11.2	71.2
53	0.0	0.0	30.0
89	0.8	0.0	30.8

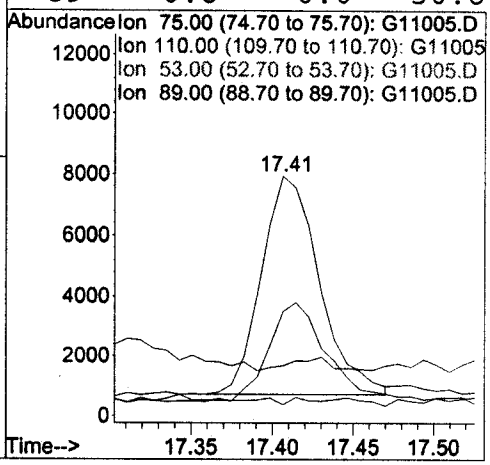

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11006.D
Acq On : 11 Jul 2007 5:17 pm
Sample : 100ppt #7060083
Misc : 25mL Initial Cal
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35:23 2007

Vial: 6
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	20782	50.00 ng/L	0.00
Target Compounds					Qvalue
2) 1,2,3-Trichloropropane	17.41	75	39027	103.69 ng/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11006.D
Acq On : 11 Jul 2007 5:17 pm
Sample : 100ppt #7060083
Misc : 25mL Initial Cal
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35 2007

Vial: 6
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration

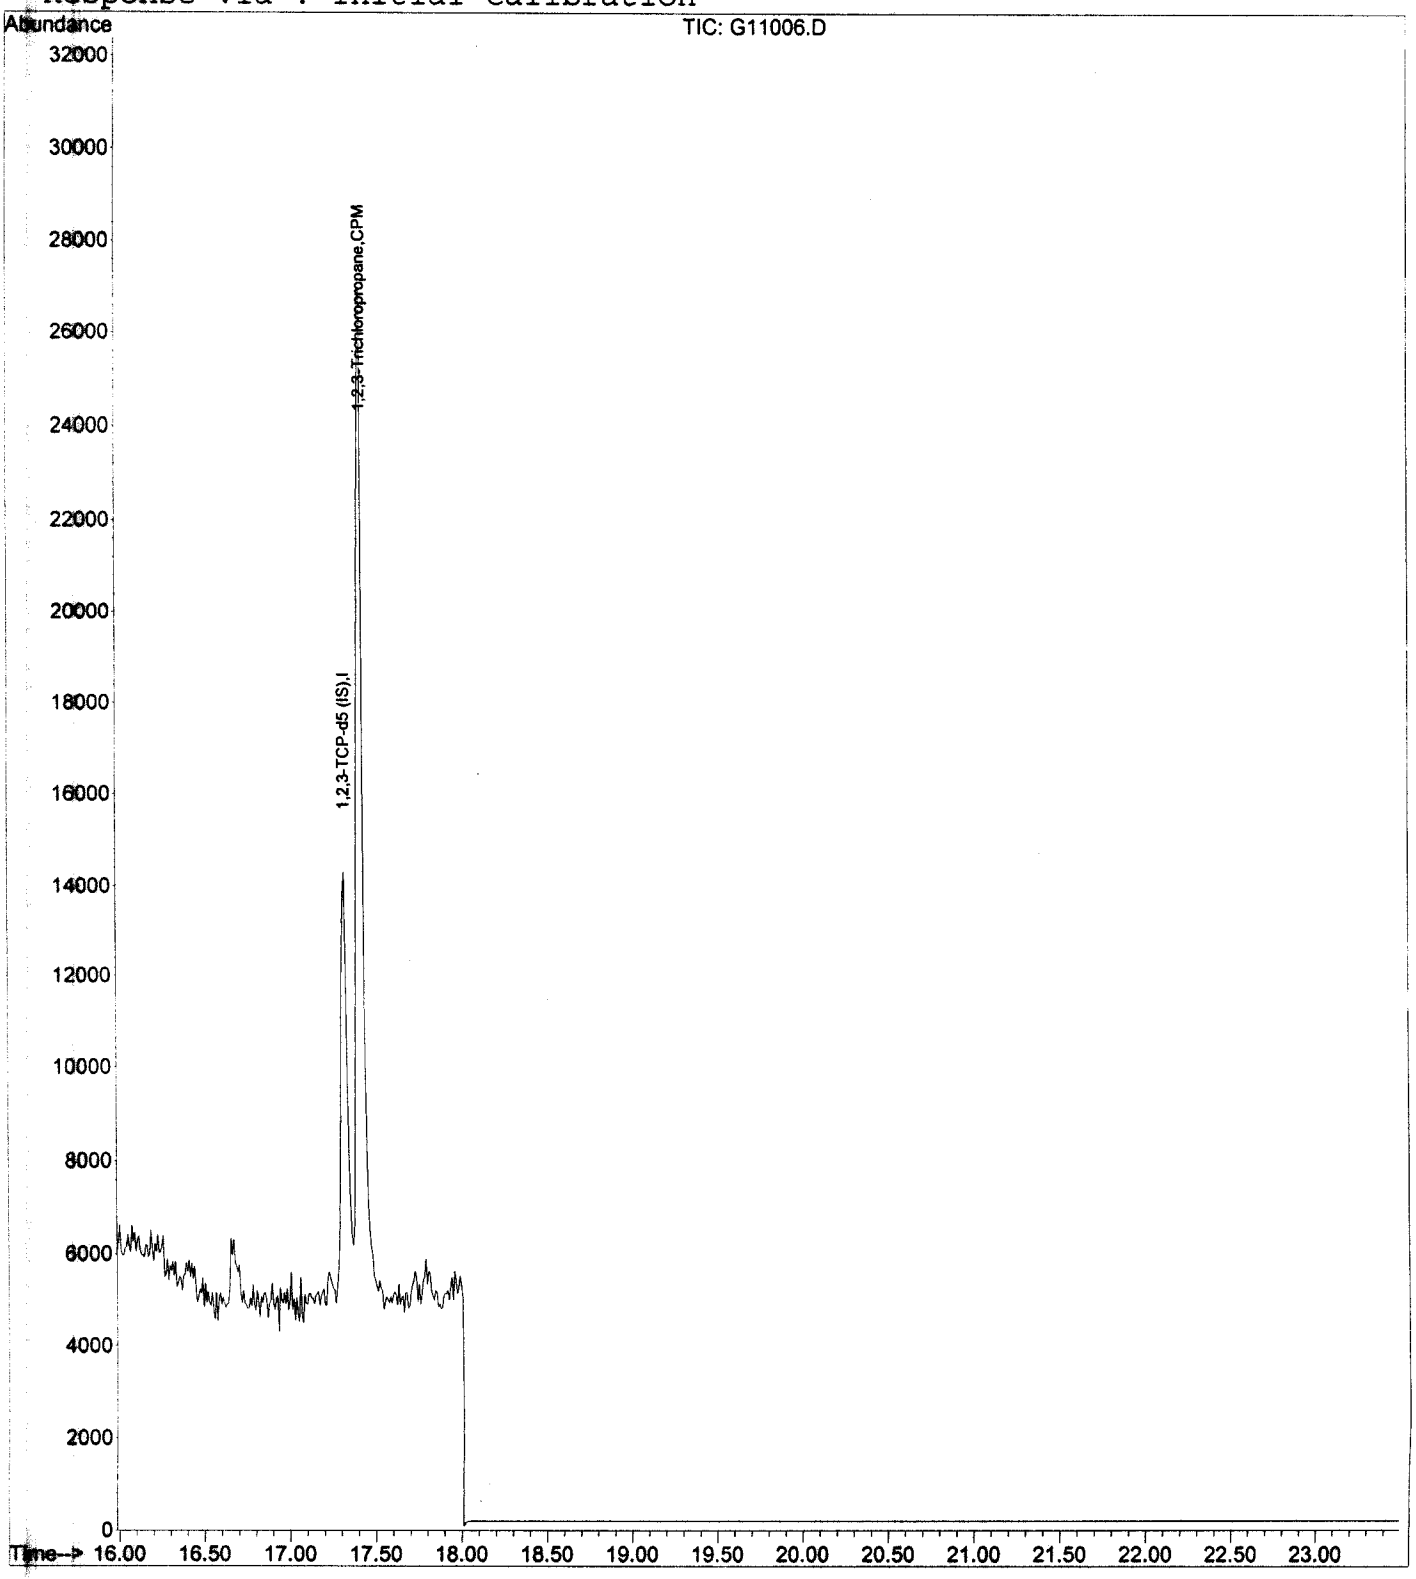

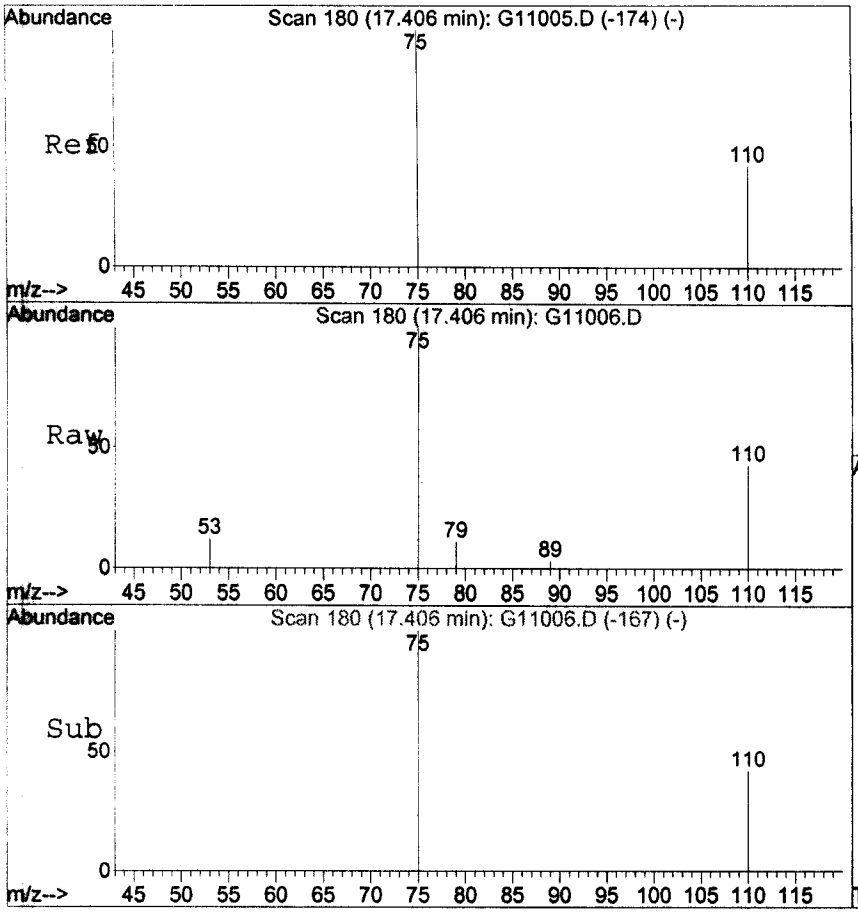

#2
1,2,3-Trichloropropane
Concen: 103.69 ng/L
RT: 17.41 min Scan# 180
Delta R.T. -0.00 min
Lab File: G11006.D
Acq: 11 Jul 2007 5:17 pm

Tgt Ion: 75 Resp: 39027

Ion	Ratio	Lower	Upper
75	100		
110	41.5	11.2	71.2
53	0.5	0.0	30.0
89	0.2	0.0	30.8

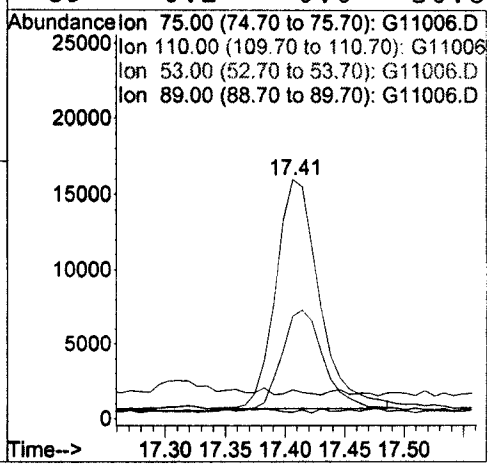

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11007.D
Acq On : 11 Jul 2007 5:50 pm
Sample : 200ppt #7060083
Misc : 25mL Initial Cal
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35:25 2007

Vial: 7
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	22449	50.00 ng/L	0.00
Target Compounds					Qvalue
2) 1,2,3-Trichloropropane	17.41	75	78205	192.36 ng/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11007.D
Acq On : 11 Jul 2007 5:50 pm
Sample : 200ppt #7060083
Misc : 25mL Initial Cal
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35 2007

Vial: 7
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration

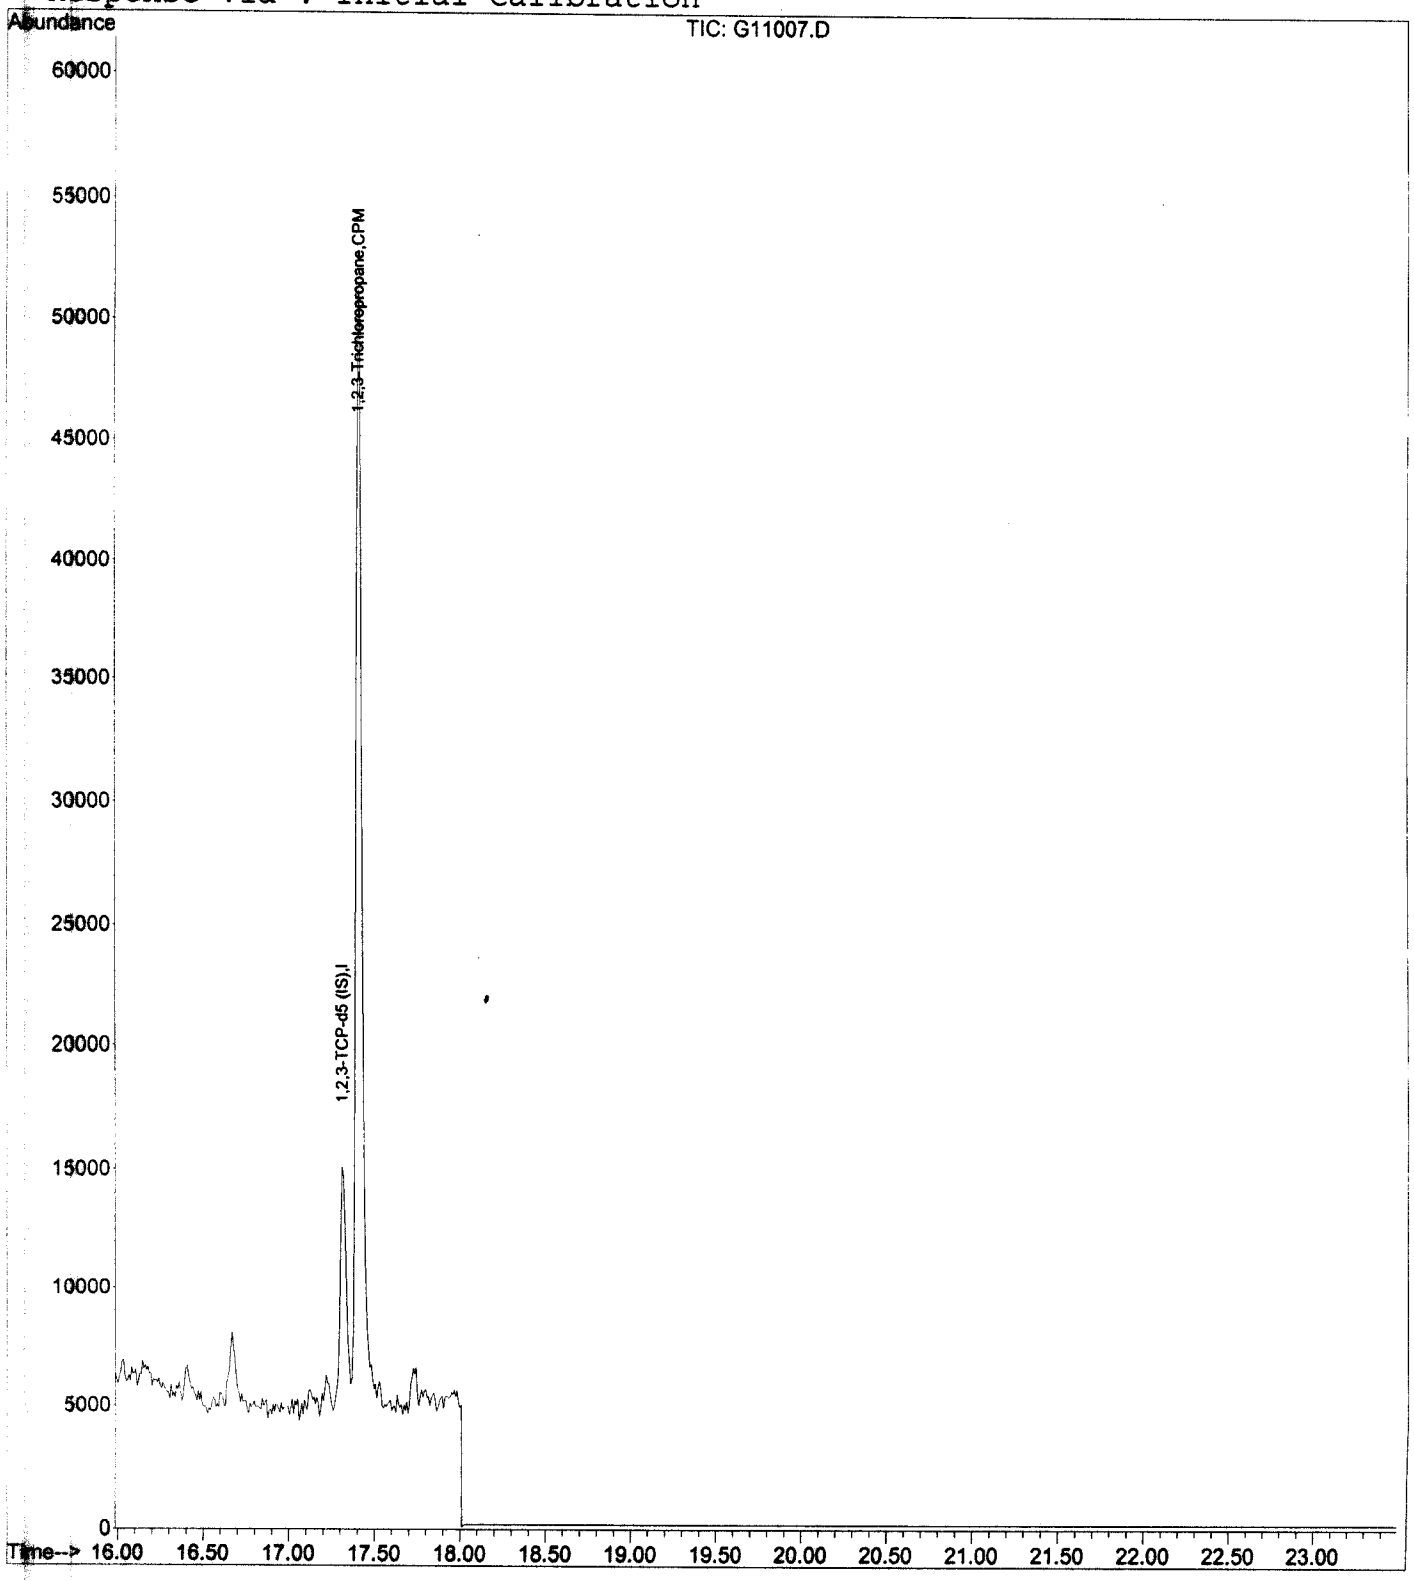

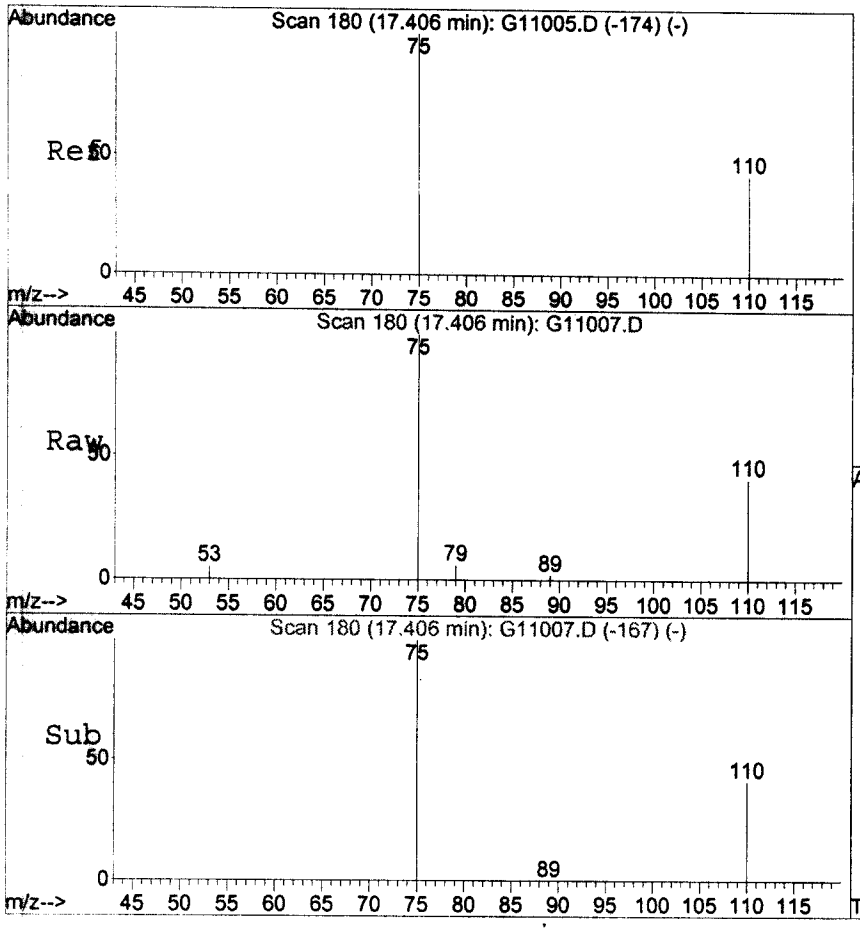

#2
1,2,3-Trichloropropane
Concen: 192.36 ng/L
RT: 17.41 min Scan# 180
Delta R.T. -0.00 min
Lab File: G11007.D
Acq: 11 Jul 2007 5:50 pm

Tgt Ion: 75 Resp: 78205

Ion	Ratio	Lower	Upper
75	100		
110	43.2	11.2	71.2
53	0.4	0.0	30.0
89	0.6	0.0	30.8

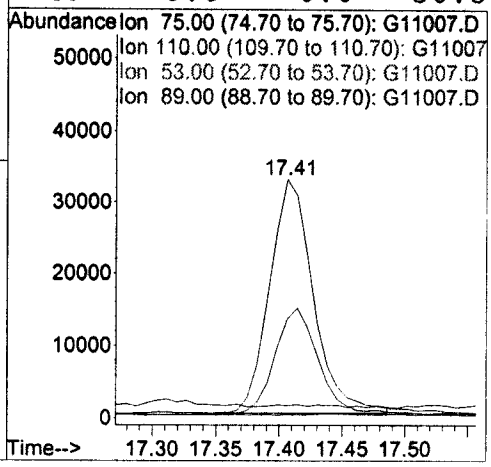

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11008.D
Acq On : 11 Jul 2007 6:22 pm
Sample : 500ppt #7060083
Misc : 25mL Initial Cal
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35:27 2007

Vial: 8
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.31	79	26639	50.00 ng/L	0.00
Target Compounds					Qvalue
2) 1,2,3-Trichloropropane	17.41	75	227168	470.87 ng/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL11\G11008.D
Acq On : 11 Jul 2007 6:22 pm
Sample : 500ppt #7060083
Misc : 25mL Initial Cal
MS Integration Params: RTEINT.P
Quant Time: Jul 12 16:35 2007

Vial: 8
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 16:34:52 2007
Response via : Initial Calibration

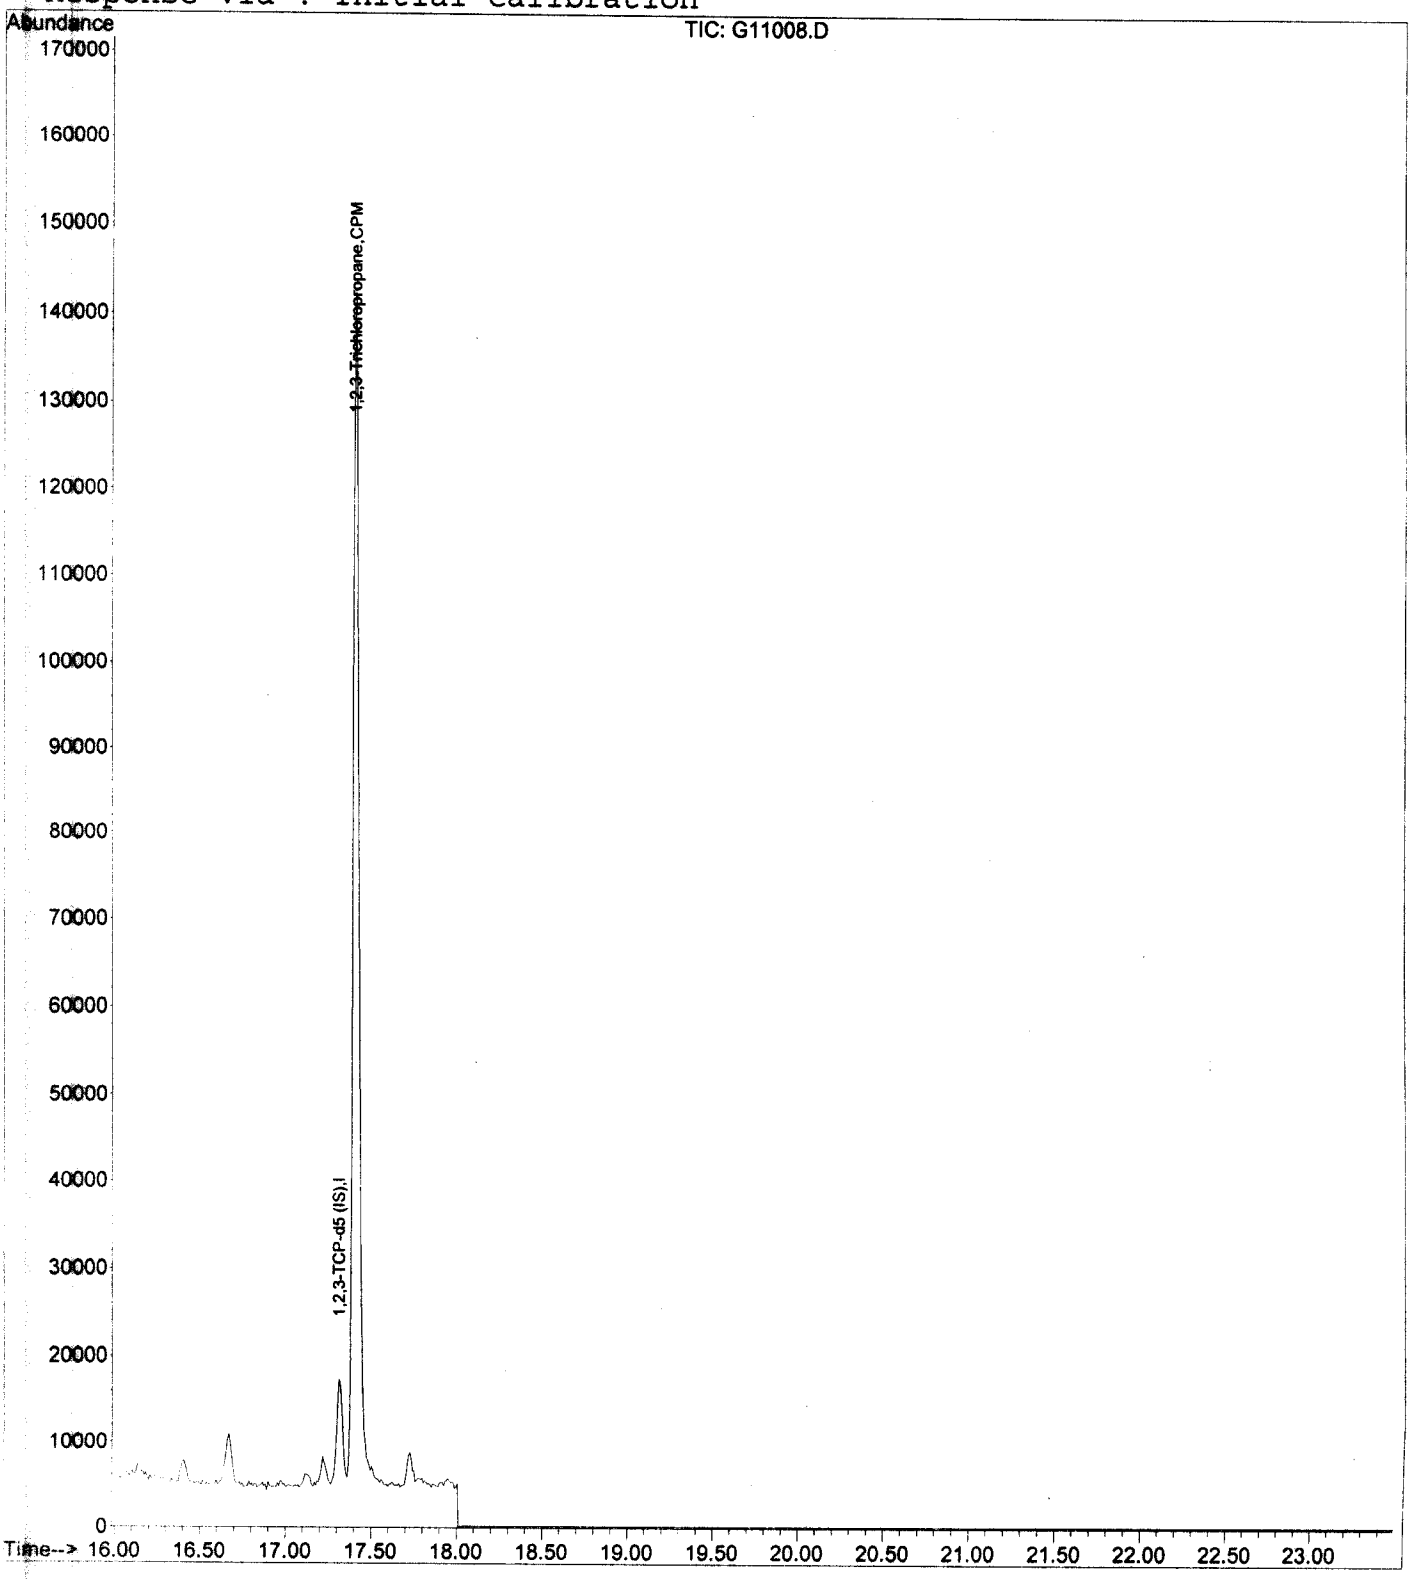

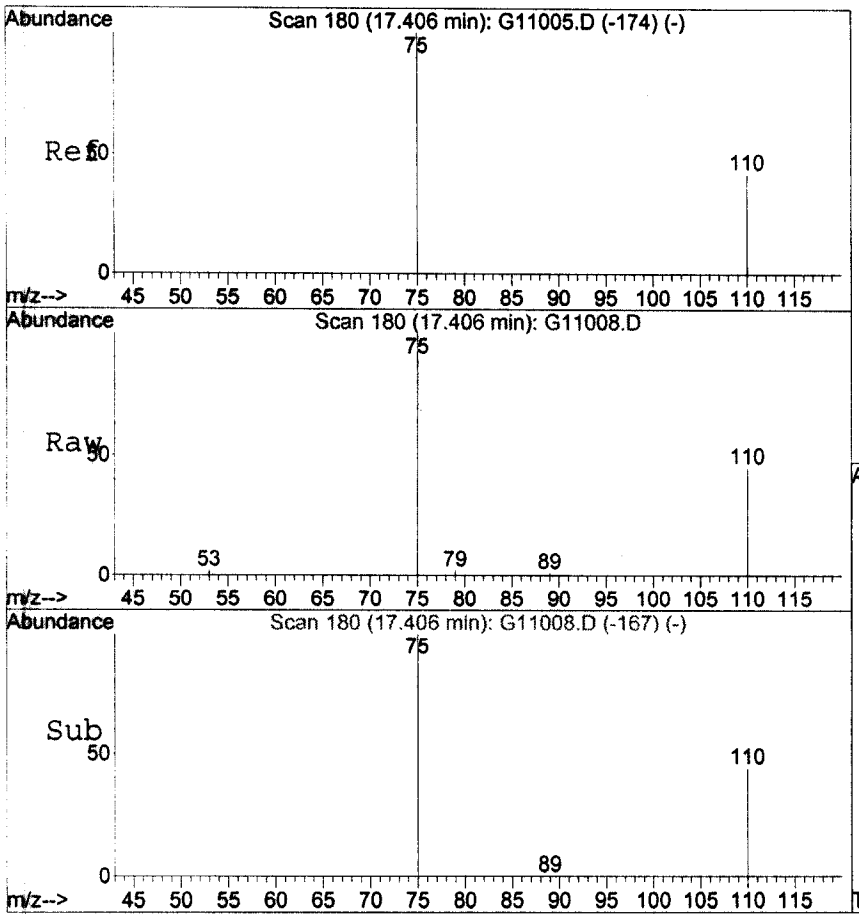

#2
1,2,3-Trichloropropane
Concen: 470.87 ng/L
RT: 17.41 min Scan# 180
Delta R.T. 0.00 min
Lab File: G11008.D
Acq: 11 Jul 2007 6:22 pm

Tgt Ion: 75 Resp: 227168

Ion	Ratio	Lower	Upper
75	100		
110	43.7	11.2	71.2
53	1.1	0.0	30.0
89	0.3	0.0	30.8

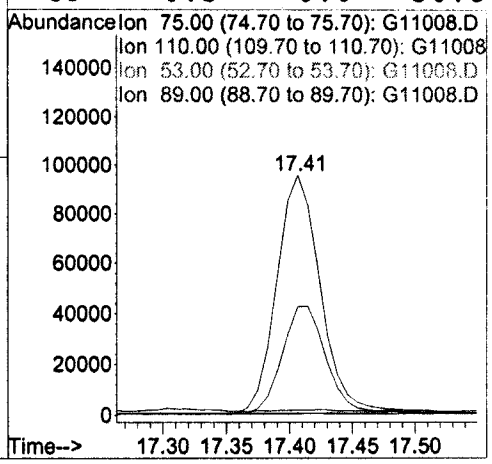

TOPLEVEL PARAMETERS

Method Information For: C:\MSDCHEM\1\METHODS\123-TCP071107.M

Method Sections To Run:

( ) Save Copy of Method With Data
( ) Pre-Run Cmd/Macro =
(X) Data Acquisition
(X) Data Analysis
( ) Post-Run Cmd/Macro =

Method Comments:
This is the DHS method for 1,2,3-TCP

END OF TOPLEVEL PARAMETERS

INSTRUMENT CONTROL PARAMETERS

Sample Inlet: GC
Injection Source: Manual
Injection Location: Front
Mass Spectrometer: Enabled

6890 GC METHOD

OVEN
Initial temp: 40 'C (On)
Initial time: 3.00 min
Maximum temp: 350 'C
Equilibration time: 0.00 min
Ramps:

#	Rate	Final temp	Final time
1	12.00	70	1.00
2	10.00	190	0.00
3	25.00	230	3.40
4	0.0(Off)		

Post temp: 70 'C
Post time: 0.00 min
Run time: 23.50 min

FRONT INLET (UNKNOWN)
Mode: Split
Initial temp: 200 'C (On)
Pressure: 19.11 psi (On)
Split ratio: 13:1
Split flow: 15.1 mL/min
Total flow: 18.7 mL/min
Gas saver: Off
Gas type: Helium

BACK INLET ()

COLUMN 1
Capillary Column
Model Number: Agilent 122-1564
DB-VRX, 0.25mm * 60m * 1.4um
Max temperature: 260 'C
Nominal length: 60.0 m
Nominal diameter: 250.00 um
Nominal film thickness: 1.40 um
Mode: constant flow
Initial flow: 1.2 mL/min
Nominal init pressure: 19.12 psi
Average velocity: 28 cm/sec
Inlet: Front Inlet
Outlet: MSD
Outlet pressure: vacuum

COLUMN 2
(not installed)

FRONT DETECTOR (NO DET)

BACK DETECTOR (NO DET)

SIGNAL 1
Data rate: 20 Hz
Type: test plot
Save Data: Off
Zero: 0.0 (Off)
Range: 0
Fast Peaks: Off
Attenuation: 0

SIGNAL 2
Data rate: 20 Hz
Type: test plot
Save Data: Off
Zero: 0.0 (Off)
Range: 0
Fast Peaks: Off
Attenuation: 0

COLUMN COMP 1
(No Detectors Installed)

COLUMN COMP 2
(No Detectors Installed)

THERMAL AUX 2
Use: MSD Transfer Line Heater
Description:
Initial temp: 240 'C (On)
Initial time: 0.00 min

#	Rate	Final temp	Final time
1	0.0(Off)		

POST RUN
Post Time: 0.00 min

TIME TABLE

Time	Specifier	Parameter & Setpoint

7673 Injector

Front Injector:
Injector not configured, use these parameters if it becomes configured

Sample Washes	2	
Sample Pumps	4	
Injection Volume	1.0	microliters
Syringe Size	10.0	microliters
PostInj Solvent A Washes	4	
PostInj Solvent B Washes	0	
Viscosity Delay	0	seconds
Plunger Speed	Slow	

Back Injector:

No parameters specified

MS ACQUISITION PARAMETERS

General Information
------- -----------

Tune File : bfb.u
Acquistion Mode : SIM

MS Information
-- -----------

Solvent Delay : 15.90 min

EM Absolute : False
EM Offset : 306
Resulting EM Voltage : 1858.8

[Sim Parameters]

GROUP 1
Group ID : 1
Resolution : Low
Plot 1 Ion : 75.0
Ions/Dwell In Group (Mass, Dwell) (Mass, Dwell) (Mass, Dwell)
(53.0, 50) (75.0, 150) (79.0, 50)
(89.0, 50) (110.0, 100)

[MSZones]

MS Quad : 150 C maximum 200 C
MS Source : 230 C maximum 250 C
Timed Events
----- ------

[Timed MS Detector Entries]

Time (min) State (MS on/off)
18.00 Off

END OF MS ACQUISITION PARAMETERS

END OF INSTRUMENT CONTROL PARAMETERS

DATA ANALYSIS PARAMETERS

Method Name: C:\MSDCHEM\1\METHODS\123-TCP071107.M

Percent Report Settings

Sort By: Signal

Output Destination
    Screen: No
    Printer: Yes
    File: No

Integration Events: Meth Default

Generate Report During Run Method: No

Signal Correlation Window: 0.020

Quantitative Report Settings

Report Type: Summary

Output Destination
    Screen: Yes
    Printer: No
    File: No

Generate Report During Run Method: No

1,2,3-TCP by GCMS SIM
Calibration Last Updated: Thu Jul 12 12:36:02 2007

Reference Window: 0.50 Minutes
Non-Reference Window: 0.50 Minutes
Correlation Window: 0.10 minutes
Default Multiplier: 1.00
Default Sample Concentration: 0.00

Compound Information

---

1) 1,2,3-TCP-d5 (IS) (ISTD TR)
Ret. Time 17.31 min., Extract & Integrate from 17.21 to 17.41 min.

Lvl ID	Conc (ng/L)	Response
5	50.000	17996
10	50.000	16353
20	50.000	18685
50	50.000	20175
100	50.000	20782
200	50.000	22449
500	50.000	26639

ISTD conc: 50.000 ng/L
Curve Fit: Avg. RF

---

2) 1,2,3-Trichloropropane ( )
Ret. Time 17.41 min., Extract & Integrate from 17.31 to 17.51 min.

Lvl	ID	Conc (ng/L)	Response
5		5.000	1842
10		10.000	3239
20		20.000	5698
50		50.000	18153
100		100.000	39027
200		200.000	78205
500		500.000	227168

Curve Fit: Avg. RF

END OF DATA ANALYSIS PARAMETERS

Fri Jul 13 09:22:03 2007

Additional Information for 123-TCP031504.M
File created Fri Mar 12 12:56:50 2004

Method D:\MSDCHEM\1\METHODS\123-TCP031004.M (GCMS 9) renamed as D:\MSDCHEM\1\METHODS\123-TCP031504.M
Fri Mar 12 12:56:50 2004 (GCMS 7)

Method D:\MSDCHEM\1\METHODS\123-TCP031504.M renamed as D:\MSDCHEM\1\METHODS\123-TCP031704.M
Wed Mar 17 12:53:52 2004

Method D:\MSDCHEM\1\METHODS\123-TCP031704.M renamed as D:\MSDCHEM\1\METHODS\123-TCP050404.M
Tue May 04 16:23:19 2004

Method D:\MSDCHEM\1\METHODS\123-TCP050404.M renamed as D:\MSDCHEM\1\METHODS\123-TCP061404.M
Mon Jun 14 15:54:54 2004

Method D:\MSDCHEM\1\METHODS\123-TCP061404.M renamed as D:\MSDCHEM\1\METHODS\123-TCP072904.M
Thu Jul 29 09:15:27 2004

Method D:\MSDCHEM\1\METHODS\123-TCP072904.M renamed as D:\MSDCHEM\1\METHODS\123-TCP110404.M
Thu Nov 04 17:20:37 2004

Method D:\MSDCHEM\1\METHODS\123-TCP110404.M renamed as D:\MSDCHEM\1\METHODS\123-TCP121004.M
Fri Dec 10 16:20:45 2004

Method D:\MSDCHEM\1\METHODS\123-TCP121004.M renamed as D:\MSDCHEM\1\METHODS\123-TCP010605.M
Fri Jan 07 09:03:10 2005

Method D:\MSDCHEM\1\METHODS\123-TCP010605.M renamed as D:\MSDCHEM\1\METHODS\123-TCP053105.M
Wed Jun 01 09:06:34 2005

Method D:\MSDCHEM\1\METHODS\123-TCP053105.M renamed as D:\MSDCHEM\1\METHODS\123-TCP060305.M
Mon Jun 06 08:40:48 2005

Method C:\MSDCHEM\1\METHODS\123-TCP060305.M renamed as C:\MSDCHEM\1\METHODS\123-TCP071505.M
Fri Jul 15 12:17:26 2005

Method C:\MSDCHEM\1\METHODS\123-TCP071505.M renamed as C:\MSDCHEM\1\METHODS\123-

Mon Feb 19 22:14:38 2007

Method C:\MSDCHEM\1\METHODS\123-TCP021907.M renamed as C:\MSDCHEM\1\METHODS\123-TCP032207.M
Fri Mar 23 08:06:38 2007

Method C:\MSDCHEM\1\METHODS\123-TCP032207.M renamed as C:\MSDCHEM\1\METHODS\123-TCP042507.M
Thu Apr 26 10:20:53 2007

Method C:\MSDCHEM\1\METHODS\123-TCP042507.M renamed as C:\MSDCHEM\1\METHODS\123-TCP051507.M
Wed May 16 08:15:14 2007

Method C:\MSDCHEM\1\METHODS\123-TCP051507.M renamed as C:\MSDCHEM\1\METHODS\123-TCP061307.M
Thu Jun 14 08:19:23 2007

Method C:\MSDCHEM\1\METHODS\123-TCP061307.M renamed as C:\MSDCHEM\1\METHODS\123-TCP061807.M
Tue Jun 19 08:04:44 2007

Method C:\MSDCHEM\1\METHODS\123-TCP061807.M renamed as C:\MSDCHEM\1\METHODS\123-TCP070307.M
Tue Jul 03 16:25:47 2007

Method C:\MSDCHEM\1\METHODS\123-TCP070307.M renamed as C:\MSDCHEM\1\METHODS\123-TCP071107.M
Thu Jul 12 08:13:38 2007

IQG1460 / CQG0634
LEVEL IV DATA PACKAGE

SRL 524M-123 TCP
SAMPLE RAW DATA

Injection Log

Directory: C:\DATA\07JUL18

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	1	G18001.d	1.	Equil Rinse	25mL	18 Jul 2007 10:28
2	2	G18002.d	1.	Equil Rinse	25mL	18 Jul 2007 11:00
3	3	G18003.d	1.	Equil Rinse	25mL	18 Jul 2007 11:33
4	4	G18004.d	1.	CCV	25mL w/ 50ppt #7060083	18 Jul 2007 12:05
5	5	G18005.d	1.	C7G1807-BS1	25mL w/ 5ppt #7060083	18 Jul 2007 12:37
6	6	G18006.d	1.	C7G1807-BLK1	25mL w/ #7060081	18 Jul 2007 13:10
7	7	G18007.d	1.	~~CQG0524-04~~ CQG0524-04	25mL	18 Jul 2007 14:12
8	8	G18008.d	1.	~~CQG0466-01RE1~~ CQG0466-01RE1	25mL	18 Jul 2007 14:45
9	9	G18009.d	1.	C7G1807-MS1	25mL w/ #7060083; 466-01	18 Jul 2007 15:17
10	10	G18010.d	1.	C7G1807-MSD1	25mL w/ #7060083; 466-01	18 Jul 2007 15:50
11	11	G18011.d	1.	CQG0524-05	25mL	18 Jul 2007 16:22
12	12	G18012.d	1.	CQG0577-01	25mL	18 Jul 2007 16:55
13	13	G18013.d	1.	CQG0577-02	25mL	18 Jul 2007 17:28
14	14	G18014.d	1.	CQG0577-03	25mL	18 Jul 2007 18:01
15	15	G18015.d	1.	CQG0634-01	25mL	18 Jul 2007 18:33
16	16	G18016.d	1.	CQG0634-02	25mL	18 Jul 2007 19:06
17	17	G18017.d	1.	CQG0634-03	25mL	18 Jul 2007 19:38
18	18	G18018.d	1.	CQG0634-04	25mL	18 Jul 2007 20:11
19	19	G18019.d	1.	CCV	25mL w/ 50ppt #7060083	18 Jul 2007 20:43

PREPARATION BENCH SHEET

C7G1807

TestAmerica - Ontario, CA

Printed: 7/19/2007 2:43:03PM

Matrix: Water **Prepared using: GCMS-Volatiles - EPA 524.2** **Surrogate used: 7060081**

Lab Number	Analysis	Prepared	Initial (ml)	Final (ml)	Source ID	Spike 1	ul Spike	Spike 2	ul Spike	ul Surr	Initials	Extraction Comments
C7G1807-BLK1	QC	07/18/07 12:05	25	25			0		0	5		
C7G1807-BS1	QC	07/18/07 12:05	25	25		7060083	0.5		100	5		
C7G1807-MS1	QC	07/18/07 12:05	25	25	CQG0466-01RE1	7060083	5		100	5		
C7G1807-MSD1	QC	07/18/07 12:05	25	25	CQG0466-01RE1	7060083	5		100	5		
CQG0466-01RE	524.2 CA 1,2,3-TCP (SIM)	07/18/07 12:05	25	25						5		From C7G1605 by PM on 07/18/07
CQG0524-04	524.2 CA 1,2,3-TCP (SIM)	07/18/07 12:05	25	25						5		
CQG0524-05	524.2 CA 1,2,3-TCP (SIM)	07/18/07 12:05	25	25						5		
CQG0577-01	524.2 CA 1,2,3-TCP (SIM)	07/18/07 12:05	25	25						5		
CQG0577-02	524.2 CA 1,2,3-TCP (SIM)	07/18/07 12:05	25	25						5		
CQG0577-03	524.2 CA 1,2,3-TCP (SIM)	07/18/07 12:05	25	25						5		
CQG0634-01	524.2 CA 1,2,3-TCP (SIM)	07/18/07 12:05	25	25						5		
CQG0634-02	524.2 CA 1,2,3-TCP (SIM)	07/18/07 12:05	25	25						5		
CQG0634-03	524.2 CA 1,2,3-TCP (SIM)	07/18/07 12:05	25	25						5		
CQG0634-04	524.2 CA 1,2,3-TCP (SIM)	07/18/07 12:05	25	25						5		

Reagents used in Batch

Reagent	Description	Solvent

GCMS #39

Posted
PM 7/19/07

7-20-07

Spiking Witnessed By Date

Preparation Reviewed By Date

Extracts Received By Date

Mint Miner 2.02 (70108) Directory Scan: x:\07JUL18

20 Jul 2007 07:38

Level	Status	Code	Operator	Instrument	Sample ID
Scan File Path: x:\07JUL18\G18001.D					
Original Path: x:\07JUL18\G18001.D					
0	No Audit				
Scan File Path: x:\07JUL18\G18002.D					
Original Path: x:\07JUL18\G18002.D					
0	No Audit				
Scan File Path: x:\07JUL18\G18003.D					
Original Path: x:\07JUL18\G18003.D					
0	No Audit				
Scan File Path: x:\07JUL18\G18004.D					
Original Path: C:\DATA\07JUL18\G18004.D					
5	Scanned	QD(1)	PM	GCMS39	CCV (25mL w/ 50ppt #7060083)
Scan File Path: x:\07JUL18\G18005.D					
Original Path: C:\DATA\07JUL18\G18005.D					
5	Scanned	QD(1)	PM	GCMS39	C7G1807-BS1 (25mL w/ 5ppt #7060083)
Scan File Path: x:\07JUL18\G18006.D					
Original Path: C:\DATA\07JUL18\G18006.D					
5	Scanned	QD(1)	PM	GCMS39	C7G1807-BLK1 (25mL w/ #7060081)
Scan File Path: x:\07JUL18\G18007.D					
Original Path: C:\DATA\07JUL18\G18007.D					
5	Scanned	QD(1)	PM	GCMS39	CQG524-04 (25mL)
Scan File Path: x:\07JUL18\G18008.D					
Original Path: C:\DATA\07JUL18\G18008.D					
5	Scanned	QD(1)	PM	GCMS39	CQG466-01RE1 (25mL)
Scan File Path: x:\07JUL18\G18009.D					
Original Path: C:\DATA\07JUL18\G18009.D					
5	Scanned	QD(1)	PM	GCMS39	C7G1807-MS1 (25mL w/ #7060083; 466-01)
Scan File Path: x:\07JUL18\G18010.D					
Original Path: C:\DATA\07JUL18\G18010.D					
5	Scanned	QD(1)	PM	GCMS39	C7G1807-MSD1 (25mL w/ #7060083; 466-01)
Scan File Path: x:\07JUL18\G18011.D					
Original Path: C:\DATA\07JUL18\G18011.D					
5	Scanned	QD(1)	PM	GCMS39	CQG0524-05 (25mL)

Level	Status	Code	Operator	Instrument	Sample ID
Scan File Path: x:\07JUL18\G18012.D					
Original Path: C:\DATA\07JUL18\G18012.D					
5	Scanned	QD(1)	PM	GCMS39	CQG0577-01 (25mL)
Scan File Path: x:\07JUL18\G18013.D					
Original Path: C:\DATA\07JUL18\G18013.D					
5	Scanned	QD(1)	PM	GCMS39	CQG0577-02 (25mL)
Scan File Path: x:\07JUL18\G18014.D					
Original Path: C:\DATA\07JUL18\G18014.D					
5	Scanned	QD(1)	PM	GCMS39	CQG0577-03 (25mL)
Scan File Path: x:\07JUL18\G18015.D					
Original Path: C:\DATA\07JUL18\G18015.D					
5	Scanned	QD(1)	PM	GCMS39	CQG0634-01 (25mL)
Scan File Path: x:\07JUL18\G18016.D					
Original Path: C:\DATA\07JUL18\G18016.D					
5	Scanned	QD(1)	PM	GCMS39	CQG0634-02 (25mL)
Scan File Path: x:\07JUL18\G18017.D					
Original Path: C:\DATA\07JUL18\G18017.D					
5	Scanned	QD(1)	PM	GCMS39	CQG0634-03 (25mL)
Scan File Path: x:\07JUL18\G18018.D					
Original Path: C:\DATA\07JUL18\G18018.D					
5	Scanned	QD(1)	PM	GCMS39	CQG0634-04 (25mL)
Scan File Path: x:\07JUL18\G18019.D					
Original Path: C:\DATA\07JUL18\G18019.D					
5	Scanned	QD(1)	PM	GCMS39	CCV (25mL w/ 50ppt #7060083)

No time travel
~~Compat~~ software
error DW 20
7-19-07

QD = Method Last Update date after Quantitation date

ScanSummary.rpt

Total Files Scanned	Beginning Analyzed Date
Methods	Ending Analyzed Date
Samples	Analyzed Range
Tunes	Greatest Time Between Tunes
CCCs	Greatest Time Between CCCs

Distinct Method Last Updated count

Operators Intruments

GC/MS QA-QC Check Report

Tune File : C:\DATA\07JUL18\G18004.D
Tune Time : 18 Jul 2007 12:05 pm

Daily Calibration File : C:\DATA\07JUL11\G11005.D

File	Sample	Internal Std Responses 20175
G18004.D	CCV	18349
G18005.D	C7G1807-BS1	18192
G18006.D	C7G1807-BLK1	18679
G18007.D	~~CQG524-04~~ CQG0524-04	17616
G18008.D	~~CQG466-01RB1~~ CQG0466-01RE1	18522
G18009.D	C7G1807-MS1	21245
G18010.D	C7G1807-MSD1	16778
G18011.D	CQG0524-05	21291
G18012.D	CQG0577-01	22304
G18013.D	CQG0577-02	19995
G18014.D	CQG0577-03	21376
G18015.D	CQG0634-01	19554
G18016.D	CQG0634-02	20743
G18017.D	CQG0634-03	21933
G18018.D	CQG0634-04	20680
G18019.D	CCV	20897

- fails 12hr time check * - fails criteria

Created: Thu Jul 19 09:38:23 2007 GCMS39

GC/MS # 39 page 1 of 1

Date: 7/18/07

Analyst: JM

Port #	Sample	Amount	Dil.	Ph	Res. Cl2	Comments
1	Equil. Rinse	25mL	1	N/A		
2		25mL	1			
3		25mL	1			
4	CCV	25mL	1			50ppt #7060083
5	C7G1807-BS1	25mL	1			5ppt #7060083
6	-BLK1	25mL	1			#7060081
7	CQG0524-04	25mL	1			
8	CQG0466-01RE1	25mL	1			
9	C7G1807-MS1	25mL	1			#7060083; 466-01
10	-MSD1	25mL	1			
11	CQG0524-05	25mL	1			
12	CQG0577-01	25mL	1			
13	-02	25mL	1			
14	-03	25mL	1			
15	CQG0634-01	25mL	1			
16	-02	25mL	1			
17	-03	25mL	1			
18	-04	25mL	1			
19	CCV	25mL	1			50ppt #7060083

1,2,3-Trichloropropane by GC/MS Calibration Verification Check

7/19/07

File:	G18004.D	**Instrument:**	GCMS39
Operator:	PM		
Date:	18 Jul 2007 12:05 pm	**QC BATCH # :**	CCV

	Source	Response	% Recovery	Control Limits
2) 1,2,3-Trichloropropane	50	48.09	96.2	80-120

* Denotes values out of expected range

Evaluate Continuing Calibration Report

Data File : C:\DATA\07JUL18\G18004.D
Acq On : 18 Jul 2007 12:05 pm
Sample : CCV
Misc : 25mL w/ 50ppt #7060083
MS Integration Params: RTEINT.P

Vial: 4
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Multiple Level Calibration

Min. RRF : 0.000 Min. Rel. Area : 80% Max. R.T. Dev 0.50min
Max. RRF Dev : 20% Max. Rel. Area : 200%

		Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1	I	1,2,3-TCP-d5 (IS)	1.000	1.000	0.0	91	0.00
2	CPM	1,2,3-Trichloropropane	0.906	0.871	3.9	88	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 0

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18004.D
Acq On : 18 Jul 2007 12:05 pm
Sample : CCV
Misc : 25mL w/ 50ppt #7060083
MS Integration Params: RTEINT.P
Quant Time: Jul 19 09:36:49 2007

Vial: 4
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	18349	50.00 ng/L	0.00
Target Compounds					Qvalue
2) 1,2,3-Trichloropropane	17.41	75	15980	48.09 ng/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18004.D
Acq On : 18 Jul 2007 12:05 pm
Sample : CCV
Misc : 25mL w/ 50ppt #7060083
MS Integration Params: RTEINT.P
Quant Time: Jul 19 9:36 2007

Vial: 4
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration

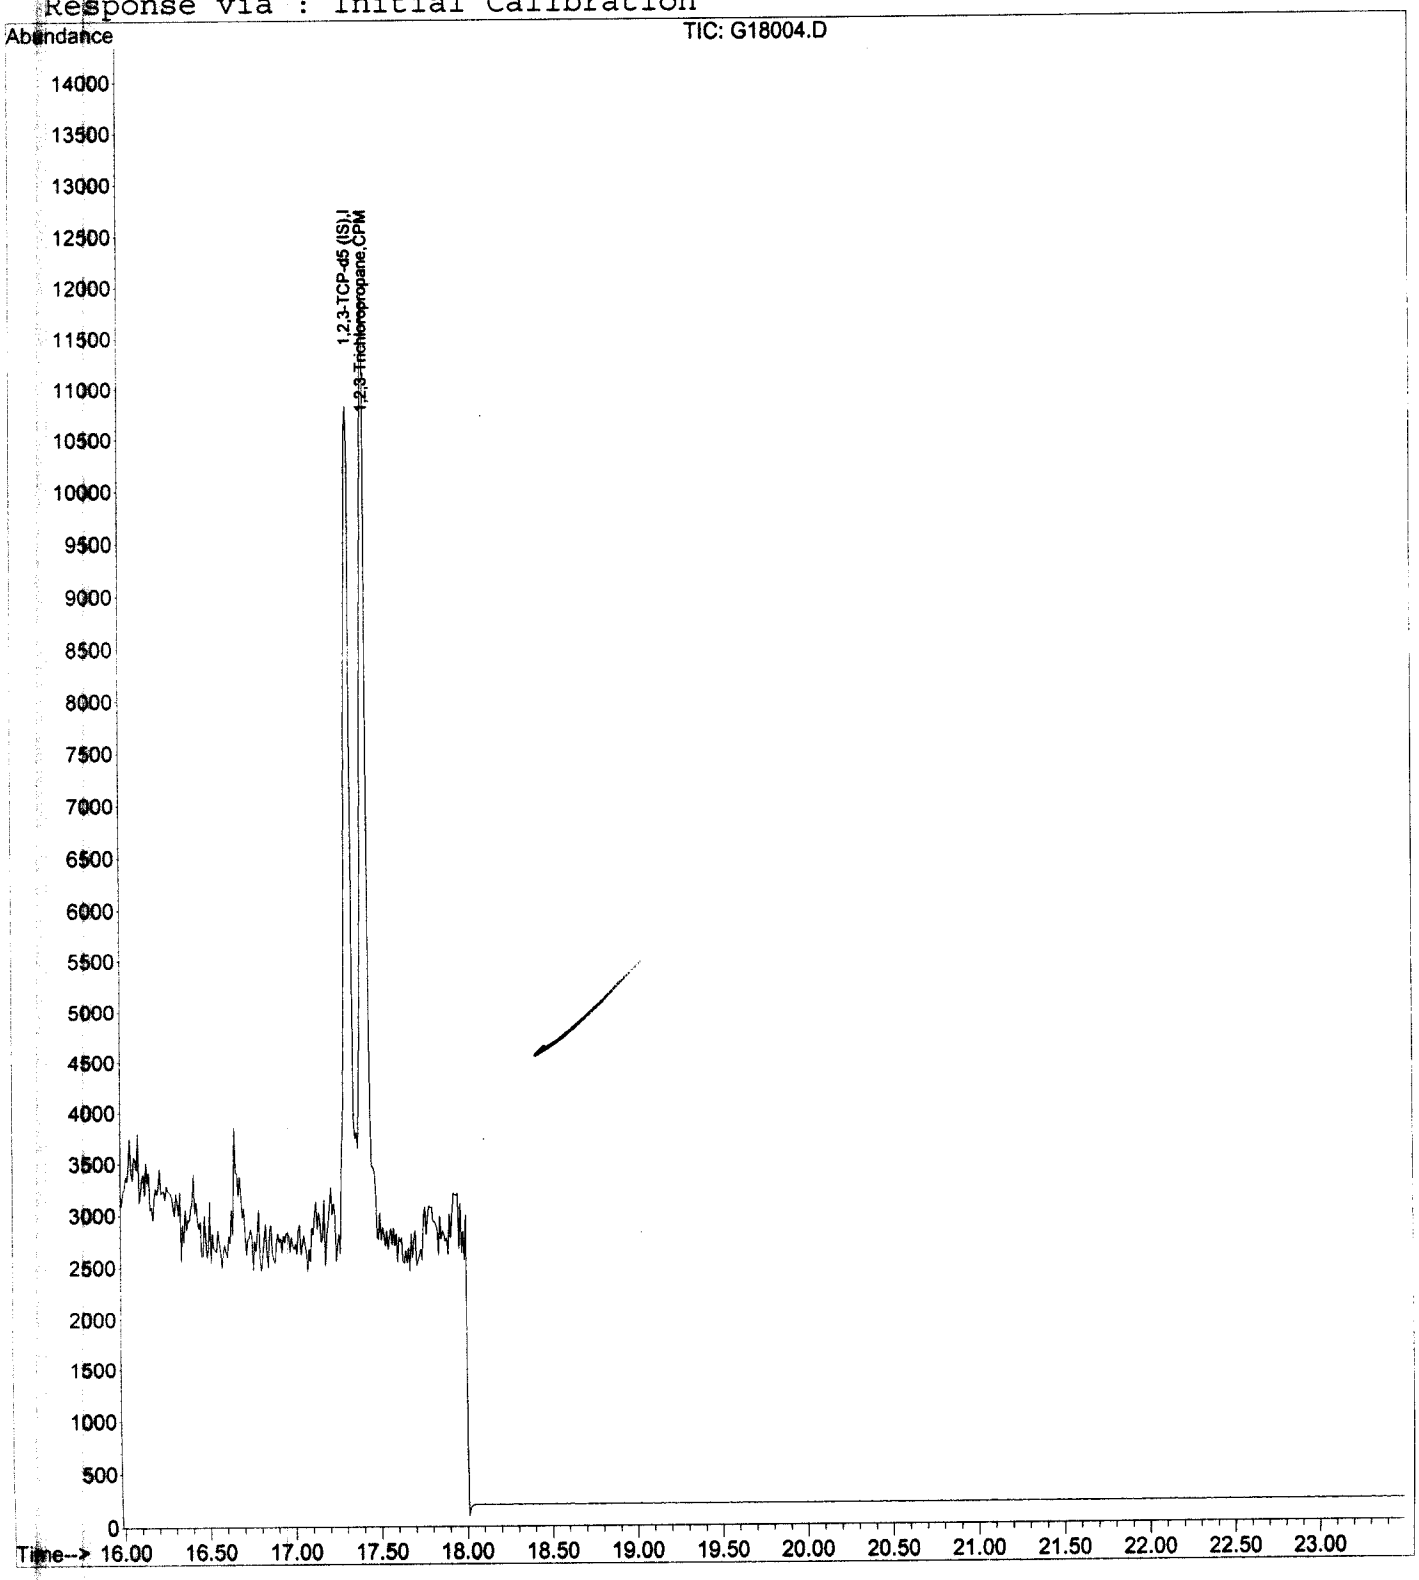

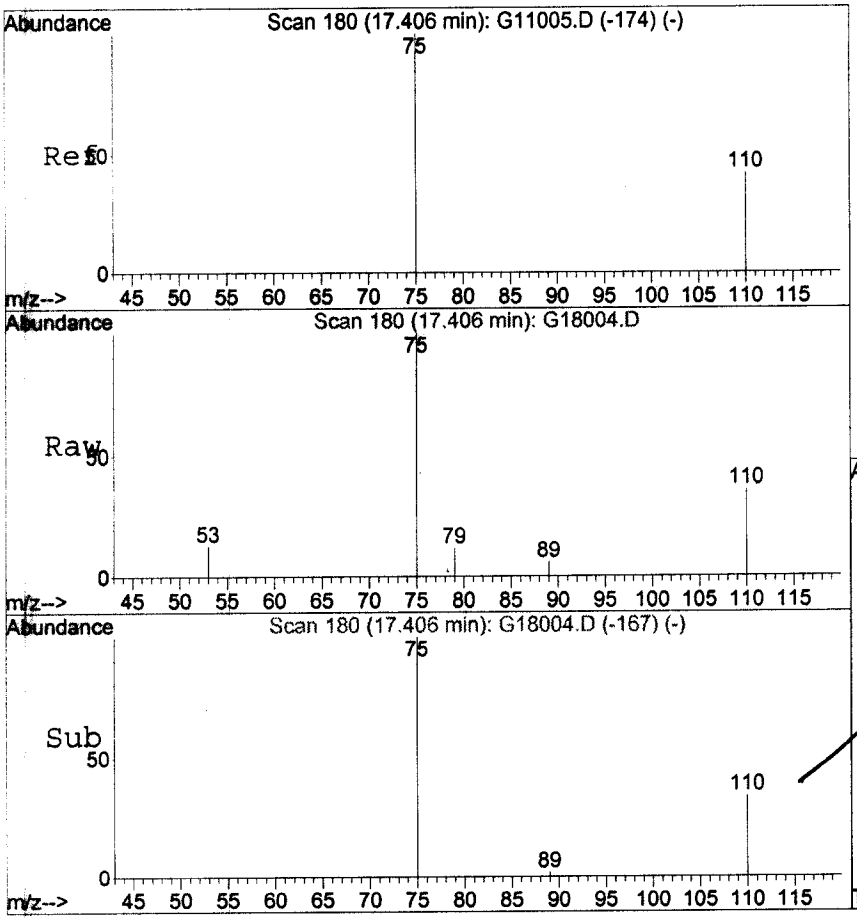

#2
1,2,3-Trichloropropane
Concen: 48.09 ng/L
RT: 17.41 min Scan# 180
Delta R.T. 0.00 min
Lab File: G18004.D
Acq: 18 Jul 2007 12:05 pm

Tgt Ion: 75 Resp: 15980

Ion	Ratio	Lower	Upper
75	100		
110	41.2	11.2	71.2
53	2.7	0.0	30.0
89	0.8	0.0	30.8

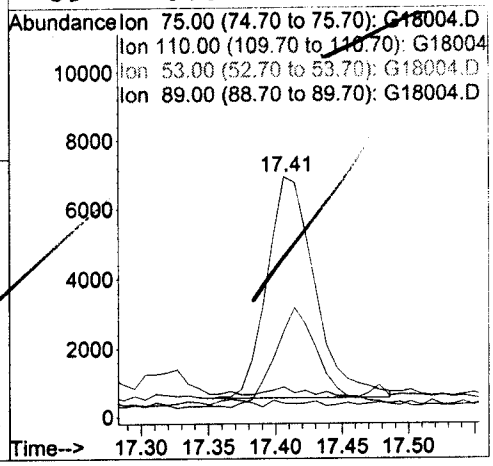

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18005.D
Acq On : 18 Jul 2007 12:37 pm
Sample : C7G1807-BS1
Misc : 25mL w/ 5ppt #7060083
MS Integration Params: RTEINT.P
Quant Time: Jul 19 09:37:18 2007

Vial: 5
Operator: PM
Inst : GCMS39
Multiplr: 1.00

7/19/07

Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	18192	50.00 ng/L	0.00
Target Compounds					Qvalue
2) 1,2,3-Trichloropropane	17.41	75	1654	5.02 ng/L	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18005.D
Acq On : 18 Jul 2007 12:37 pm
Sample : C7G1807-BS1
Misc : 25mL w/ 5ppt #7060083
MS Integration Params: RTEINT.P
Quant Time: Jul 19 9:37 2007

Vial: 5
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration

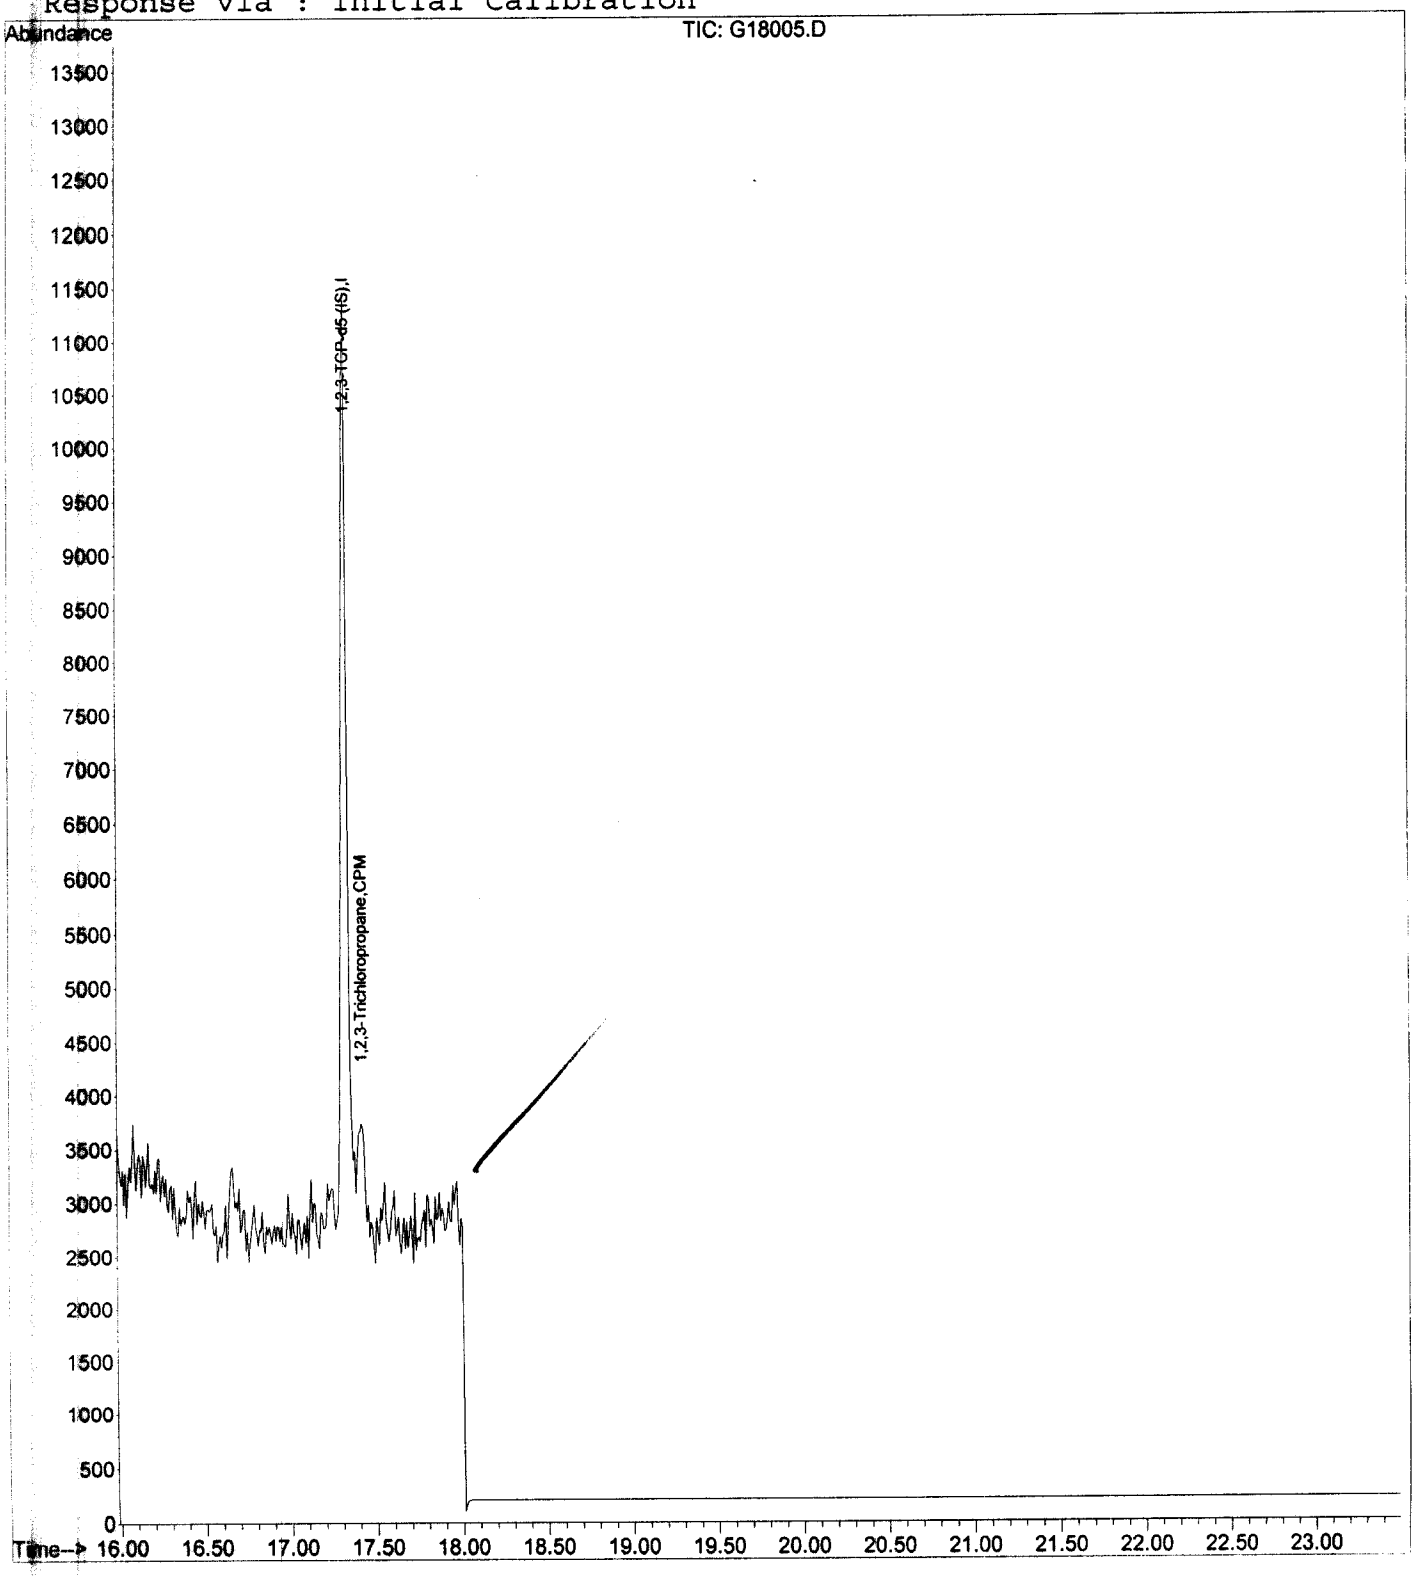

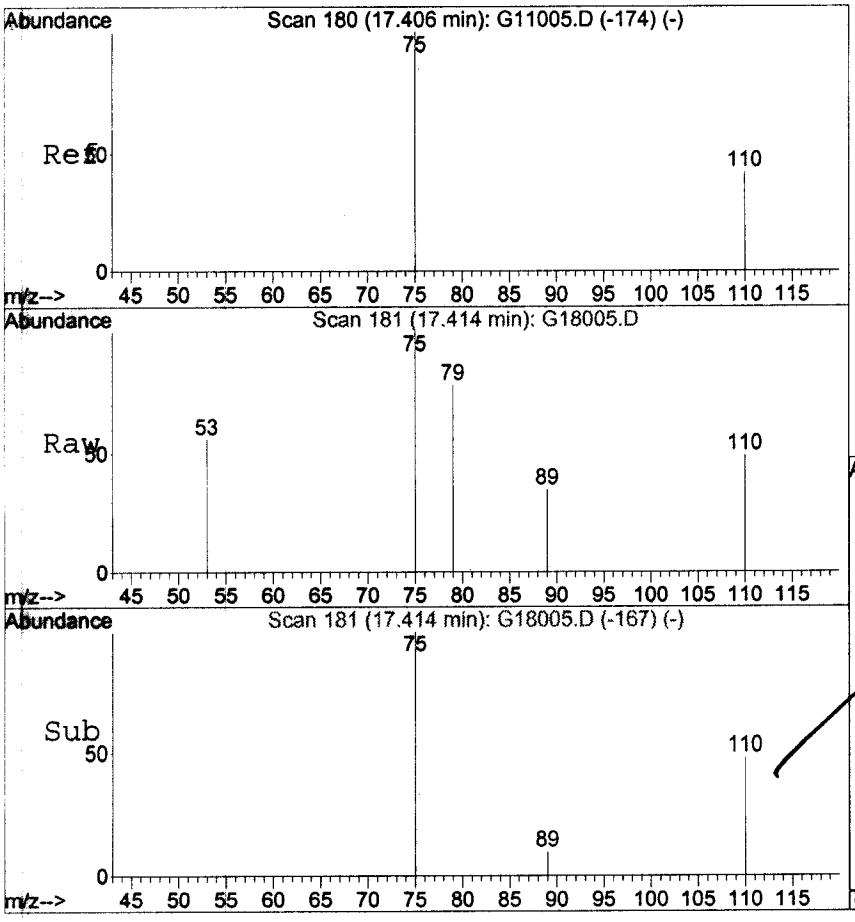

#2
1,2,3-Trichloropropane
Concen: 5.02 ng/L
RT: 17.41 min Scan# 181
Delta R.T. 0.01 min
Lab File: G18005.D
Acq: 18 Jul 2007 12:37 pm

Tgt Ion: 75 Resp: 1654

Ion	Ratio	Lower	Upper
75	100		
110	56.5	11.2	71.2
53	28.7	0.0	30.0
89	7.4	0.0	30.8

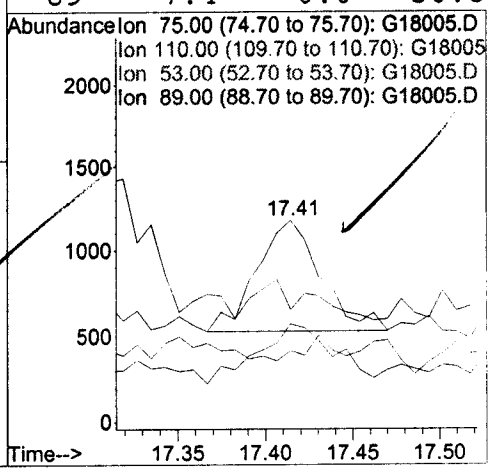

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18006.D
Acq On : 18 Jul 2007 1:10 pm
Sample : C7G1807-BLK1
Misc : 25mL w/ #7060081
MS Integration Params: RTEINT.P
Quant Time: Jul 19 09:37:19 2007

Vial: 6
Operator: PM
Inst : GCMS39
Multiplr: 1.00

7/19/07

Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	18679	50.00 ng/L	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18006.D
Acq On : 18 Jul 2007 1:10 pm
Sample : C7G1807-BLK1
Misc : 25mL w/ #7060081
MS Integration Params: RTEINT.P
Quant Time: Jul 19 9:37 2007

Vial: 6
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration

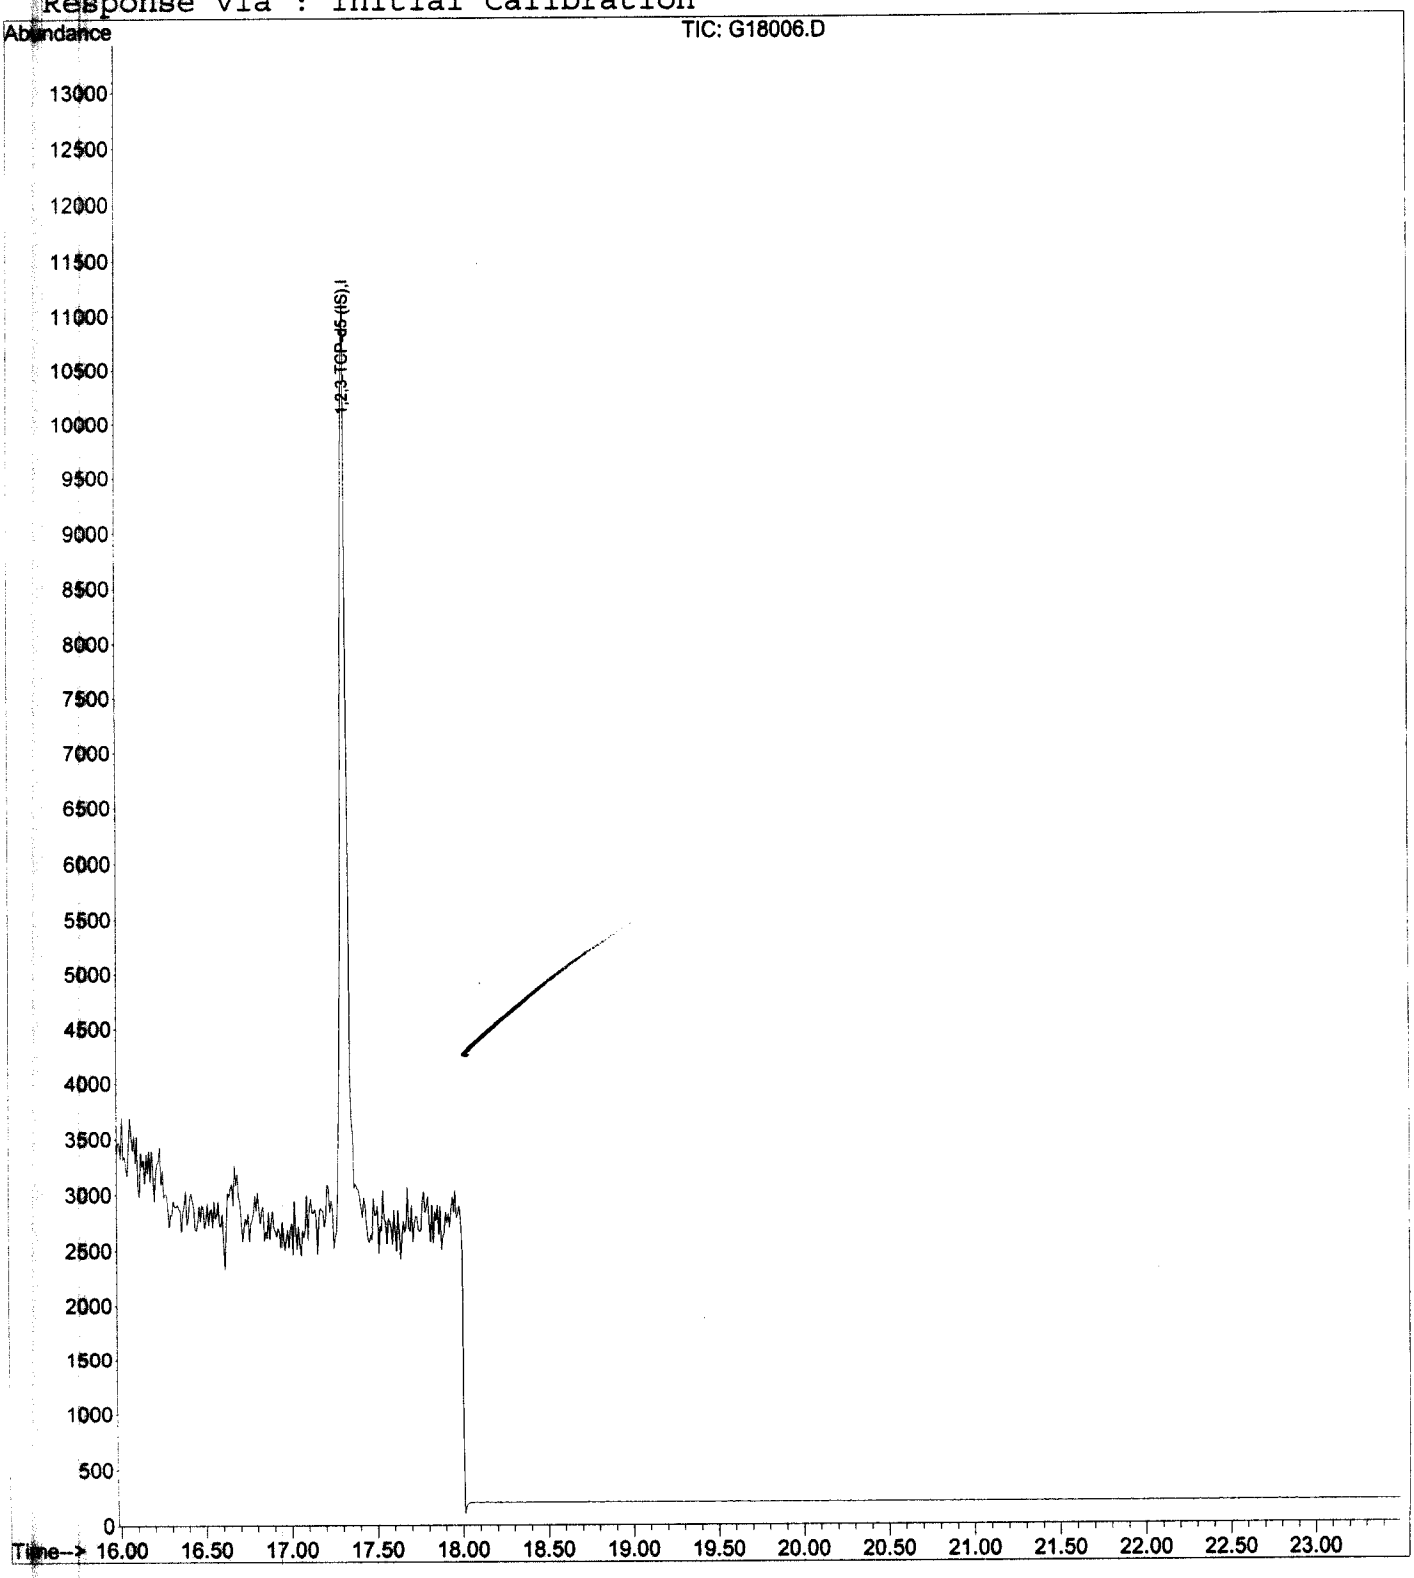

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18008.D
Acq On : 18 Jul 2007 2:45 pm
Sample : ~~CQG466-01RE1~~ CQG0466-01RE1
Misc : 25mL
MS Integration Params: RTEINT.P
Quant Time: Jul 19 09:37:22 2007

Vial: 8
Operator: PM
Inst : GCMS09
Multiplr: 1.00

7/19/07

7/19/07

Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Client requests sample for MS/MSD

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	18522	50.00	ng/L	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18008.D
Acq On : 18 Jul 2007 2:45 pm
Sample : CQG466-01RE1
Misc : 25mL
MS Integration Params: RTEINT.P
Quant Time: Jul 19 9:37 2007

Vial: 8
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration

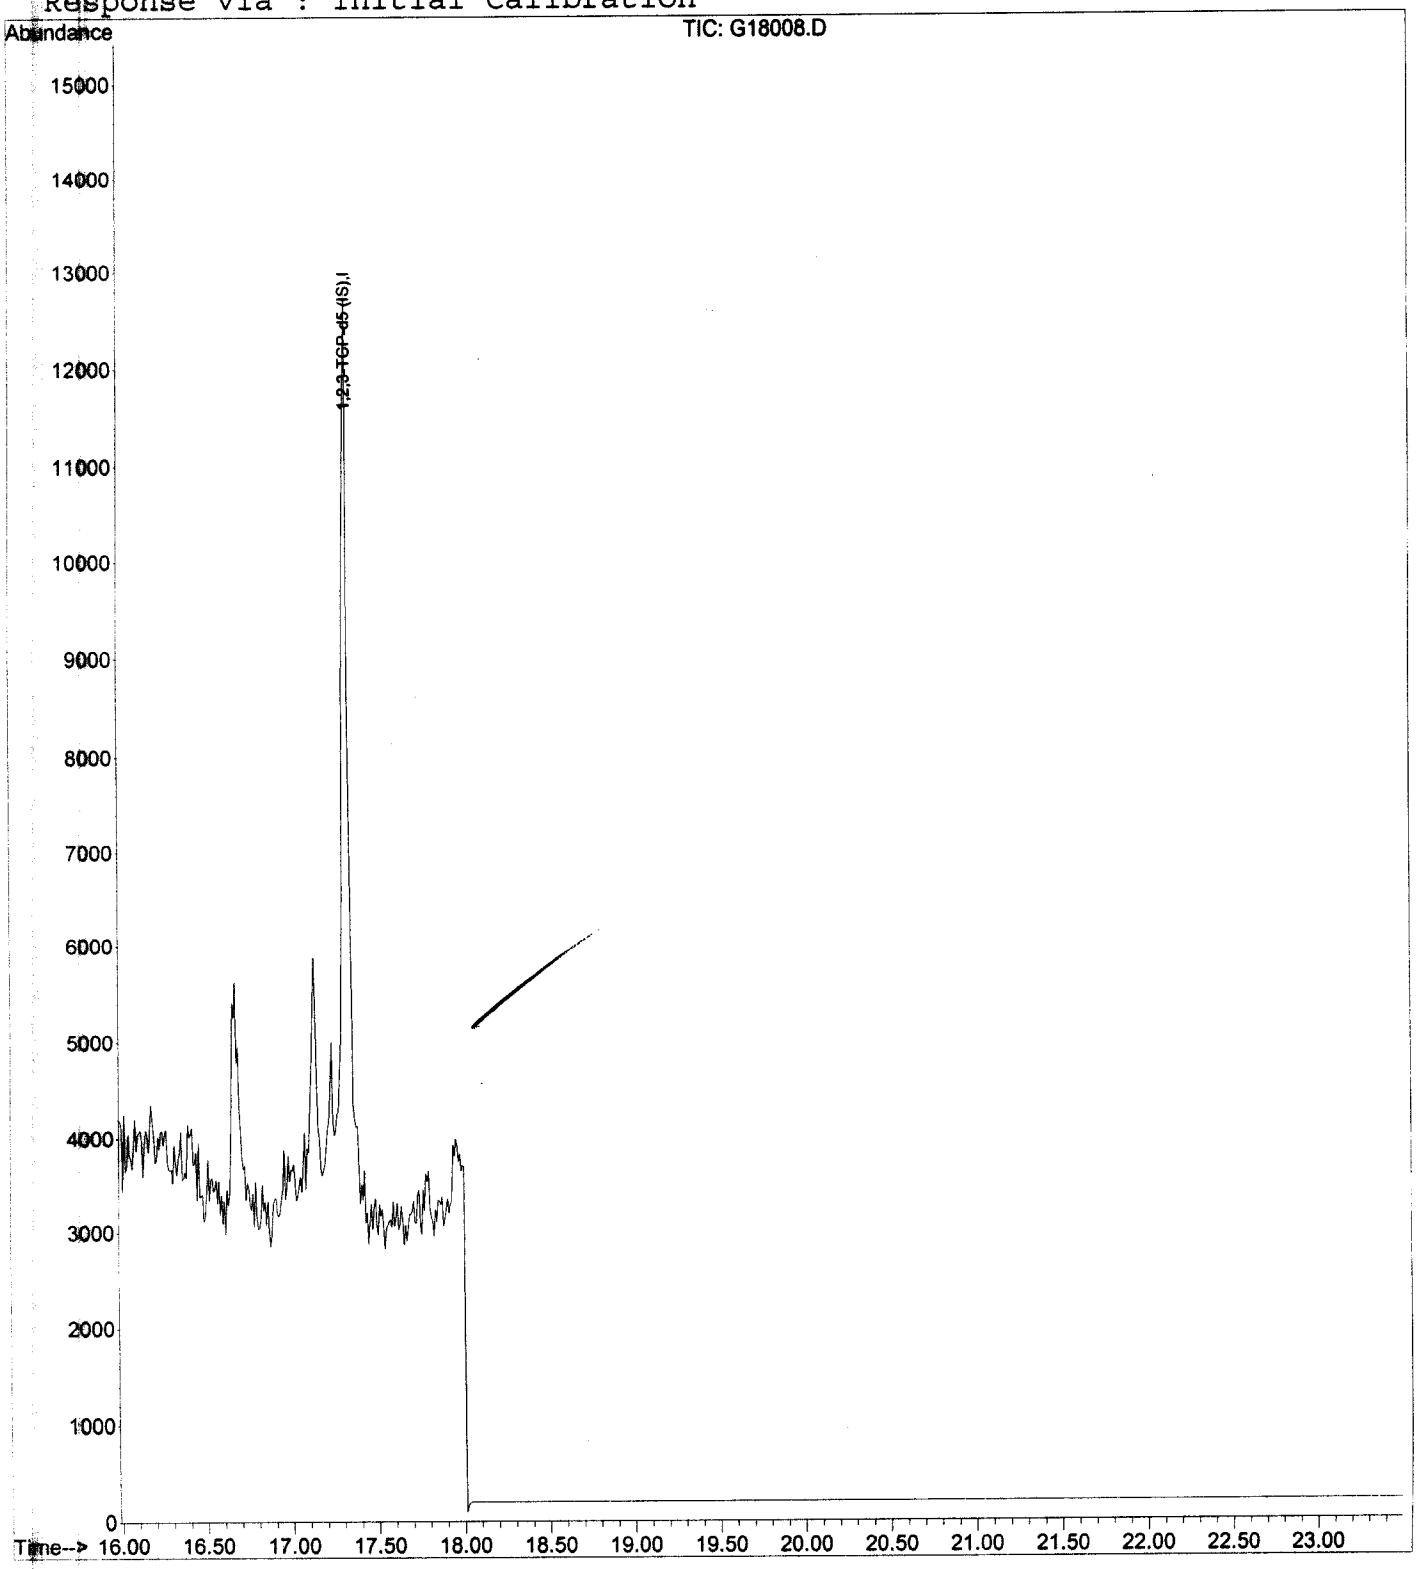

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18009.D
Acq On : 18 Jul 2007 3:17 pm
Sample : C7G1807-MS1
Misc : 25mL w/ #7060083; 466-01
MS Integration Params: RTEINT.P
Quant Time: Jul 19 09:37:24 2007

Vial: 9
Operator: PM
Inst : GCMS3
Multiplr: 1.00

7/19/07

Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.31	79	21245	50.00 ng/L	0.00
Target Compounds					Qvalue
2) 1,2,3-Trichloropropane	17.41	75	16510	42.91 ng/L #	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18009.D
Acq On : 18 Jul 2007 3:17 pm
Sample : C7G1807-MS1
Misc : 25mL w/ #7060083; 466-01
MS Integration Params: RTEINT.P
Quant Time: Jul 19 9:37 2007

Vial: 9
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration

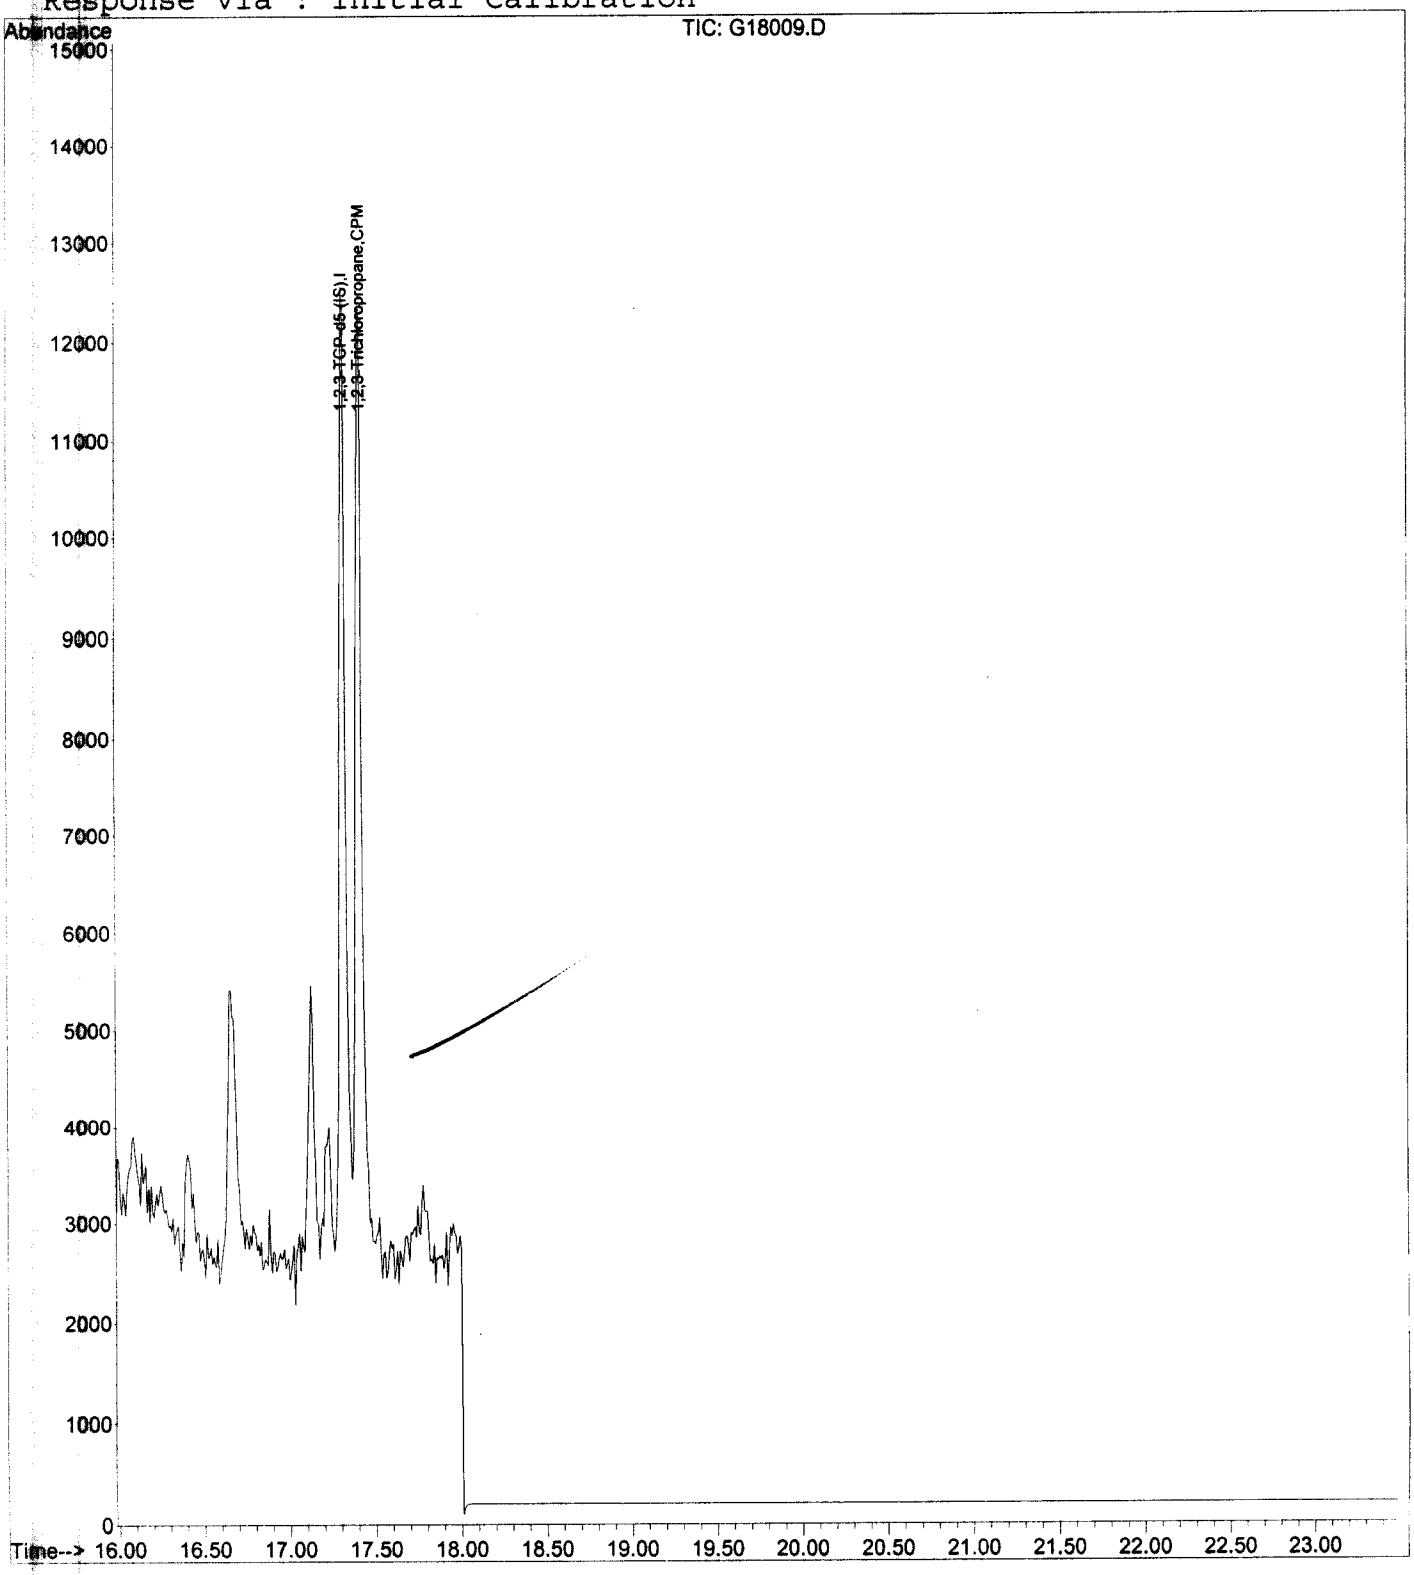

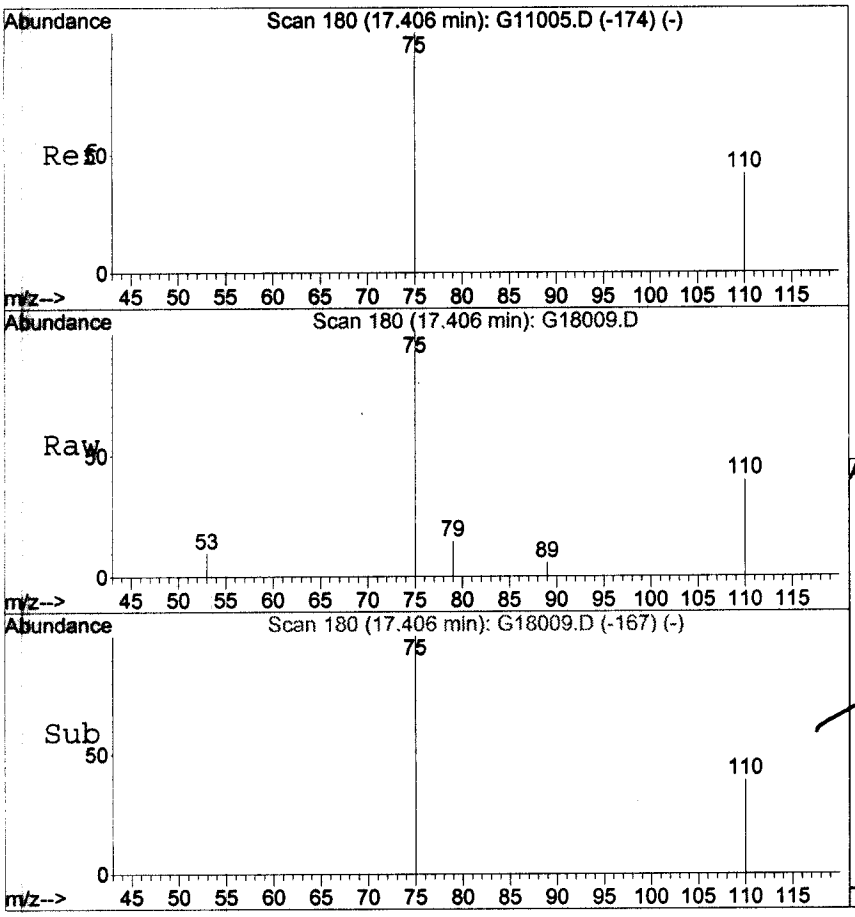

#2
1,2,3-Trichloropropane
Concen: 42.91 ng/L
RT: 17.41 min Scan# 180
Delta R.T. 0.00 min
Lab File: G18009.D
Acq: 18 Jul 2007 3:17 pm

Tgt Ion: 75 Resp: 16510

Ion	Ratio	Lower	Upper
75	100		
110	43.5	11.2	71.2
53	0.0	0.0	30.0
89	1.3	0.0	30.8

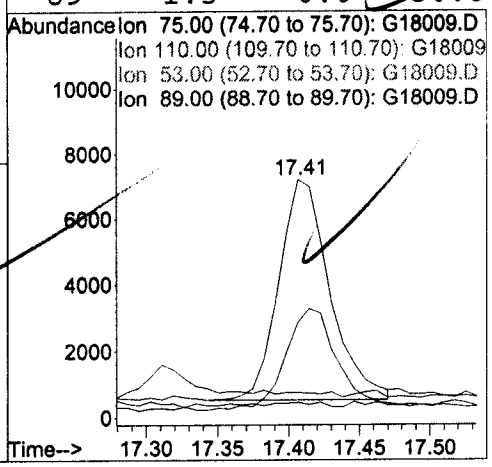

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18010.D
Acq On : 18 Jul 2007 3:50 pm
Sample : C7G1807-MSD1
Misc : 25mL w/ #7060083; 466-01
MS Integration Params: RTEINT.P
Quant Time: Jul 19 09:37:26 2007

Vial: 10
Operator: PM
Inst : GCMS39
Multiplr: 1.00

7/19/07

Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	16778	50.00 ng/L	0.00
Target Compounds					Qvalue
2) 1,2,3-Trichloropropane	17.41	75	16108	53.01 ng/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18010.D
Acq On : 18 Jul 2007 3:50 pm
Sample : C7G1807-MSD1
Misc : 25mL w/ #7060083; 466-01
MS Integration Params: RTEINT.P
Quant Time: Jul 19 9:37 2007

Vial: 10
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration

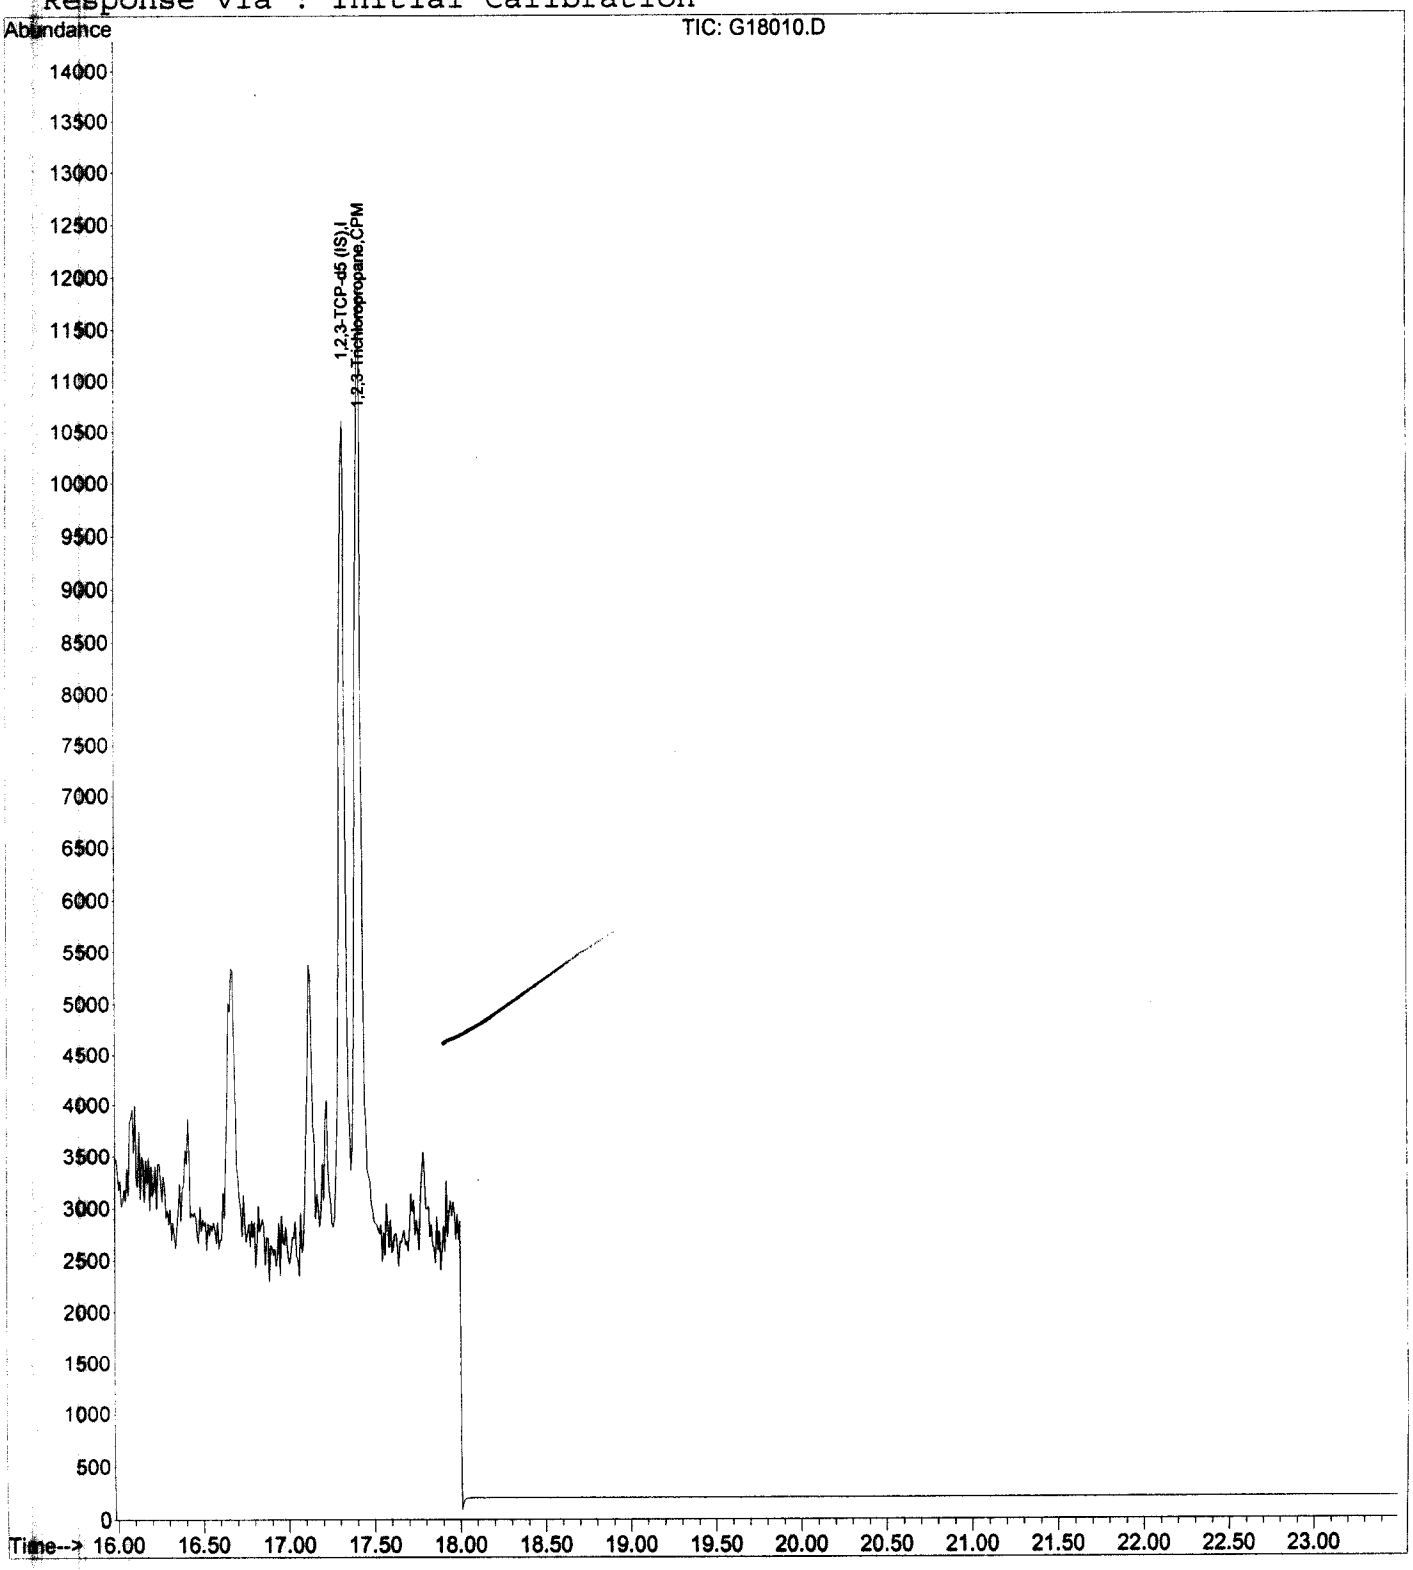

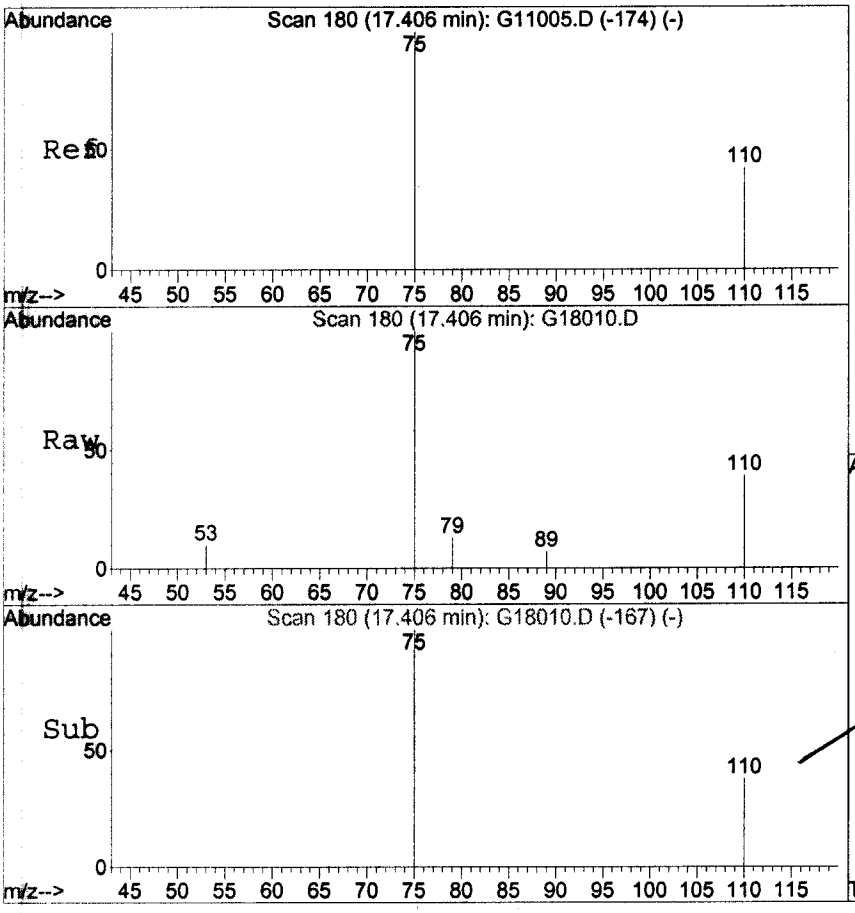

#2
1,2,3-Trichloropropane
Concen: 53.01 ng/L
RT: 17.41 min Scan# 180
Delta R.T. -0.00 min
Lab File: G18010.D
Acq: 18 Jul 2007 3:50 pm

Tgt Ion: 75 Resp: 16108

Ion	Ratio	Lower	Upper
75	100		
110	39.3	11.2	71.2
53	3.4	0.0	30.0
89	1.9	0.0	30.8

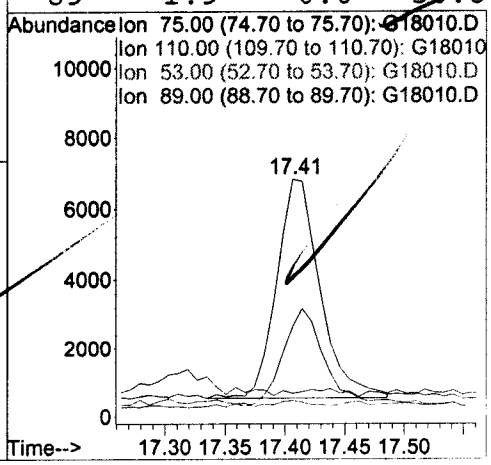

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18015.D
Acq On : 18 Jul 2007 6:33 pm
Sample : CQG0634-01
Misc : 25mL
MS Integration Params: RTEINT.P
Quant Time: Jul 19 09:37:32 2007

Vial: 15
Operator: PM
Inst : GCMS39
Multiplr: 1.00

7/19/07

Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	19554	50.00 ng/L	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18015.D
Acq On : 18 Jul 2007 6:33 pm
Sample : CQG0634-01
Misc : 25mL
MS Integration Params: RTEINT.P
Quant Time: Jul 19 9:37 2007

Vial: 15
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration

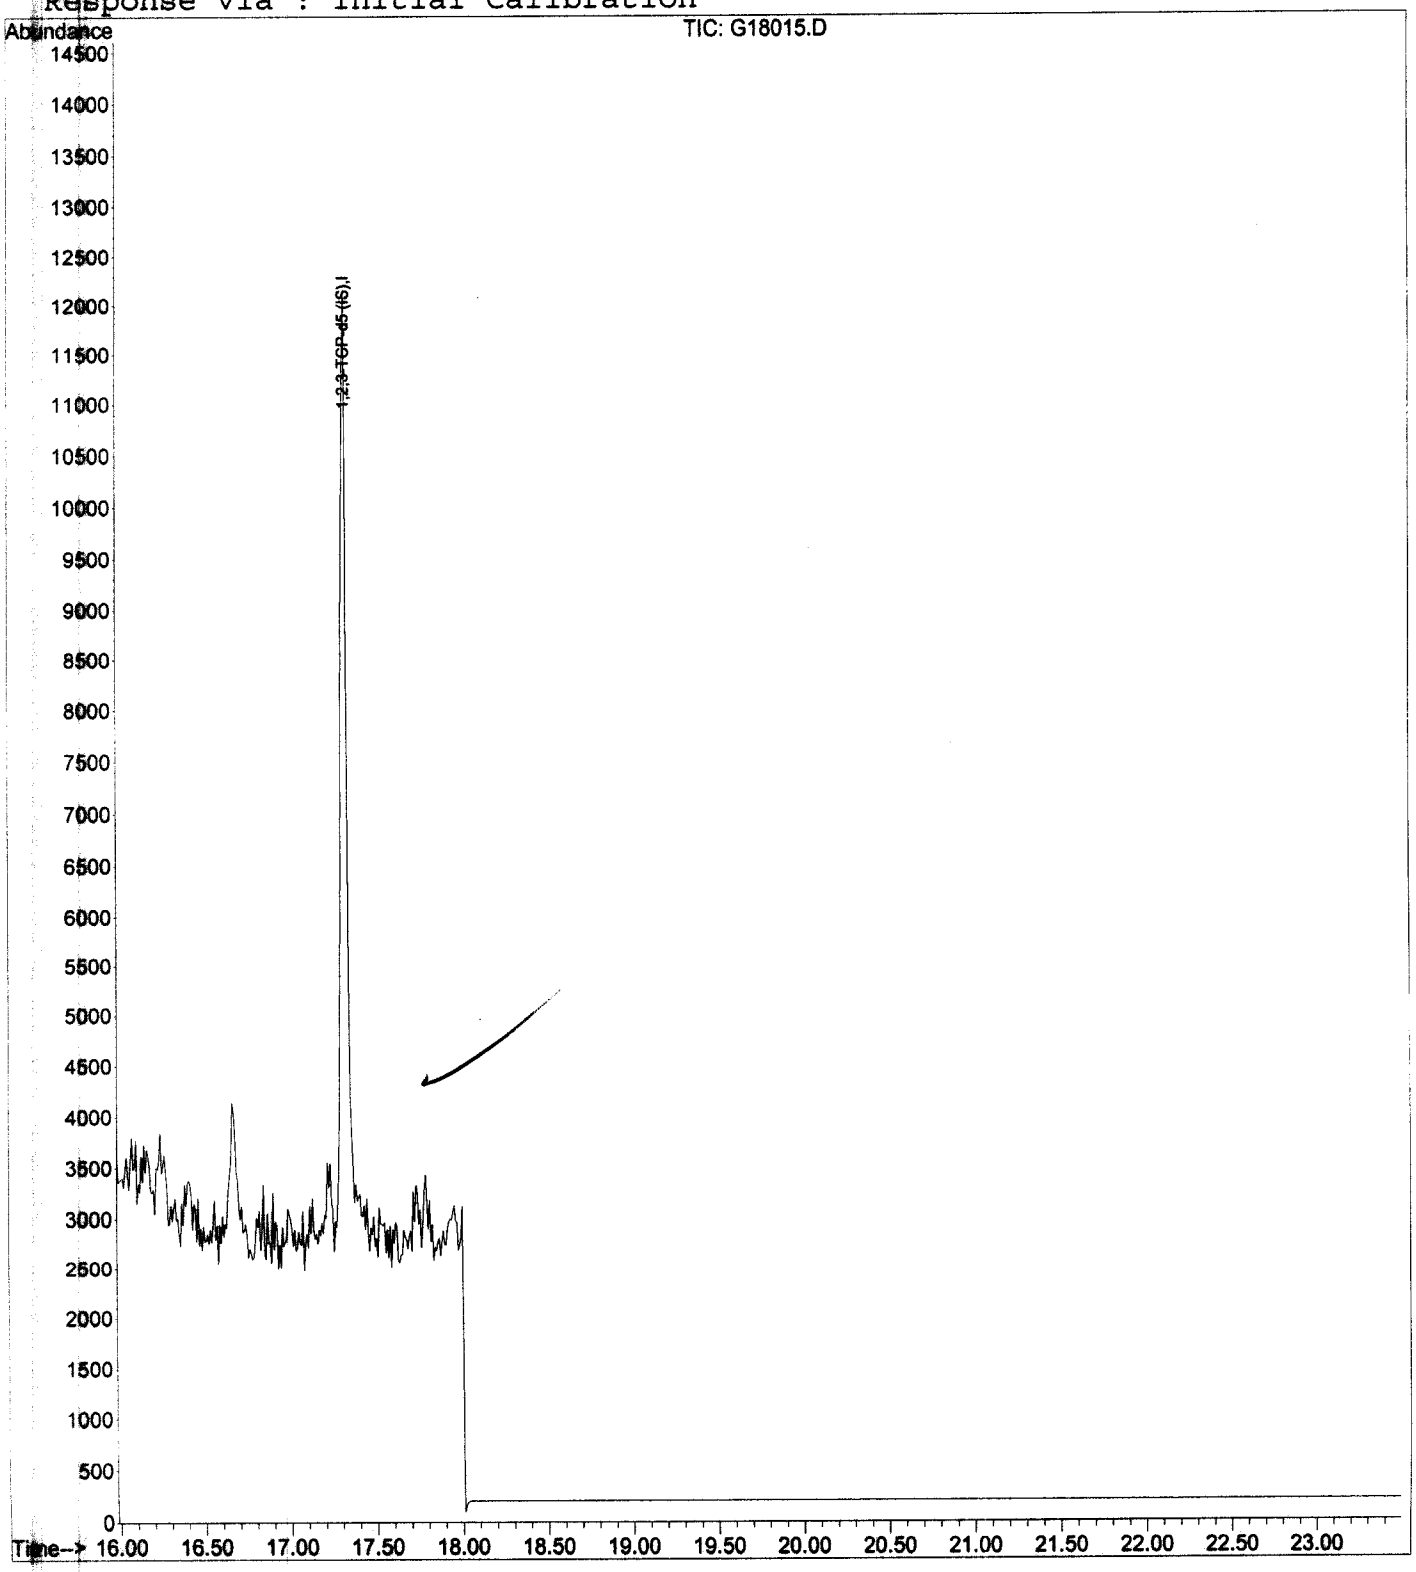

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18016.D
Acq On : 18 Jul 2007 7:06 pm
Sample : CQG0634-02
Misc : 25mL
MS Integration Params: RTEINT.P
Quant Time: Jul 19 09:37:32 2007

Vial: 16
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	20743	50.00	ng/L	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18016.D
Acq On : 18 Jul 2007 7:06 pm
Sample : CQG0634-02
Misc : 25mL
MS Integration Params: RTEINT.P
Quant Time: Jul 19 9:37 2007

Vial: 16
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration

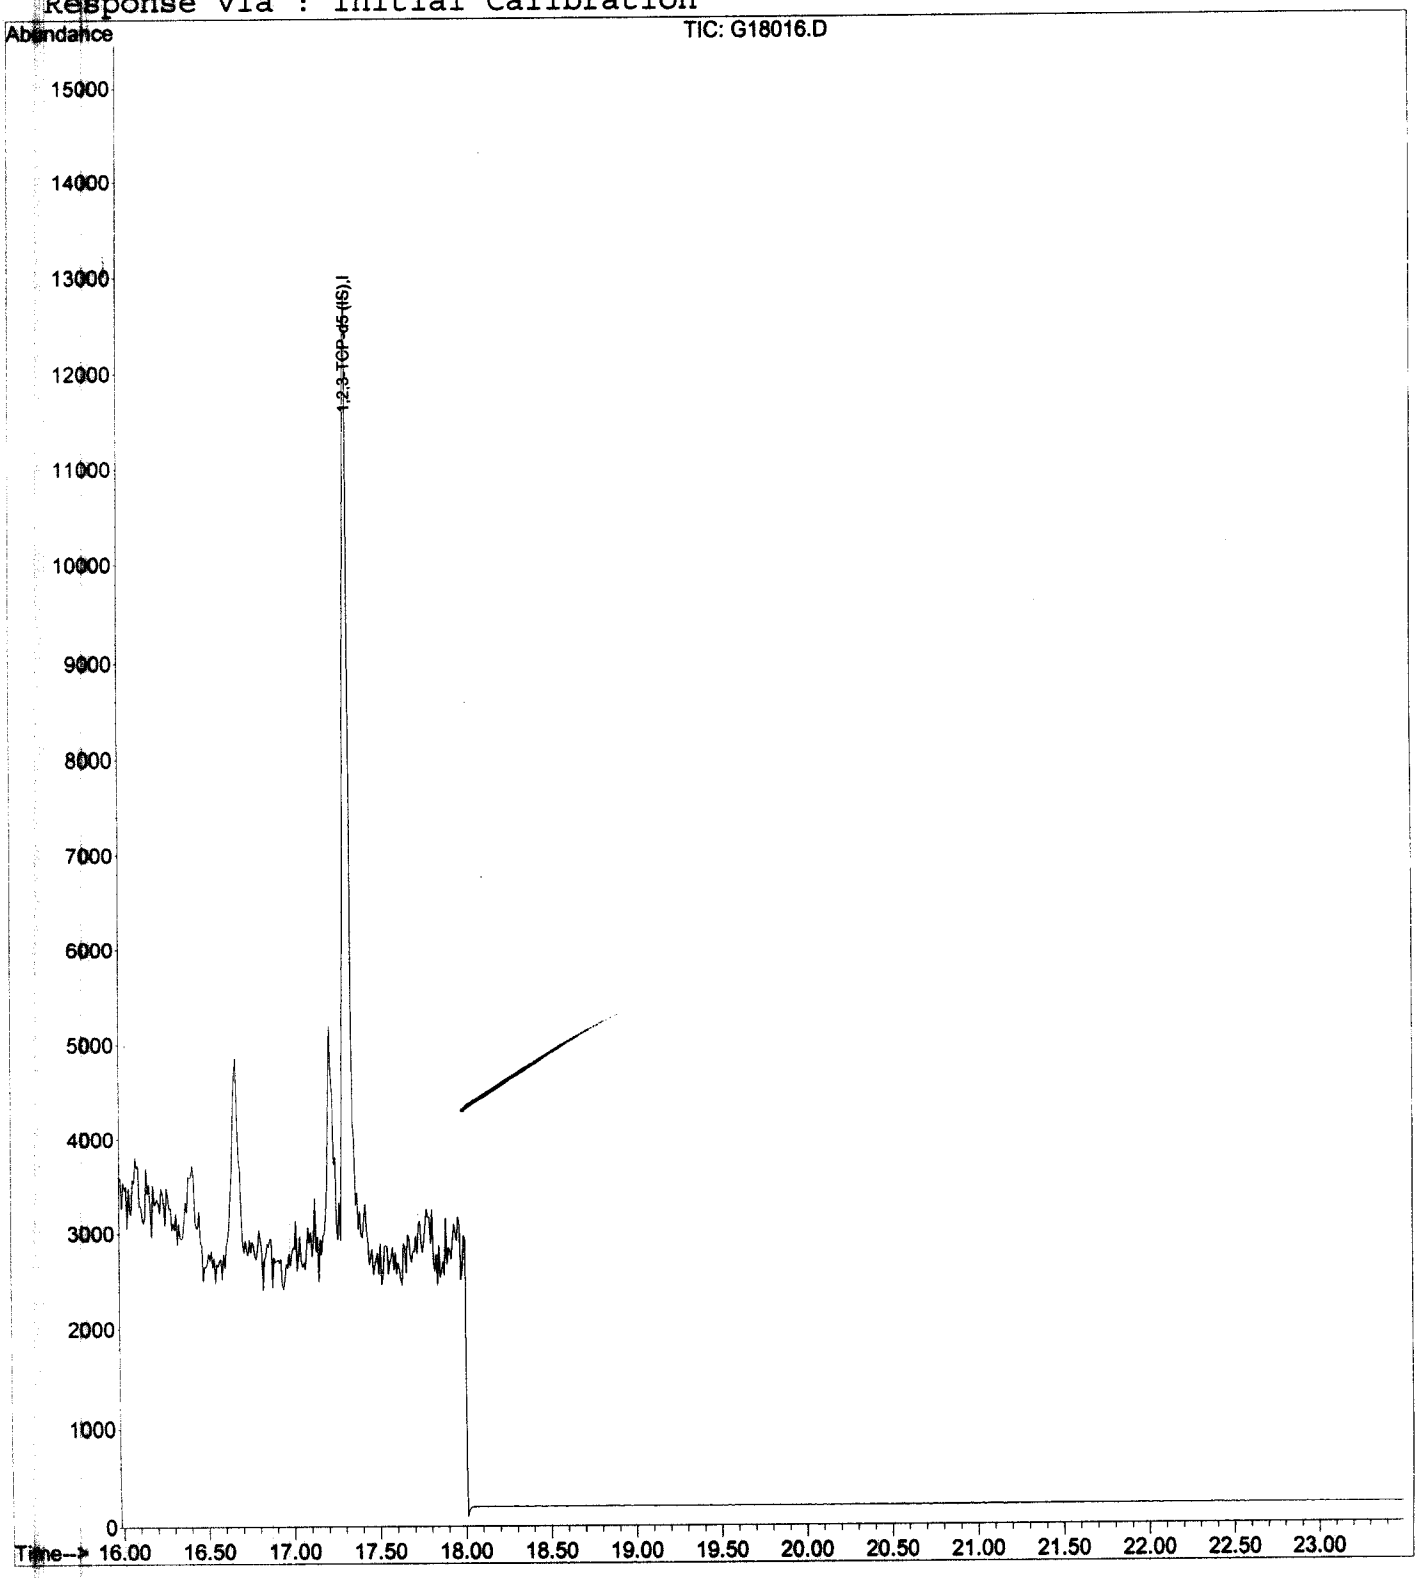

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18017.D
Acq On : 18 Jul 2007 7:38 pm
Sample : CQG0634-03
Misc : 25mL
MS Integration Params: RTEINT.P
Quant Time: Jul 19 09:37:32 2007

Vial: 17
Operator: PM
Inst : GCMS39
Multiplr: 1.00

7/19/07

Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	21933	50.00	ng/L	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18017.D
Acq On : 18 Jul 2007 7:38 pm
Sample : CQG0634-03
Misc : 25mL
MS Integration Params: RTEINT.P
Quant Time: Jul 19 9:37 2007

Vial: 17
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration

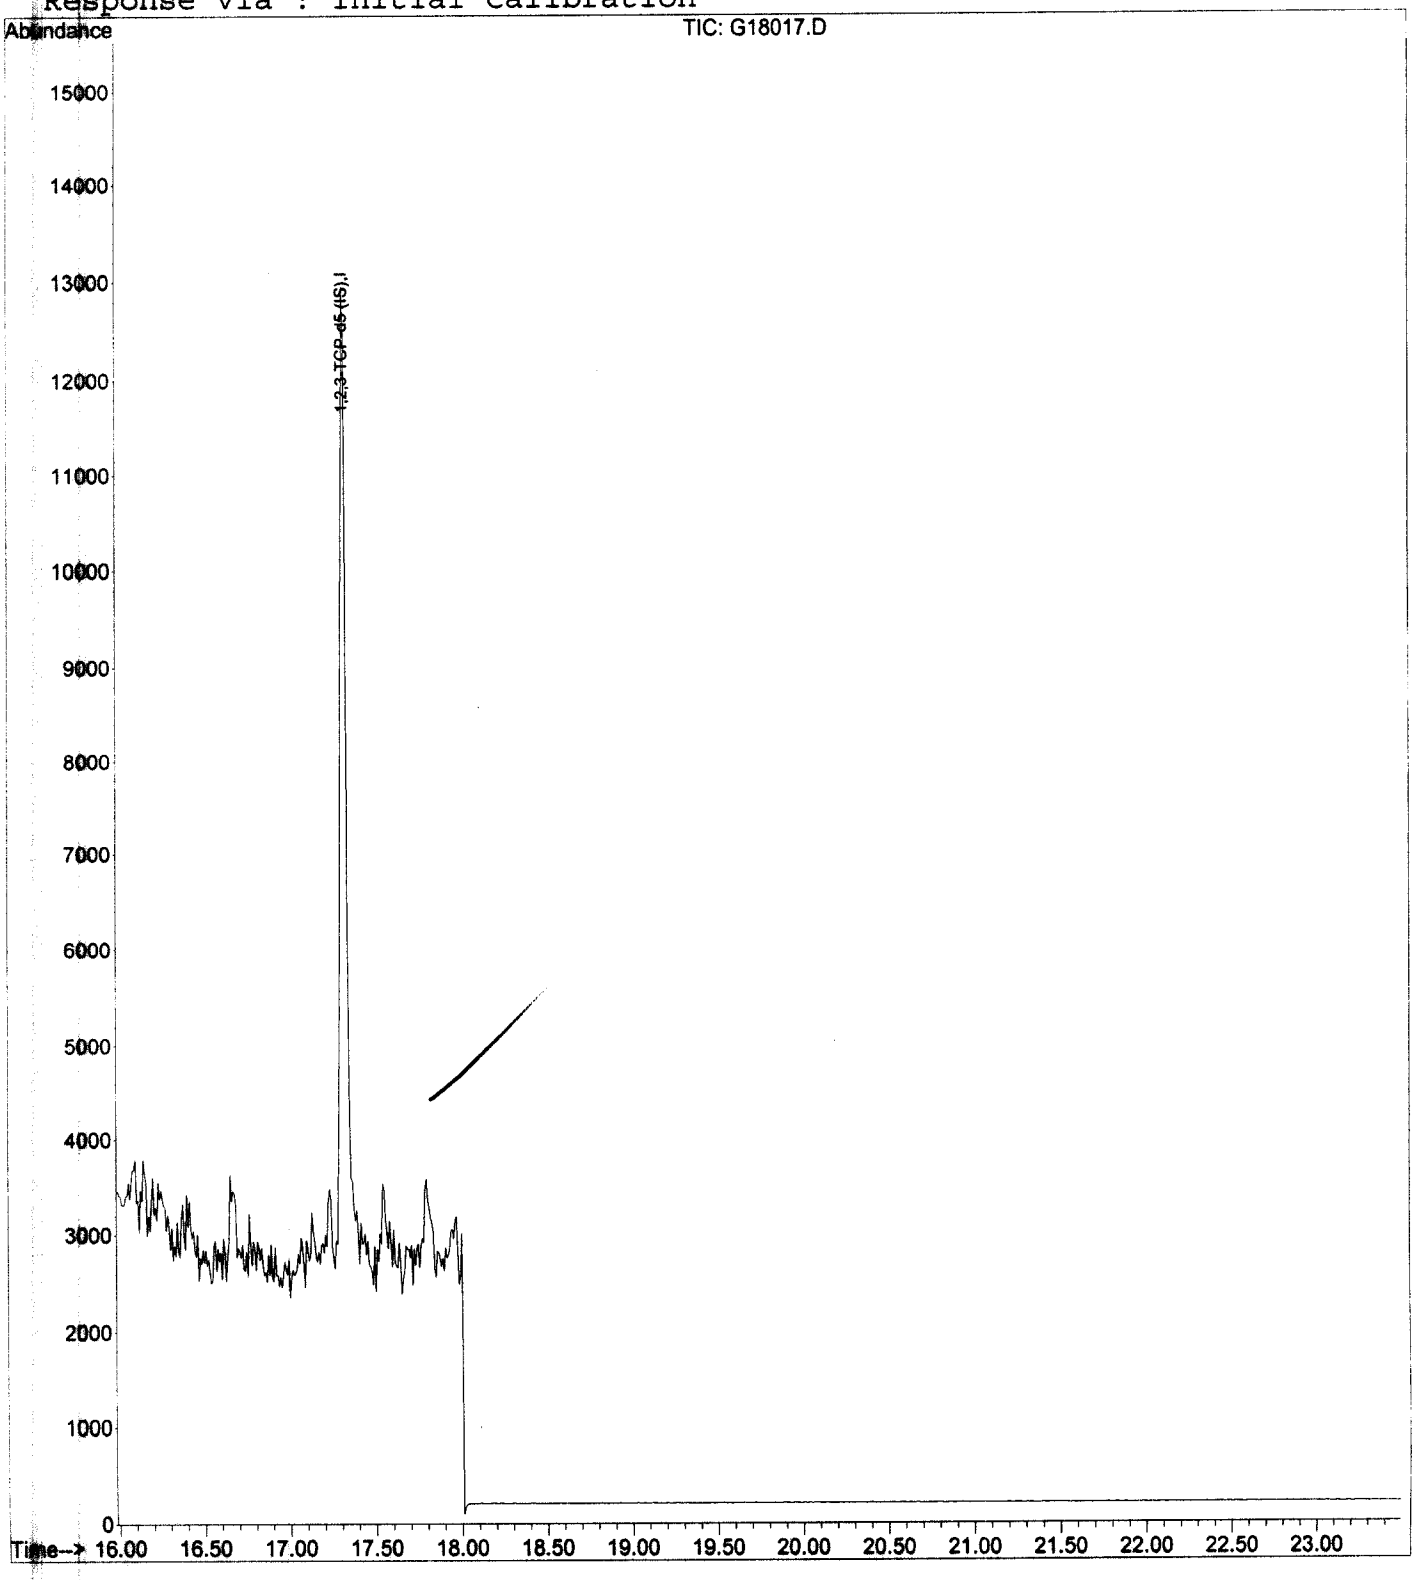

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18018.D
Acq On : 18 Jul 2007 8:11 pm
Sample : CQG0634-04
Misc : 25mL
MS Integration Params: RTEINT.P
Quant Time: Jul 19 09:37:33 2007

Vial: 18
Operator: PM
Inst : GCMS3
Multiplr: 1.00

Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.31	79	20680	50.00	ng/L	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18018.D
Acq On : 18 Jul 2007 8:11 pm
Sample : CQG0634-04
Misc : 25mL
MS Integration Params: RTEINT.P
Quant Time: Jul 19 9:37 2007

Vial: 18
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration

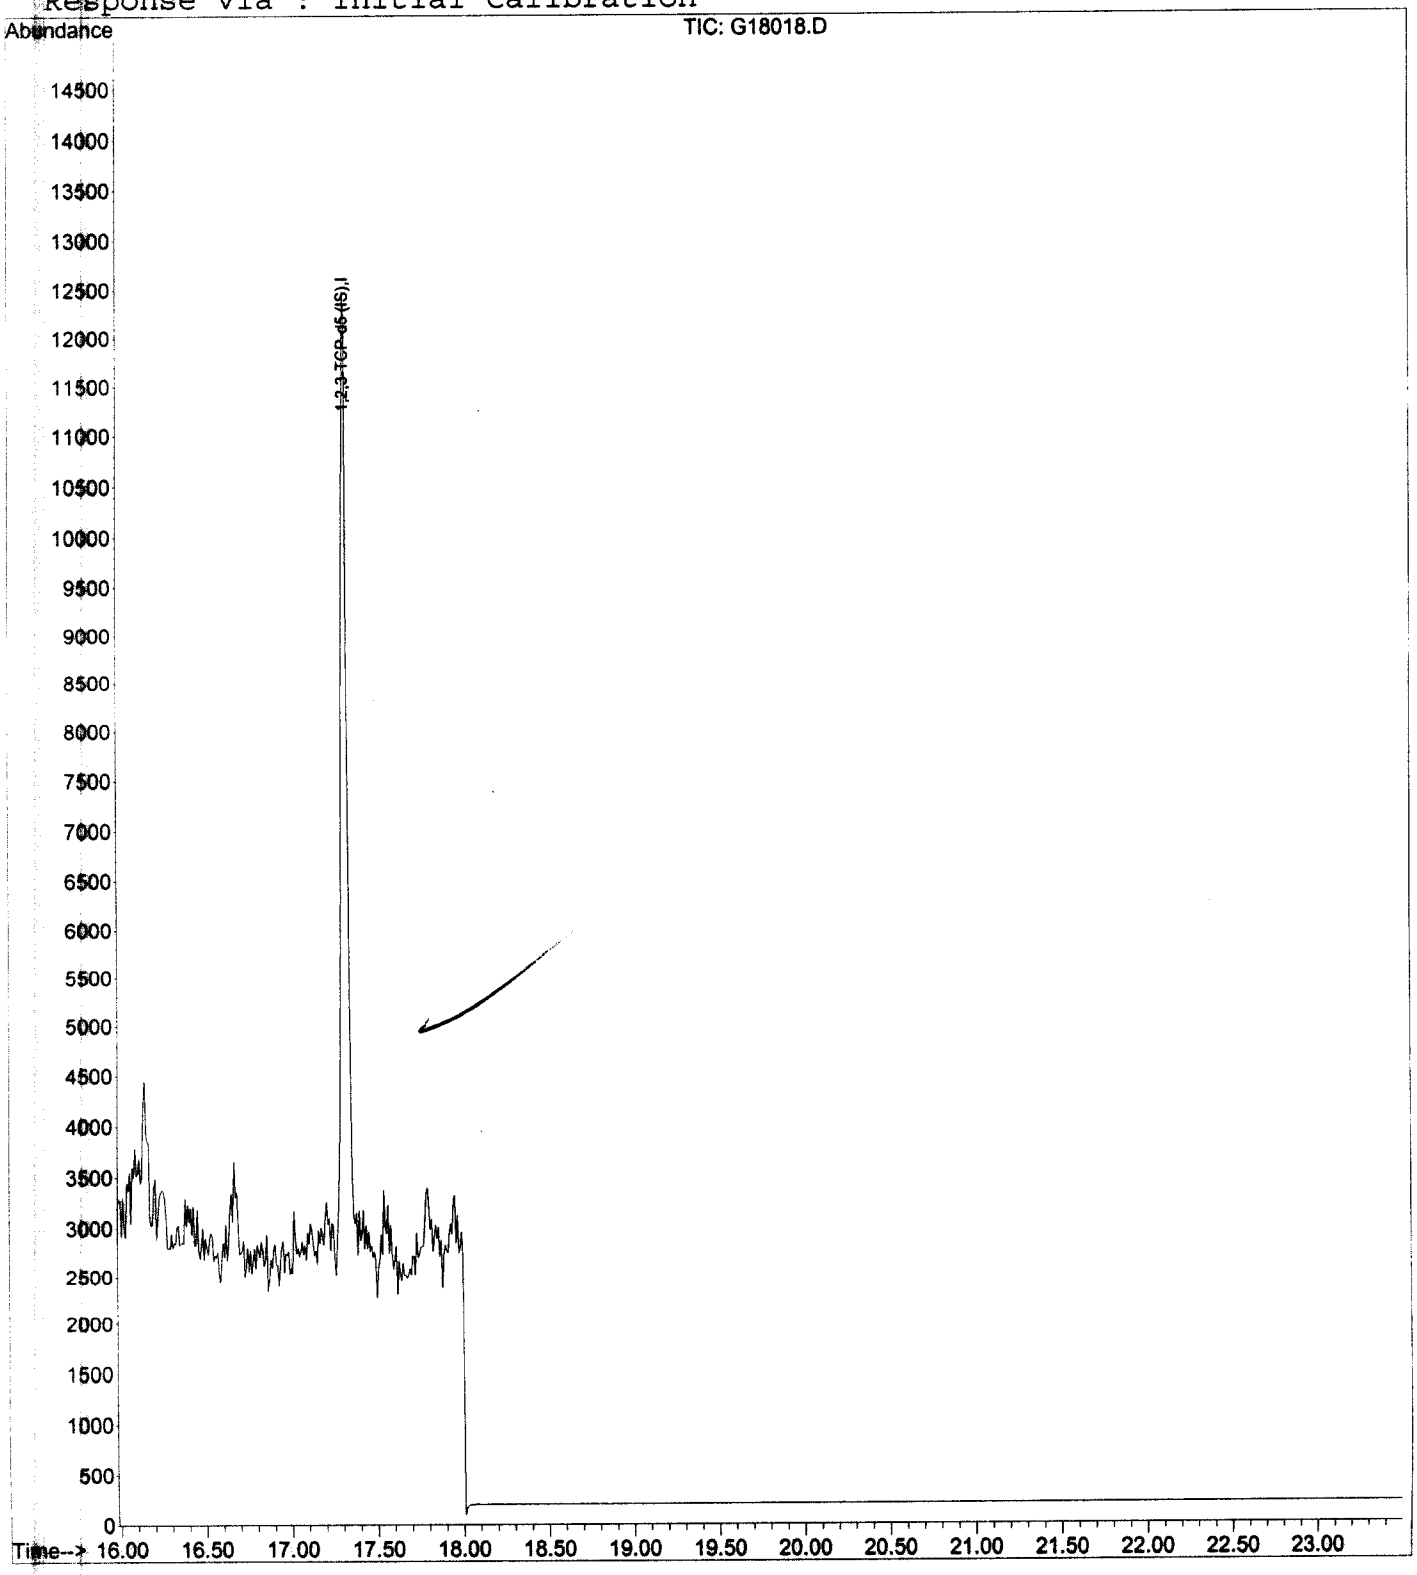

1,2,3-Trichloropropane by GC/MS Calibration Verification Check

7/19/07

File:	G18019.D	**Instrument:**	GCMS39
Operator:	PM		
Date:	18 Jul 2007 8:43 pm	**QC BATCH # :**	CCV

	Source	Response	% Recovery	Control Limits
2) 1,2,3-Trichloropropane	50	49.86	99.7	80-120

* Denotes values out of expected range

Evaluate Continuing Calibration Report

Data File : C:\DATA\07JUL18\G18019.D
Acq On : 18 Jul 2007 8:43 pm
Sample : CCV
Misc : 25mL w/ 50ppt #7060083
MS Integration Params: RTEINT.P

Vial: 19
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Multiple Level Calibration

Min. RRF : 0.000 Min. Rel. Area : 80% Max. R.T. Dev 0.50min
Max. RRF Dev : 20% Max. Rel. Area : 200%

		Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1	I	1,2,3-TCP-d5 (IS)	1.000	1.000	0.0	104	0.00
2	CPM	1,2,3-Trichloropropane	0.906	0.903	0.3	104	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 0

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18019.D
Acq On : 18 Jul 2007 8:43 pm
Sample : CCV
Misc : 25mL w/ 50ppt #7060083
MS Integration Params: RTEINT.P
Quant Time: Jul 19 09:37:35 2007

Vial: 19
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP071107.R

Quant Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration
DataAcq Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) 1,2,3-TCP-d5 (IS)	17.32	79	20897	50.00 ng/L	0.00

Target Compounds					Qvalue
2) 1,2,3-Trichloropropane	17.41	75	18870	49.86 ng/L #	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

Data File : C:\DATA\07JUL18\G18019.D
Acq On : 18 Jul 2007 8:43 pm
Sample : CCV
Misc : 25mL w/ 50ppt #7060083
MS Integration Params: RTEINT.P
Quant Time: Jul 19 9:37 2007

Vial: 19
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP07110

Method : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration

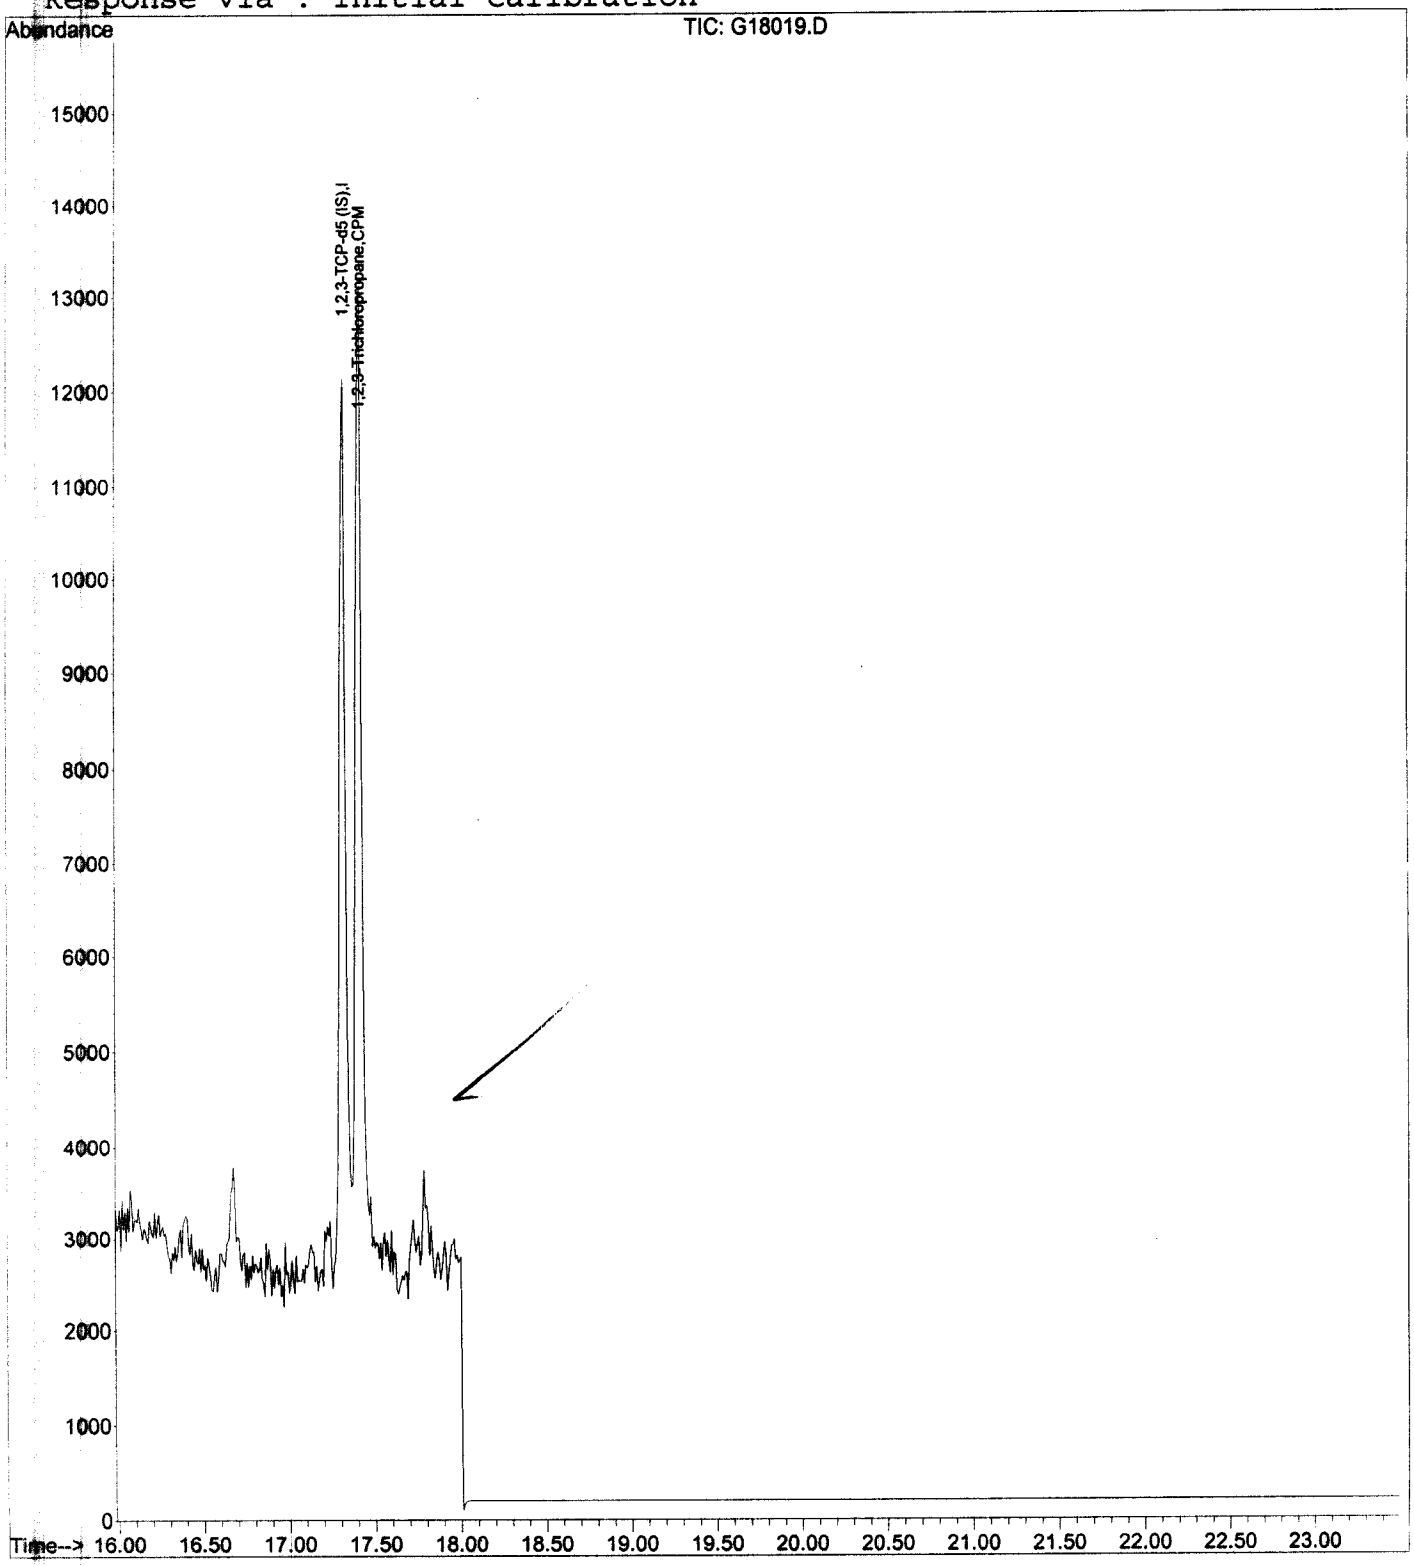

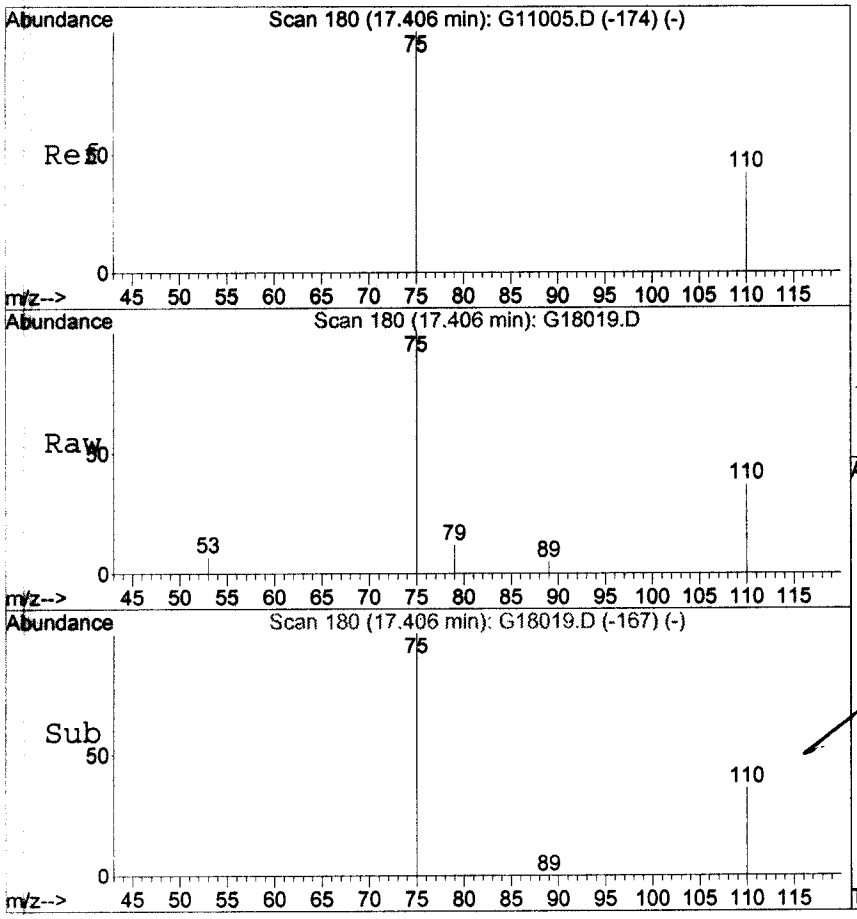

#2
1,2,3-Trichloropropane
Concen: 49.86 ng/L
RT: 17.41 min Scan# 180
Delta R.T. 0.00 min
Lab File: G18019.D
Acq: 18 Jul 2007 8:43 pm

Tgt Ion: 75 Resp: 18870

Ion	Ratio	Lower	Upper
75	100		
110	39.2	11.2	71.2
53	0.0	0.0	30.0
89	0.5	0.0	30.8

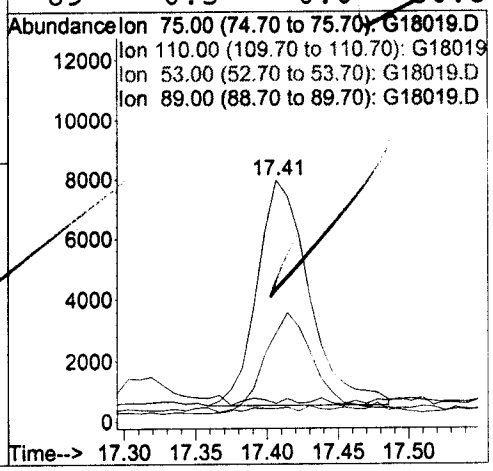

Mini Miner 2.02 (70108) Directory Scan: x:\07JUL26 7/27/07 27 Jul 2007 10:29

Level	Status	Code	Operator	Instrument	Sample ID
[illegible] x:\07JUL26\G26001.D [illegible] x:\07JUL26\G26001.D	No Audit				
[illegible] x:\07JUL26\G26002.D [illegible] x:\07JUL26\G26002.D	No Audit				
[illegible] x:\07JUL26\G26003.D [illegible] C:\DATA\07JUL26\G26003.D	Scanned	QD(1)	PM	GCMS39	Equil Rinse (25mL)
[illegible] x:\07JUL26\G26004.D [illegible] C:\DATA\07JUL26\G26004.D	Scanned	QD(1)	PM	GCMS39	CCV (25mL w/ 50ppt #7070110)
[illegible] x:\07JUL26\G26005.D [illegible] C:\DATA\07JUL26\G26005.D	Scanned	QD(1)	PM	GCMS39	C7G2611-BS1 (25mL w/ 5ppt #7070110)
[illegible] x:\07JUL26\G26006.D [illegible] C:\DATA\07JUL26\G26006.D	Scanned	QD(1)	PM	GCMS39	C7G2611-BLK1 (25mL w/ #7070111)
[illegible] x:\07JUL26\G26007.D [illegible] C:\DATA\07JUL26\G26007.D	Scanned	QD(1)	PM	GCMS39	CQG0634-05 (25mL)
[illegible] x:\07JUL26\G26008.D [illegible] C:\DATA\07JUL26\G26008.D	Scanned	QD(1)	PM	GCMS39	CQG0634-06 (25mL)
[illegible] x:\07JUL26\G26009.D [illegible] C:\DATA\07JUL26\G26009.D	Scanned	QD(1)	PM	GCMS39	CQG0698-01 (25mL)
[illegible] x:\07JUL26\G26010.D [illegible] C:\DATA\07JUL26\G26010.D	Scanned	QD(1)	PM	GCMS39	CQG0702-01 (25mL)
[illegible] x:\07JUL26\G26011.D [illegible] C:\DATA\07JUL26\G26011.D	Scanned	QD(1)	PM	GCMS39	C7G2611-MS1 (25mL w/#7070110; 702-01)

Level	Status	Code	Operator	Instrument	Sample ID
		07JUL26\G26012.D			
		DATA\07JUL26\G26012.D			
	Scanned	QD(1)	PM	GCMS39	C7G2611-MSD1 (25mL w/#7070110; 702-01)
		07JUL26\G26013.D			
		DATA\07JUL26\G26013.D			
	Scanned	QD(1)	PM	GCMS39	CQG0702-02 (25mL)
		07JUL26\G26014.D			
		DATA\07JUL26\G26014.D			
	Scanned	QD(1)	PM	GCMS39	CQG0702-03 (25mL)
		07JUL26\G26015.D			
		DATA\07JUL26\G26015.D			
	Scanned	QD(1)	PM	GCMS39	CQG0702-04 (25mL)
		07JUL26\G26016.D			
		DATA\07JUL26\G26016.D			
	Scanned	QD(1)	PM	GCMS39	CQG0702-05 (25mL)
		07JUL26\G26017.D			
		DATA\07JUL26\G26017.D			
	Scanned	QD(1)	PM	GCMS39	CQG0740-01 (25mL)
		07JUL26\G26018.D			
		DATA\07JUL26\G26018.D			
	Scanned	QD(1)	PM	GCMS39	CQG0740-02 (25mL)
		07JUL26\G26019.D			
		DATA\07JUL26\G26019.D			
	Scanned	QD(1)	PM	GCMS39	CCV (25mL w/ 50ppt #7070110)
		07JUL26\G26020.D			
		DATA\07JUL26\G26020.D			
	Scanned		PM	GCMS39	BLANK (25mL w/ #7070111)
		07JUL26\G26021.D			
		DATA\07JUL26\G26021.D			
	Scanned	QD(1)	PM	GCMS39	IDOC1 (25mL w/ 50ppt #7070110; KC)
		07JUL26\G26022.D			
		DATA\07JUL26\G26022.D			
	Scanned	QD(1)	PM	GCMS39	IDOC2 (25mL w/ 50ppt #7070110; KC)

Status	Code	Operator	Instrument	Sample ID
x:\07JUL26\G26023.D				
C:\DATA\07JUL26\G26023.D				
Scanned	QD(1)	PM	GCMS39	IDOC3 (25mL w/ 50ppt #7070110; KC)
x:\07JUL26\G26024.D				
C:\DATA\07JUL26\G26024.D				
Scanned	QD(1)	PM	GCMS39	IDOC4 (25mL w/ 50ppt #7070110; KC)
x:\07JUL26\G26025.D				
C:\DATA\07JUL26\G26025.D				
Scanned	QD(1)	PM	GCMS39	IDOC5 (25mL w/ 50ppt #7070110; KC)
x:\07JUL26\G26026.D				
C:\DATA\07JUL26\G26026.D				
Scanned	QD(1)	PM	GCMS39	IDOC6 (25mL w/ 50ppt #7070110L; KC)
x:\07JUL26\G26027.D				
C:\DATA\07JUL26\G26027.D				
Scanned	QD(1)	PM	GCMS39	IDOC7 (25mL w/ 50ppt #7070110L; KC)

Method Last Update date after Quantitation date

ScanSummary.rpt

Data Files Scanned	Beginning Analyzed Date
Methods	Ending Analyzed Date
Samples	Analyzed Range
Tunes	Greatest Time Between Tunes
CCCs	Greatest Time Between CCCs

Method Last Updated count

Operators Intruments

PREPARATION BENCHSHEET

C7G2611

TestAmerica - Ontario, CA

Printed: 7/27/2007 10:26:52 AM

Matrix: Water

Prepared using: GCMS Volatiles - EPA 524.2

Surrogate used: 7070111

Lab Number	Analysis	Prepared	Initial (ml)	Final (ml)	Source ID	Spike 1	ul Spike	Spike 2	ul Spike	ul Surr	Initials	Extraction Comments
C7G2611-BLK1	QC	07/26/07 12:13	25	25			0		0	5		
C7G2611-BS1	QC	07/26/07 12:13	25	25		7070110	0.5		100	5		
C7G2611-MS1	QC	07/26/07 12:13	25	25	CQG0702-01	7070110	5		100	5		
C7G2611-MSD	QC	07/26/07 12:13	25	25	CQG0702-01	7070110	5		100	5		
CQG0634-05	524.2 CA 1,2,3-TCP (SIM)	07/26/07 12:13	25	25						5		
CQG0634-06	524.2 CA 1,2,3-TCP (SIM)	07/26/07 12:13	25	25						5		
CQG0698-01	524.2 CA 1,2,3-TCP (SIM)	07/26/07 12:13	25	25						5		Sub DMAC level 3
CQG0702-01	524.2 CA 1,2,3-TCP (SIM)	07/26/07 12:13	25	25						5		
CQG0702-02	524.2 CA 1,2,3-TCP (SIM)	07/26/07 12:13	25	25						5		
CQG0702-03	524.2 CA 1,2,3-TCP (SIM)	07/26/07 12:13	25	25						5		
CQG0702-04	524.2 CA 1,2,3-TCP (SIM)	07/26/07 12:13	25	25						5		
CQG0702-05	524.2 CA 1,2,3-TCP (SIM)	07/26/07 12:13	25	25						5		
CQG0740-01	524.2 CA 1,2,3-TCP (SIM)	07/26/07 12:13	25	25						5		
CQG0740-02	524.2 CA 1,2,3-TCP (SIM)	07/26/07 12:13	25	25						5		

Reagents used in Batch

Reagent	Description	Solvent

GCMS #39

Posted
7/27/07

Spiking Witnessed By Date

Preparation Reviewed By Date

Extracts Received By Date

Injection Log

[illegible]	[illegible]	[illegible]	[illegible]	[illegible]	[illegible]	[illegible]
1	1	G26001.d	1.	Equil Rinse	25mL	26 Jul 2007 10:35
2	2	G26002.d	1.	Equil Rinse	25ml	26 Jul 2007 11:08
3	3	G26003.d	1.	Equil Rinse	25mL	26 Jul 2007 11:40
4	4	G26004.d	1.	CCV	25mL w/ 50ppt #7070110	26 Jul 2007 12:13
5	5	G26005.d	1.	C7G2611-BS1	25mL w/ 5ppt #7070110	26 Jul 2007 12:46
6	6	G26006.d	1.	C7G2611-BLK1	25mL w/ #7070111	26 Jul 2007 13:18
7	7	G26007.d	1.	CQG0634-05	25mL	26 Jul 2007 14:08
8	8	G26008.d	1.	CQG0634-06	25mL	26 Jul 2007 14:41
9	9	G26009.d	1.	CQG0698-01	25mL	26 Jul 2007 15:14
10	10	G26010.d	1.	CQG0702-01	25mL	26 Jul 2007 15:46
11	11	G26011.d	1.	C7G2611-MS1	25mL w/#7070110; 702-01	26 Jul 2007 16:19
12	12	G26012.d	1.	C7G2611-MSD1	25mL w/#7070110; 702-01	26 Jul 2007 16:52
13	13	G26013.d	1.	CQG0702-02	25mL	26 Jul 2007 17:24
14	14	G26014.d	1.	CQG0702-03	25mL	26 Jul 2007 17:57
15	15	G26015.d	1.	CQG0702-04	25mL	26 Jul 2007 18:29
16	16	G26016.d	1.	CQG0702-05	25mL	26 Jul 2007 19:02
17	17	G26017.d	1.	CQG0740-01	25mL	26 Jul 2007 19:34
18	18	G26018.d	1.	CQG0740-02	25mL	26 Jul 2007 20:07
19	19	G26019.d	1.	CCV	25mL w/ 50ppt #7070110	26 Jul 2007 20:40
20	20	G26020.d	1.	BLANK	25mL w/ #7070111	26 Jul 2007 21:12
21	21	G26021.d	1.	IDOC1	25mL w/ 50ppt #7070110; KC	26 Jul 2007 21:45
22	22	G26022.d	1.	IDOC2	25mL w/ 50ppt #7070110; KC	26 Jul 2007 22:18
23	23	G26023.d	1.	IDOC3	25mL w/ 50ppt #7070110; KC	26 Jul 2007 22:50
24	24	G26024.d	1.	IDOC4	25mL w/ 50ppt #7070110; KC	26 Jul 2007 23:23
25	25	G26025.d	1.	IDOC5	25mL w/ 50ppt #7070110; KC	26 Jul 2007 23:55
26	26	G26026.d	1.	IDOC6	25mL w/ 50ppt #7070110L; KC	27 Jul 2007 00:28
27	27	G26027.d	1.	IDOC7	25mL w/ 50ppt #7070110L; KC	27 Jul 2007 01:00

GC/MS QA-QC Check Report

DATA\07JUL26\G26004.D
26 Jul 2007 12:13 pm

Calibration File : C:\DATA\07JUL11\G11005.D

20175

Sample	Internal Std Responses
CCV	18466
07G2611-BS1	17563
07G2611-BLK1	17066
QCG0634-05	16843
QCG0634-06	22435
QCG0698-01	20533
QCG0702-01	22149
07G2611-MS1	21119
07G2611-MSD1	23137
QCG0702-02	22433
QCG0702-03	22911
QCG0702-04	22502
QCG0702-05	22241
QCG0740-01	21499
QCG0740-02	24201
CCV	21806
BLANK	19707
IDOC1	19366
IDOC2	20159
IDOC3	17663
IDOC4	18799
IDOC5	18882
* IDOC6	18245
* IDOC7	15660*

12hr time check * - fails criteria

Jul 27 08:50:49 2007 GCMS39

GC/MS # 39

Date: 7/26/07

Analyst: JM / KC

page 1 of ~~X~~ 2

JM 7/26/07

#	Sample	Amount	Dil.	Ph	Res. Cl	Comments
	Rinse	25mL	1	N/A		
		25mL	1			
		25mL	1			
		25mL	1			50ppt #7070110
	611 - BS1	25mL	1			5ppt #7070110
	-BLK1	25mL	1			#7070111
	634-05	25mL	1			
	-06	25mL	1			
	698-01	25mL	1			
	702-01	25mL	1			
	611 - MS1	25mL	1			#7070110; 702-01
	-MSD1	25mL	1			
	702-02	25mL	1			
	-03	25mL	1			
	-04	25mL	1			
	-05	25mL	1			
	740-01	25mL	1			
	-02	25mL	1			
		25mL	1			50ppt #7070110
	BLANK	25ML	1			KC 7/26/07 ~~5ppt #7070110~~ #7070111
	[illegible]	25ML	1			50ppt #7070110
	[illegible]	25ML	1			
	[illegible]	25ML	1			
	[illegible]	25ML	1			

GC/MS # 39 page 2 of 2

Date: 7/26/07

Analyst: KC

#	Sample	Amount	Dil.	Ph	Res. Cl_2	Comments
	IP005	25ML	1			50ppt #707011C
	IP006	25ML	1			↓
	IP007	25ML	1			✓

7/26/07

1,2,3-Trichloropropane by GC/MS Calibration Verification Check

File:	G26004.D	**Instrument:**	GCMS39
Operator:	PM		
Date:	26 Jul 2007 12:13 pm	**QC BATCH # :**	CCV

	Source	Response	% Recovery	Control Limits
1,2,3-Trichloropropane	50	51.46	102.9	80-120

[illegible] out of expected range

7/26/2007 1:29 PM

C:\MSDchem\Custrpt\123TCP.CRT

Evaluate Continuing Calibration Report

C:\DATA\07JUL26\G26004.D
26 Jul 2007 12:13 pm
CCV
25mL w/ 50ppt #7070110
ion Params: RTEINT.P

Vial: 4
Operator: PM
Inst : GCMS39
Multiplr: 1.00

: C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
: Thu Jul 12 12:36:02 2007
: Multiple Level Calibration

: 0.000 Min. Rel. Area : 80% Max. R.T. Dev 0.50min
Lev : 20% Max. Rel. Area : 200%

nd	AvgRF	CCRF	%Dev	Area%	Dev(min)
CP-d5 (IS)	1.000	1.000	0.0	92	0.00
richloropropane	0.906	0.932	-2.9	95	0.00

Range SPCC's out = 0 CCC's out = 0
TCP071107.M Thu Jul 26 13:29:43 2007 Page 1

Quantitation Report (Not Reviewed)

:\DATA\07JUL26\G26004.D
26 Jul 2007 12:13 pm
CV
5mL w/ 50ppt #7070110
Params: RTEINT.P
Jul 26 13:11:38 2007

Vial: 4
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP071107.R

: C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
: Thu Jul 12 12:36:02 2007
: Initial Calibration
: 123-TCP

ndards	R.T.	QIon	Response	Conc Units	Dev(Min)
-d5 (IS)	17.32	79	18466	50.00 ng/L	0.00
unds					Qvalue
Trichloropropane	17.41	75	17211	51.46 ng/L	99

ier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

: C:\DATA\07JUL26\G26004.D
: 26 Jul 2007 12:13 pm
: CCV
: 25mL w/ 50ppt #7070110
egration Params: RTEINT.P
Time: Jul 26 13:11 2007

Vial: 4
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP071

: C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
Date : Thu Jul 12 12:36:02 2007
ria : Initial Calibration

TIC: G26004.D

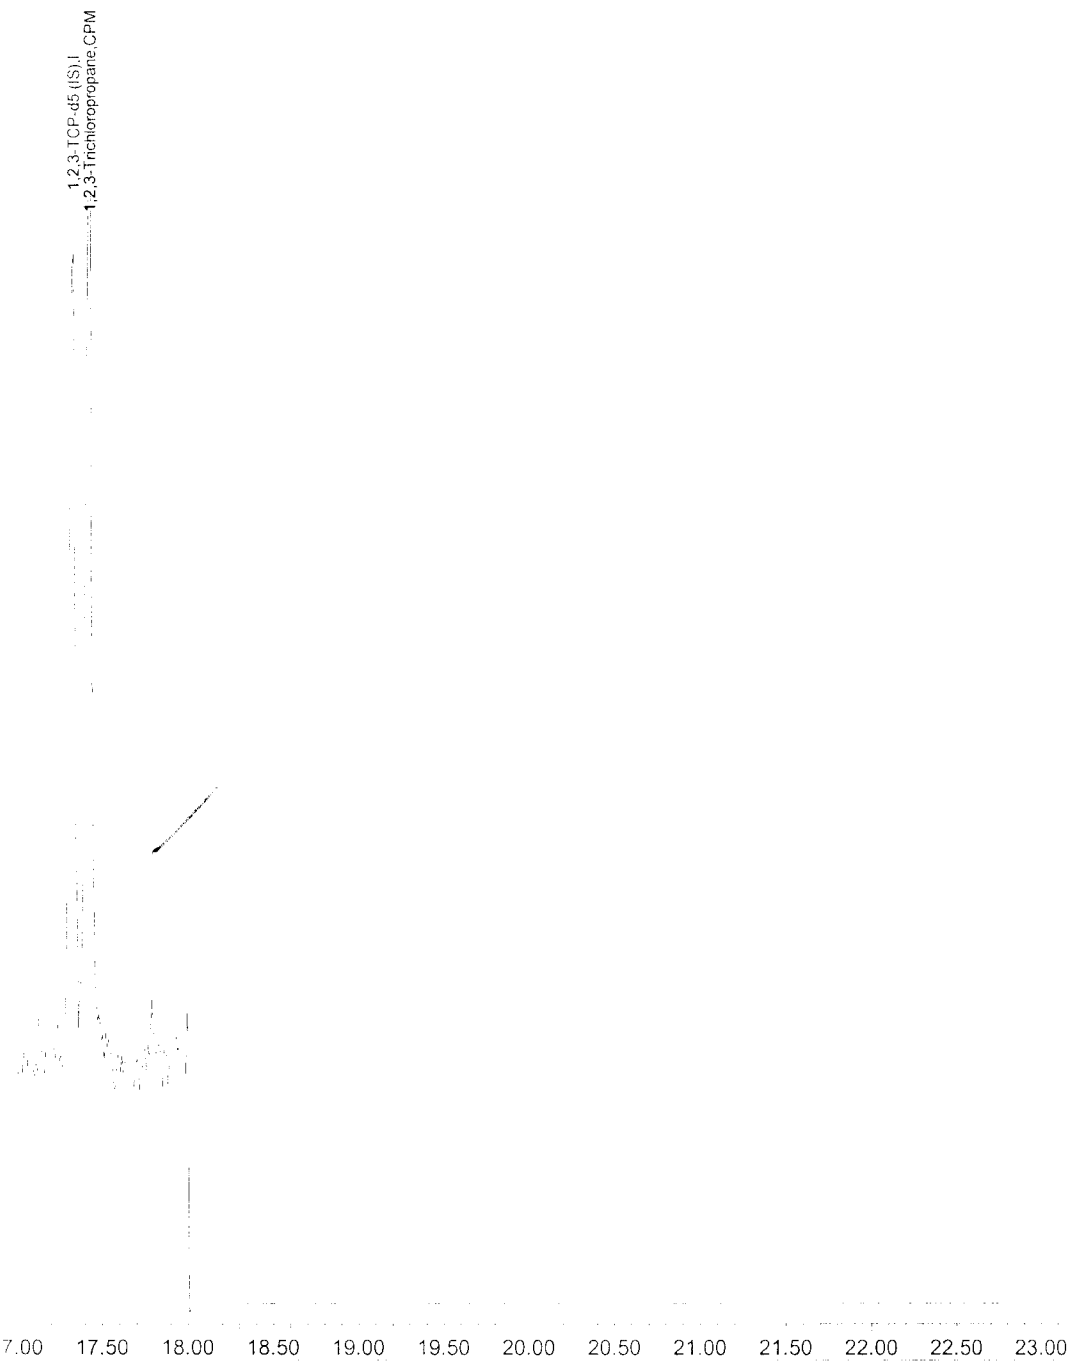

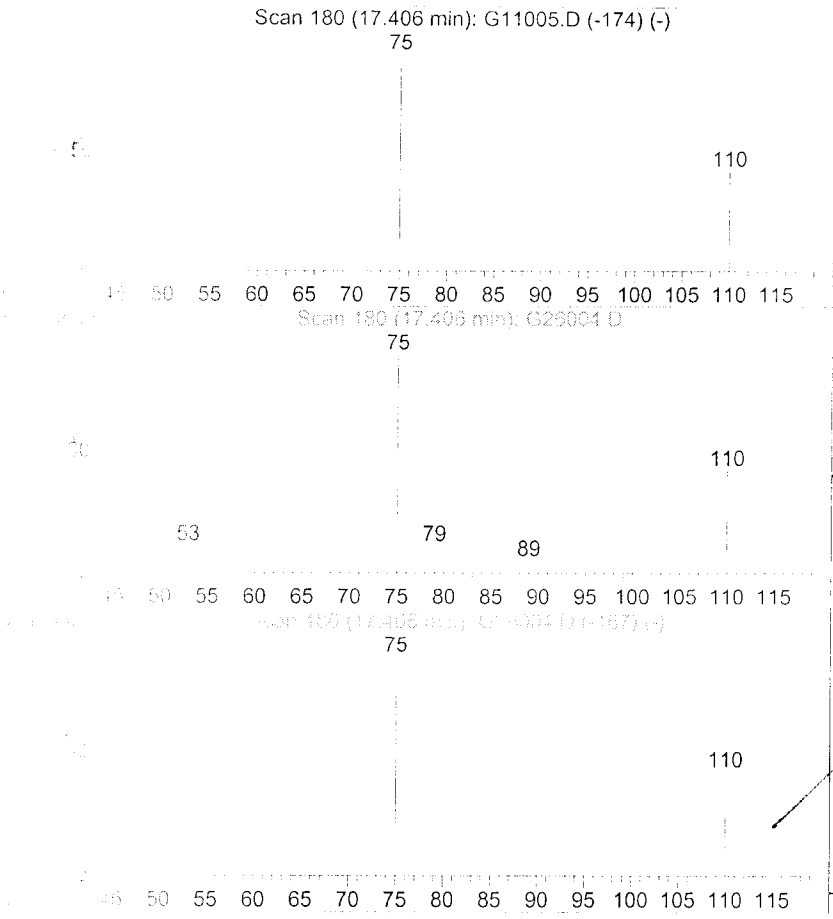

#2
1,2,3-Trichloropropane
Concen: 51.46 ng/L
RT: 17.41 min Scan# 180
Delta R.T. 0.00 min
Lab File: G26004.D
Acq: 26 Jul 2007 12:13 pm

Tgt Ion: 75 Resp: 17211

Ion	Ratio	Lower	Upper
75	100		
110	41.7	11.2	71.2
53	1.1	0.0	30.0
89	0.6	0.0	30.8

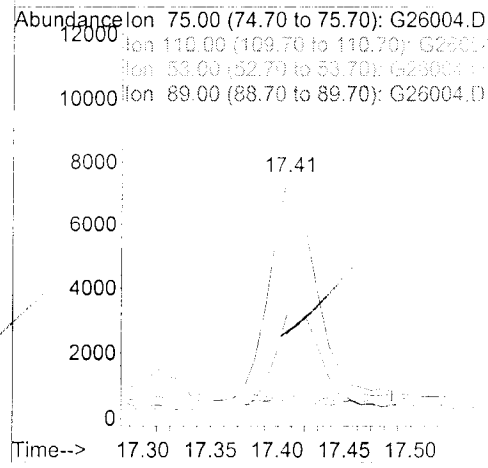

1,2,3-Trichloropropane by GC/MS LFB Check

7/26/07

File:	G26005.D	**Instrument:**	GCMS39
Operator:	PM		
Date:	26 Jul 2007 12:46 pm	**QC BATCH # :**	C7G2611-BS1

	Source	Response	% Recovery	Control Limits
1,2,3-Trichloropropane	5	4.08	81.7	80-120

* Values out of expected range

7/26/2007 1:32 PM

C:\MSDchem\Custrpt\123TCP- BS.CRT

Quantitation Report (Not Reviewed)

:\DATA\07JUL26\G26005.D
26 Jul 2007 12:46 pm
7G2611-BS1
25mL w/ 5ppt #7070110
on Params: RTEINT.P
Jul 26 13:31:54 2007

Vial: 5
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP071107.R

: C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
: Thu Jul 12 12:36:02 2007
: Initial Calibration
: 123-TCP

andards	R.T.	QIon	Response	Conc Units	Dev(Min)
TCP-d5 (IS)	17.32	79	17563	50.00 ng/L	0.00

ompounds					Qvalue
Trichloropropane	17.41	75	1299	4.08 ng/L #	40

ier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

: C:\DATA\07JUL26\G26005.D
: 26 Jul 2007 12:46 pm
: C7G2611-BS1
: 25mL w/ 5ppt #7070110
ion Params: RTEINT.P
ime: Jul 26 13:31 2007

Vial: 5
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP07110

: C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
: Thu Jul 12 12:36:02 2007
via : Initial Calibration

TIC: G26005.D

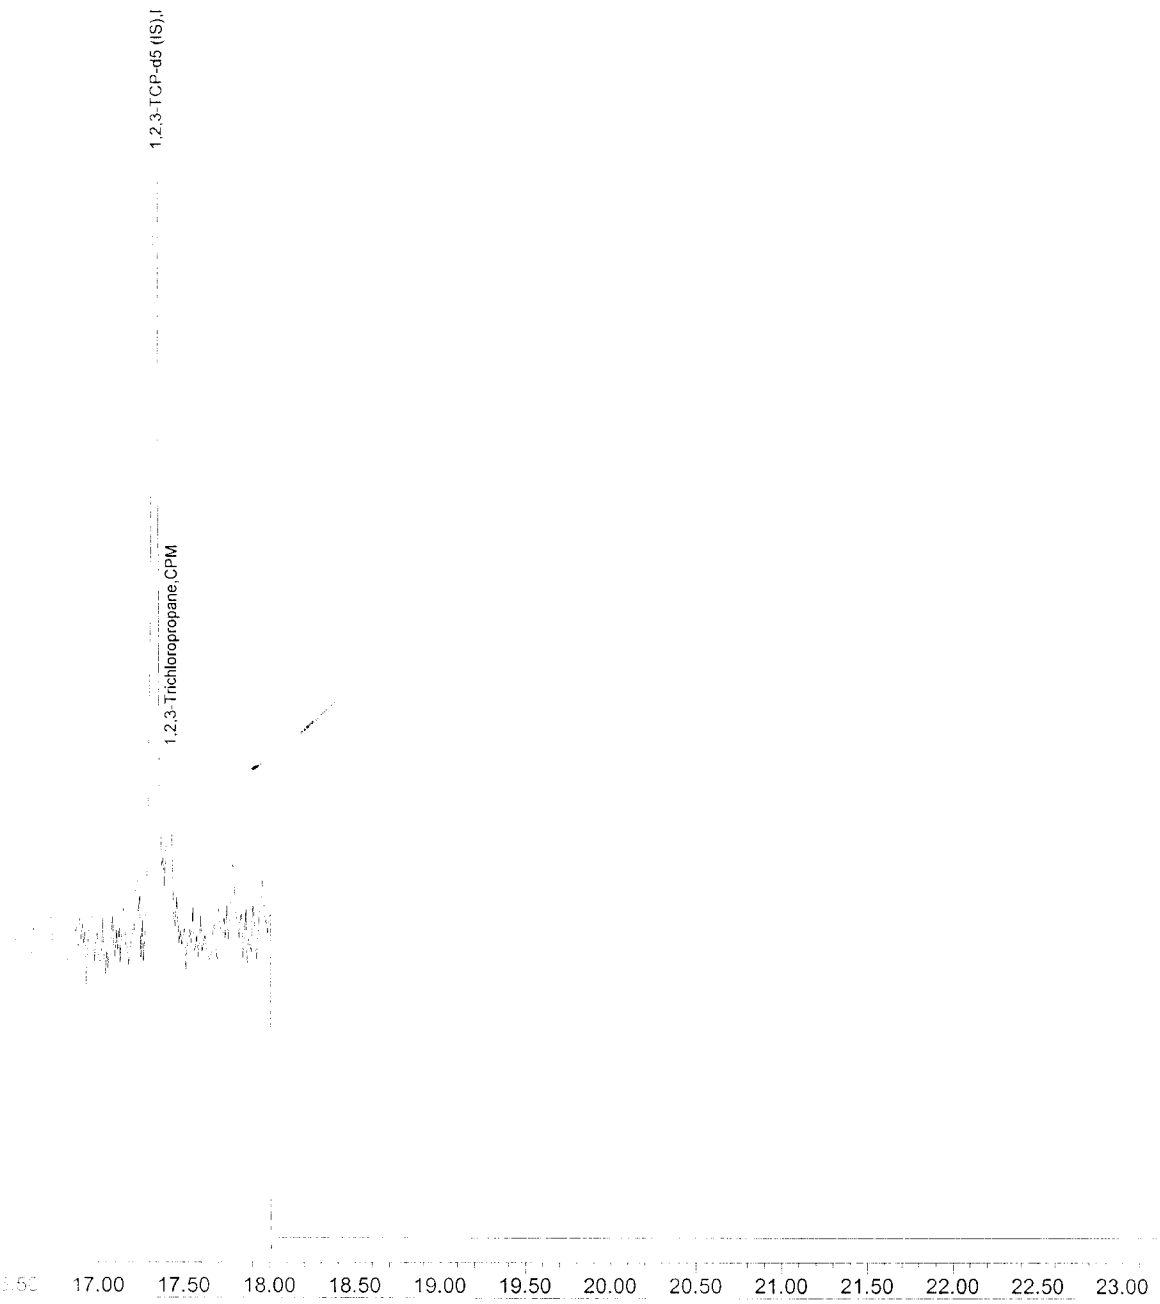

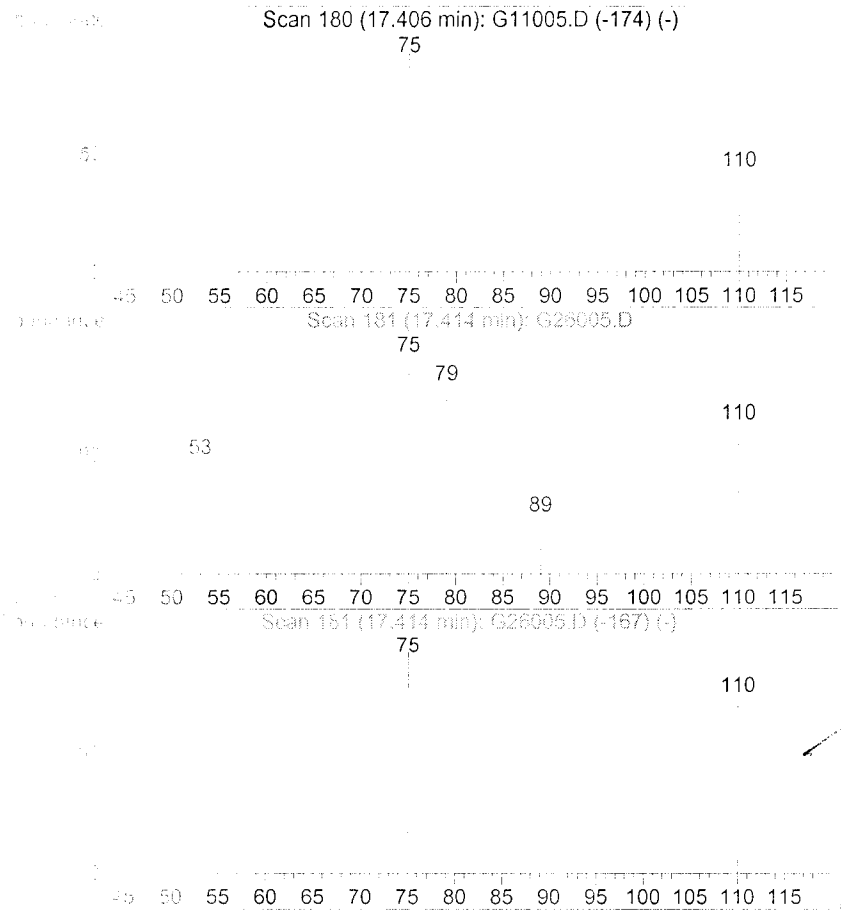

#2
1,2,3-Trichloropropane
Concen: 4.08 ng/L
RT: 17.41 min Scan# 181
Delta R.T. 0.01 min
Lab File: G26005.D
Acq: 26 Jul 2007 12:46 pm

Tgt Ion: 75 Resp: 1299

Ion	Ratio	Lower	Upper
75	100		
110	79.7	11.2	71.2#
53	11.6	0.0	30.0
89	0.0	0.0	30.8

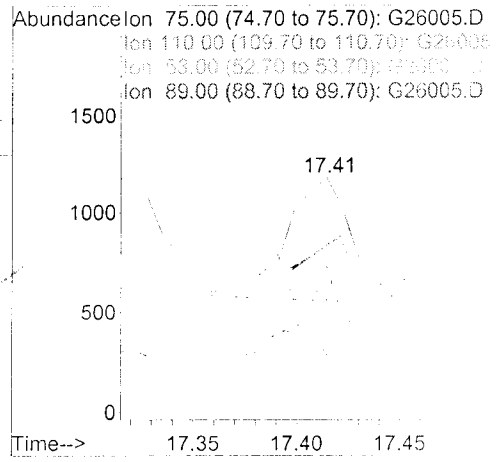

Quantitation Report (Not Reviewed)

7/26/07

C:\DATA\07JUL26\G26006.D
26 Jul 2007 1:18 pm
07G2611-BLK1
25mL w/ #7070111
Integration Params: RTEINT.P
Thu Jul 26 13:49:02 2007

Vial: 6
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP071107.R

Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
Title : 1,2,3-TCP by GCMS SIM
Last Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration
Data Path : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1,2,3-TCP-d5 (IS)	17.32	79	17066	50.00	ng/L	0.[illegible]

Compounds	Qvalue

Qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

: C:\DATA\07JUL26\G26006.D
: 26 Jul 2007 1:18 pm
: C7G2611-BLK1
: 25mL w/ #7070111
ion Params: RTEINT.P
: Jul 26 13:49 2007

Vial: 6
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP07110

: C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
: Thu Jul 12 12:36:02 2007
: Initial Calibration

TIC: G26006.D

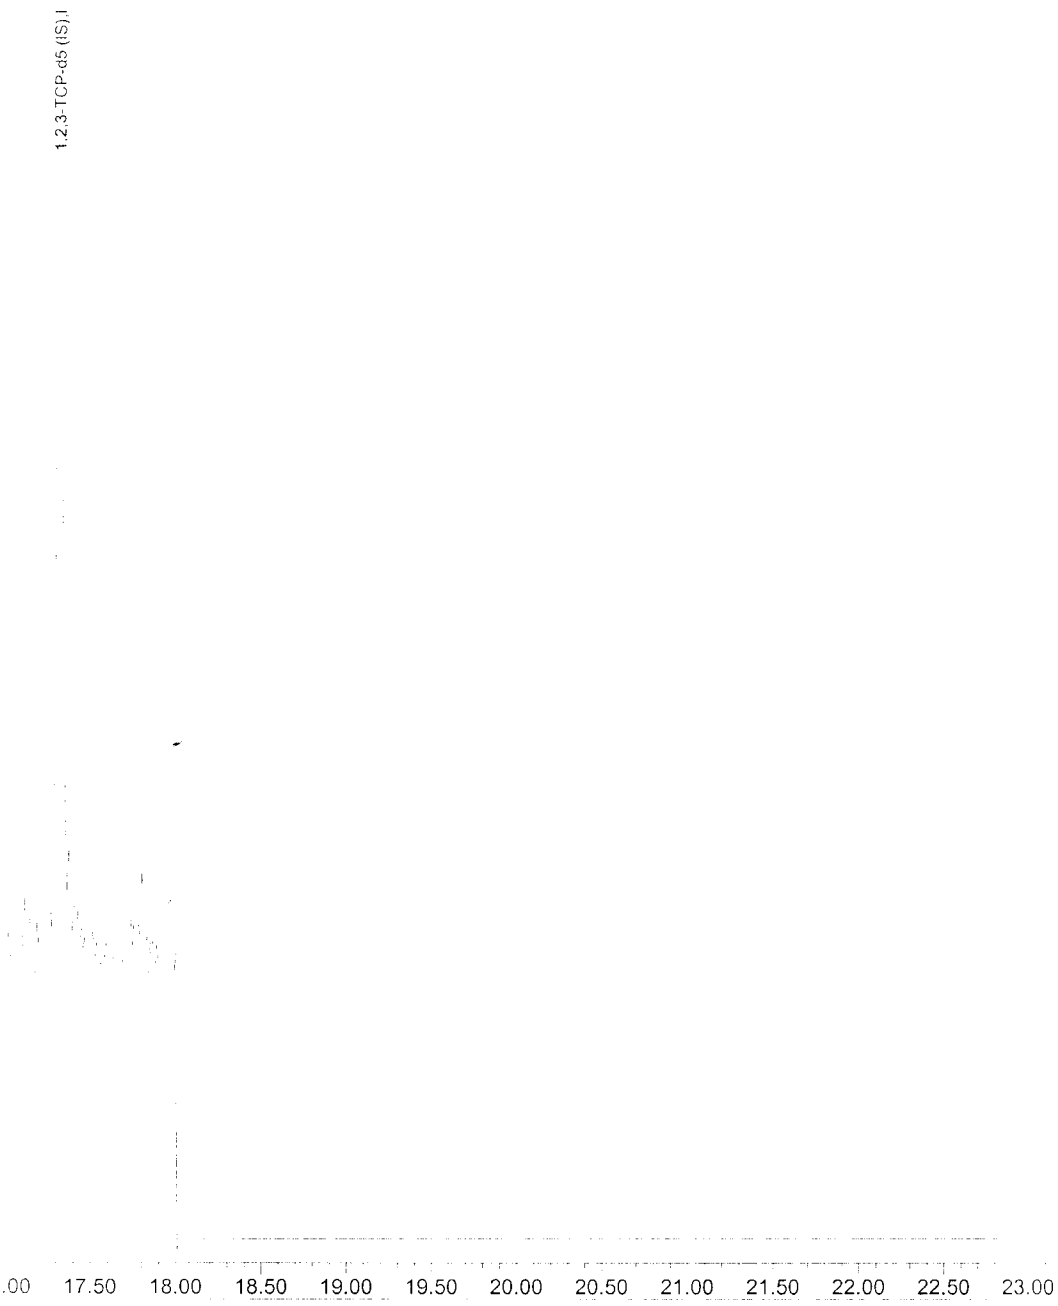

Quantitation Report (Not Reviewed)

DATA\07JUL26\G26007.D
Jul 2007 2:08 pm
G0634-05
mL

Vial: 7
Operator: PM
Inst : GCMS3
Multiplr: 1.00

7/27/07

Params: RTEINT.P
Jul 27 08:32:17 2007

Quant Results File: 123-TCP071107.R

: C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
: Thu Jul 12 12:36:02 2007
: Initial Calibration
: 123-TCP

ndards	R.T.	QIon	Response	Conc Units	Dev(Min)
TCP-d5 (IS)	17.31	79	16843	50.00 ng/L	0.00

ompounds					Qvalue
Trichloropropane	17.43	75	1074	~~3.52 ng/L~~	# ^c 46

ier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

: C:\DATA\07JUL26\G26007.D
: 26 Jul 2007 2:08 pm
: CQG0634-05
: 25mL
ion Params: RTEINT.P
: Jul 27 8:32 2007

Vial: 7
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP071107

: C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
: Thu Jul 12 12:36:02 2007
via : Initial Calibration

TIC: G26007.D

17.00 17.50 18.00 18.50 19.00 19.50 20.00 20.50 21.00 21.50 22.00 22.50 23.00

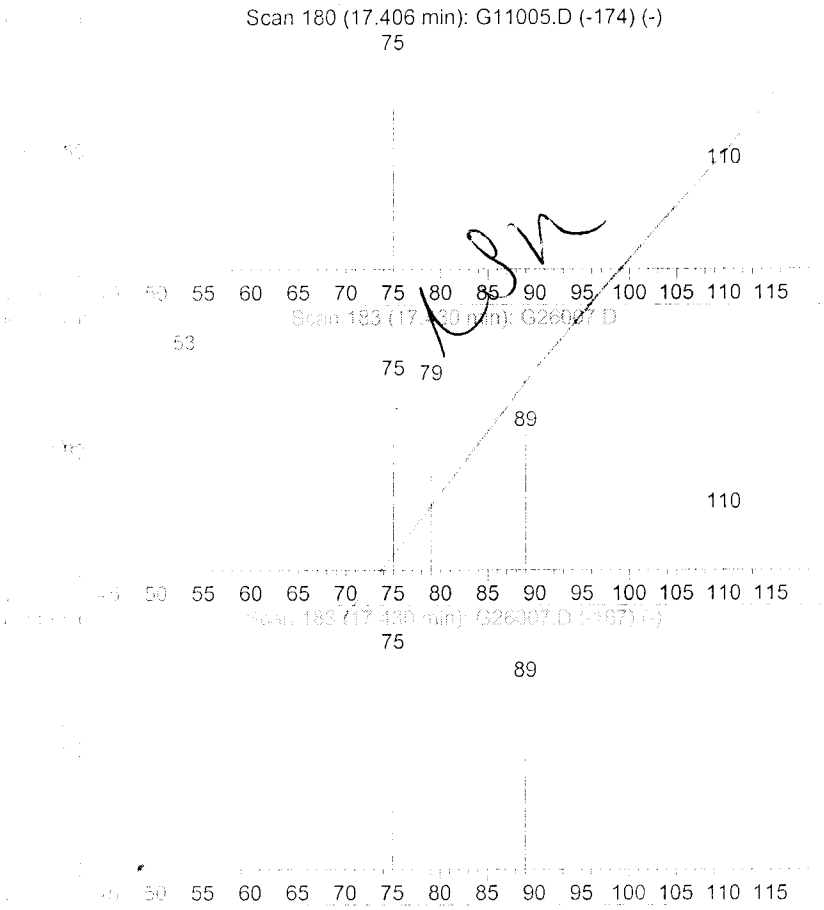

#2
1,2,3-Trichloropropane
Concen: 3.52 ng/L
RT: 17.43 min Scan# 183
Delta R.T. 0.02 min
Lab File: G26007.D
Acq: 26 Jul 2007 2:08 pm

Tgt Ion: 75 Resp: 1074

Ion	Ratio	Lower	Upper
75	100		
110	8.1	11.2	71.2#
53	124.0	0.0	30.0#
89	48.8	0.0	30.8#

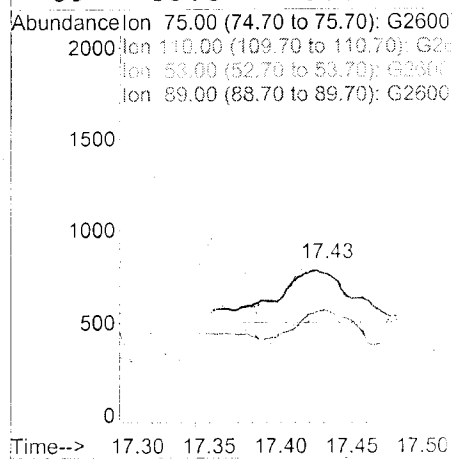

Quantitation Report (Not Reviewed)

C:\DATA\07JUL26\G26008.D
26 Jul 2007 2:41 pm
CQG0634-06
25mL

Vial: 8
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Integration Params: RTEINT.P
Jul 27 08:32:19 2007

Quant Results File: 123-TCP071107.R

Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
Updated : Thu Jul 12 12:36:02 2007
Calibration File : Initial Calibration
Quant Method : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
TCP-d5 (IS)	17.31	79	22435	50.00	ng/L	0.00

Compounds	Qvalue

Qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

: C:\DATA\07JUL26\G26008.D
: 26 Jul 2007 2:41 pm
: CQG0634-06
: 25mL
Vial: 8
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Integration Params: RTEINT.P
Time: Jul 27 8:32 2007
Quant Results File: 123-TCP07110

: C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
Update : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration

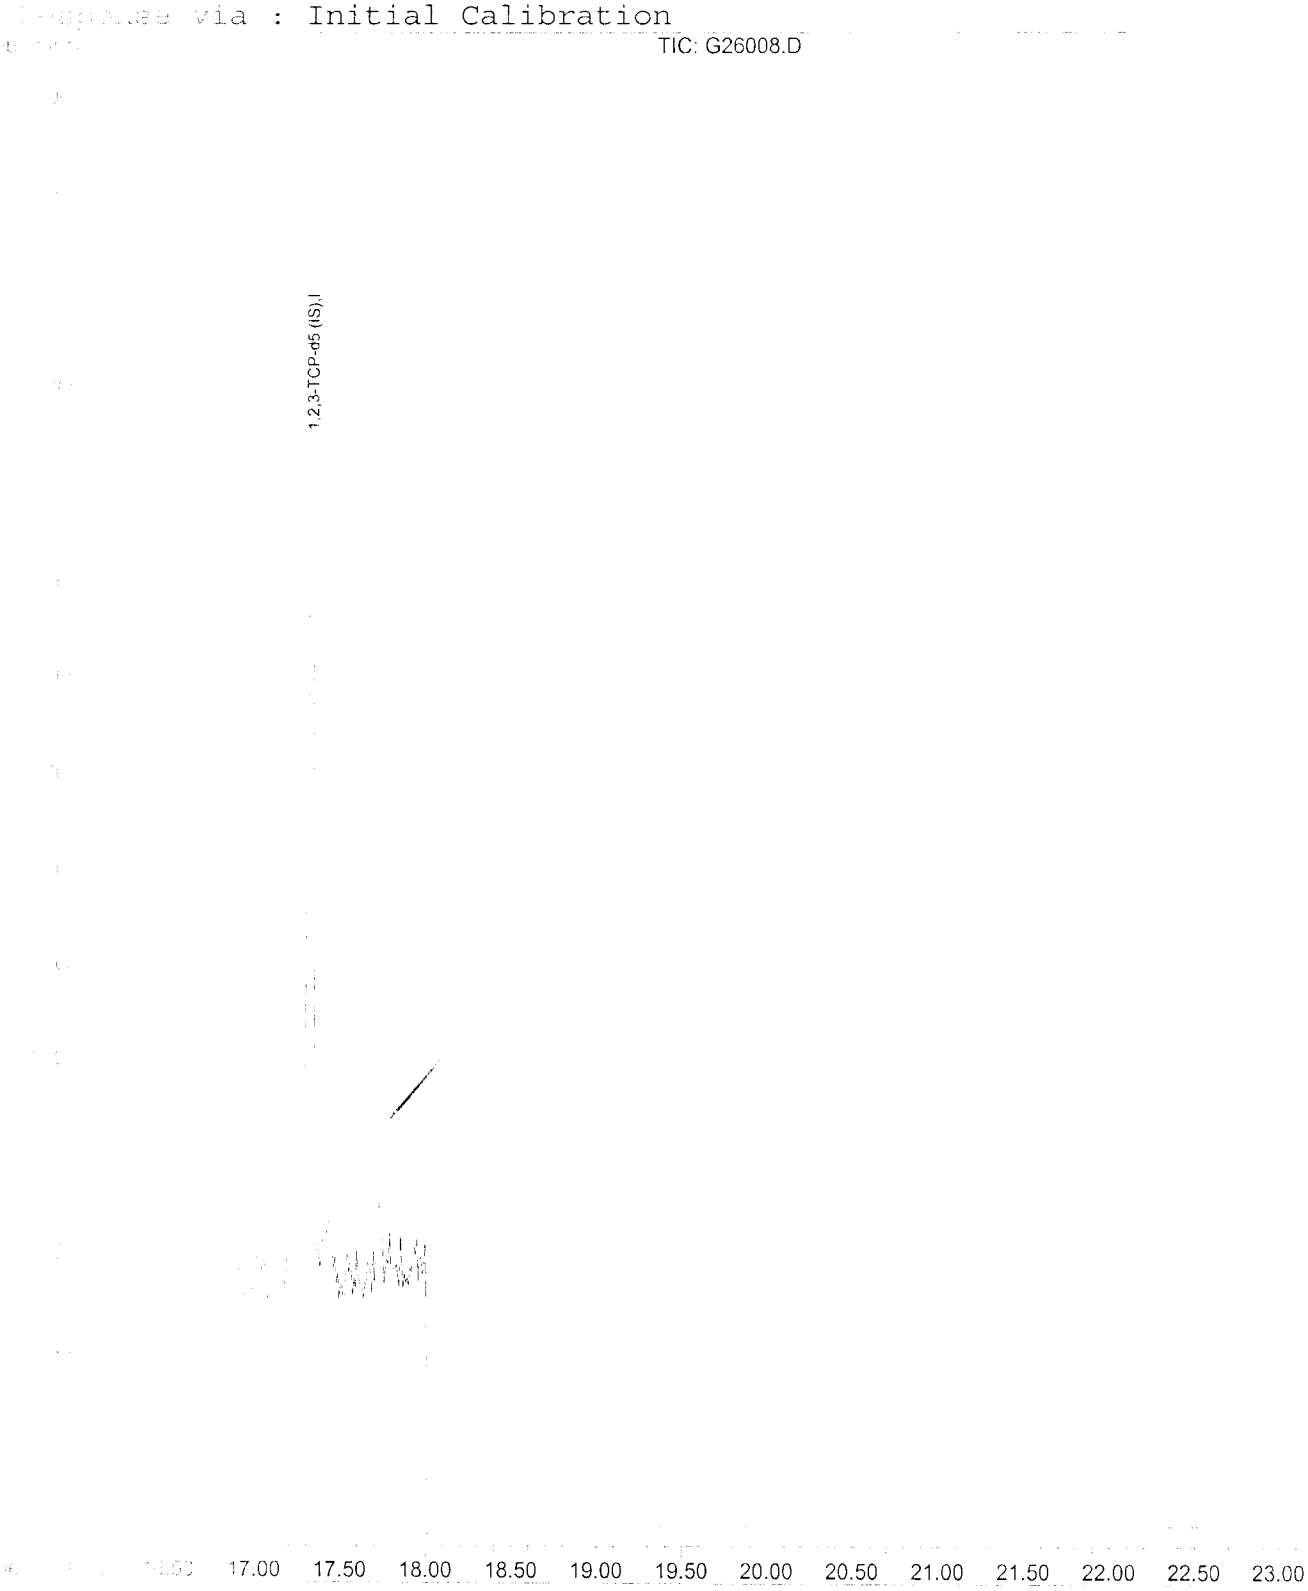

Quantitation Report (Not Reviewed)

C:\DATA\07JUL26\G26010.D
26 Jul 2007 3:46 pm
CQG0702-01
25mL
Integration Params: RTEINT.P
Jul 27 08:32:23 2007

Vial: 10
Operator: PM
Inst : GCMS39
Multiplr: 1.00

7/27/07

Quant Results File: 123-TCP071107.R

Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
Date : Thu Jul 12 12:36:02 2007
Criteria : Initial Calibration
Math : 123-TCP

Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
TCP-d5 (IS)	17.32	79	22149	50.00 ng/L	0.00

Compounds	Qvalue

Qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

: C:\DATA\07JUL26\G26010.D
: 26 Jul 2007 3:46 pm
: CQG0702-01
: 25mL
ration Params: RTEINT.P
ine: Jul 27 8:32 2007

Vial: 10
Operator: PM
Inst : GCMS3
Multiplr: 1.00
Quant Results File: 123-TCP071107

: C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
plate : Thu Jul 12 12:36:02 2007
use via : Initial Calibration

TIC: G26010.D

Quantitation Report (Not Reviewed)

DATA\07JUL26\G26011.D
Jul 2007 4:19 pm
2611-MS1
L w/#7070110; 702-01
Params: RTEINT.P
Jul 27 08:32:25 2007

Vial: 11
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP071107.R

: C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
: Thu Jul 12 12:36:02 2007
: Initial Calibration
: 123-TCP

ndards	R.T.	QIon	Response	Conc Units	Dev(Min)
TCP-d5 (IS)	17.32	79	21119	50.00 ng/L	
ds					Qva
richloropropane	17.41	75	19036	49.77 ng/L	

fier out of range (m) = manual integration (+) = signals summed
-TCP071107.M Fri Jul 27 08:32:26 2007 Page

Quantitation Report (Not Reviewed)

: C:\DATA\07JUL26\G26011.D
: 26 Jul 2007 4:19 pm
: C7G2611-MS1
: 25mL w/#7070110; 702-01
ion Params: RTEINT.P
: Jul 27 8:32 2007

Vial: 11
Operator: PM
Inst : GCMS3
Multiplr: 1.00
Quant Results File: 123-T

: C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
: Thu Jul 12 12:36:02 2007
via : Initial Calibration

TIC: G26011.D



17.00 17.50 18.00 18.50 19.00 19.50 20.00 20.50 21.00 21.50 22.00 22.50 23.00

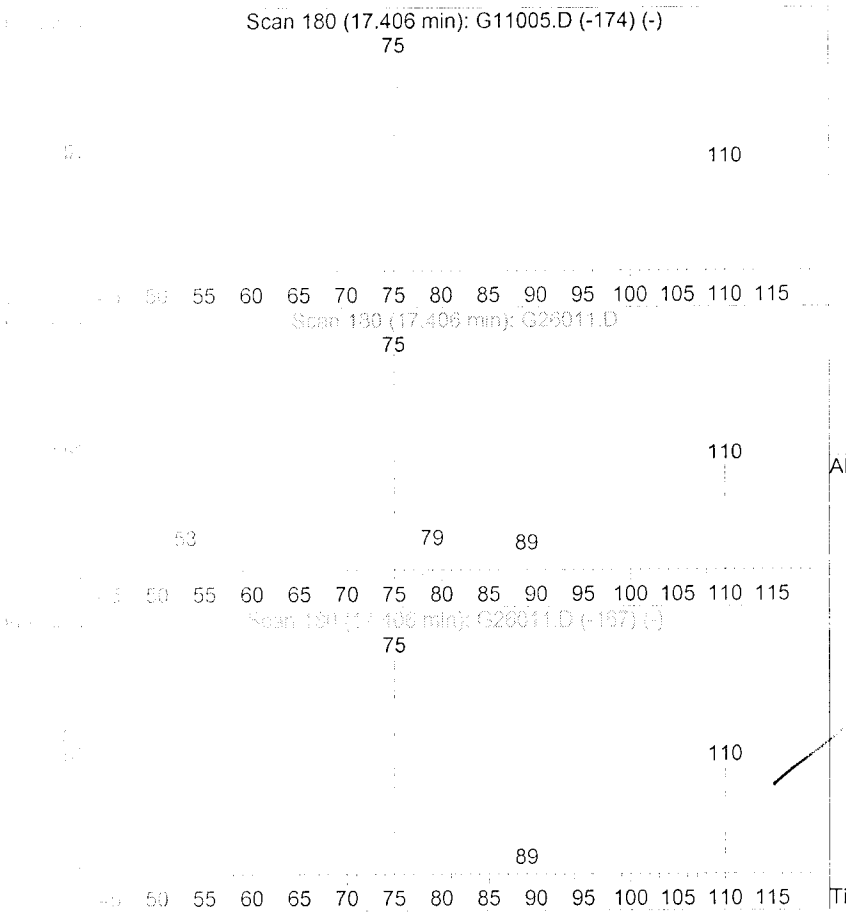

#2
1,2,3-Trichloropropane
Concen: 49.77 ng/L
RT: 17.41 min Scan# 1[illegible]
Delta R.T. 0.00 min
Lab File: G26011.D
Acq: 26 Jul 2007 4:1[illegible] pm

Tgt Ion: 75 Resp: 19[illegible]

Ion	Ratio	Lower	Upper
75	100		
110	43.6	11.2	71.2
53	1.0	0.0	30.0
89	0.8	0.0	30.[illegible]

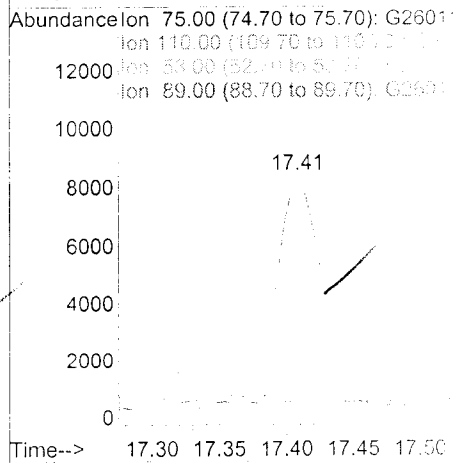

Quantitation Report (Not Reviewed)

C:\DATA\07JUL26\G26012.D
26 Jul 2007 4:52 pm
07G2611-MSD1
35mL w/#7070110; 702-01
Integration Params: RTEINT.P
Jul 27 08:32:27 2007

Vial: 12
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP071107.R

: C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
: Thu Jul 12 12:36:02 2007
: Initial Calibration
: 123-TCP

Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
TCP-d5 (IS)	17.32	79	23137	50.00 ng/L	0.00
Compounds					Qvalue
1 : Trichloropropane	17.41	75	20118	48.01 ng/L #	35

Qualifier out of range (m) = manual integration (+) = signals summed
123-TCP071107.M Fri Jul 27 08:32:28 2007 Page 1

Quantitation Report (Not Reviewed)

Data : C:\DATA\07JUL26\G26012.D
: 26 Jul 2007 4:52 pm
: C7G2611-MSD1
: 25mL w/#7070110; 702-01
Integration Params: RTEINT.P
Quant Time: Jul 27 8:32 2007

Vial: 12
Operator: PM
Inst : GCMS3
Multiplr: 1.00
Quant Results File: 123-TCP07110

: C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
Quantitate : Thu Jul 12 12:36:02 2007
Response via : Initial Calibration

TIC: G26012.D





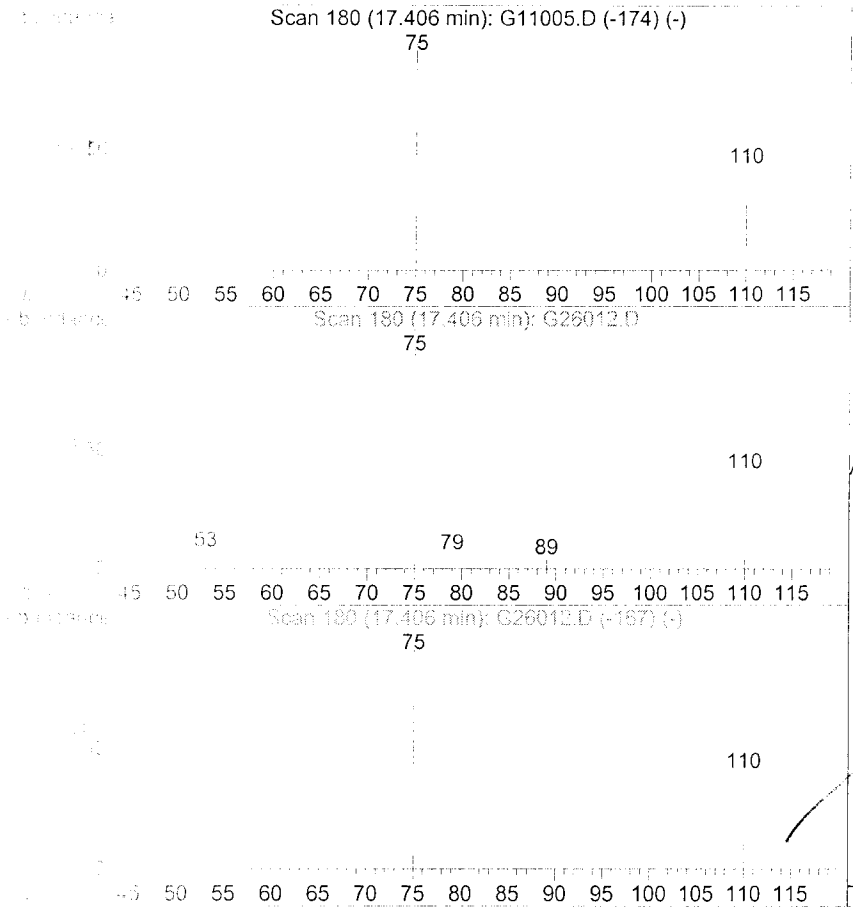

#2
1,2,3-Trichloropropane
Concen: 48.01 ng/L
RT: 17.41 min Scan# 18
Delta R.T. 0.00 min
Lab File: G26012.D
Acq: 26 Jul 2007 4:52 pm

Tgt Ion: 75 Resp: 20118

Ion	Ratio	Lower	Upper
75	100		
110	0.0	11.2	71.2#
53	0.8	0.0	30.0
89	0.4	0.0	30.2

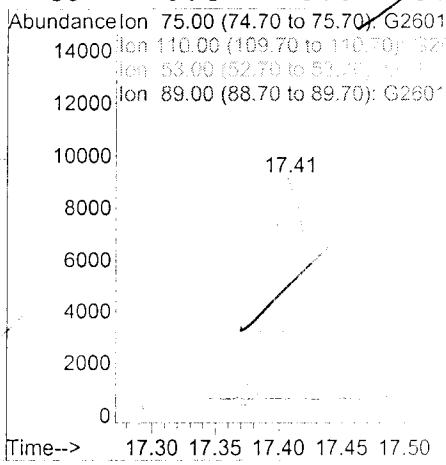

Evaluate Continuing Calibration Report

[illegible]	C:\DATA\07JUL26\G26019.D	Vial:	19
[illegible]	26 Jul 2007 8:40 pm	Operator:	PM
[illegible]	CCV	Inst :	GCMS39
[illegible]	25mL w/ 50ppt #7070110	Multiplr:	1.00
[illegible]	[illegible]ation Params: RTEINT.P		

[illegible] : C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
[illegible] : 1,2,3-TCP by GCMS SIM
[illegible] Update : Thu Jul 12 12:36:02 2007
Response via : Multiple Level Calibration

[illegible] RRF : 0.000 Min. Rel. Area : 80% Max. R.T. Dev 0.50min
[illegible] RRF Dev : 20% Max. Rel. Area : 200%

[illegible]mpound	AvgRF	CCRF	%Dev	Area%	Dev(min)
[illegible]-TCP-d5 (IS)	1.000	1.000	0.0	108	0.00
[illegible]-Trichloropropane	0.906	0.822	9.3	99	0.00

[illegible] of Range SPCC's out = 0 CCC's out = 0
[illegible] 123-TCP071107.M Fri Jul 27 08:35:46 2007 Page 1

351

Quantitation Report (Not Reviewed)

C:\DATA\07JUL26\G26019.D
26 Jul 2007 8:40 pm
CCV
25mL w/ 50ppt #7070110
Integration Params: RTEINT.P
Jul 27 08:32:34 2007

Vial: 19
Operator: PM
Inst : GCMS39
Multiplr: 1.00
Quant Results File: 123-TCP071107.R

Method : C:\MSDCHEM\1...\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
Date : Thu Jul 12 12:36:02 2007
Quant Via : Initial Calibration
Quant Meth : 123-TCP

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1,2,3-TCP-d5 (IS)	17.32	79	21806	50.00 ng/L	0.00

Target Compounds					Qvalue
1,2,3-Trichloropropane	17.41	75	17929	45.40 ng/L	94

Qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Not Reviewed)

: C:\DATA\07JUL26\G26019.D
: 26 Jul 2007 8:40 pm
: CCV
: 25mL w/ 50ppt #7070110
tion Params: RTEINT.P
: Jul 27 8:32 2007

Vial: 19
Operator: PM
Inst : GCMS39
Multiplr: 1.00

Quant Results File: 123-TCP071

: C:\MSDCHEM\1\METHODS\123-TCP071107.M (RTE Integrator)
: 1,2,3-TCP by GCMS SIM
: Thu Jul 12 12:36:02 2007
via : Initial Calibration

TIC: G26019.D

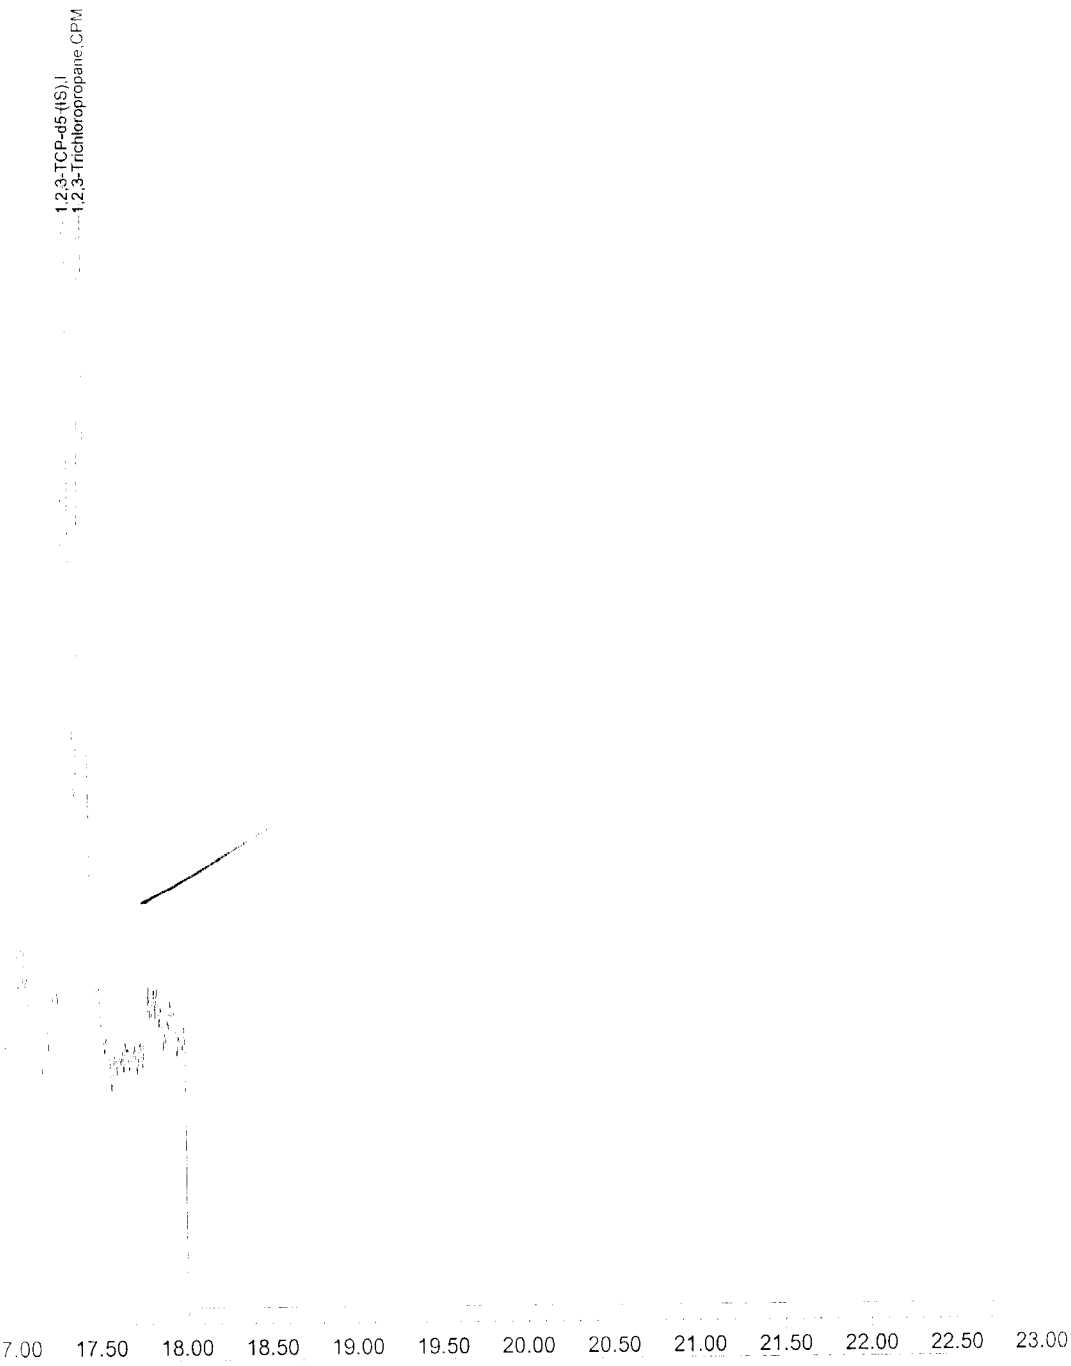

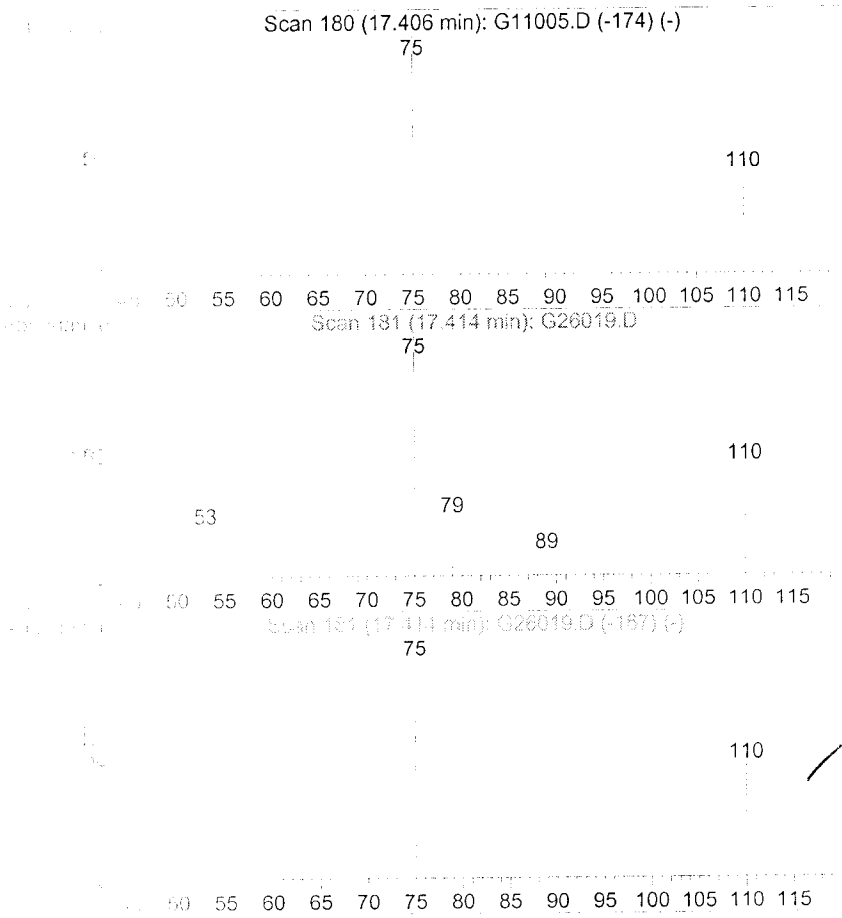

#2
1,2,3-Trichloropropane
Concen: 45.40 ng/L
RT: 17.41 min Scan# 181
Delta R.T. 0.01 min
Lab File: G26019.D
Acq: 26 Jul 2007 8:40 pm

Tgt Ion: 75 Resp: 17929
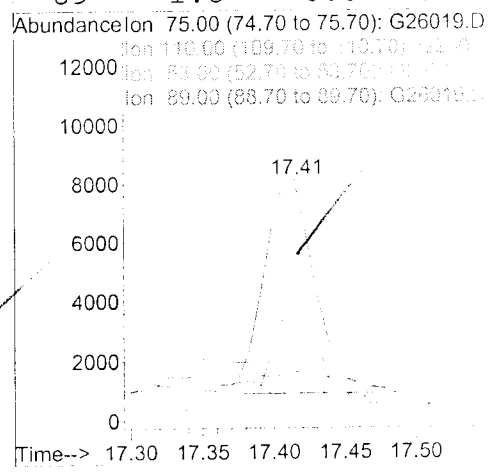
Ion	Ratio	Lower	Upper
75	100		
110	45.1	11.2	71.2
53	2.9	0.0	30.0
89	1.8	0.0	30.8